

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR060722\
 Data File : PR054753.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jun 2022 01:08
 Operator : AJ\MA
 Sample : N3209-11
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 WC-14B-2-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/08/2022
 Supervised By :Ankita Jodhani 06/08/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 02:30:52 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR053122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 01 05:23:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.653	2.930	48925958	25913733	12.120	13.976
2) SA Decachlor...	9.540	8.152	23832246	23843184	14.583m	14.255

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR060722\
Data File : PR054753.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jun 2022 01:08
Operator : AJ\MA
Sample : N3209-11
Misc :
ALS Vial : 52 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
WC-14B-2-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/08/2022
Supervised By :Ankita Jodhani 06/08/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 02:30:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR053122.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 01 05:23:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

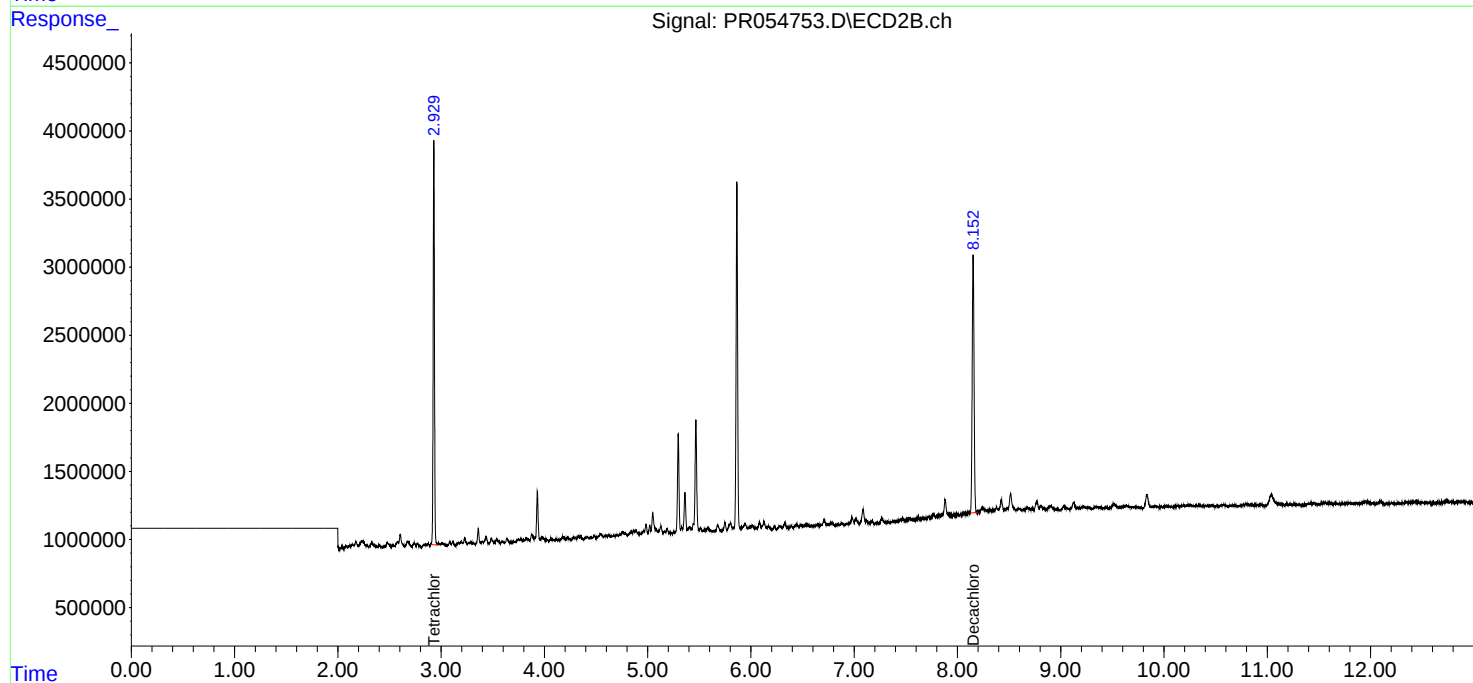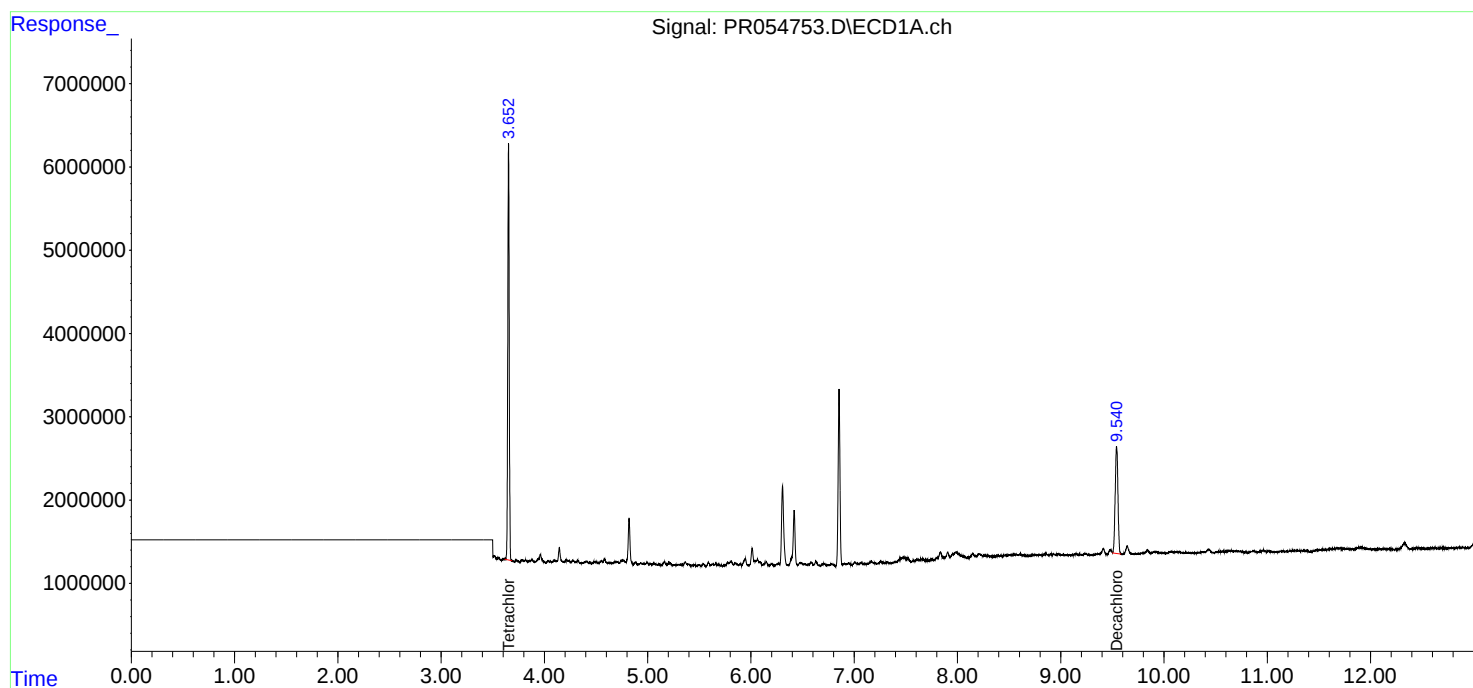

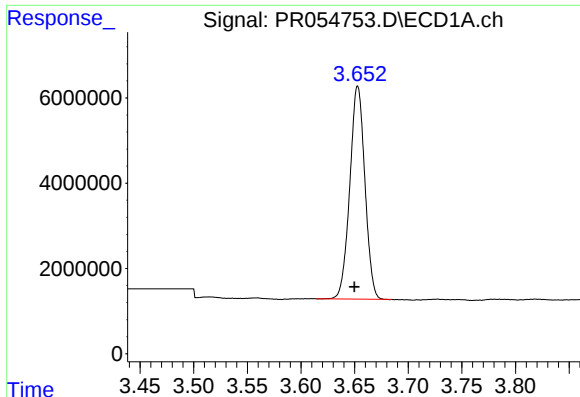


#1 Tetrachloro-m-xylene

R.T.: 3.653 min
Delta R.T.: 0.003 min
Response: 48925958
Conc: 12.12 ng/ml

Instrument :
ECD_R
ClientSampleId :
WC-14B-2-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/08/2022
Supervised By :Ankita Jodhani 06/08/2022

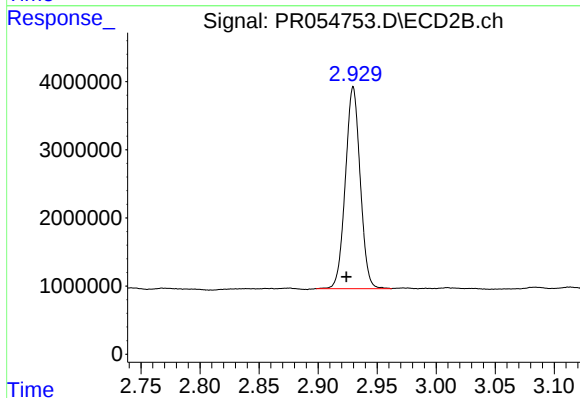


#1 Tetrachloro-m-xylene

R.T.: 2.930 min
Delta R.T.: 0.006 min
Response: 25913733
Conc: 13.98 ng/ml

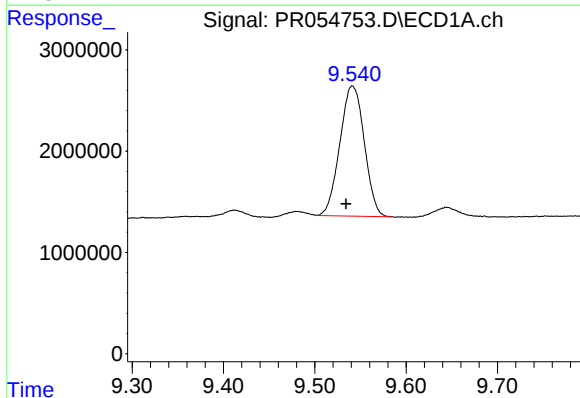

#2 Decachlorobiphenyl

R.T.: 9.540 min
Delta R.T.: 0.006 min
Response: 23832246
Conc: 14.58 ng/ml m

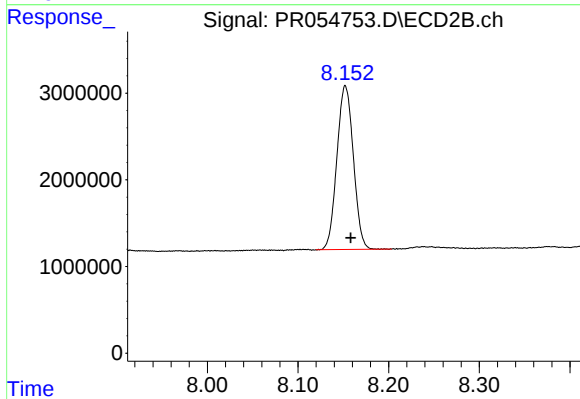

#2 Decachlorobiphenyl

R.T.: 8.152 min
Delta R.T.: -0.006 min
Response: 23843184
Conc: 14.26 ng/ml