

Data Path : Z:\PESTPCBSRV\HPCHEM1\ECD_R\Data\PR061018\
 Data File : PR028765.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jun 2018 16:52
 Operator : UA/SM
 Sample : J3276-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 ES-ASBESTOS-PIPE

Manual Integrations
 APPROVED

UGO
 6/6/2018 6:29:27 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 06 17:05:55 2018
 Quant Method : \\TERASTORAGE\Terastorage\PESTPCBSRV\HPCHEM1\ECD_R\Method\PR061018.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 06 14:28:54 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.578	3.729	95309677	204.4E6	3.862m	4.193
2) SA Decachlor...	10.358	8.684	91159445	221.4E6	4.287	3.882

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\PESTPCBSRV\HPCHEM1\ECD_R\Data\PR061018\
Data File : PR028765.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jun 2018 16:52
Operator : UA/SM
Sample : J3276-02
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
ES-ASBESTOS-PIPE


Manual Integrations
APPROVED

UGO
6/6/2018 6:29:27 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 06 17:05:55 2018
Quant Method : \\TERASTORAGE\Terastorage\PESTPCBSRV\HPCHEM1\ECD_R\Method\PR061018.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 06 14:28:54 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

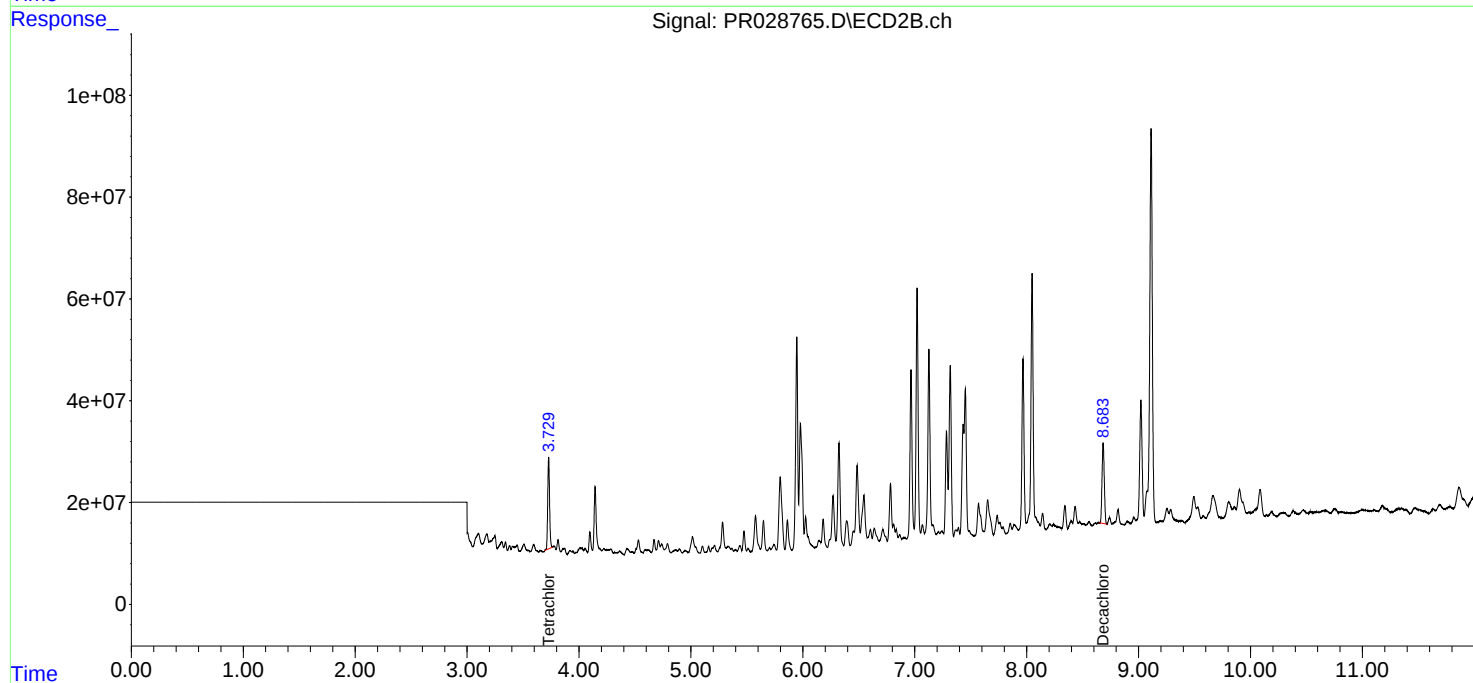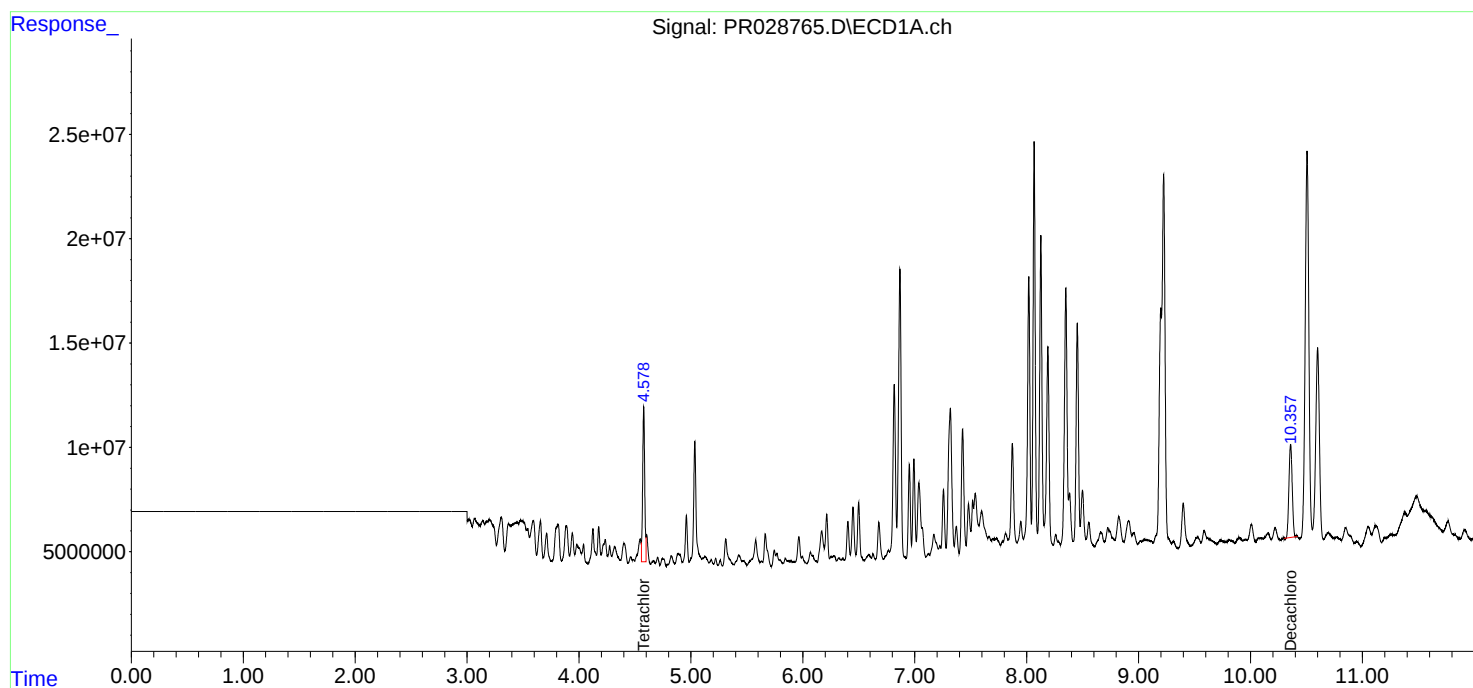

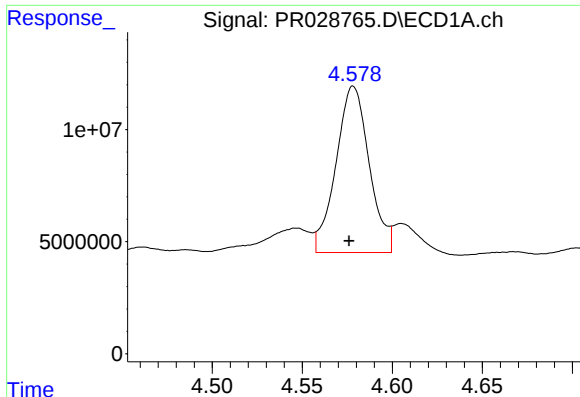


#1 Tetrachloro-m-xylene

R.T.: 4.578 min
Delta R.T.: 0.002 min
Response: 95309677
Conc: 3.86 ng/ml m

Instrument :
ECD_R
ClientSampleId :
ES-ASBESTOS-PIPE


Manual Integrations
APPROVED

UGO
6/6/2018 6:29:27 PM

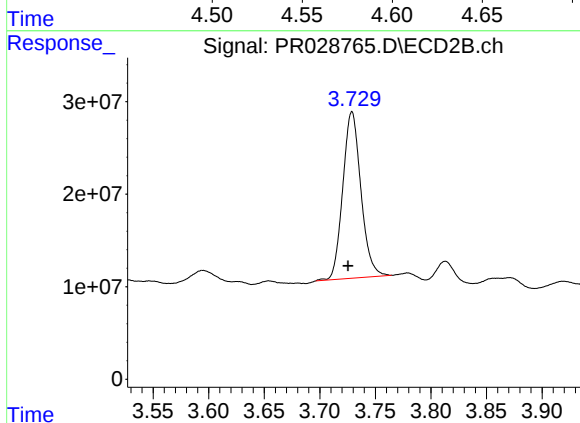


#1 Tetrachloro-m-xylene

R.T.: 3.729 min
Delta R.T.: 0.004 min
Response: 204442575
Conc: 4.19 ng/ml

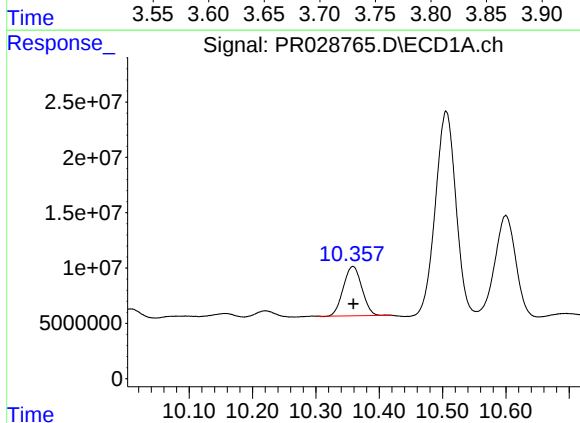

#2 Decachlorobiphenyl

R.T.: 10.358 min
Delta R.T.: 0.000 min
Response: 91159445
Conc: 4.29 ng/ml

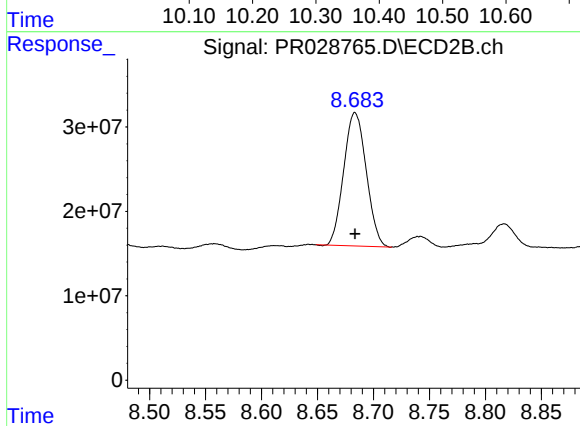

#2 Decachlorobiphenyl

R.T.: 8.684 min
Delta R.T.: 0.000 min
Response: 221361592
Conc: 3.88 ng/ml