

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR061923\
 Data File : PR061876.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2023 15:17
 Operator : YP\AJ
 Sample : 03289-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 SB-01-4.0-6.0

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/20/2023
 Supervised By :Ankita Jodhani 06/20/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 22:19:14 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR061923.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 19 13:30:08 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.691	2.962	60663994	77288922	27.588	28.136
2) SA Decachlor...	9.626	8.249	37657505	94673535	26.025m	26.696

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR061923\
Data File : PR061876.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2023 15:17
Operator : YP\AJ
Sample : 03289-02
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
SB-01-4.0-6.0


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/20/2023
Supervised By :Ankita Jodhani 06/20/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 22:19:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR061923.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 19 13:30:08 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

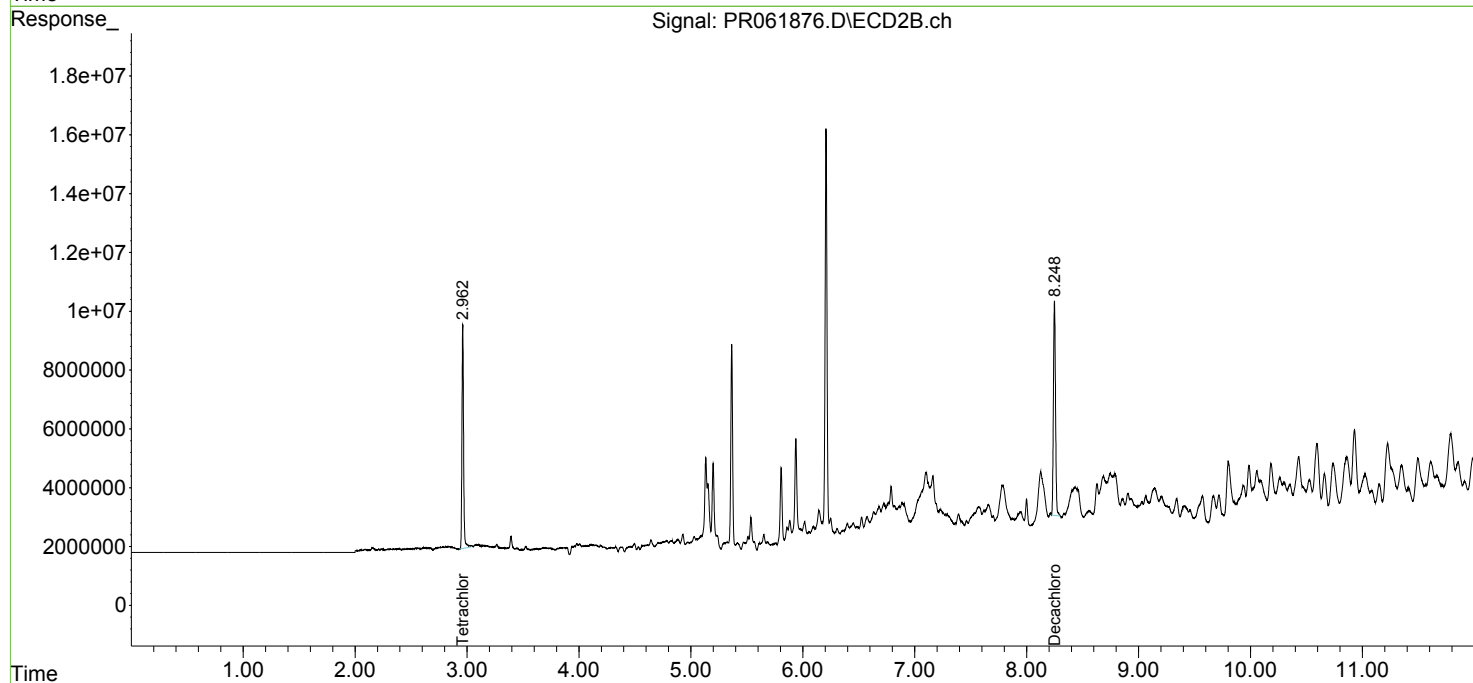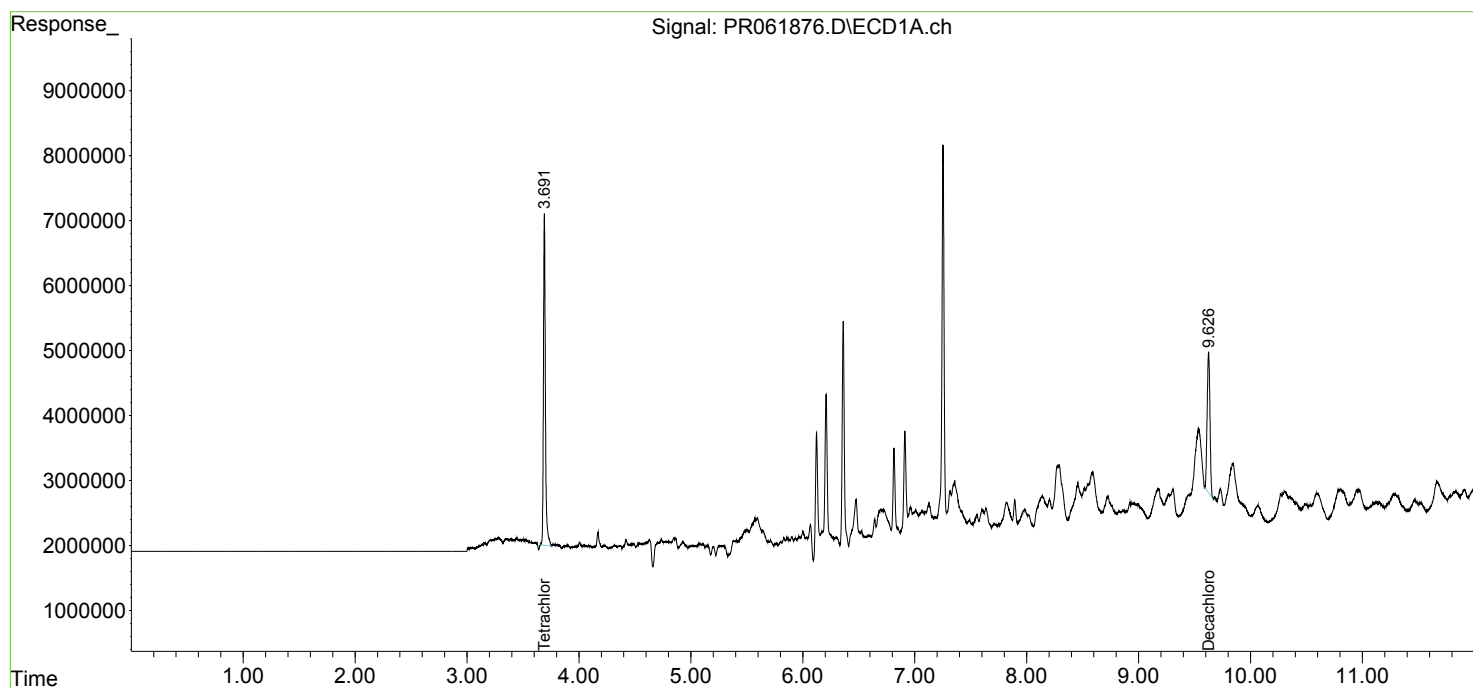

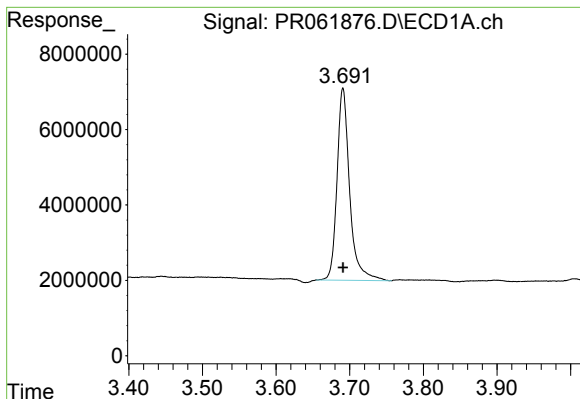

#1 Tetrachloro-m-xylene

R.T.: 3.691 min
Delta R.T.: 0.000 min
Response: 60663994
Conc: 27.59 ng/ml

Instrument :

ECD_R


ClientSampleId :

SB-01-4.0-6.0

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 06/20/2023
Supervised By :Ankita Jodhani 06/20/2023

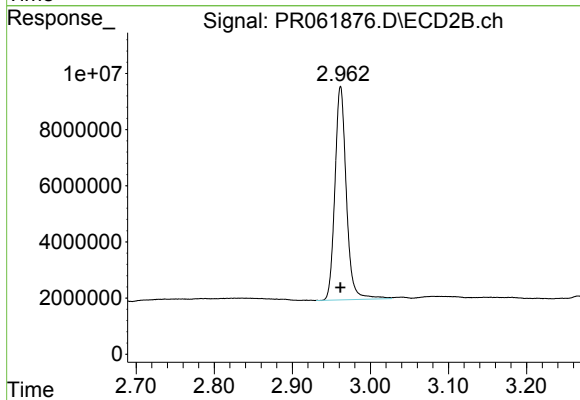


#1 Tetrachloro-m-xylene

R.T.: 2.962 min
Delta R.T.: 0.000 min
Response: 77288922
Conc: 28.14 ng/ml

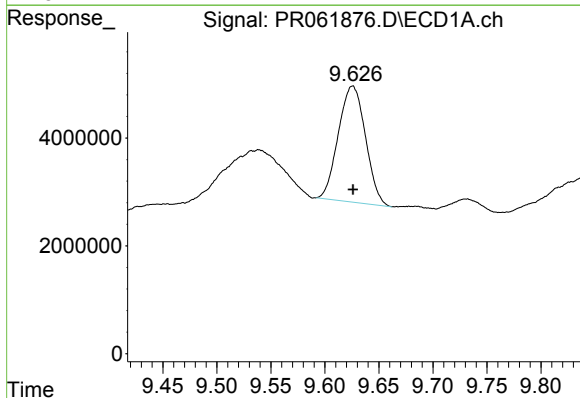

#2 Decachlorobiphenyl

R.T.: 9.626 min
Delta R.T.: 0.000 min
Response: 37657505
Conc: 26.03 ng/ml m

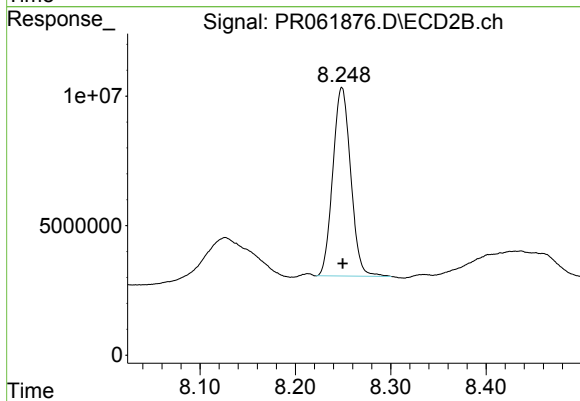

#2 Decachlorobiphenyl

R.T.: 8.249 min
Delta R.T.: 0.000 min
Response: 94673535
Conc: 26.70 ng/ml