

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR061923\
 Data File : PR061877.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2023 15:31
 Operator : YP\AJ
 Sample : 03289-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 SB-02-0-2.0

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/20/2023
 Supervised By :Ankita Jodhani 06/20/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 22:21:07 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR061923.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 19 13:30:08 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.691	2.962	58759855	77429511	26.722	28.187
2) SA Decachlor...	9.627	8.248	32973534	81631100	22.788m	23.018

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR061923\
Data File : PR061877.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2023 15:31
Operator : YP\AJ
Sample : 03289-04
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
SB-02-0-2.0


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/20/2023
Supervised By :Ankita Jodhani 06/20/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 22:21:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR061923.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 19 13:30:08 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

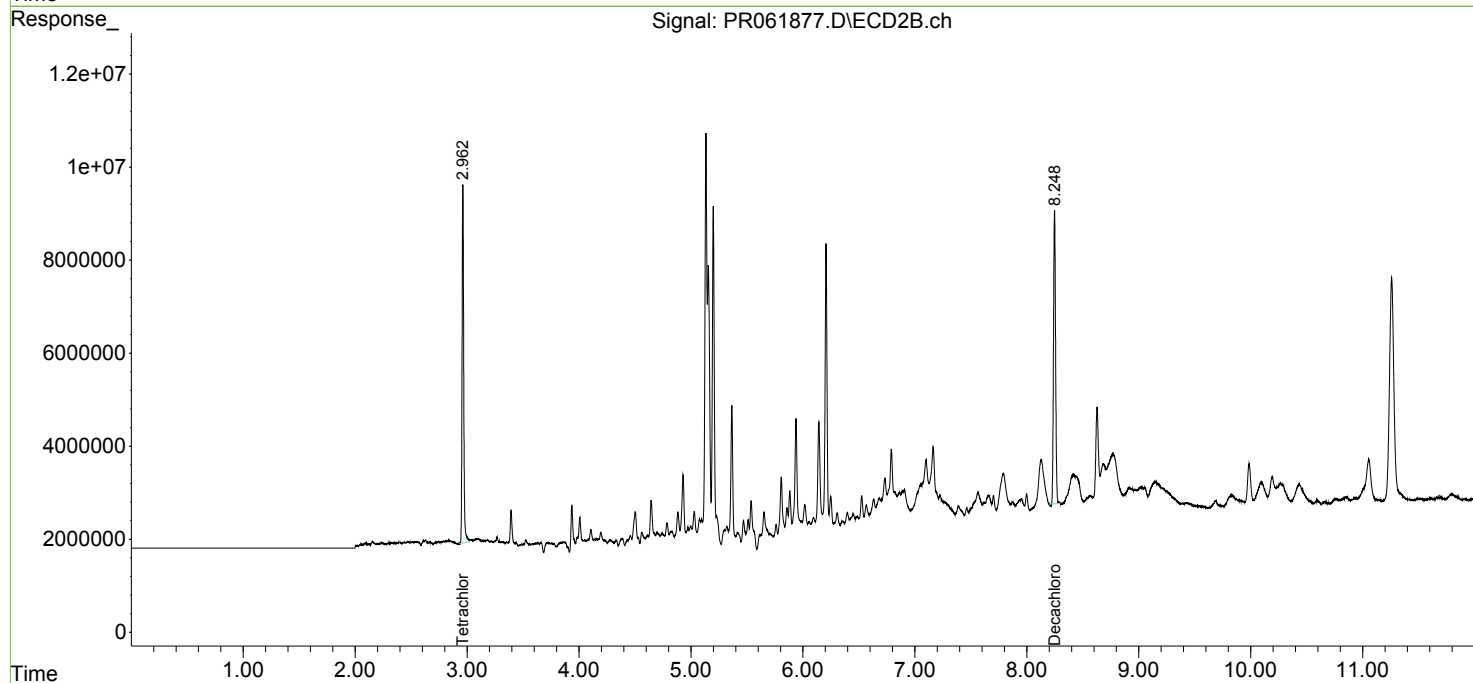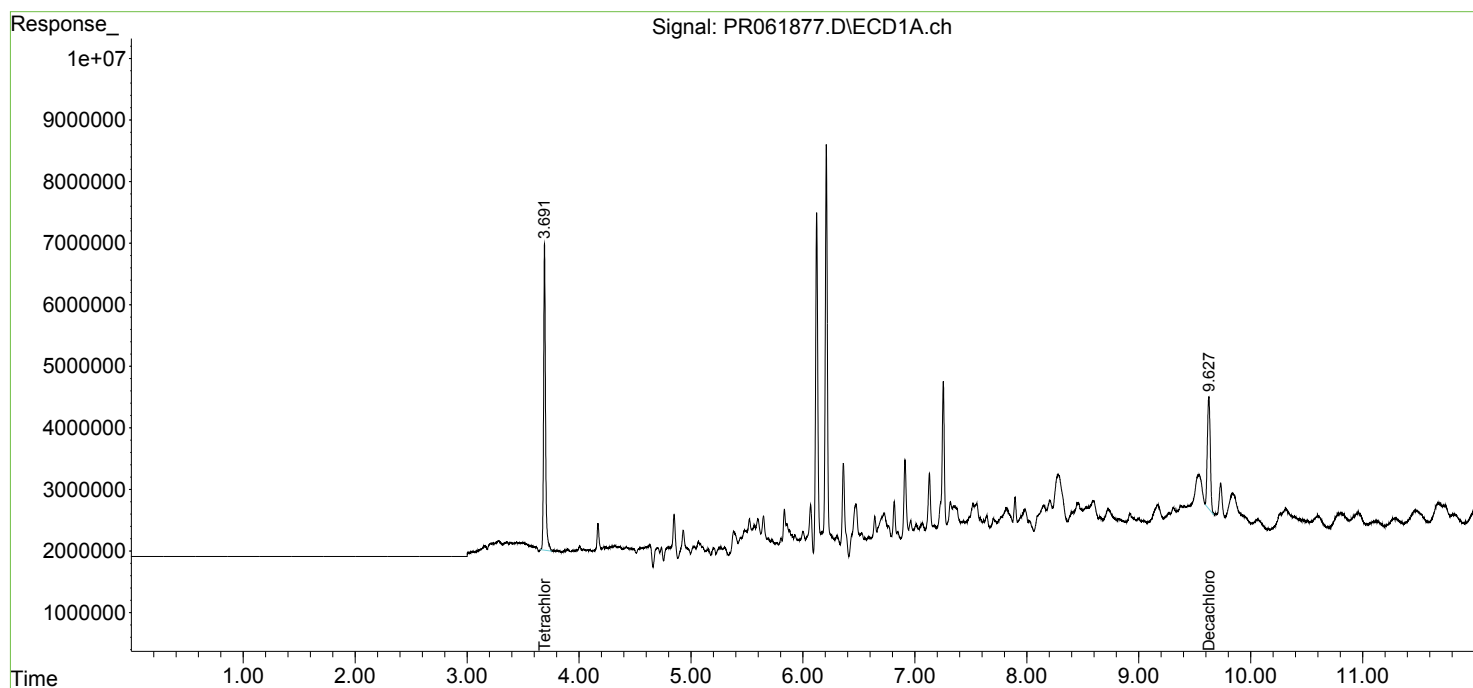

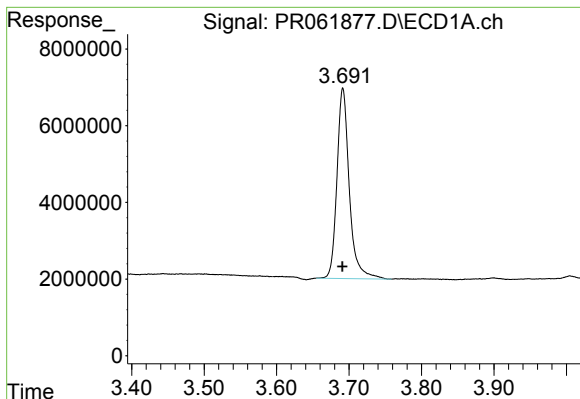


#1 Tetrachloro-m-xylene

R.T.: 3.691 min
Delta R.T.: 0.000 min
Response: 58759855
Conc: 26.72 ng/ml

Instrument :
ECD_R
ClientSampleId :
SB-02-0-2.0


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/20/2023
Supervised By :Ankita Jodhani 06/20/2023

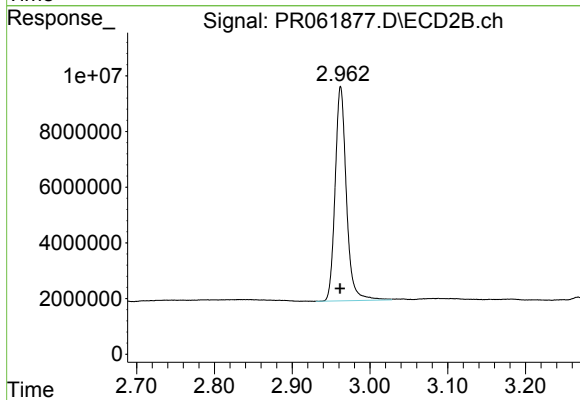


#1 Tetrachloro-m-xylene

R.T.: 2.962 min
Delta R.T.: 0.000 min
Response: 77429511
Conc: 28.19 ng/ml

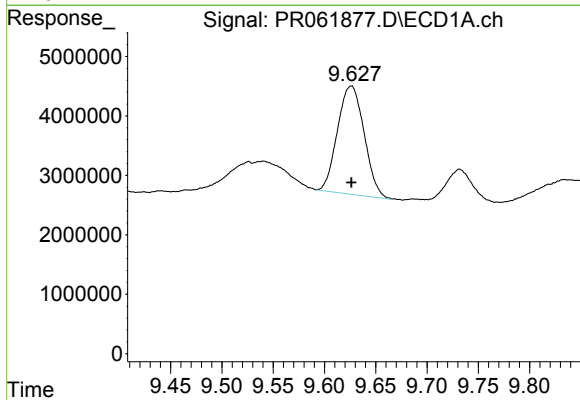

#2 Decachlorobiphenyl

R.T.: 9.627 min
Delta R.T.: 0.000 min
Response: 32973534
Conc: 22.79 ng/ml m

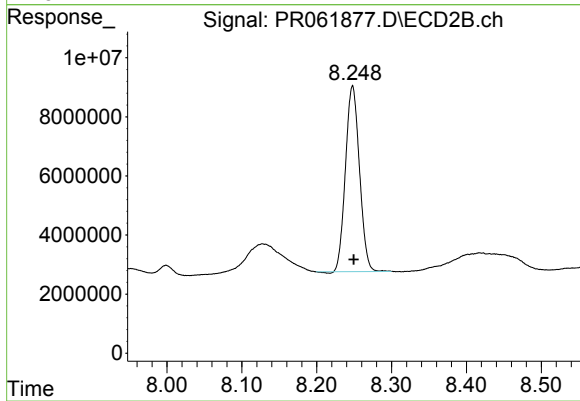

#2 Decachlorobiphenyl

R.T.: 8.248 min
Delta R.T.: -0.002 min
Response: 81631100
Conc: 23.02 ng/ml