

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061924\
 Data File : PD083747.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2024 15:37
 Operator : AR\AJ
 Sample : PIBLK195
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 PIBLK154

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 22:34:44 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 07 04:03:14 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.561	2.772	20767459	97534362	15.910	17.893
2)	SA Decachlor...	9.111	7.895	46328174	125.7E6	23.825	20.706
Target Compounds							
10)	B trans-Chl...	6.003	0.000	1417426	0	0.696	N.D. #
11)	B cis-Chlor...	6.003f	0.000	1417426	0	0.681	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061924\
Data File : PD083747.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2024 15:37
Operator : AR\AJ
Sample : PIBLK195
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 22:34:44 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 07 04:03:14 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

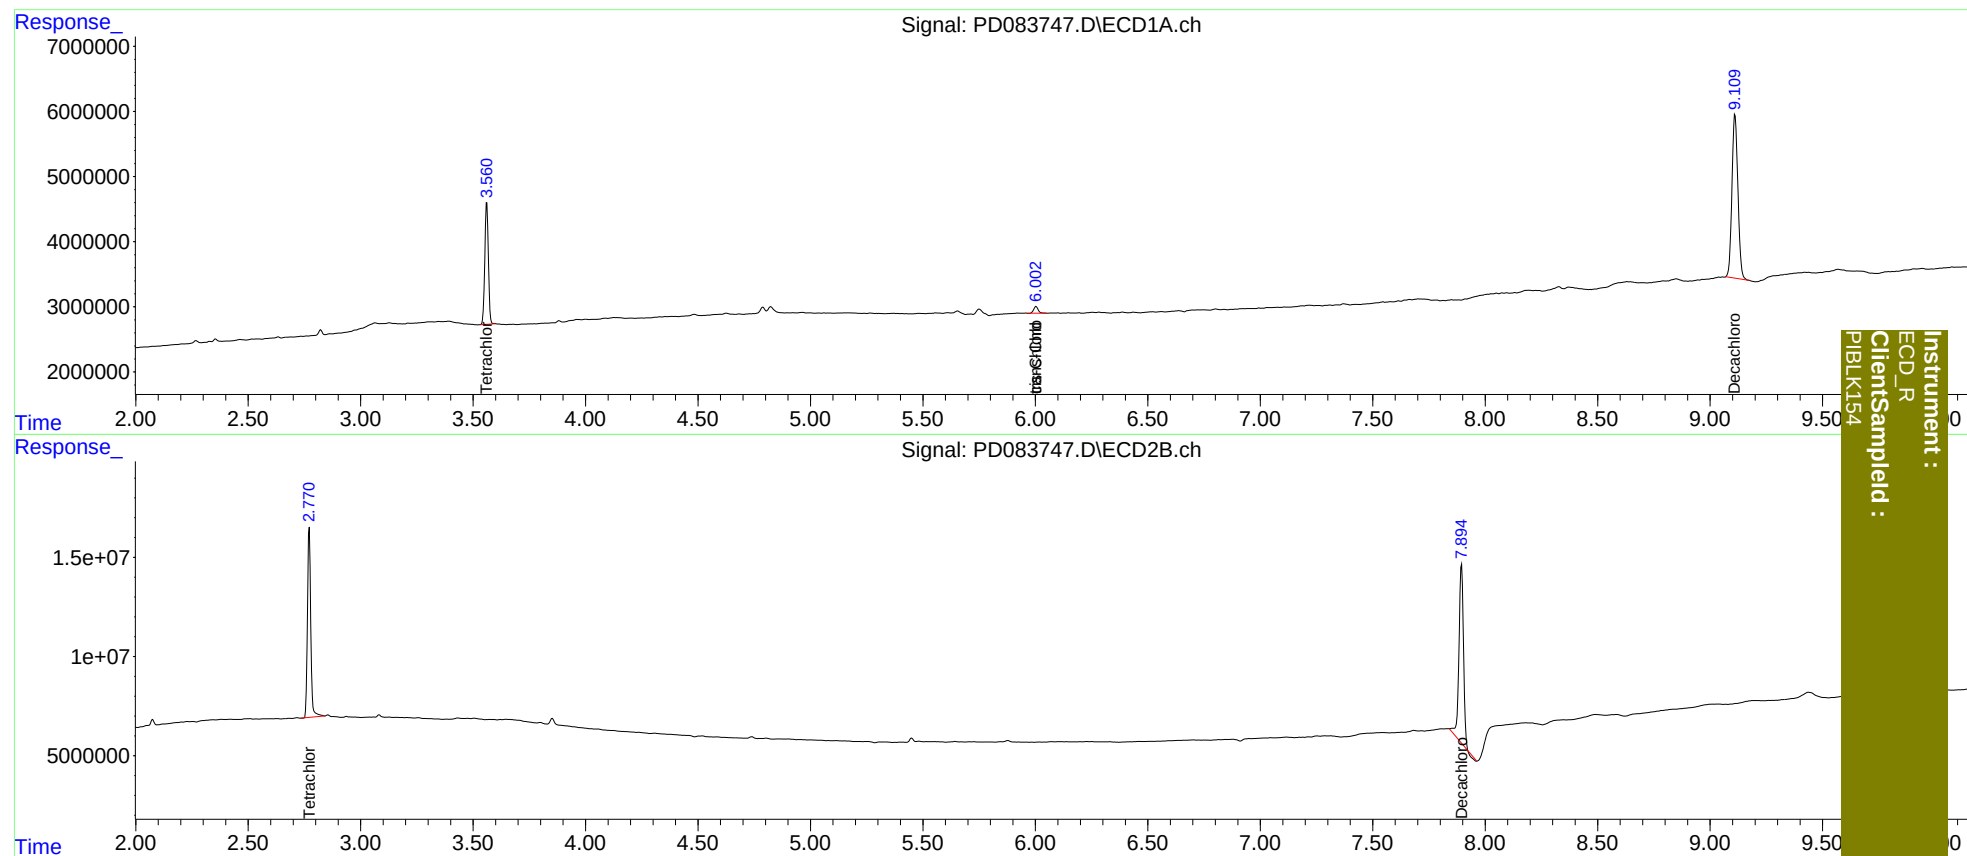


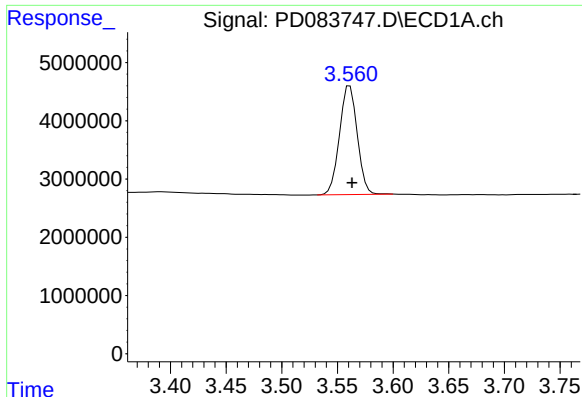

#1 Tetrachloro-m-xylene


R.T.: 3.561 min
Delta R.T.: -0.002 min
Response: 20767459
Conc: 15.91 ng/ml

Instrument :
ECD_R
ClientSampleId :
PIBLK154

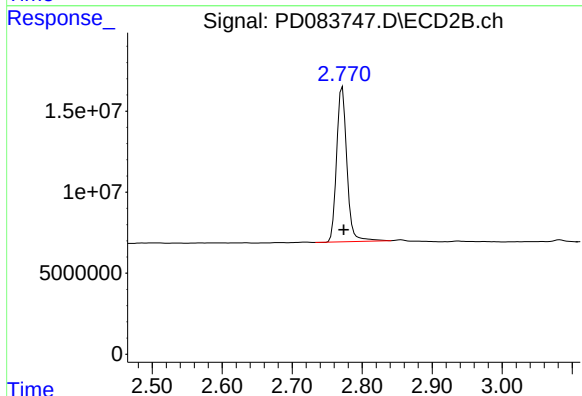


#1 Tetrachloro-m-xylene

R.T.: 2.772 min
Delta R.T.: -0.002 min
Response: 97534362
Conc: 17.89 ng/ml

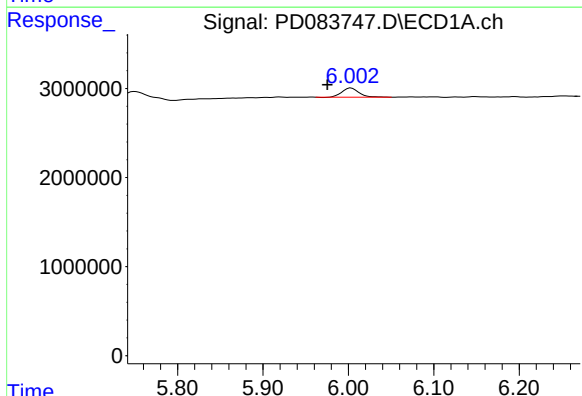


#10 trans-Chlordane

R.T.: 6.003 min
Delta R.T.: 0.028 min
Response: 1417426
Conc: 0.70 ng/ml

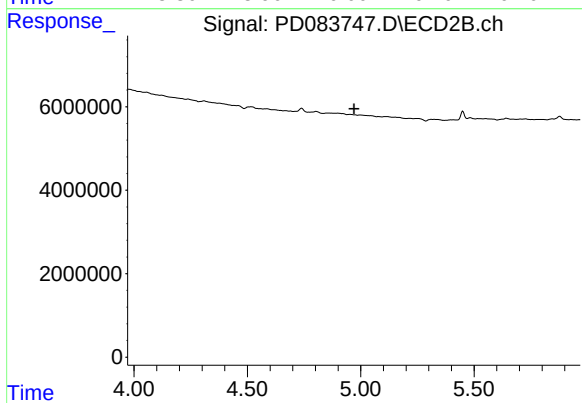

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 4.970 min
Response: 0
Conc: N.D.

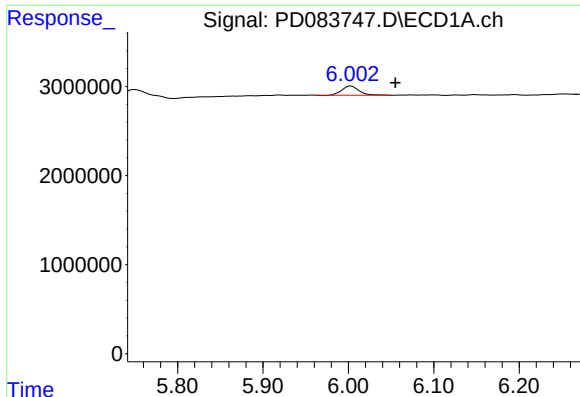

#11 cis-Chlordane


R.T.: 6.003 min
Delta R.T.: -0.052 min
Response: 1417426
Conc: 0.68 ng/ml

Instrument :
ECD_R
ClientSampleId :
PIBLK154

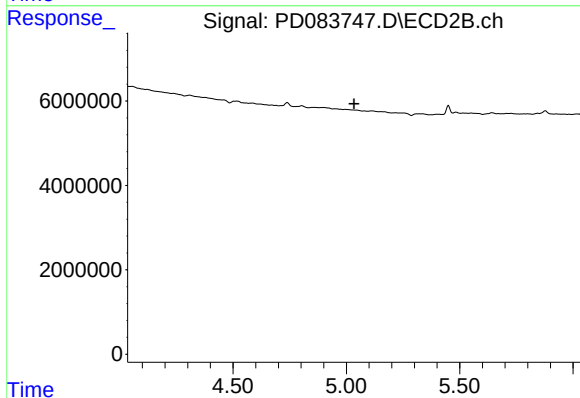


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.034 min
Response: 0
Conc: N.D.

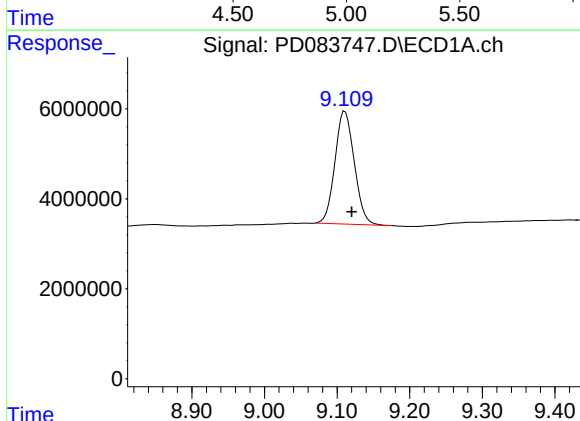

#27 Decachlorobiphenyl

R.T.: 9.111 min
Delta R.T.: -0.009 min
Response: 46328174
Conc: 23.83 ng/ml

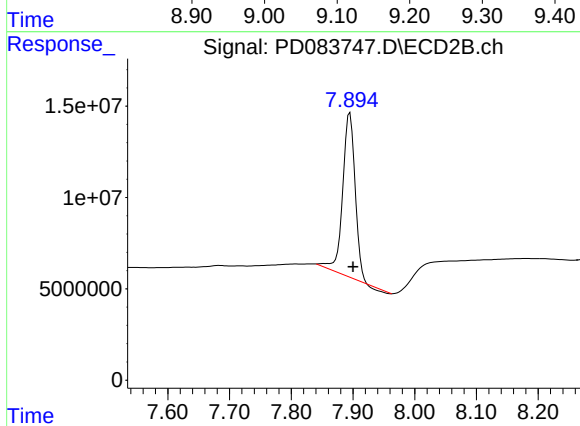

#27 Decachlorobiphenyl

R.T.: 7.895 min
Delta R.T.: -0.006 min
Response: 125732859
Conc: 20.71 ng/ml