

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR062023\
 Data File : PR061921.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2023 16:46
 Operator : YP\AJ
 Sample : 03312-10
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 R034-4A

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/21/2023
 Supervised By :Ankita Jodhani 06/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 20 22:42:50 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR061923.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 19 13:30:08 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.690	2.961	51827421	76509353	23.570m	27.852
2) SA Decachlor...	9.623	8.246	30499813	68752678	21.079	19.387

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR062023\
Data File : PR061921.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2023 16:46
Operator : YP\AJ
Sample : 03312-10
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
R034-4A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/21/2023
Supervised By :Ankita Jodhani 06/21/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 22:42:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR061923.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 19 13:30:08 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

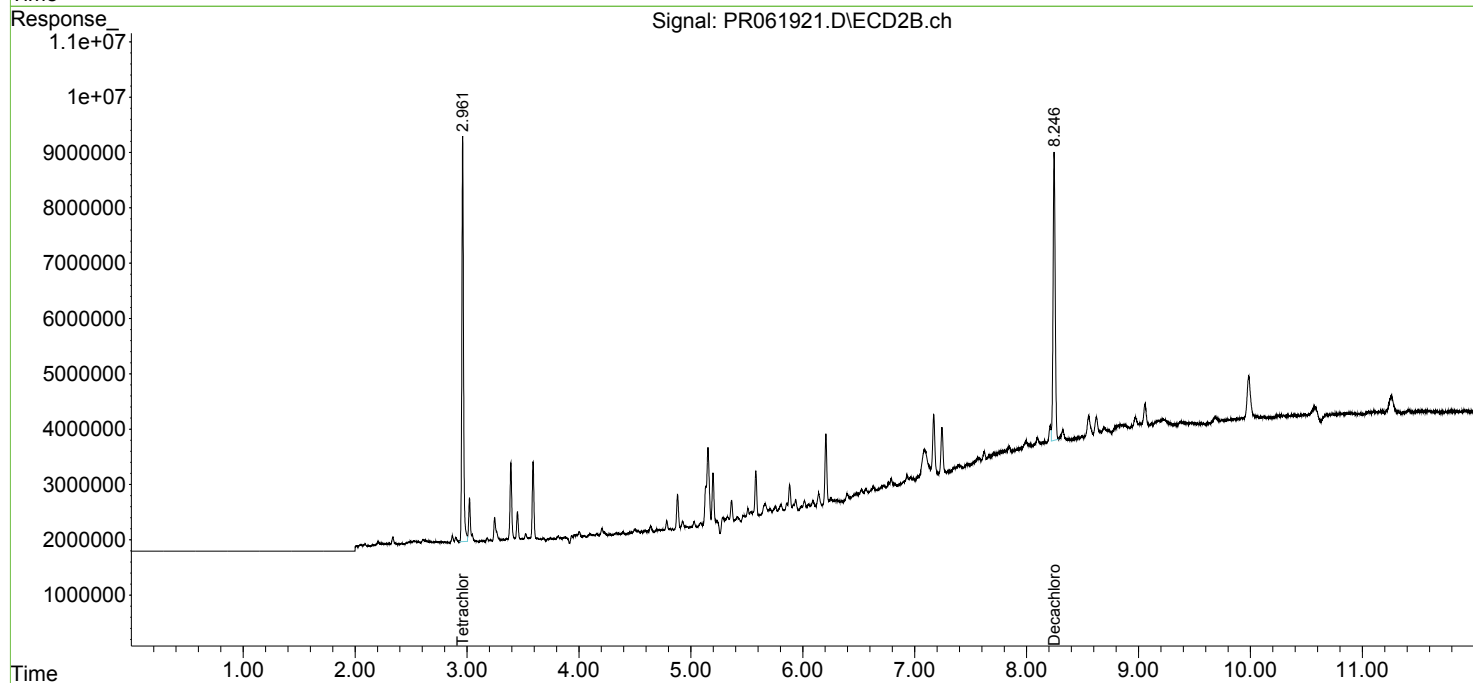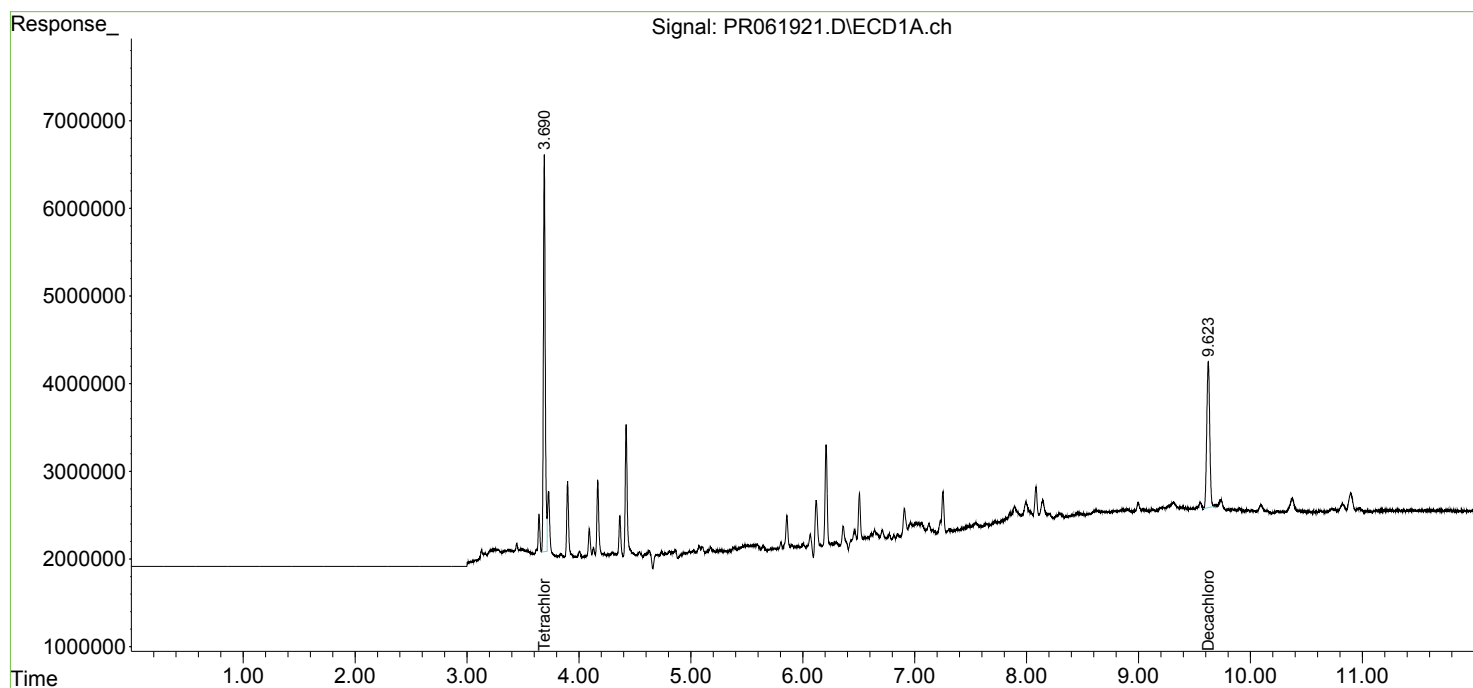

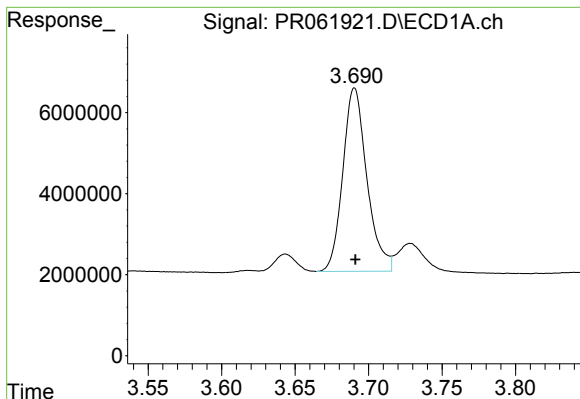


#1 Tetrachloro-m-xylene

R.T.: 3.690 min
Delta R.T.: 0.000 min
Response: 51827421
Conc: 23.57 ng/ml

Instrument :
ECD_R
ClientSampleId :
R034-4A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/21/2023
Supervised By :Ankita Jodhani 06/21/2023

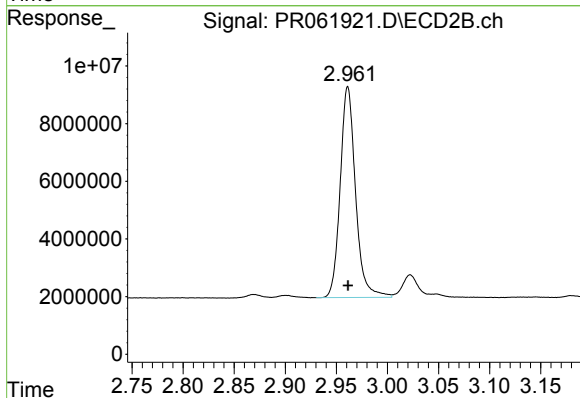


#1 Tetrachloro-m-xylene

R.T.: 2.961 min
Delta R.T.: 0.000 min
Response: 76509353
Conc: 27.85 ng/ml

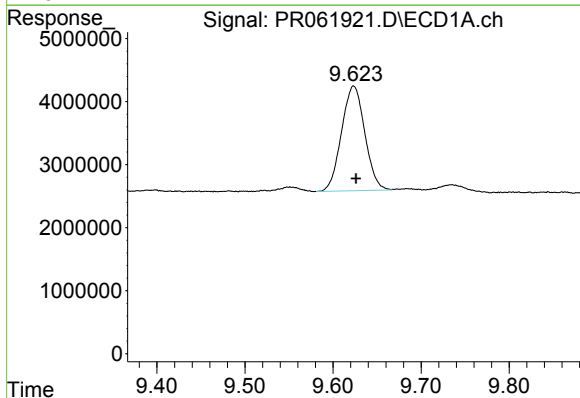

#2 Decachlorobiphenyl

R.T.: 9.623 min
Delta R.T.: -0.003 min
Response: 30499813
Conc: 21.08 ng/ml

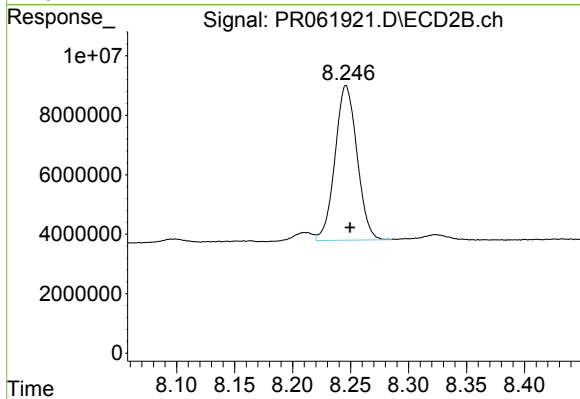

#2 Decachlorobiphenyl

R.T.: 8.246 min
Delta R.T.: -0.003 min
Response: 68752678
Conc: 19.39 ng/ml