

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR062221\
 Data File : PR050940.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2021 11:16
 Operator : DD\AJ
 Sample : PB137216BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 ABLK216

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 00:59:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR060121CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 02 05:07:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.635	3.814	170.2E6	152.0E6	26.669	23.377
2)	SA Decachlor...	10.515	8.840	311.1E6	310.9E6	42.828	40.091
Target Compounds							
8)	L2 AR-1221-1	0.000	3.974f	0	897394	N.D.	12.828 #
9)	L2 AR-1221-2	4.946	4.115	2119383	1900030	41.706	38.010
10)	L2 AR-1221-3	4.946f	0.000	2119383	0	12.507	N.D. #
11)	L3 AR-1232-1	4.946f	0.000	2119383	0	15.252	N.D. #
34)	L7 AR-1260-4	0.000	7.159	0	682045	N.D.	1.709 #
35)	L7 AR-1260-5	0.000	7.419	0	4685293	N.D.	4.811 #
37)	L8 AR-1262-2	0.000	7.419	0	4685293	N.D.	3.547 #
45)	L9 AR-1268-5	10.162	8.576	2220185	1937916	0.572	0.468



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR062221\
Data File : PR050940.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2021 11:16
Operator : DD\AJ
Sample : PB137216BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
ABLK216

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 00:59:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR060121CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 02 05:07:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

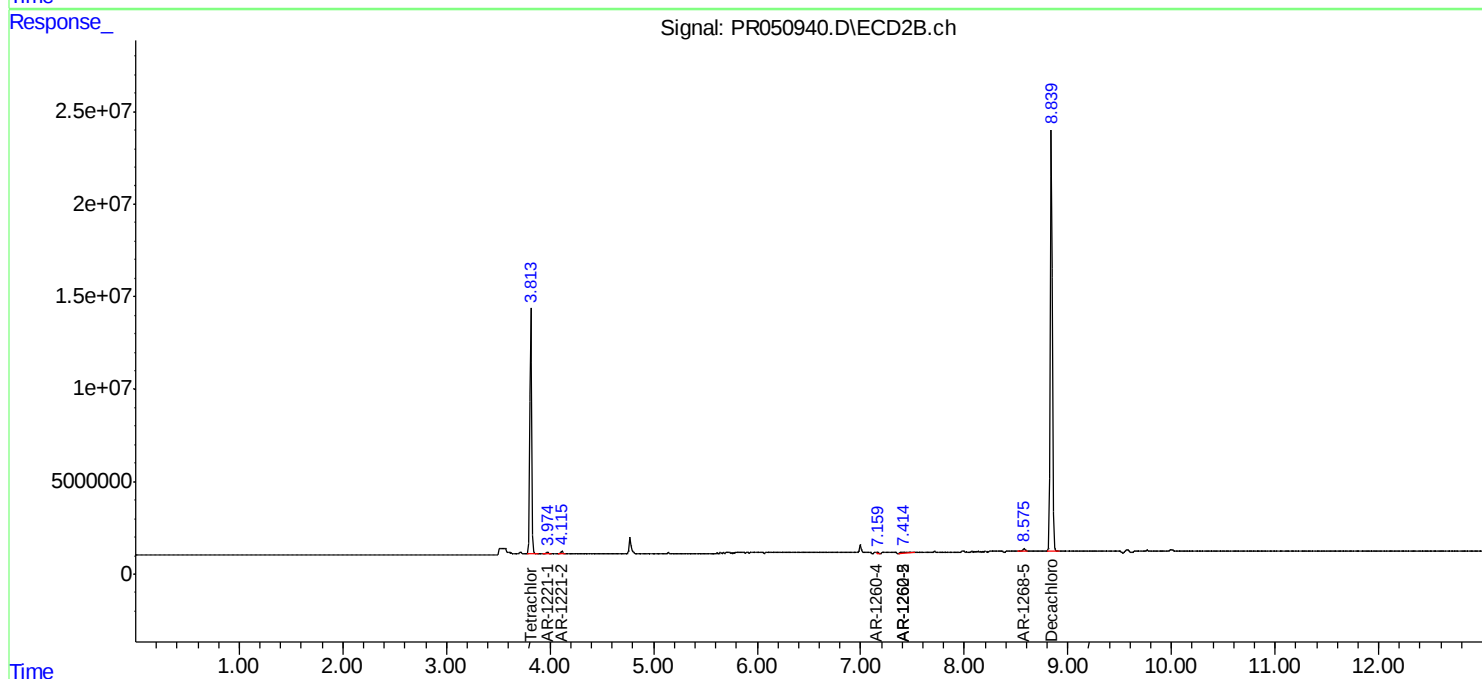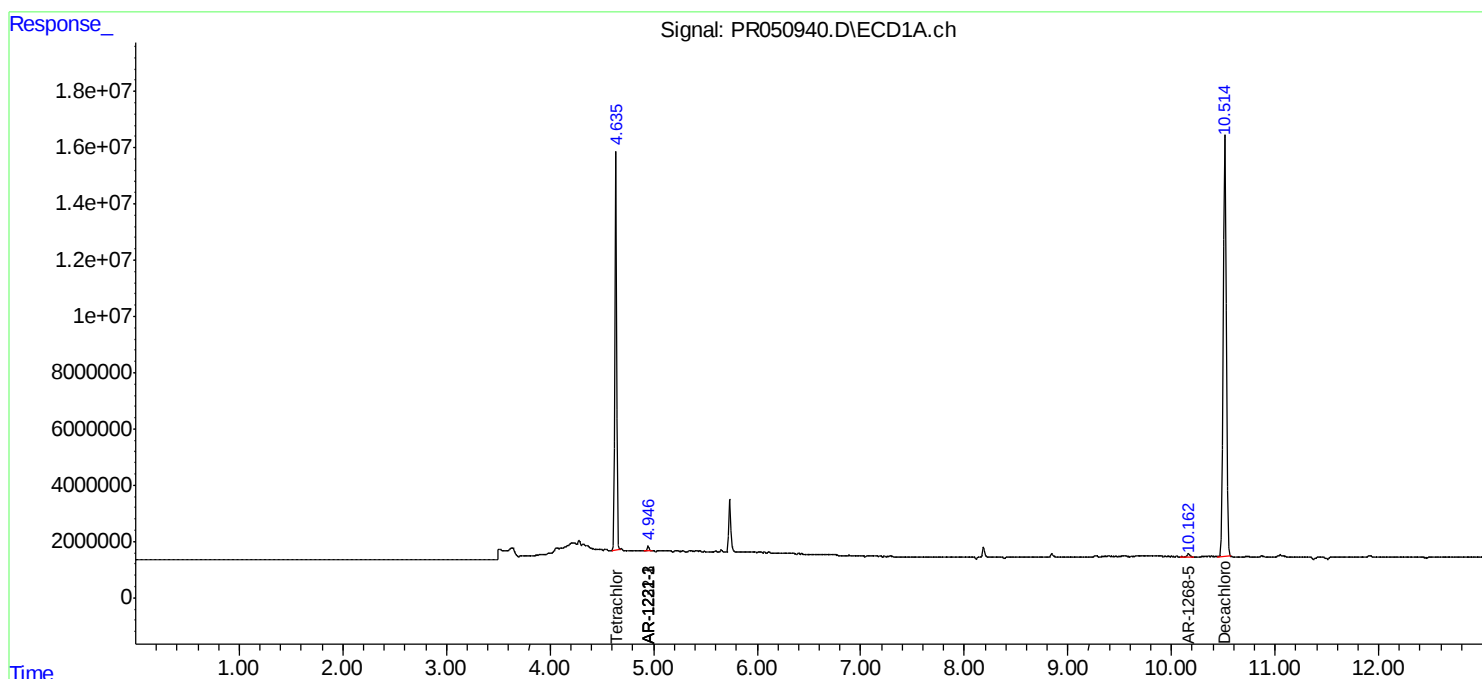


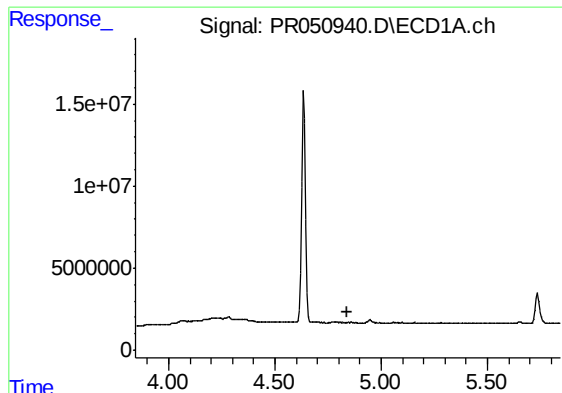

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T.: 4.844 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
ABLK216

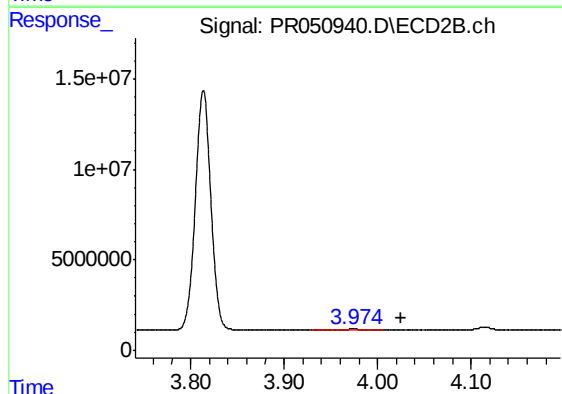


#8 AR-1221-1

R.T.: 3.974 min
Delta R.T.: -0.050 min
Response: 897394
Conc: 12.83 ng/ml

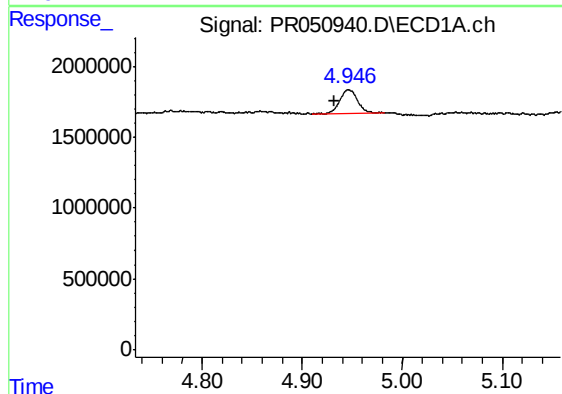


#9 AR-1221-2

R.T.: 4.946 min
Delta R.T.: 0.014 min
Response: 2119383
Conc: 41.71 ng/ml

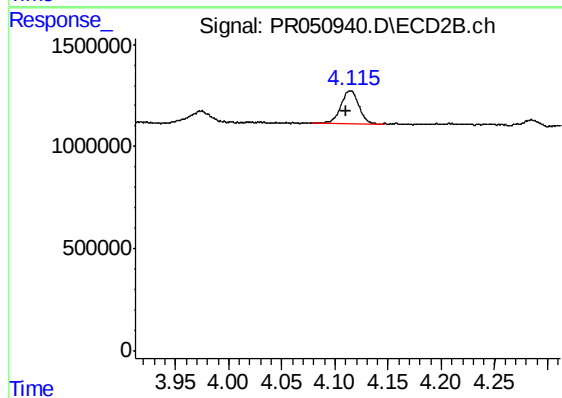

#9 AR-1221-2


R.T.: 4.115 min
Delta R.T.: 0.004 min
Response: 1900030
Conc: 38.01 ng/ml

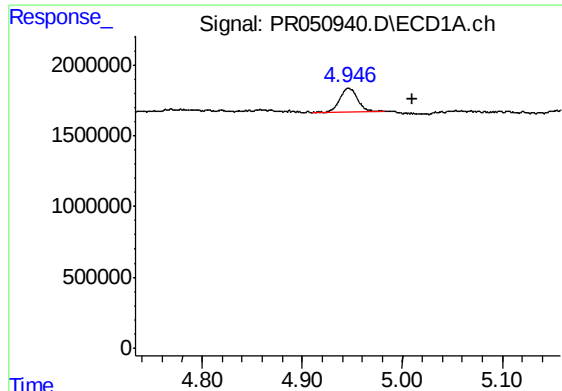

#10 AR-1221-3


R.T.: 4.946 min
Delta R.T.: -0.065 min
Response: 2119383
Conc: 12.51 ng/ml

Instrument :
ECD_R
ClientSampleId :
ABLK216

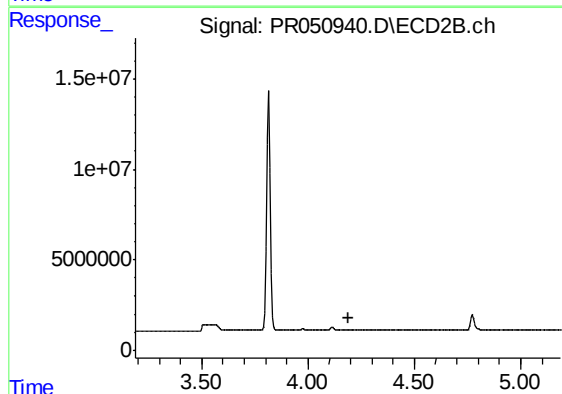


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 4.188 min
Response: 0
Conc: N.D.

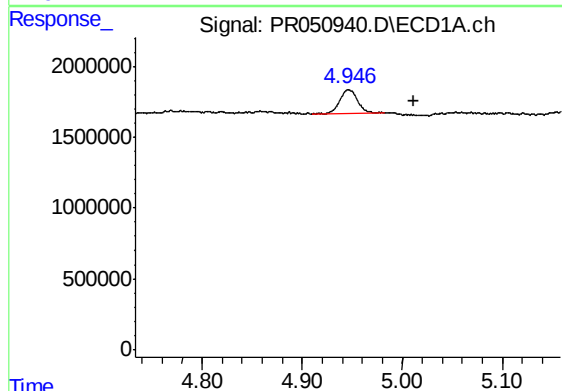


#11 AR-1232-1

R.T.: 4.946 min
Delta R.T.: -0.065 min
Response: 2119383
Conc: 15.25 ng/ml

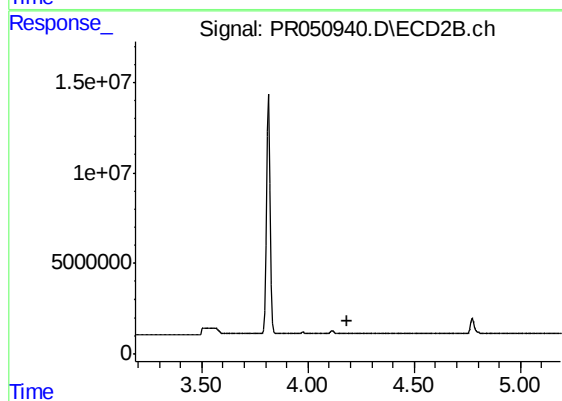

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T. : 4.188 min
Response: 0
Conc: N.D.

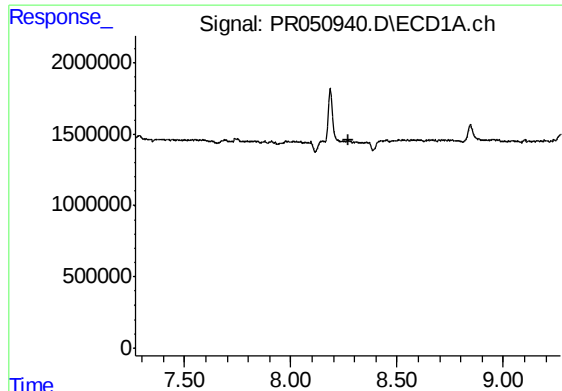

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 8.269 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
ABLK216

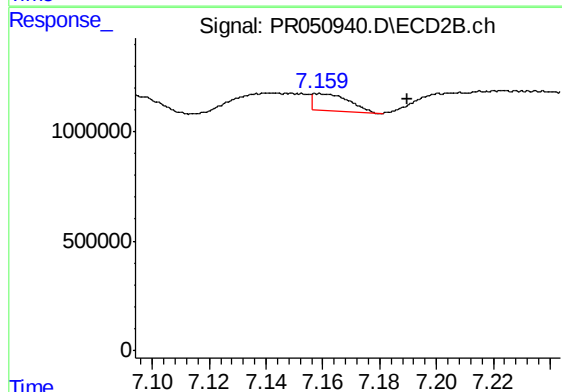


#34 AR-1260-4

R.T.: 7.159 min
Delta R.T.: -0.031 min
Response: 682045
Conc: 1.71 ng/ml

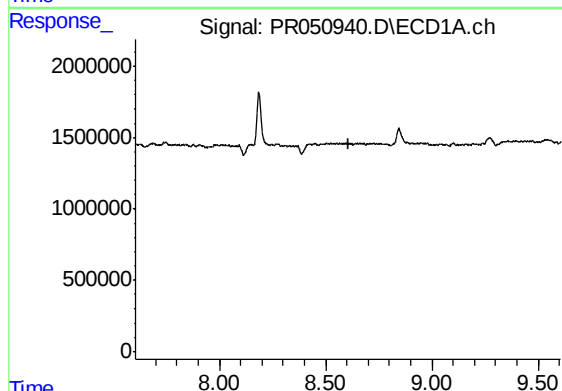


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 8.605 min
Response: 0
Conc: N.D.

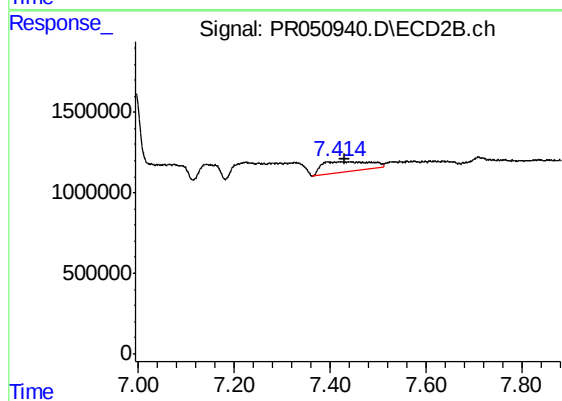

#35 AR-1260-5


R.T.: 7.419 min
Delta R.T.: -0.010 min
Response: 4685293
Conc: 4.81 ng/ml

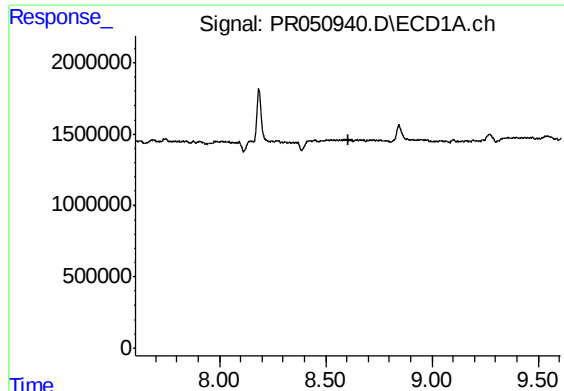

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 8.605 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
ABLK216

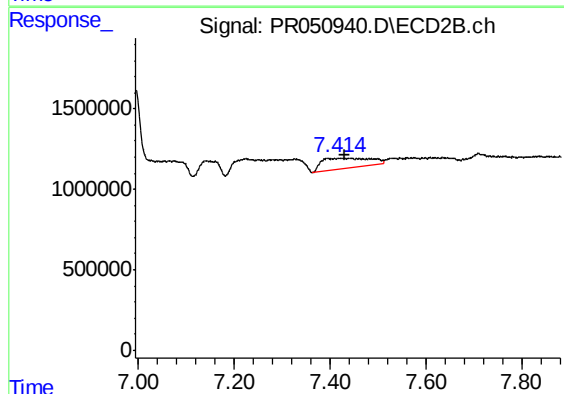


#37 AR-1262-2

R.T.: 7.419 min
Delta R.T.: -0.010 min
Response: 4685293
Conc: 3.55 ng/ml

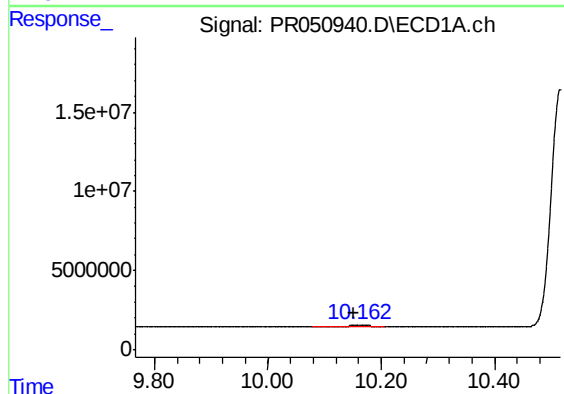

#45 AR-1268-5

R.T.: 10.162 min
Delta R.T.: 0.011 min
Response: 2220185
Conc: 0.57 ng/ml

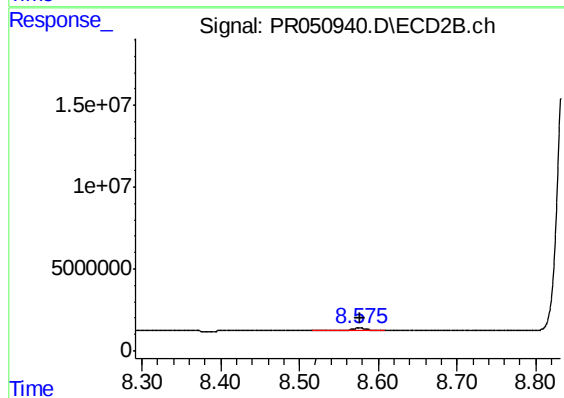

#45 AR-1268-5

R.T.: 8.576 min
Delta R.T.: 0.000 min
Response: 1937916
Conc: 0.47 ng/ml