

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062321\
 Data File : PS015924.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2021 08:49
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 01:40:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 15 18:15:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

2) T	3,5-DICHL...	6.443	0.000	240.5E6	0	107.162	N.D. #
3) T	4-Nitroph...	6.979	0.000	3572078	0	3.929	N.D. #
5) T	DICAMBA	0.000	6.985f	0	95112964	N.D.	45.838
6) T	MCP	7.629f	6.985f	16837427	95112964	3.100	57.064 #
9) T	2,4-D	8.366f	0.000	223.0E6	0	127.249	N.D. #
13) T	2,4-DB	9.990	0.000	15155378	0	7.409	N.D. #
15) T	Picloram	10.947	10.816	213.0E6	24002904	15.581	5.707 #
16) T	DCPA	11.379f	10.816	148.1E6	24002904	11.194	5.709 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062321\
Data File : PS015924.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2021 08:49
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 01:40:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
Quant Title : 8080.M
QLast Update : Tue Jun 15 18:15:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

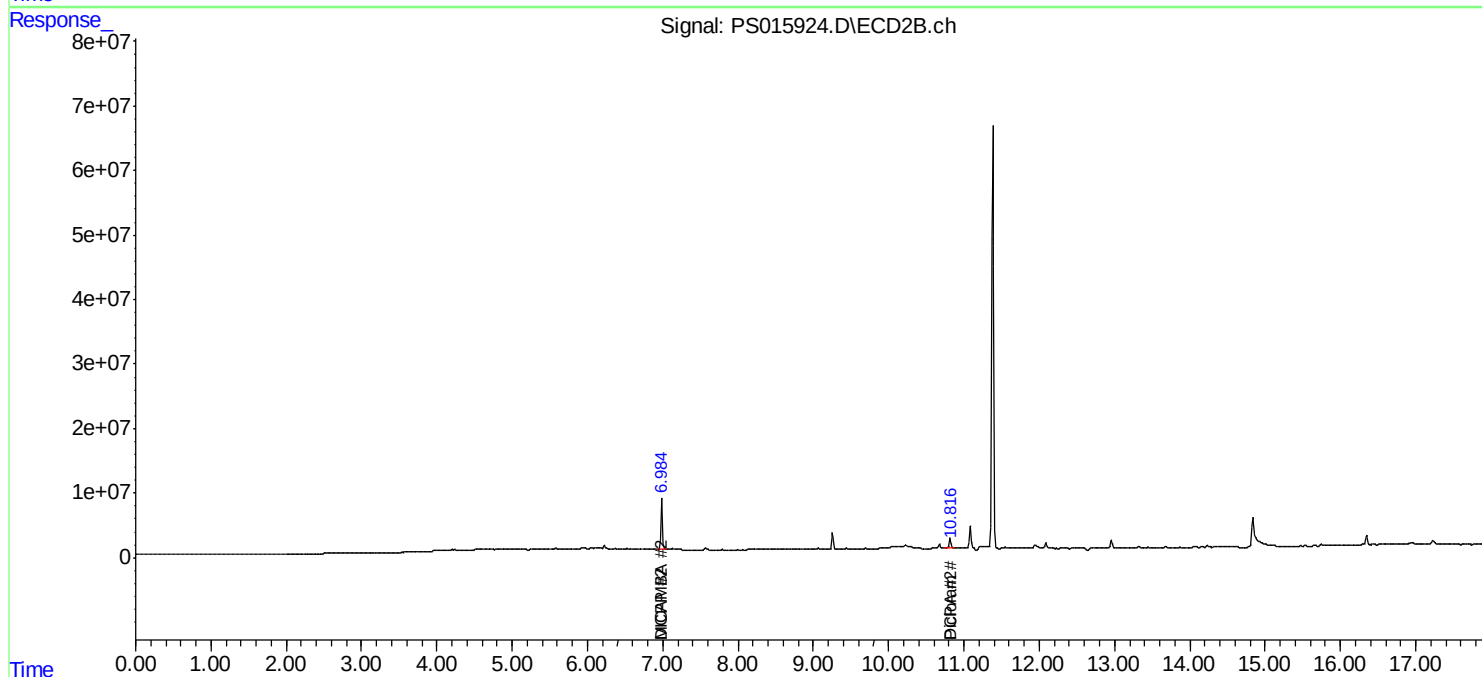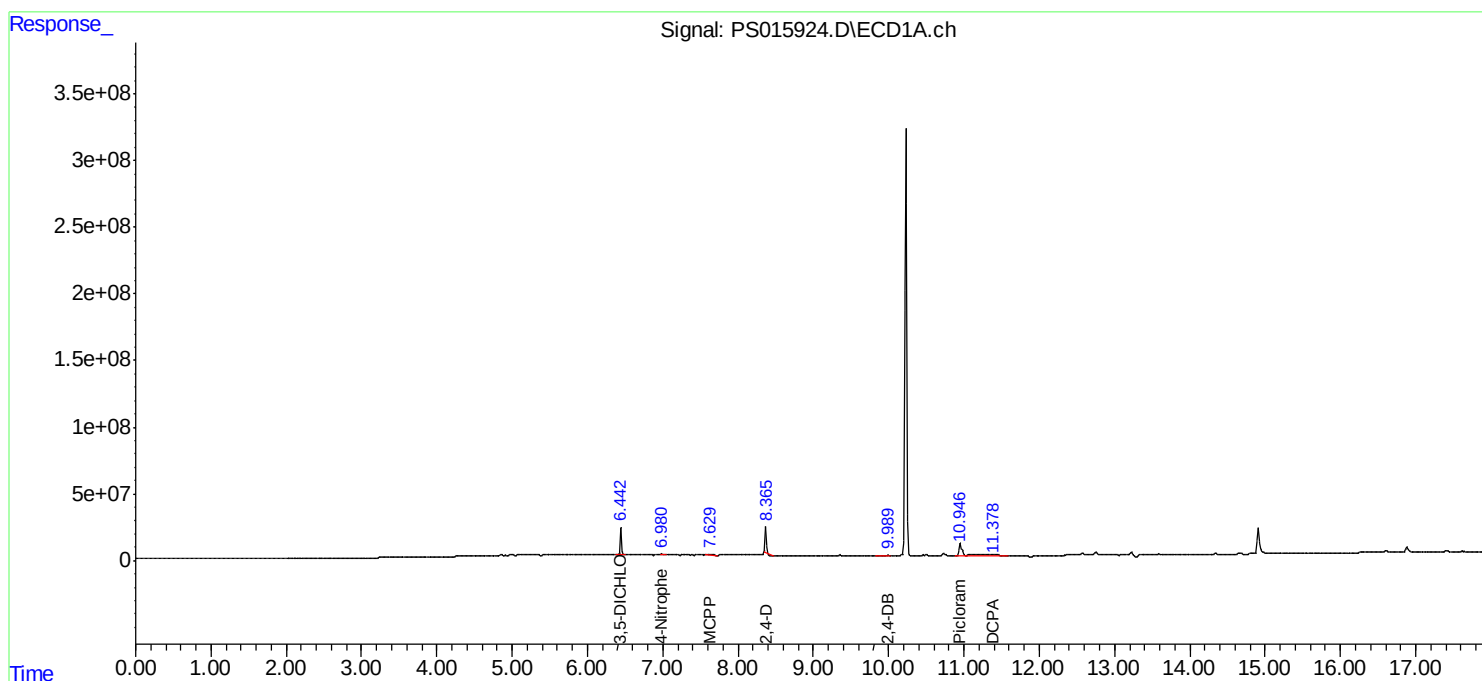


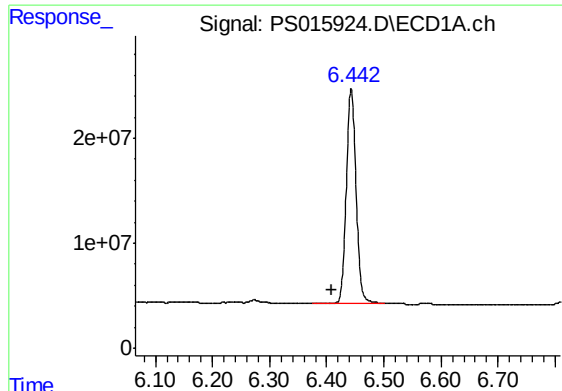

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.443 min
Delta R.T.: 0.033 min
Response: 240518101
Conc: 107.16 ng/ml

Instrument :
ECD_R
ClientSampleId :
HEXANE

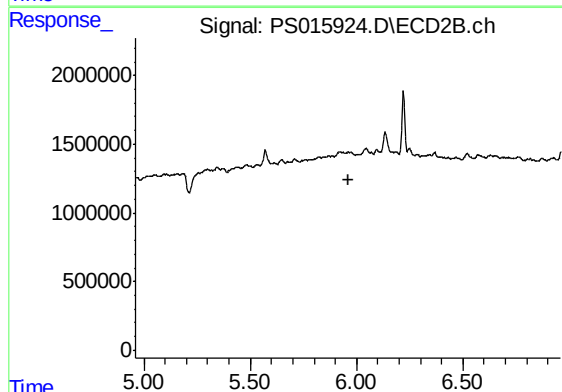


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.960 min
Response: 0
Conc: N.D.

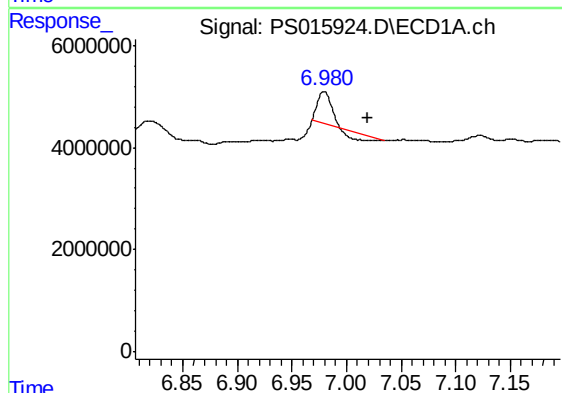


#3 4-Nitrophenol

R.T.: 6.979 min
Delta R.T.: -0.040 min
Response: 3572078
Conc: 3.93 ng/ml

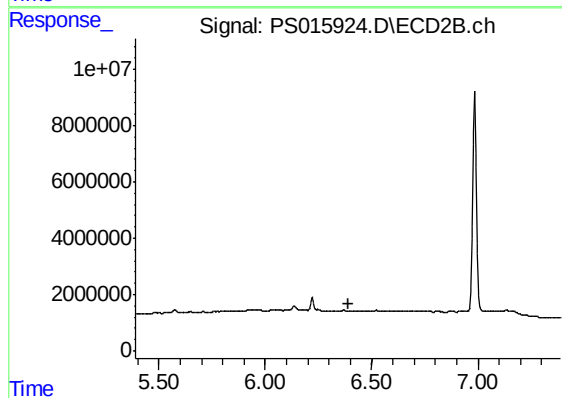

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.389 min
Response: 0
Conc: N.D.

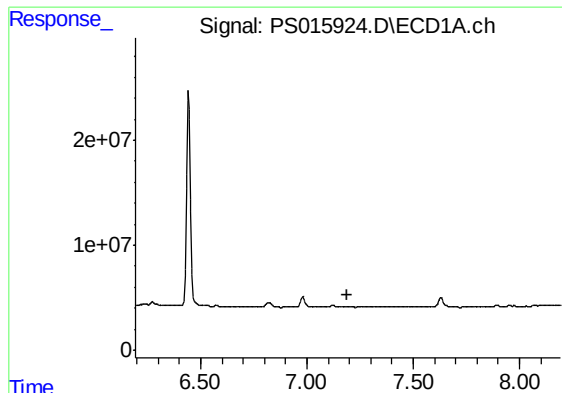

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 7.193 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
HEXANE

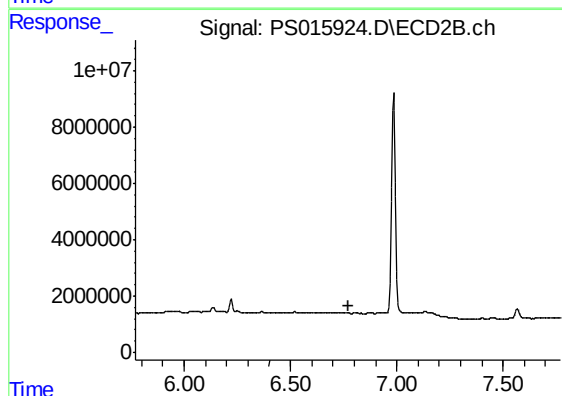


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.771 min
Response: 0
Conc: N.D.

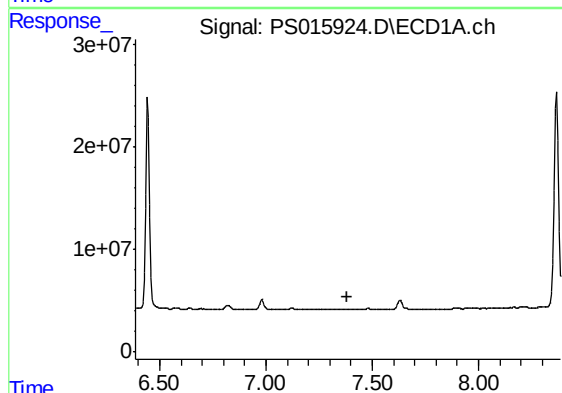


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.385 min
Response: 0
Conc: N.D.

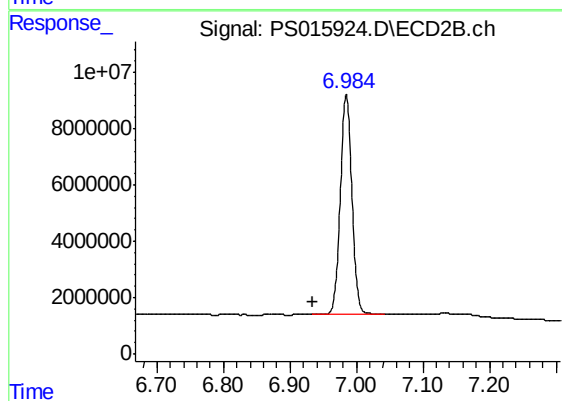

#5 DICAMBA


R.T.: 6.985 min
Delta R.T.: 0.050 min
Response: 95112964
Conc: 45.84 ng/ml

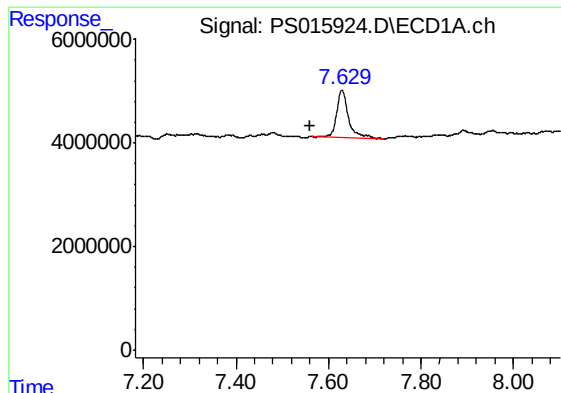

#6 MCPP


R.T.: 7.629 min
Delta R.T.: 0.068 min
Response: 16837427
Conc: 3.10 ug/ml

Instrument :
ECD_R
ClientSampleId :
HEXANE

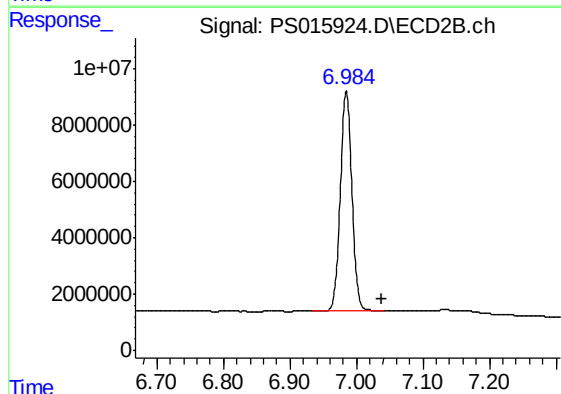


#6 MCPP

R.T.: 6.985 min
Delta R.T.: -0.054 min
Response: 95112964
Conc: 57.06 ug/ml

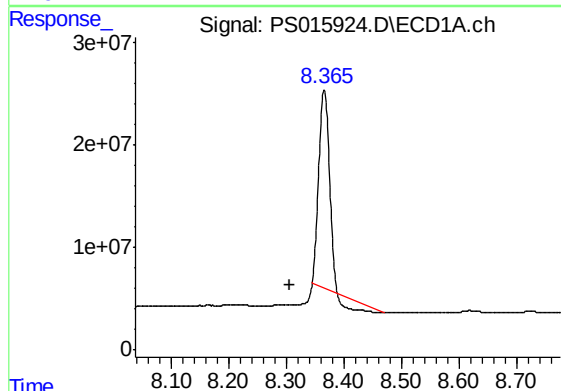


#9 2,4-D

R.T.: 8.366 min
Delta R.T.: 0.061 min
Response: 223012090
Conc: 127.25 ng/ml

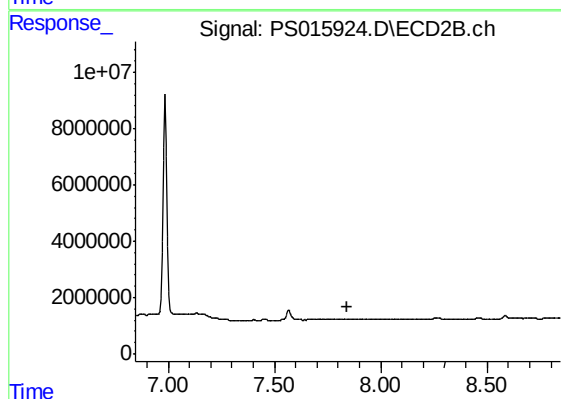

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.845 min
Response: 0
Conc: N.D.

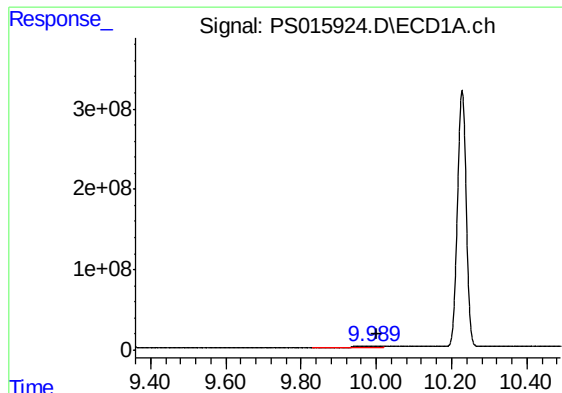

#13 2,4-DB


R.T.: 9.990 min
Delta R.T.: -0.010 min
Response: 15155378
Conc: 7.41 ng/ml

Instrument :
ECD_R
ClientSampleId :
HEXANE

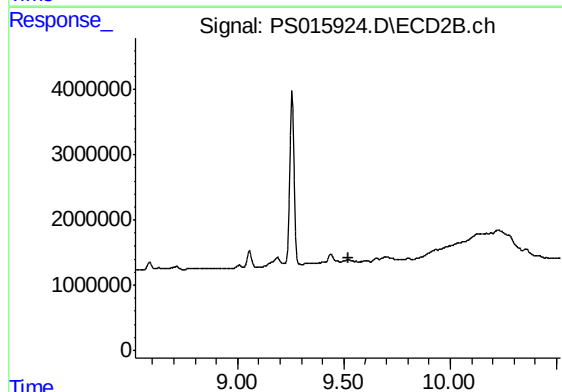


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.519 min
Response: 0
Conc: N.D.

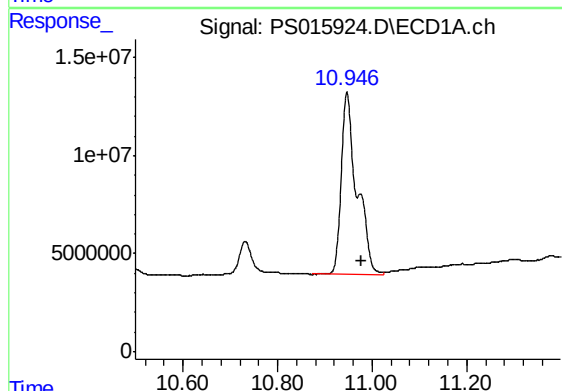


#15 Picloram

R.T.: 10.947 min
Delta R.T.: -0.031 min
Response: 213000871
Conc: 15.58 ng/ml

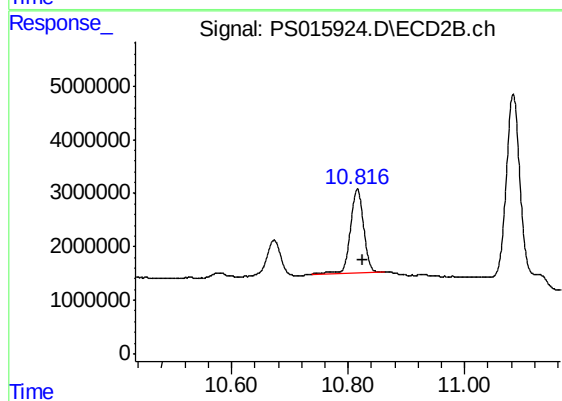

#15 Picloram


R.T.: 10.816 min
Delta R.T.: -0.008 min
Response: 24002904
Conc: 5.71 ng/ml

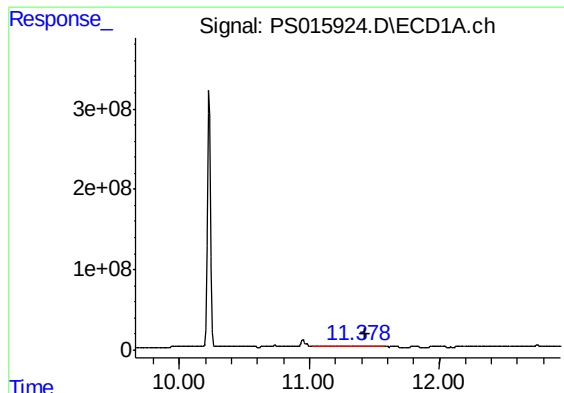

#16 DCPA

R.T.: 11.379 min
Delta R.T.: -0.051 min
Response: 148058546
Conc: 11.19 ng/ml

Instrument :
ECD_R
ClientSampleId :
HEXANE

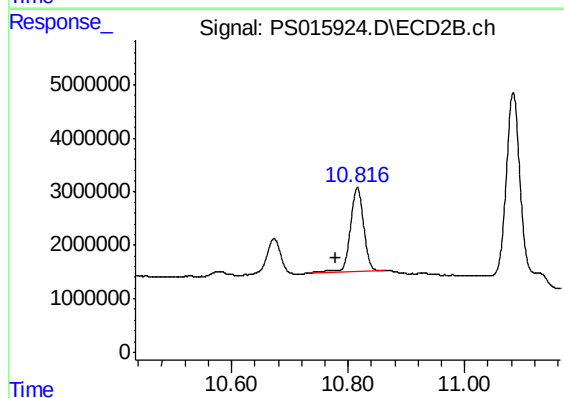

#16 DCPA

R.T.: 10.816 min
Delta R.T.: 0.037 min
Response: 24002904
Conc: 5.71 ng/ml