

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062321\
 Data File : PS015925.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2021 09:13
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 01:41:00 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 15 18:15:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.189	6.765	803.2E6	291.3E6	483.437	578.054
Target Compounds							
9) T	2,4-D	8.374f	0.000	13556674	0	7.735	N.D. #
15) T	Picloram	10.979	10.820	36623602	13984281	2.679	3.325
16) T	DCPA	0.000	10.820f	0	13984281	N.D.	3.326



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062321\
Data File : PS015925.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2021 09:13
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 01:41:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
Quant Title : 8080.M
QLast Update : Tue Jun 15 18:15:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

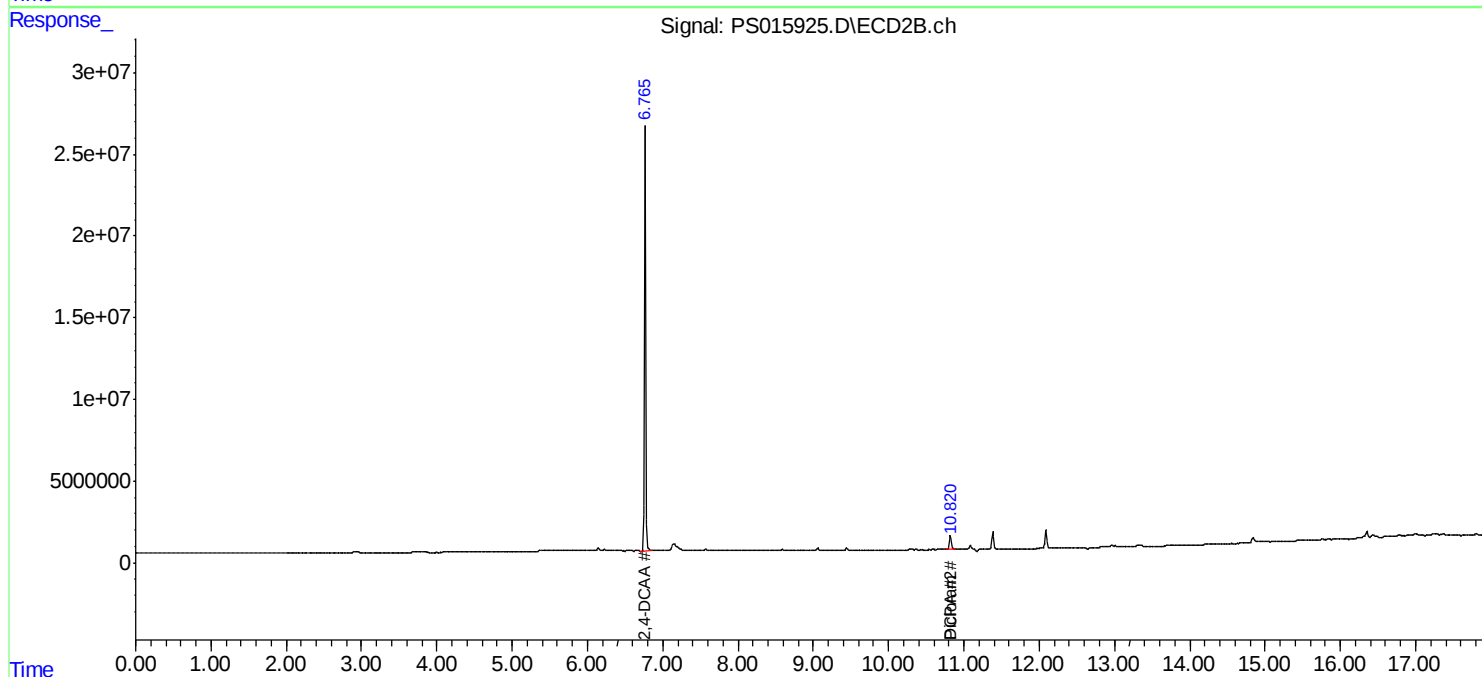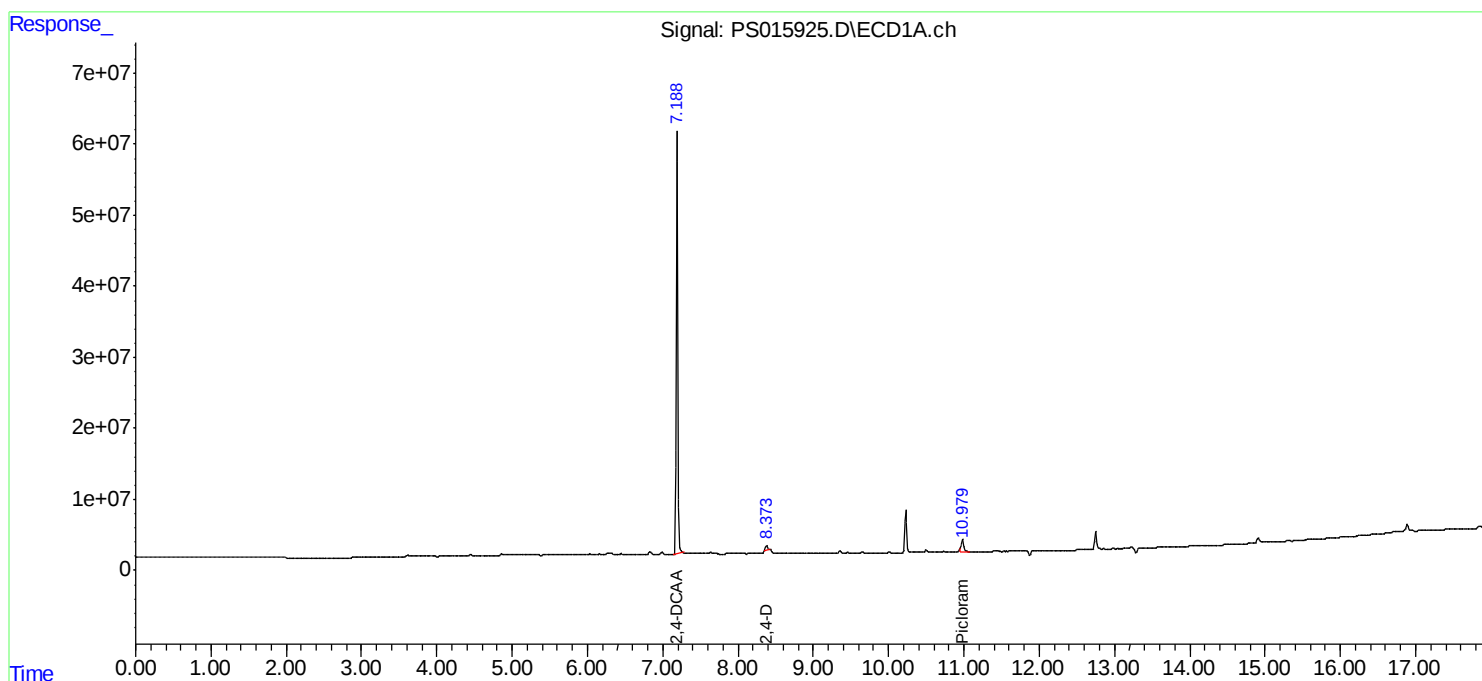


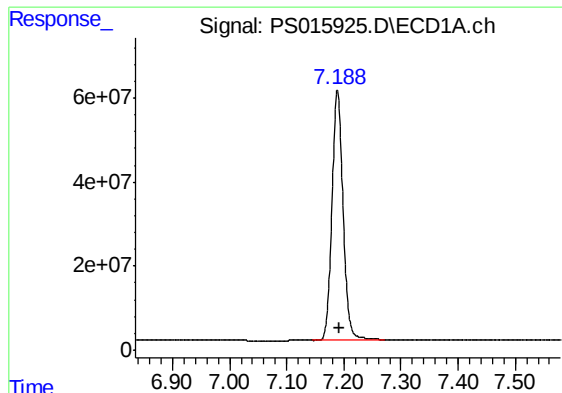

#4 2,4-DCAA


R.T.: 7.189 min
Delta R.T.: -0.004 min
Response: 803204457
Conc: 483.44 ng/ml

Instrument :
ECD_R
ClientSampleId :
I.BLK

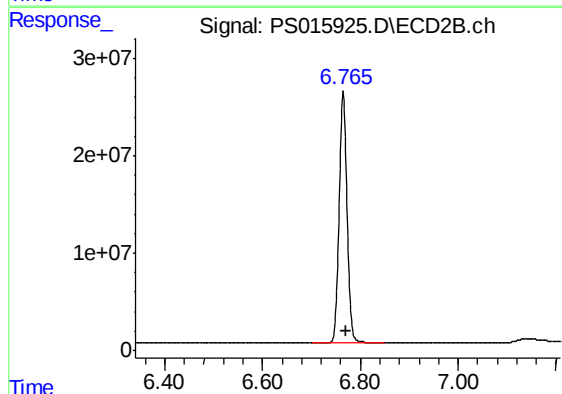


#4 2,4-DCAA

R.T.: 6.765 min
Delta R.T.: -0.006 min
Response: 291253468
Conc: 578.05 ng/ml

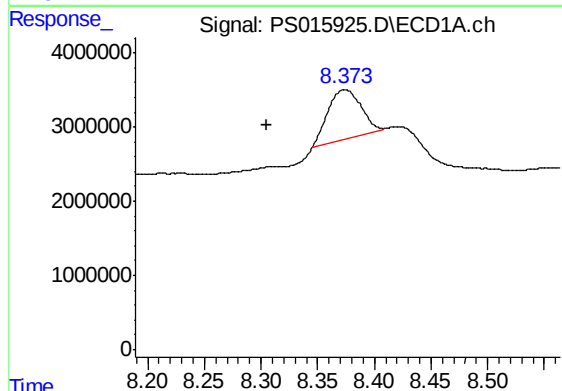


#9 2,4-D

R.T.: 8.374 min
Delta R.T.: 0.069 min
Response: 13556674
Conc: 7.74 ng/ml

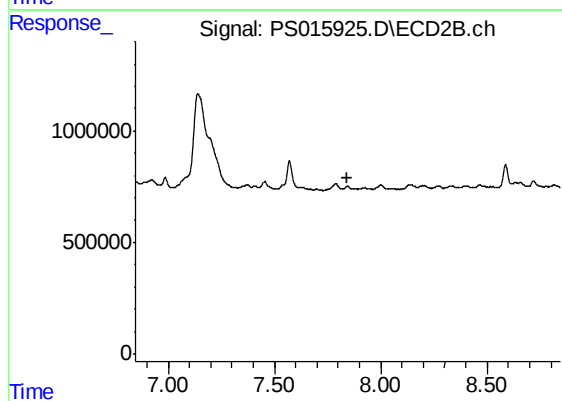

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.845 min
Response: 0
Conc: N.D.

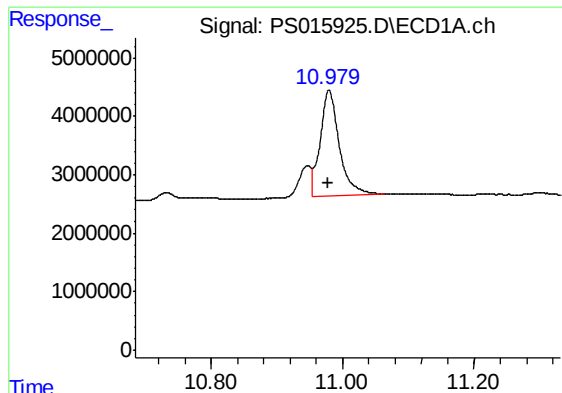

#15 Picloram


R.T.: 10.979 min
Delta R.T.: 0.001 min
Response: 36623602
Conc: 2.68 ng/ml

Instrument :
ECD_R
ClientSampleId :
I.BLK

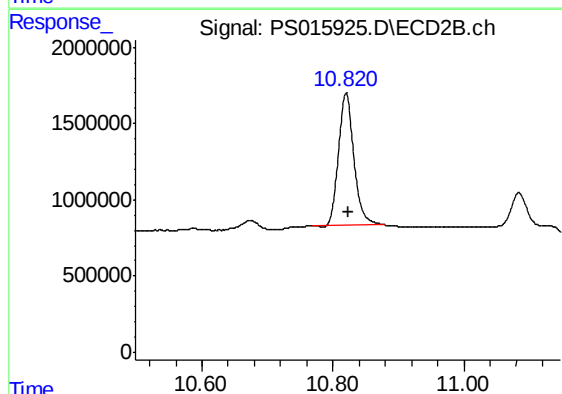


#15 Picloram

R.T.: 10.820 min
Delta R.T.: -0.004 min
Response: 13984281
Conc: 3.33 ng/ml

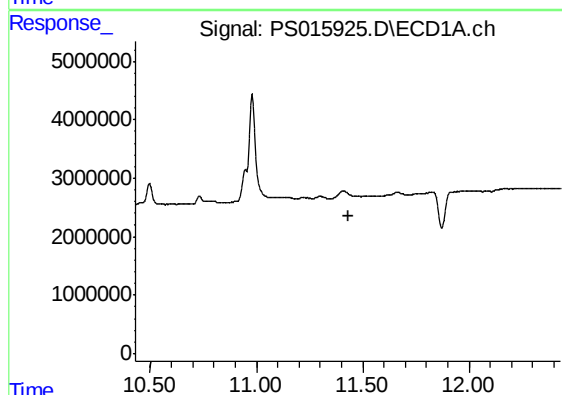

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.431 min
Response: 0
Conc: N.D.

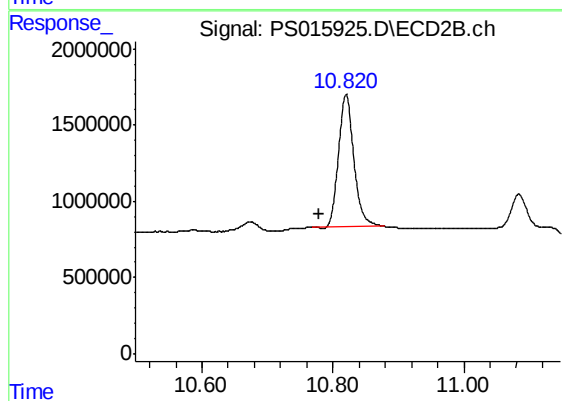

#16 DCPA

R.T.: 10.820 min
Delta R.T.: 0.042 min
Response: 13984281
Conc: 3.33 ng/ml