

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR062418\
 Data File : PR029273.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2018 15:08
 Operator : UA/SM
 Sample : J3508-01RE
 Misc :
 ALS Vial : 115 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 KGS-SIDE-1RE

Manual Integrations
 APPROVED

UGO
 6/21/2018 2:45:25 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 15:22:29 2018
 Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_R\Method\PR062418.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jun 19 13:41:09 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.579	3.728	359.4E6	857.9E6	14.457m	20.237 #
2)	SA Decachlor...	10.353	8.666	269.7E6	218.5E6	9.728	9.615m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR062418\
Data File : PR029273.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2018 15:08
Operator : UA/SM
Sample : J3508-01RE
Misc :
ALS Vial : 115 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
KGS-SIDE-1RE


Manual Integrations
APPROVED

UGO
6/21/2018 2:45:25 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 15:22:29 2018
Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_R\Method\PR062418.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 19 13:41:09 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

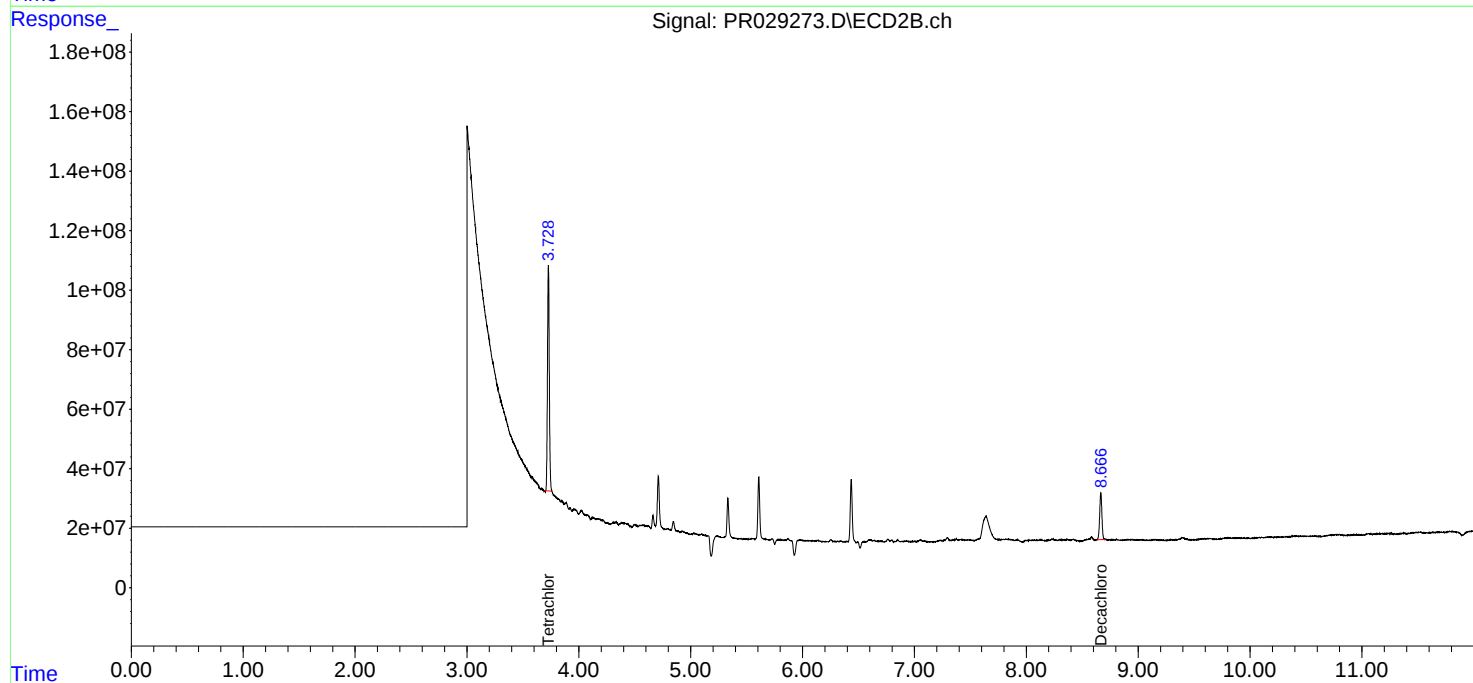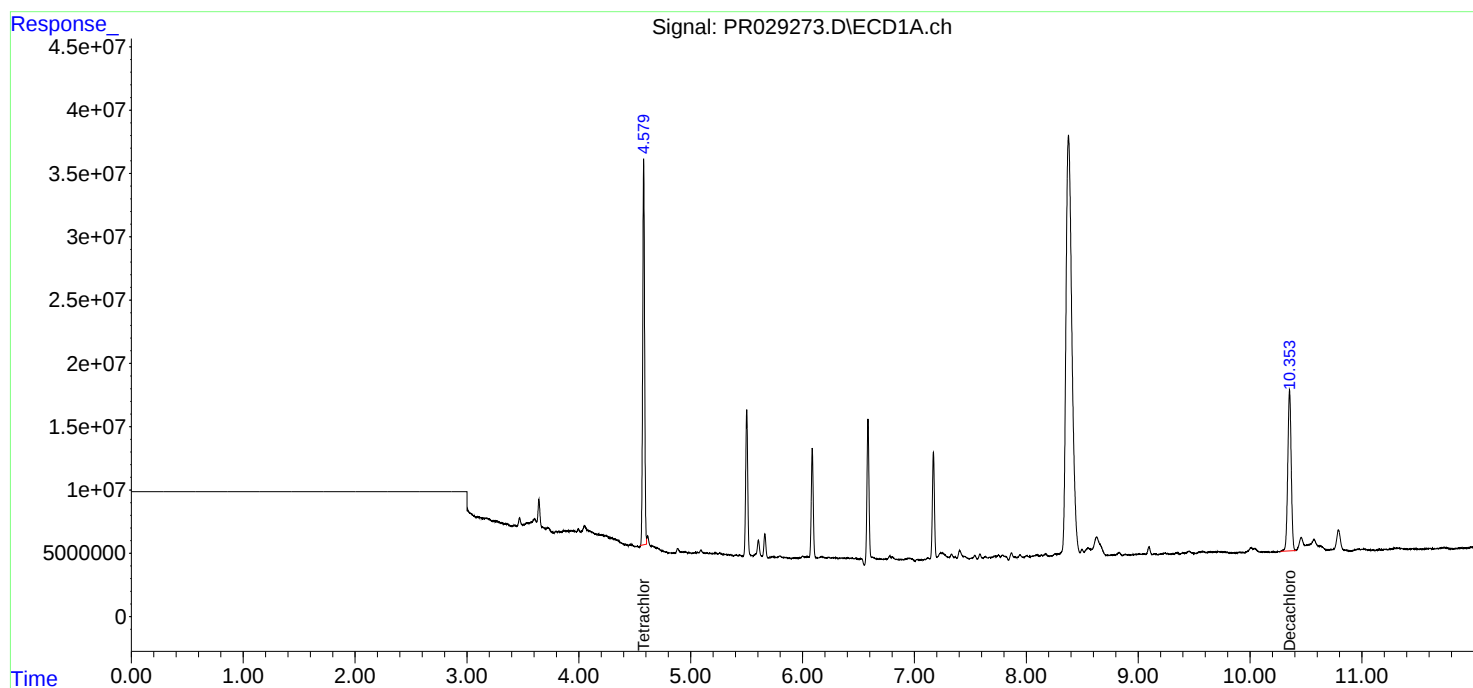

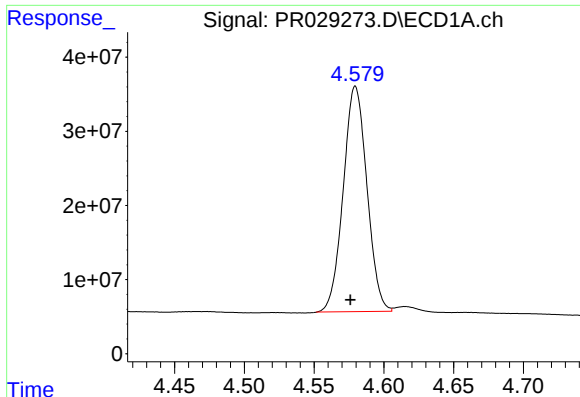


#1 Tetrachloro-m-xylene

R.T.: 4.579 min
Delta R.T.: 0.003 min
Response: 359424127
Conc: 14.46 ng/ml m

Instrument :
ECD_R
ClientSampleId :
KGS-SIDE-1RE


Manual Integrations
APPROVED

UGO
6/21/2018 2:45:25 PM

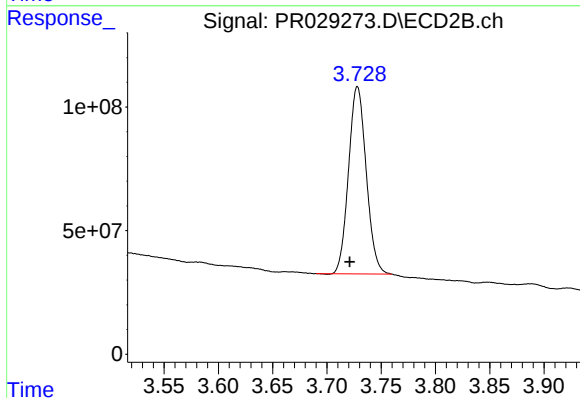


#1 Tetrachloro-m-xylene

R.T.: 3.728 min
Delta R.T.: 0.007 min
Response: 857943907
Conc: 20.24 ng/ml

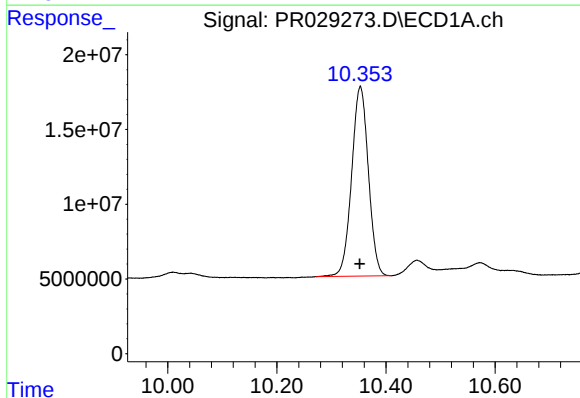

#2 Decachlorobiphenyl

R.T.: 10.353 min
Delta R.T.: 0.001 min
Response: 269664542
Conc: 9.73 ng/ml

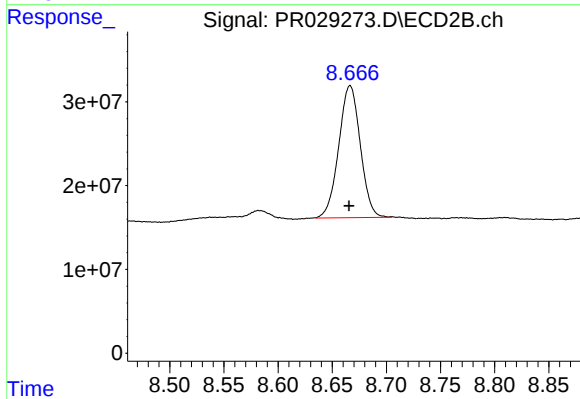

#2 Decachlorobiphenyl

R.T.: 8.666 min
Delta R.T.: 0.000 min
Response: 218464188
Conc: 9.62 ng/ml m