

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR062418\
 Data File : PR029274.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2018 15:22
 Operator : UA/SM
 Sample : J3508-04
 Misc :
 ALS Vial : 116 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 KGS-SIDE-2-3

Manual Integrations
 APPROVED

UGO
 6/21/2018 2:45:29 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 15:43:35 2018
 Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_R\Method\PR062418.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jun 19 13:41:09 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.578	3.727	467.0E6	944.5E6	18.785	22.279
2) SA Decachlor...	10.351	8.665	224.7E6	208.0E6	8.106	9.155m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR062418\
Data File : PR029274.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2018 15:22
Operator : UA/SM
Sample : J3508-04
Misc :
ALS Vial : 116 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
KGS-SIDE-2-3


Manual Integrations
APPROVED

UGO
6/21/2018 2:45:29 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 15:43:35 2018
Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_R\Method\PR062418.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 19 13:41:09 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

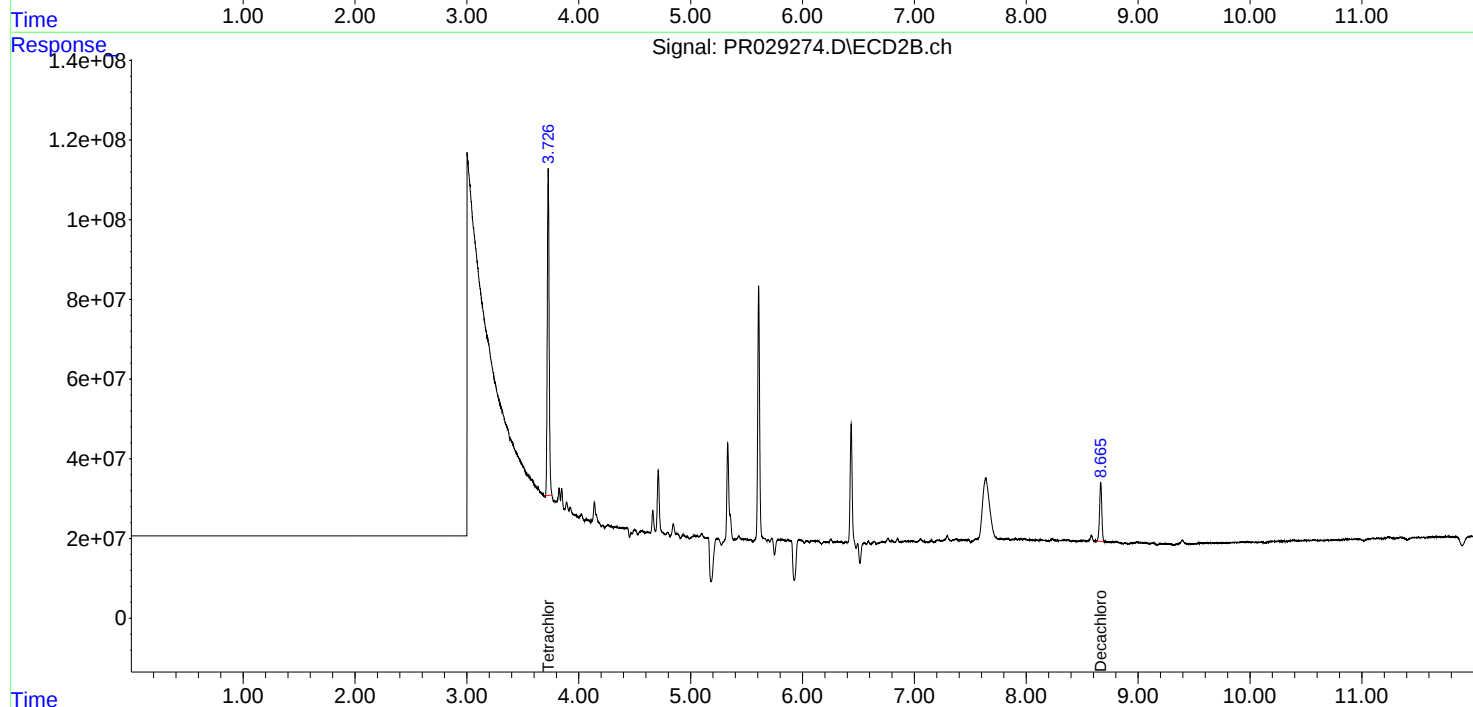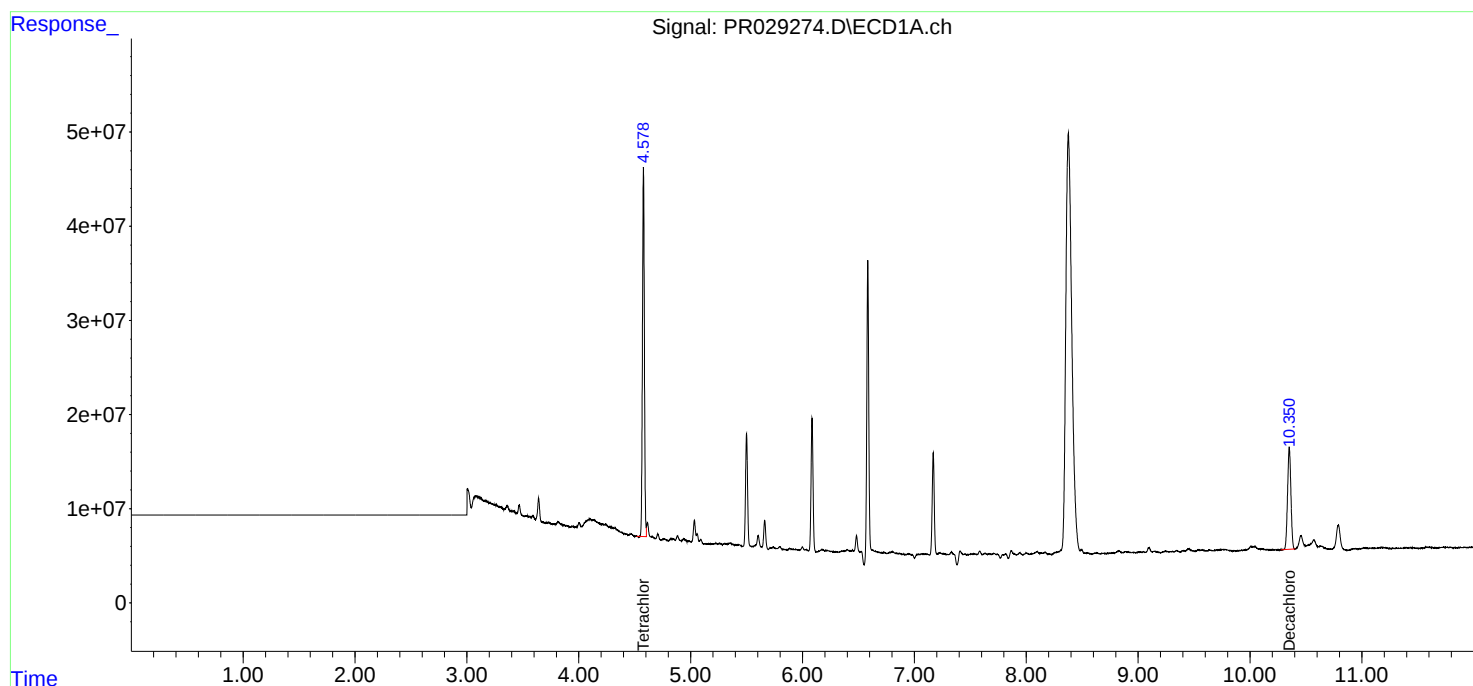

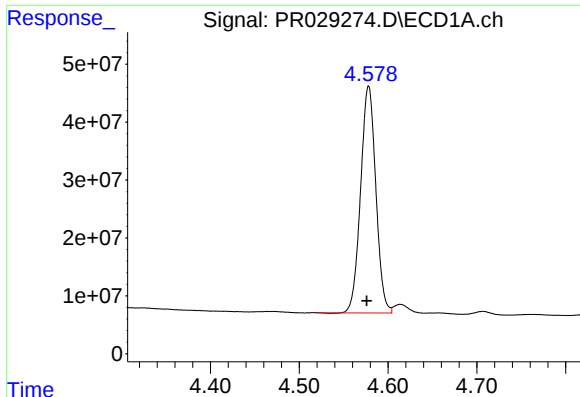


#1 Tetrachloro-m-xylene

R.T.: 4.578 min
Delta R.T.: 0.002 min
Response: 467035981
Conc: 18.78 ng/ml

Instrument :
ECD_R
ClientSampleId :
KGS-SIDE-2-3


Manual Integrations
APPROVED

UGO
6/21/2018 2:45:29 PM

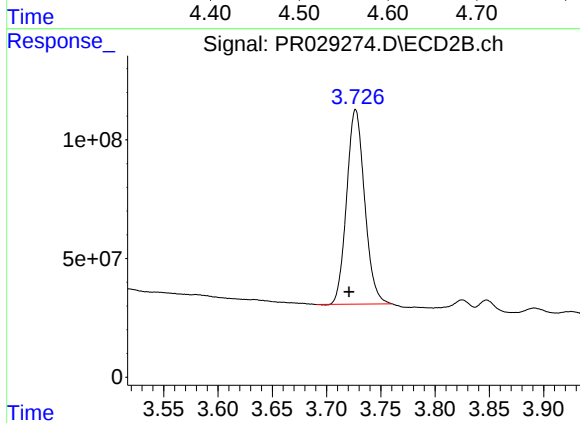


#1 Tetrachloro-m-xylene

R.T.: 3.727 min
Delta R.T.: 0.006 min
Response: 944538935
Conc: 22.28 ng/ml

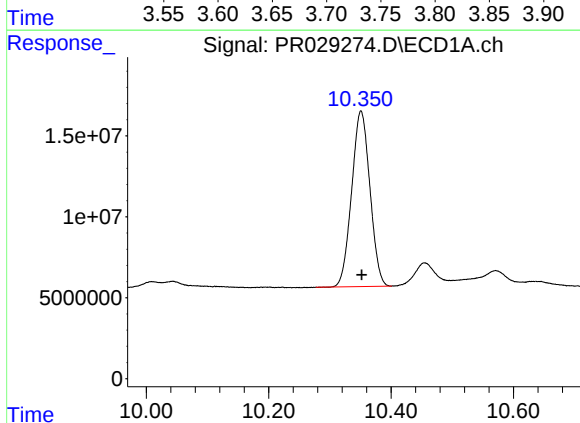

#2 Decachlorobiphenyl

R.T.: 10.351 min
Delta R.T.: -0.001 min
Response: 224696308
Conc: 8.11 ng/ml

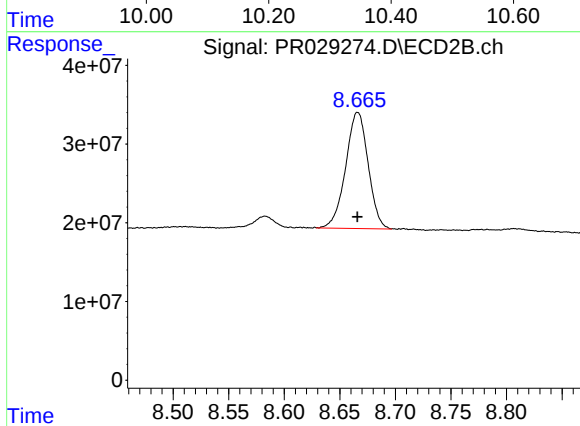

#2 Decachlorobiphenyl

R.T.: 8.665 min
Delta R.T.: 0.000 min
Response: 208016385
Conc: 9.16 ng/ml m