

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR062722\
 Data File : PR055014.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2022 00:08
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/28/2022
 Supervised By :Ankita Jodhani 06/28/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 03:03:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR062722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 27 17:05:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.640	2.912	93468274	42358013	25.697	25.373
2) SA Decachlor...	9.532	8.139	40897761	38810179	28.363	27.622m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR062722\
Data File : PR055014.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2022 00:08
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/28/2022
Supervised By :Ankita Jodhani 06/28/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 03:03:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR062722.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 27 17:05:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

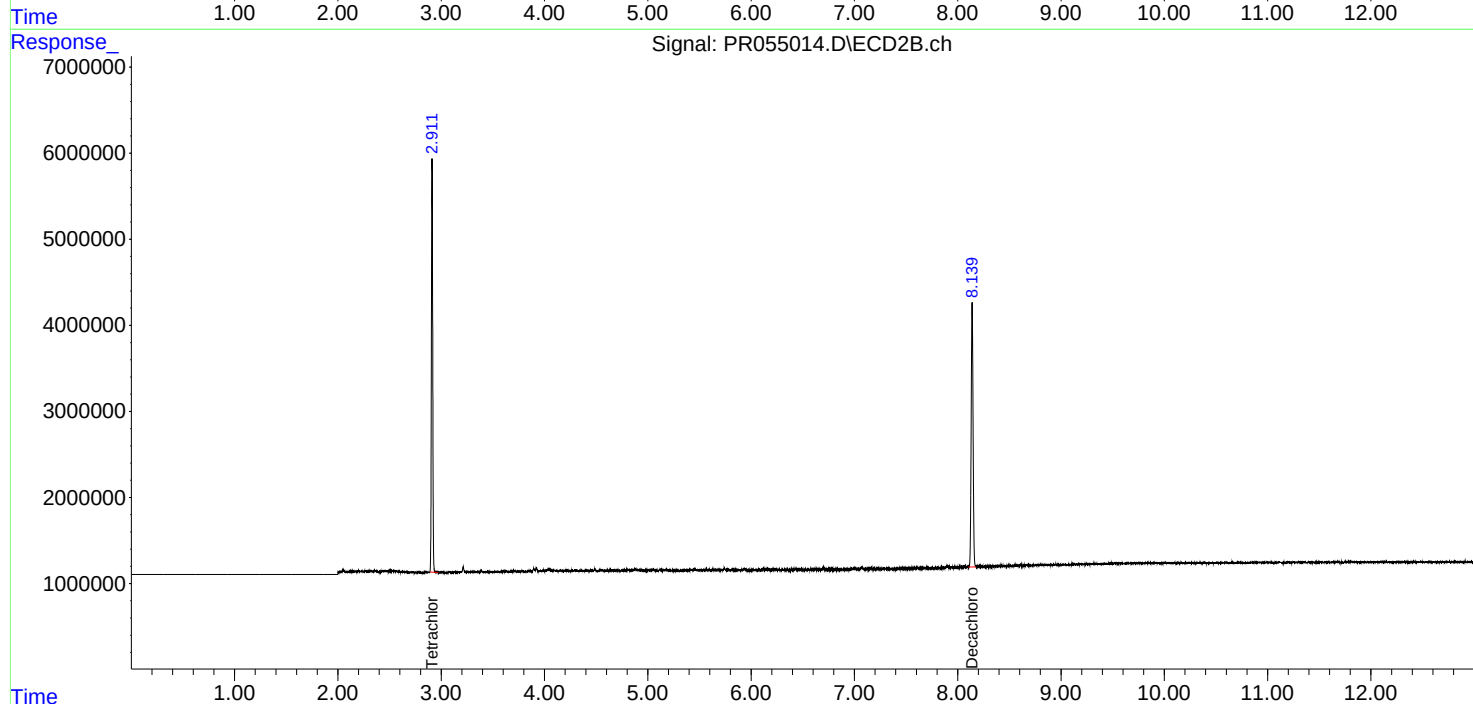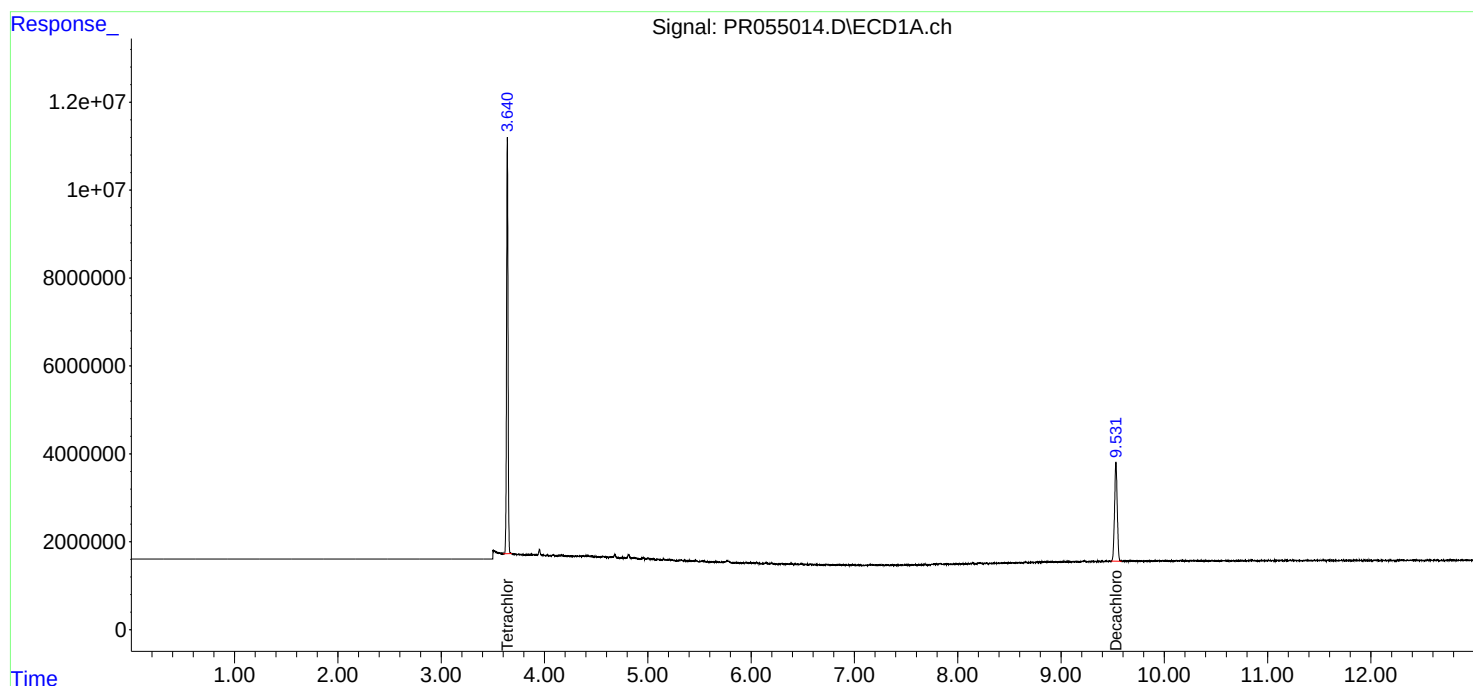

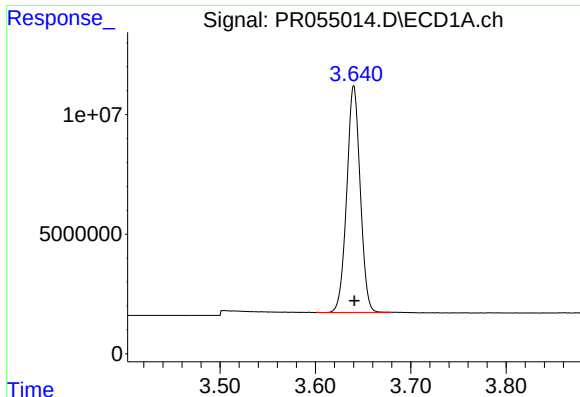


#1 Tetrachloro-m-xylene

R.T.: 3.640 min
Delta R.T.: 0.000 min
Response: 93468274
Conc: 25.70 ng/ml

Instrument :
ECD_R
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/28/2022
Supervised By :Ankita Jodhani 06/28/2022

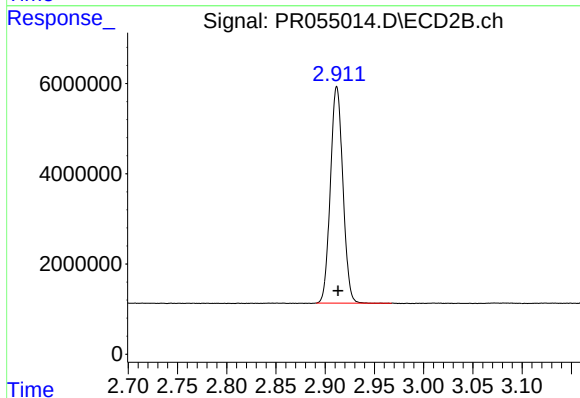


#1 Tetrachloro-m-xylene

R.T.: 2.912 min
Delta R.T.: -0.001 min
Response: 42358013
Conc: 25.37 ng/ml

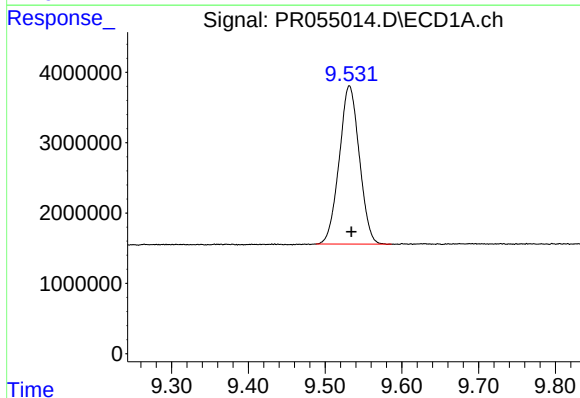

#2 Decachlorobiphenyl

R.T.: 9.532 min
Delta R.T.: -0.002 min
Response: 40897761
Conc: 28.36 ng/ml

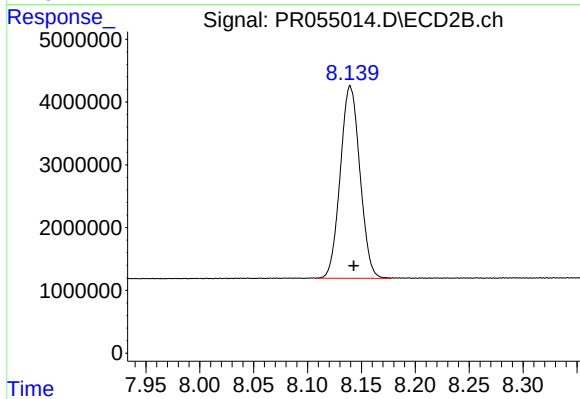

#2 Decachlorobiphenyl

R.T.: 8.139 min
Delta R.T.: -0.004 min
Response: 38810179
Conc: 27.62 ng/ml m