

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR062722\
 Data File : PR055031.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2022 05:49
 Operator : AJ\MA
 Sample : N3472-03 10X
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 D2560

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/28/2022
 Supervised By :Ankita Jodhani 06/28/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 06:37:25 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR062722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 27 17:05:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.646	2.912	7798041	1822307	2.144m	1.092 #
2) SA Decachlor...	9.532	8.139	2216129	2025871	1.537	1.442m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR062722\
Data File : PR055031.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2022 05:49
Operator : AJ\MA
Sample : N3472-03 10X
Misc :
ALS Vial : 52 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
D2560


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/28/2022
Supervised By :Ankita Jodhani 06/28/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 06:37:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR062722.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 27 17:05:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

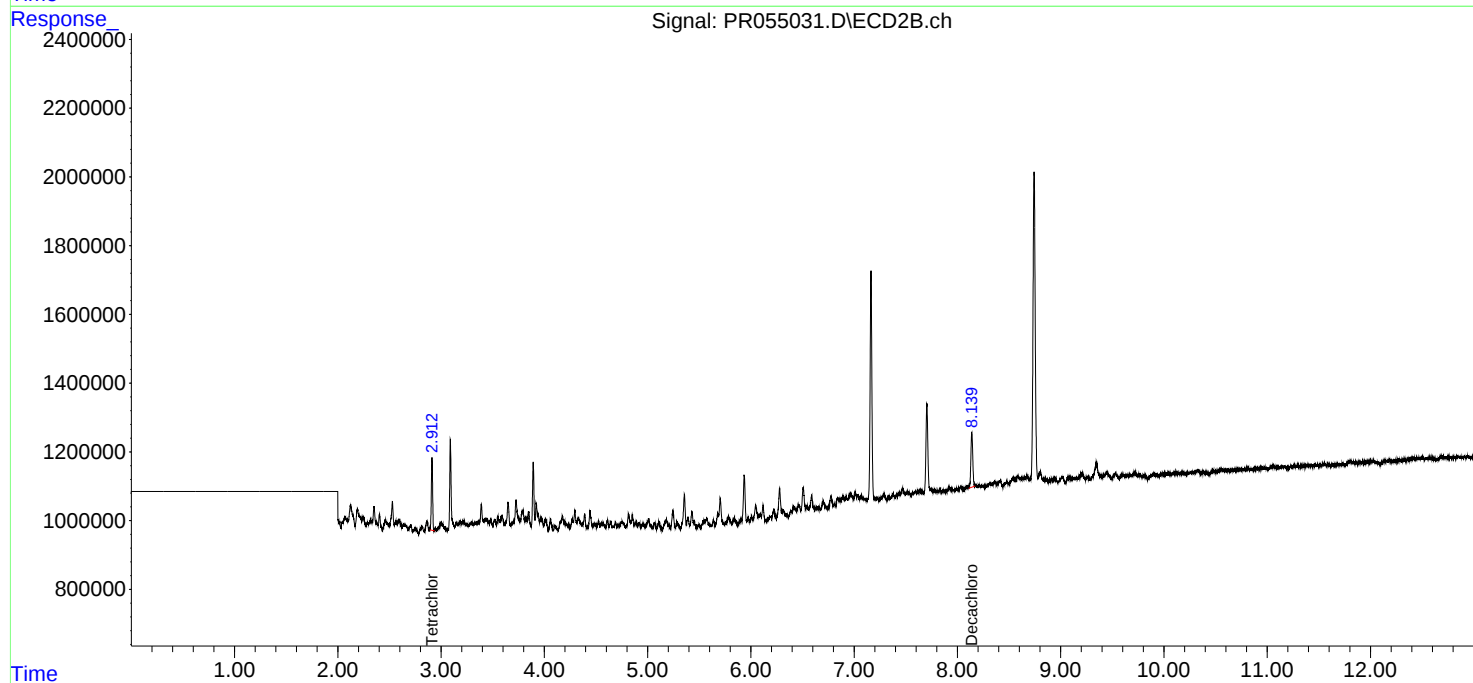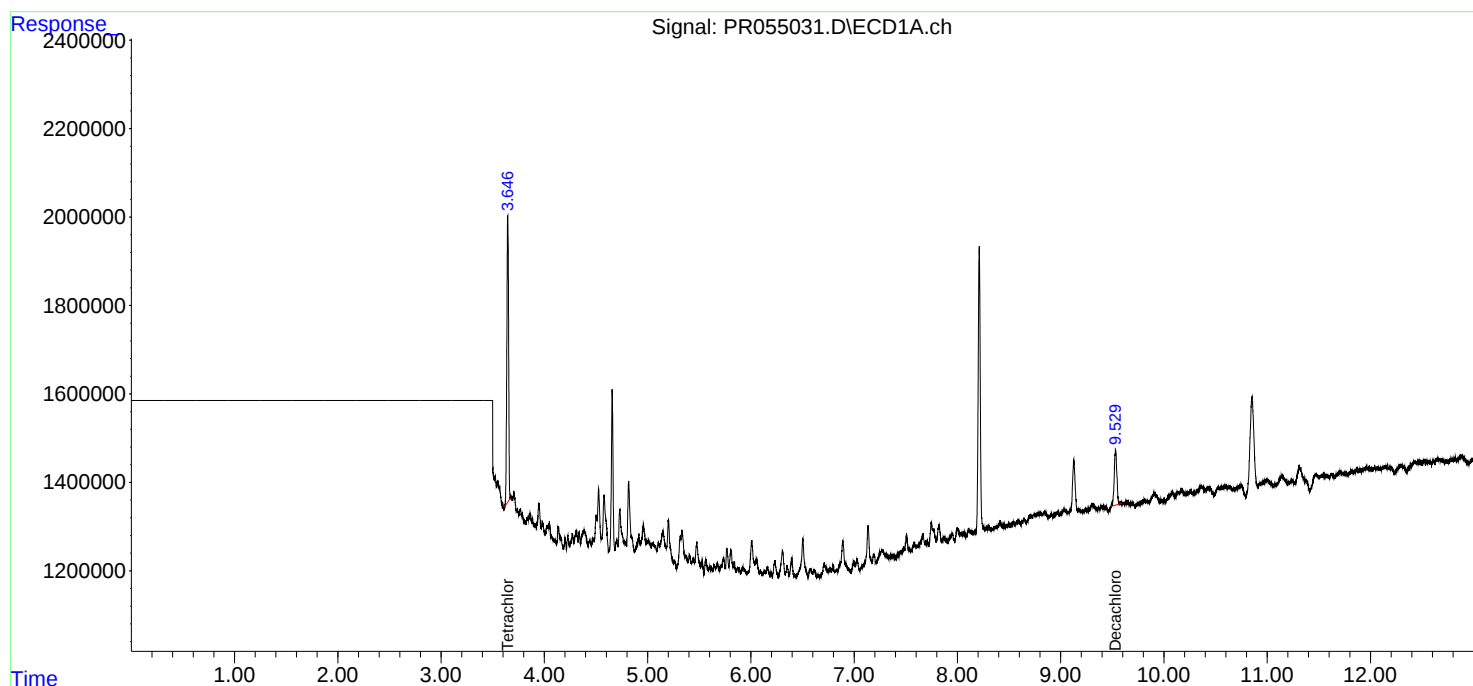

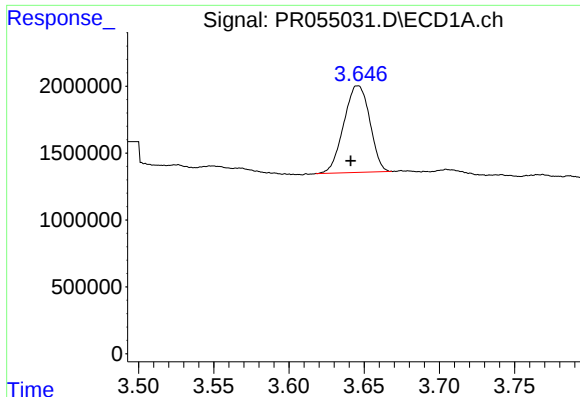


#1 Tetrachloro-m-xylene

R.T.: 3.646 min
Delta R.T.: 0.005 min
Response: 7798041
Conc: 2.14 ng/ml

Instrument :
ECD_R
ClientSampleId :
D2560


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/28/2022
Supervised By :Ankita Jodhani 06/28/2022

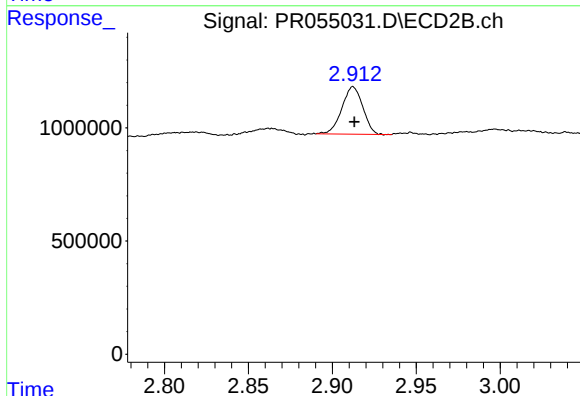


#1 Tetrachloro-m-xylene

R.T.: 2.912 min
Delta R.T.: 0.000 min
Response: 1822307
Conc: 1.09 ng/ml

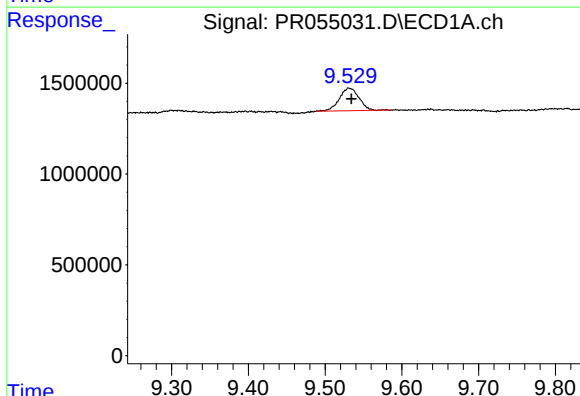

#2 Decachlorobiphenyl

R.T.: 9.532 min
Delta R.T.: -0.002 min
Response: 2216129
Conc: 1.54 ng/ml

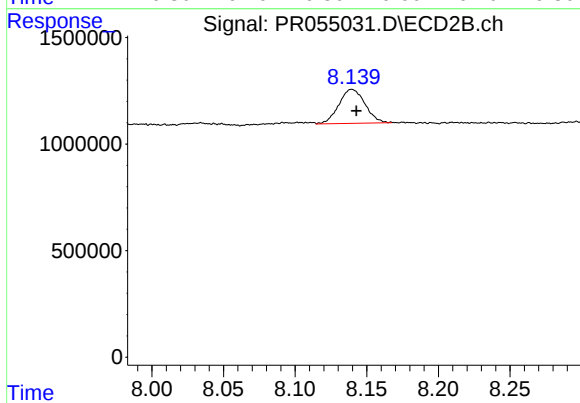

#2 Decachlorobiphenyl

R.T.: 8.139 min
Delta R.T.: -0.004 min
Response: 2025871
Conc: 1.44 ng/ml m