

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR062722\
 Data File : PR055047.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2022 11:00
 Operator : AJ\MA
 Sample : N3472-06
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 D2559

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/28/2022
 Supervised By :Ankita Jodhani 06/28/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 11:30:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR062722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 27 17:05:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.644	2.917	51896419	28042792	14.268m	16.798
2) SA Decachlor...	9.547	8.158	13608413	13248457	9.438	9.429

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR062722\
Data File : PR055047.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2022 11:00
Operator : AJ\MA
Sample : N3472-06
Misc :
ALS Vial : 65 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
D2559


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/28/2022
Supervised By :Ankita Jodhani 06/28/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 11:30:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR062722.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 27 17:05:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

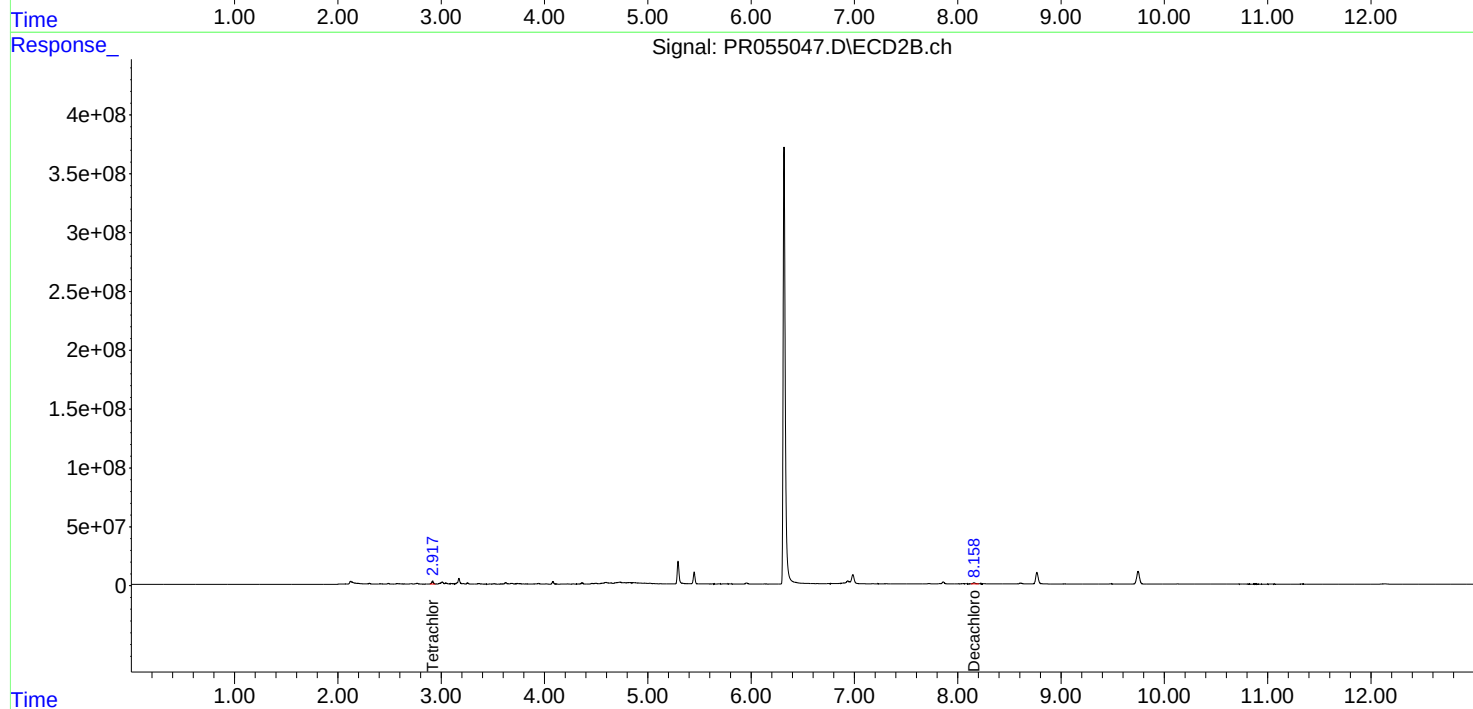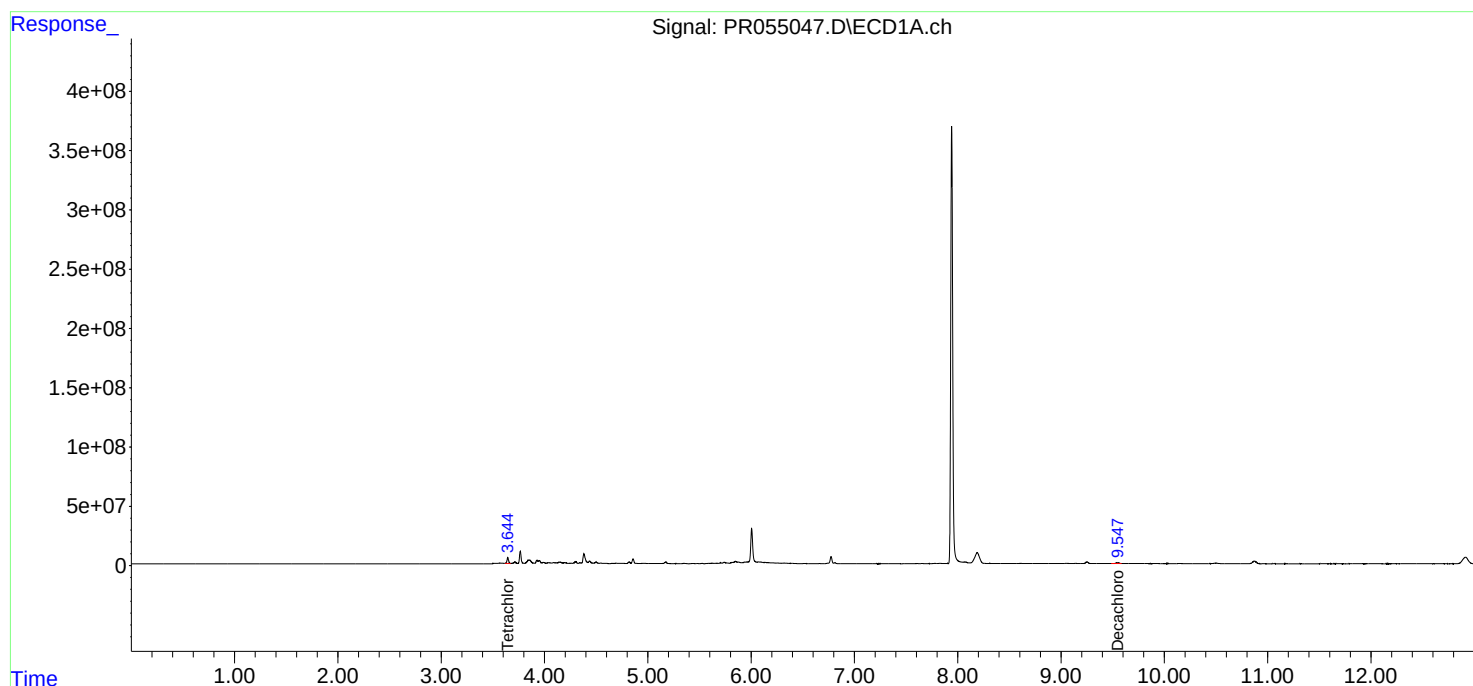

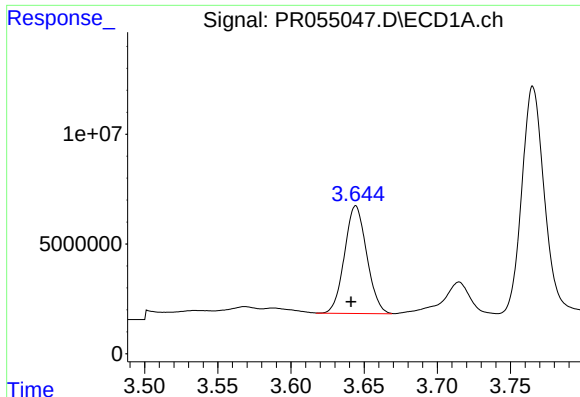


#1 Tetrachloro-m-xylene

R.T.: 3.644 min
Delta R.T.: 0.003 min
Response: 51896419
Conc: 14.27 ng/ml

Instrument :
ECD_R
ClientSampleId :
D2559


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/28/2022
Supervised By :Ankita Jodhani 06/28/2022

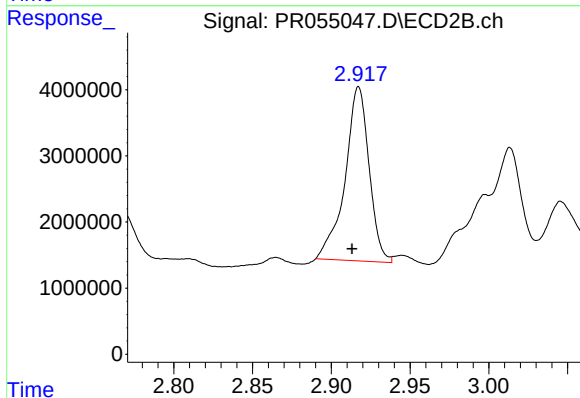


#1 Tetrachloro-m-xylene

R.T.: 2.917 min
Delta R.T.: 0.004 min
Response: 28042792
Conc: 16.80 ng/ml

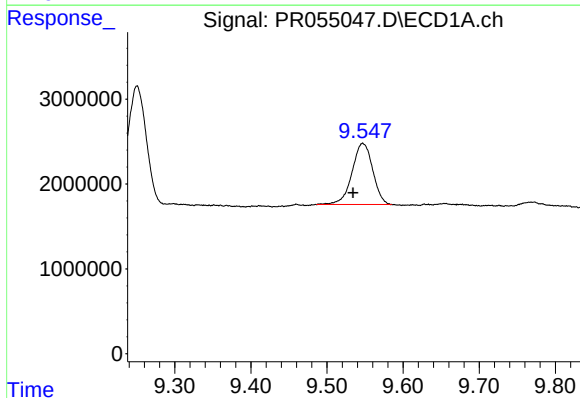

#2 Decachlorobiphenyl

R.T.: 9.547 min
Delta R.T.: 0.013 min
Response: 13608413
Conc: 9.44 ng/ml

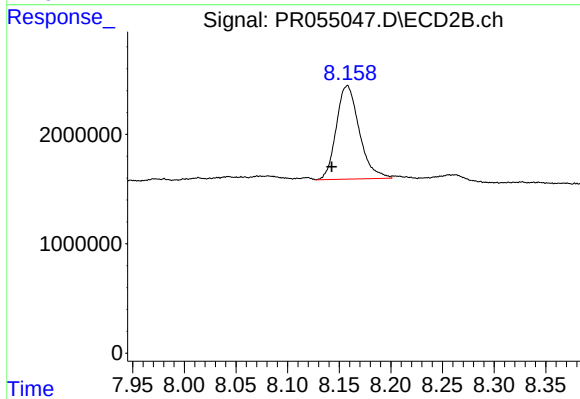

#2 Decachlorobiphenyl

R.T.: 8.158 min
Delta R.T.: 0.015 min
Response: 13248457
Conc: 9.43 ng/ml