

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR063022\
 Data File : PR055131.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jun 2022 04:15
 Operator : AJ\MA
 Sample : N3214-07
 Misc : AR1254 LOD 40 PPB
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 30 06:41:49 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR062722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 27 17:05:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.639	2.911	82603503	37285110	22.710	22.334
2) SA Decachlor...	9.529	8.136	34564396	33723793	23.971	24.002
Target Compounds						
26) L6 AR-1254-1	5.768	4.850	4191401	3496442	45.022	39.971
27) L6 AR-1254-2	6.004	5.009	6109741	3167219	46.767	41.059
28) L6 AR-1254-3	6.395	5.428	6220352	4929479	49.243	39.990
29) L6 AR-1254-4	6.707	5.673	4254429	2937284	45.879	37.325
30) L6 AR-1254-5	7.162	6.115	4414174	4269184	44.903	37.318



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR063022\
Data File : PR055131.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jun 2022 04:15
Operator : AJ\MA
Sample : N3214-07
Misc : AR1254 LOD 40 PPB
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 30 06:41:49 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR062722.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 27 17:05:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

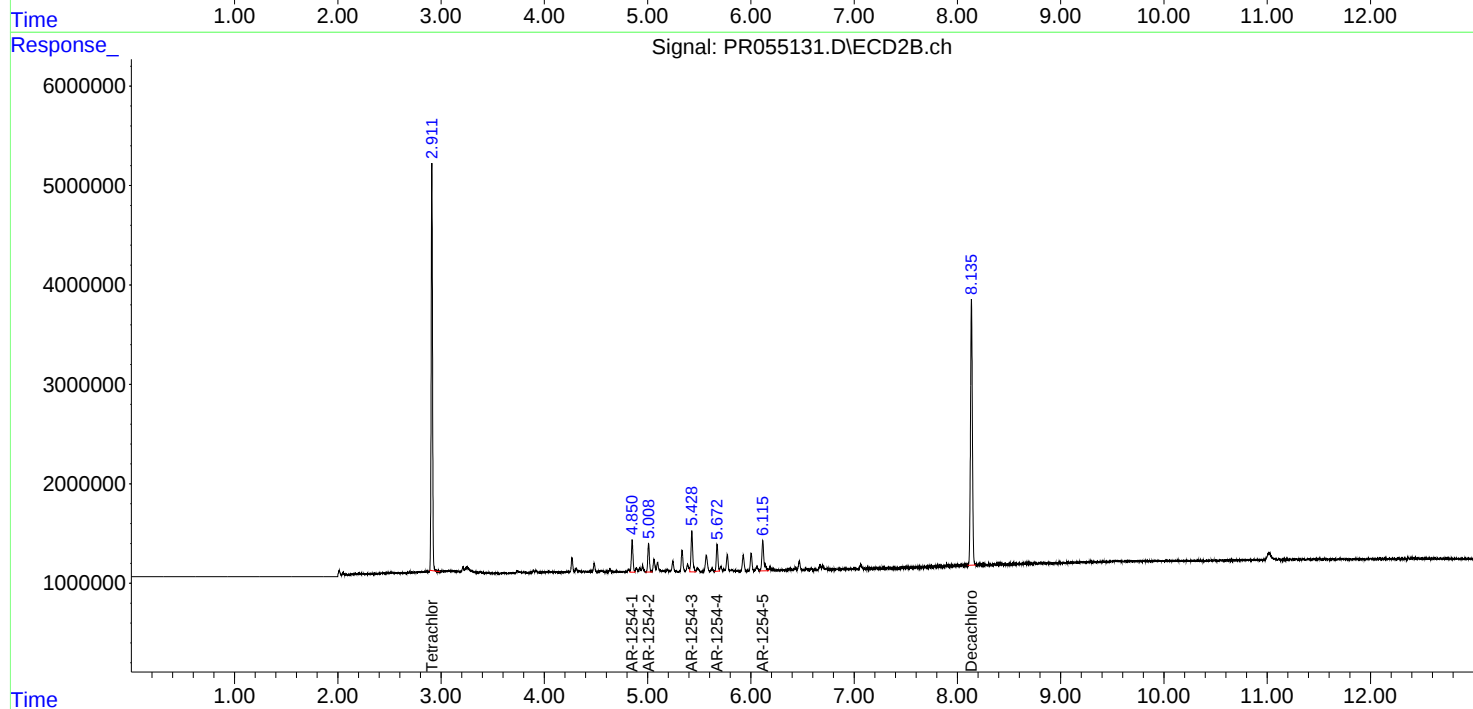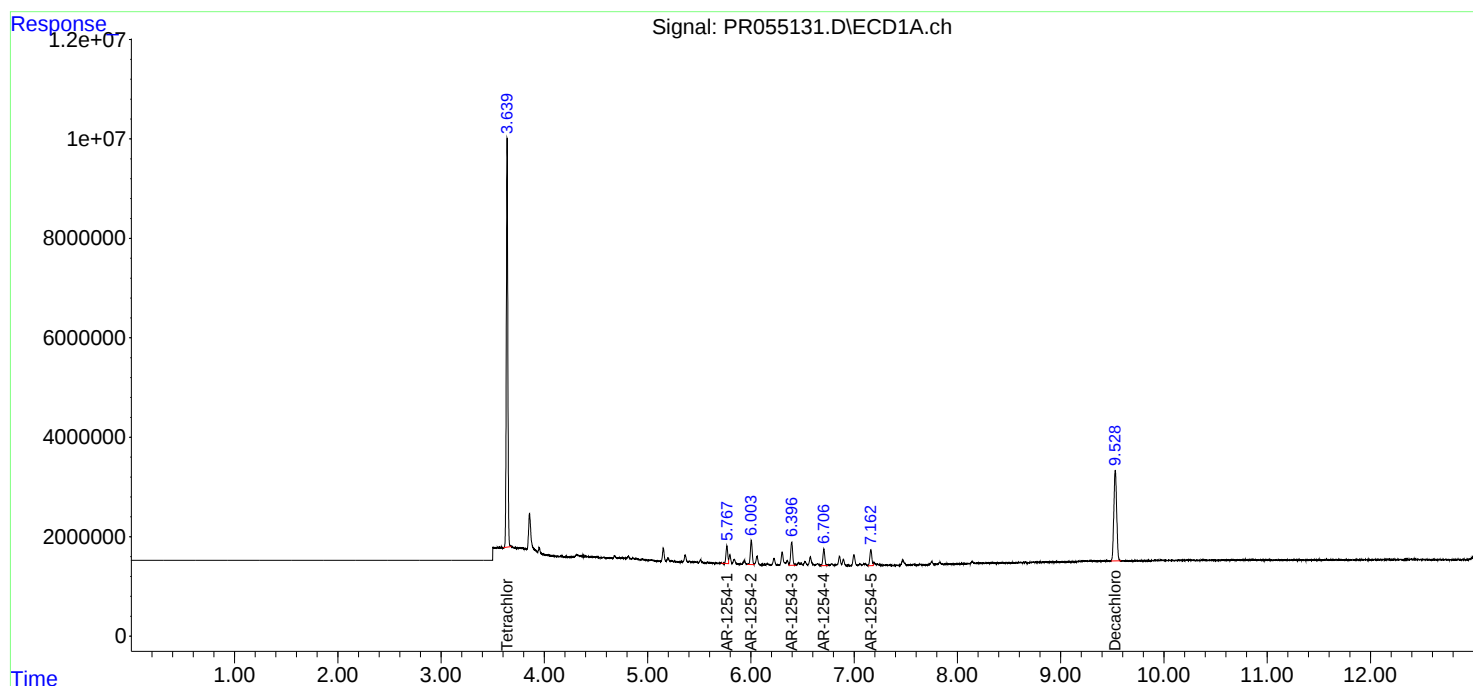


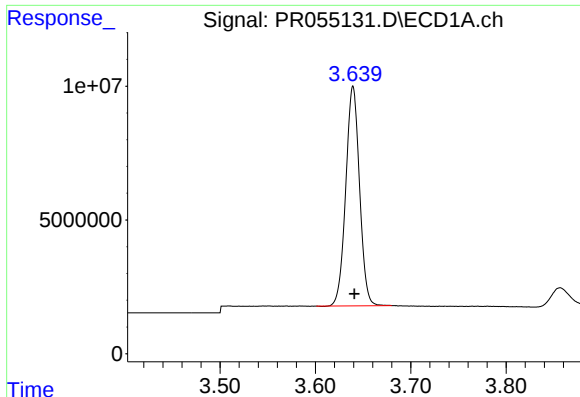

#1 Tetrachloro-m-xylene


R.T.: 3.639 min
Delta R.T.: -0.002 min
Response: 82603503
Conc: 22.71 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

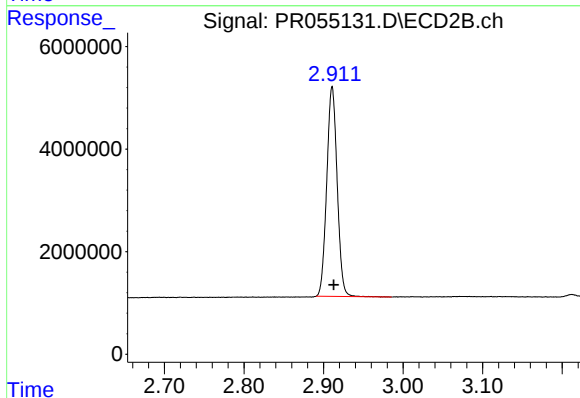


#1 Tetrachloro-m-xylene

R.T.: 2.911 min
Delta R.T.: -0.002 min
Response: 37285110
Conc: 22.33 ng/ml

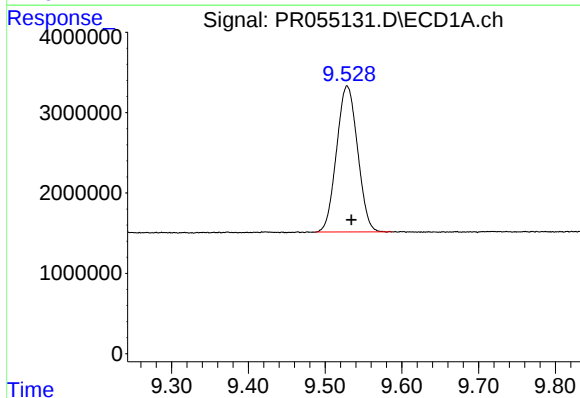


#2 Decachlorobiphenyl

R.T.: 9.529 min
Delta R.T.: -0.005 min
Response: 34564396
Conc: 23.97 ng/ml

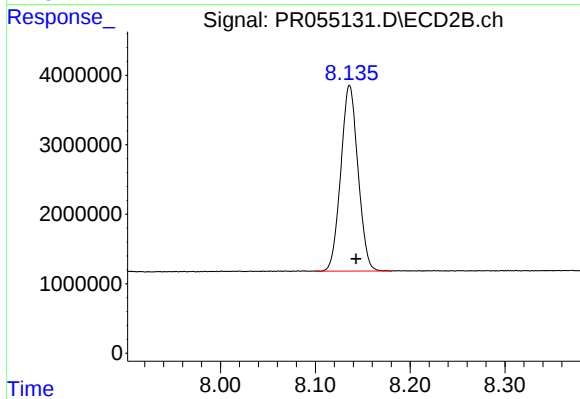

#2 Decachlorobiphenyl


R.T.: 8.136 min
Delta R.T.: -0.007 min
Response: 33723793
Conc: 24.00 ng/ml

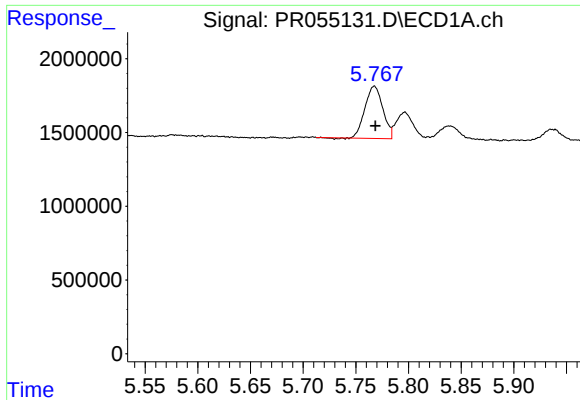

#26 AR-1254-1


R.T.: 5.768 min
Delta R.T.: -0.001 min
Response: 4191401
Conc: 45.02 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

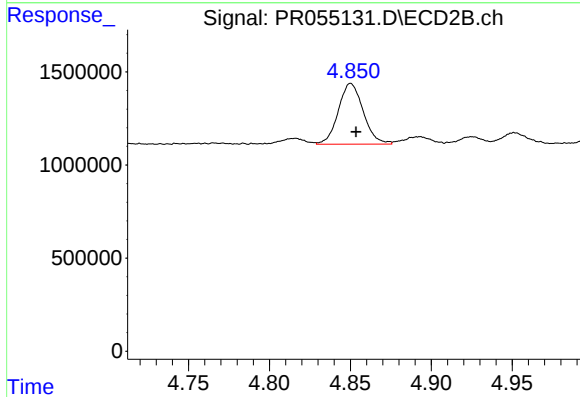


#26 AR-1254-1

R.T.: 4.850 min
Delta R.T.: -0.003 min
Response: 3496442
Conc: 39.97 ng/ml

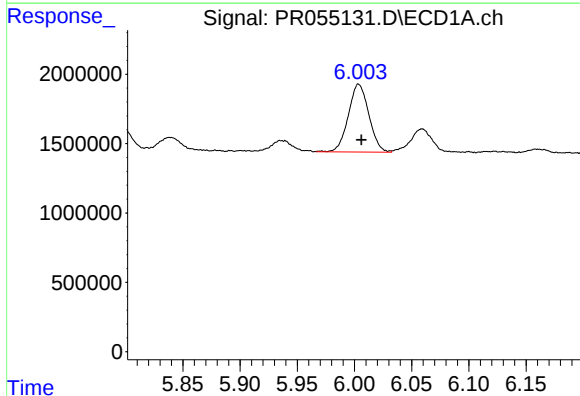


#27 AR-1254-2

R.T.: 6.004 min
Delta R.T.: -0.002 min
Response: 6109741
Conc: 46.77 ng/ml

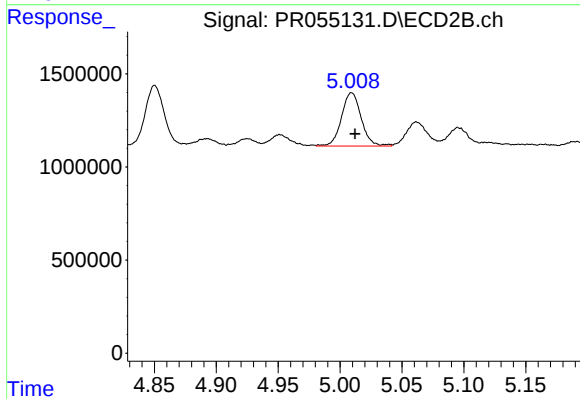

#27 AR-1254-2


R.T.: 5.009 min
Delta R.T.: -0.003 min
Response: 3167219
Conc: 41.06 ng/ml

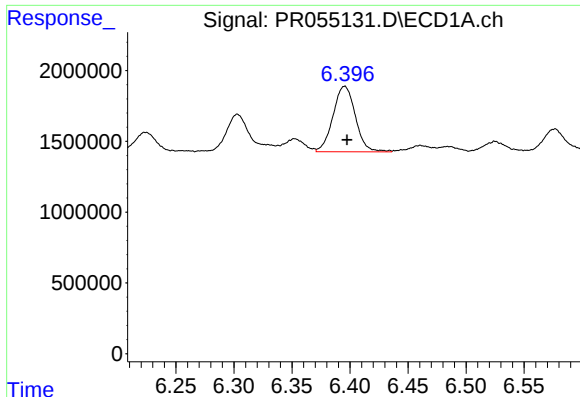

#28 AR-1254-3


R.T.: 6.395 min
Delta R.T.: -0.002 min
Response: 6220352
Conc: 49.24 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

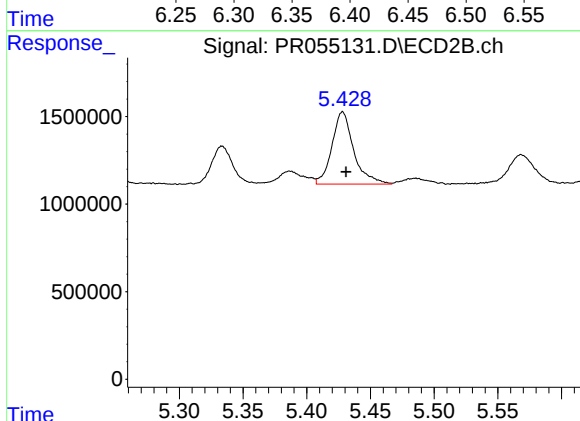


#28 AR-1254-3

R.T.: 5.428 min
Delta R.T.: -0.003 min
Response: 4929479
Conc: 39.99 ng/ml

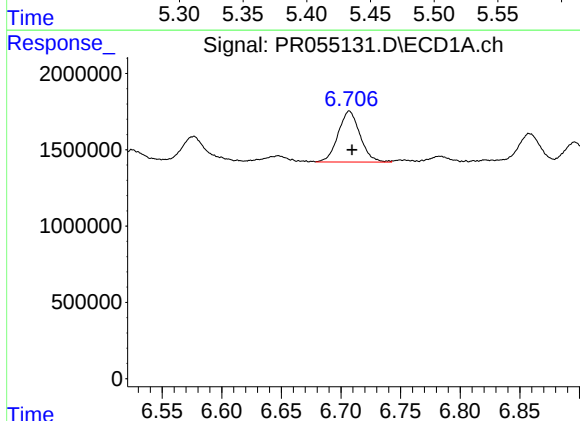


#29 AR-1254-4

R.T.: 6.707 min
Delta R.T.: -0.002 min
Response: 4254429
Conc: 45.88 ng/ml

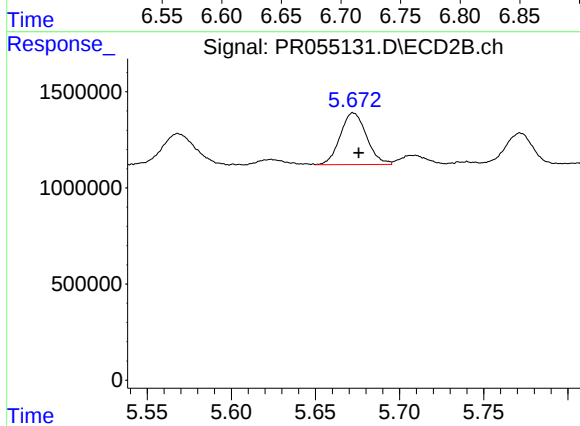

#29 AR-1254-4


R.T.: 5.673 min
Delta R.T.: -0.003 min
Response: 2937284
Conc: 37.33 ng/ml

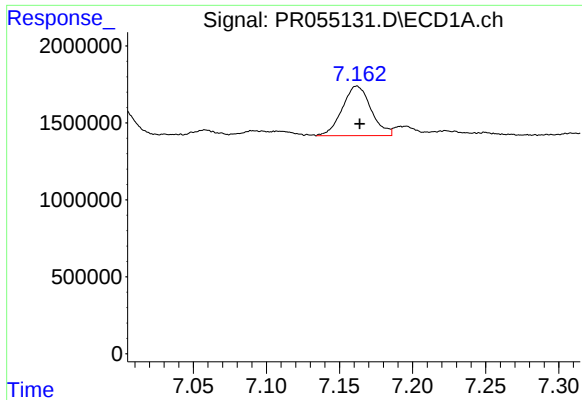

#30 AR-1254-5

R.T.: 7.162 min
Delta R.T.: -0.002 min
Response: 4414174
Conc: 44.90 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

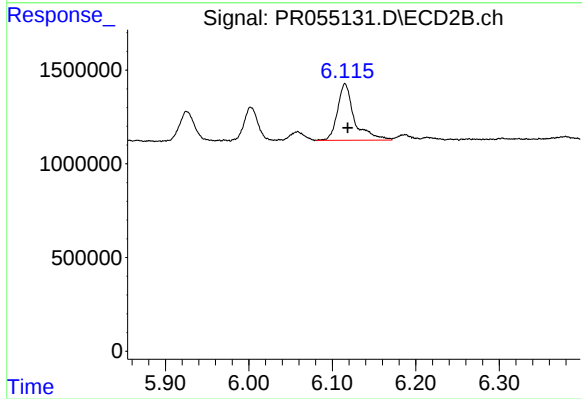

#30 AR-1254-5

R.T.: 6.115 min
Delta R.T.: -0.003 min
Response: 4269184
Conc: 37.32 ng/ml