

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR070118\
 Data File : PR029607.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jun 2018 11:32
 Operator : UA/SM
 Sample : J3502-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 20180367-SITE-WATER

Manual Integrations
 APPROVED

UGO
 6/28/2018 11:53:41 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 27 11:47:33 2018
 Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_R\Method\PR062718.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jun 23 08:41:26 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.567	3.721	390.3E6	644.9E6	16.958m	13.641
2) SA Decachlor...	10.331	8.646	428.8E6	332.9E6	15.315m	16.854

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR070118\
Data File : PR029607.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jun 2018 11:32
Operator : UA/SM
Sample : J3502-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
20180367-SITE-WATER


Manual Integrations
APPROVED

UGO
6/28/2018 11:53:41 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 11:47:33 2018
Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_R\Method\PR062718.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jun 23 08:41:26 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

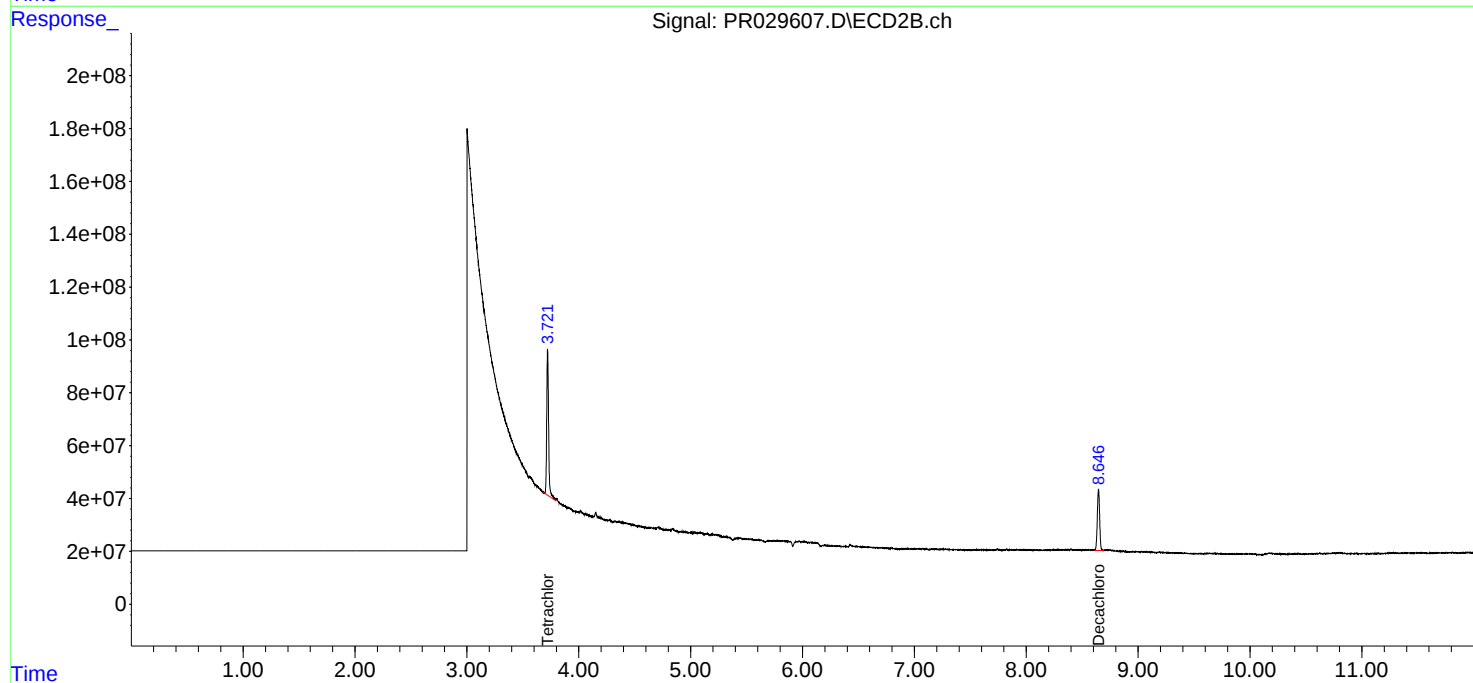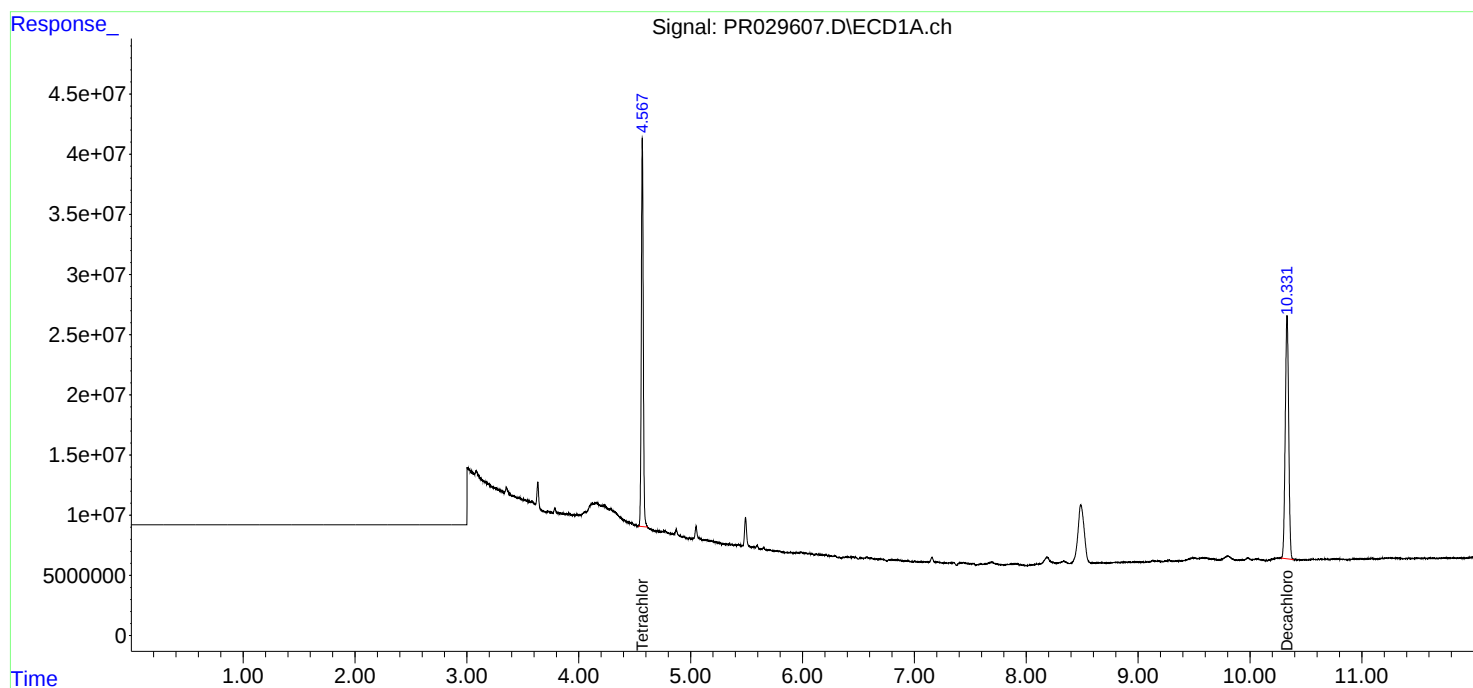

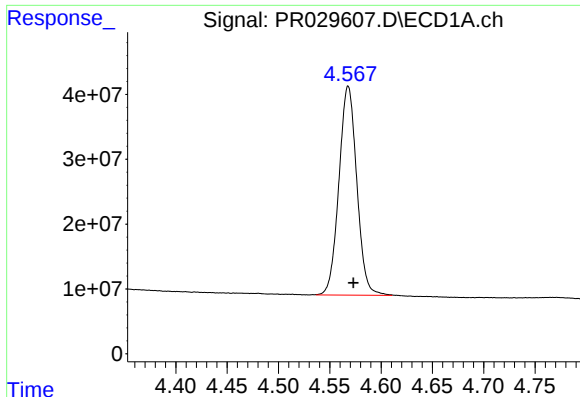


#1 Tetrachloro-m-xylene

R.T.: 4.567 min
Delta R.T.: -0.006 min
Response: 390292291
Conc: 16.96 ng/ml m

Instrument :
ECD_R
ClientSampleId :
20180367-SITE-WATER


Manual Integrations
APPROVED

UGO
6/28/2018 11:53:41 AM

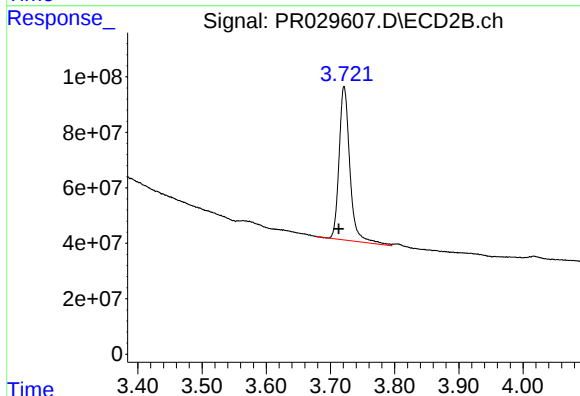


#1 Tetrachloro-m-xylene

R.T.: 3.721 min
Delta R.T.: 0.008 min
Response: 644878368
Conc: 13.64 ng/ml

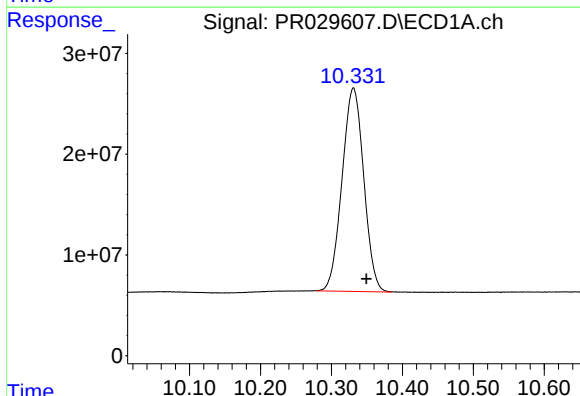

#2 Decachlorobiphenyl

R.T.: 10.331 min
Delta R.T.: -0.019 min
Response: 428752548
Conc: 15.31 ng/ml m

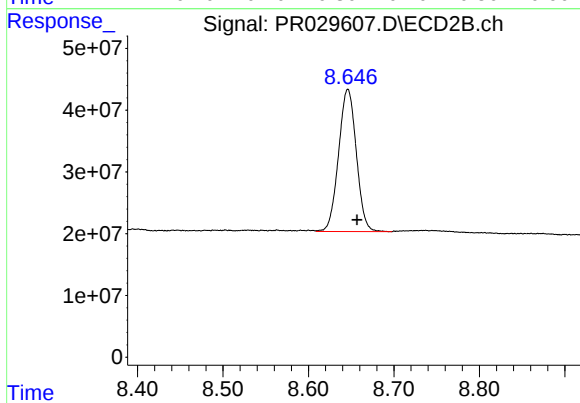

#2 Decachlorobiphenyl

R.T.: 8.646 min
Delta R.T.: -0.011 min
Response: 332859007
Conc: 16.85 ng/ml