

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR070122\
 Data File : PR055175.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jun 2022 20:02
 Operator : AJ\MA
 Sample : N3214-09
 Misc : AR1254 MDL 25 PPB
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-WATER-03-QT2-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 01 00:42:47 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR062722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 27 17:05:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.639	2.911	79700674	35655651	21.912	21.358
2) SA Decachlor...	9.531	8.137	35331624	33351829	24.503	23.738
Target Compounds						
26) L6 AR-1254-1	5.766	4.850	3109292	2231619	33.399	25.512
27) L6 AR-1254-2	6.003	5.008	4001912	2090441	30.632	27.100
28) L6 AR-1254-3	6.394	5.427	4429501	3535431	35.066	28.681
29) L6 AR-1254-4	6.707	5.672	2896177	1954881	31.232	24.842
30) L6 AR-1254-5	7.161	6.115	2816272	2300284	28.648	20.108 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR070122\
Data File : PR055175.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jun 2022 20:02
Operator : AJ\MA
Sample : N3214-09
Misc : AR1254 MDL 25 PPB
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 01 00:42:47 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR062722.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 27 17:05:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

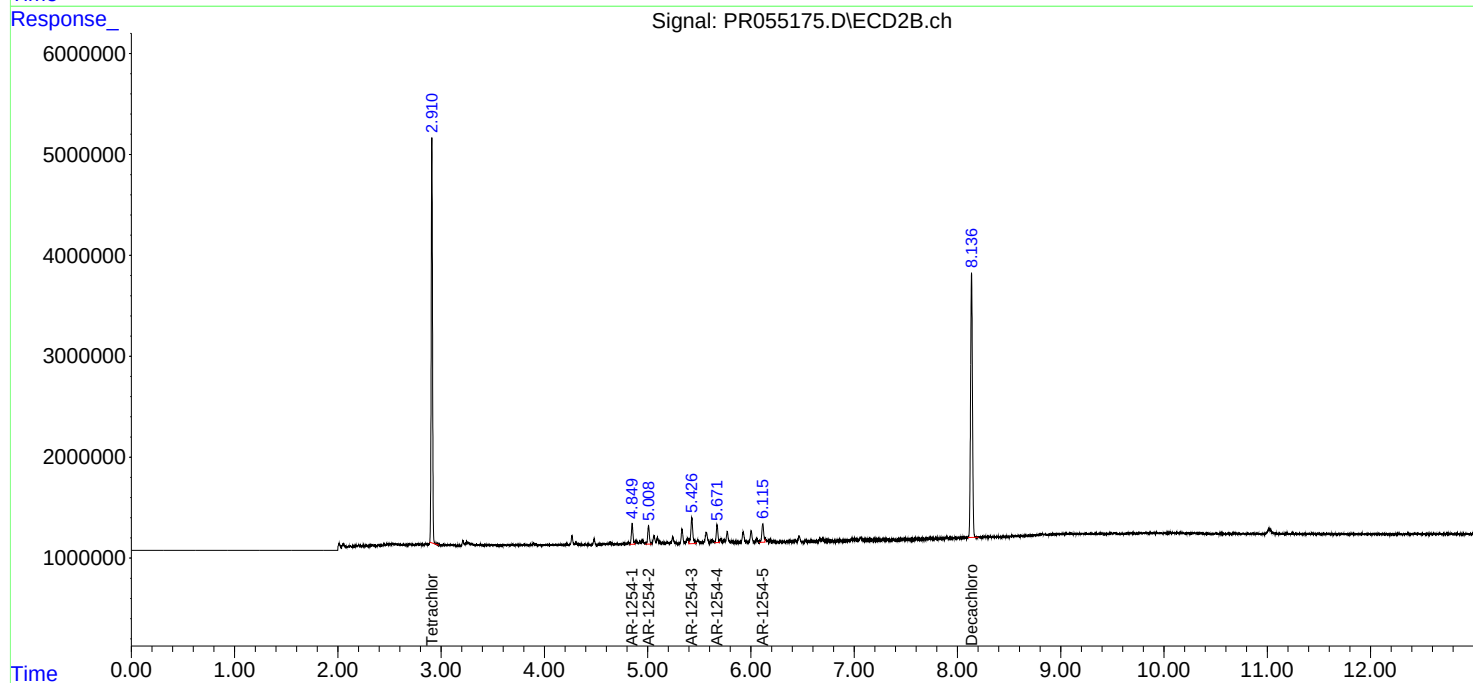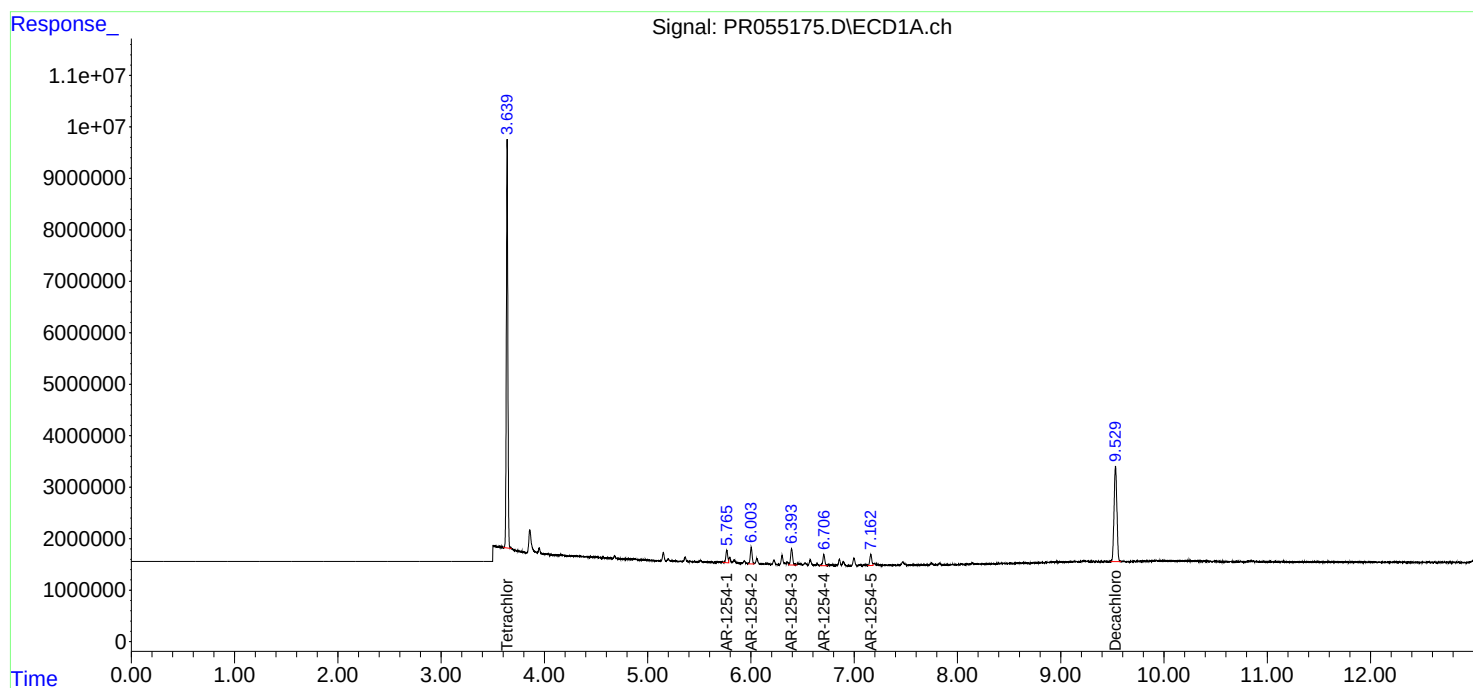


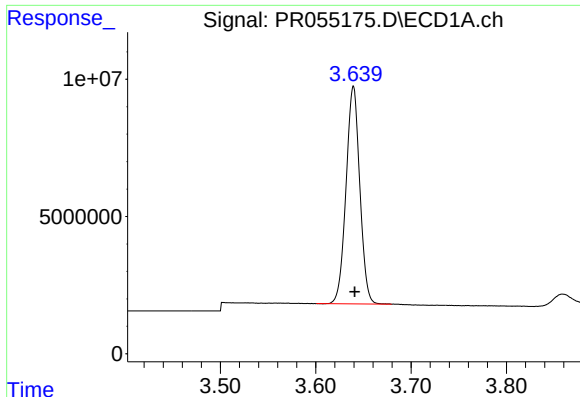

#1 Tetrachloro-m-xylene


R.T.: 3.639 min
Delta R.T.: -0.002 min
Response: 79700674
Conc: 21.91 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2022

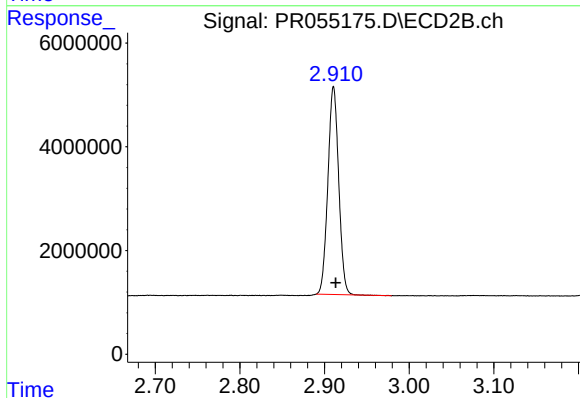


#1 Tetrachloro-m-xylene

R.T.: 2.911 min
Delta R.T.: -0.002 min
Response: 35655651
Conc: 21.36 ng/ml

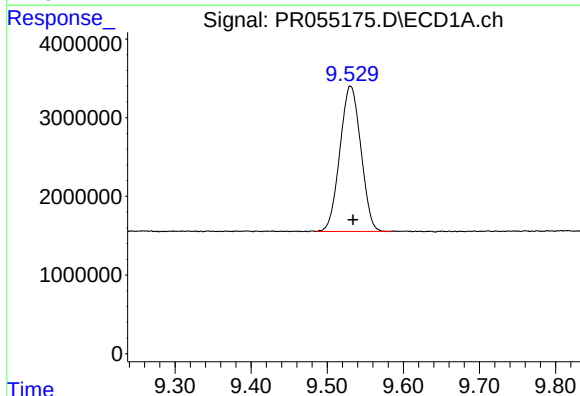


#2 Decachlorobiphenyl

R.T.: 9.531 min
Delta R.T.: -0.003 min
Response: 35331624
Conc: 24.50 ng/ml

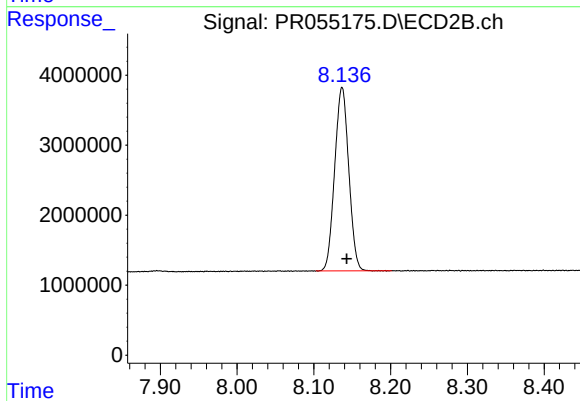

#2 Decachlorobiphenyl


R.T.: 8.137 min
Delta R.T.: -0.006 min
Response: 33351829
Conc: 23.74 ng/ml

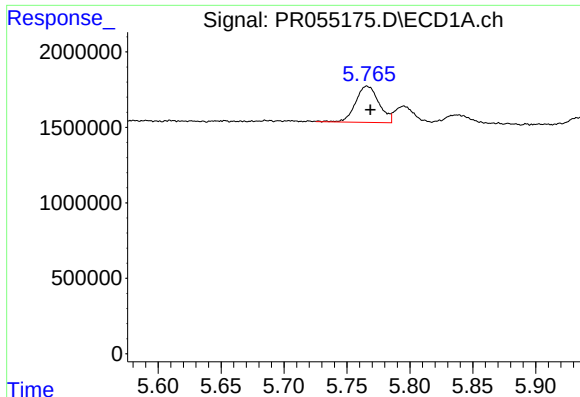

#26 AR-1254-1


R.T.: 5.766 min
Delta R.T.: -0.002 min
Response: 3109292
Conc: 33.40 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2022

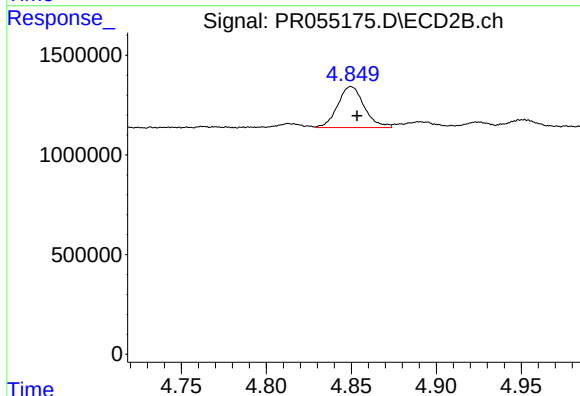


#26 AR-1254-1

R.T.: 4.850 min
Delta R.T.: -0.004 min
Response: 2231619
Conc: 25.51 ng/ml

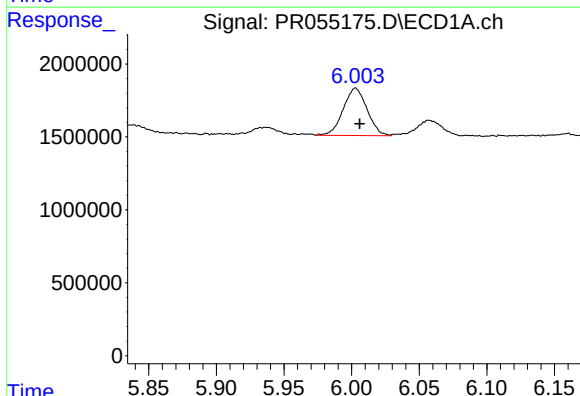


#27 AR-1254-2

R.T.: 6.003 min
Delta R.T.: -0.003 min
Response: 4001912
Conc: 30.63 ng/ml

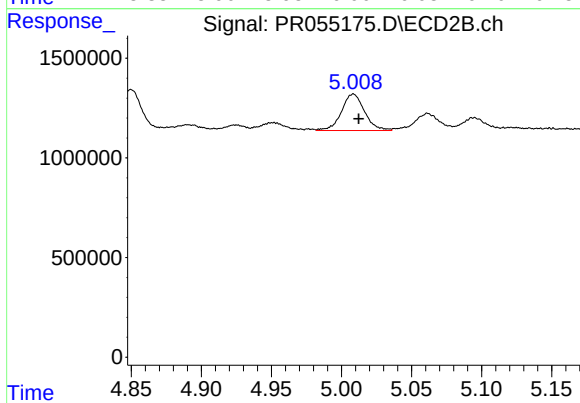

#27 AR-1254-2


R.T.: 5.008 min
Delta R.T.: -0.004 min
Response: 2090441
Conc: 27.10 ng/ml

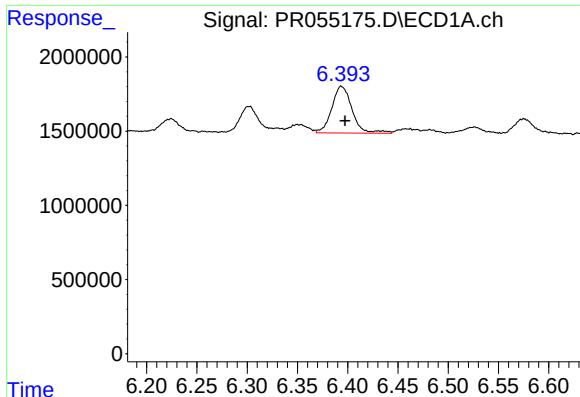

#28 AR-1254-3


R.T.: 6.394 min
Delta R.T.: -0.003 min
Response: 4429501
Conc: 35.07 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2022

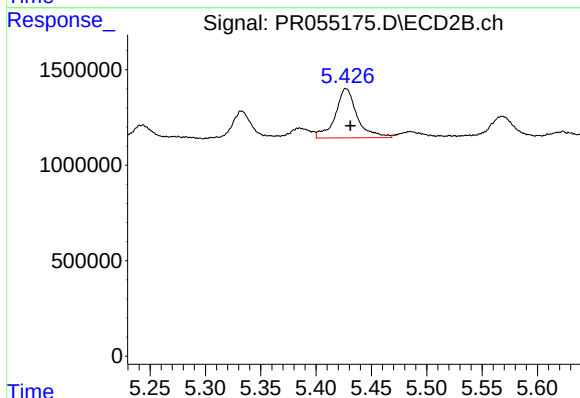


#28 AR-1254-3

R.T.: 5.427 min
Delta R.T.: -0.004 min
Response: 3535431
Conc: 28.68 ng/ml

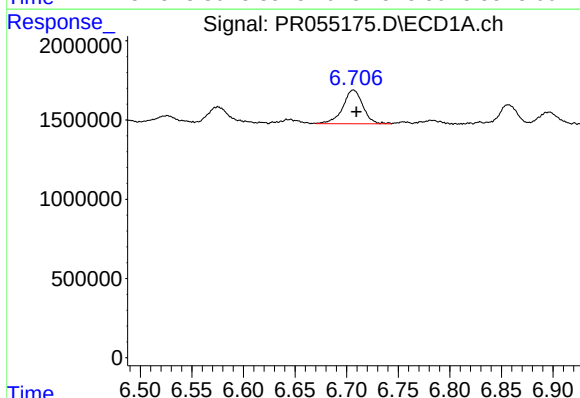


#29 AR-1254-4

R.T.: 6.707 min
Delta R.T.: -0.003 min
Response: 2896177
Conc: 31.23 ng/ml

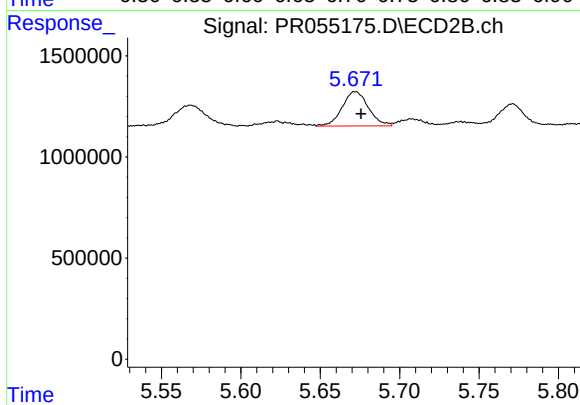

#29 AR-1254-4


R.T.: 5.672 min
Delta R.T.: -0.004 min
Response: 1954881
Conc: 24.84 ng/ml

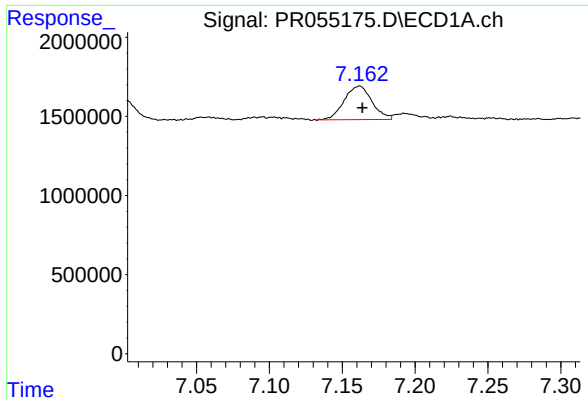

#30 AR-1254-5

R.T.: 7.161 min
Delta R.T.: -0.003 min
Response: 2816272
Conc: 28.65 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2022

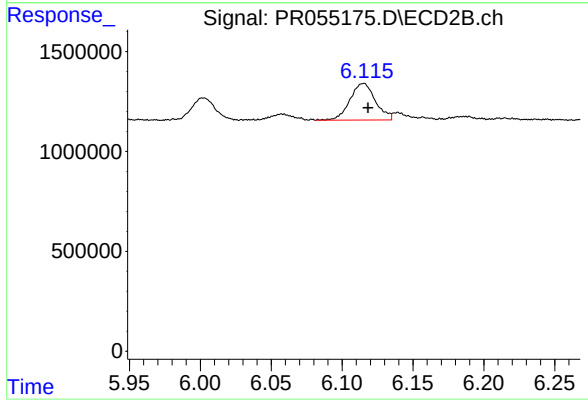

#30 AR-1254-5

R.T.: 6.115 min
Delta R.T.: -0.003 min
Response: 2300284
Conc: 20.11 ng/ml