

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR070618\
 Data File : PR029882.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jul 2018 11:36
 Operator : UA/SM
 Sample : J3755-01RE
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 PS-BASELINEWATERRE

Manual Integrations
 APPROVED

mohammad
 7/5/2018 8:26:20 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 11:56:30 2018
 Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_R\Method\PR070518.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 03 11:16:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.563	3.710	557.0E6	741.6E6	21.588m	17.188
2) SA Decachlor...	10.328	8.633	160.6E6	141.5E6	6.218	6.823m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR070618\
Data File : PR029882.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jul 2018 11:36
Operator : UA/SM
Sample : J3755-01RE
Misc :
ALS Vial : 48 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
PS-BASELINEWATERRE


Manual Integrations
APPROVED

mohammad
7/5/2018 8:26:20 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 11:56:30 2018
Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_R\Method\PR070518.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 03 11:16:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

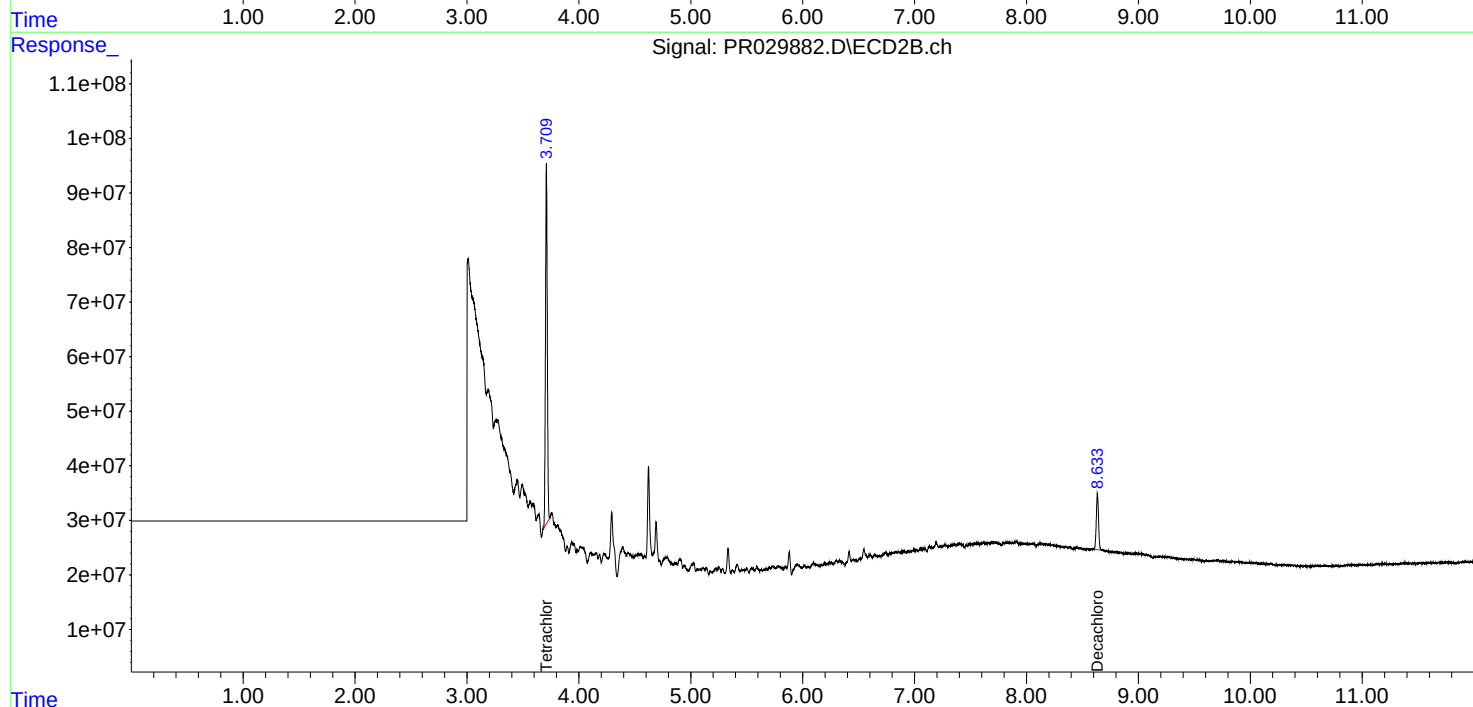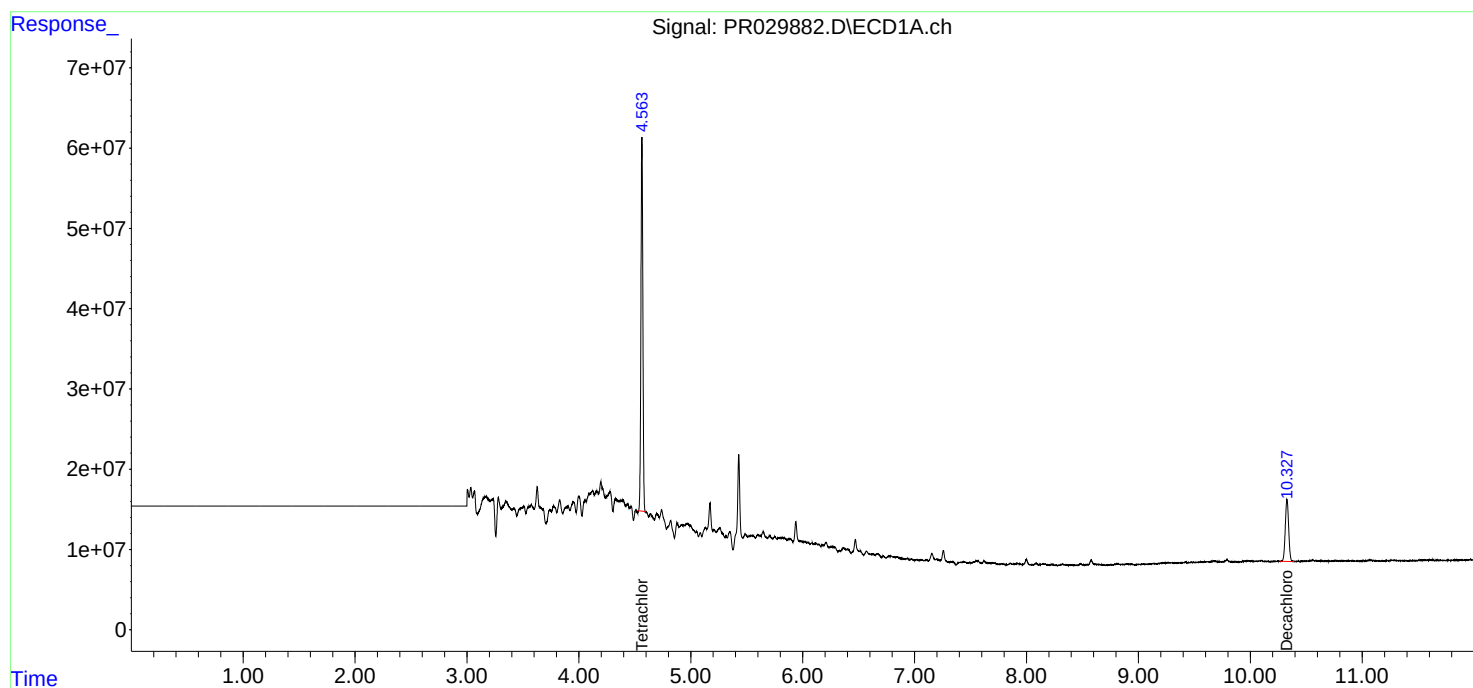

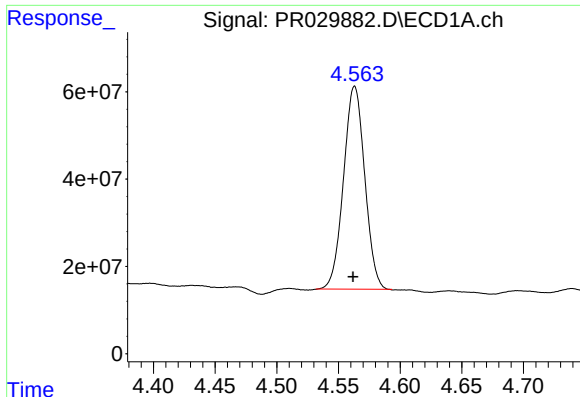


#1 Tetrachloro-m-xylene

R.T.: 4.563 min
Delta R.T.: 0.000 min
Response: 556957097
Conc: 21.59 ng/ml m

Instrument :
ECD_R
ClientSampleId :
PS-BASELINEWATERRE


Manual Integrations
APPROVED

mohammad
7/5/2018 8:26:20 AM

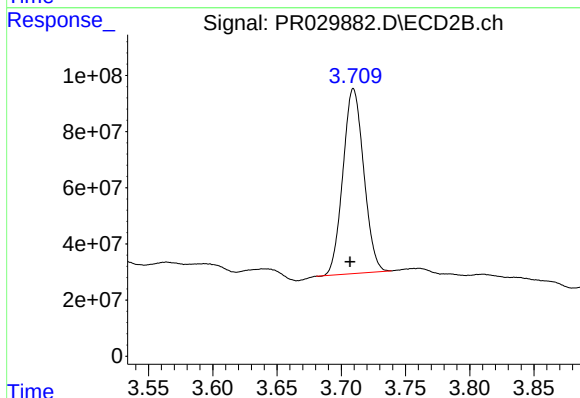


#1 Tetrachloro-m-xylene

R.T.: 3.710 min
Delta R.T.: 0.003 min
Response: 741585159
Conc: 17.19 ng/ml

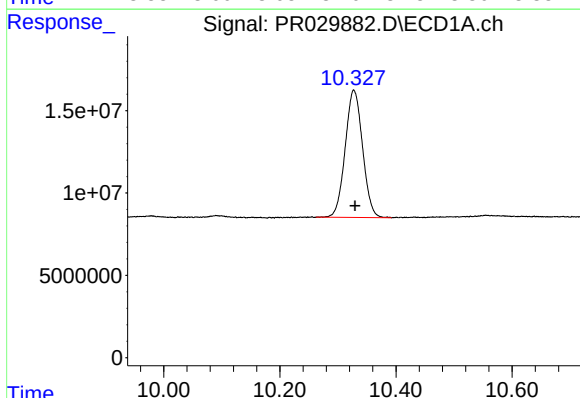

#2 Decachlorobiphenyl

R.T.: 10.328 min
Delta R.T.: -0.002 min
Response: 160583762
Conc: 6.22 ng/ml

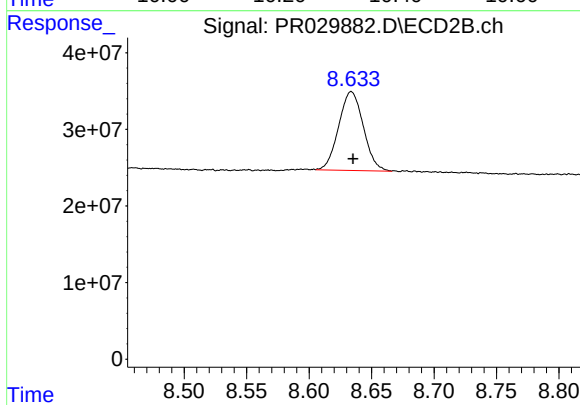

#2 Decachlorobiphenyl

R.T.: 8.633 min
Delta R.T.: -0.002 min
Response: 141543221
Conc: 6.82 ng/ml m