

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR071118\
 Data File : PR030157.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jul 2018 17:30
 Operator : MA/SM
 Sample : J3912-02
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 GS-CONCRETE-PIPE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 11 04:31:13 2018
 Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_R\Method\PR071018.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 10 01:27:38 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.561	3.707	285.2E6	629.2E6	18.163	23.726 #
2) SA Decachlor...	10.326	8.622	411.4E6	279.9E6	14.263	12.414

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR071118\
Data File : PR030157.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jul 2018 17:30
Operator : MA/SM
Sample : J3912-02
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
GS-CONCRETE-PIPE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 11 04:31:13 2018
Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_R\Method\PR071018.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 10 01:27:38 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

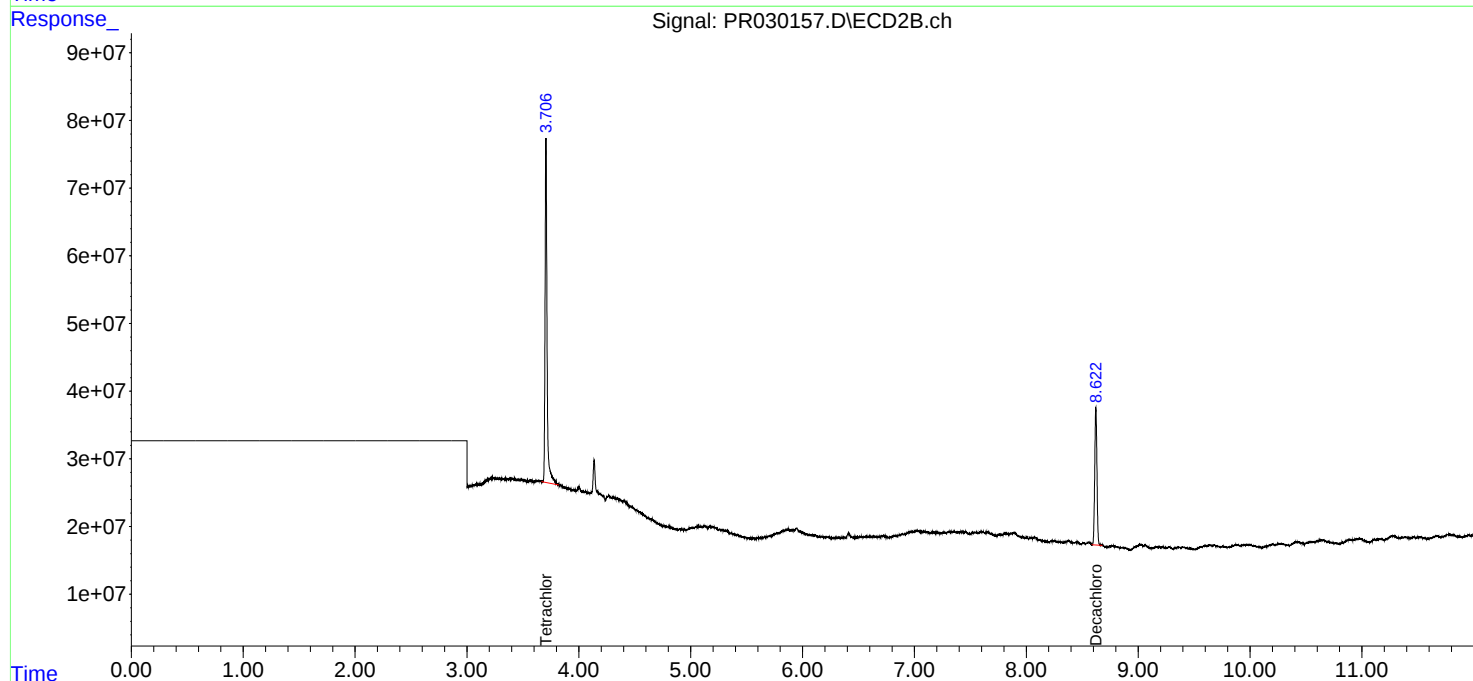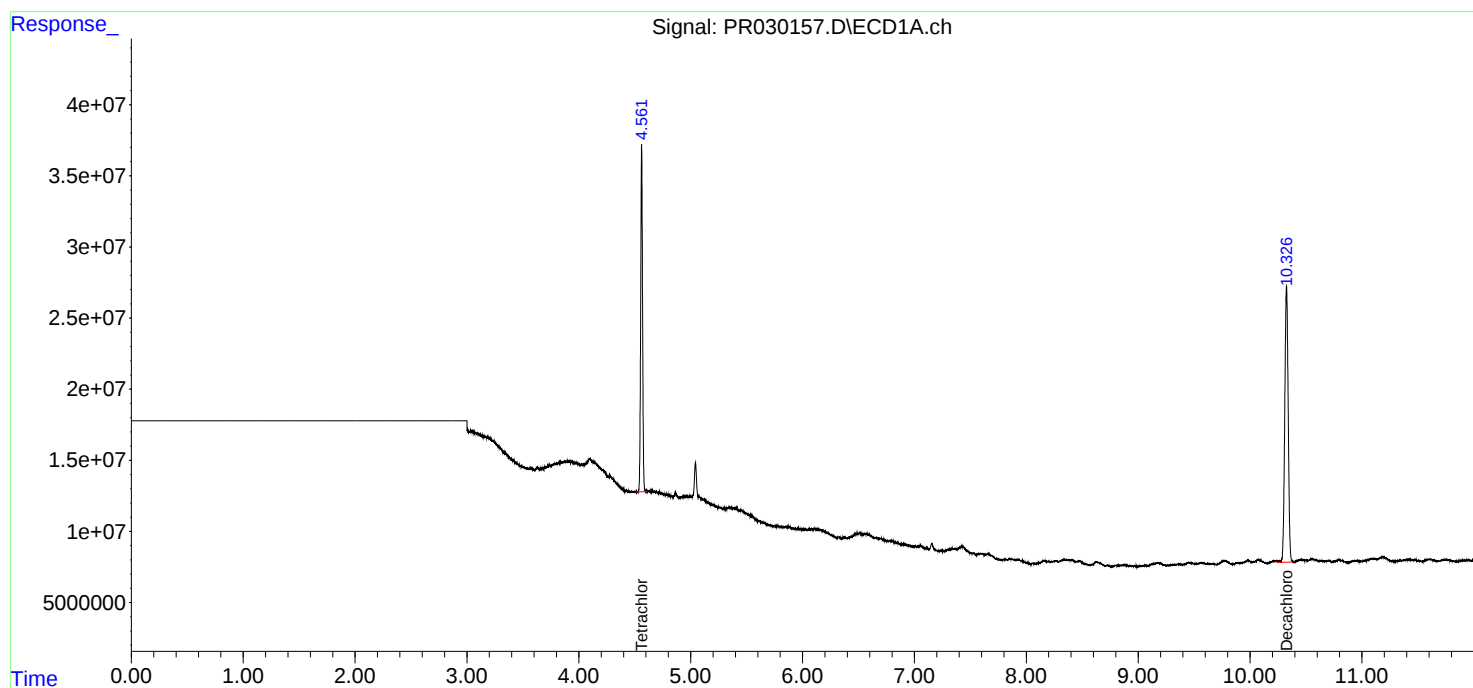


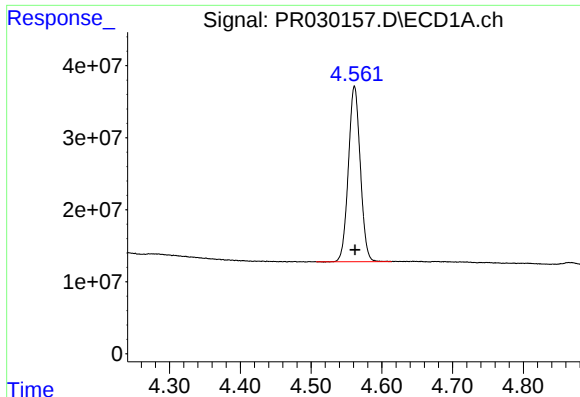

#1 Tetrachloro-m-xylene


R.T.: 4.561 min
Delta R.T.: 0.000 min
Response: 285176631
Conc: 18.16 ng/ml

Instrument :
ECD_R
ClientSampleId :
GS-CONCRETE-PIPE

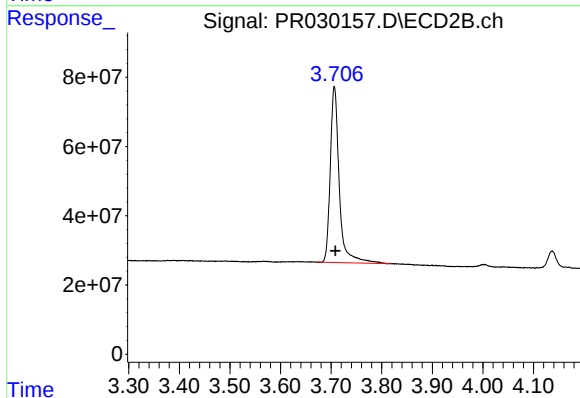


#1 Tetrachloro-m-xylene

R.T.: 3.707 min
Delta R.T.: -0.002 min
Response: 629238894
Conc: 23.73 ng/ml

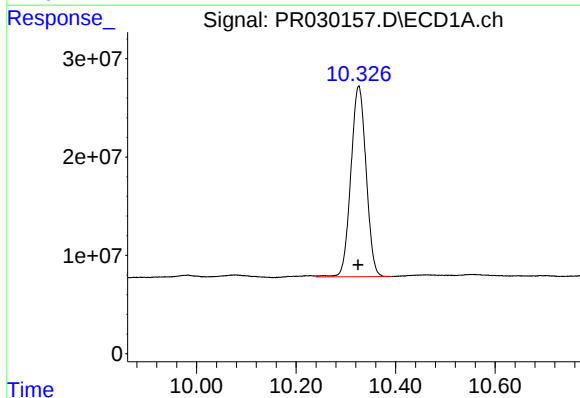

#2 Decachlorobiphenyl

R.T.: 10.326 min
Delta R.T.: 0.000 min
Response: 411380040
Conc: 14.26 ng/ml

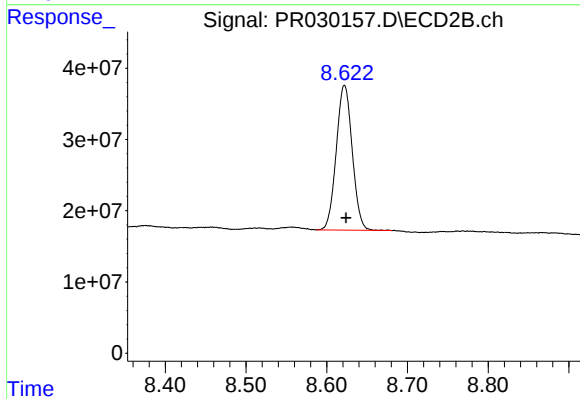

#2 Decachlorobiphenyl

R.T.: 8.622 min
Delta R.T.: -0.002 min
Response: 279946358
Conc: 12.41 ng/ml