

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR071519\
 Data File : PR039326.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2019 14:20
 Operator : SM\AJ
 Sample : AR1254ICC050
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 AR1254ICC050

Manual Integrations
 APPROVED

Ankita
 7/17/2019 9:51:43 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 01:46:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR071519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 16 01:44:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.763	4.610	7809715	32043563	3.920m	4.111
2)	SA Decachlor...	8.704	10.349	14215253	48151188	5.383m	5.371
Target Compounds							
26)	L6 AR-1254-1	5.618	6.609	6321053	15347687	46.479	46.766m
27)	L6 AR-1254-2	5.764	6.824	5783822	25358636	48.434	48.632
28)	L6 AR-1254-3	6.161	7.188	9843654	31256315	46.561	52.000
29)	L6 AR-1254-4	6.385	7.470	7078768	20855091	44.789m	47.136
30)	L6 AR-1254-5	6.796	7.884	8595764	22434904	44.665	46.453m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR071519\
Data File : PR039326.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2019 14:20
Operator : SM\AJ
Sample : AR1254ICC050
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampled :
AR1254ICC050


Manual Integrations
APPROVED

Ankita
7/17/2019 9:51:43 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 01:46:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR071519.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 16 01:44:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

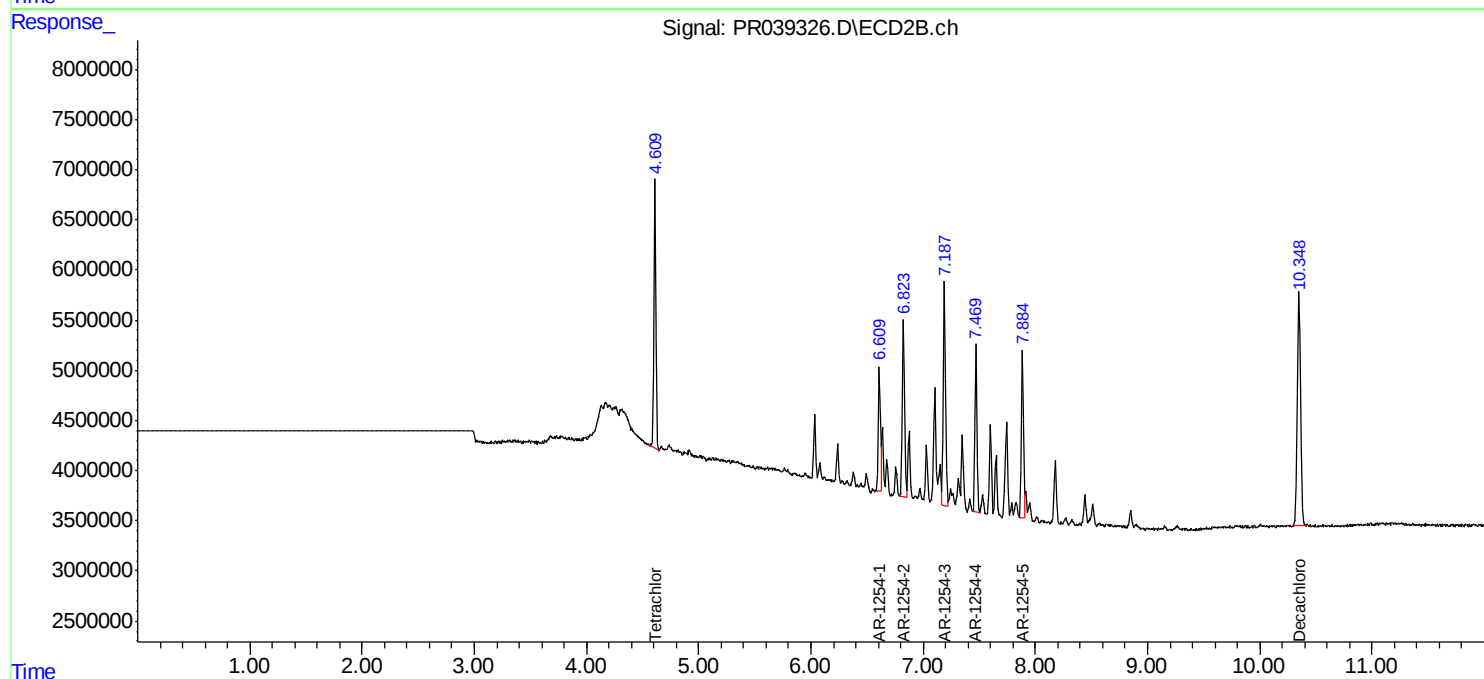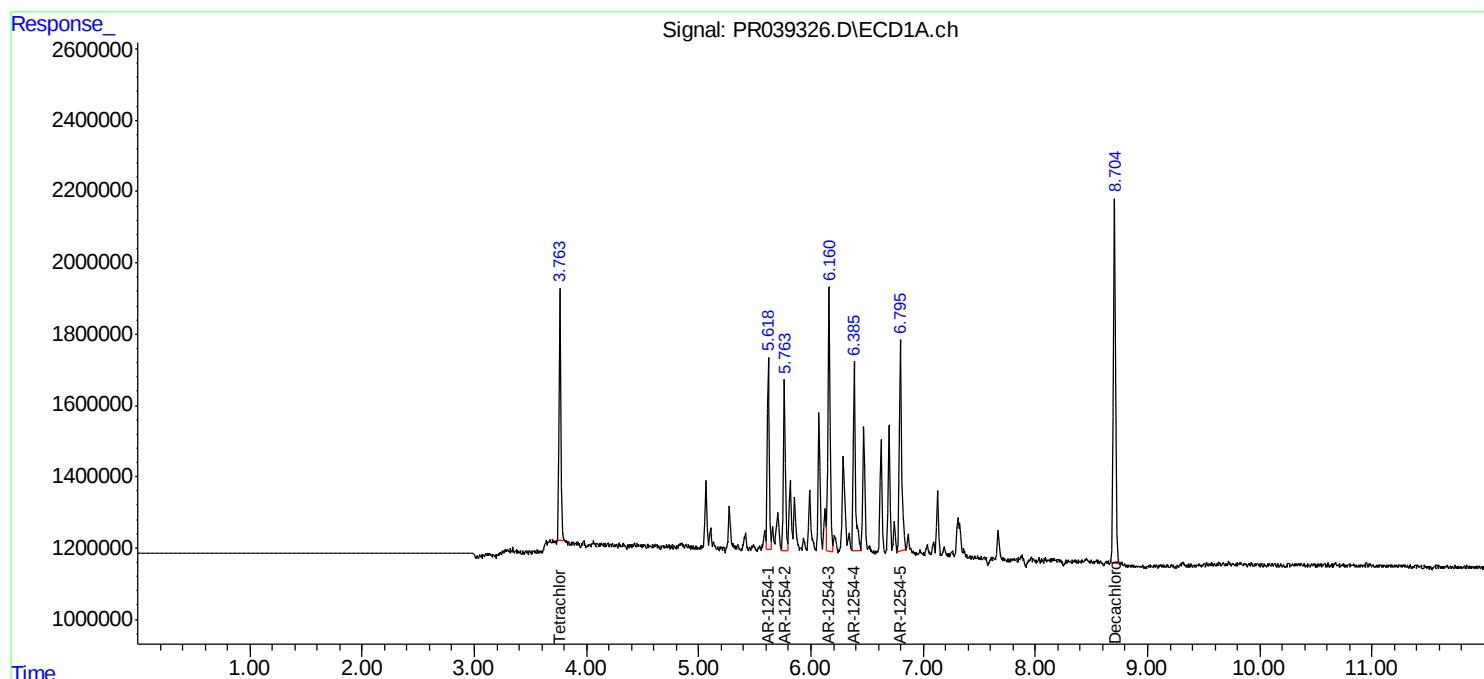

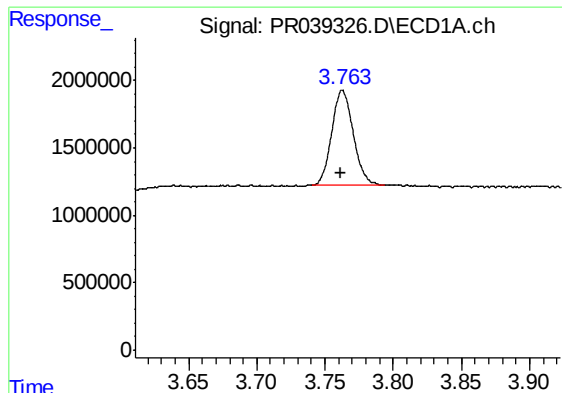


#1 Tetrachloro-m-xylene

R.T.: 3.763 min
Delta R.T.: 0.000 min
Response: 7809715
Conc: 3.92 ng/ml m

Instrument :
ECD_R
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Ankita
7/17/2019 9:51:43 AM

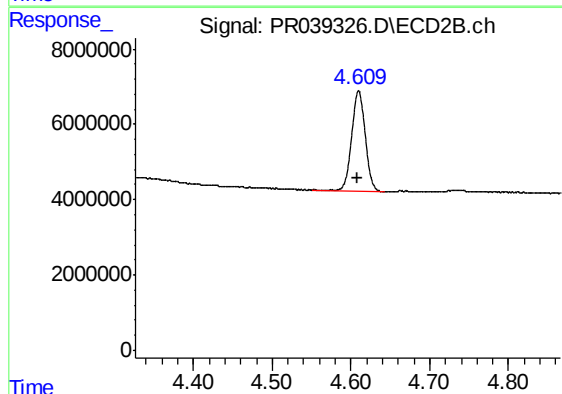


#1 Tetrachloro-m-xylene

R.T.: 4.610 min
Delta R.T.: 0.000 min
Response: 32043563
Conc: 4.11 ng/ml

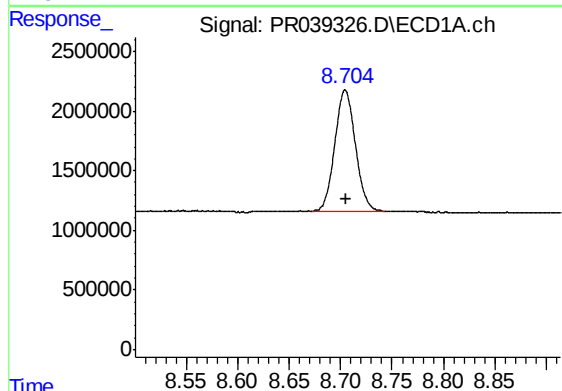


#2 Decachlorobiphenyl

R.T.: 8.704 min
Delta R.T.: 0.000 min
Response: 14215253
Conc: 5.38 ng/ml m

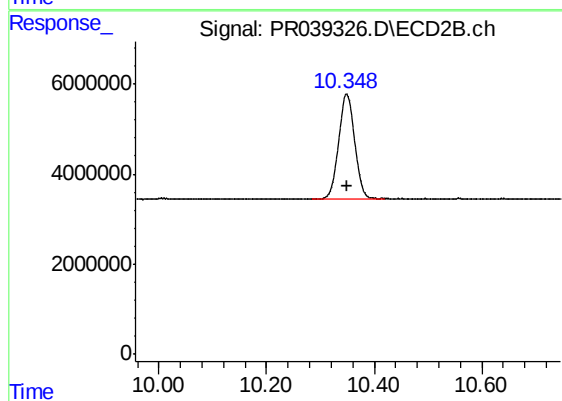

#2 Decachlorobiphenyl

R.T.: 10.349 min
Delta R.T.: 0.000 min
Response: 48151188
Conc: 5.37 ng/ml

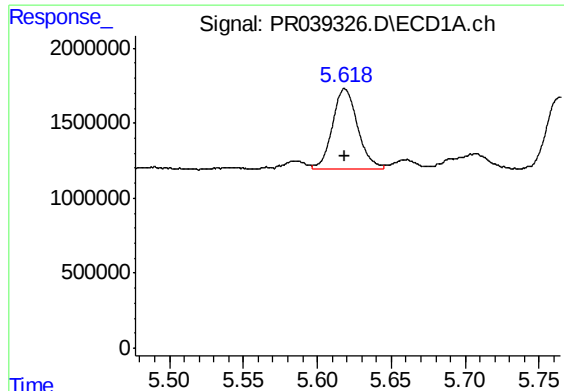


#26 AR-1254-1

R.T.: 5.618 min
Delta R.T.: 0.000 min
Response: 6321053
Conc: 46.48 ng/ml

Instrument :
ECD_R
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Ankita
7/17/2019 9:51:43 AM

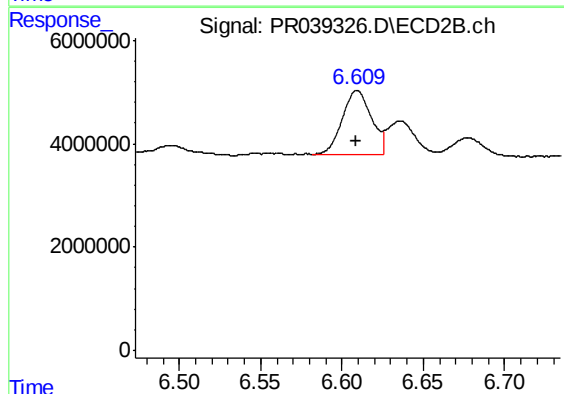


#26 AR-1254-1

R.T.: 6.609 min
Delta R.T.: 0.000 min
Response: 15347687
Conc: 46.77 ng/ml m

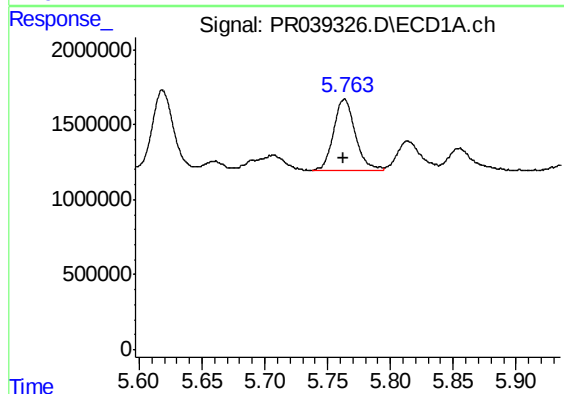


#27 AR-1254-2

R.T.: 5.764 min
Delta R.T.: 0.000 min
Response: 5783822
Conc: 48.43 ng/ml

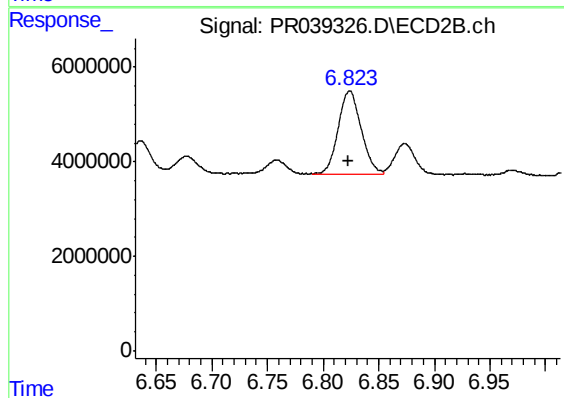

#27 AR-1254-2

R.T.: 6.824 min
Delta R.T.: 0.000 min
Response: 25358636
Conc: 48.63 ng/ml

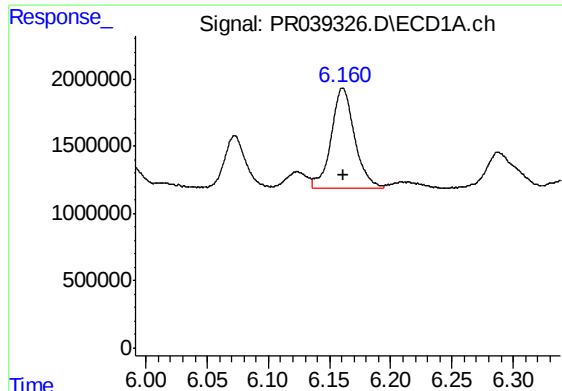


#28 AR-1254-3

R.T.: 6.161 min
Delta R.T.: 0.000 min
Response: 9843654
Conc: 46.56 ng/ml

Instrument :
ECD_R
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Ankita
7/17/2019 9:51:43 AM

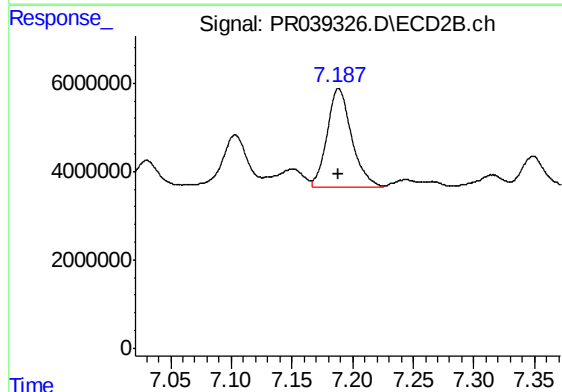


#28 AR-1254-3

R.T.: 7.188 min
Delta R.T.: 0.000 min
Response: 31256315
Conc: 52.00 ng/ml

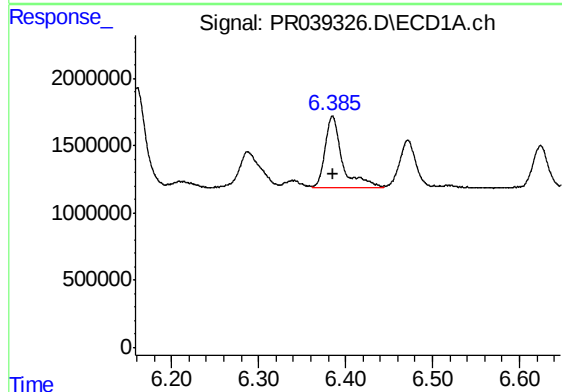


#29 AR-1254-4

R.T.: 6.385 min
Delta R.T.: 0.000 min
Response: 7078768
Conc: 44.79 ng/ml m

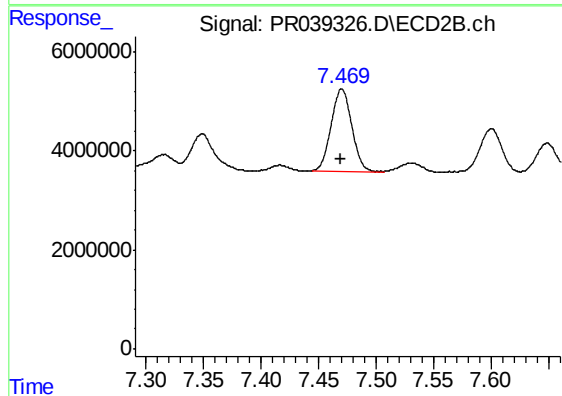

#29 AR-1254-4

R.T.: 7.470 min
Delta R.T.: 0.000 min
Response: 20855091
Conc: 47.14 ng/ml

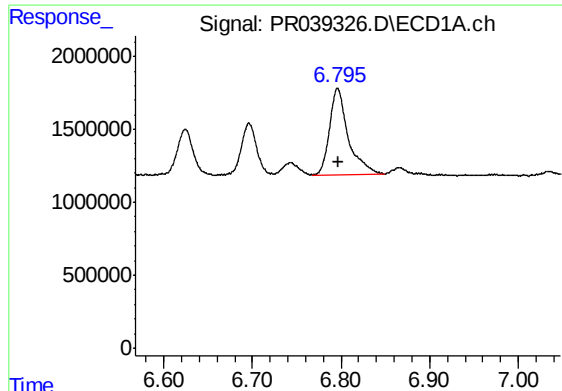


#30 AR-1254-5

R.T.: 6.796 min
Delta R.T.: 0.000 min
Response: 8595764
Conc: 44.66 ng/ml

Instrument :
ECD_R
ClientSampleId :
AR1254ICC050

Manual Integrations
APPROVED

Ankita
7/17/2019 9:51:43 AM

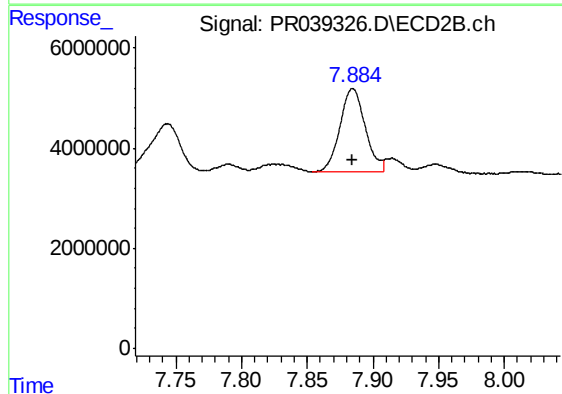

#30 AR-1254-5

R.T.: 7.884 min
Delta R.T.: 0.000 min
Response: 22434904
Conc: 46.45 ng/ml m