

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR071618\
 Data File : PR030373.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2018 06:45
 Operator : MA/SM
 Sample : LOD-LOQ BL WATER
 Misc : 100PPB LOQ ECD_R WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 LOD-LOQ BL WATER

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 09:36:21 2018
 Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_R\Method\PR071618.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 17 04:28:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.557	3.699	534.3E6	678.3E6	15.461	14.020
2) SA Decachlor...	10.323	8.610	539.7E6	337.2E6	17.823	16.829

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR071618\
Data File : PR030373.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2018 06:45
Operator : MA/SM
Sample : LOD-LOQ BL WATER
Misc : 100PPB LOQ ECD_R WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
LOD-LOQ BL WATER

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 09:36:21 2018
Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_R\Method\PR071618.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 17 04:28:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

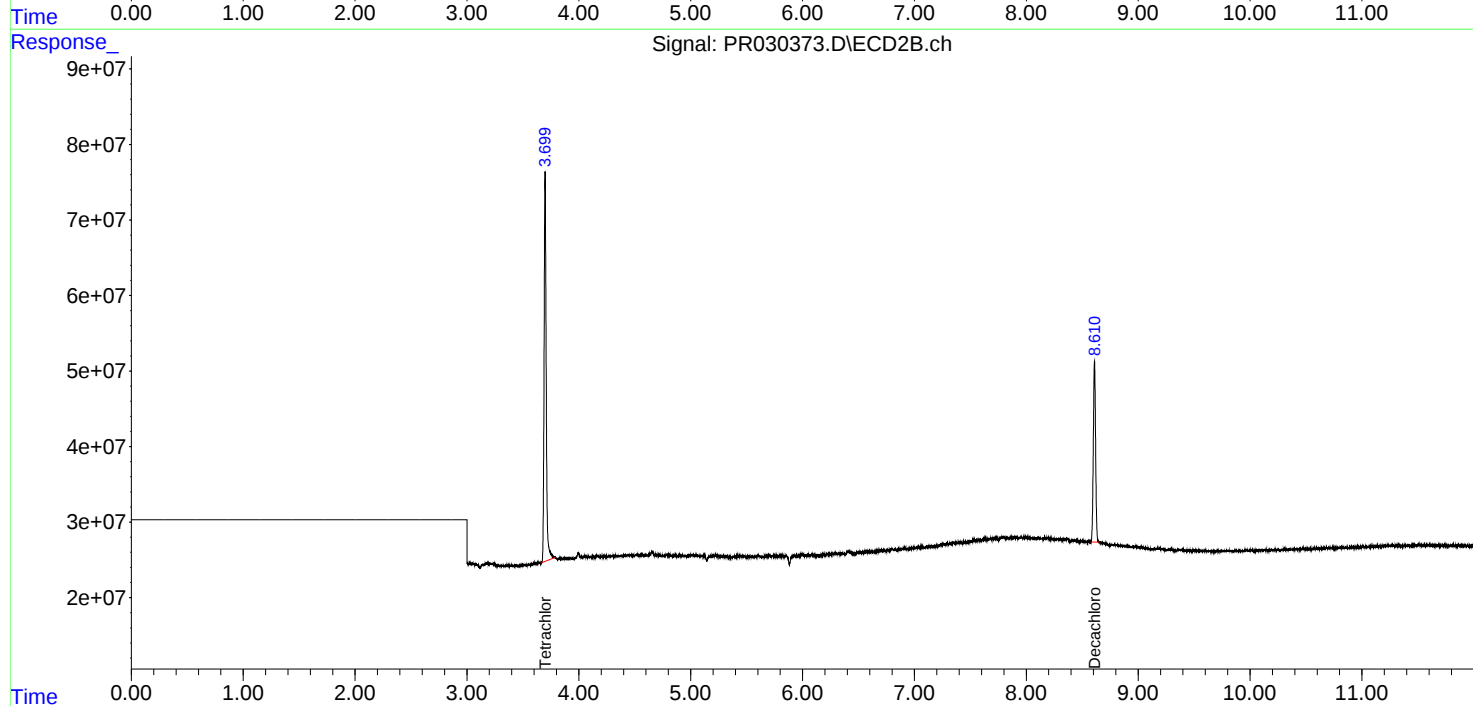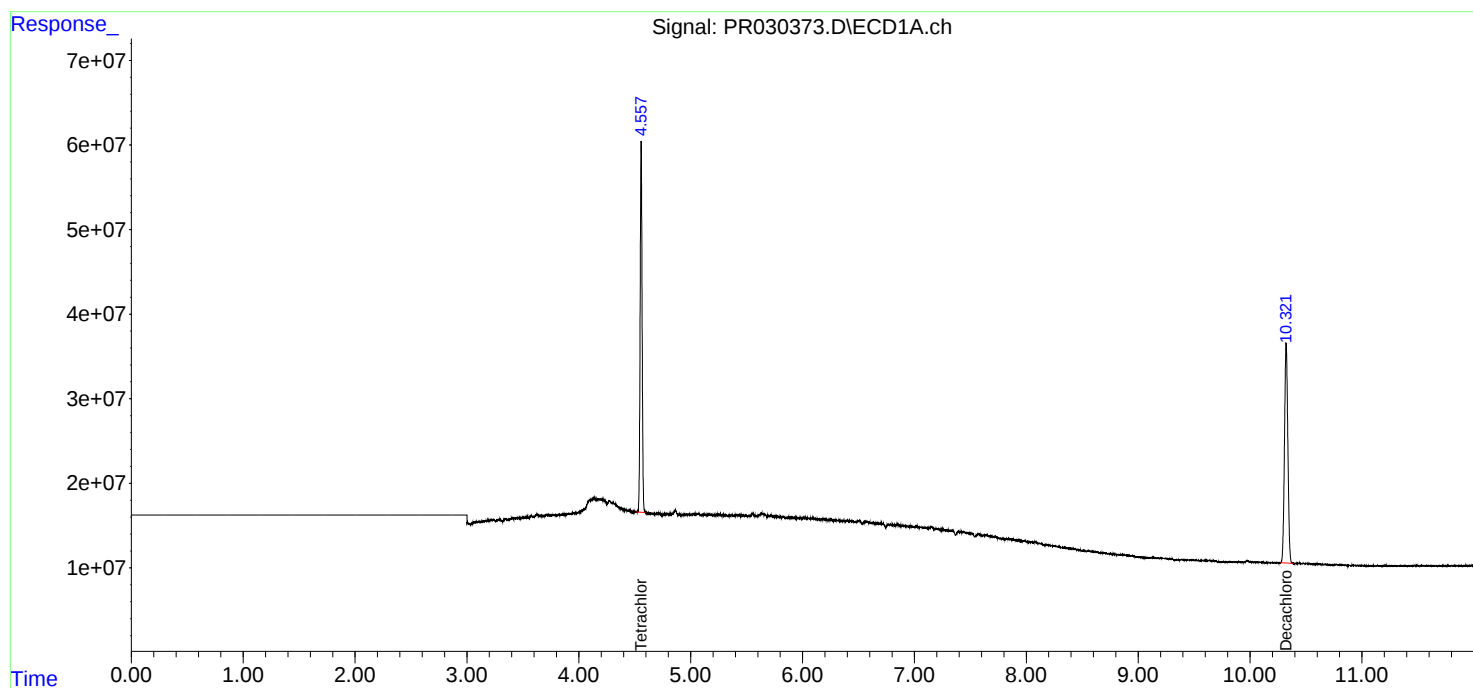


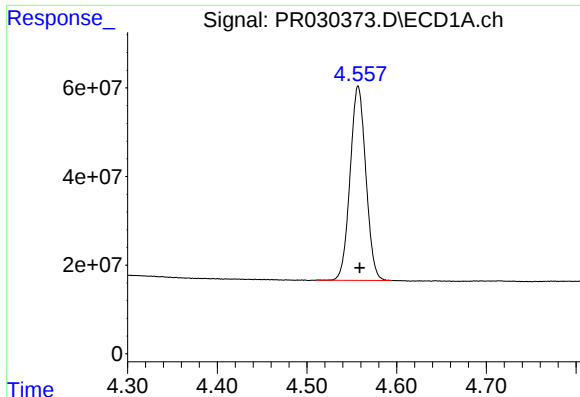

#1 Tetrachloro-m-xylene


R.T.: 4.557 min
Delta R.T.: -0.002 min
Response: 534276539
Conc: 15.46 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-LOQ BL WATER

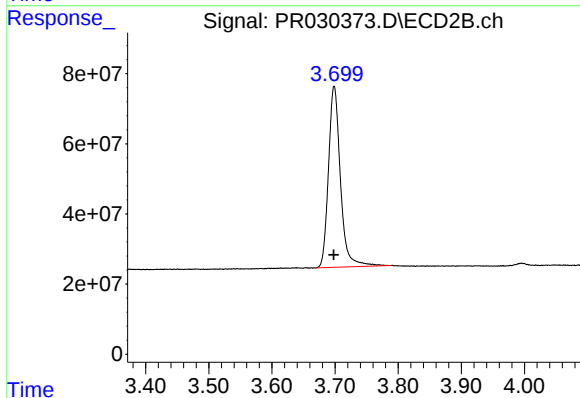


#1 Tetrachloro-m-xylene

R.T.: 3.699 min
Delta R.T.: 0.000 min
Response: 678261116
Conc: 14.02 ng/ml

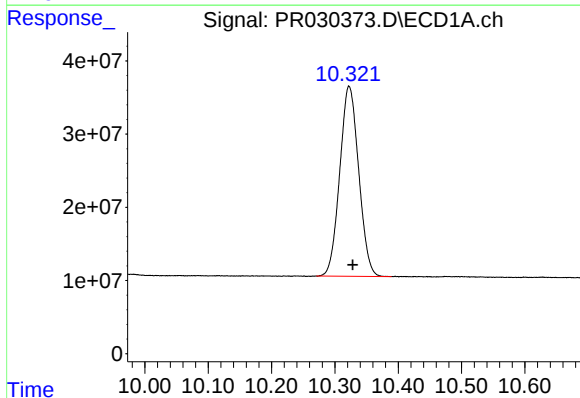

#2 Decachlorobiphenyl

R.T.: 10.323 min
Delta R.T.: -0.005 min
Response: 539671720
Conc: 17.82 ng/ml

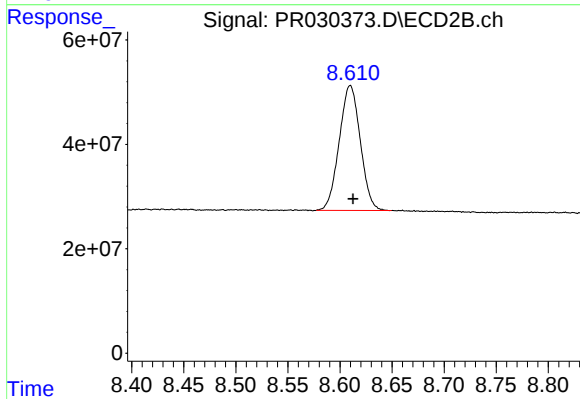

#2 Decachlorobiphenyl

R.T.: 8.610 min
Delta R.T.: -0.003 min
Response: 337156703
Conc: 16.83 ng/ml