

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR071719\
 Data File : PR039360.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2019 14:50
 Operator : SM\AJ
 Sample : K3740-04
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 COMP-23

Manual Integrations
 APPROVED

Ankita
 7/18/2019 4:56:49 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 15:18:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR071519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 16 02:56:01 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.765	4.610	44731318	148.9E6	28.879	23.020
2)	SA Decachlor...	8.703	10.346	65662090	254.9E6	26.852m	29.782
Target Compounds							
31)	L7 AR-1260-1	6.286	7.345	59943711	203.5E6	523.056	560.352
32)	L7 AR-1260-2	6.469	7.597	78475740	307.3E6	520.357m	702.583 #
33)	L7 AR-1260-3	6.622	7.953	63558053	157.9E6	472.258	465.386
34)	L7 AR-1260-4	7.088	8.183	46330566	217.1E6	387.086	534.304 #
35)	L7 AR-1260-5	7.325	8.509	133.2E6	421.0E6	443.345	492.287

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR071719\
Data File : PR039360.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2019 14:50
Operator : SM\AJ
Sample : K3740-04
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampled :
COMP-23


Manual Integrations
APPROVED

Ankita
7/18/2019 4:56:49 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 15:18:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR071519.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 16 02:56:01 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

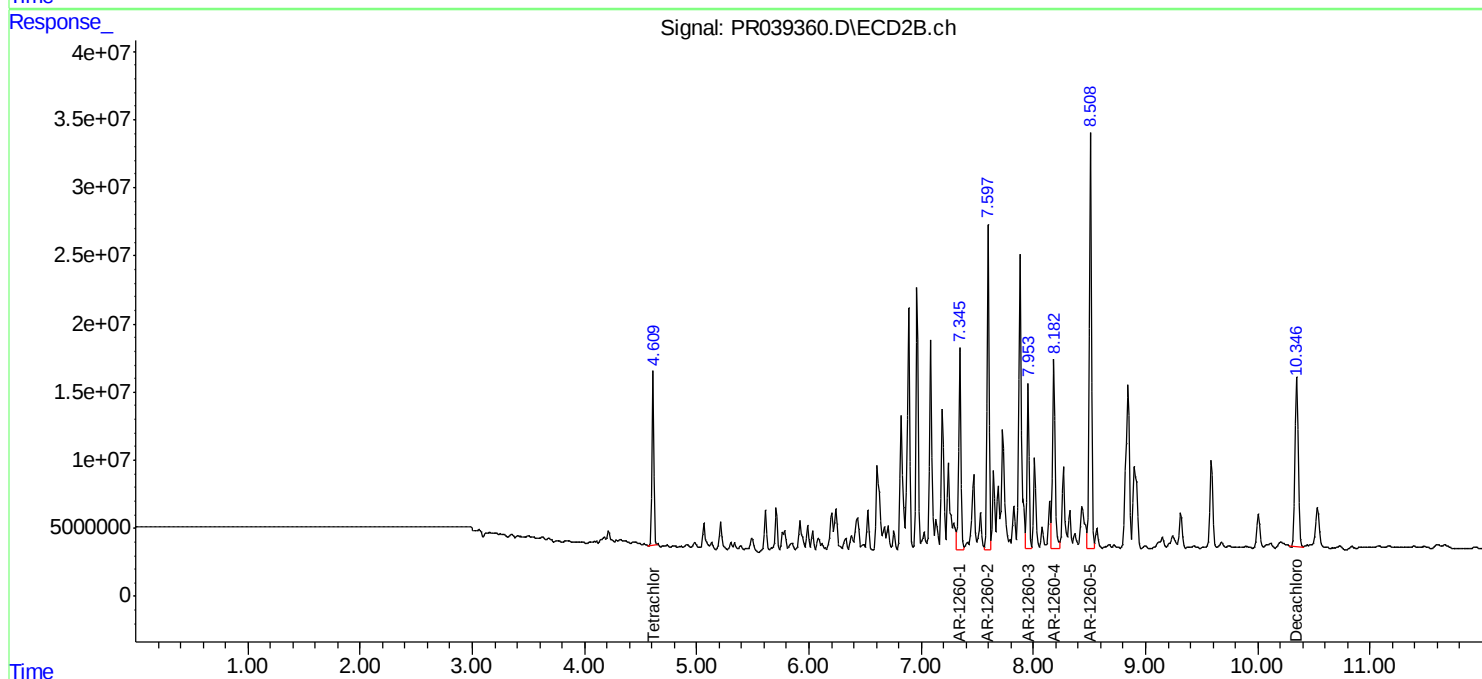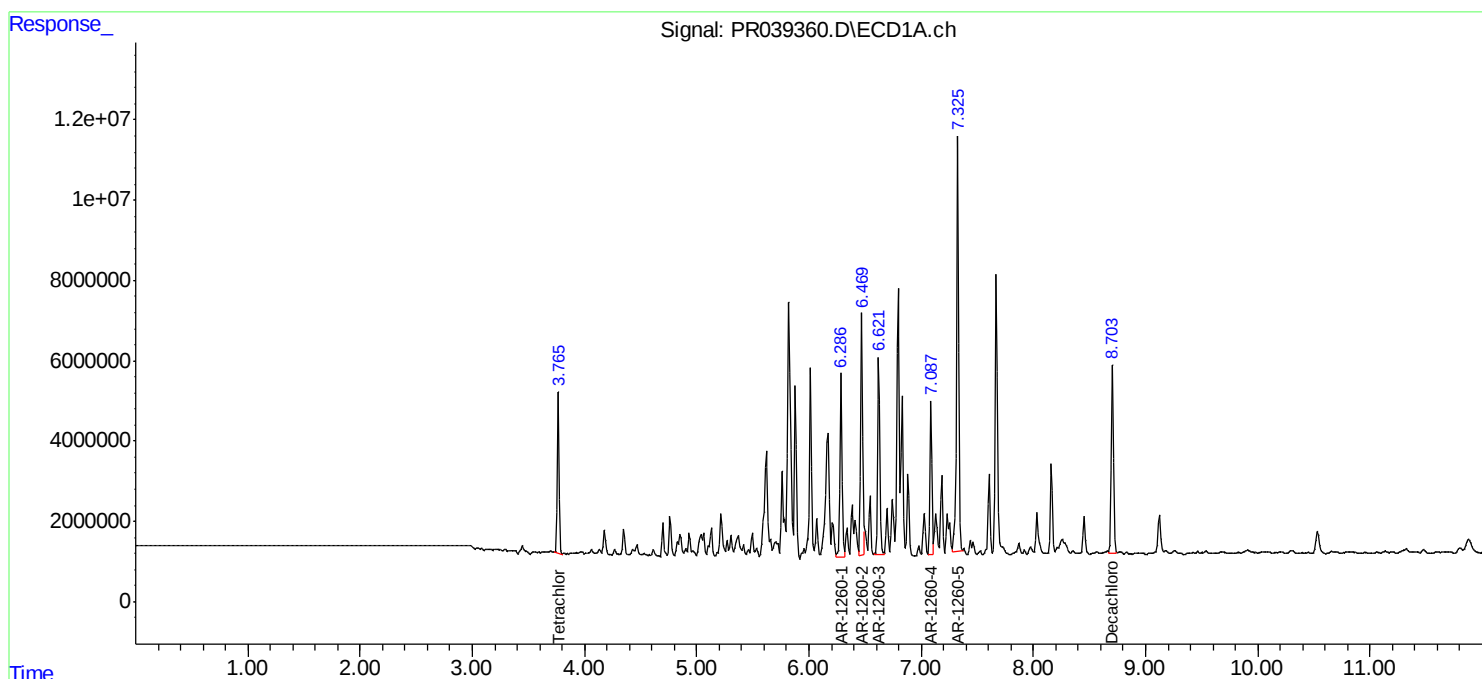

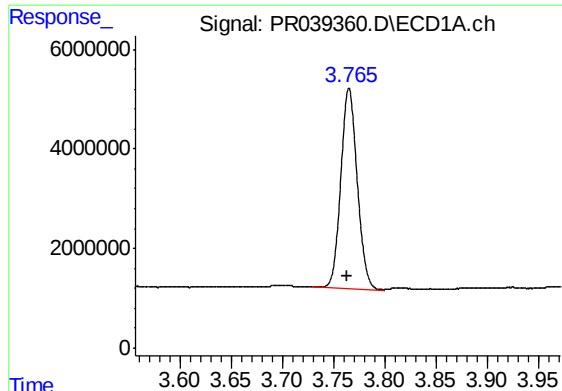


#1 Tetrachloro-m-xylene

R.T.: 3.765 min
Delta R.T.: 0.002 min
Response: 44731318
Conc: 28.88 ng/ml

Instrument :
ECD_R
ClientSampleId :
COMP-23


Manual Integrations
APPROVED

Ankita
7/18/2019 4:56:49 PM

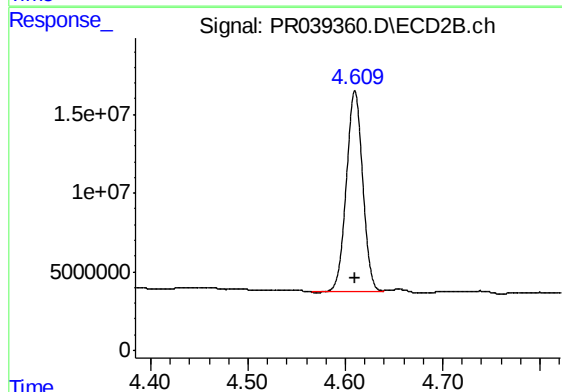


#1 Tetrachloro-m-xylene

R.T.: 4.610 min
Delta R.T.: 0.000 min
Response: 148878710
Conc: 23.02 ng/ml

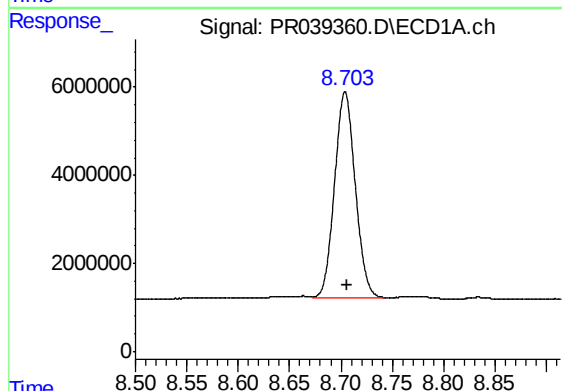


#2 Decachlorobiphenyl

R.T.: 8.703 min
Delta R.T.: -0.002 min
Response: 65662090
Conc: 26.85 ng/ml m

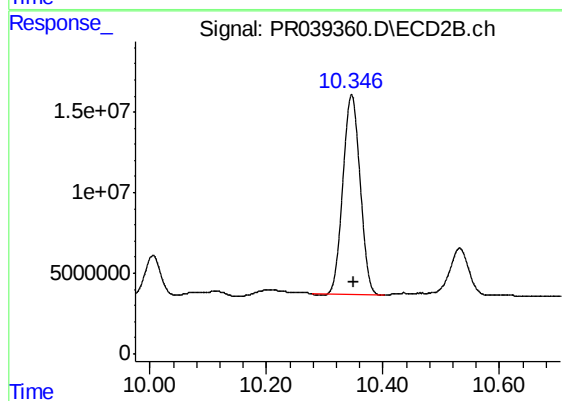

#2 Decachlorobiphenyl

R.T.: 10.346 min
Delta R.T.: -0.003 min
Response: 254867614
Conc: 29.78 ng/ml

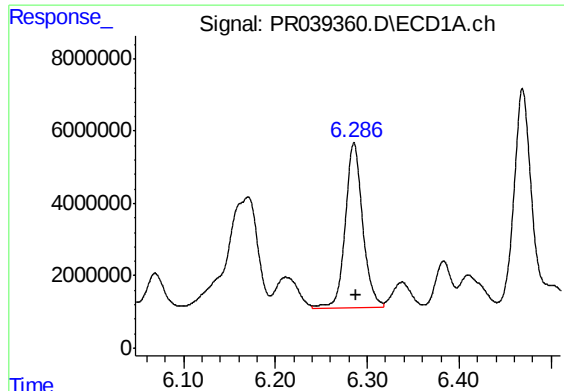


#31 AR-1260-1

R.T.: 6.286 min
Delta R.T.: -0.002 min
Response: 59943711
Conc: 523.06 ng/ml

Instrument :
ECD_R
ClientSampleId :
COMP-23


Manual Integrations
APPROVED

Ankita
7/18/2019 4:56:49 PM

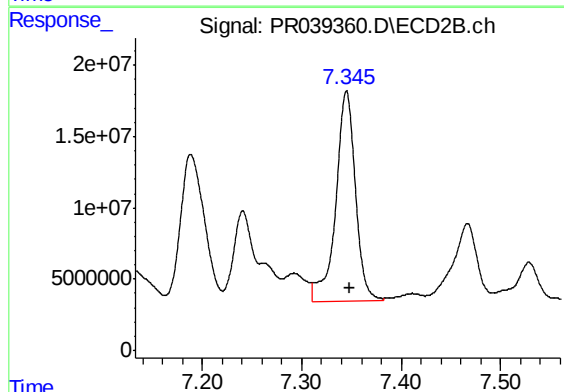


#31 AR-1260-1

R.T.: 7.345 min
Delta R.T.: -0.003 min
Response: 203480390
Conc: 560.35 ng/ml

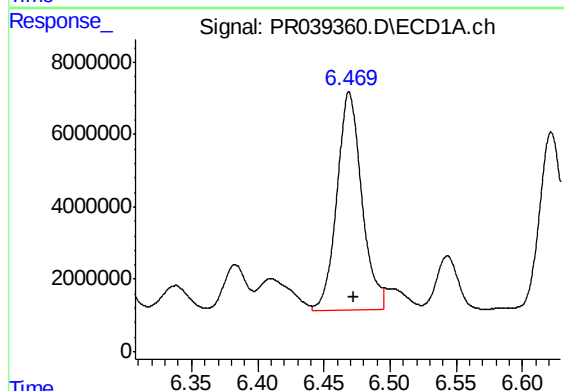


#32 AR-1260-2

R.T.: 6.469 min
Delta R.T.: -0.003 min
Response: 78475740
Conc: 520.36 ng/ml m

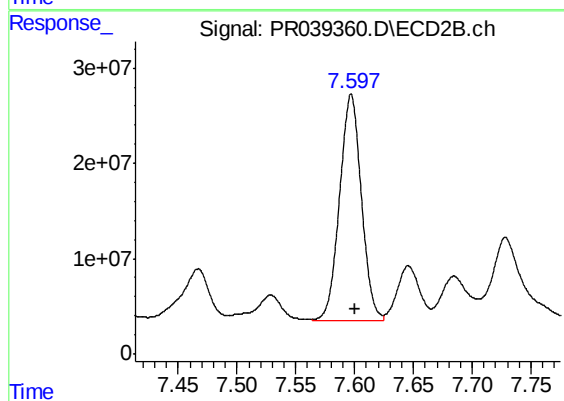

#32 AR-1260-2

R.T.: 7.597 min
Delta R.T.: -0.003 min
Response: 307312762
Conc: 702.58 ng/ml

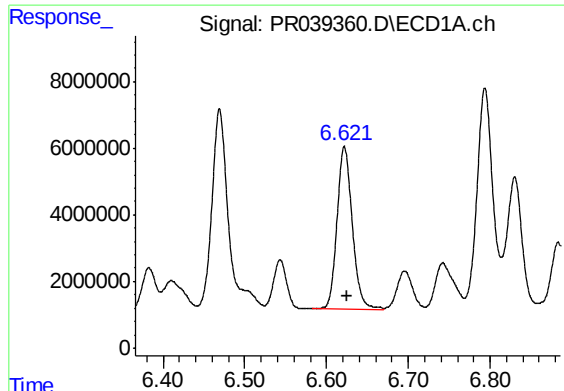


#33 AR-1260-3

R.T.: 6.622 min
Delta R.T.: -0.003 min
Response: 63558053
Conc: 472.26 ng/ml

Instrument :
ECD_R
ClientSampleId :
COMP-23


Manual Integrations
APPROVED

Ankita
7/18/2019 4:56:49 PM

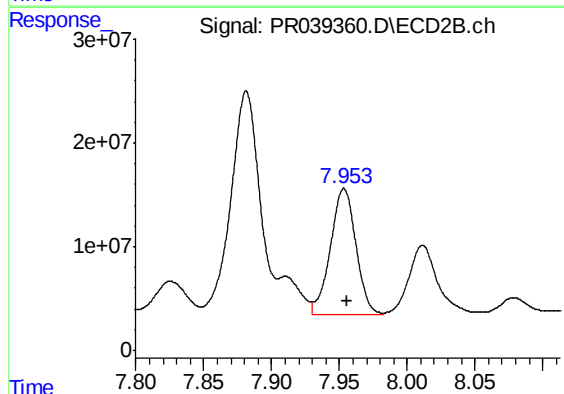


#33 AR-1260-3

R.T.: 7.953 min
Delta R.T.: -0.002 min
Response: 157942555
Conc: 465.39 ng/ml

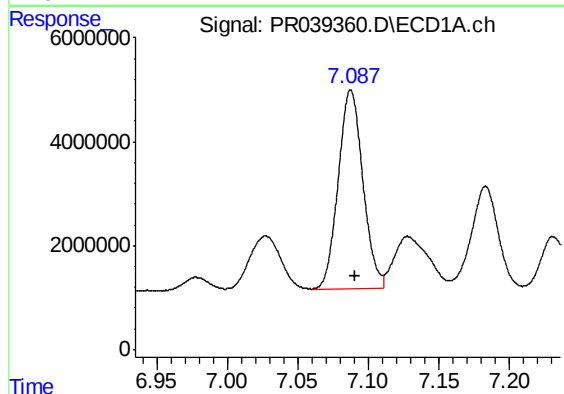


#34 AR-1260-4

R.T.: 7.088 min
Delta R.T.: -0.002 min
Response: 46330566
Conc: 387.09 ng/ml

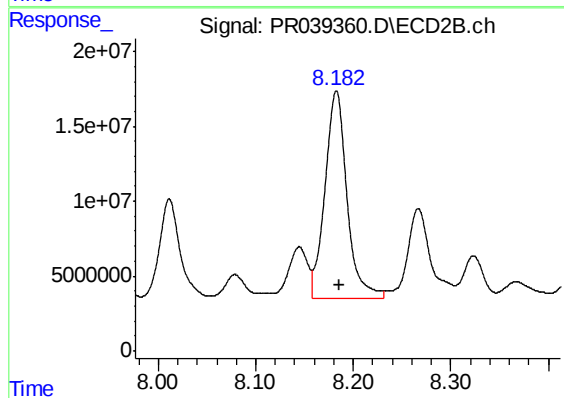

#34 AR-1260-4

R.T.: 8.183 min
Delta R.T.: -0.003 min
Response: 217128182
Conc: 534.30 ng/ml

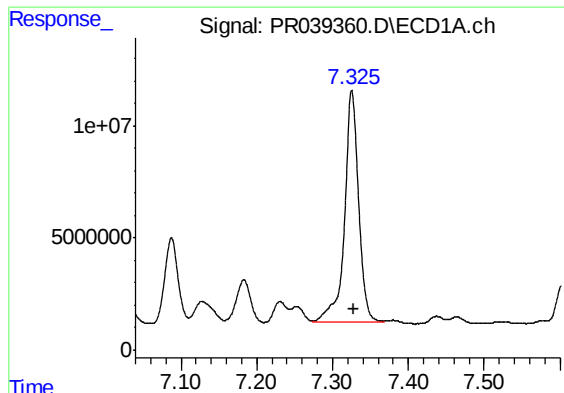


#35 AR-1260-5

R.T.: 7.325 min
Delta R.T.: -0.003 min
Response: 133239690
Conc: 443.35 ng/ml

Instrument :
ECD_R
ClientSampleId :
COMP-23

Manual Integrations
APPROVED

Ankita
7/18/2019 4:56:49 PM

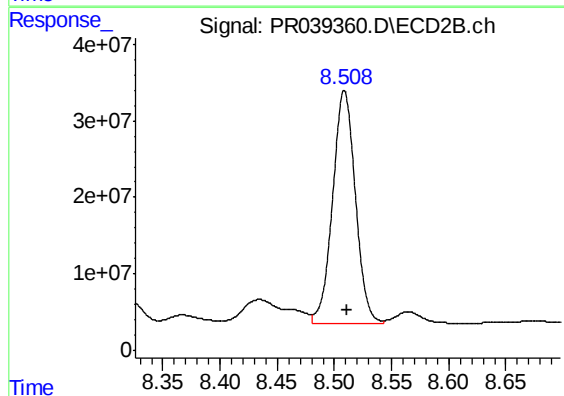

#35 AR-1260-5

R.T.: 8.509 min
Delta R.T.: -0.003 min
Response: 420977893
Conc: 492.29 ng/ml