

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR071719\
 Data File : PR039361.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2019 15:09
 Operator : SM\AJ
 Sample : K3740-04RE
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 COMP-23RE

Manual Integrations
 APPROVED

Ankita
 7/18/2019 4:56:51 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 15:21:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR071519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 16 02:56:01 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.768	4.610	47501321	153.5E6	30.668	23.734
2)	SA Decachlor...	8.711	10.350	64969329	253.0E6	26.569m	29.561
Target Compounds							
31)	L7 AR-1260-1	6.291	7.348	64835655	209.5E6	565.742	576.971
32)	L7 AR-1260-2	6.475	7.600	87560198	317.5E6	580.594m	725.979 #
33)	L7 AR-1260-3	6.628	7.956	68601616	161.9E6	509.733	476.906
34)	L7 AR-1260-4	7.094	8.185	48475512	223.5E6	405.007	550.034 #
35)	L7 AR-1260-5	7.333	8.512	136.1E6	440.6E6	452.737	515.204

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR071719\
Data File : PR039361.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2019 15:09
Operator : SM\AJ
Sample : K3740-04RE
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampled :
COMP-23RE


Manual Integrations
APPROVED

Ankita
7/18/2019 4:56:51 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 15:21:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR071519.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 16 02:56:01 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

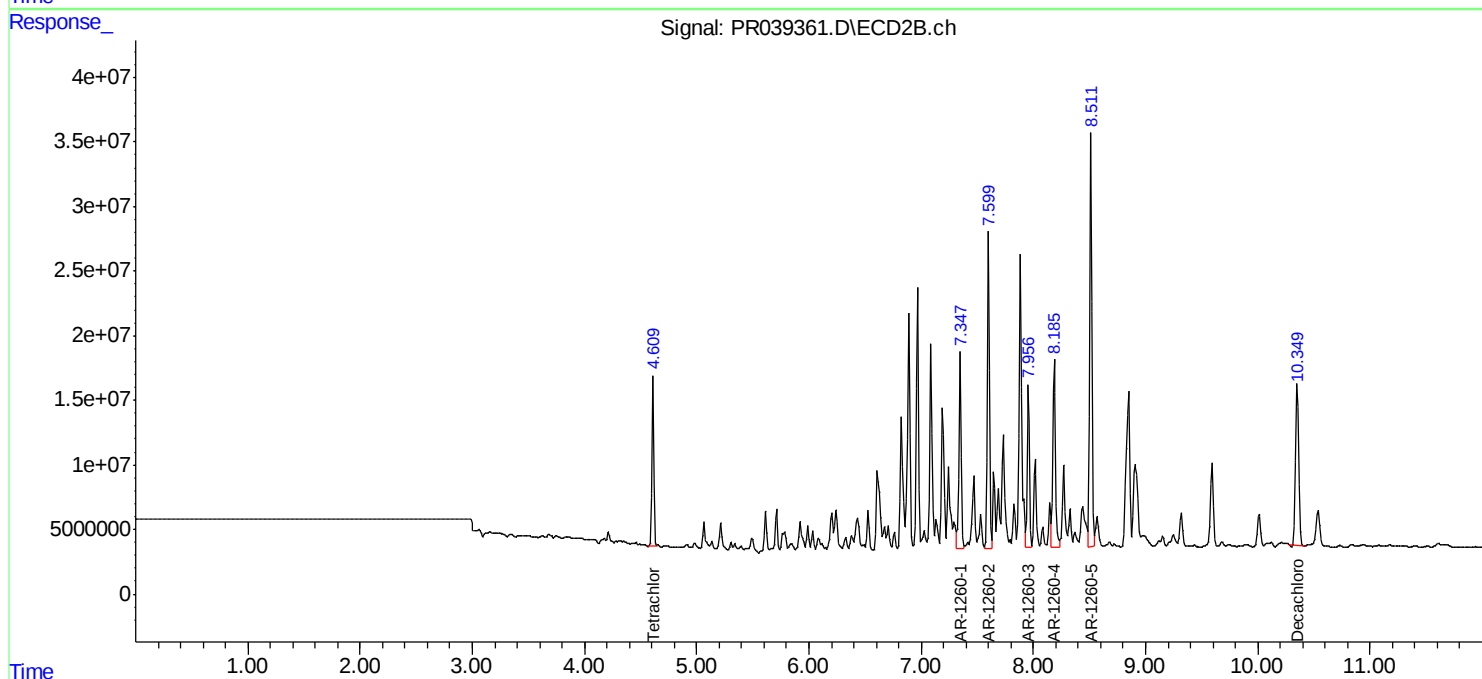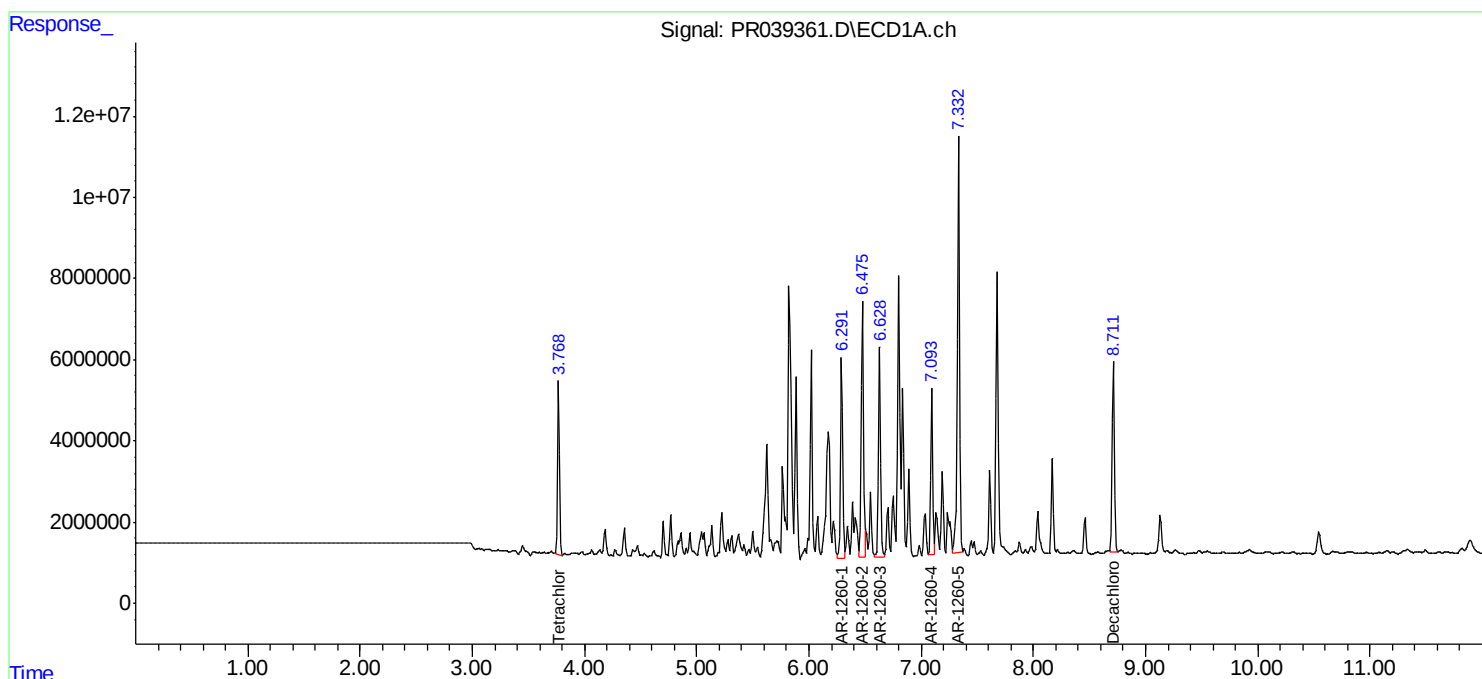

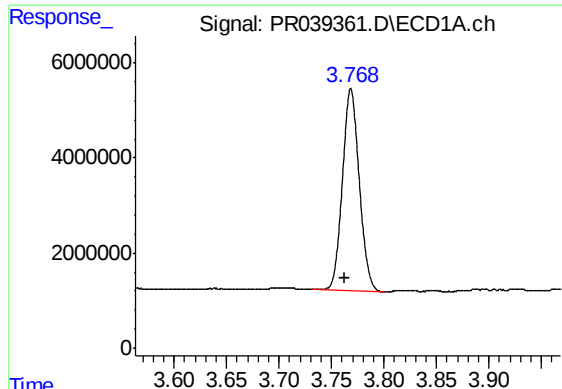


#1 Tetrachloro-m-xylene

R.T.: 3.768 min
Delta R.T.: 0.005 min
Response: 47501321
Conc: 30.67 ng/ml

Instrument :
ECD_R
ClientSampleId :
COMP-23RE


Manual Integrations
APPROVED

Ankita
7/18/2019 4:56:51 PM

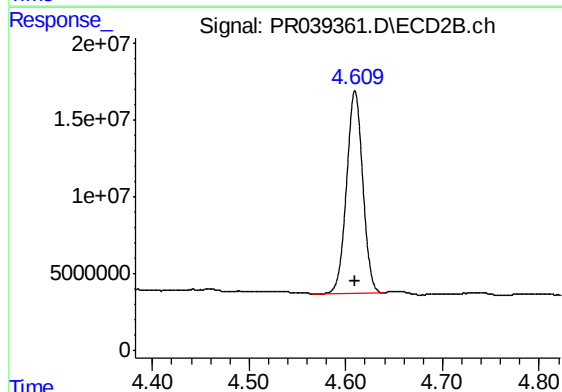


#1 Tetrachloro-m-xylene

R.T.: 4.610 min
Delta R.T.: 0.000 min
Response: 153493329
Conc: 23.73 ng/ml

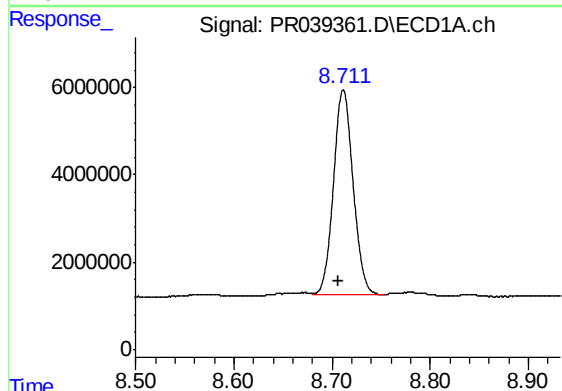


#2 Decachlorobiphenyl

R.T.: 8.711 min
Delta R.T.: 0.005 min
Response: 64969329
Conc: 26.57 ng/ml m

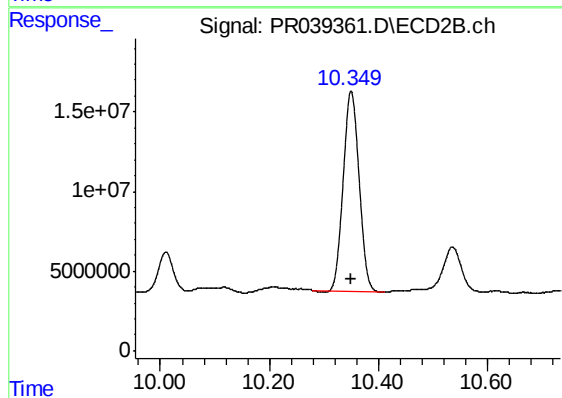

#2 Decachlorobiphenyl

R.T.: 10.350 min
Delta R.T.: 0.000 min
Response: 252976095
Conc: 29.56 ng/ml

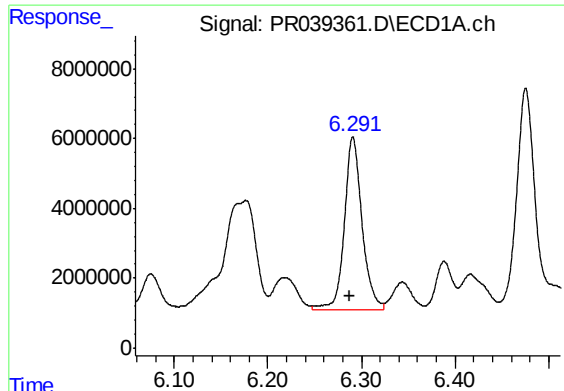


#31 AR-1260-1

R.T.: 6.291 min
Delta R.T.: 0.003 min
Response: 64835655
Conc: 565.74 ng/ml

Instrument :
ECD_R
ClientSampleId :
COMP-23RE


Manual Integrations
APPROVED

Ankita
7/18/2019 4:56:51 PM

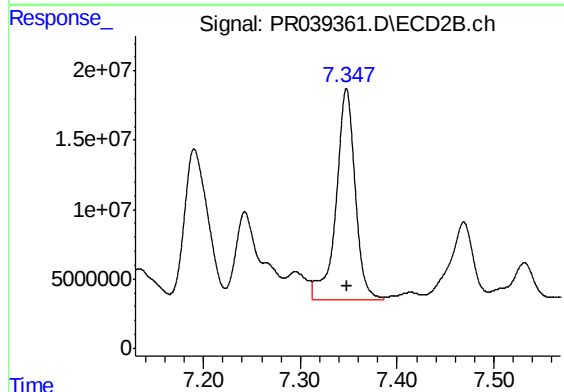


#31 AR-1260-1

R.T.: 7.348 min
Delta R.T.: 0.000 min
Response: 209515359
Conc: 576.97 ng/ml

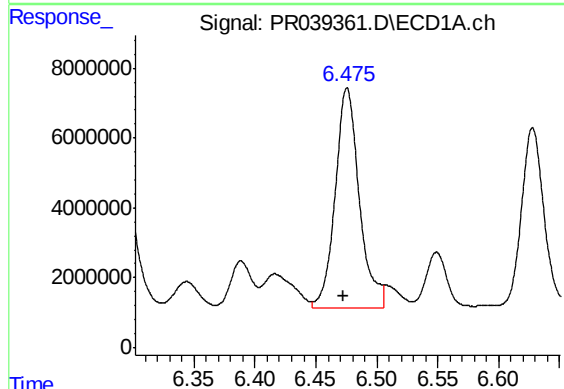


#32 AR-1260-2

R.T.: 6.475 min
Delta R.T.: 0.003 min
Response: 87560198
Conc: 580.59 ng/ml m

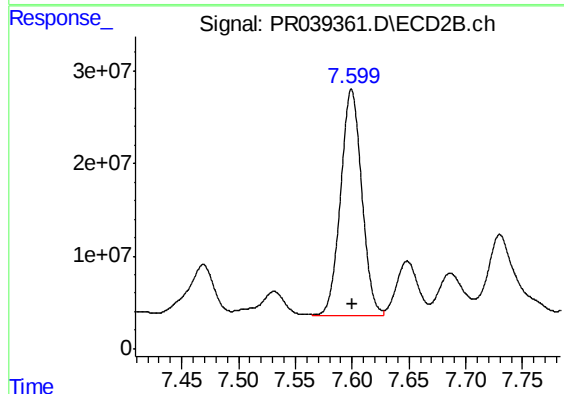

#32 AR-1260-2

R.T.: 7.600 min
Delta R.T.: 0.000 min
Response: 317545958
Conc: 725.98 ng/ml

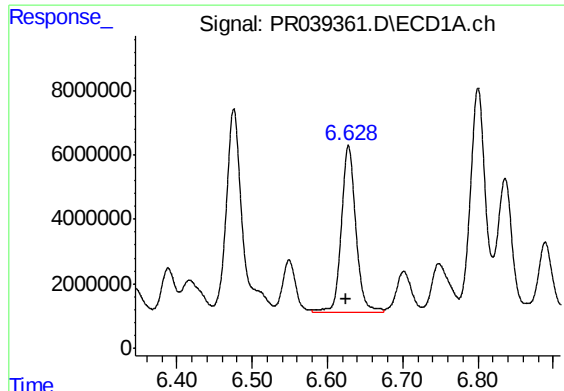


#33 AR-1260-3

R.T.: 6.628 min
Delta R.T.: 0.003 min
Response: 68601616
Conc: 509.73 ng/ml

Instrument :
ECD_R
ClientSampleId :
COMP-23RE


Manual Integrations
APPROVED

Ankita
7/18/2019 4:56:51 PM

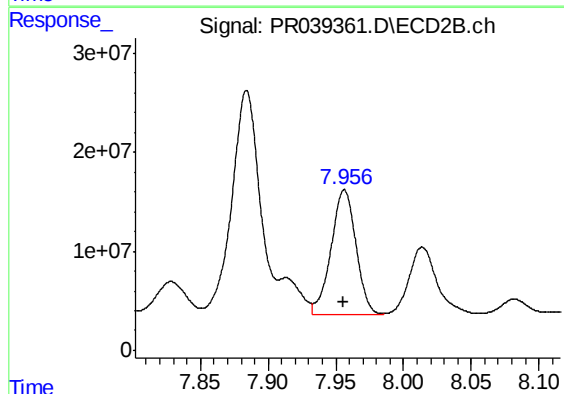


#33 AR-1260-3

R.T.: 7.956 min
Delta R.T.: 0.000 min
Response: 161852027
Conc: 476.91 ng/ml

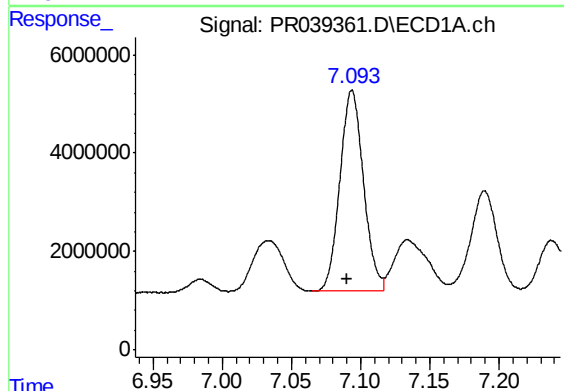


#34 AR-1260-4

R.T.: 7.094 min
Delta R.T.: 0.004 min
Response: 48475512
Conc: 405.01 ng/ml

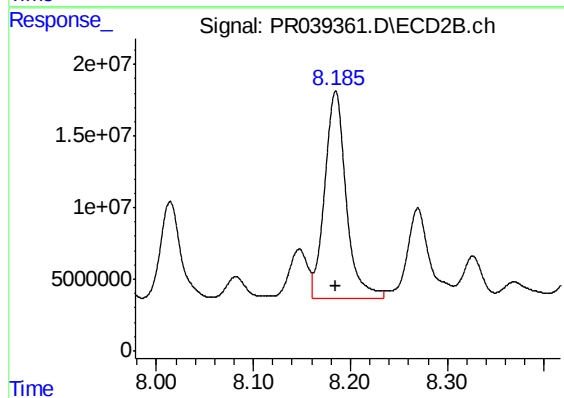

#34 AR-1260-4

R.T.: 8.185 min
Delta R.T.: 0.000 min
Response: 223520761
Conc: 550.03 ng/ml

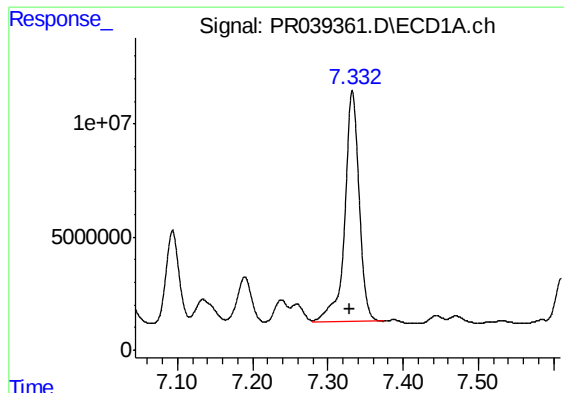


#35 AR-1260-5

R.T.: 7.333 min
Delta R.T.: 0.004 min
Response: 136062256
Conc: 452.74 ng/ml

Instrument :
ECD_R
ClientSampleId :
COMP-23RE

Manual Integrations
APPROVED

Ankita
7/18/2019 4:56:51 PM

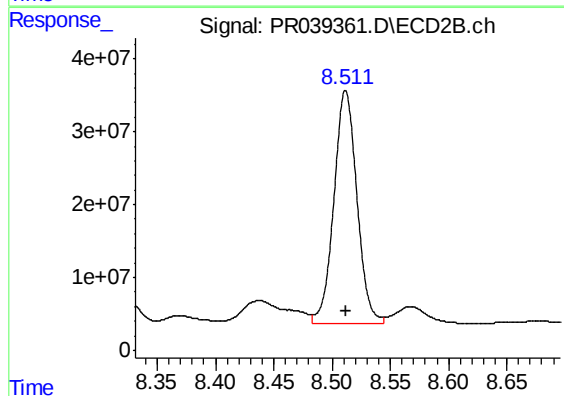

#35 AR-1260-5

R.T.: 8.512 min
Delta R.T.: 0.000 min
Response: 440575434
Conc: 515.20 ng/ml