

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR071919\
 Data File : PR039440.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jul 2019 11:55
 Operator : SM\AJ
 Sample : K3838-03RE
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 WARINANCO-CITY-SEWER-INSTAL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 12:19:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR071519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 16 02:56:01 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.764	4.605	21366816	93800148	13.795	14.504
2) SA Decachlor...	8.707	10.347	17295005	50853067	7.073	5.942
Target Compounds						
3) L1 AR-1016-1	4.840	0.000	14940077	0	248.441	N.D. #
4) L1 AR-1016-2	4.840	0.000	14940077	0	152.088	N.D. #
12) L3 AR-1232-2	4.840	5.535	14940077	7554778	404.726	126.043 #
16) L4 AR-1242-1	4.840	0.000	14940077	0	282.763	N.D. #
17) L4 AR-1242-2	4.840	0.000	14940077	0	171.433	N.D. #
21) L5 AR-1248-1	4.840	0.000	14940077	0	345.191	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR071919\
Data File : PR039440.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jul 2019 11:55
Operator : SM\AJ
Sample : K3838-03RE
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
WARINANCO-CITY-SEWER-INSTAL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 12:19:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR071519.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 16 02:56:01 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

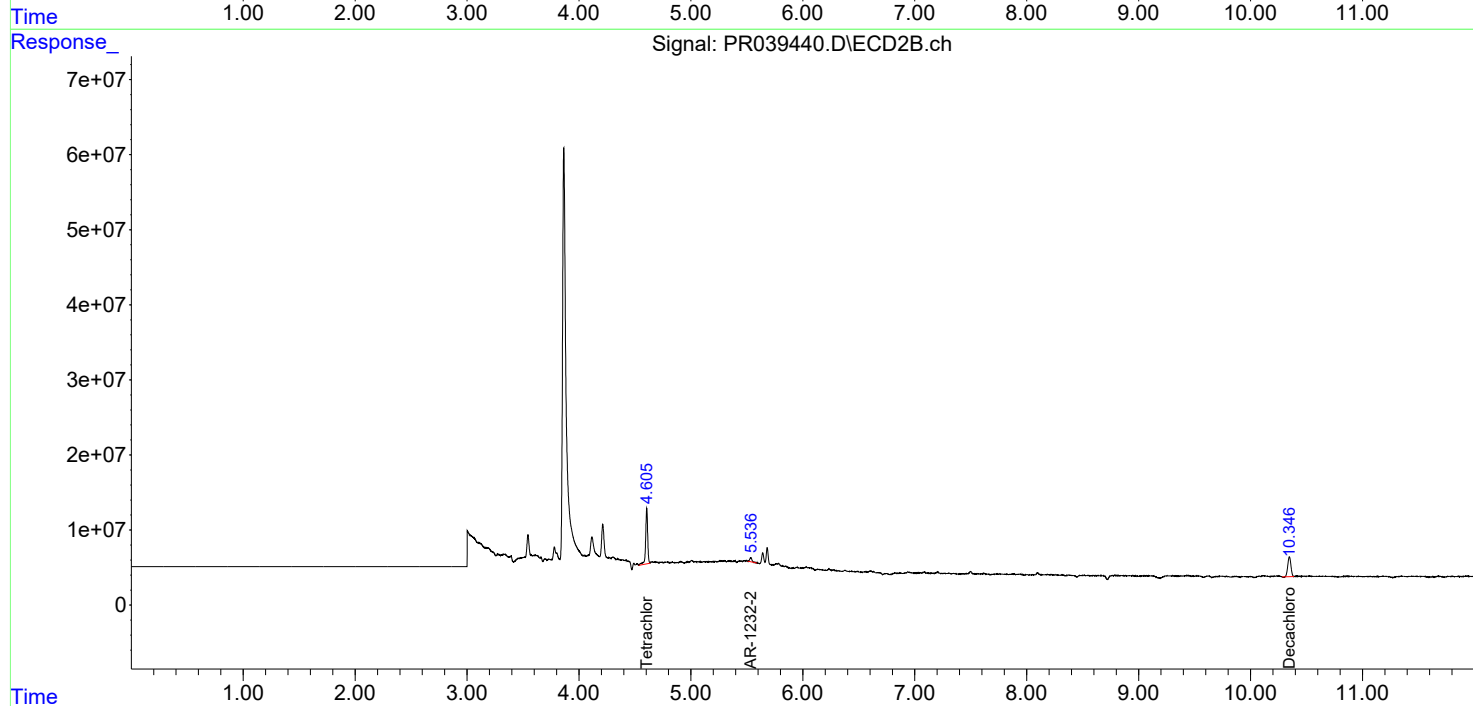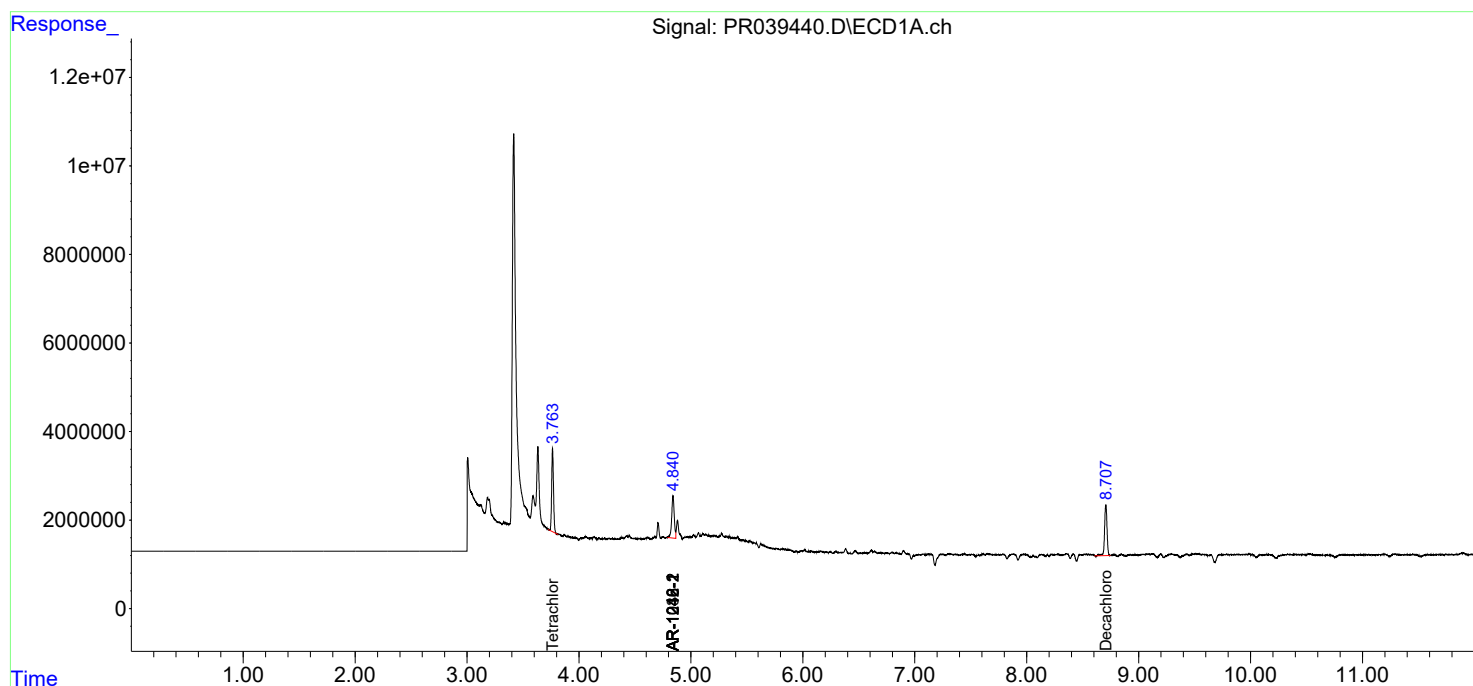


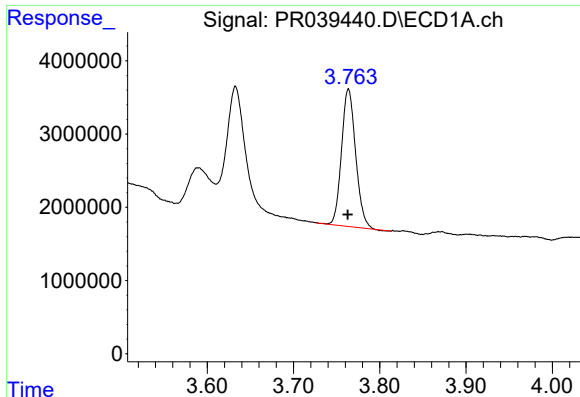

#1 Tetrachloro-m-xylene


R.T.: 3.764 min
Delta R.T.: 0.000 min
Response: 21366816
Conc: 13.79 ng/ml

Instrument :
ECD_R
ClientSampleId :
WARINANCO-CITY-SEWER-INSTAL

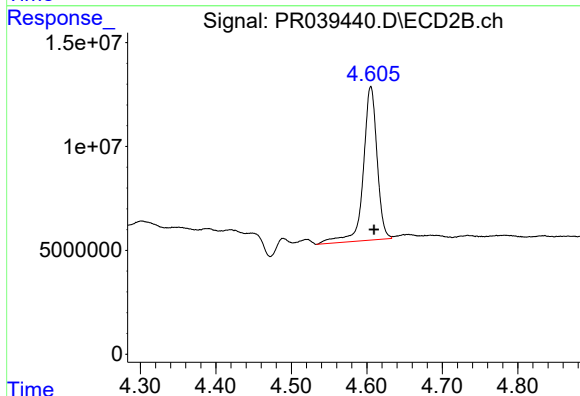


#1 Tetrachloro-m-xylene

R.T.: 4.605 min
Delta R.T.: -0.005 min
Response: 93800148
Conc: 14.50 ng/ml

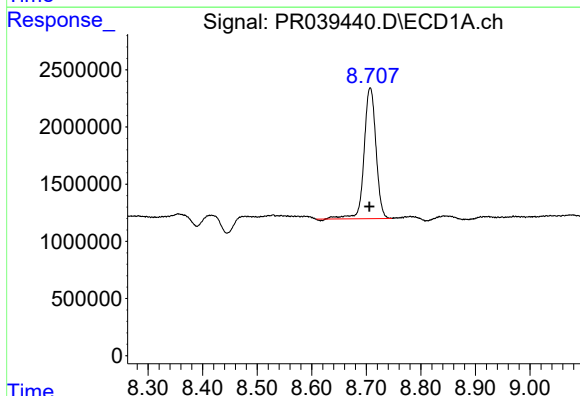


#2 Decachlorobiphenyl

R.T.: 8.707 min
Delta R.T.: 0.001 min
Response: 17295005
Conc: 7.07 ng/ml

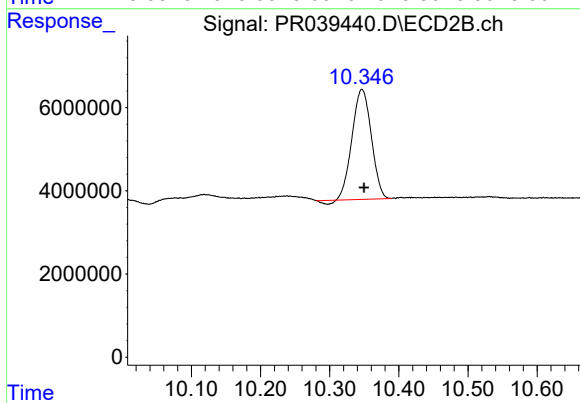

#2 Decachlorobiphenyl


R.T.: 10.347 min
Delta R.T.: -0.003 min
Response: 50853067
Conc: 5.94 ng/ml

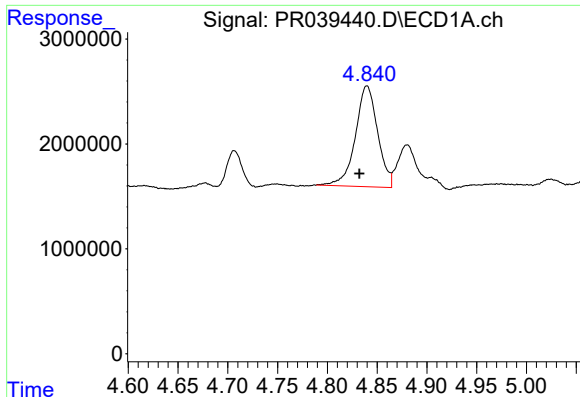

#3 AR-1016-1


R.T.: 4.840 min
Delta R.T.: 0.007 min
Response: 14940077
Conc: 248.44 ng/ml

Instrument :
ECD_R
ClientSampleId :
WARINANCO-CITY-SEWER-INSTAL

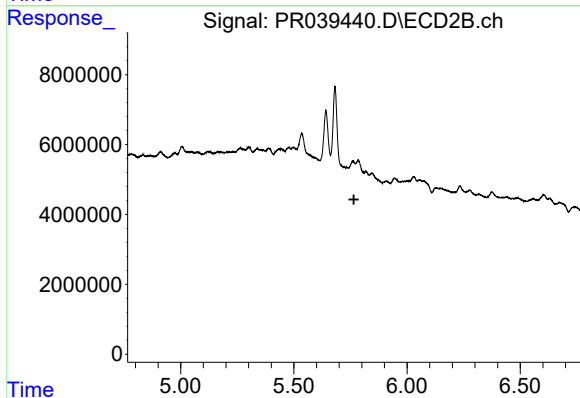


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 5.765 min
Response: 0
Conc: N.D.

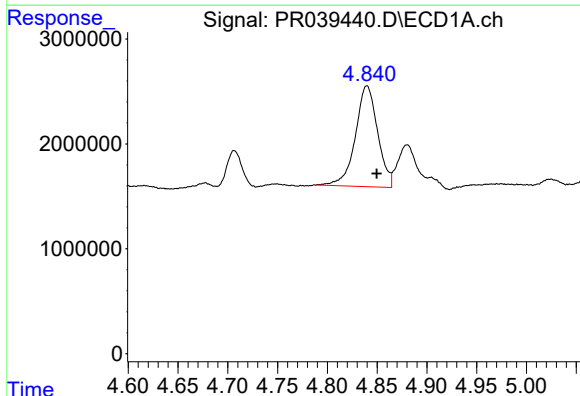


#4 AR-1016-2

R.T.: 4.840 min
Delta R.T.: -0.010 min
Response: 14940077
Conc: 152.09 ng/ml

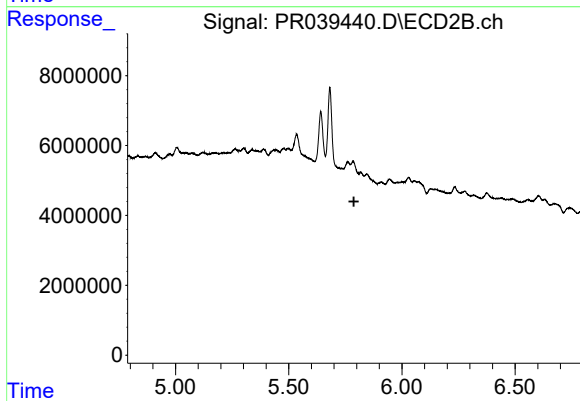

#4 AR-1016-2


R.T.: 0.000 min
Exp R.T. : 5.788 min
Response: 0
Conc: N.D.

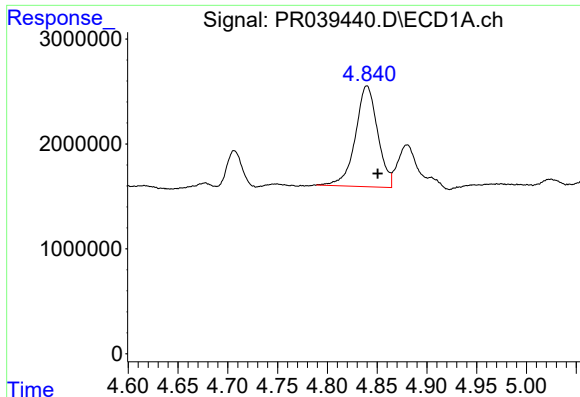

#12 AR-1232-2


R.T.: 4.840 min
Delta R.T.: -0.011 min
Response: 14940077
Conc: 404.73 ng/ml

Instrument :
ECD_R
ClientSampleId :
WARINANCO-CITY-SEWER-INSTAL

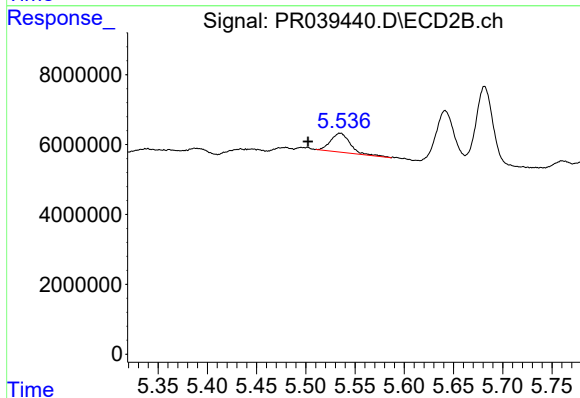


#12 AR-1232-2

R.T.: 5.535 min
Delta R.T.: 0.032 min
Response: 7554778
Conc: 126.04 ng/ml

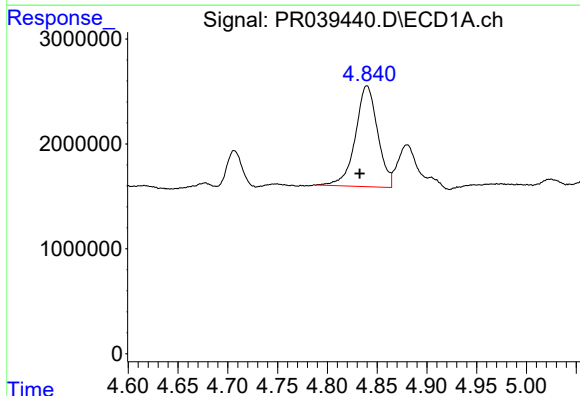


#16 AR-1242-1

R.T.: 4.840 min
Delta R.T.: 0.007 min
Response: 14940077
Conc: 282.76 ng/ml

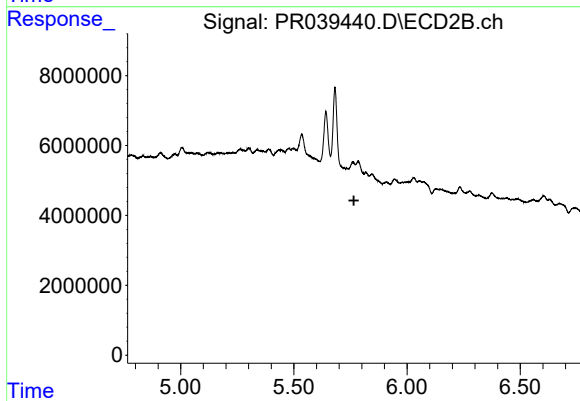

#16 AR-1242-1


R.T.: 0.000 min
Exp R.T.: 5.765 min
Response: 0
Conc: N.D.

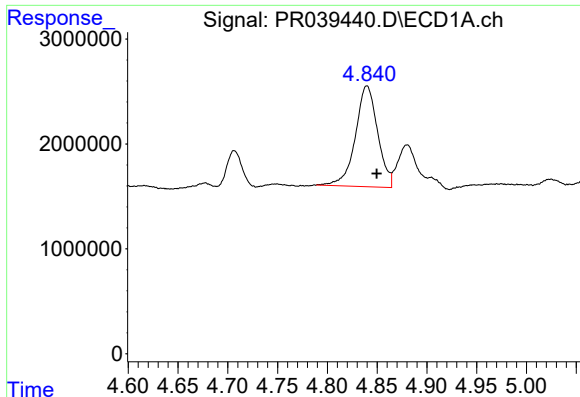

#17 AR-1242-2


R.T.: 4.840 min
Delta R.T.: -0.010 min
Response: 14940077
Conc: 171.43 ng/ml

Instrument :
ECD_R
ClientSampleId :
WARINANCO-CITY-SEWER-INSTAL

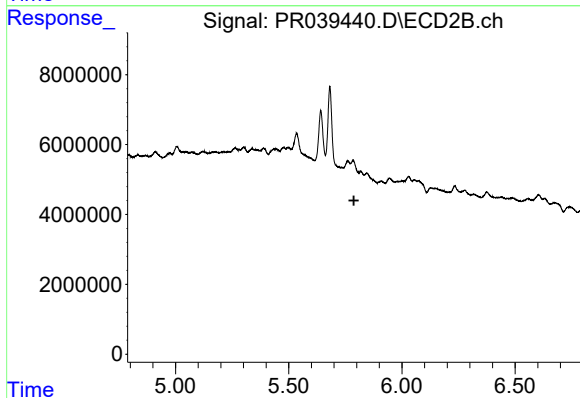


#17 AR-1242-2

R.T.: 0.000 min
Exp R.T. : 5.788 min
Response: 0
Conc: N.D.

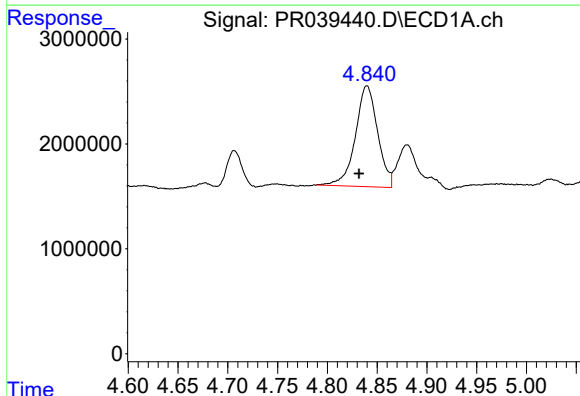

#21 AR-1248-1

R.T.: 4.840 min
Delta R.T.: 0.008 min
Response: 14940077
Conc: 345.19 ng/ml

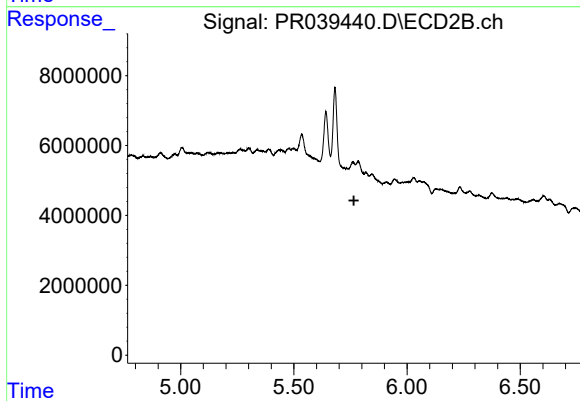

#21 AR-1248-1

R.T.: 0.000 min
Exp R.T. : 5.765 min
Response: 0
Conc: N.D.