

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR071919\
 Data File : PR039440.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jul 2019 11:55
 Operator : SM\AJ
 Sample : K3838-03RE
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 WARINANCO-CITY-SEWER-INSTAL

Manual Integrations
 APPROVED

Ankita
 7/21/2019 11:56:59 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 12:19:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR071519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 16 02:56:01 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.764	4.605	21366816	83577912	13.795	12.923m
2)	SA Decachlor...	8.707	10.346	16655835	53813881	6.811m	6.288m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR071919\
Data File : PR039440.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jul 2019 11:55
Operator : SM\AJ
Sample : K3838-03RE
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
WARINANCO-CITY-SEWER-INSTAL


Manual Integrations
APPROVED

Ankita
7/21/2019 11:56:59 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 12:19:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR071519.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 16 02:56:01 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

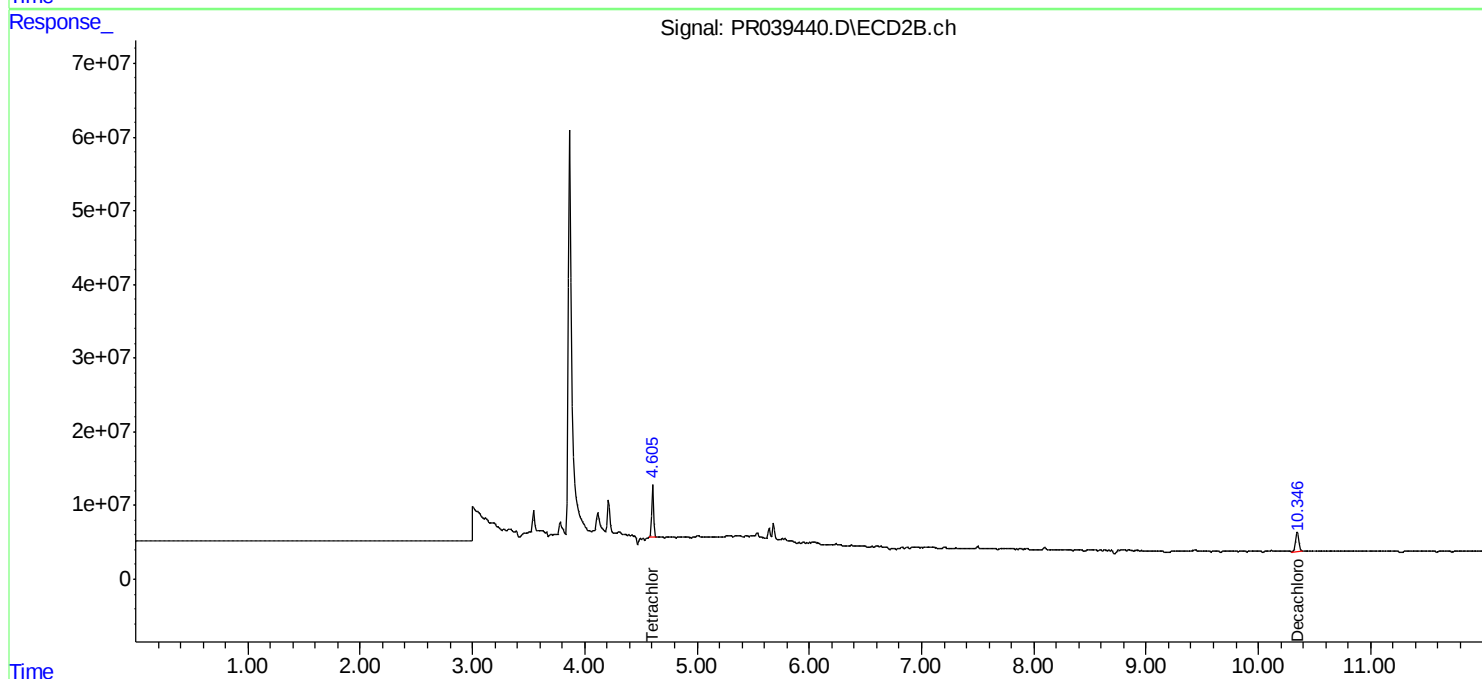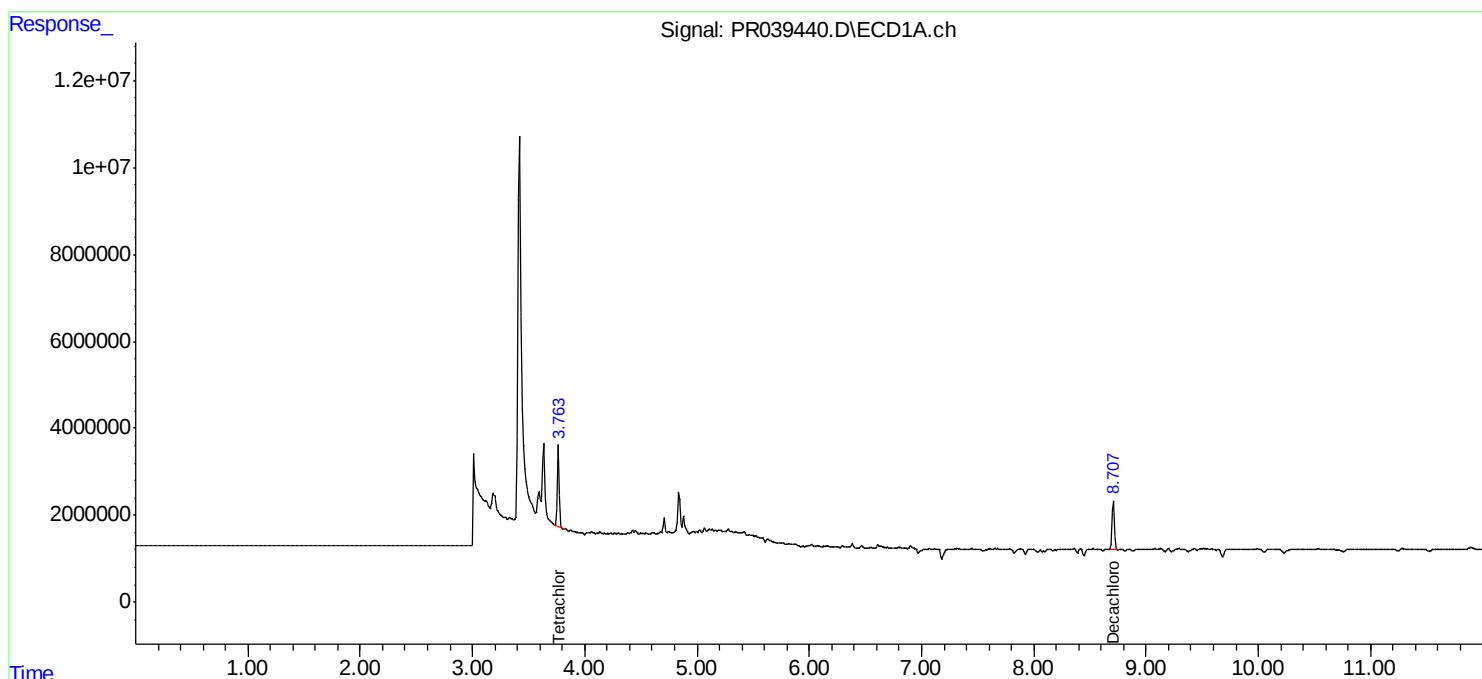

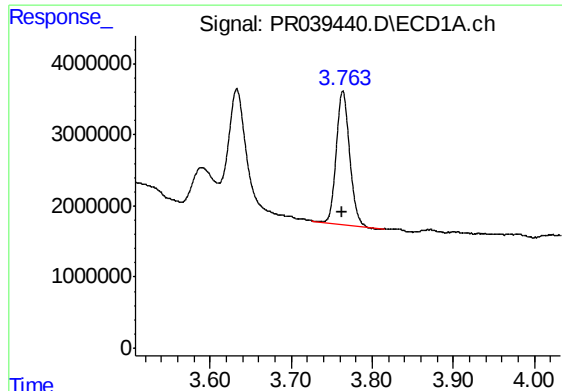


#1 Tetrachloro-m-xylene

R.T.: 3.764 min
Delta R.T.: 0.000 min
Response: 21366816
Conc: 13.79 ng/ml

Instrument :
ECD_R
ClientSampleId :
WARINANCO-CITY-SEWER-INSTAL


Manual Integrations
APPROVED

Ankita
7/21/2019 11:56:59 AM

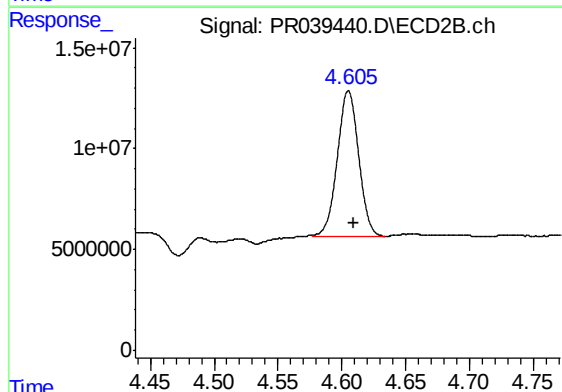


#1 Tetrachloro-m-xylene

R.T.: 4.605 min
Delta R.T.: -0.005 min
Response: 83577912
Conc: 12.92 ng/ml m

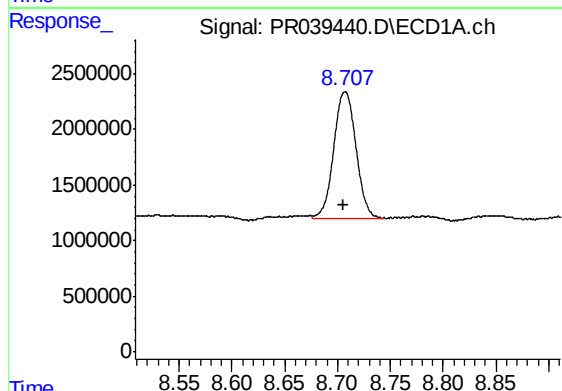

#2 Decachlorobiphenyl

R.T.: 8.707 min
Delta R.T.: 0.000 min
Response: 16655835
Conc: 6.81 ng/ml m

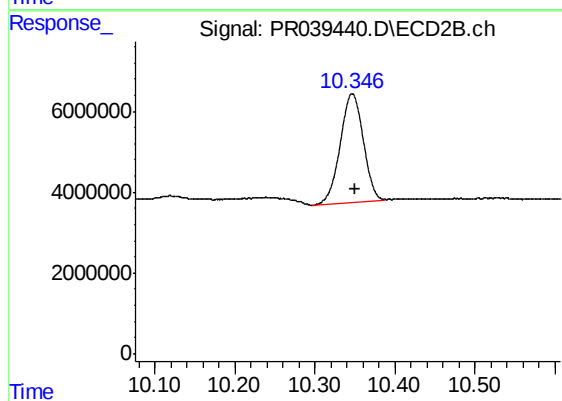

#2 Decachlorobiphenyl

R.T.: 10.346 min
Delta R.T.: -0.004 min
Response: 53813881
Conc: 6.29 ng/ml m