

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR071919\
 Data File : PR039451.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jul 2019 16:18
 Operator : SM\AJ
 Sample : K3896-08DL 4X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 TRAN-105DL

Manual Integrations
 APPROVED

Ankita
 7/21/2019 11:57:09 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 16:54:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR071519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 16 02:56:01 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.772	4.610	9203775	34797899	5.942m	5.381m
2)	SA Decachlor...	8.707	10.348	10234372	43748708	4.185	5.112
Target Compounds							
31)	L7 AR-1260-1	6.300	7.355	54602742	195.4E6	476.452	538.015
32)	L7 AR-1260-2	6.485	7.607	73300471	272.6E6	486.041	623.237 #
33)	L7 AR-1260-3	6.635	7.961	63963950	222.1E6	475.273	654.529 #
34)	L7 AR-1260-4	7.097	8.189	55942304	234.5E6	467.391	576.956
35)	L7 AR-1260-5	7.334	8.514	150.5E6	565.4E6	500.938	661.147 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR071919\
Data File : PR039451.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jul 2019 16:18
Operator : SM\AJ
Sample : K3896-08DL 4X
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampled :
TRAN-105DL


Manual Integrations
APPROVED

Ankita
7/21/2019 11:57:09 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 16:54:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR071519.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 16 02:56:01 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

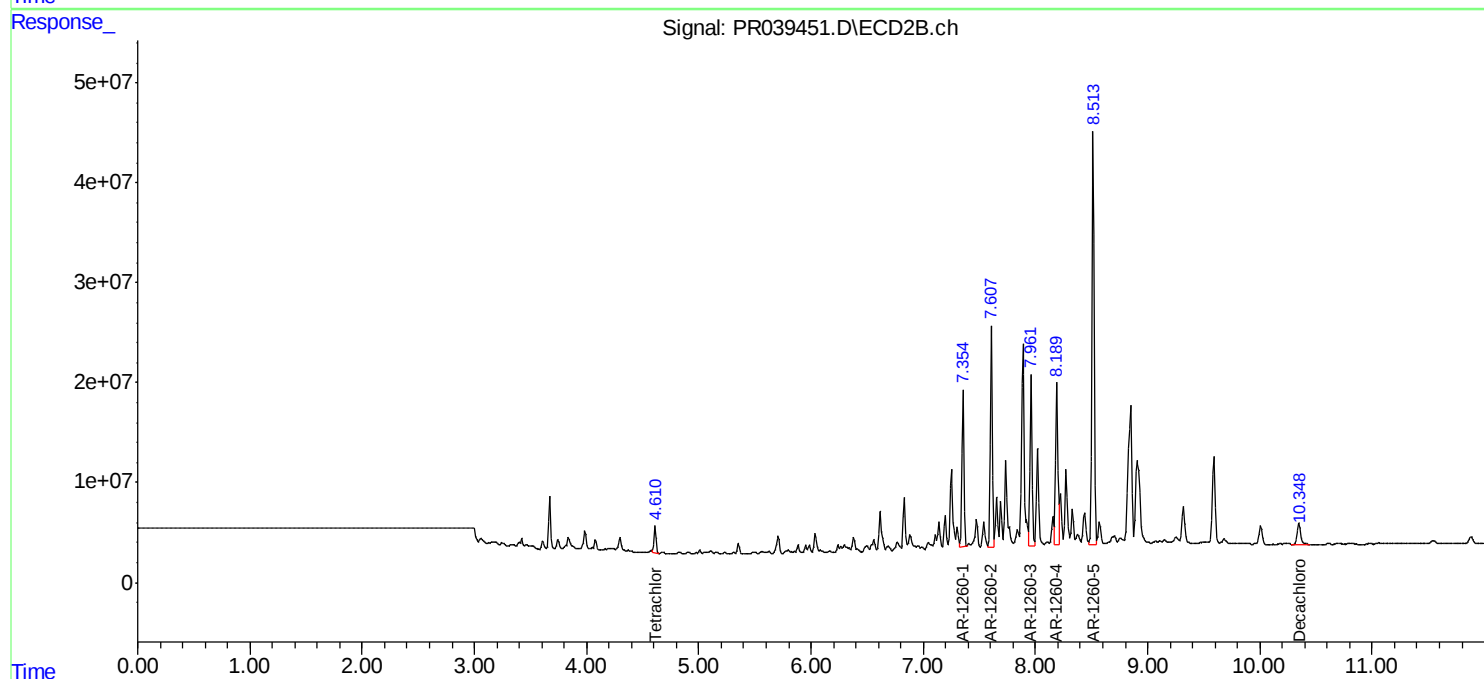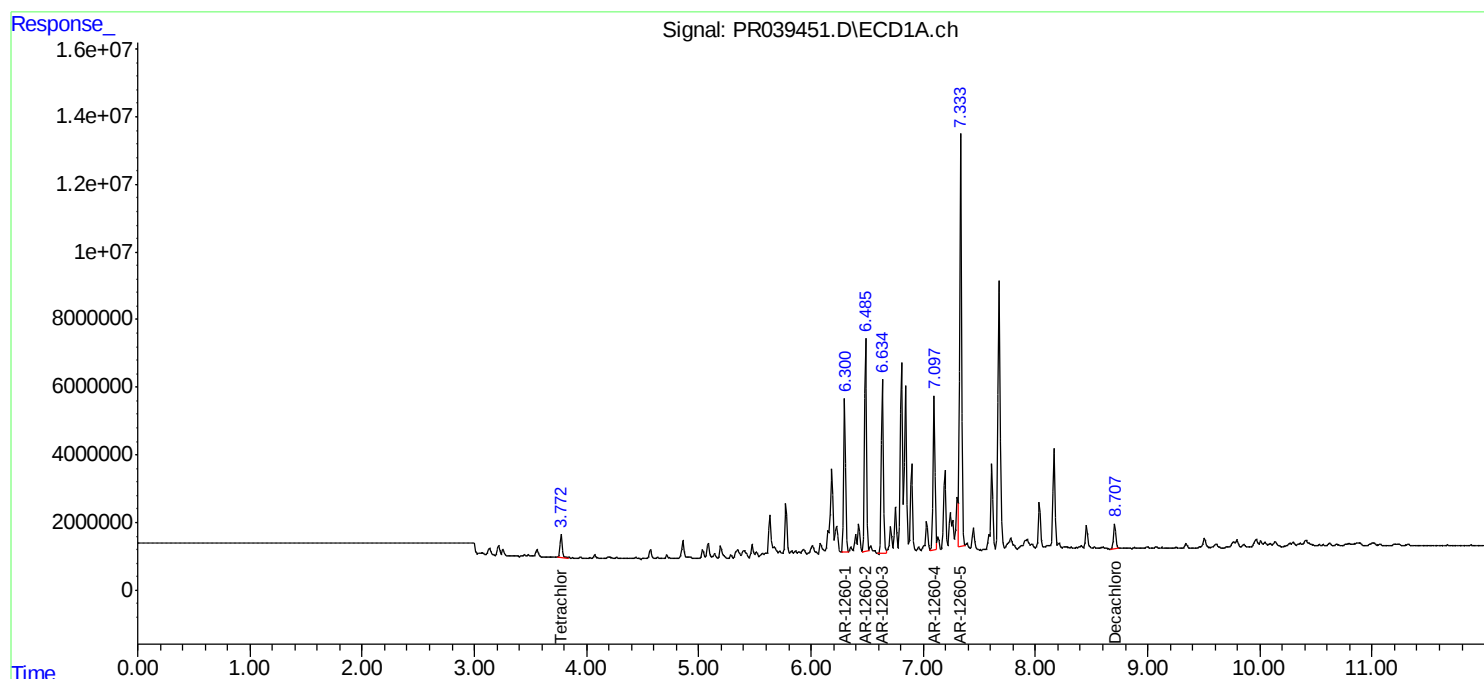

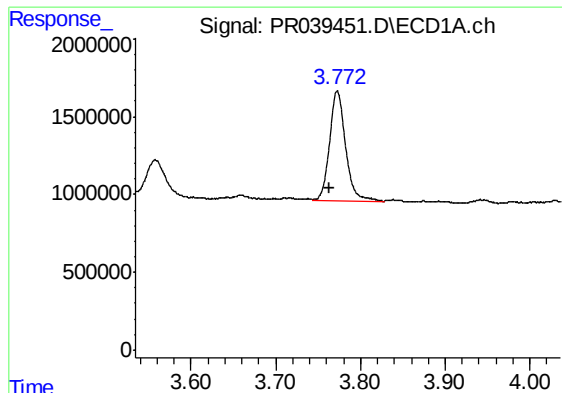


#1 Tetrachloro-m-xylene

R.T.: 3.772 min
Delta R.T.: 0.009 min
Response: 9203775
Conc: 5.94 ng/ml m

Instrument :
ECD_R
ClientSampleId :
TRAN-105DL


Manual Integrations
APPROVED

Ankita
7/21/2019 11:57:09 AM

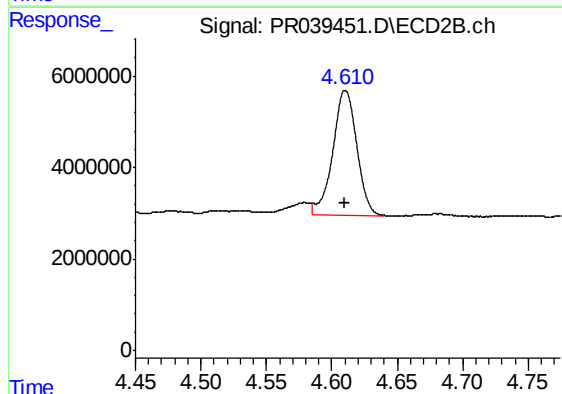


#1 Tetrachloro-m-xylene

R.T.: 4.610 min
Delta R.T.: 0.000 min
Response: 34797899
Conc: 5.38 ng/ml m

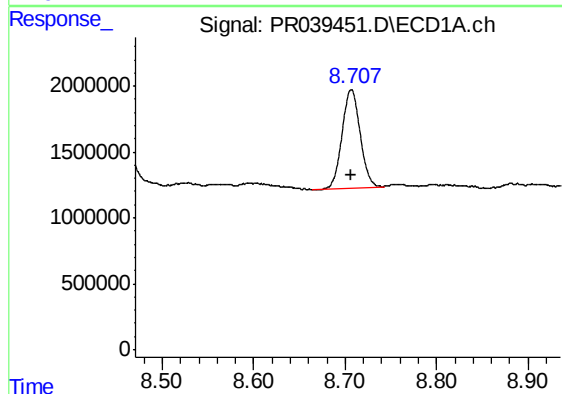


#2 Decachlorobiphenyl

R.T.: 8.707 min
Delta R.T.: 0.000 min
Response: 10234372
Conc: 4.19 ng/ml

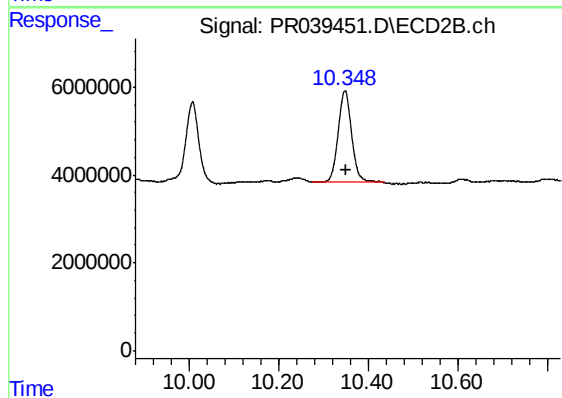

#2 Decachlorobiphenyl

R.T.: 10.348 min
Delta R.T.: -0.002 min
Response: 43748708
Conc: 5.11 ng/ml

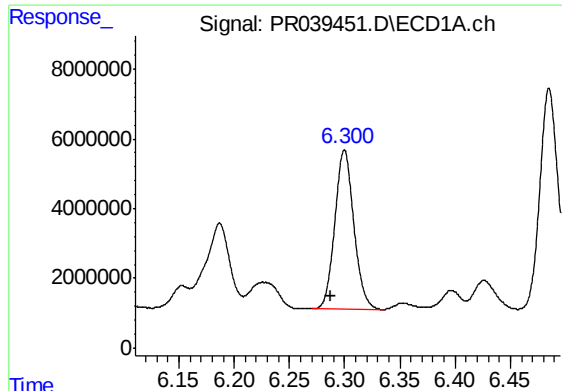


#31 AR-1260-1

R.T.: 6.300 min
Delta R.T.: 0.012 min
Response: 54602742
Conc: 476.45 ng/ml

Instrument :
ECD_R
ClientSampleId :
TRAN-105DL


Manual Integrations
APPROVED

Ankita
7/21/2019 11:57:09 AM

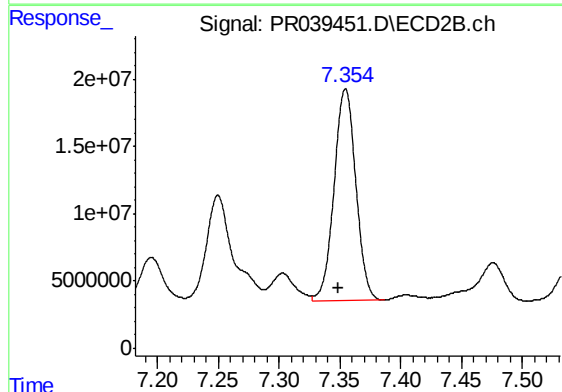


#31 AR-1260-1

R.T.: 7.355 min
Delta R.T.: 0.006 min
Response: 195369448
Conc: 538.02 ng/ml

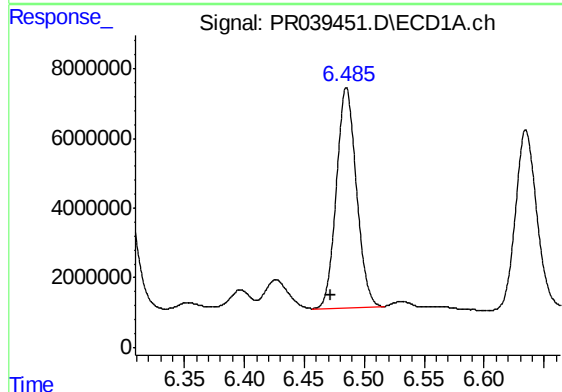


#32 AR-1260-2

R.T.: 6.485 min
Delta R.T.: 0.013 min
Response: 73300471
Conc: 486.04 ng/ml

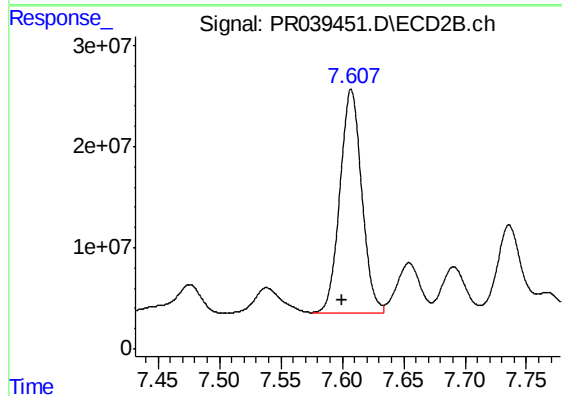

#32 AR-1260-2

R.T.: 7.607 min
Delta R.T.: 0.007 min
Response: 272606539
Conc: 623.24 ng/ml

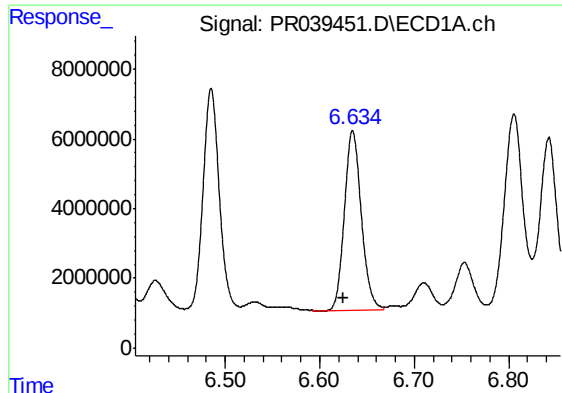


#33 AR-1260-3

R.T.: 6.635 min
Delta R.T.: 0.010 min
Response: 63963950
Conc: 475.27 ng/ml

Instrument :
ECD_R
ClientSampleId :
TRAN-105DL


Manual Integrations
APPROVED

Ankita
7/21/2019 11:57:09 AM

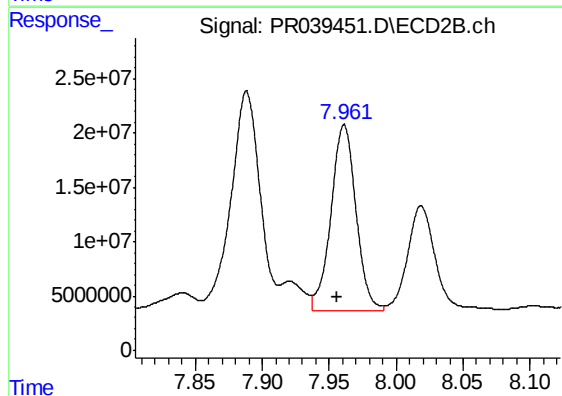


#33 AR-1260-3

R.T.: 7.961 min
Delta R.T.: 0.005 min
Response: 222133876
Conc: 654.53 ng/ml

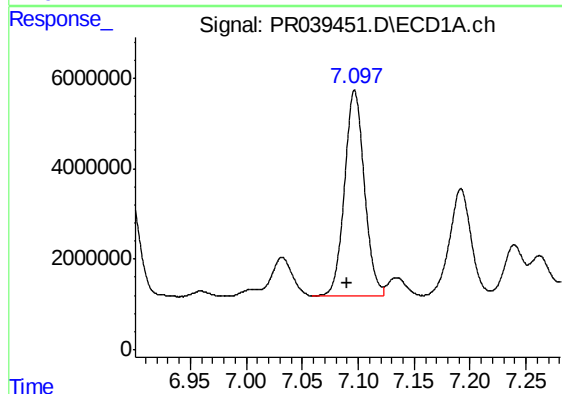


#34 AR-1260-4

R.T.: 7.097 min
Delta R.T.: 0.007 min
Response: 55942304
Conc: 467.39 ng/ml

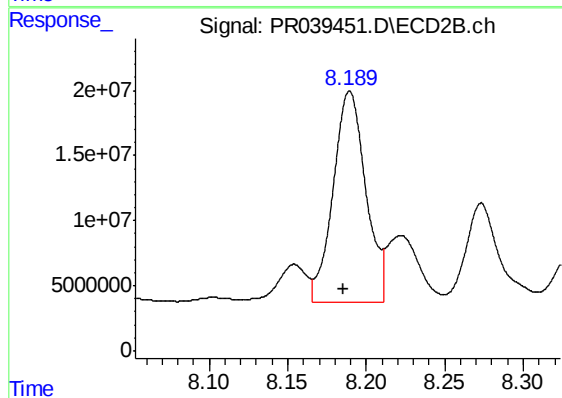

#34 AR-1260-4

R.T.: 8.189 min
Delta R.T.: 0.004 min
Response: 234461135
Conc: 576.96 ng/ml

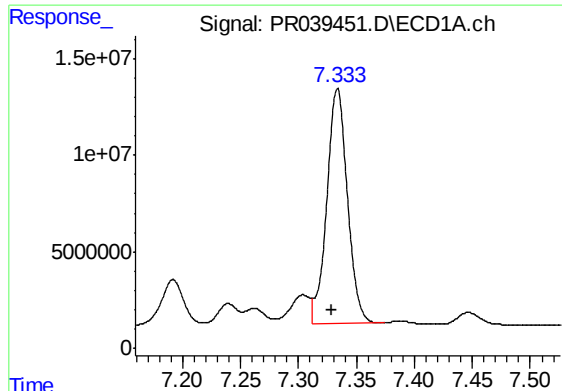


#35 AR-1260-5

R.T.: 7.334 min
Delta R.T.: 0.005 min
Response: 150548244
Conc: 500.94 ng/ml

Instrument :
ECD_R
ClientSampleId :
TRAN-105DL

Manual Integrations
APPROVED

Ankita
7/21/2019 11:57:09 AM

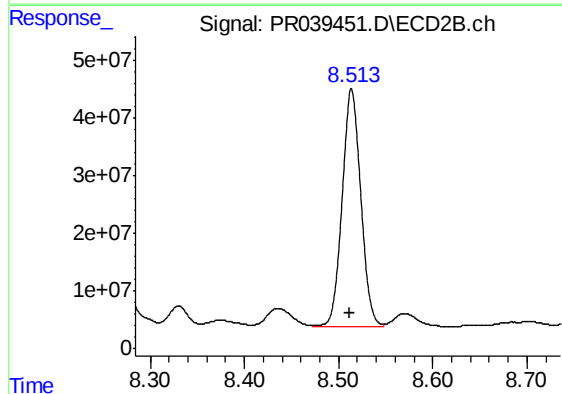

#35 AR-1260-5

R.T.: 8.514 min
Delta R.T.: 0.002 min
Response: 565378525
Conc: 661.15 ng/ml