

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072418\
 Data File : FF001471.D
 Signal(s) : FID2B.ch
 Acq On : 24 Jul 2018 14:19
 Operator : AJ\SJ
 Sample : J4095-10
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 25 08:01:07 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
 Quant Title :
 QLast Update : Mon Jul 02 13:42:46 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.441	2425731	22.518 ug/ml
Target Compounds			
4) N-TETRADECANE	8.070	691016	5.494 ug/ml
7) N-EICOSANE	12.402	613885	4.935 ug/ml
10) N-TETRACOSANE	14.625	391936	3.215 ug/ml
11) N-HEXACOSANE	15.664	108226	0.893 ug/ml
12) N-OCTACOSANE	16.654	245236	2.036 ug/ml
13) N-TRIACONTANE	17.496	140000	1.165 ug/ml
14) N-DOTRIACONTANE	18.323	250013	2.120 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072418\
Data File : FF001471.D
Signal(s) : FID2B.ch
Acq On : 24 Jul 2018 14:19
Operator : AJ\SJ
Sample : J4095-10
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 25 08:01:07 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

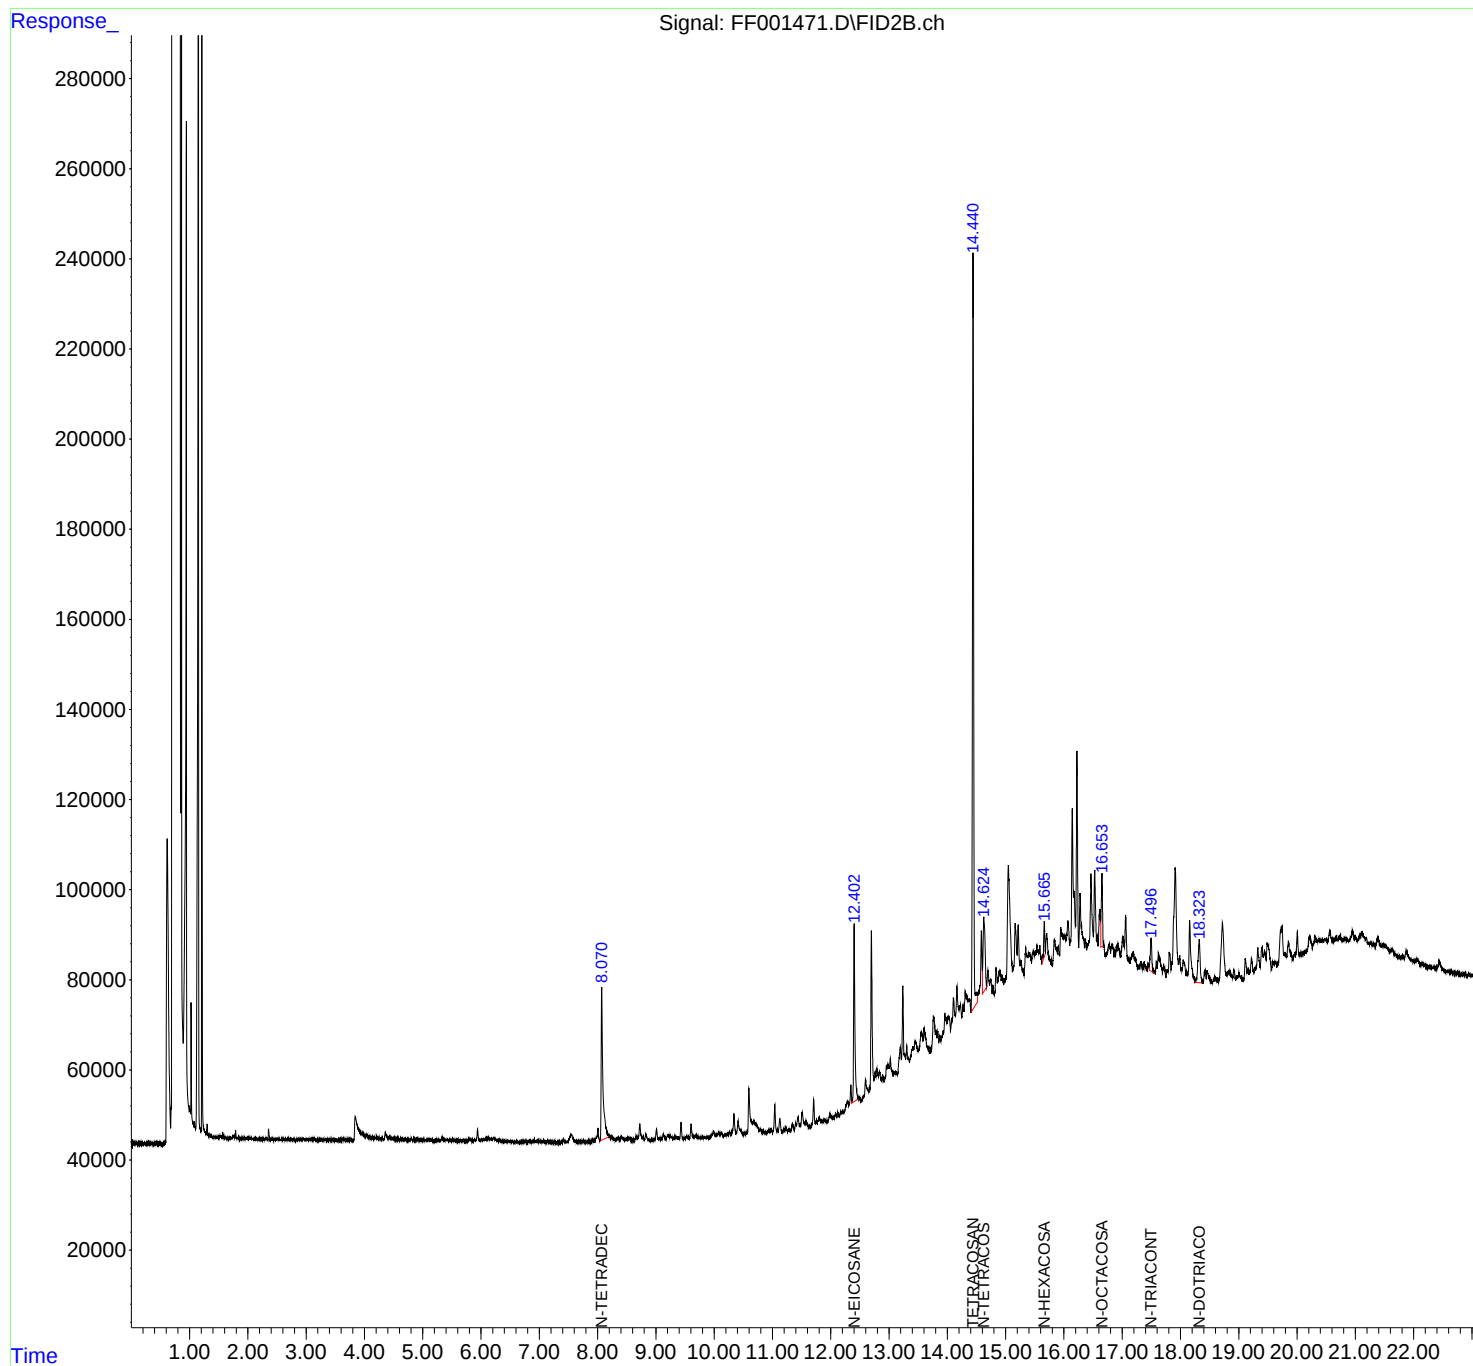


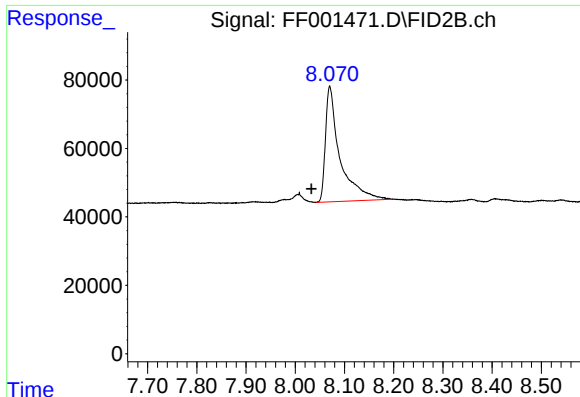

#4 N-TETRADECANE


R.T.: 8.070 min
Delta R.T.: 0.037 min
Response: 691016
Conc: 5.49 ug/ml

Instrument :
ECD_R
ClientSampleId :

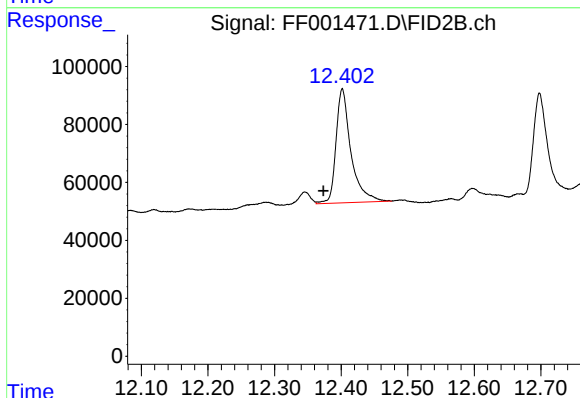


#7 N-EICOSANE

R.T.: 12.402 min
Delta R.T.: 0.028 min
Response: 613885
Conc: 4.94 ug/ml

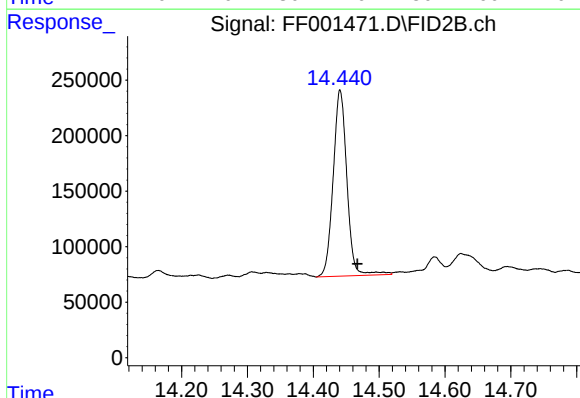


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.441 min
Delta R.T.: -0.026 min
Response: 2425731
Conc: 22.52 ug/ml

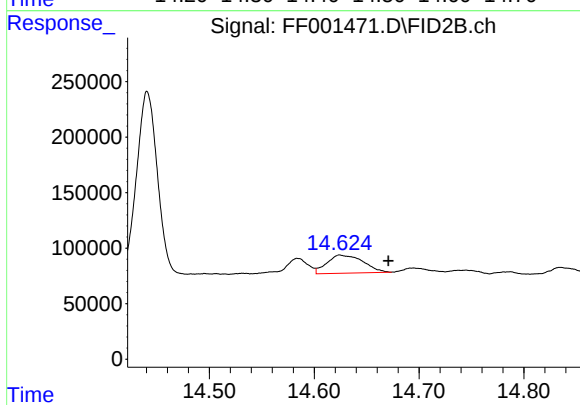

#10 N-TETRACOSANE


R.T.: 14.625 min
Delta R.T.: -0.046 min
Response: 391936
Conc: 3.22 ug/ml

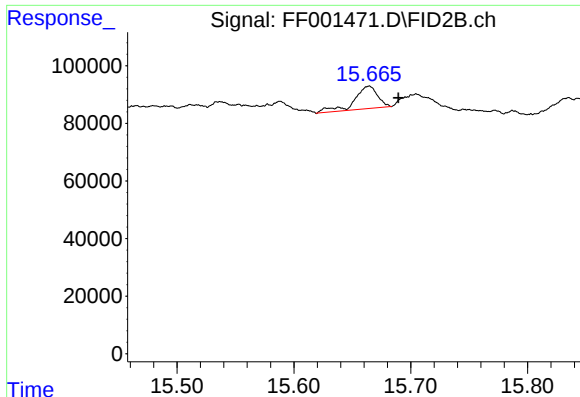

#11 N-HEXACOSANE


R.T.: 15.664 min
Delta R.T.: -0.025 min
Response: 108226
Conc: 0.89 ug/ml

Instrument :
ECD_R
ClientSampleId :

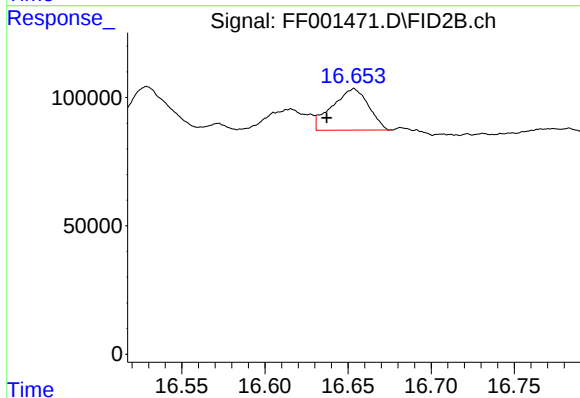


#12 N-OCTACOSANE

R.T.: 16.654 min
Delta R.T.: 0.016 min
Response: 245236
Conc: 2.04 ug/ml

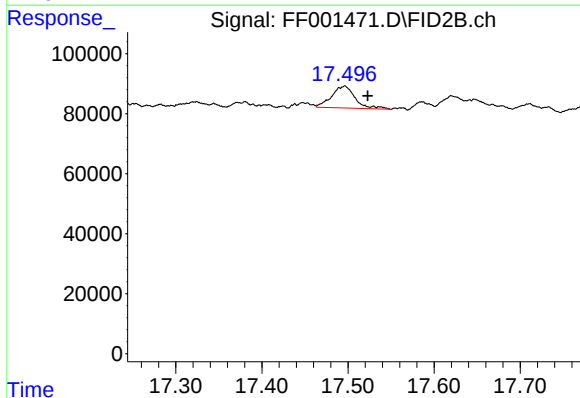

#13 N-TRIACONTANE

R.T.: 17.496 min
Delta R.T.: -0.026 min
Response: 140000
Conc: 1.16 ug/ml

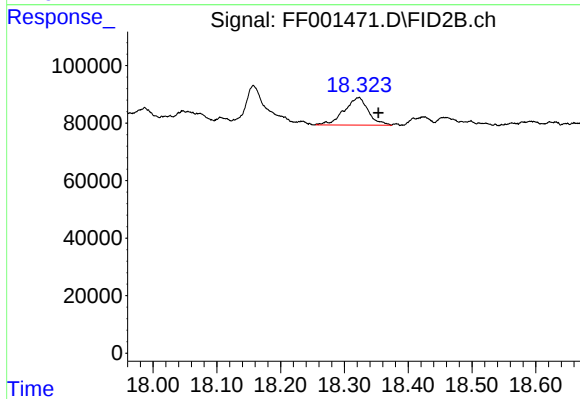

#14 N-DOTRIACONTANE

R.T.: 18.323 min
Delta R.T.: -0.031 min
Response: 250013
Conc: 2.12 ug/ml