

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR072721\
 Data File : PR051368.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jul 2021 21:40
 Operator : AJ\MA
 Sample : M2940-07
 Misc : AR1242 LOD 25 PPB
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 28 03:09:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR072721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 28 02:51:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.628	3.808	148.5E6	137.9E6	18.174	18.541
2)	SA Decachlor...	10.504	8.831	202.8E6	154.8E6	21.118	19.362

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR072721\
Data File : PR051368.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2021 21:40
Operator : AJ\MA
Sample : M2940-07
Misc : AR1242 LOD 25 PPB
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 28 03:09:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR072721.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 28 02:51:26 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

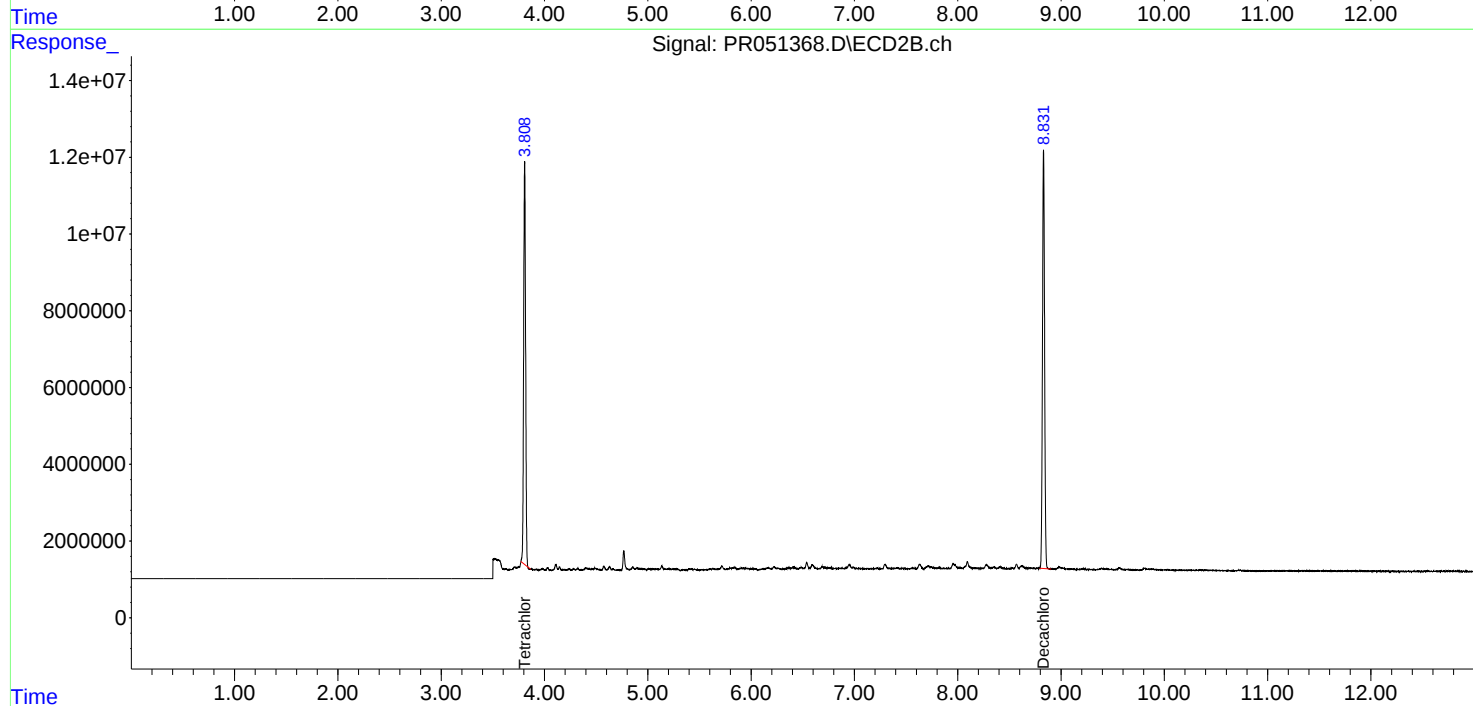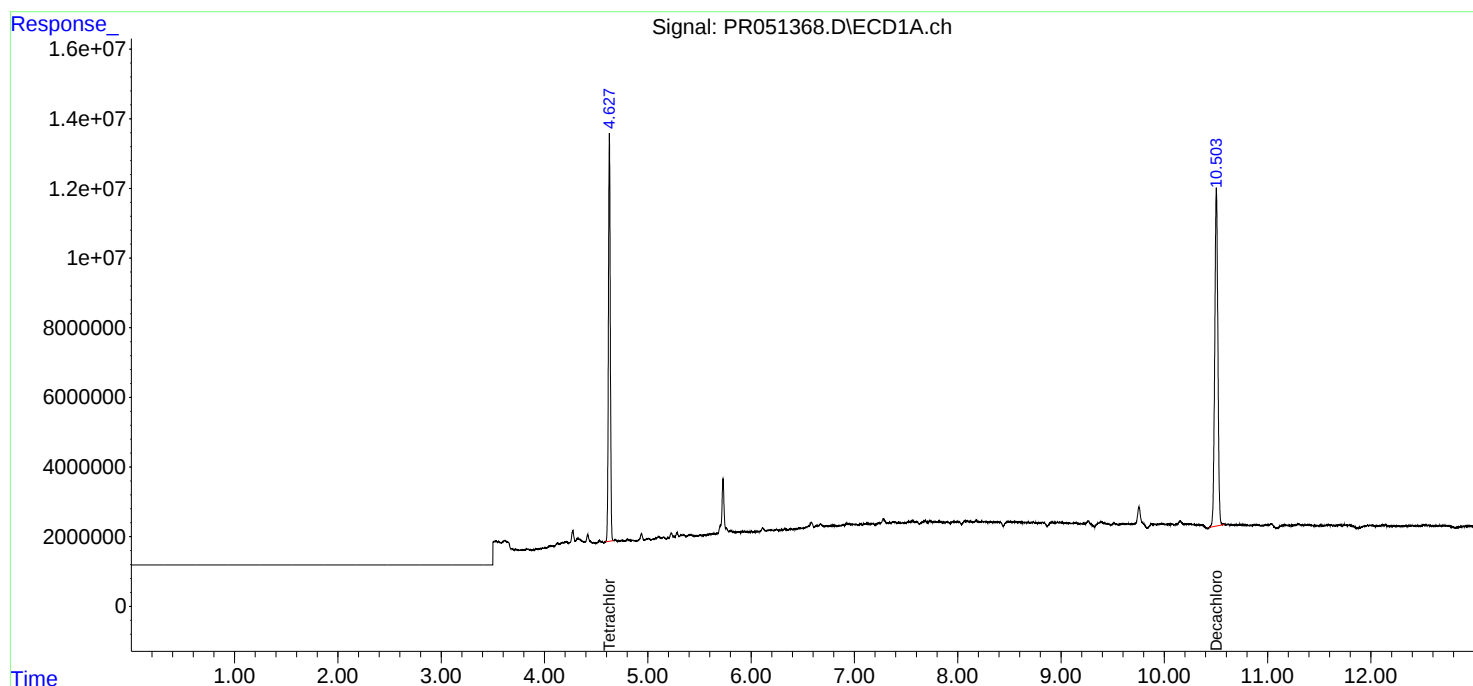


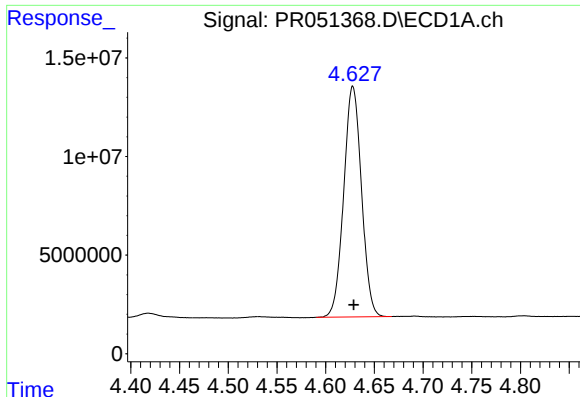

#1 Tetrachloro-m-xylene


R.T.: 4.628 min
Delta R.T.: -0.001 min
Response: 148538450
Conc: 18.17 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

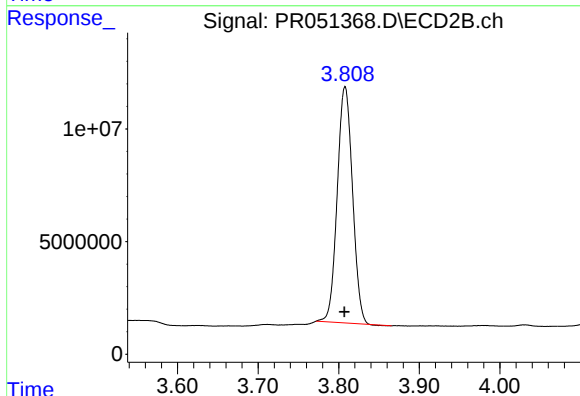


#1 Tetrachloro-m-xylene

R.T.: 3.808 min
Delta R.T.: 0.000 min
Response: 137864683
Conc: 18.54 ng/ml

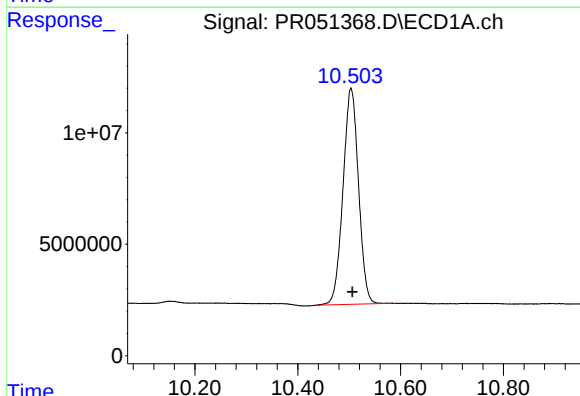

#2 Decachlorobiphenyl

R.T.: 10.504 min
Delta R.T.: -0.002 min
Response: 202847771
Conc: 21.12 ng/ml

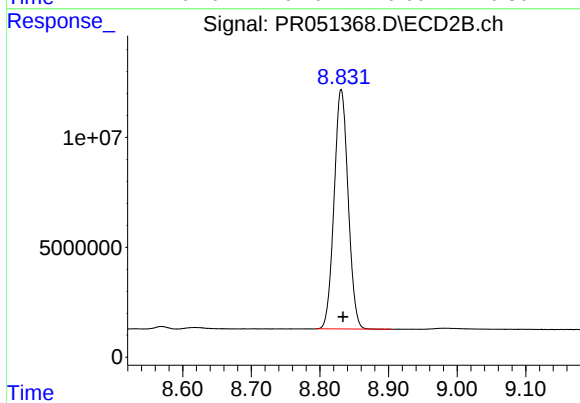

#2 Decachlorobiphenyl

R.T.: 8.831 min
Delta R.T.: -0.003 min
Response: 154807230
Conc: 19.36 ng/ml