

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR072820\
 Data File : PR046558.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jul 2020 23:05
 Operator : AJ\MA
 Sample : L3439-07 2X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 20200444-3002D

Manual Integrations
 APPROVED

Ankita
 7/29/2020 4:40:45 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 04:07:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR072820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 29 03:56:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.765	3.989	599192	4755358	0.379m	0.475m#
2) SA Decachlor...	10.766	9.111	418296	1729982	0.189m	0.115m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR072820\
Data File : PR046558.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jul 2020 23:05
Operator : AJ\MA
Sample : L3439-07 2X
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
20200444-3002D


Manual Integrations
APPROVED

Ankita
7/29/2020 4:40:45 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 04:07:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR072820.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 29 03:56:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

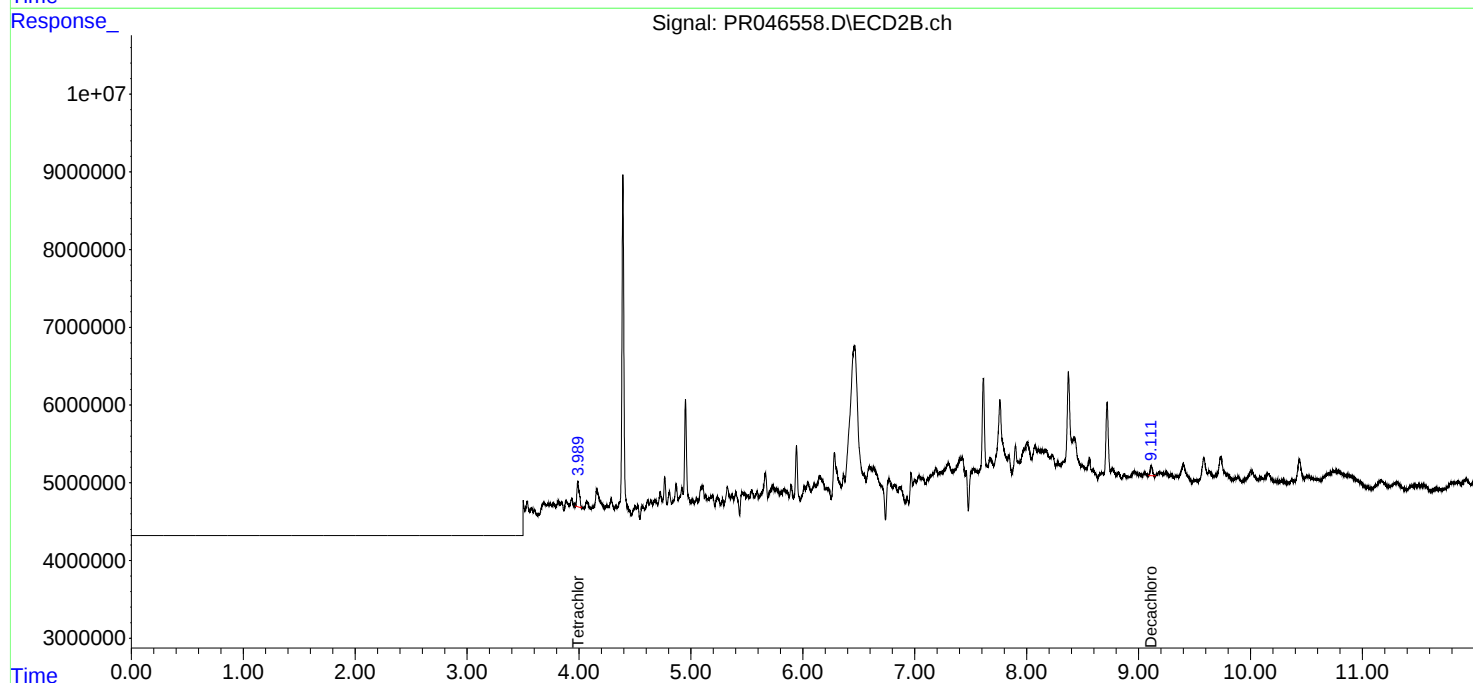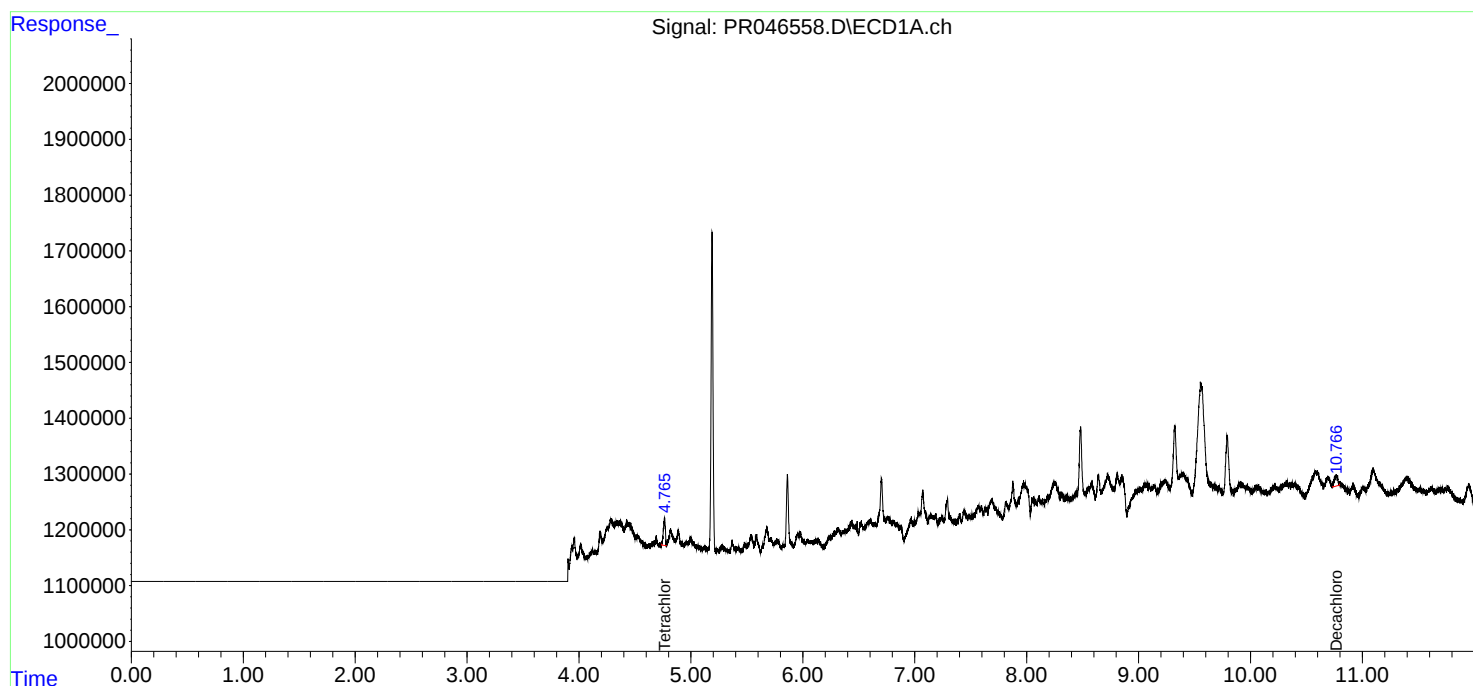

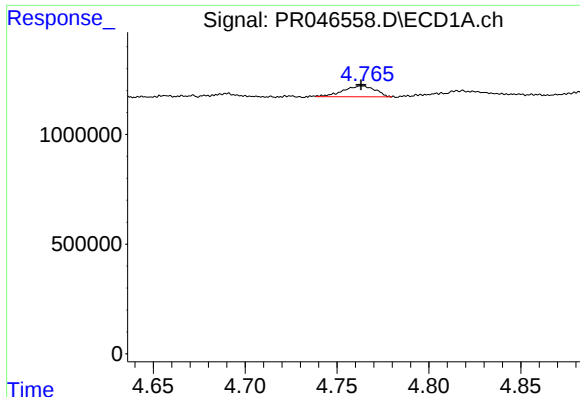


#1 Tetrachloro-m-xylene

R.T.: 4.765 min
Delta R.T.: 0.002 min
Response: 599192
Conc: 0.38 ng/ml m

Instrument :
ECD_R
ClientSampleId :
20200444-3002D


Manual Integrations
APPROVED

Ankita
7/29/2020 4:40:45 PM

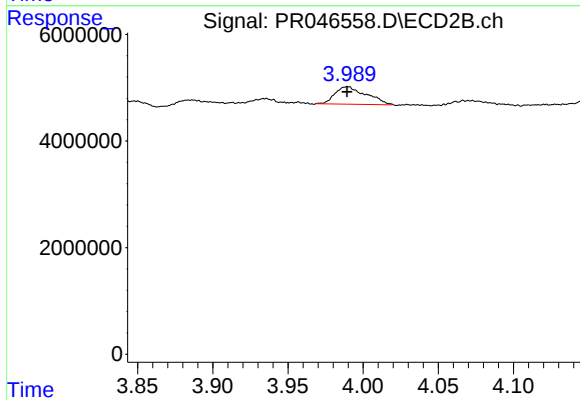


#1 Tetrachloro-m-xylene

R.T.: 3.989 min
Delta R.T.: 0.000 min
Response: 4755358
Conc: 0.48 ng/ml m

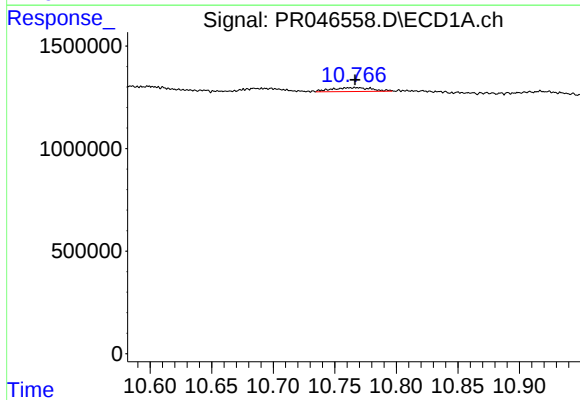

#2 Decachlorobiphenyl

R.T.: 10.766 min
Delta R.T.: 0.000 min
Response: 418296
Conc: 0.19 ng/ml m

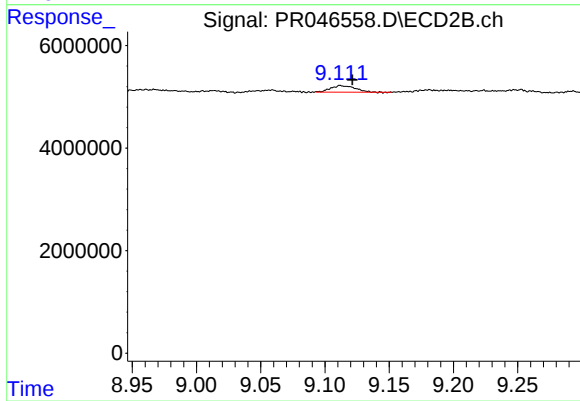

#2 Decachlorobiphenyl

R.T.: 9.111 min
Delta R.T.: -0.010 min
Response: 1729982
Conc: 0.11 ng/ml m