

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR080223\
Data File : PR062478.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Aug 2023 14:29
Operator : YP\AJ
Sample : 03805-08DL 20X
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
X3H67DL

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/03/2023
Supervised By :Ankita Jodhani 08/03/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 22:19:58 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR072723CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 27 05:18:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

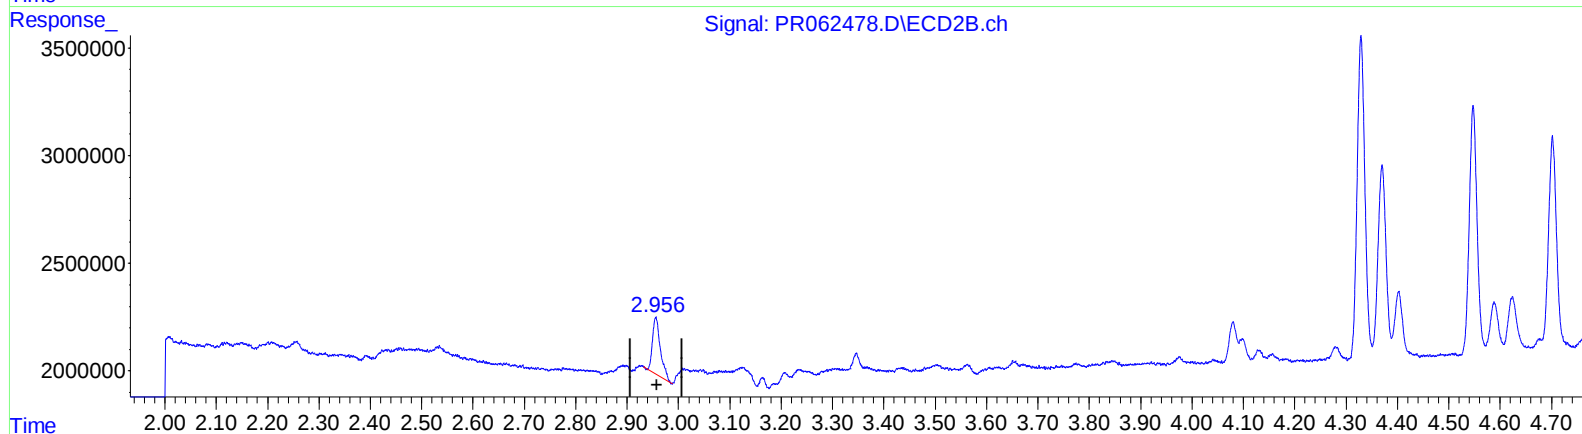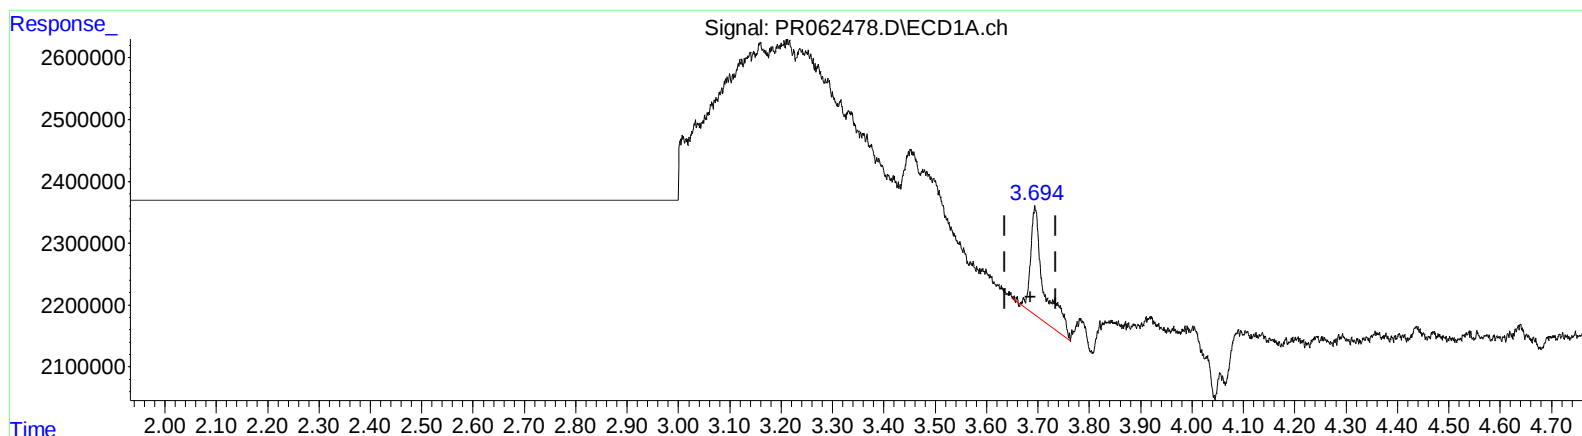

QEdit

(1) Tetrachloro-m-xylene (SA)

3.695min 1.496 ng/ml

response 3212639

(1) Tetrachloro-m-xylene #2 (SA)

2.956min 0.909 ng/ml

response 2817980

(+) = Expected Retention Time

PR072723CLP.M Thu Aug 03 01:56:26 2023

Page: 1

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR080223\
Data File : PR062478.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Aug 2023 14:29
Operator : YP\AJ
Sample : 03805-08DL 20X
Misc :
ALS Vial : 17 Sample Multiplier: 1


Instrument :
ECD_R
ClientSampleId :
X3H67DL

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/03/2023
Supervised By :Ankita Jodhani 08/03/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 22:19:58 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR072723CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 27 05:18:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

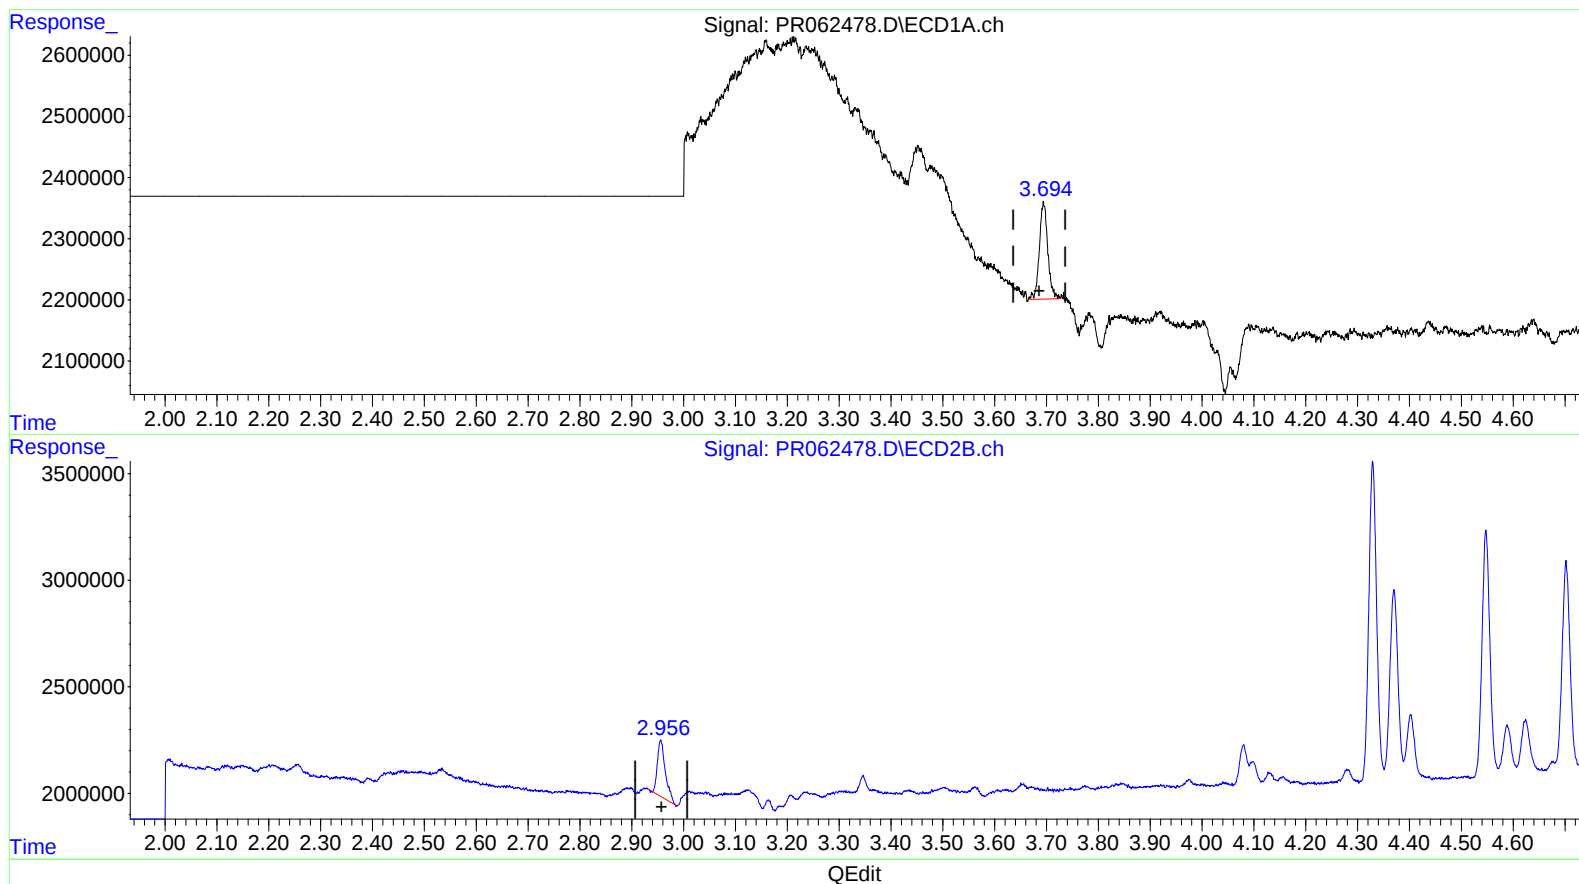

(1) Tetrachloro-m-xylene (SA)

3.694min 0.830 ng/ml m

response 1781662

(1) Tetrachloro-m-xylene #2 (SA)

2.956min 0.909 ng/ml

response 2817980