

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS080621\  
 Data File : PS016287.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 06 Aug 2021 15:27  
 Operator : DD\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_R  
 ClientSampleId :  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Aug 09 01:05:30 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS080221.M  
 Quant Title : 8080.M  
 QLast Update : Mon Aug 02 14:10:19 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound | RT#1  | RT#2   | Resp#1  | Resp#2   | ng/ml   | ng/ml   |
|-----------------------------|----------|-------|--------|---------|----------|---------|---------|
| -----                       |          |       |        |         |          |         |         |
| System Monitoring Compounds |          |       |        |         |          |         |         |
| 4) S                        | 2,4-DCAA | 7.189 | 6.767  | 643.3E6 | 275.4E6  | 437.282 | 527.876 |
| Target Compounds            |          |       |        |         |          |         |         |
| 15) T                       | Picloram | 0.000 | 10.852 | 0       | 15088942 | N.D.    | 3.747   |
| -----                       |          |       |        |         |          |         |         |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS080621\  
Data File : PS016287.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 06 Aug 2021 15:27  
Operator : DD\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_R  
ClientSampleId :  
I.BLK

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Aug 09 01:05:30 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS080221.M  
Quant Title : 8080.M  
QLast Update : Mon Aug 02 14:10:19 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

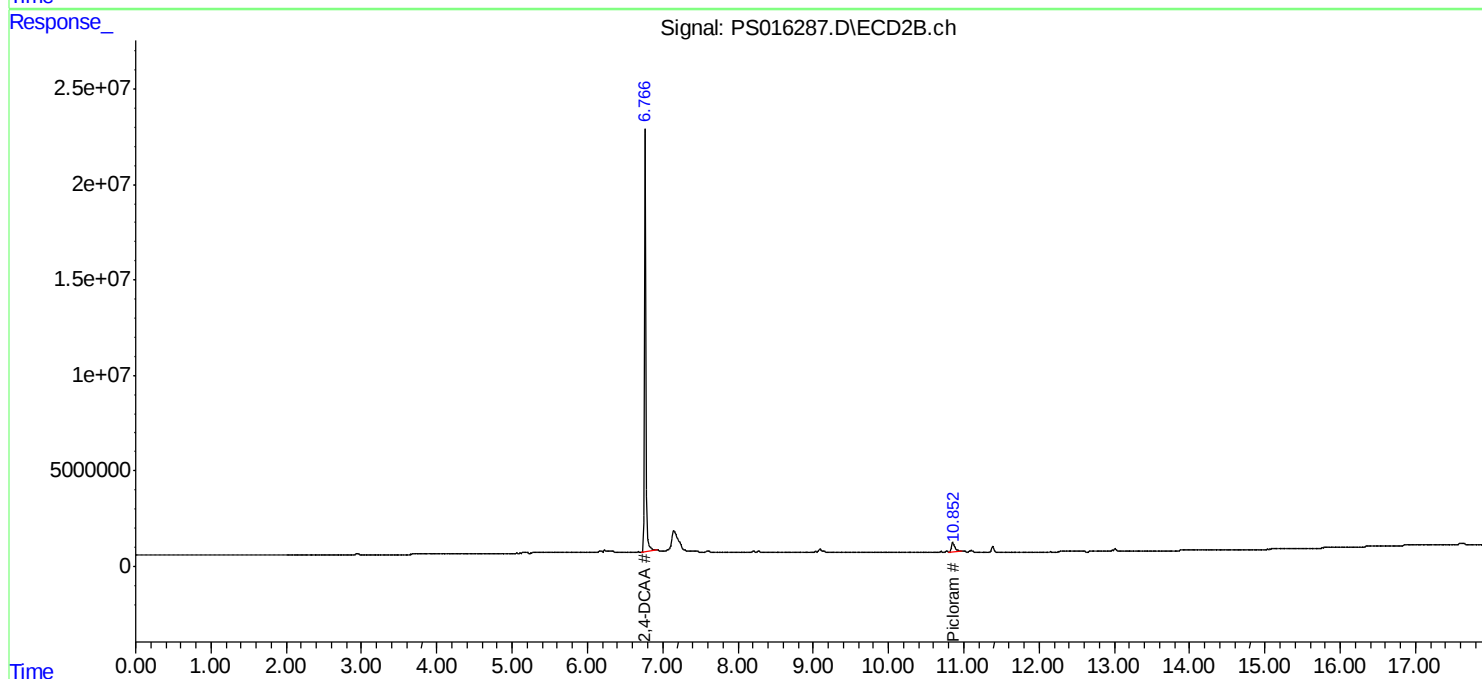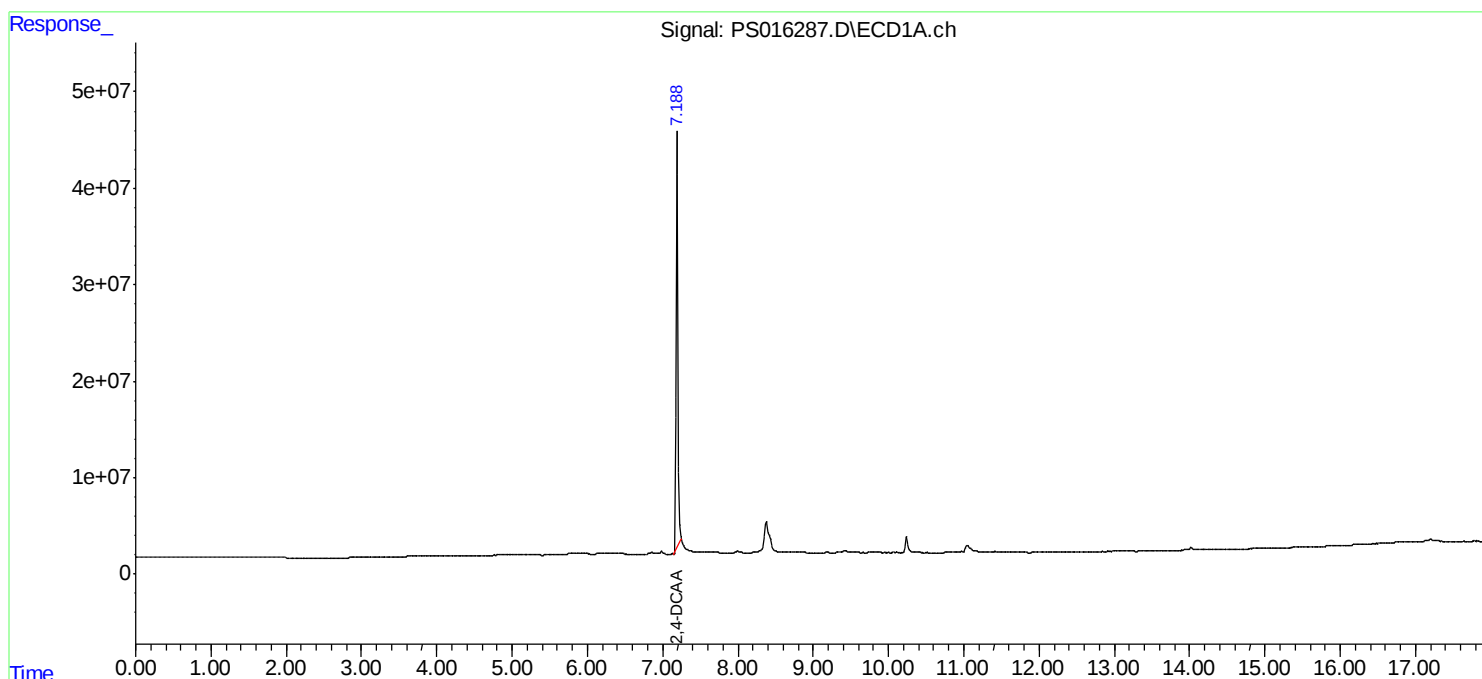


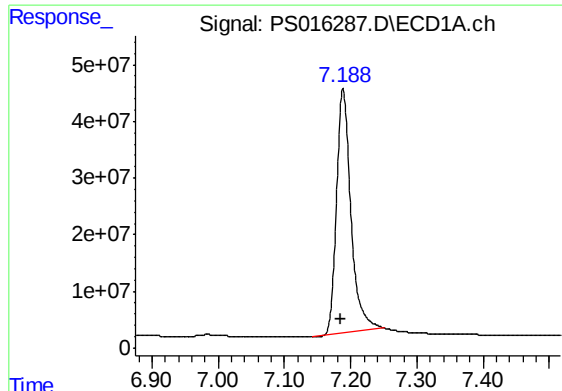

#4 2,4-DCAA


R.T.: 7.189 min  
Delta R.T.: 0.003 min  
Response: 643288321  
Conc: 437.28 ng/ml

Instrument :  
ECD\_R  
ClientSampleId :  
I.BLK

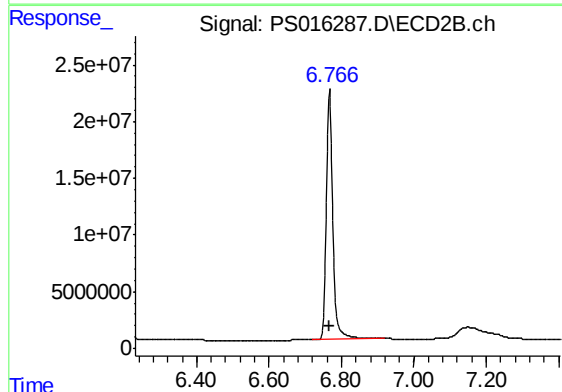


#4 2,4-DCAA

R.T.: 6.767 min  
Delta R.T.: 0.000 min  
Response: 275352949  
Conc: 527.88 ng/ml

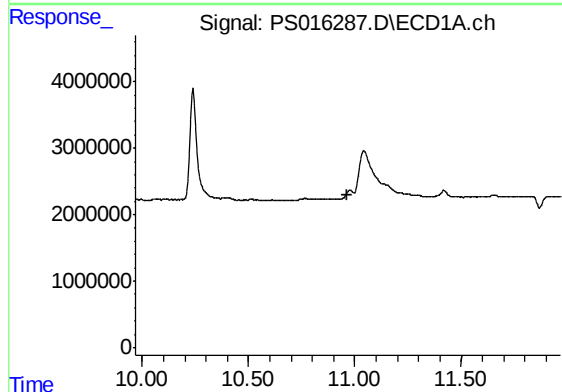

#15 Picloram

R.T.: 0.000 min  
Exp R.T. : 10.967 min  
Response: 0  
Conc: N.D.

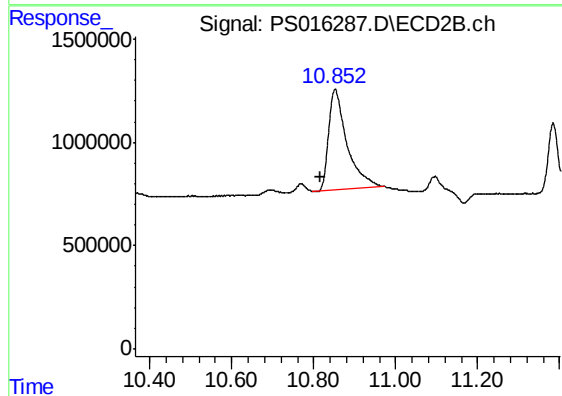

#15 Picloram

R.T.: 10.852 min  
Delta R.T.: 0.037 min  
Response: 15088942  
Conc: 3.75 ng/ml