

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR080622\
 Data File : PR055679.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Aug 2022 22:21
 Operator : AJ\MA
 Sample : N3980-07
 Misc : AR1254 LOD 40 PPB
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 03:57:51 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080522.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 05 12:39:02 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.635	2.905	86199819	41625498	20.201	20.732
2) SA Decachlor...	9.527	8.121	37651435	37989321	21.176	20.884
Target Compounds						
26) L6 AR-1254-1	5.763	4.840	4597688	4163805	44.892	38.107
27) L6 AR-1254-2	6.000	4.999	6698637	3540036	45.569	36.559
28) L6 AR-1254-3	6.391	5.417	6693341	6072985	45.686	39.869
29) L6 AR-1254-4	6.703	5.662	4461356	3807453	43.035	38.641
30) L6 AR-1254-5	7.159	6.104	4787113	5268361	44.149	38.885



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR080622\
Data File : PR055679.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Aug 2022 22:21
Operator : AJ\MA
Sample : N3980-07
Misc : AR1254 LOD 40 PPB
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 03:57:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080522.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 05 12:39:02 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

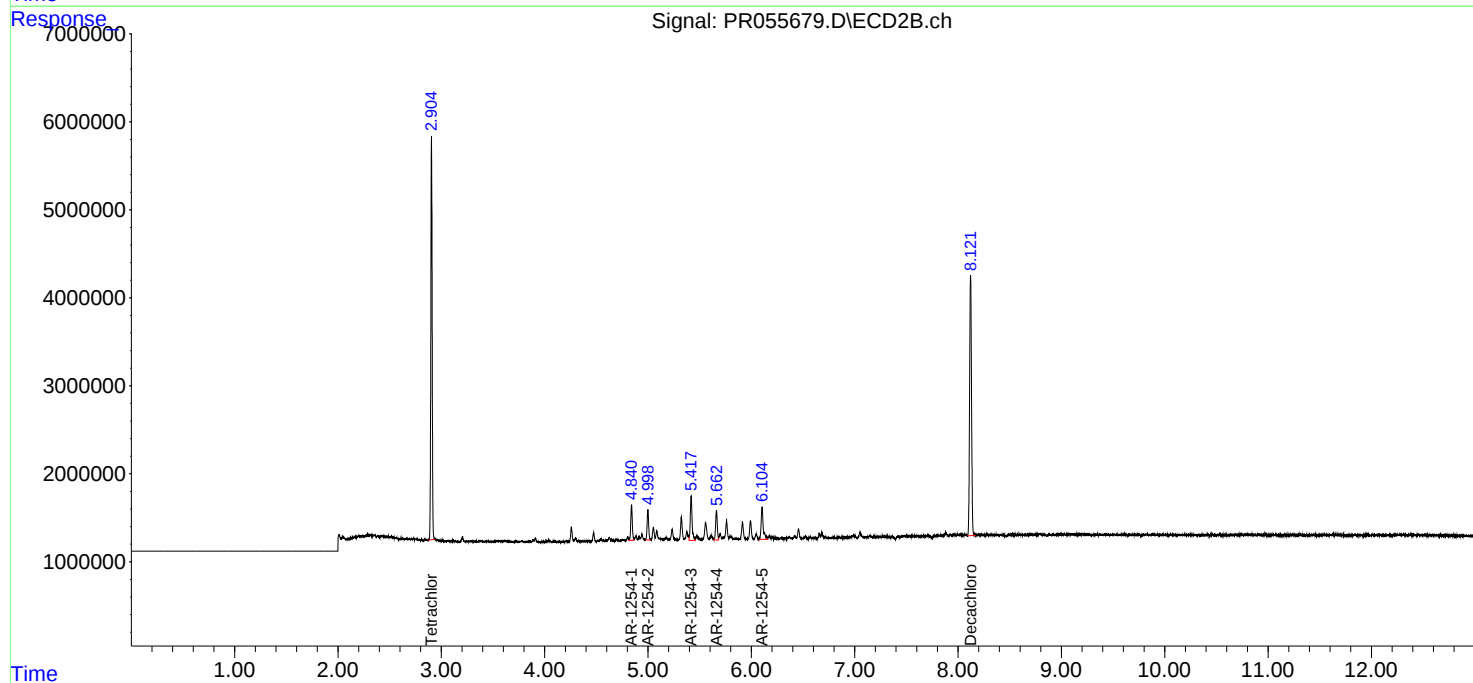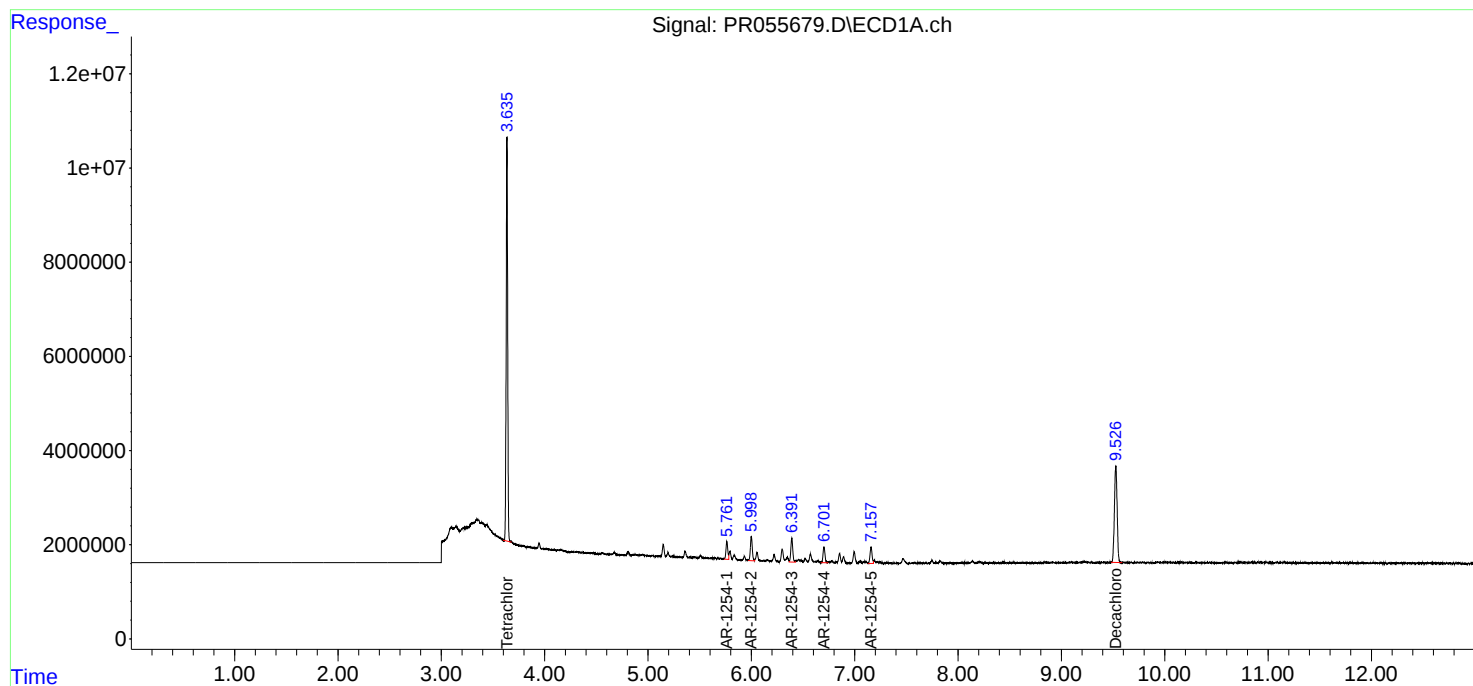


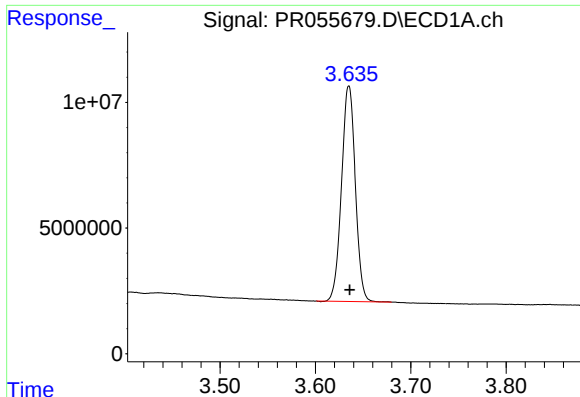

#1 Tetrachloro-m-xylene


R.T.: 3.635 min
Delta R.T.: 0.000 min
Response: 86199819
Conc: 20.20 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

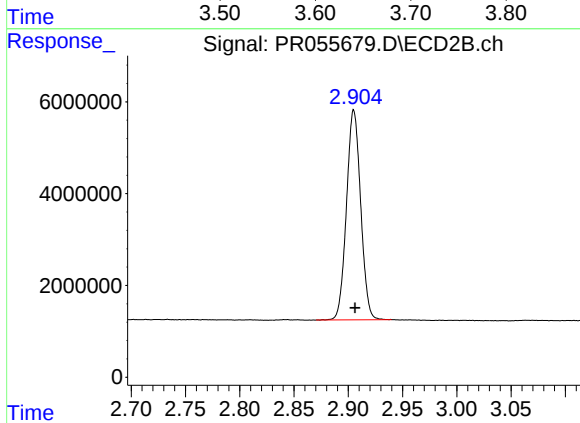


#1 Tetrachloro-m-xylene

R.T.: 2.905 min
Delta R.T.: -0.001 min
Response: 41625498
Conc: 20.73 ng/ml

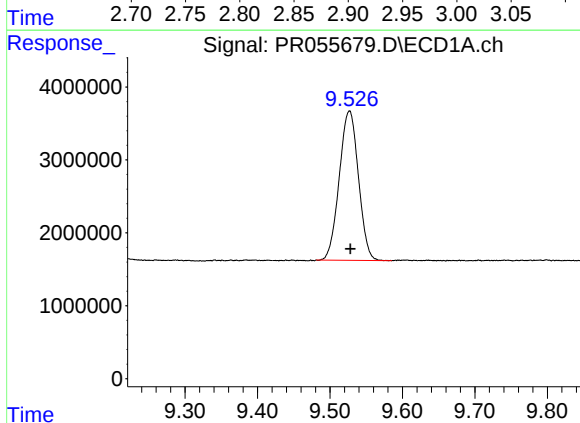


#2 Decachlorobiphenyl

R.T.: 9.527 min
Delta R.T.: -0.002 min
Response: 37651435
Conc: 21.18 ng/ml

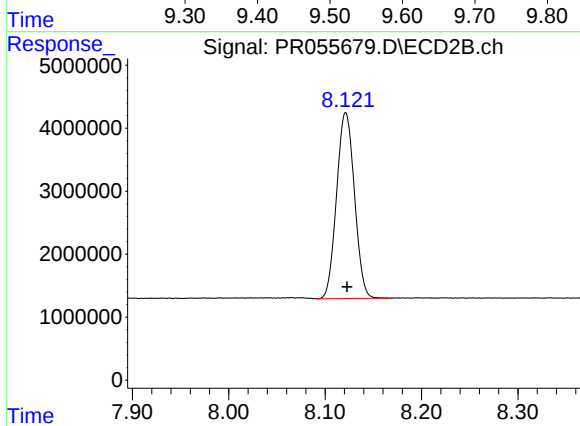

#2 Decachlorobiphenyl


R.T.: 8.121 min
Delta R.T.: -0.002 min
Response: 37989321
Conc: 20.88 ng/ml

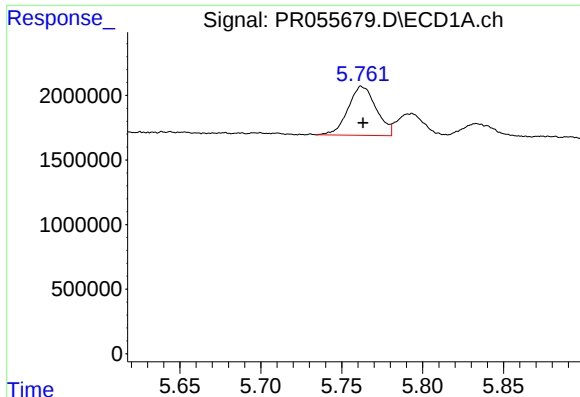

#26 AR-1254-1


R.T.: 5.763 min
Delta R.T.: 0.000 min
Response: 4597688
Conc: 44.89 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

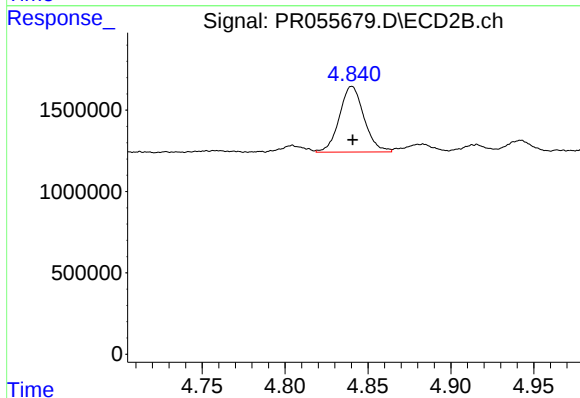


#26 AR-1254-1

R.T.: 4.840 min
Delta R.T.: 0.000 min
Response: 4163805
Conc: 38.11 ng/ml

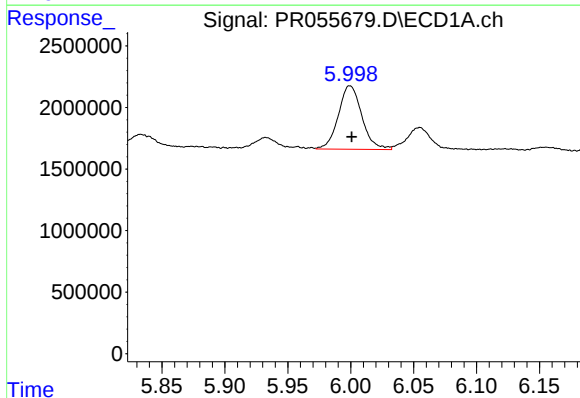


#27 AR-1254-2

R.T.: 6.000 min
Delta R.T.: -0.001 min
Response: 6698637
Conc: 45.57 ng/ml

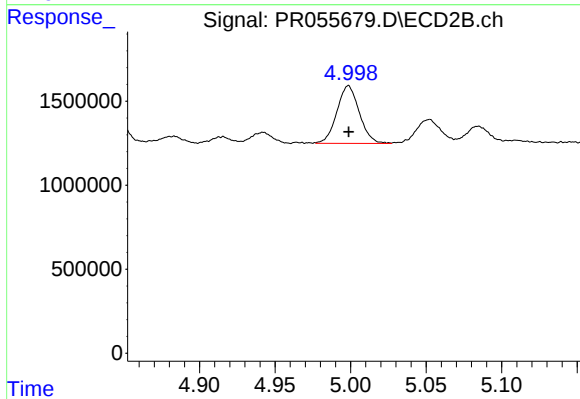

#27 AR-1254-2


R.T.: 4.999 min
Delta R.T.: 0.000 min
Response: 3540036
Conc: 36.56 ng/ml

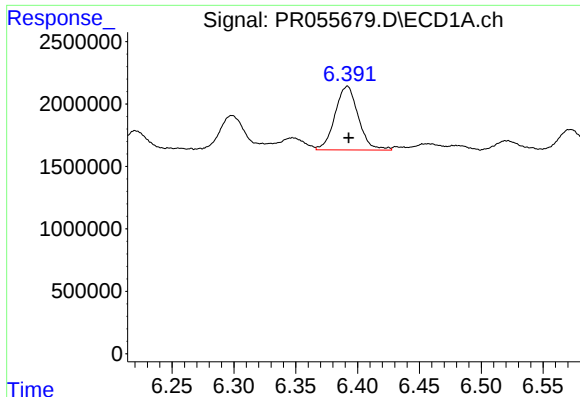

#28 AR-1254-3


R.T.: 6.391 min
Delta R.T.: -0.001 min
Response: 6693341
Conc: 45.69 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

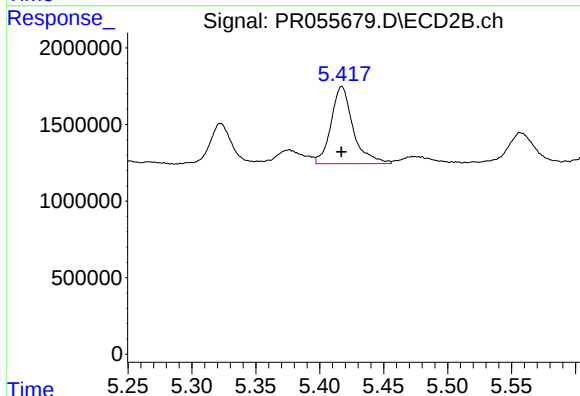


#28 AR-1254-3

R.T.: 5.417 min
Delta R.T.: 0.000 min
Response: 6072985
Conc: 39.87 ng/ml

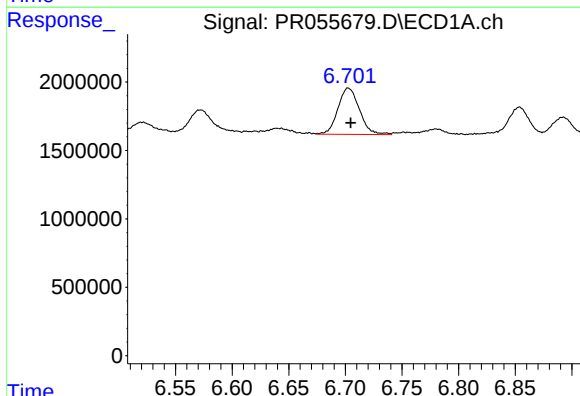


#29 AR-1254-4

R.T.: 6.703 min
Delta R.T.: -0.002 min
Response: 4461356
Conc: 43.03 ng/ml

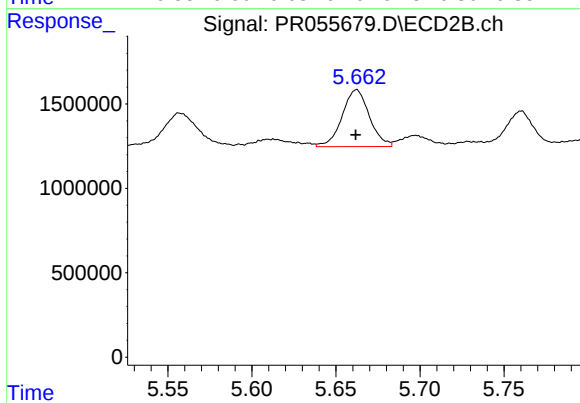

#29 AR-1254-4


R.T.: 5.662 min
Delta R.T.: 0.000 min
Response: 3807453
Conc: 38.64 ng/ml

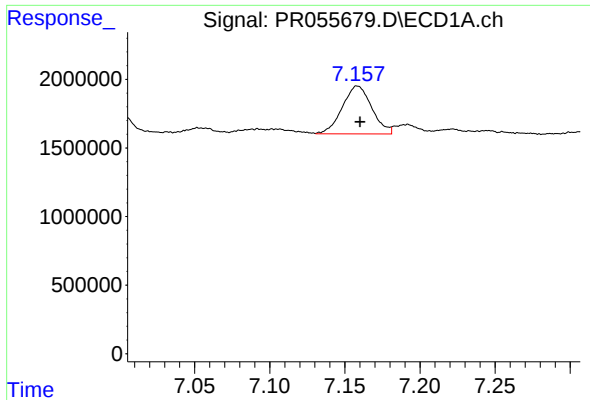

#30 AR-1254-5

R.T.: 7.159 min
Delta R.T.: -0.002 min
Response: 4787113
Conc: 44.15 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

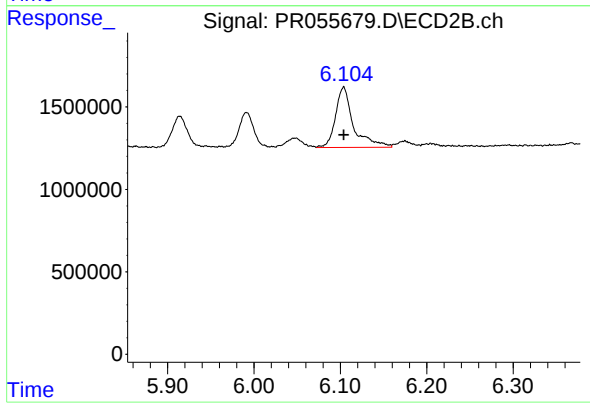

#30 AR-1254-5

R.T.: 6.104 min
Delta R.T.: 0.000 min
Response: 5268361
Conc: 38.88 ng/ml