

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR080622\
 Data File : PR055711.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2022 08:18
 Operator : AJ\MA
 Sample : N3980-09
 Misc : AR1254 MDL 25 PPB
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-WATER-03-QT3-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 14:24:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080522.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 05 12:39:02 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.634	2.905	83823755	39822883	19.645	19.834
2) SA Decachlor...	9.526	8.123	38792193	38837341	21.817	21.350
Target Compounds						
26) L6 AR-1254-1	5.762	4.840	3910617	2930206	38.184	26.817 #
27) L6 AR-1254-2	5.999	4.998	4910815	2613739	33.407	26.993
28) L6 AR-1254-3	6.391	5.416	4944898	4465216	33.752	29.314
29) L6 AR-1254-4	6.703	5.661	3312437	2671781	31.952	27.115
30) L6 AR-1254-5	7.158	6.103	3636022	3502698	33.533	25.853



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR080622\
Data File : PR055711.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2022 08:18
Operator : AJ\MA
Sample : N3980-09
Misc : AR1254 MDL 25 PPB
ALS Vial : 53 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 14:24:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080522.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 05 12:39:02 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

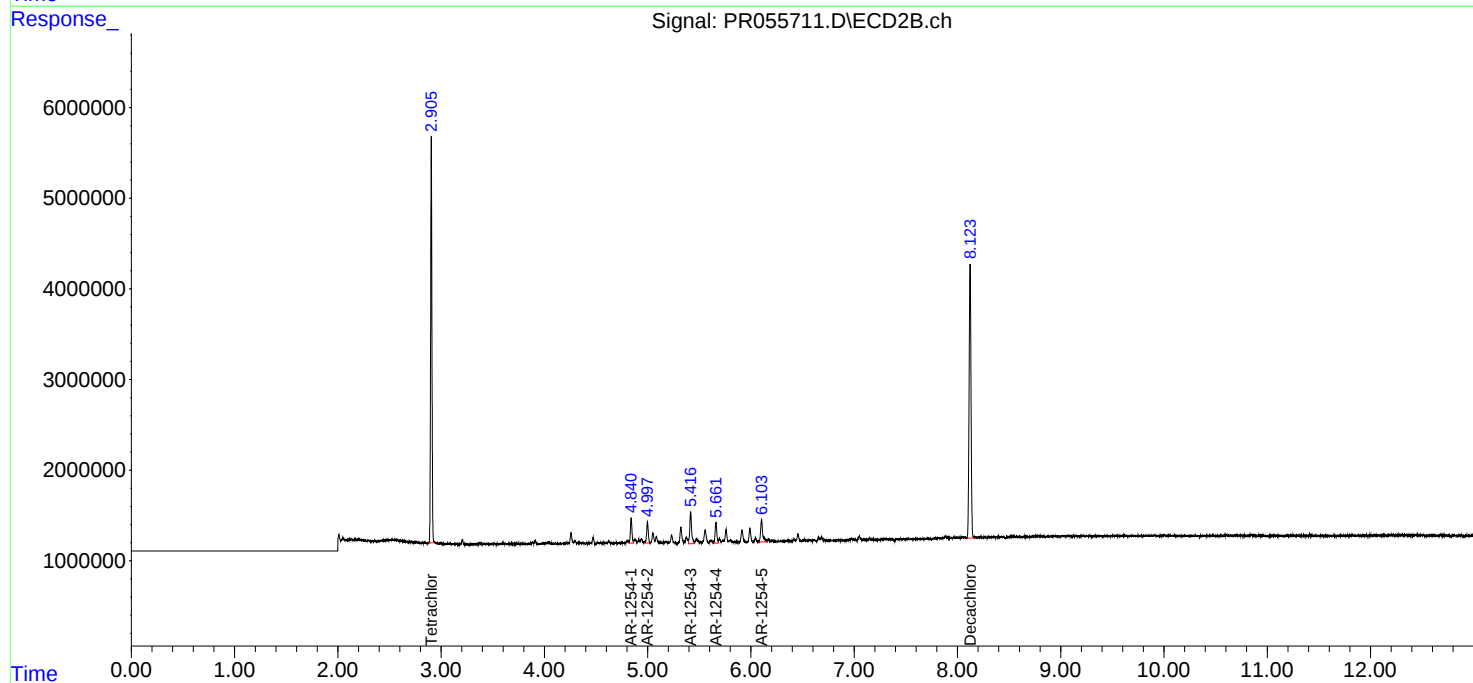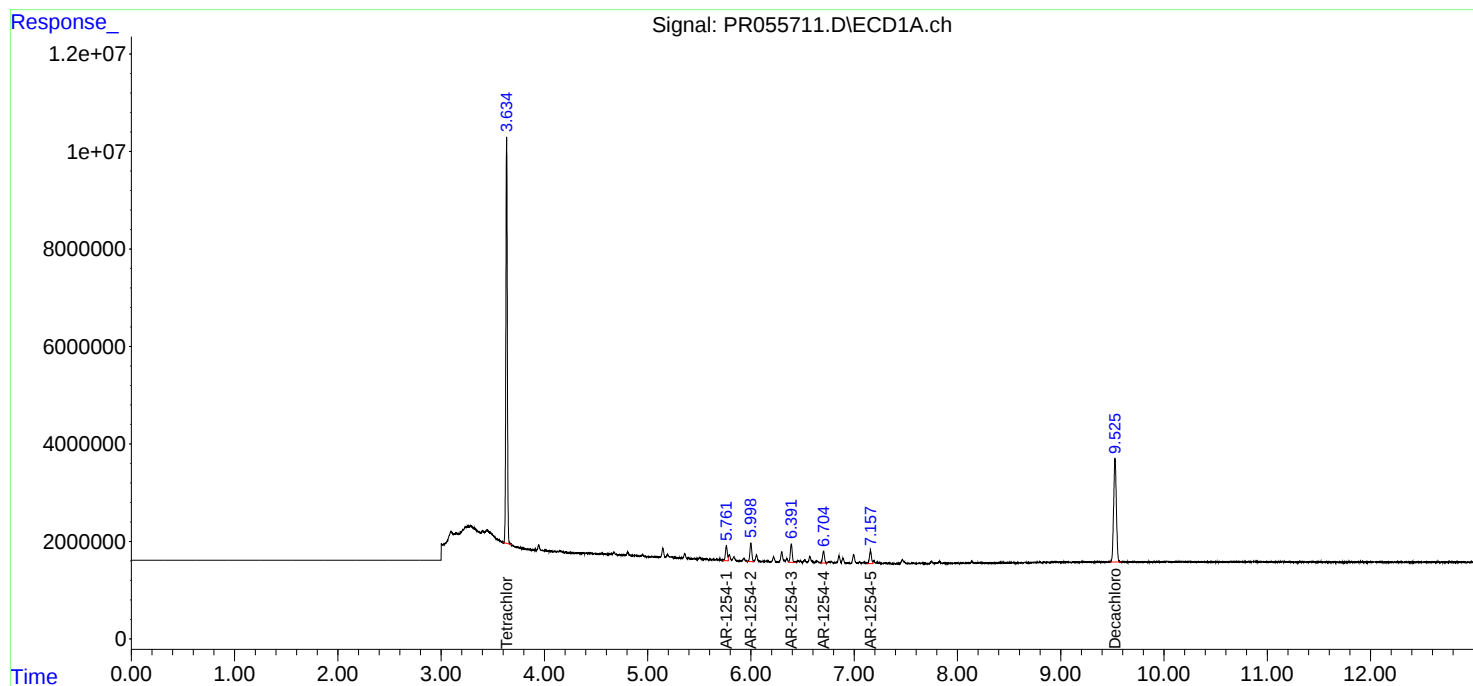


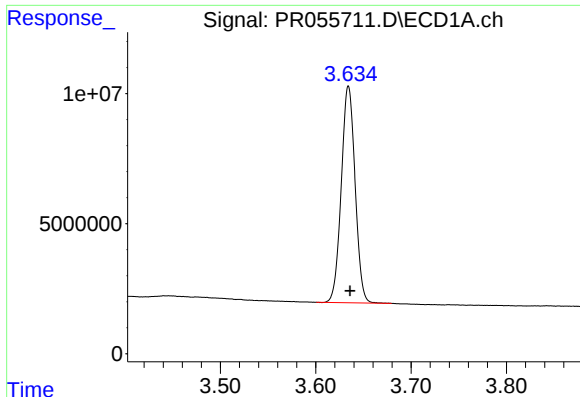

#1 Tetrachloro-m-xylene


R.T.: 3.634 min
Delta R.T.: -0.002 min
Response: 83823755
Conc: 19.64 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2022

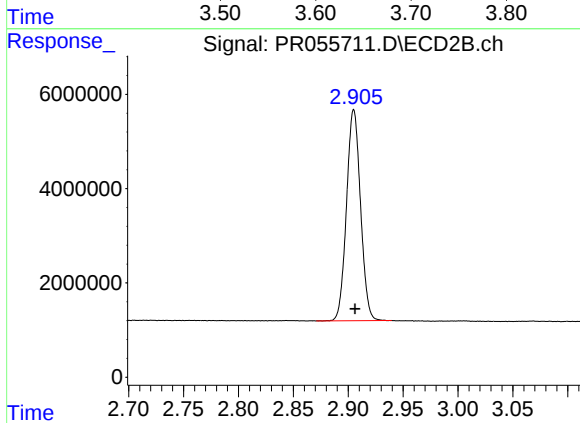


#1 Tetrachloro-m-xylene

R.T.: 2.905 min
Delta R.T.: -0.001 min
Response: 39822883
Conc: 19.83 ng/ml

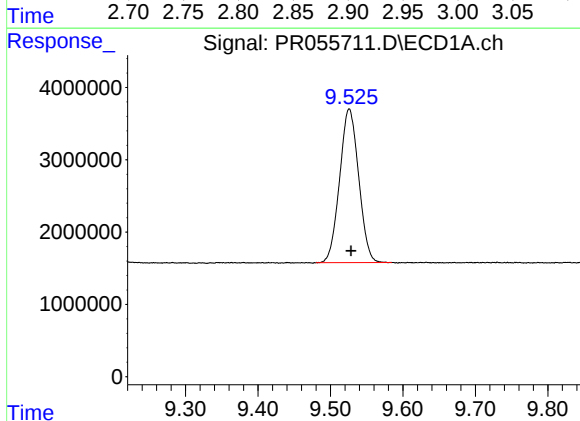


#2 Decachlorobiphenyl

R.T.: 9.526 min
Delta R.T.: -0.003 min
Response: 38792193
Conc: 21.82 ng/ml

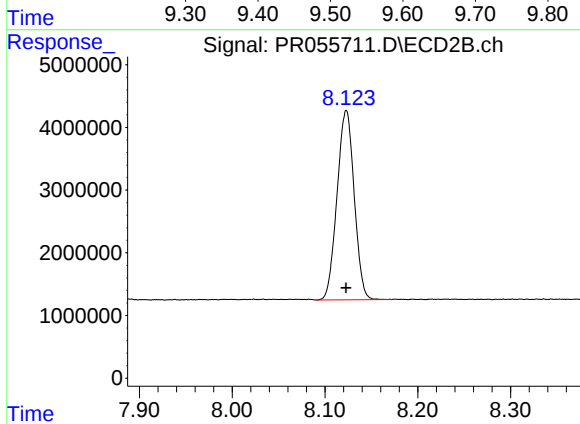

#2 Decachlorobiphenyl


R.T.: 8.123 min
Delta R.T.: 0.000 min
Response: 38837341
Conc: 21.35 ng/ml

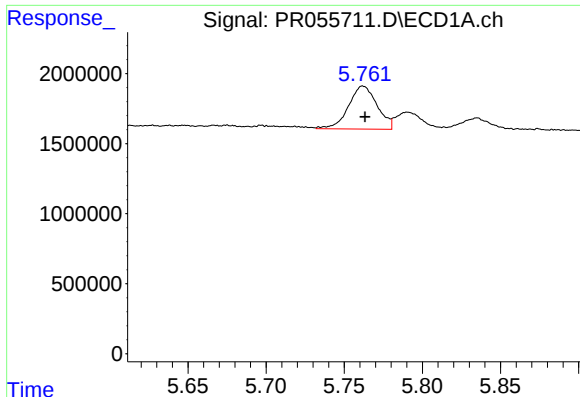

#26 AR-1254-1


R.T.: 5.762 min
Delta R.T.: -0.001 min
Response: 3910617
Conc: 38.18 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2022

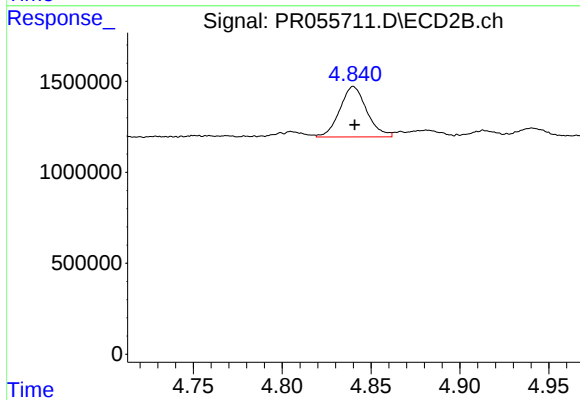


#26 AR-1254-1

R.T.: 4.840 min
Delta R.T.: 0.000 min
Response: 2930206
Conc: 26.82 ng/ml

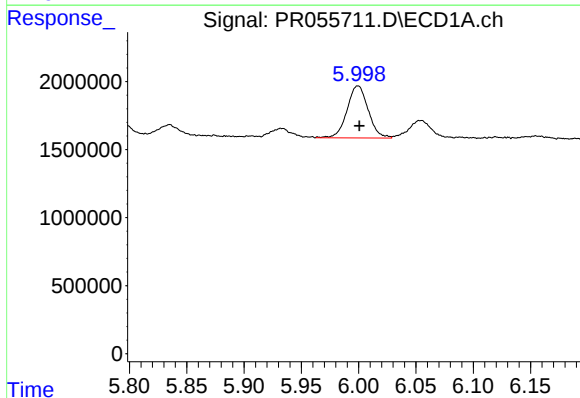


#27 AR-1254-2

R.T.: 5.999 min
Delta R.T.: -0.001 min
Response: 4910815
Conc: 33.41 ng/ml

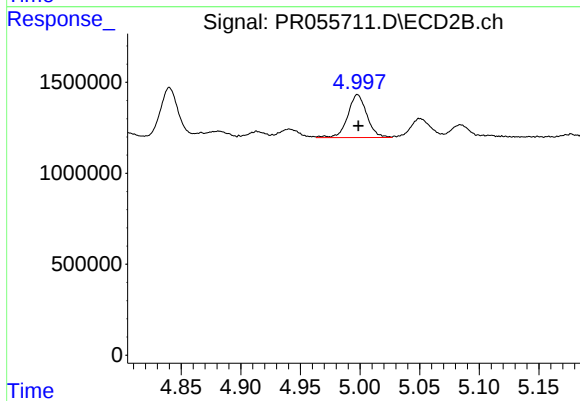

#27 AR-1254-2


R.T.: 4.998 min
Delta R.T.: 0.000 min
Response: 2613739
Conc: 26.99 ng/ml

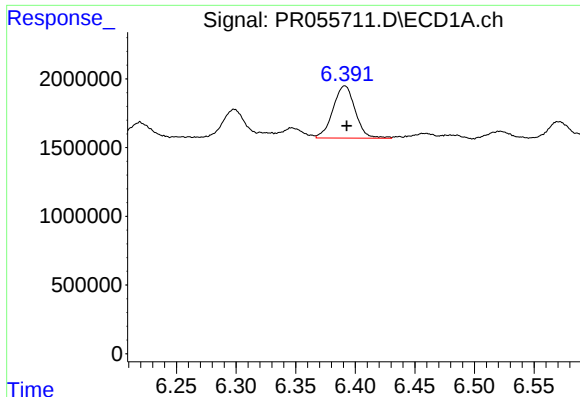

#28 AR-1254-3


R.T.: 6.391 min
Delta R.T.: -0.002 min
Response: 4944898
Conc: 33.75 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2022

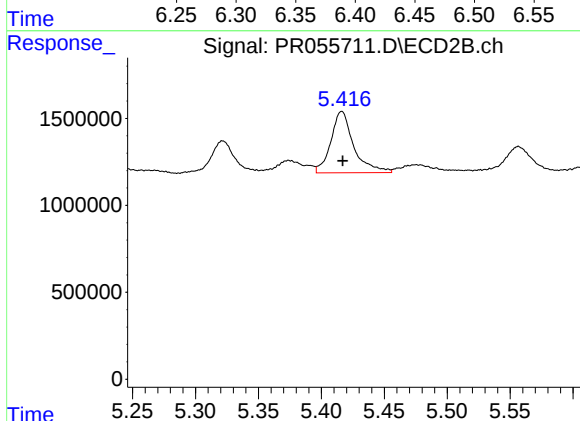


#28 AR-1254-3

R.T.: 5.416 min
Delta R.T.: 0.000 min
Response: 4465216
Conc: 29.31 ng/ml

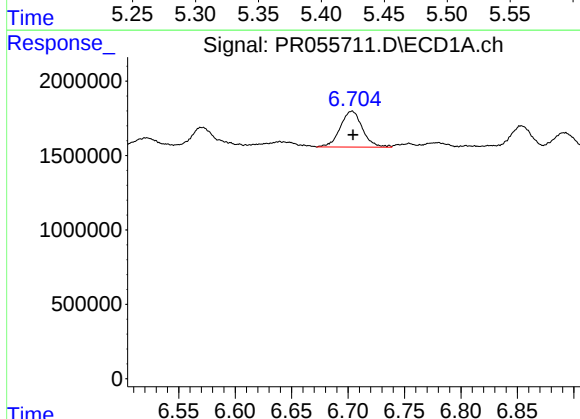


#29 AR-1254-4

R.T.: 6.703 min
Delta R.T.: -0.001 min
Response: 3312437
Conc: 31.95 ng/ml

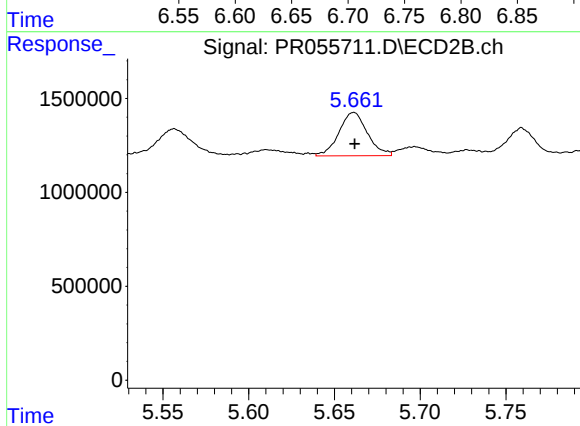

#29 AR-1254-4


R.T.: 5.661 min
Delta R.T.: 0.000 min
Response: 2671781
Conc: 27.12 ng/ml

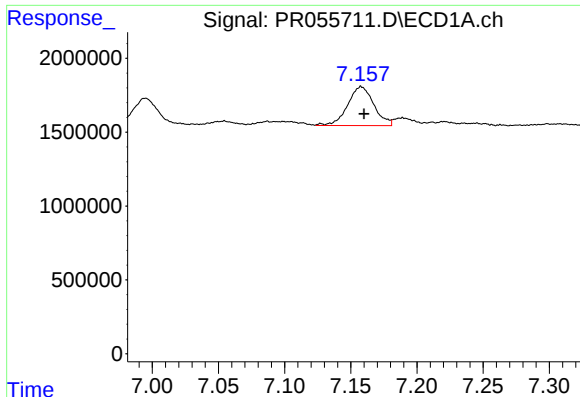

#30 AR-1254-5

R.T.: 7.158 min
Delta R.T.: -0.002 min
Response: 3636022
Conc: 33.53 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2022

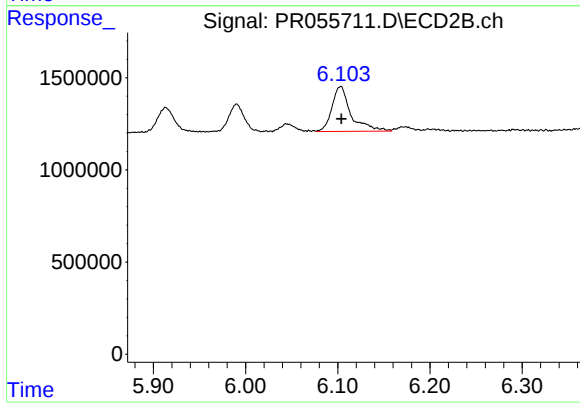

#30 AR-1254-5

R.T.: 6.103 min
Delta R.T.: 0.000 min
Response: 3502698
Conc: 25.85 ng/ml