

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR080622\
 Data File : PR055713.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2022 08:50
 Operator : AJ\MA
 Sample : N3980-09
 Misc : AR1268 MDL 25 PPB
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-WATER-03-QT3-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 14:26:29 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080522.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 05 12:39:02 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.635	2.905	89203082	42154359	20.905	20.995
2) SA Decachlor...	9.527	8.122	44529208	44039738	25.044	24.210
Target Compounds						
41) L9 AR-1268-1	8.128	6.986	8824910	8512526	35.392	30.263
42) L9 AR-1268-2	8.218	7.056	8177214	7599409	35.816	29.704
43) L9 AR-1268-3	8.435	7.275	7115438	6507062	36.949	30.235
44) L9 AR-1268-4	8.838	7.591	2884716	2899789	32.707	30.516
45) L9 AR-1268-5	9.219	7.883	20136487	20105755	32.932	29.506



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR080622\
Data File : PR055713.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2022 08:50
Operator : AJ\MA
Sample : N3980-09
Misc : AR1268 MDL 25 PPB
ALS Vial : 55 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 14:26:29 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080522.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 05 12:39:02 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

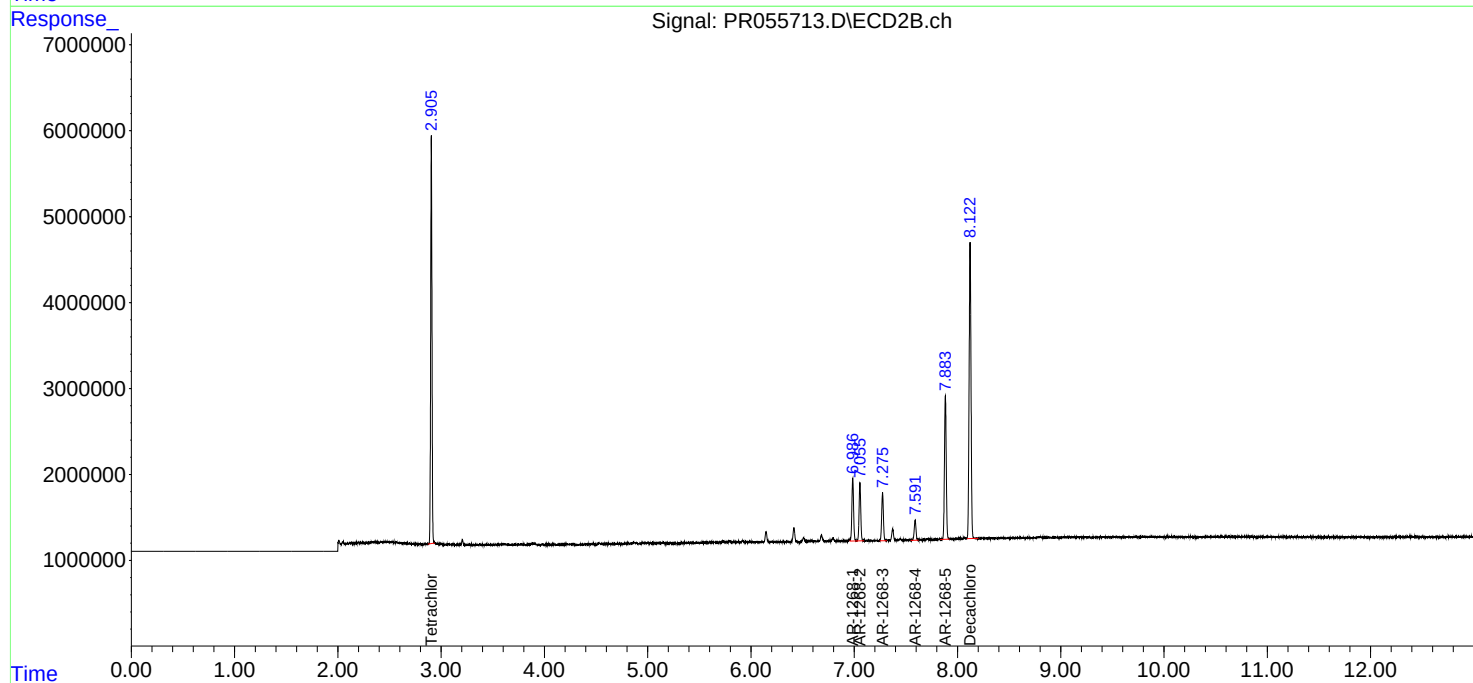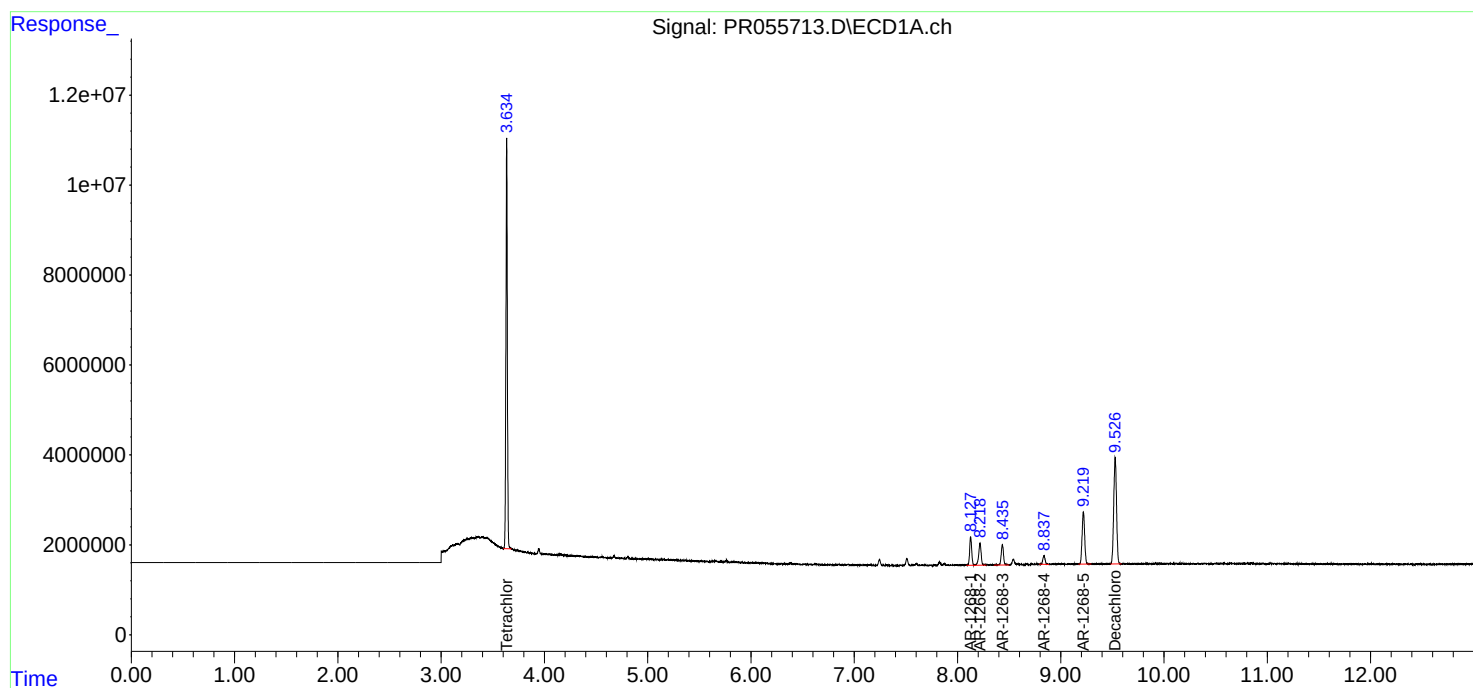


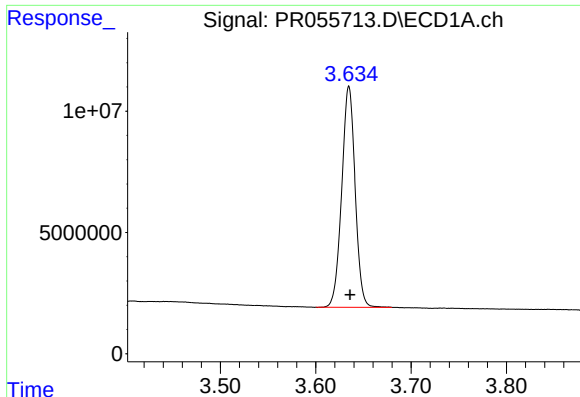

#1 Tetrachloro-m-xylene


R.T.: 3.635 min
Delta R.T.: -0.001 min
Response: 89203082
Conc: 20.91 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2022

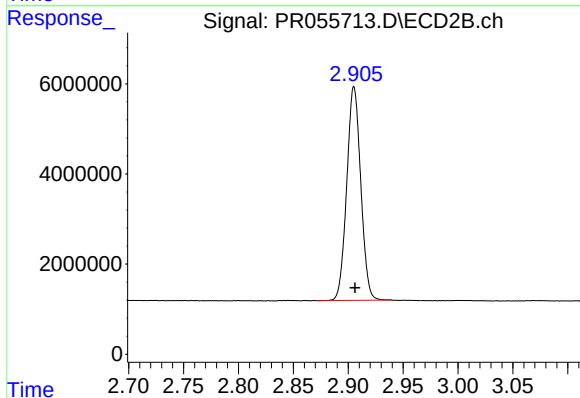


#1 Tetrachloro-m-xylene

R.T.: 2.905 min
Delta R.T.: 0.000 min
Response: 42154359
Conc: 21.00 ng/ml

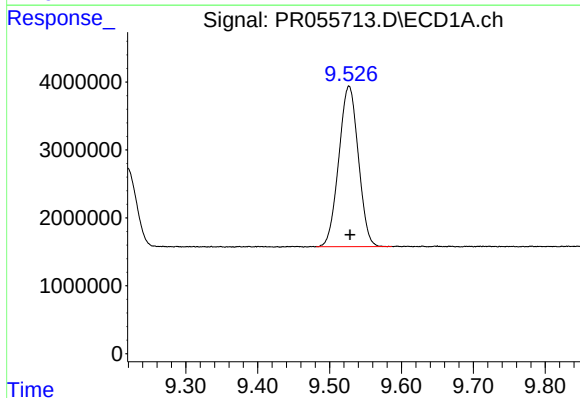


#2 Decachlorobiphenyl

R.T.: 9.527 min
Delta R.T.: -0.001 min
Response: 44529208
Conc: 25.04 ng/ml

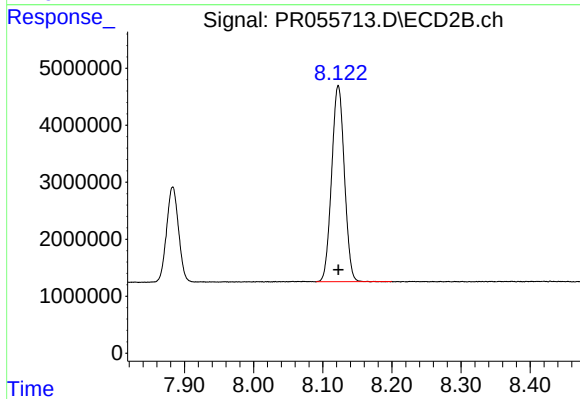

#2 Decachlorobiphenyl


R.T.: 8.122 min
Delta R.T.: 0.000 min
Response: 44039738
Conc: 24.21 ng/ml

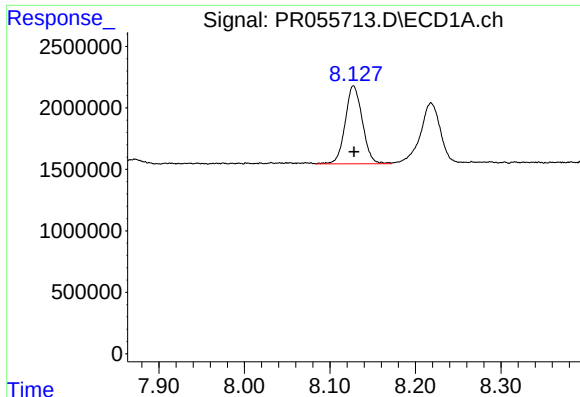

#41 AR-1268-1


R.T.: 8.128 min
Delta R.T.: 0.000 min
Response: 8824910
Conc: 35.39 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2022

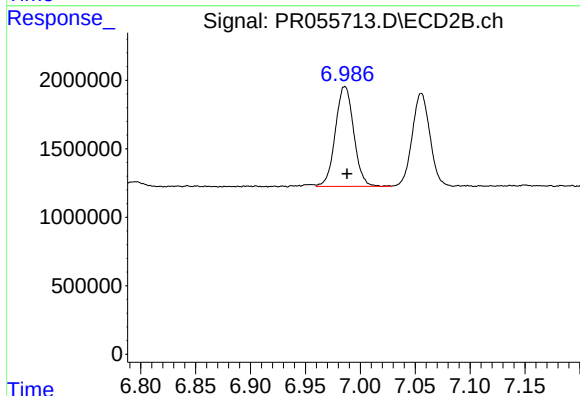


#41 AR-1268-1

R.T.: 6.986 min
Delta R.T.: -0.002 min
Response: 8512526
Conc: 30.26 ng/ml

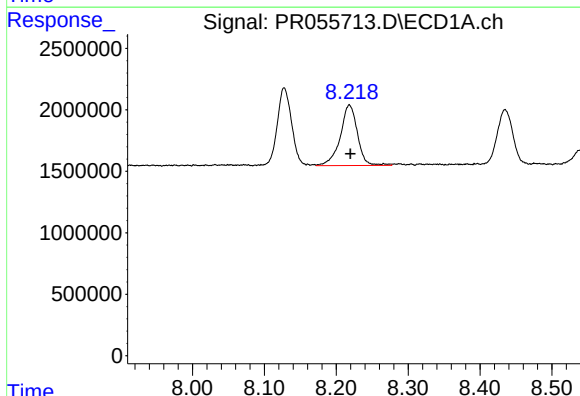


#42 AR-1268-2

R.T.: 8.218 min
Delta R.T.: -0.002 min
Response: 8177214
Conc: 35.82 ng/ml

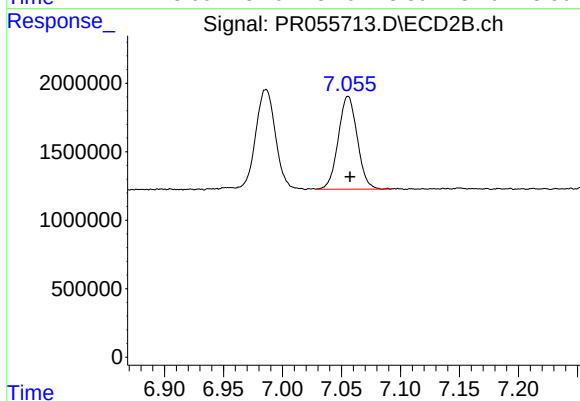

#42 AR-1268-2


R.T.: 7.056 min
Delta R.T.: -0.002 min
Response: 7599409
Conc: 29.70 ng/ml

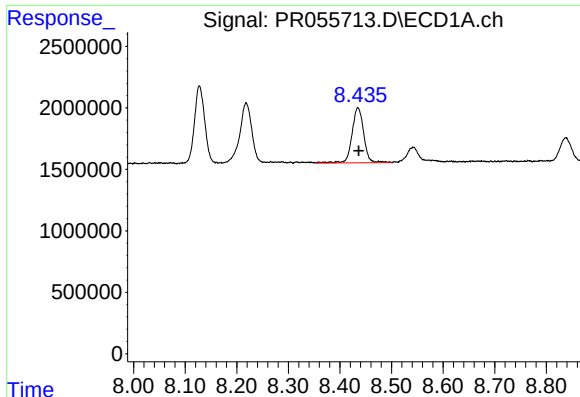

#43 AR-1268-3


R.T.: 8.435 min
Delta R.T.: -0.001 min
Response: 7115438
Conc: 36.95 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2022

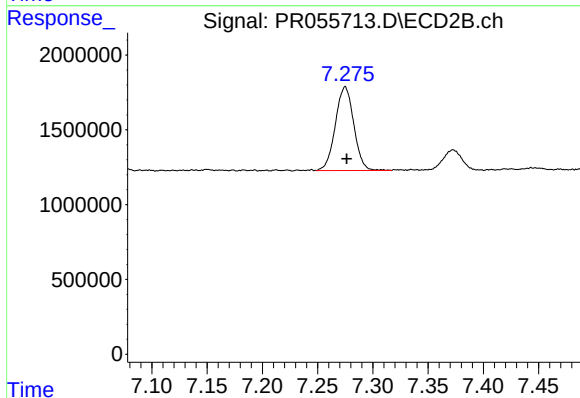


#43 AR-1268-3

R.T.: 7.275 min
Delta R.T.: -0.001 min
Response: 6507062
Conc: 30.24 ng/ml

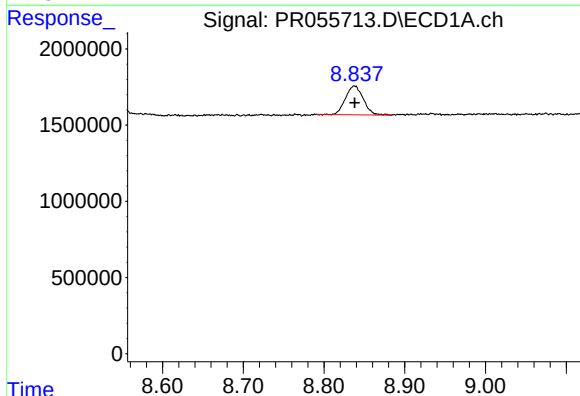


#44 AR-1268-4

R.T.: 8.838 min
Delta R.T.: 0.000 min
Response: 2884716
Conc: 32.71 ng/ml

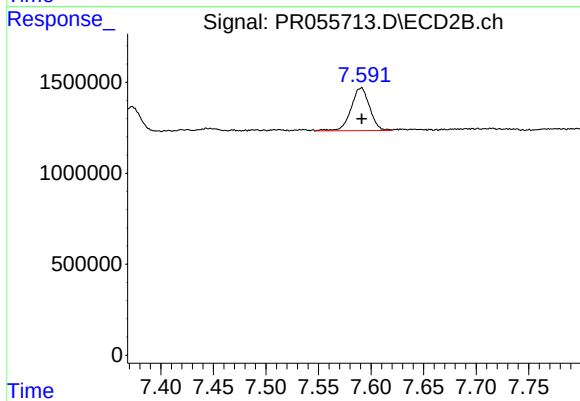

#44 AR-1268-4


R.T.: 7.591 min
Delta R.T.: 0.000 min
Response: 2899789
Conc: 30.52 ng/ml

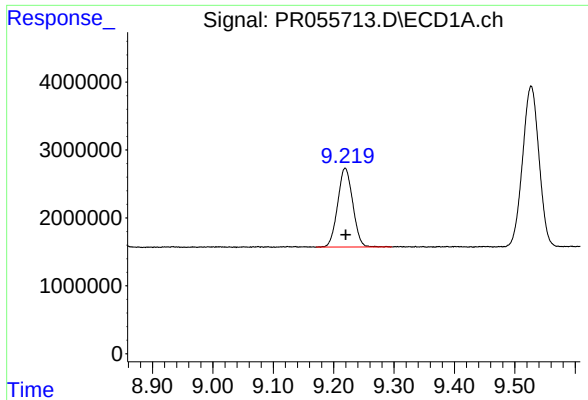

#45 AR-1268-5

R.T.: 9.219 min
Delta R.T.: -0.001 min
Response: 20136487
Conc: 32.93 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2022

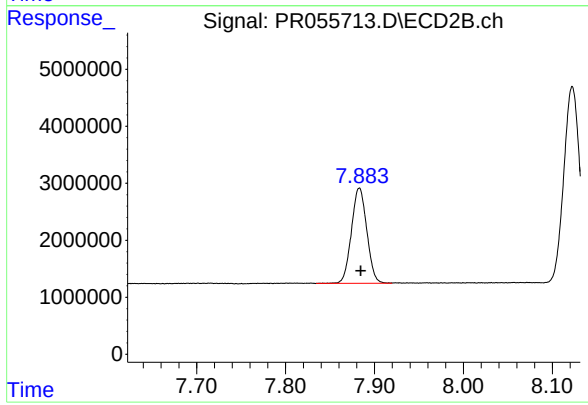

#45 AR-1268-5

R.T.: 7.883 min
Delta R.T.: -0.001 min
Response: 20105755
Conc: 29.51 ng/ml