

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR080624\
 Data File : PR068057.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2024 23:17
 Operator : AJ\MA
 Sample : P3390-07
 Misc : AR1660 LOD 40 PPB
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 07 03:28:21 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 07 00:26:28 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.678	3.011	49194796	96094193	19.338	22.037
2) SA Decachlor...	9.579	8.332	92532347	106.2E6	21.088	23.438
Target Compounds						
3) L1 AR-1016-1	4.902	4.144	1768301	4598729	30.257	30.600
4) L1 AR-1016-2	4.924	4.162	2937130	6233199	26.491	29.703
5) L1 AR-1016-3	4.988	4.343	2584830	3539828	33.658	31.032
6) L1 AR-1016-4	5.091	4.395	1576818	3327015	25.180	34.790 #
7) L1 AR-1016-5	5.406	4.615	1306505	3727658	26.018	31.188
8) L2 AR-1221-1	0.000	3.237	0	510008	N.D.	3.281 #
9) L2 AR-1221-2	3.990	3.320	1019983	1941976	45.391	26.441 #
10) L2 AR-1221-3	4.068	3.403	1392463	2375155	19.490	7.331 #
11) L3 AR-1232-1	4.068	3.403	1392463	2375155	23.662	23.449
12) L3 AR-1232-2	4.616	4.162	2008830	6233199	63.959	61.864
13) L3 AR-1232-3	4.924	4.343	2937130	3539828	54.482	65.181
14) L3 AR-1232-4	5.091	4.437	1576818	3597401	52.735	71.991 #
15) L3 AR-1232-5	5.193	4.615	975327	3727658	63.327	70.105
16) L4 AR-1242-1	4.902	4.144	1768301	4598729	36.148	30.167
17) L4 AR-1242-2	4.924	4.162	2937130	6233199	32.327	29.148
18) L4 AR-1242-3	4.988	4.343	2584830	3539828	41.185	33.320
19) L4 AR-1242-4	5.091	4.437	1576818	3597401	31.595	35.772
20) L4 AR-1242-5	5.879	4.990	387111	4534281	8.421	28.913 #
21) L5 AR-1248-1	4.902	4.144	1768301	4598729	46.072	38.645
22) L5 AR-1248-2	5.193	4.395	975327	3327015	18.593	17.653
23) L5 AR-1248-3	5.406	4.437	1306505	3597401	18.556	18.873
24) L5 AR-1248-4	5.840	4.615	162278	3727658	2.182	17.262 #
25) L5 AR-1248-5	5.879	5.032	387111	1371318	4.795	6.453 #
26) L6 AR-1254-1	5.809	4.990	1285426	4534281	18.012	17.730
27) L6 AR-1254-2	6.046	5.151	1085112	3554998	9.668	15.466 #
28) L6 AR-1254-3	6.432	5.578	909319	1331779	6.767	3.691 #
29) L6 AR-1254-4	6.747	5.825	489018	702785	4.679	3.270 #
30) L6 AR-1254-5	7.200	6.275	5159165	10695502	41.534	32.395
31) L7 AR-1260-1	6.616	5.720	2476099	8629373	26.791	35.248 #
32) L7 AR-1260-2	6.899	5.926	4285419	10236825	30.153	35.260
33) L7 AR-1260-3	7.288	6.087	4709327	9957333	34.009	36.259
34) L7 AR-1260-4	7.530	6.598	3841771	7523769	30.311	35.885
35) L7 AR-1260-5	7.867	6.863	11602223	15642033	31.829	32.315
36) L8 AR-1262-1	7.288	6.321	4709327	8447157	23.643	24.454
37) L8 AR-1262-2	7.867	6.863	11602223	15642033	26.793	25.716
38) L8 AR-1262-3	8.178	7.171	6927622	6022180	22.124	25.221
39) L8 AR-1262-4	8.258	7.237	5139813	12300917	18.719	27.682 #
40) L8 AR-1262-5	8.885	7.778	3297554	3846471	17.421	18.885
41) L9 AR-1268-1	8.178	7.171	6927622	6022180	11.488	8.157 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR080624\
 Data File : PR068057.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2024 23:17
 Operator : AJ\MA
 Sample : P3390-07
 Misc : AR1660 LOD 40 PPB
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 07 03:28:21 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 07 00:26:28 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.258	7.237	5139813	12300917	9.018	18.220 #
43) L9	AR-1268-3	8.479	7.464	557059	700402	1.004	1.136
44) L9	AR-1268-4	8.885	7.778	3297554	3846471	16.279	18.445
45) L9	AR-1268-5	9.270	8.076	2229119	1665251	1.425	1.166



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR080624\
Data File : PR068057.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2024 23:17
Operator : AJ\MA
Sample : P3390-07
Misc : AR1660 LOD 40 PPB
ALS Vial : 48 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 03:28:21 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 07 00:26:28 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

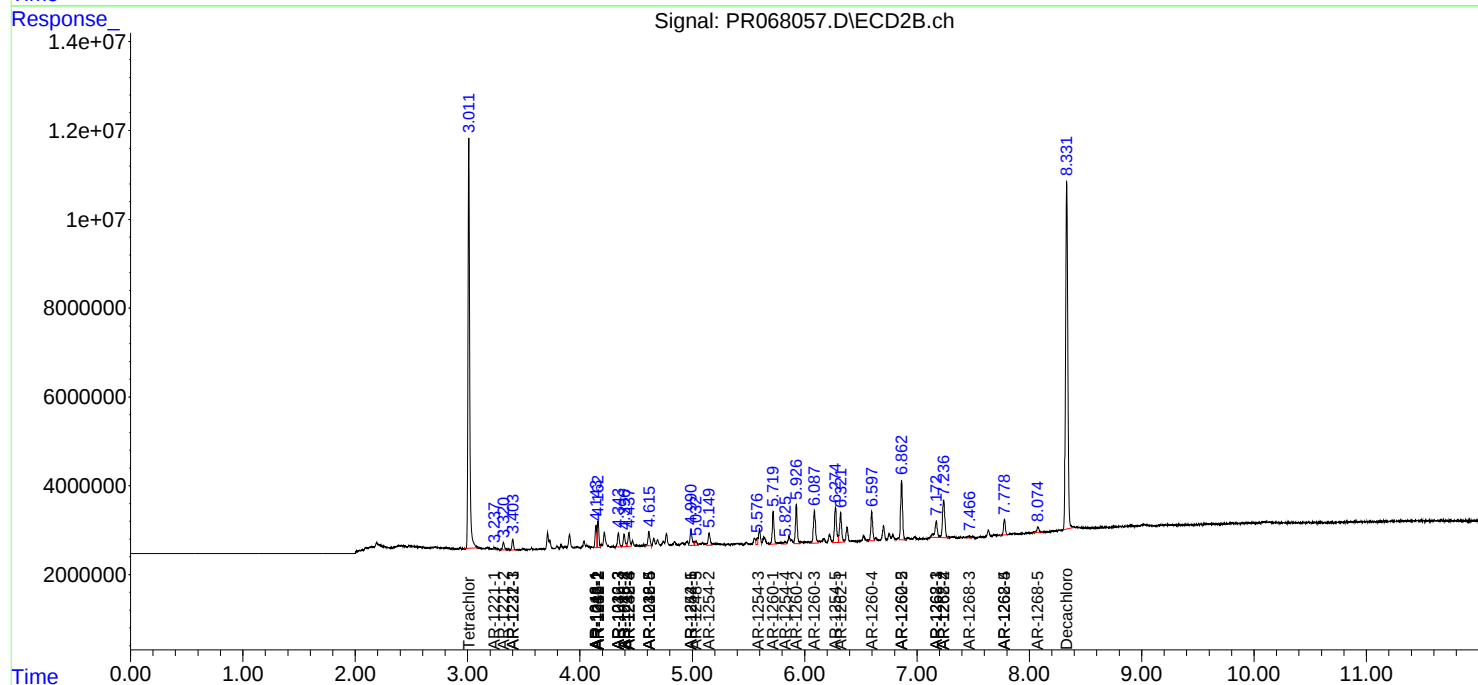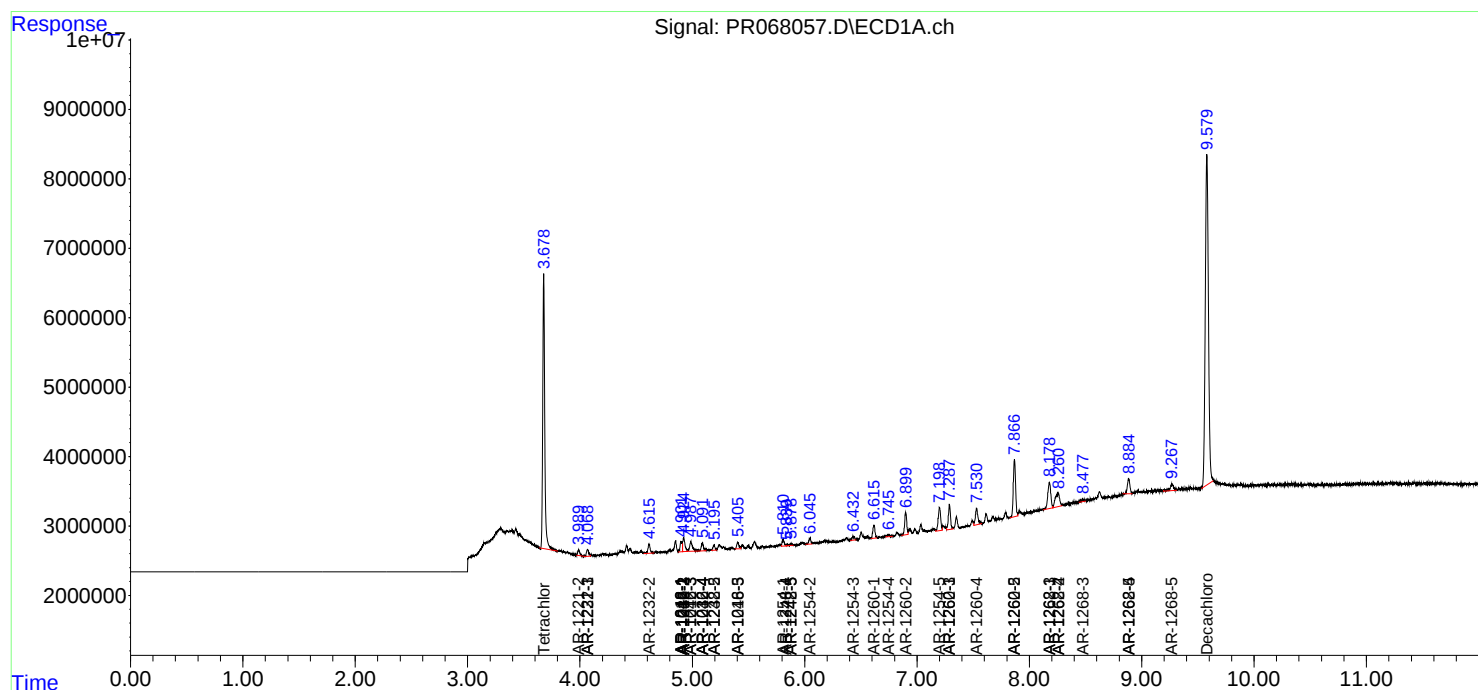


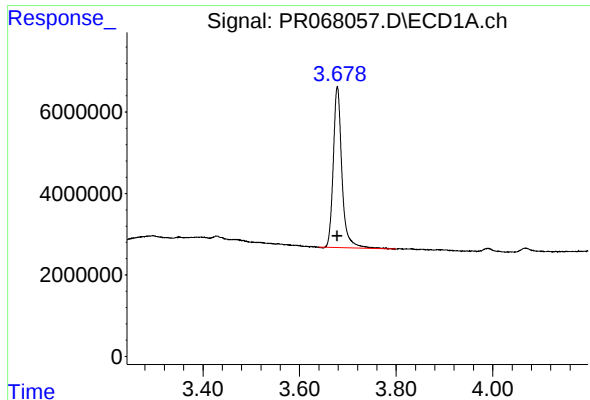

#1 Tetrachloro-m-xylene


R.T.: 3.678 min
Delta R.T.: 0.000 min
Response: 49194796
Conc: 19.34 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

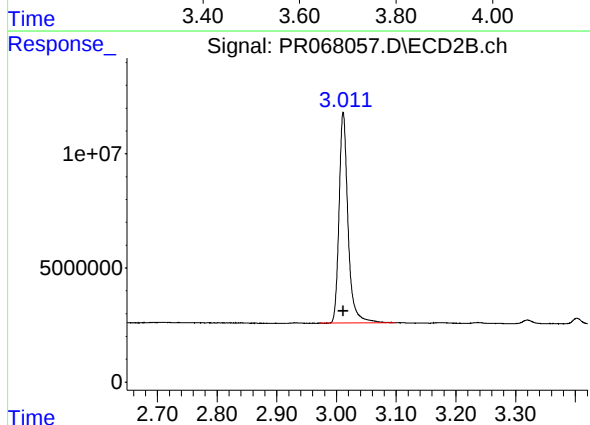


#1 Tetrachloro-m-xylene

R.T.: 3.011 min
Delta R.T.: 0.000 min
Response: 96094193
Conc: 22.04 ng/ml

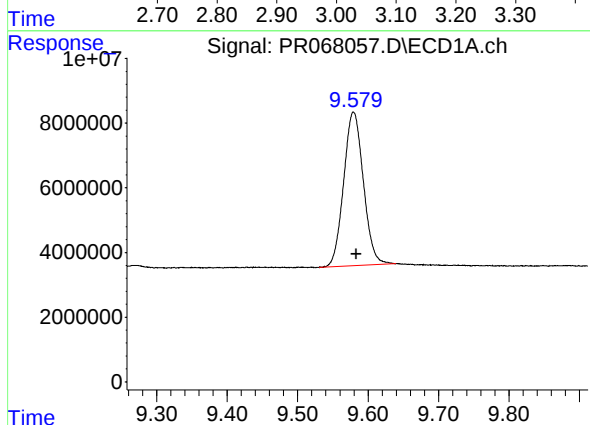


#2 Decachlorobiphenyl

R.T.: 9.579 min
Delta R.T.: -0.004 min
Response: 92532347
Conc: 21.09 ng/ml

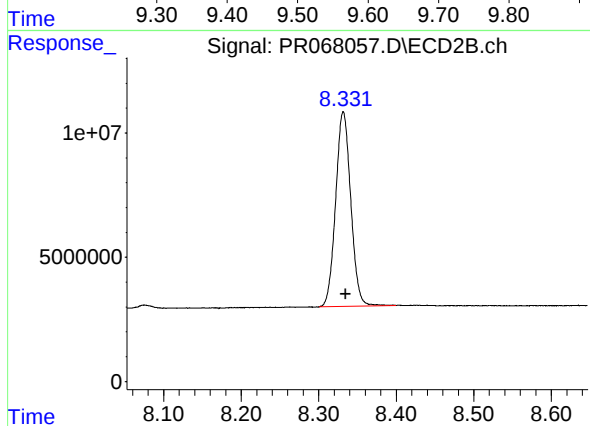

#2 Decachlorobiphenyl


R.T.: 8.332 min
Delta R.T.: -0.003 min
Response: 106197351
Conc: 23.44 ng/ml

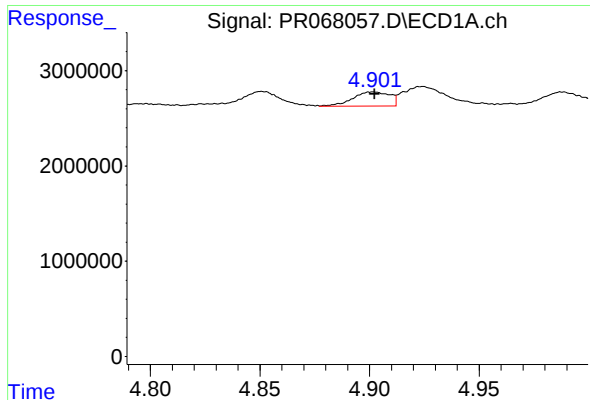

#3 AR-1016-1


R.T.: 4.902 min
Delta R.T.: 0.000 min
Response: 1768301
Conc: 30.26 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

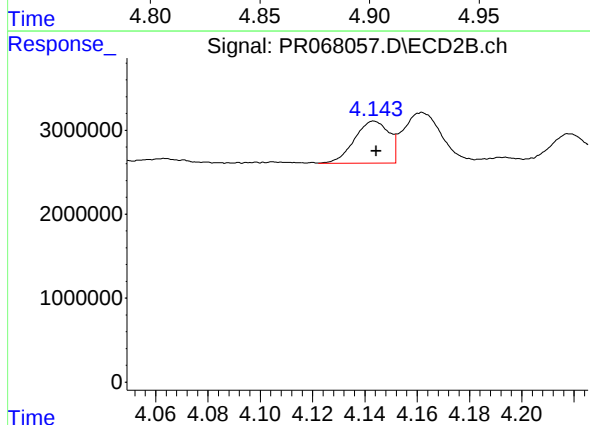


#3 AR-1016-1

R.T.: 4.144 min
Delta R.T.: 0.000 min
Response: 4598729
Conc: 30.60 ng/ml

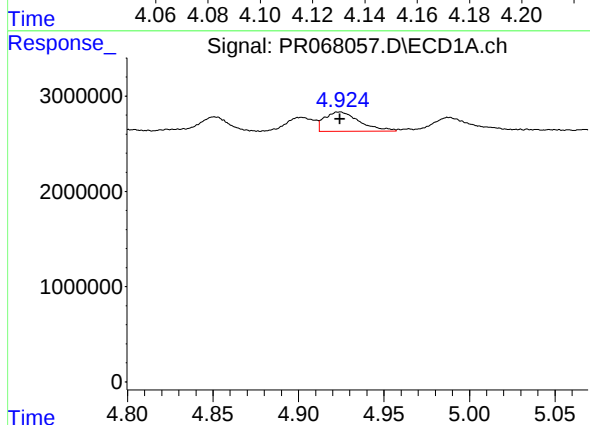


#4 AR-1016-2

R.T.: 4.924 min
Delta R.T.: 0.000 min
Response: 2937130
Conc: 26.49 ng/ml

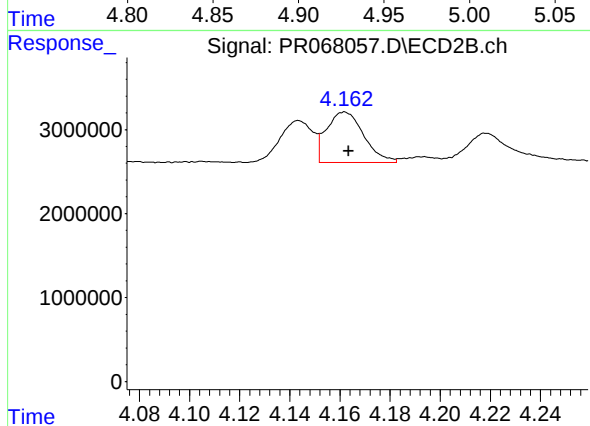

#4 AR-1016-2


R.T.: 4.162 min
Delta R.T.: -0.002 min
Response: 6233199
Conc: 29.70 ng/ml

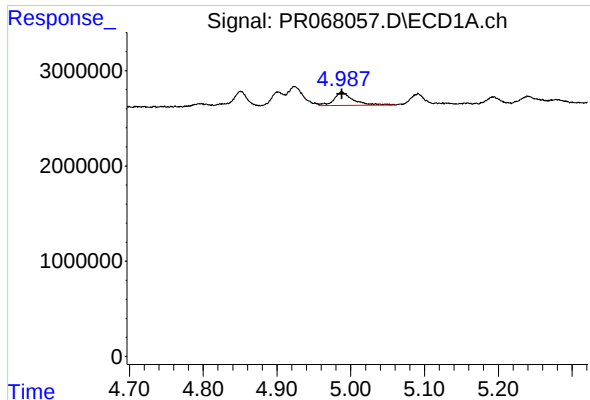

#5 AR-1016-3


R.T.: 4.988 min
Delta R.T.: 0.000 min
Response: 2584830
Conc: 33.66 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

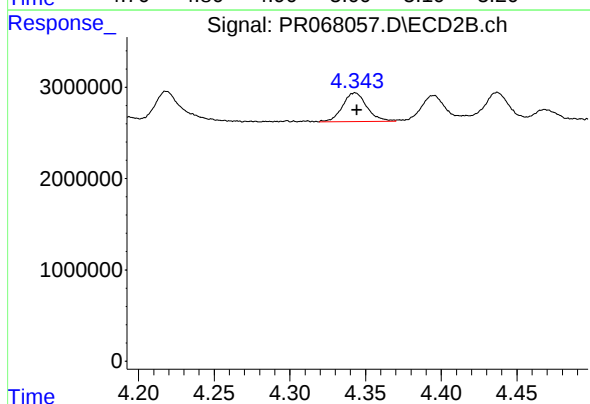


#5 AR-1016-3

R.T.: 4.343 min
Delta R.T.: -0.001 min
Response: 3539828
Conc: 31.03 ng/ml

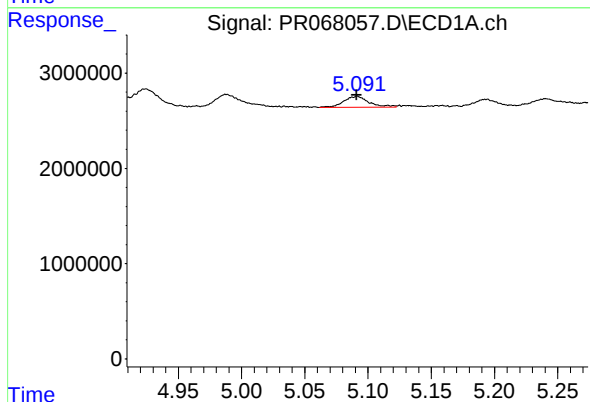


#6 AR-1016-4

R.T.: 5.091 min
Delta R.T.: 0.000 min
Response: 1576818
Conc: 25.18 ng/ml

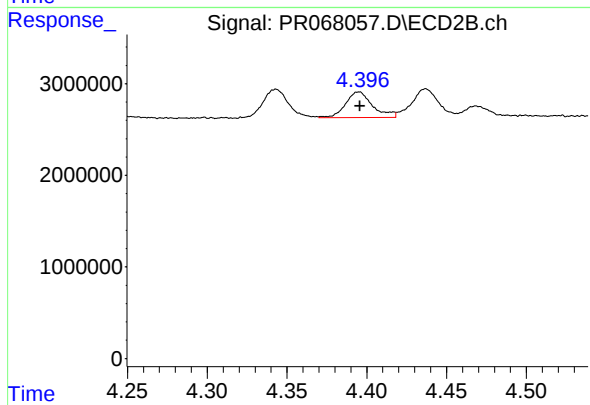

#6 AR-1016-4


R.T.: 4.395 min
Delta R.T.: 0.000 min
Response: 3327015
Conc: 34.79 ng/ml

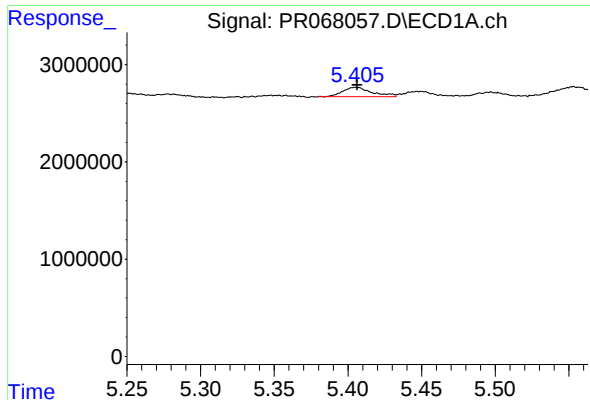

#7 AR-1016-5


R.T.: 5.406 min
Delta R.T.: 0.000 min
Response: 1306505
Conc: 26.02 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

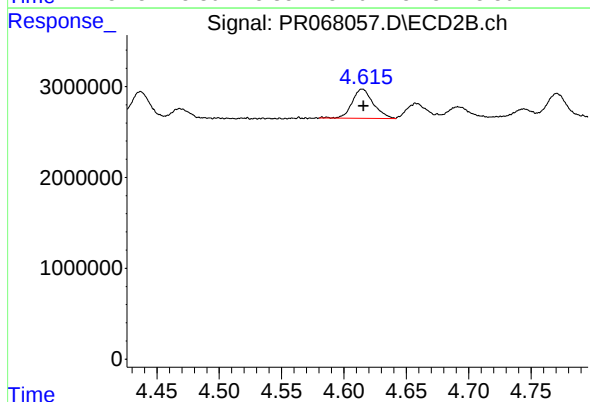


#7 AR-1016-5

R.T.: 4.615 min
Delta R.T.: -0.001 min
Response: 3727658
Conc: 31.19 ng/ml

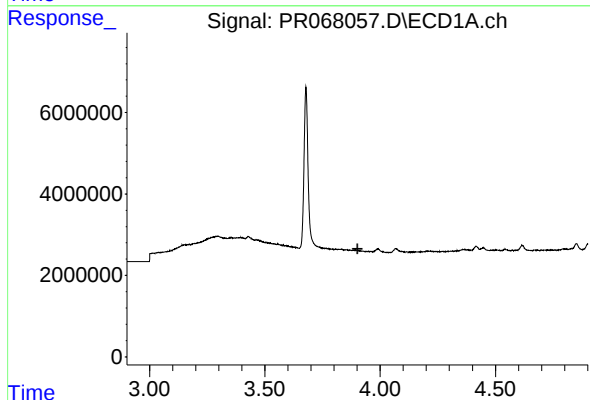


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T.: 3.902 min
Response: 0
Conc: N.D.

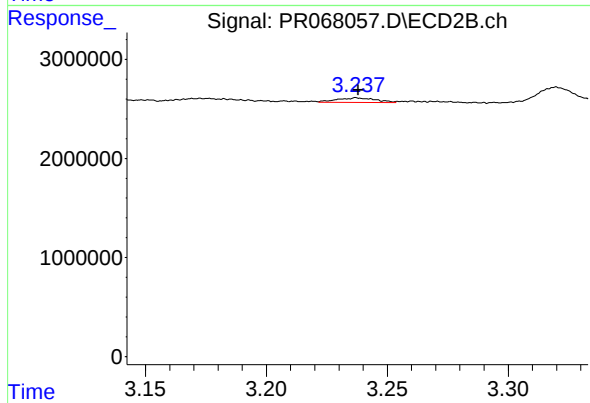

#8 AR-1221-1


R.T.: 3.237 min
Delta R.T.: 0.000 min
Response: 510008
Conc: 3.28 ng/ml

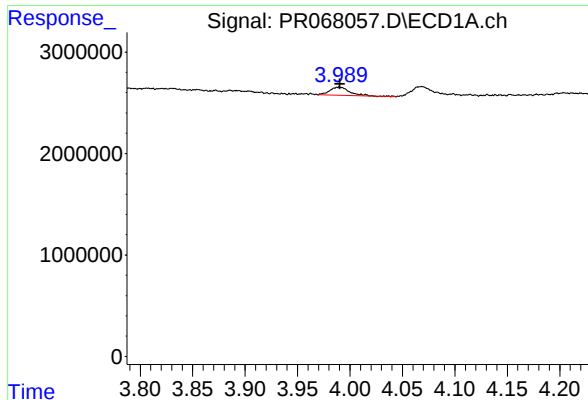

#9 AR-1221-2


R.T.: 3.990 min
Delta R.T.: 0.000 min
Response: 1019983
Conc: 45.39 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

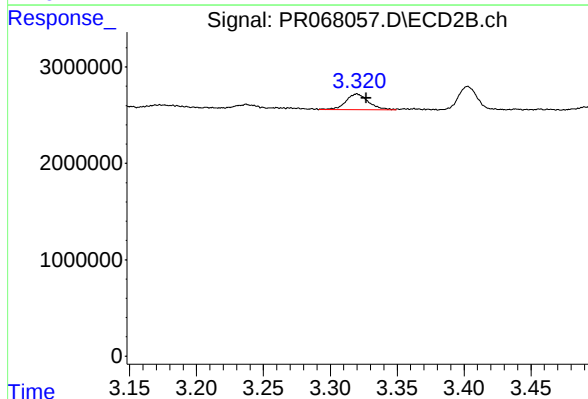


#9 AR-1221-2

R.T.: 3.320 min
Delta R.T.: -0.007 min
Response: 1941976
Conc: 26.44 ng/ml

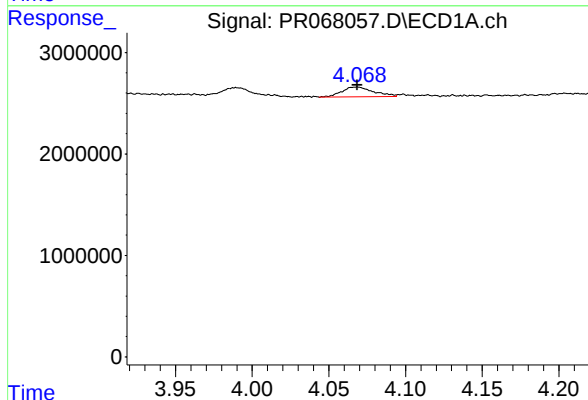


#10 AR-1221-3

R.T.: 4.068 min
Delta R.T.: 0.000 min
Response: 1392463
Conc: 19.49 ng/ml

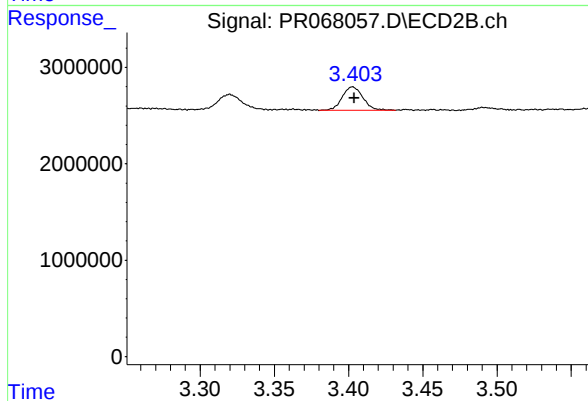

#10 AR-1221-3


R.T.: 3.403 min
Delta R.T.: -0.001 min
Response: 2375155
Conc: 7.33 ng/ml

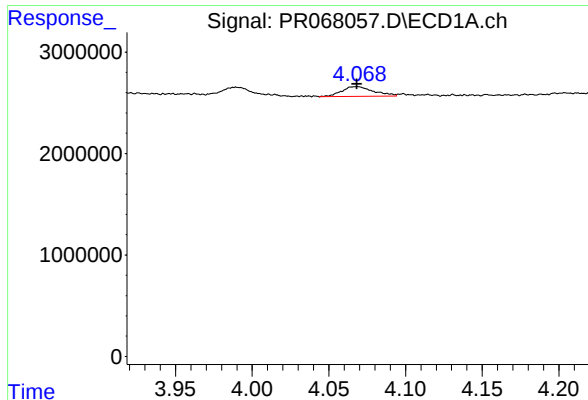

#11 AR-1232-1


R.T.: 4.068 min
Delta R.T.: 0.000 min
Response: 1392463
Conc: 23.66 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

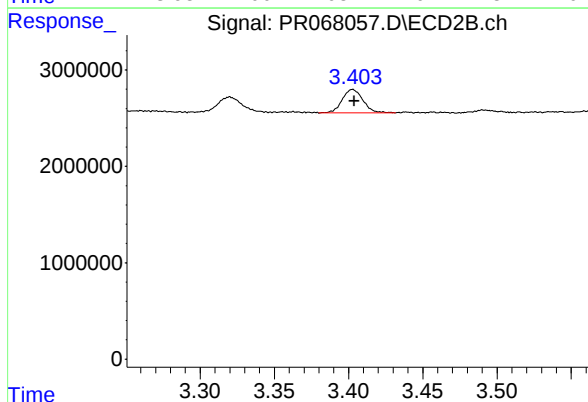


#11 AR-1232-1

R.T.: 3.403 min
Delta R.T.: -0.001 min
Response: 2375155
Conc: 23.45 ng/ml

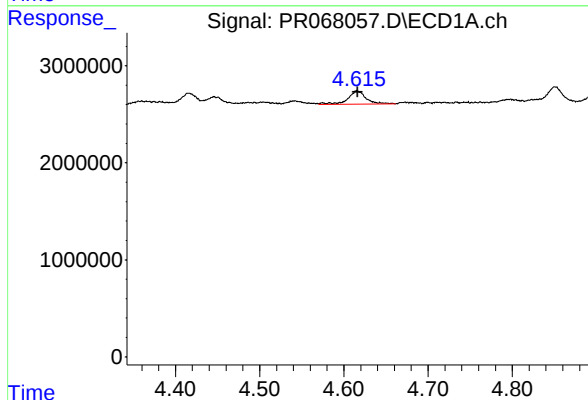


#12 AR-1232-2

R.T.: 4.616 min
Delta R.T.: 0.000 min
Response: 2008830
Conc: 63.96 ng/ml

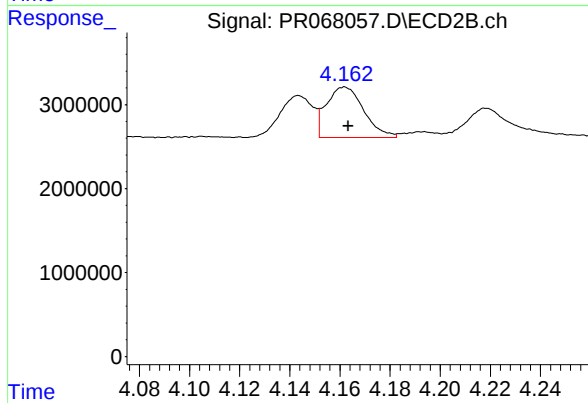

#12 AR-1232-2


R.T.: 4.162 min
Delta R.T.: -0.001 min
Response: 6233199
Conc: 61.86 ng/ml

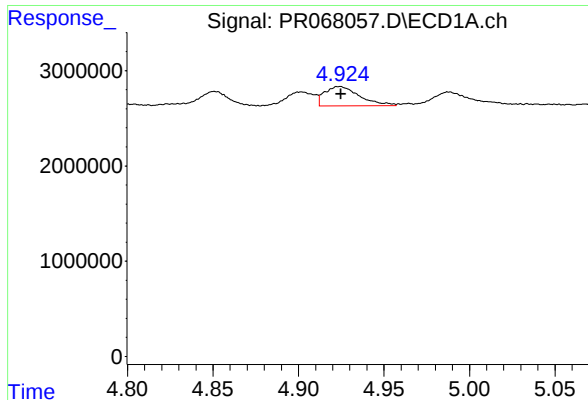

#13 AR-1232-3


R.T.: 4.924 min
Delta R.T.: 0.000 min
Response: 2937130
Conc: 54.48 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

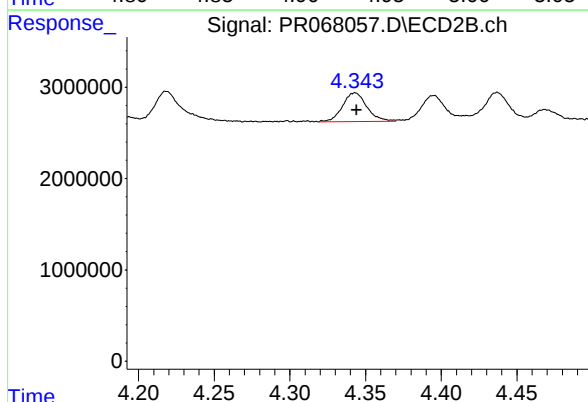


#13 AR-1232-3

R.T.: 4.343 min
Delta R.T.: -0.001 min
Response: 3539828
Conc: 65.18 ng/ml

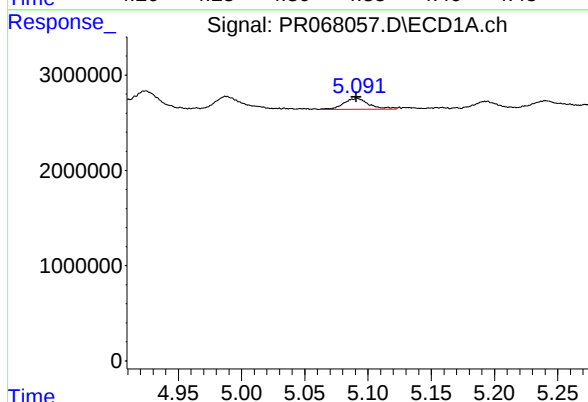


#14 AR-1232-4

R.T.: 5.091 min
Delta R.T.: 0.000 min
Response: 1576818
Conc: 52.74 ng/ml

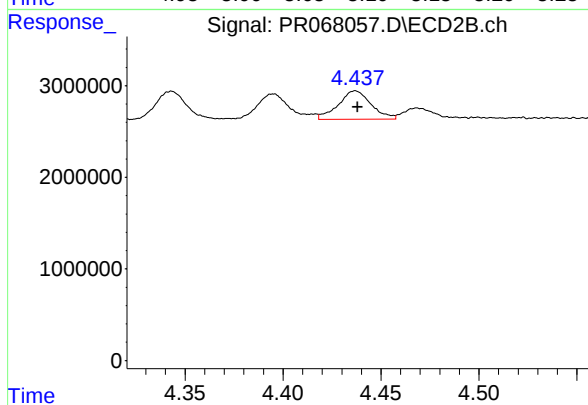

#14 AR-1232-4


R.T.: 4.437 min
Delta R.T.: -0.001 min
Response: 3597401
Conc: 71.99 ng/ml

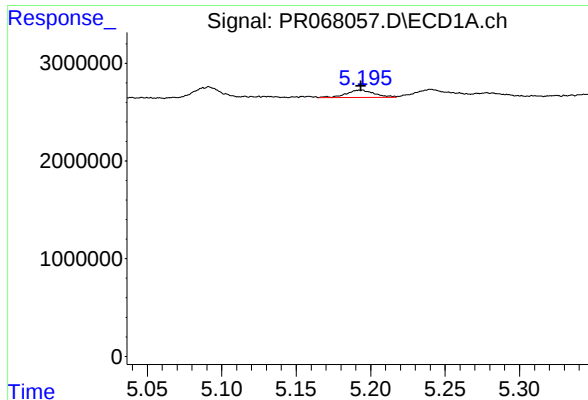

#15 AR-1232-5


R.T.: 5.193 min
Delta R.T.: 0.000 min
Response: 975327
Conc: 63.33 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

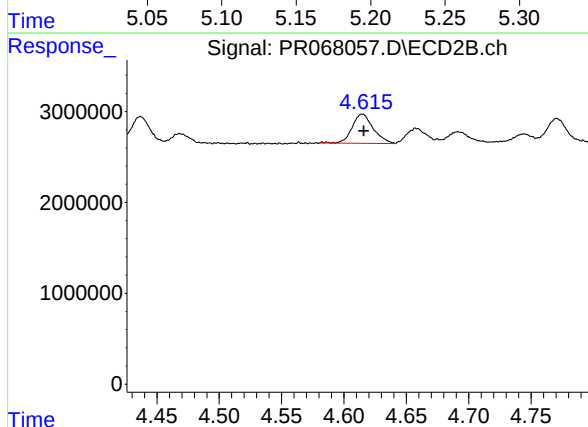


#15 AR-1232-5

R.T.: 4.615 min
Delta R.T.: -0.001 min
Response: 3727658
Conc: 70.10 ng/ml

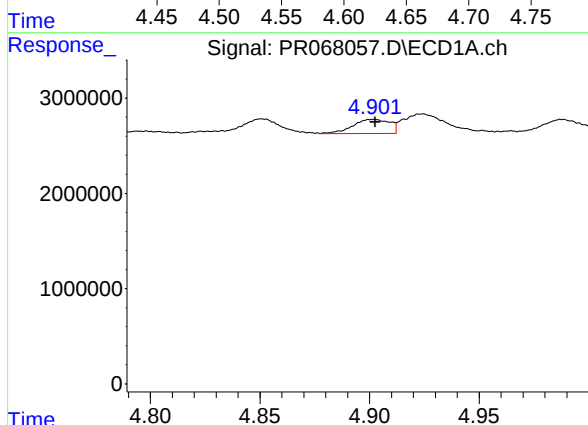


#16 AR-1242-1

R.T.: 4.902 min
Delta R.T.: -0.001 min
Response: 1768301
Conc: 36.15 ng/ml

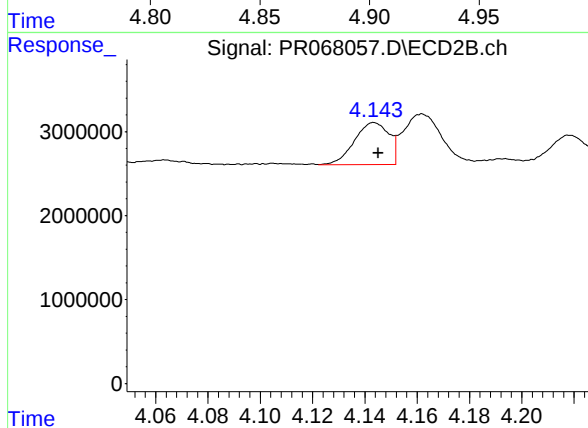

#16 AR-1242-1


R.T.: 4.144 min
Delta R.T.: -0.001 min
Response: 4598729
Conc: 30.17 ng/ml

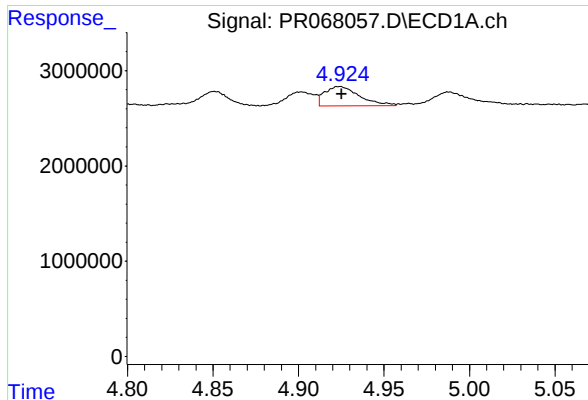

#17 AR-1242-2


R.T.: 4.924 min
Delta R.T.: -0.001 min
Response: 2937130
Conc: 32.33 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

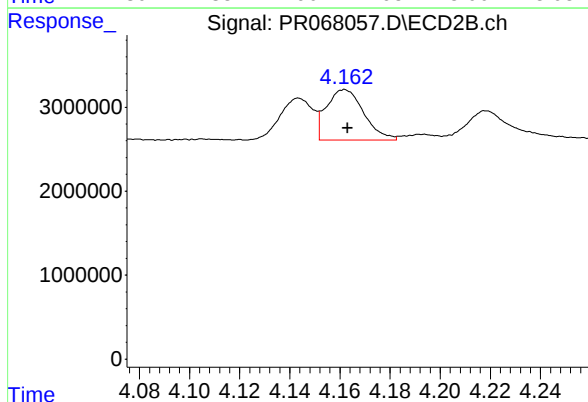


#17 AR-1242-2

R.T.: 4.162 min
Delta R.T.: -0.001 min
Response: 6233199
Conc: 29.15 ng/ml

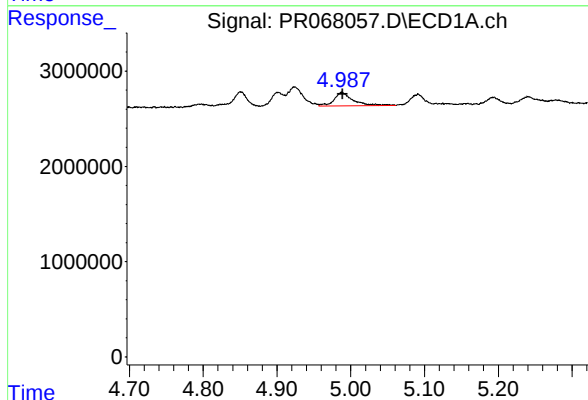


#18 AR-1242-3

R.T.: 4.988 min
Delta R.T.: -0.002 min
Response: 2584830
Conc: 41.18 ng/ml

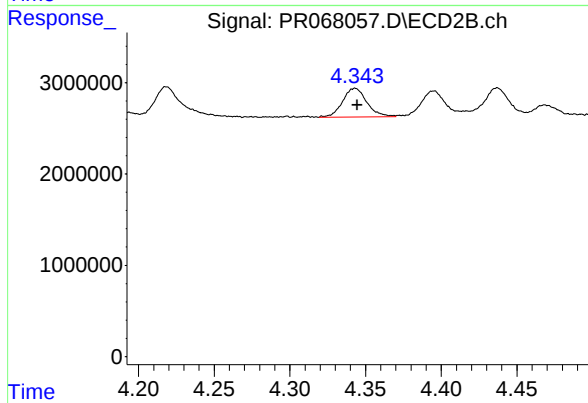

#18 AR-1242-3


R.T.: 4.343 min
Delta R.T.: -0.002 min
Response: 3539828
Conc: 33.32 ng/ml

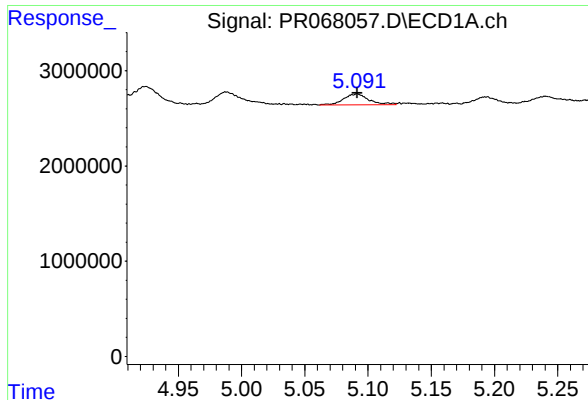

#19 AR-1242-4


R.T.: 5.091 min
Delta R.T.: 0.000 min
Response: 1576818
Conc: 31.59 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

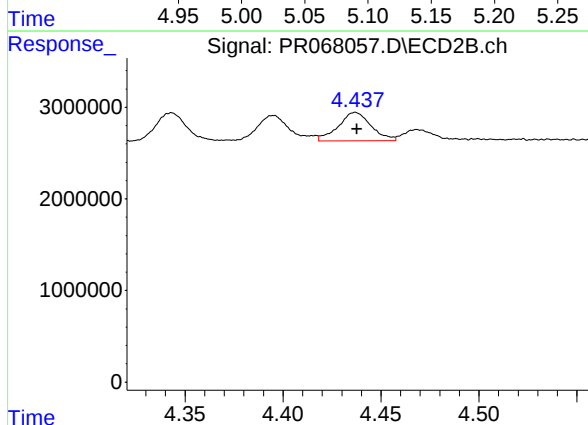


#19 AR-1242-4

R.T.: 4.437 min
Delta R.T.: 0.000 min
Response: 3597401
Conc: 35.77 ng/ml

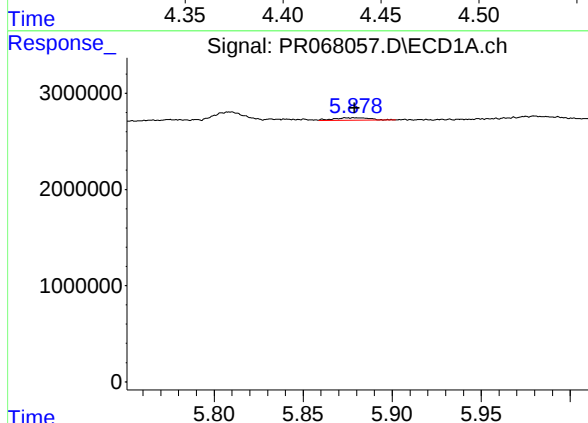


#20 AR-1242-5

R.T.: 5.879 min
Delta R.T.: 0.000 min
Response: 387111
Conc: 8.42 ng/ml

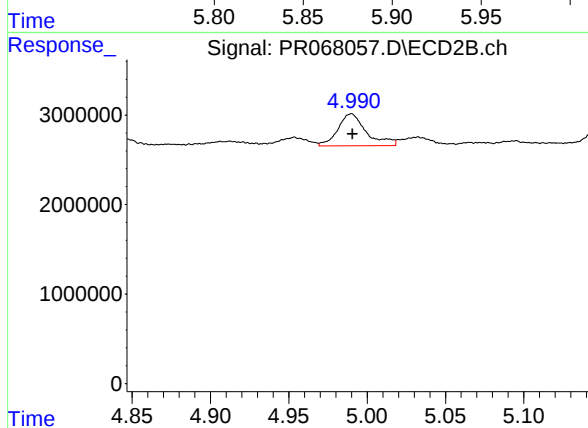

#20 AR-1242-5


R.T.: 4.990 min
Delta R.T.: 0.000 min
Response: 4534281
Conc: 28.91 ng/ml

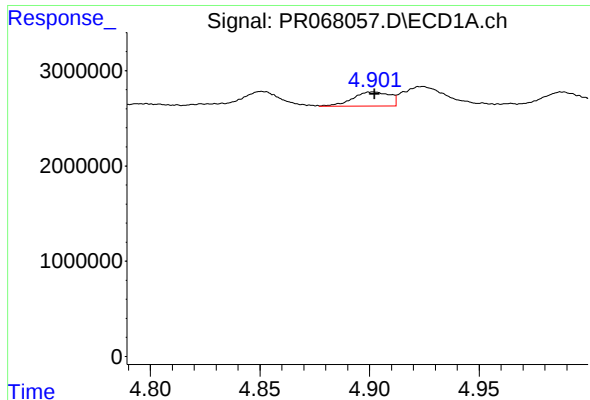

#21 AR-1248-1


R.T.: 4.902 min
Delta R.T.: 0.000 min
Response: 1768301
Conc: 46.07 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

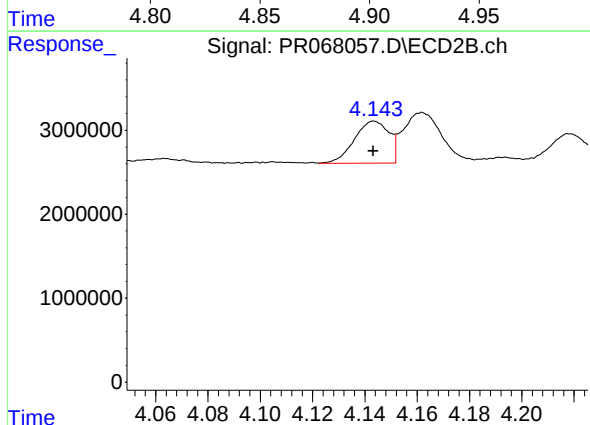


#21 AR-1248-1

R.T.: 4.144 min
Delta R.T.: 0.000 min
Response: 4598729
Conc: 38.65 ng/ml

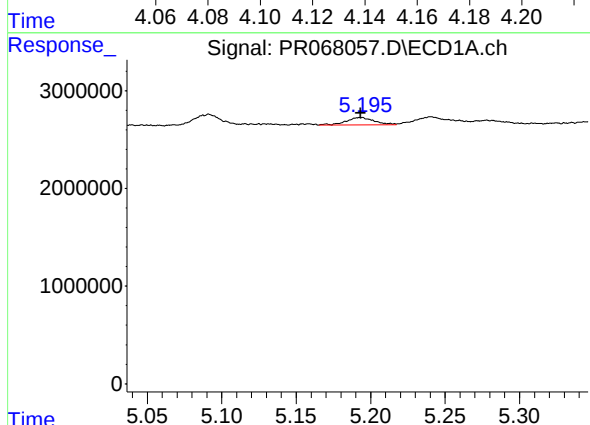


#22 AR-1248-2

R.T.: 5.193 min
Delta R.T.: 0.000 min
Response: 975327
Conc: 18.59 ng/ml

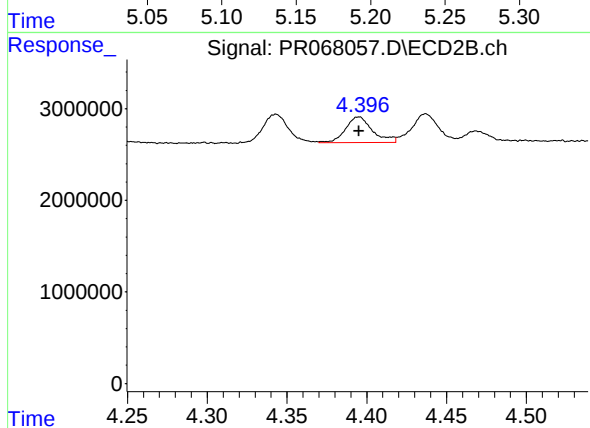

#22 AR-1248-2


R.T.: 4.395 min
Delta R.T.: 0.000 min
Response: 3327015
Conc: 17.65 ng/ml

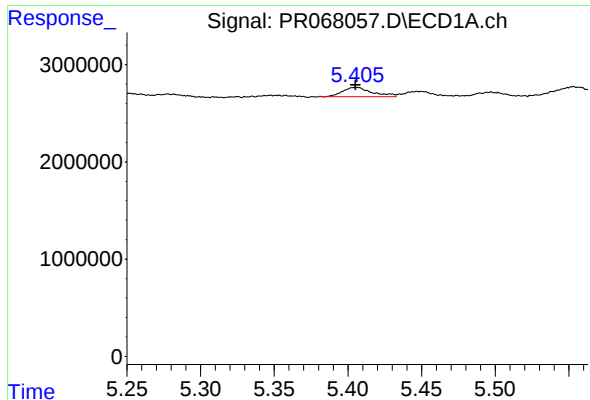

#23 AR-1248-3


R.T.: 5.406 min
Delta R.T.: 0.000 min
Response: 1306505
Conc: 18.56 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

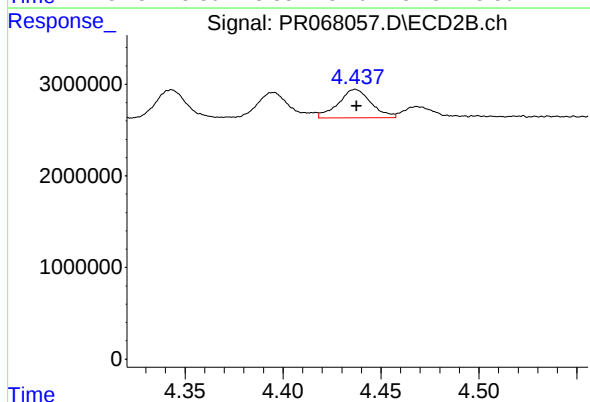


#23 AR-1248-3

R.T.: 4.437 min
Delta R.T.: 0.000 min
Response: 3597401
Conc: 18.87 ng/ml

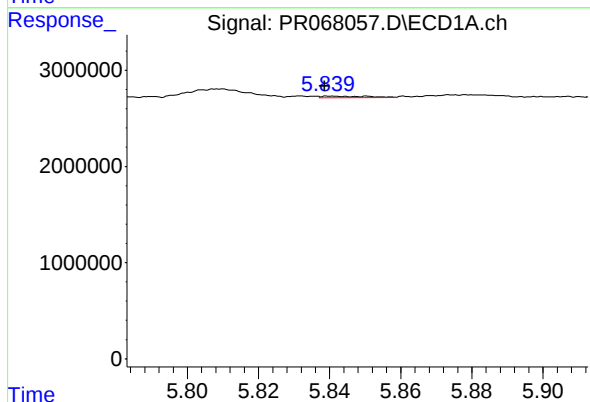


#24 AR-1248-4

R.T.: 5.840 min
Delta R.T.: 0.001 min
Response: 162278
Conc: 2.18 ng/ml

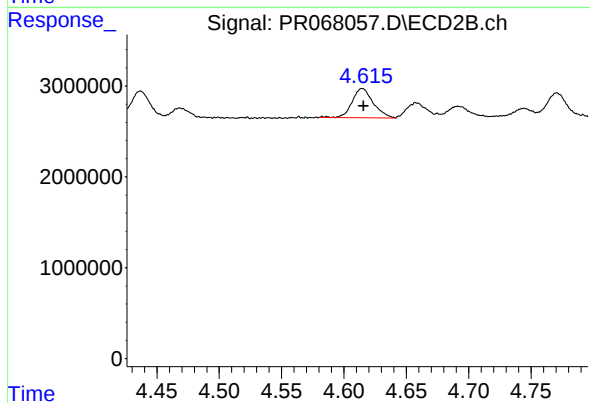

#24 AR-1248-4


R.T.: 4.615 min
Delta R.T.: -0.001 min
Response: 3727658
Conc: 17.26 ng/ml

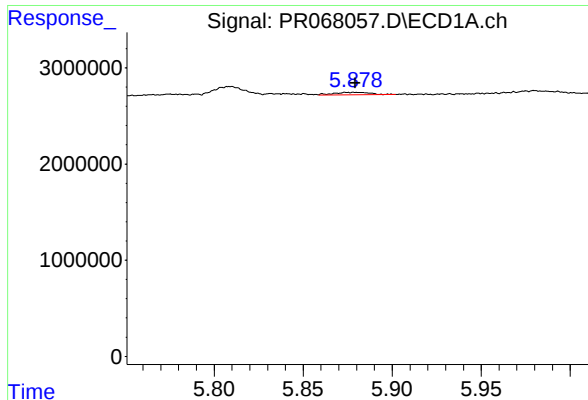

#25 AR-1248-5


R.T.: 5.879 min
Delta R.T.: 0.000 min
Response: 387111
Conc: 4.80 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

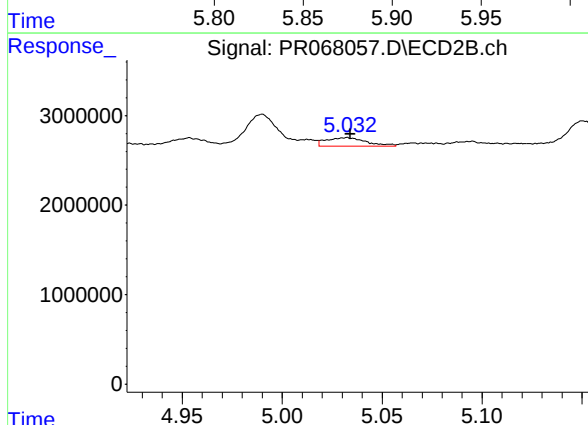


#25 AR-1248-5

R.T.: 5.032 min
Delta R.T.: -0.002 min
Response: 1371318
Conc: 6.45 ng/ml

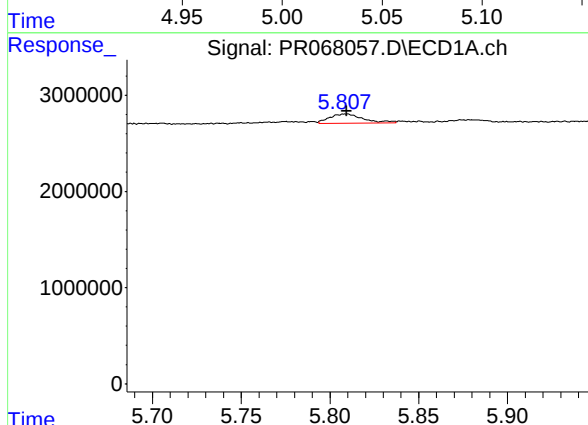


#26 AR-1254-1

R.T.: 5.809 min
Delta R.T.: 0.000 min
Response: 1285426
Conc: 18.01 ng/ml

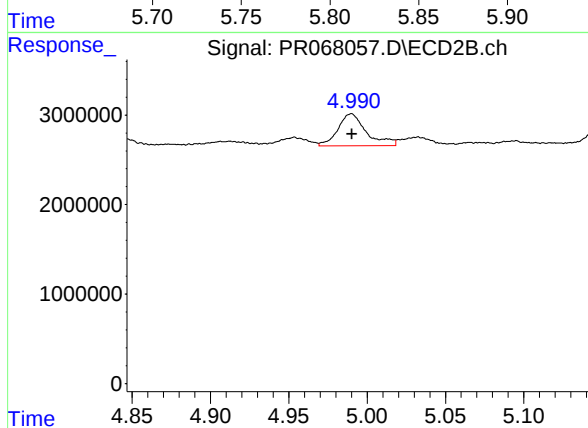

#26 AR-1254-1


R.T.: 4.990 min
Delta R.T.: 0.000 min
Response: 4534281
Conc: 17.73 ng/ml

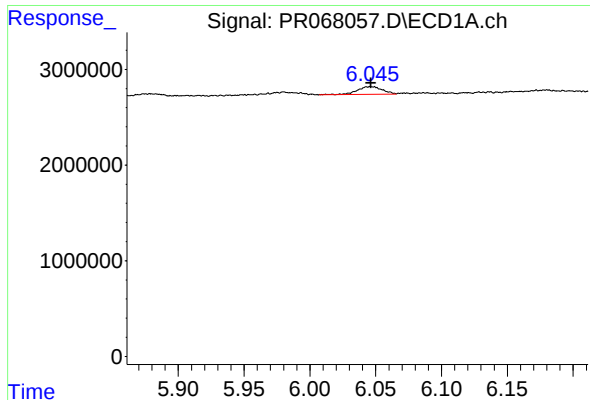

#27 AR-1254-2


R.T.: 6.046 min
Delta R.T.: 0.000 min
Response: 1085112
Conc: 9.67 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

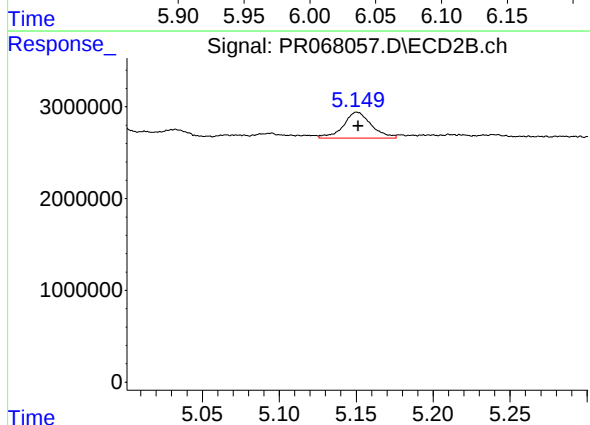


#27 AR-1254-2

R.T.: 5.151 min
Delta R.T.: 0.000 min
Response: 3554998
Conc: 15.47 ng/ml

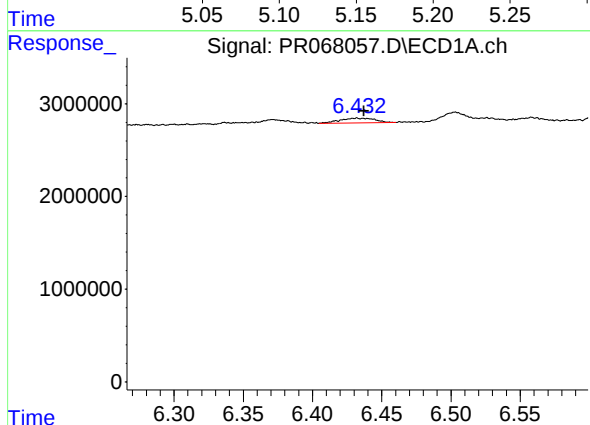


#28 AR-1254-3

R.T.: 6.432 min
Delta R.T.: -0.006 min
Response: 909319
Conc: 6.77 ng/ml

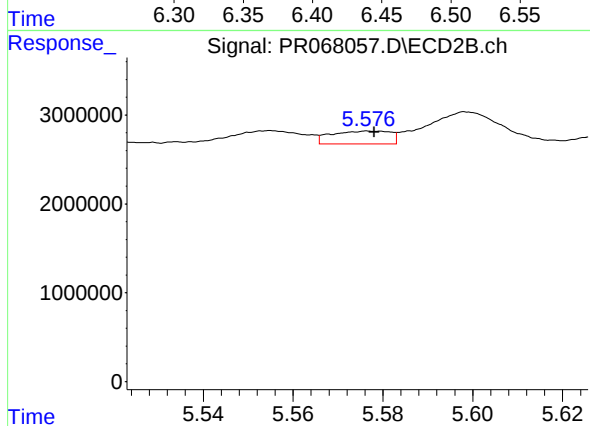

#28 AR-1254-3


R.T.: 5.578 min
Delta R.T.: 0.000 min
Response: 1331779
Conc: 3.69 ng/ml

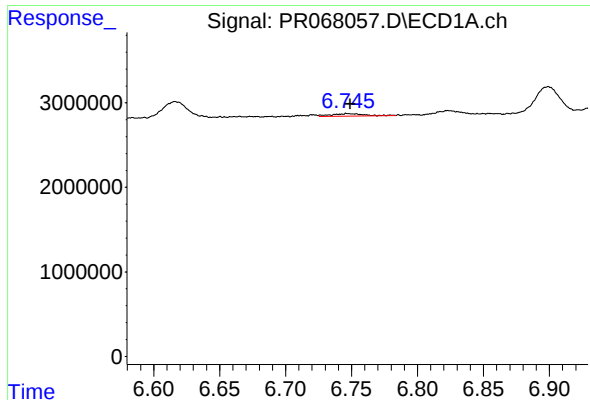

#29 AR-1254-4


R.T.: 6.747 min
Delta R.T.: -0.002 min
Response: 489018
Conc: 4.68 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

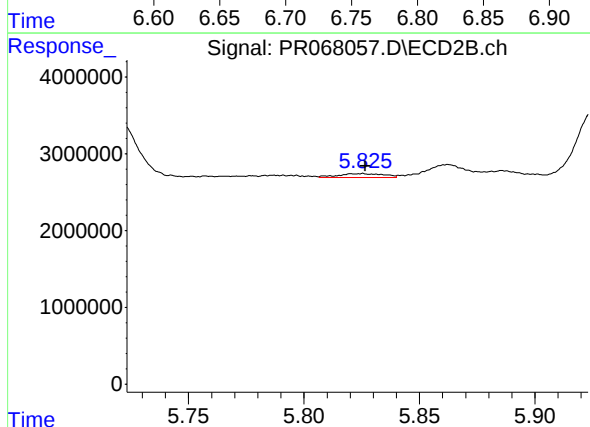


#29 AR-1254-4

R.T.: 5.825 min
Delta R.T.: 0.000 min
Response: 702785
Conc: 3.27 ng/ml

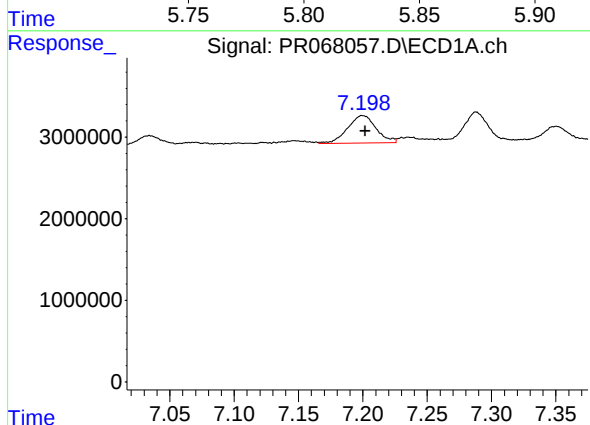


#30 AR-1254-5

R.T.: 7.200 min
Delta R.T.: -0.002 min
Response: 5159165
Conc: 41.53 ng/ml

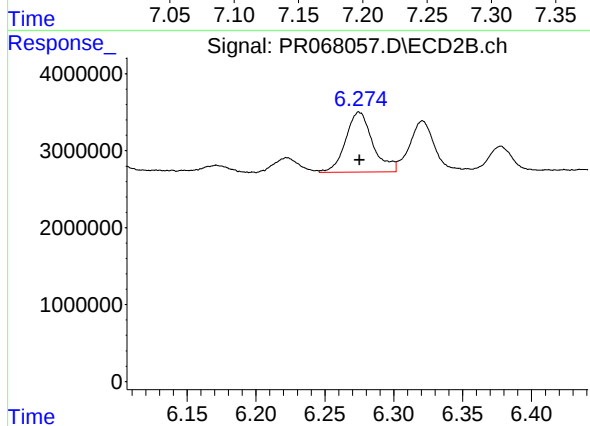

#30 AR-1254-5


R.T.: 6.275 min
Delta R.T.: 0.000 min
Response: 10695502
Conc: 32.40 ng/ml

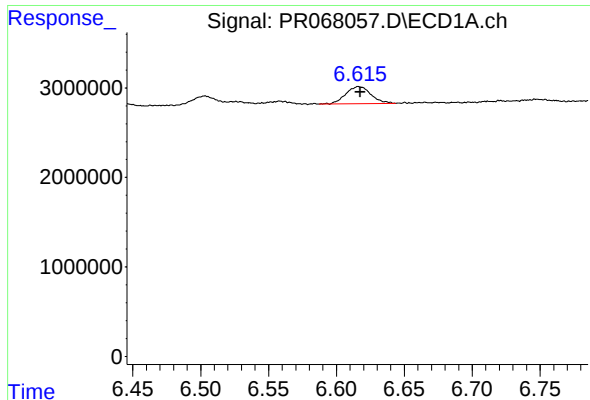

#31 AR-1260-1


R.T.: 6.616 min
Delta R.T.: -0.001 min
Response: 2476099
Conc: 26.79 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

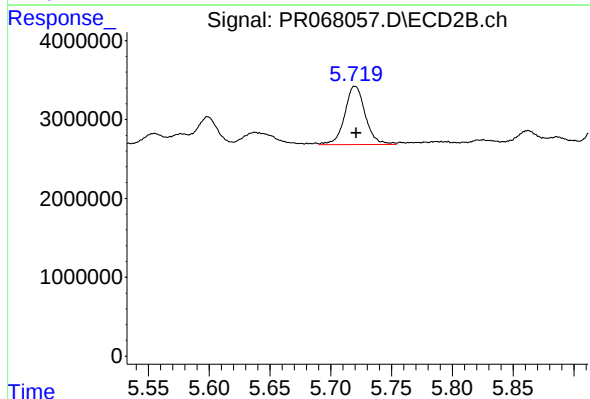


#31 AR-1260-1

R.T.: 5.720 min
Delta R.T.: 0.000 min
Response: 8629373
Conc: 35.25 ng/ml

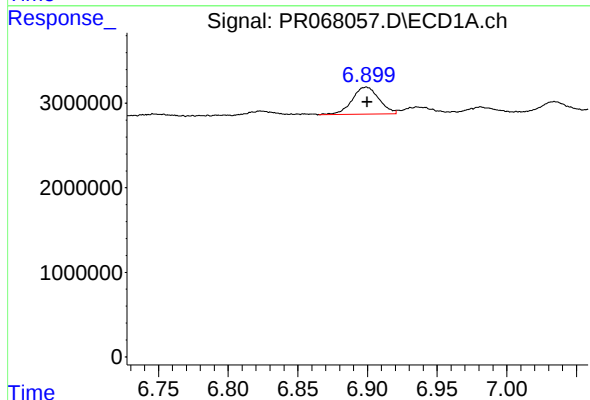


#32 AR-1260-2

R.T.: 6.899 min
Delta R.T.: 0.000 min
Response: 4285419
Conc: 30.15 ng/ml

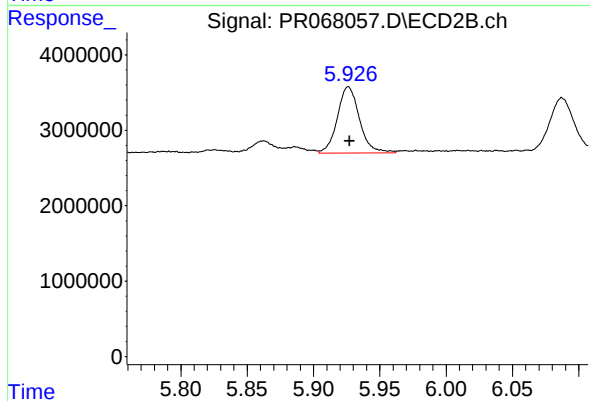

#32 AR-1260-2


R.T.: 5.926 min
Delta R.T.: 0.000 min
Response: 10236825
Conc: 35.26 ng/ml

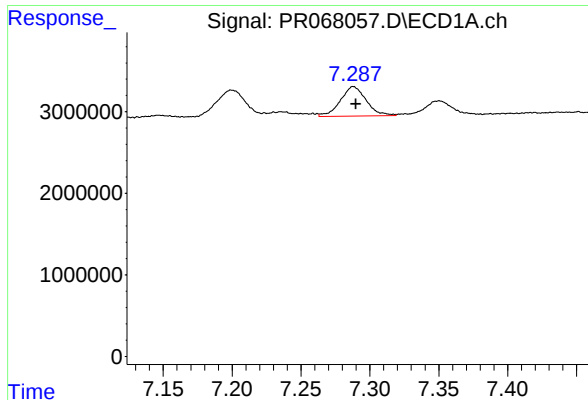

#33 AR-1260-3


R.T.: 7.288 min
Delta R.T.: -0.002 min
Response: 4709327
Conc: 34.01 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

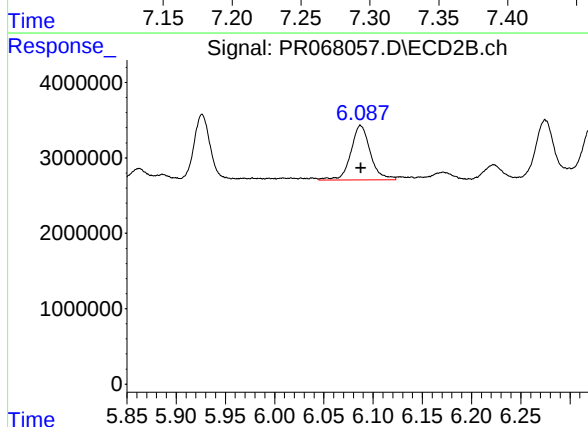


#33 AR-1260-3

R.T.: 6.087 min
Delta R.T.: 0.000 min
Response: 9957333
Conc: 36.26 ng/ml

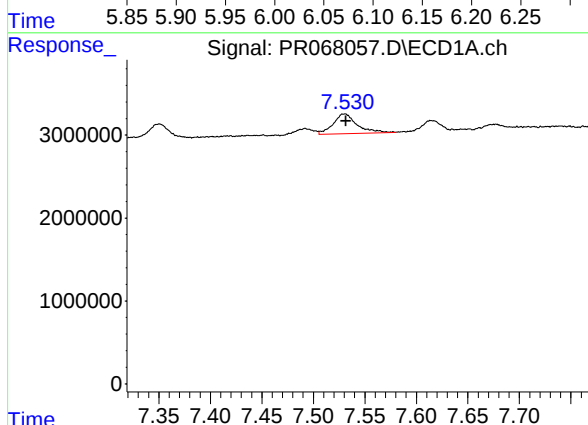


#34 AR-1260-4

R.T.: 7.530 min
Delta R.T.: -0.002 min
Response: 3841771
Conc: 30.31 ng/ml

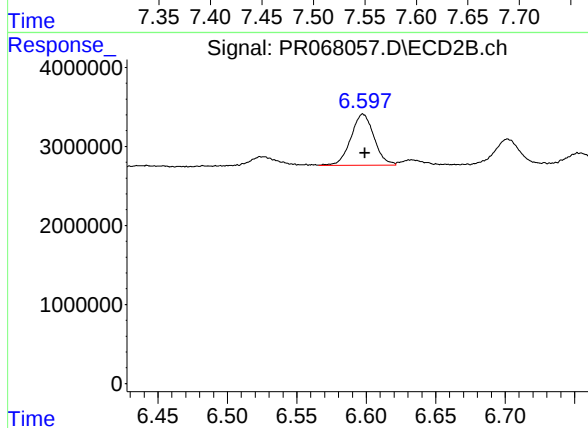

#34 AR-1260-4


R.T.: 6.598 min
Delta R.T.: -0.001 min
Response: 7523769
Conc: 35.88 ng/ml

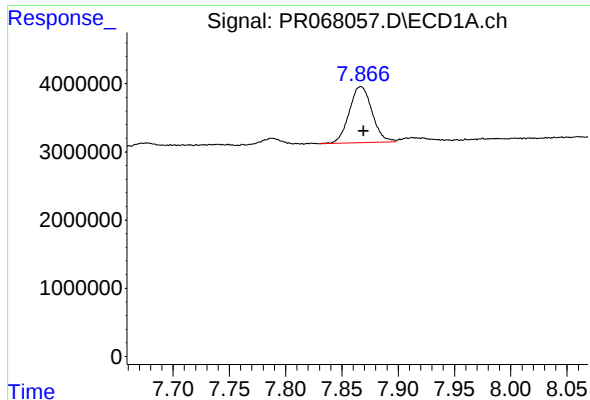

#35 AR-1260-5


R.T.: 7.867 min
Delta R.T.: -0.002 min
Response: 11602223
Conc: 31.83 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

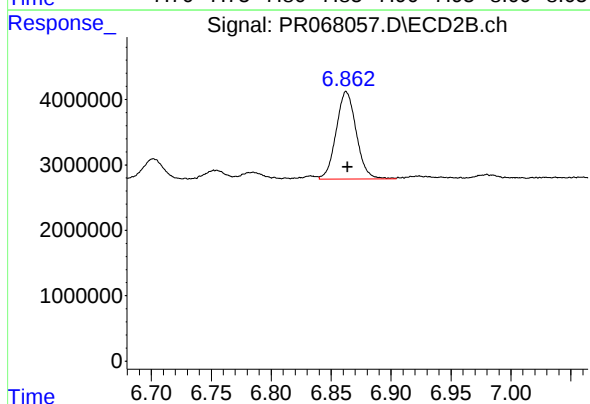


#35 AR-1260-5

R.T.: 6.863 min
Delta R.T.: -0.001 min
Response: 15642033
Conc: 32.32 ng/ml

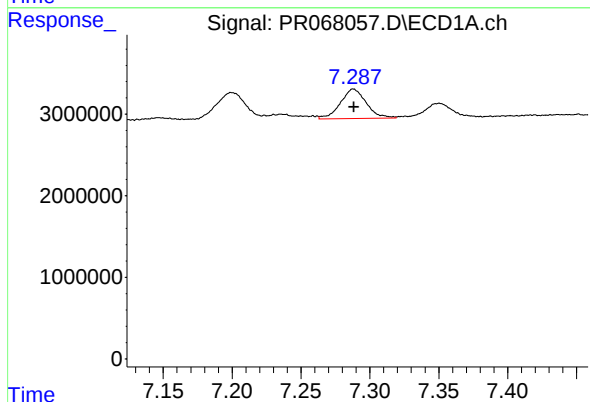


#36 AR-1262-1

R.T.: 7.288 min
Delta R.T.: 0.000 min
Response: 4709327
Conc: 23.64 ng/ml

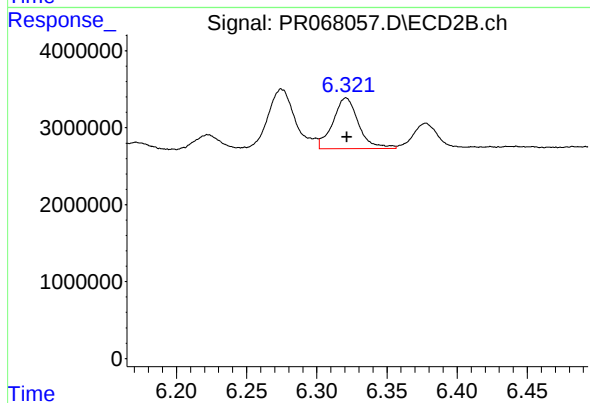

#36 AR-1262-1


R.T.: 6.321 min
Delta R.T.: 0.000 min
Response: 8447157
Conc: 24.45 ng/ml

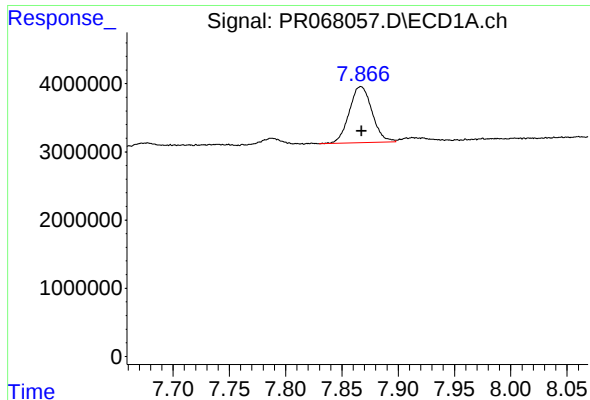

#37 AR-1262-2


R.T.: 7.867 min
Delta R.T.: 0.000 min
Response: 11602223
Conc: 26.79 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

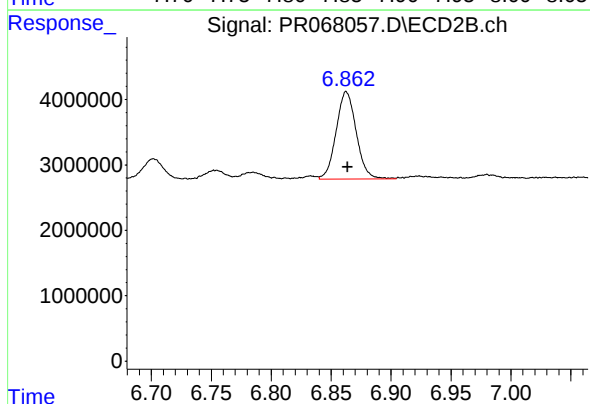


#37 AR-1262-2

R.T.: 6.863 min
Delta R.T.: 0.000 min
Response: 15642033
Conc: 25.72 ng/ml

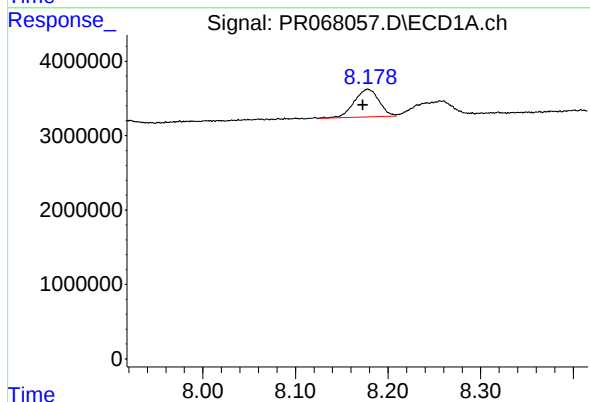


#38 AR-1262-3

R.T.: 8.178 min
Delta R.T.: 0.005 min
Response: 6927622
Conc: 22.12 ng/ml

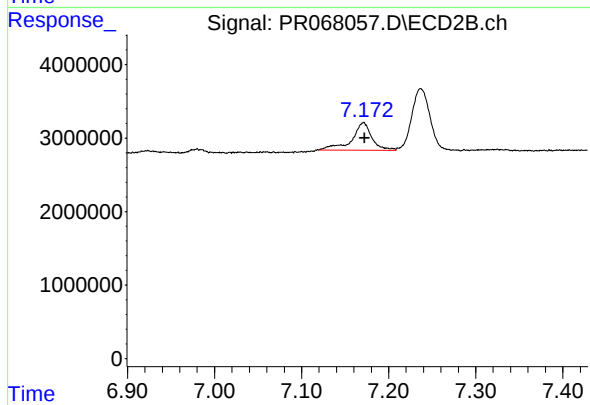

#38 AR-1262-3


R.T.: 7.171 min
Delta R.T.: -0.001 min
Response: 6022180
Conc: 25.22 ng/ml

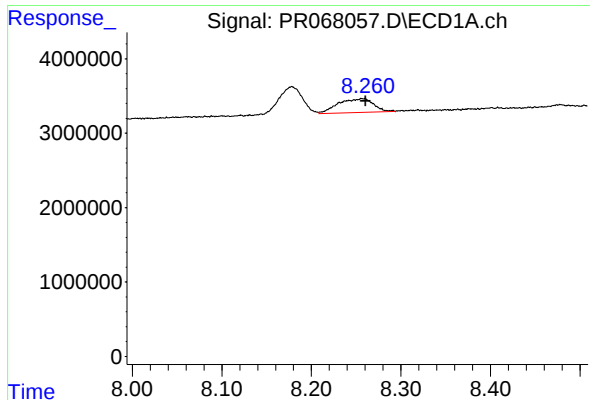

#39 AR-1262-4


R.T.: 8.258 min
Delta R.T.: -0.003 min
Response: 5139813
Conc: 18.72 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

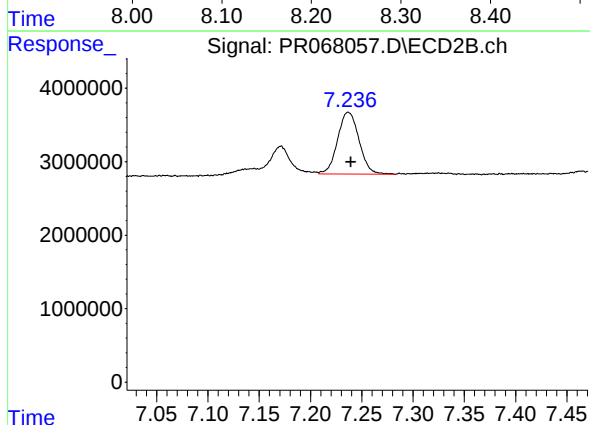


#39 AR-1262-4

R.T.: 7.237 min
Delta R.T.: -0.003 min
Response: 12300917
Conc: 27.68 ng/ml

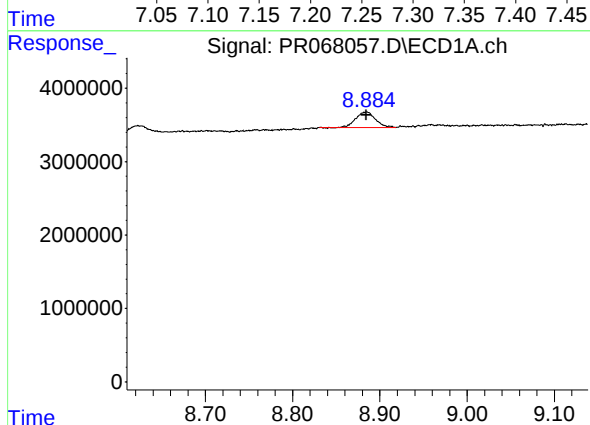


#40 AR-1262-5

R.T.: 8.885 min
Delta R.T.: 0.000 min
Response: 3297554
Conc: 17.42 ng/ml

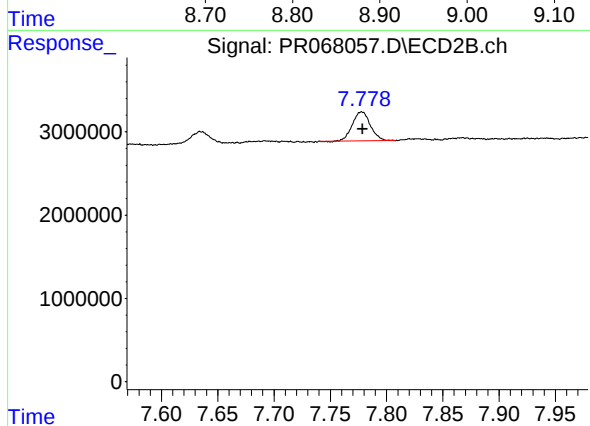

#40 AR-1262-5


R.T.: 7.778 min
Delta R.T.: 0.000 min
Response: 3846471
Conc: 18.88 ng/ml

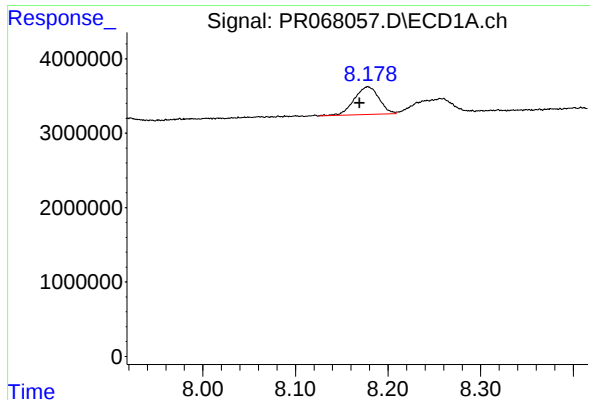

#41 AR-1268-1


R.T.: 8.178 min
Delta R.T.: 0.009 min
Response: 6927622
Conc: 11.49 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

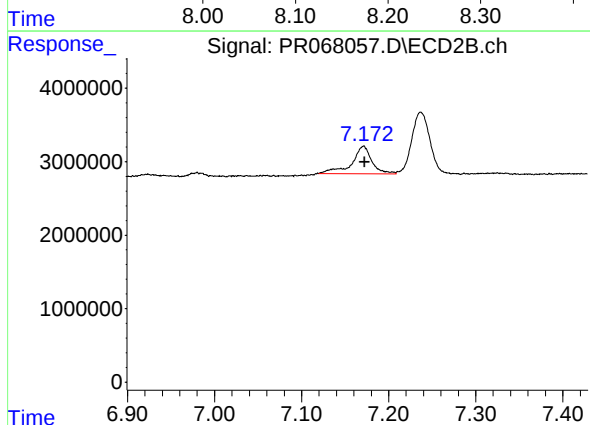


#41 AR-1268-1

R.T.: 7.171 min
Delta R.T.: -0.001 min
Response: 6022180
Conc: 8.16 ng/ml

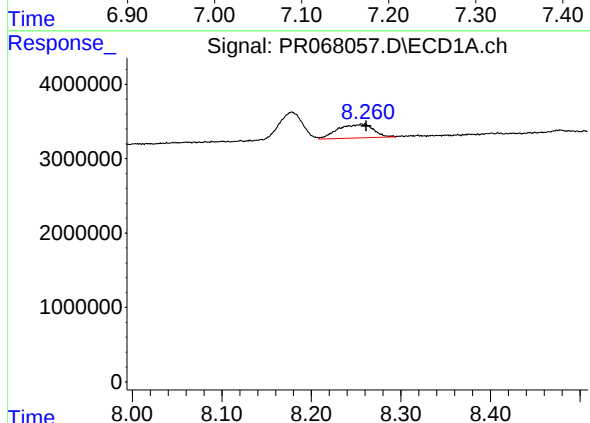


#42 AR-1268-2

R.T.: 8.258 min
Delta R.T.: -0.004 min
Response: 5139813
Conc: 9.02 ng/ml

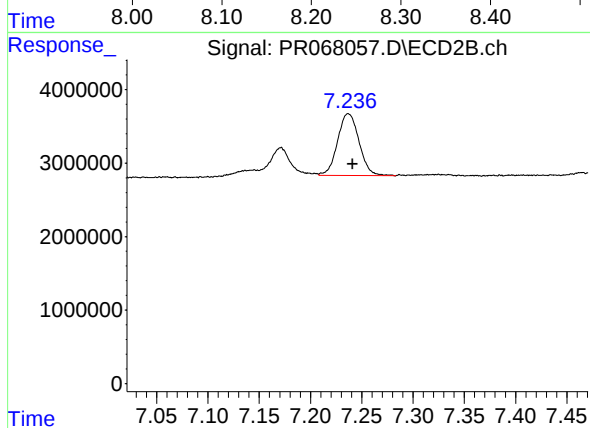

#42 AR-1268-2


R.T.: 7.237 min
Delta R.T.: -0.004 min
Response: 12300917
Conc: 18.22 ng/ml

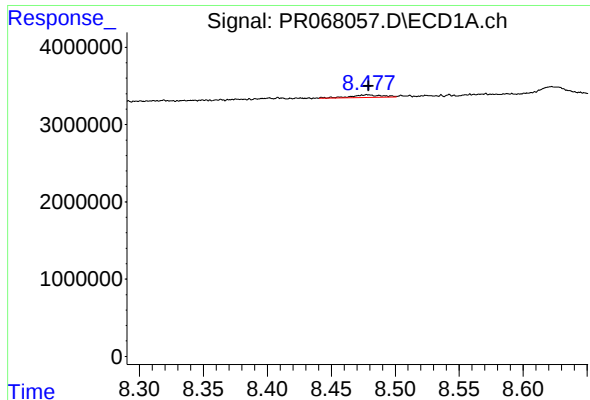

#43 AR-1268-3


R.T.: 8.479 min
Delta R.T.: 0.000 min
Response: 557059
Conc: 1.00 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

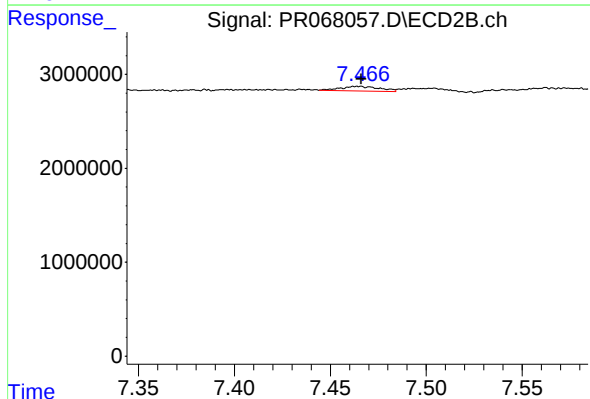


#43 AR-1268-3

R.T.: 7.464 min
Delta R.T.: -0.002 min
Response: 700402
Conc: 1.14 ng/ml

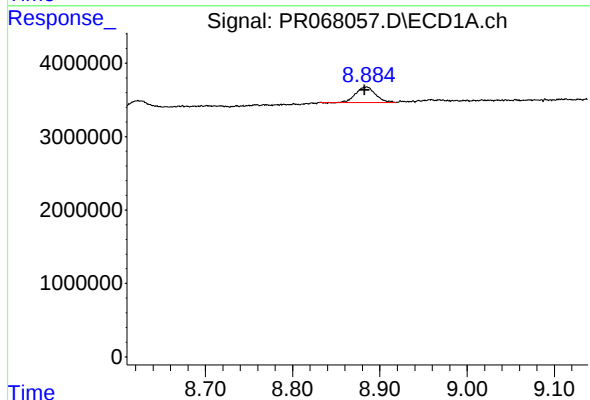


#44 AR-1268-4

R.T.: 8.885 min
Delta R.T.: 0.003 min
Response: 3297554
Conc: 16.28 ng/ml

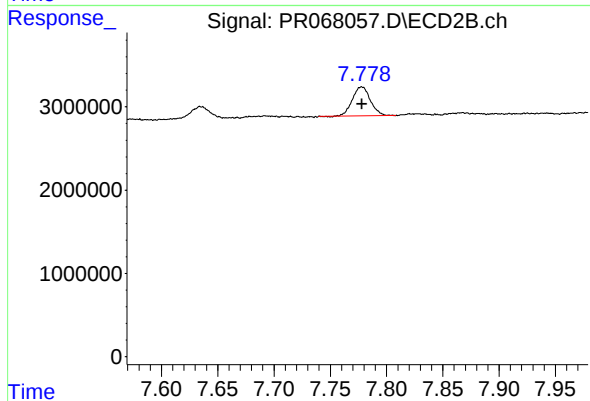

#44 AR-1268-4


R.T.: 7.778 min
Delta R.T.: 0.000 min
Response: 3846471
Conc: 18.45 ng/ml

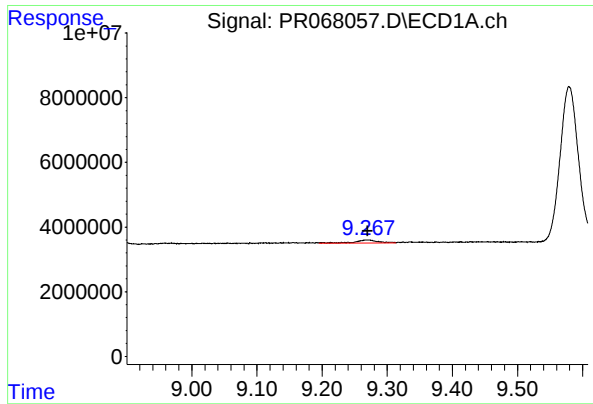

#45 AR-1268-5

R.T.: 9.270 min
Delta R.T.: 0.000 min
Response: 2229119
Conc: 1.43 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

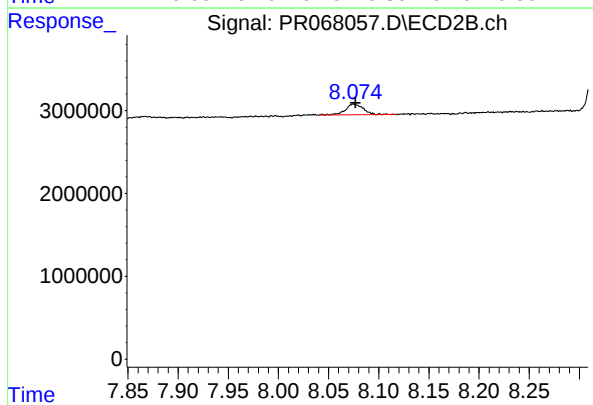

#45 AR-1268-5

R.T.: 8.076 min
Delta R.T.: -0.001 min
Response: 1665251
Conc: 1.17 ng/ml