

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR080624\
 Data File : PR068014.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2024 12:46
 Operator : AJ\MA
 Sample : PB162510BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 PB162510BL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/07/2024
 Supervised By :Ankita Jodhani 08/07/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 07 02:51:19 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 07 00:26:28 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.677	3.012	49767470	94482479	19.563m	21.667
2) SA Decachlor...	9.583	8.337	90531650	102.0E6	20.632	22.502

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR080624\
Data File : PR068014.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2024 12:46
Operator : AJ\MA
Sample : PB162510BL
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
PB162510BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/07/2024
Supervised By :Ankita Jodhani 08/07/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 02:51:19 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 07 00:26:28 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

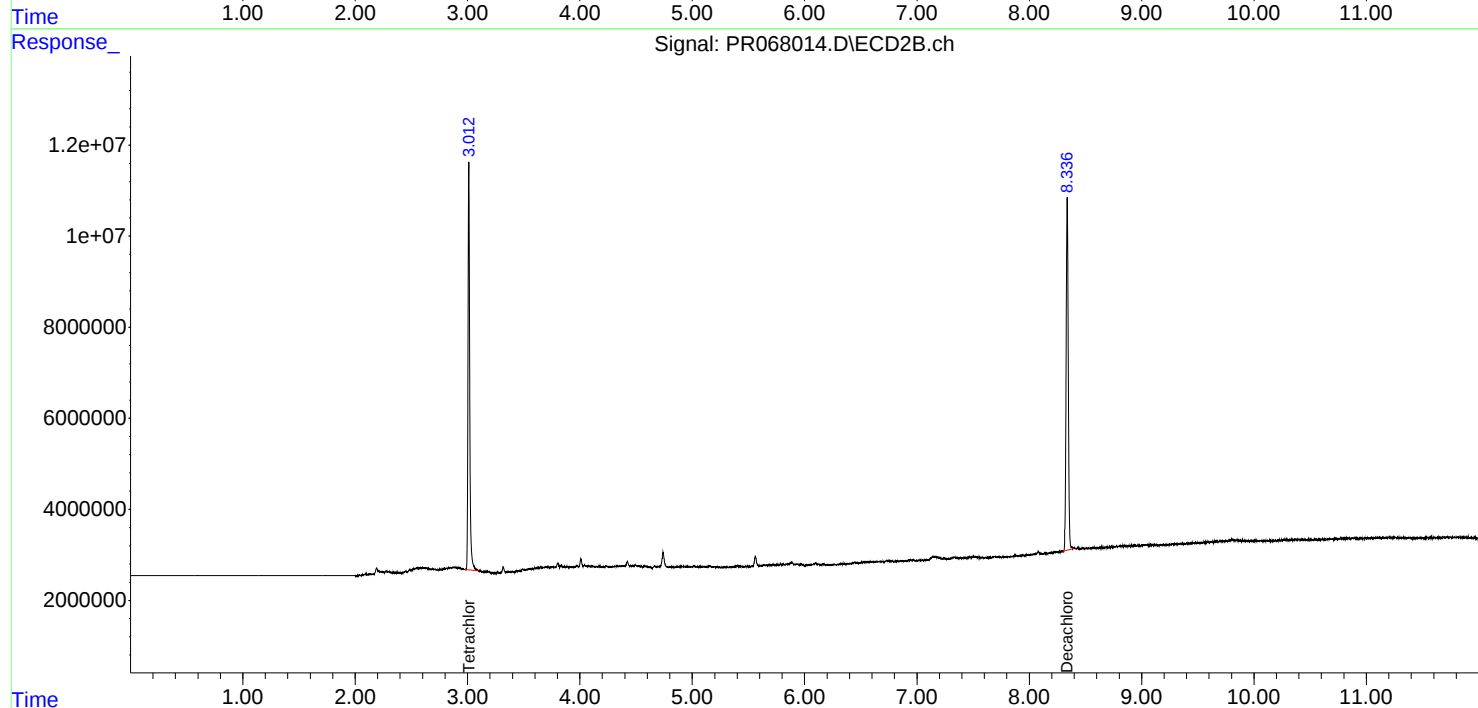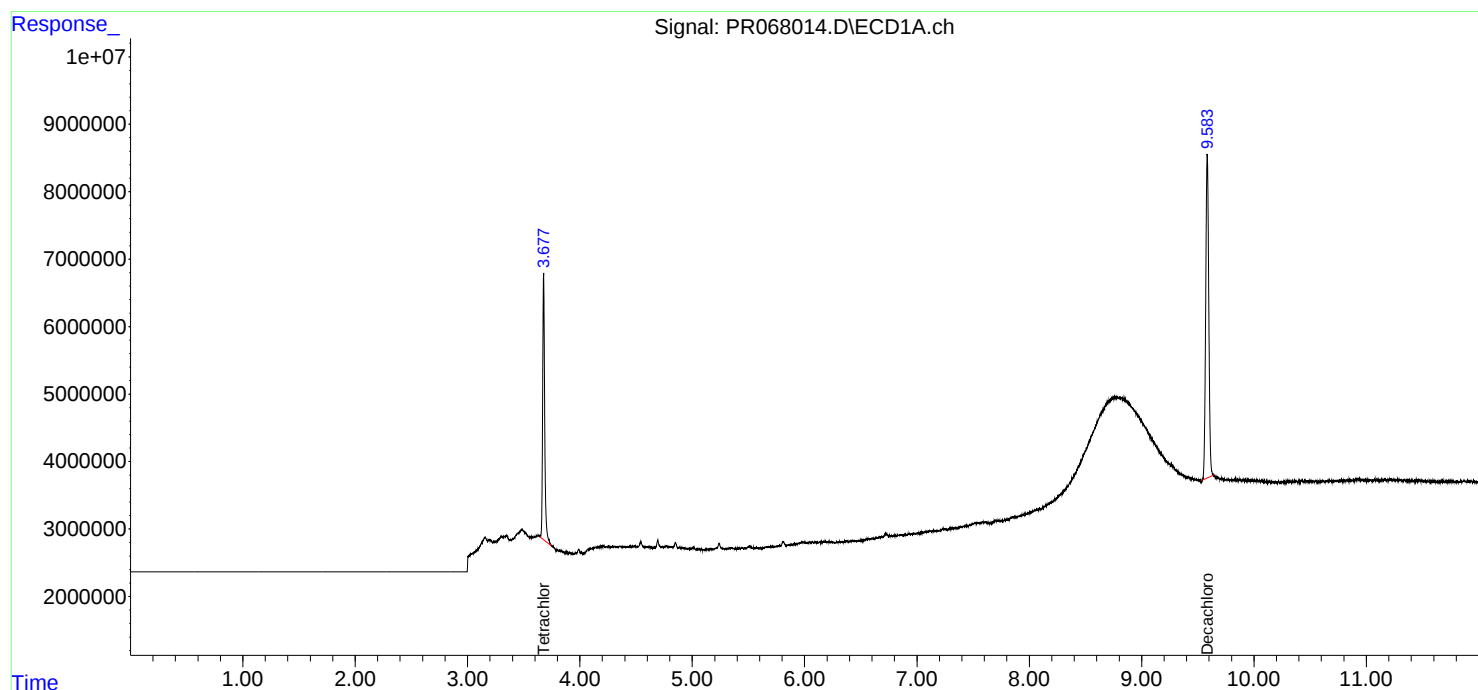

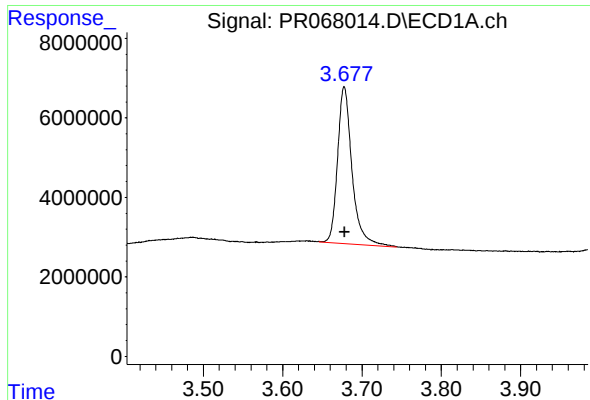


#1 Tetrachloro-m-xylene

R.T.: 3.677 min
Delta R.T.: 0.000 min
Response: 49767470
Conc: 19.56 ng/ml

Instrument :
ECD_R
ClientSampleId :
PB162510BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/07/2024
Supervised By :Ankita Jodhani 08/07/2024

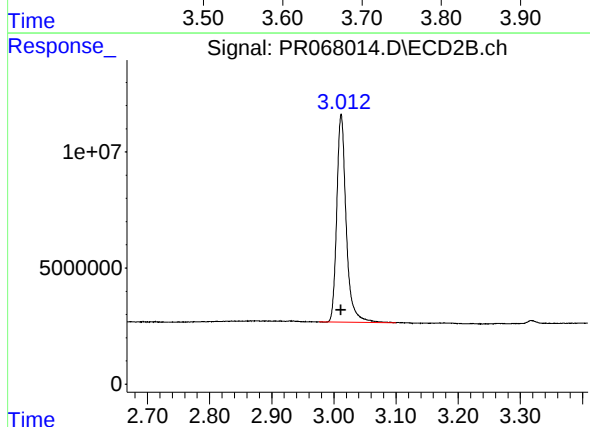


#1 Tetrachloro-m-xylene

R.T.: 3.012 min
Delta R.T.: 0.000 min
Response: 94482479
Conc: 21.67 ng/ml

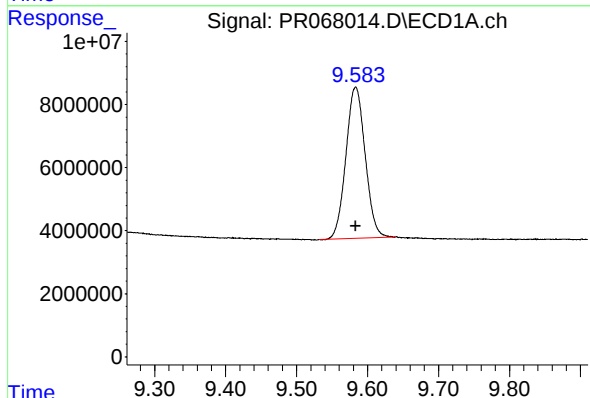

#2 Decachlorobiphenyl

R.T.: 9.583 min
Delta R.T.: 0.000 min
Response: 90531650
Conc: 20.63 ng/ml

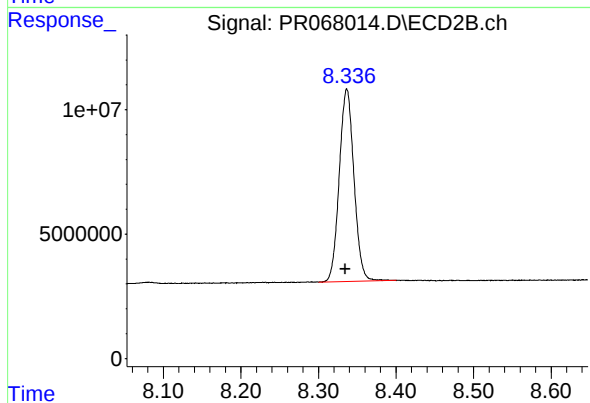

#2 Decachlorobiphenyl

R.T.: 8.337 min
Delta R.T.: 0.002 min
Response: 101959577
Conc: 22.50 ng/ml