

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR080724\
 Data File : PR068071.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Aug 2024 10:51
 Operator : AJ\MA
 Sample : P3390-09
 Misc : AR1221 MDL 25 PPB
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 07 17:08:26 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 07 00:26:28 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.677	3.011	37179423	72238634	14.615	16.566
2)	SA Decachlor...	9.580	8.331	69111781	77519650	15.750	17.109
Target Compounds							
3)	L1 AR-1016-1	4.923f	4.162f	310692	815162	5.316	5.424
4)	L1 AR-1016-2	4.923	4.162	310692	815162	2.802	3.885 #
5)	L1 AR-1016-3	5.012f	4.339	670841	248676	8.735	2.180 #
6)	L1 AR-1016-4	5.062f	4.414f	182323	232470	2.912	2.431
7)	L1 AR-1016-5	5.413	4.614	320978	333034	6.392	2.786 #
8)	L2 AR-1221-1	3.896	3.238	955204	1303564	34.753	8.387 #
9)	L2 AR-1221-2	3.989	3.320	1096891	1946660	48.813	26.505 #
10)	L2 AR-1221-3	4.068	3.402	1314174	2874710	18.395	8.873 #
11)	L3 AR-1232-1	4.068	3.402	1314174	2874710	22.331	28.381 #
12)	L3 AR-1232-2	4.608	4.162	279787	815162	8.908	8.090
13)	L3 AR-1232-3	4.923	4.339	310692	248676	5.763	4.579
14)	L3 AR-1232-4	5.062f	4.414f	182323	232470	6.098	4.652
15)	L3 AR-1232-5	5.194	4.614	408464	333034	26.521	6.263 #
16)	L4 AR-1242-1	4.923f	4.162f	310692	815162	6.351	5.347
17)	L4 AR-1242-2	4.923	4.162	310692	815162	3.420	3.812
18)	L4 AR-1242-3	5.012f	4.339	670841	248676	10.689	2.341 #
19)	L4 AR-1242-4	0.000	4.414f	0	232470	N.D.	2.312 #
20)	L4 AR-1242-5	5.885	4.993	32099	659412	0.698	4.205 #
21)	L5 AR-1248-1	4.923f	4.162f	310692	815162	8.095	6.850
22)	L5 AR-1248-2	5.194	4.414f	408464	232470	7.787	1.233 #
23)	L5 AR-1248-3	5.413	4.414f	320978	232470	4.559	1.220 #
24)	L5 AR-1248-4	5.859f	4.614	44681	333034	0.601	1.542 #
25)	L5 AR-1248-5	5.885	5.016f	32099	1051805	0.398	4.950 #
26)	L6 AR-1254-1	5.809	4.993	469655	659412	6.581	2.578 #
27)	L6 AR-1254-2	0.000	5.151	0	651069	N.D.	2.832 #
28)	L6 AR-1254-3	6.425	5.558f	1249005	3212603	9.295	8.904
29)	L6 AR-1254-4	6.724f	0.000	351791	0	3.366	N.D. #
30)	L6 AR-1254-5	0.000	6.274	0	306690	N.D.	0.929 #
31)	L7 AR-1260-1	0.000	5.712	0	484497	N.D.	1.979 #
32)	L7 AR-1260-2	6.895	5.925	902077	302633	6.347	1.042 #
33)	L7 AR-1260-3	0.000	6.093	0	492280	N.D.	1.793 #
34)	L7 AR-1260-4	7.534	6.618f	427464	191950	3.373	0.916 #
36)	L8 AR-1262-1	0.000	6.317	0	217389	N.D.	0.629 #
38)	L8 AR-1262-3	8.165	0.000	58606	0	0.187	N.D. #
39)	L8 AR-1262-4	0.000	7.236	0	304314	N.D.	0.685 #
40)	L8 AR-1262-5	8.864f	0.000	221967	0	1.173	N.D. #
41)	L9 AR-1268-1	8.165	0.000	58606	0	0.097	N.D. #
42)	L9 AR-1268-2	0.000	7.236	0	304314	N.D.	0.451 #
43)	L9 AR-1268-3	8.481	7.466	289219	204121	0.521	0.331 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR080724\
Data File : PR068071.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Aug 2024 10:51
Operator : AJ\MA
Sample : P3390-09
Misc : AR1221 MDL 25 PPB
ALS Vial : 57 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 17:08:26 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 07 00:26:28 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
44)	L9 AR-1268-4	8.864f	0.000	221967	0	1.096	N.D. #
45)	L9 AR-1268-5	9.267	8.074	992391	544213	0.635	0.381 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR080724\
Data File : PR068071.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Aug 2024 10:51
Operator : AJ\MA
Sample : P3390-09
Misc : AR1221 MDL 25 PPB
ALS Vial : 57 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 17:08:26 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 07 00:26:28 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

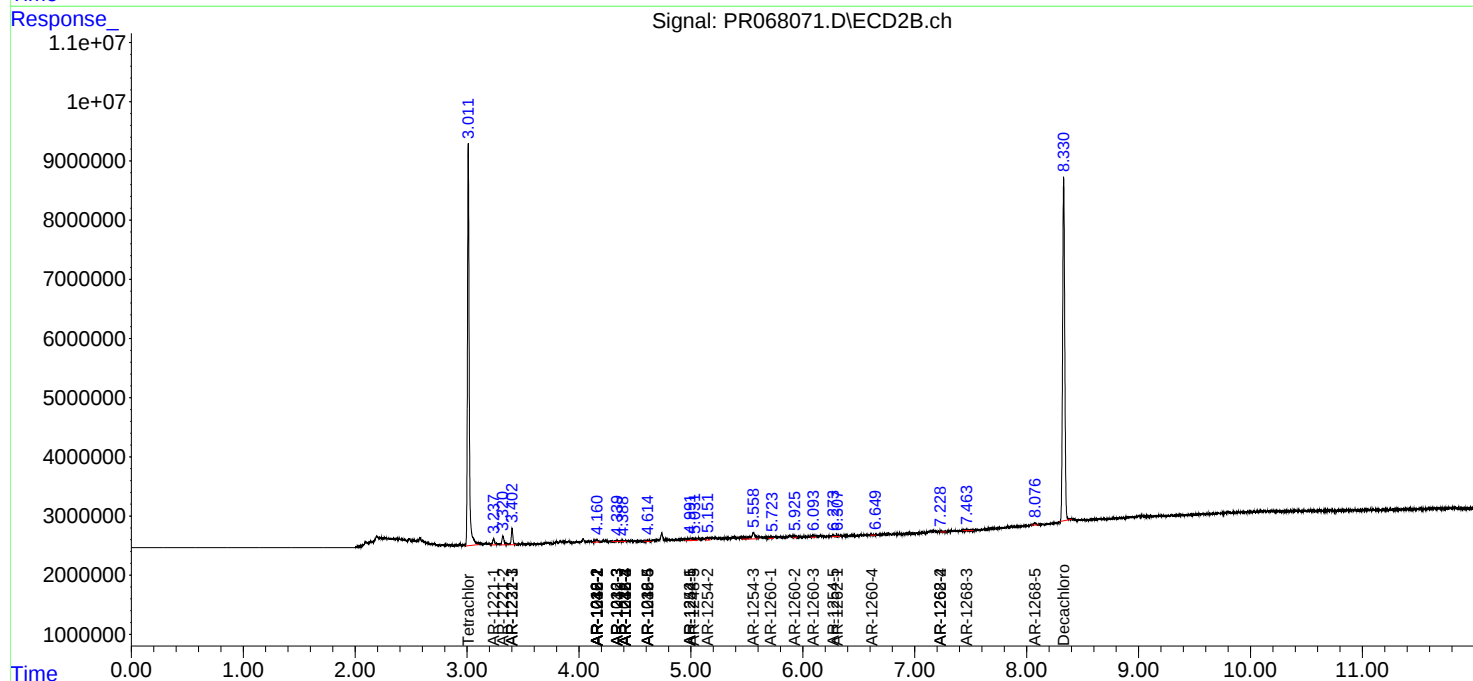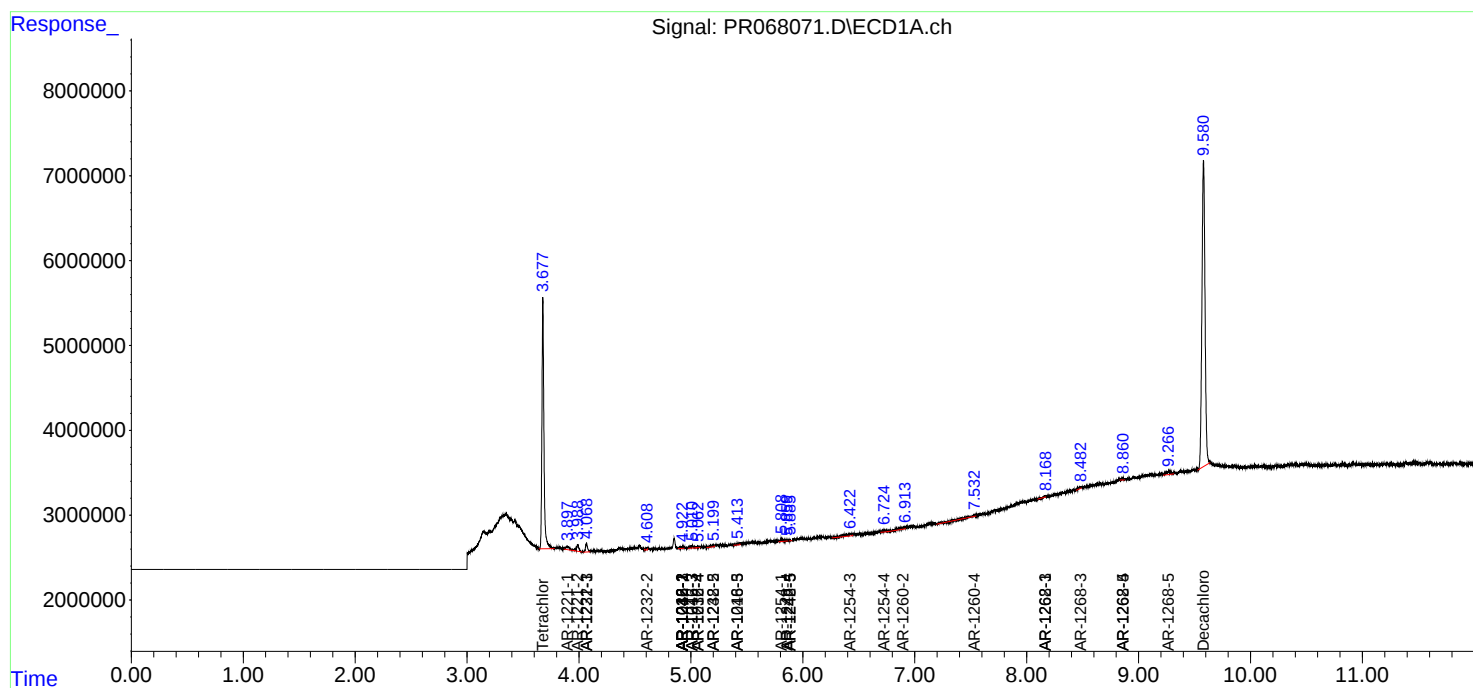


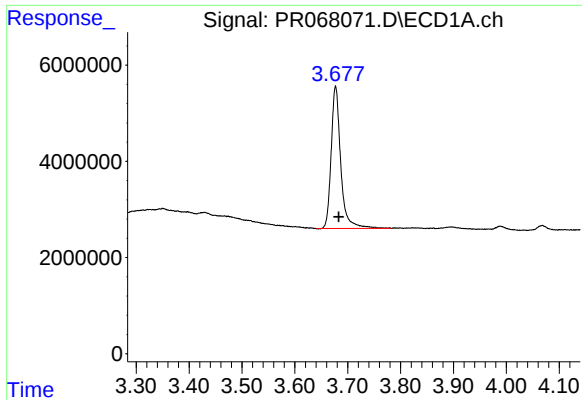

#1 Tetrachloro-m-xylene


R.T.: 3.677 min
Delta R.T.: -0.006 min
Response: 37179423
Conc: 14.62 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

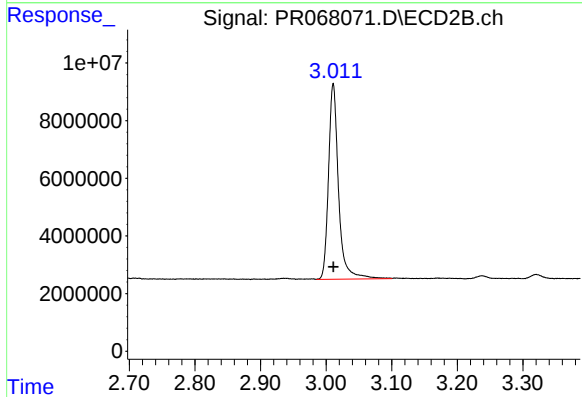


#1 Tetrachloro-m-xylene

R.T.: 3.011 min
Delta R.T.: 0.000 min
Response: 72238634
Conc: 16.57 ng/ml

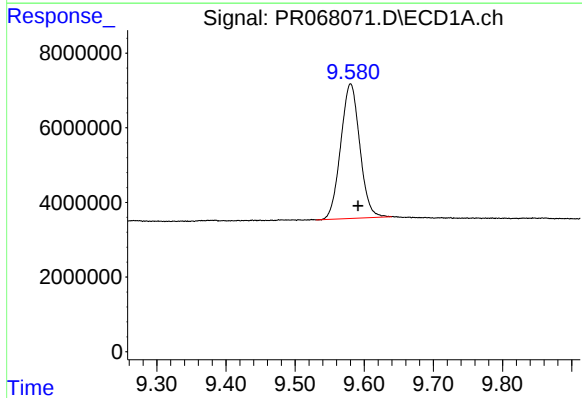


#2 Decachlorobiphenyl

R.T.: 9.580 min
Delta R.T.: -0.011 min
Response: 69111781
Conc: 15.75 ng/ml

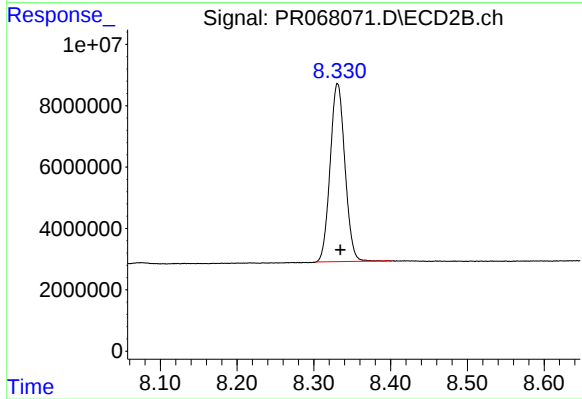

#2 Decachlorobiphenyl


R.T.: 8.331 min
Delta R.T.: -0.004 min
Response: 77519650
Conc: 17.11 ng/ml

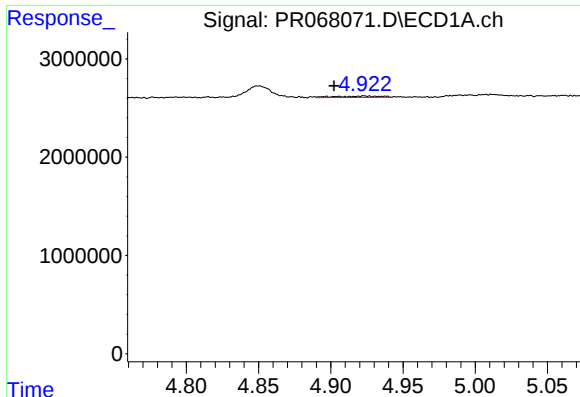

#3 AR-1016-1


R.T.: 4.923 min
Delta R.T.: 0.021 min
Response: 310692
Conc: 5.32 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

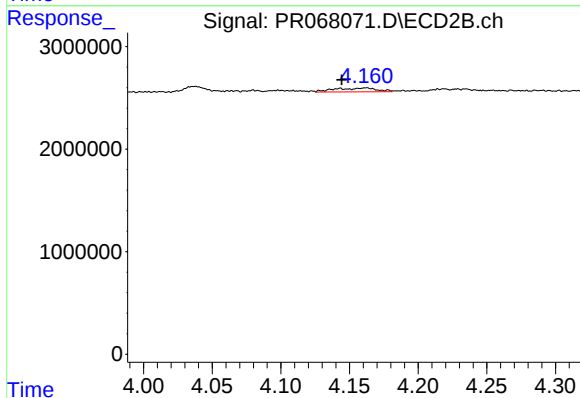


#3 AR-1016-1

R.T.: 4.162 min
Delta R.T.: 0.018 min
Response: 815162
Conc: 5.42 ng/ml

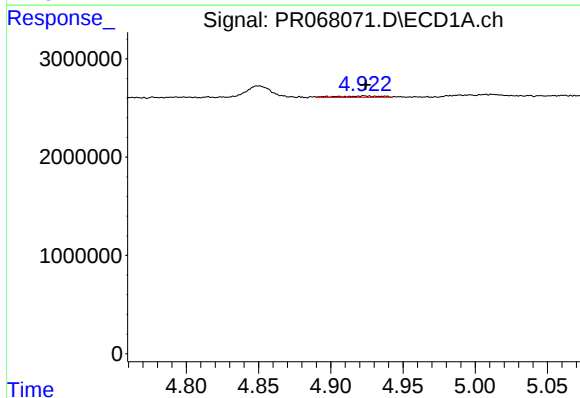


#4 AR-1016-2

R.T.: 4.923 min
Delta R.T.: -0.001 min
Response: 310692
Conc: 2.80 ng/ml

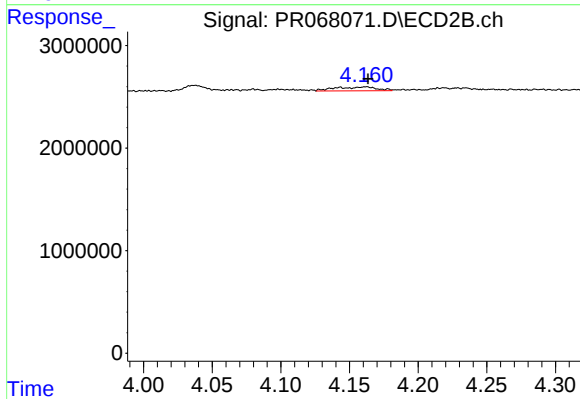

#4 AR-1016-2


R.T.: 4.162 min
Delta R.T.: -0.001 min
Response: 815162
Conc: 3.88 ng/ml

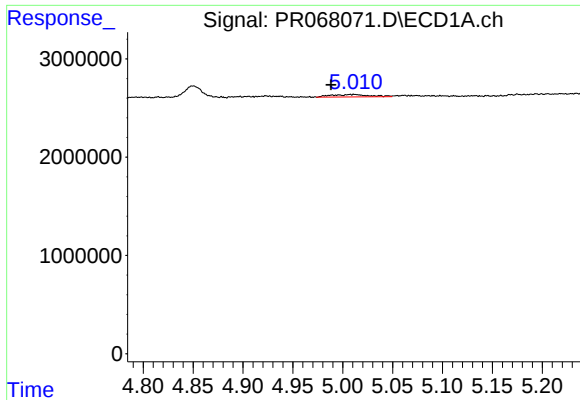

#5 AR-1016-3


R.T.: 5.012 min
Delta R.T.: 0.024 min
Response: 670841
Conc: 8.74 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

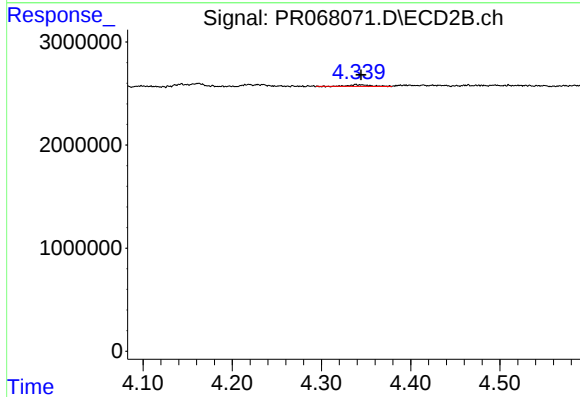


#5 AR-1016-3

R.T.: 4.339 min
Delta R.T.: -0.006 min
Response: 248676
Conc: 2.18 ng/ml

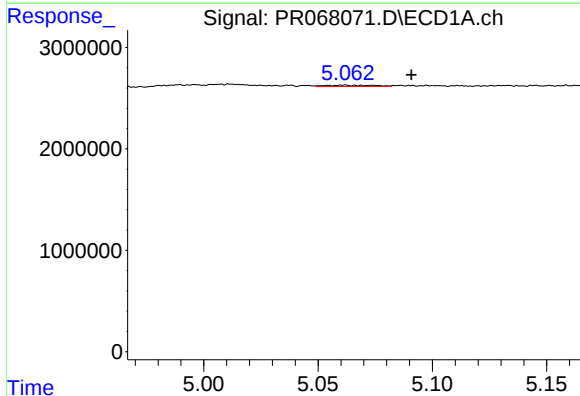


#6 AR-1016-4

R.T.: 5.062 min
Delta R.T.: -0.029 min
Response: 182323
Conc: 2.91 ng/ml

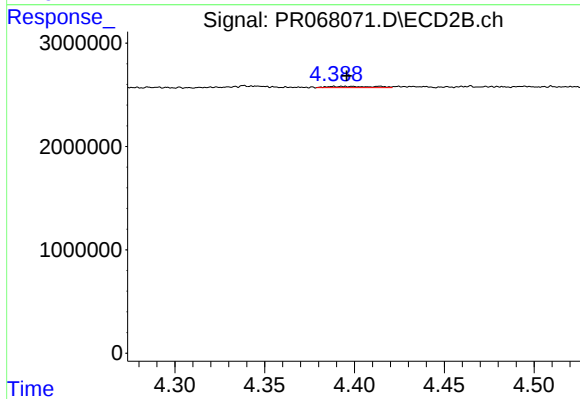

#6 AR-1016-4


R.T.: 4.414 min
Delta R.T.: 0.018 min
Response: 232470
Conc: 2.43 ng/ml

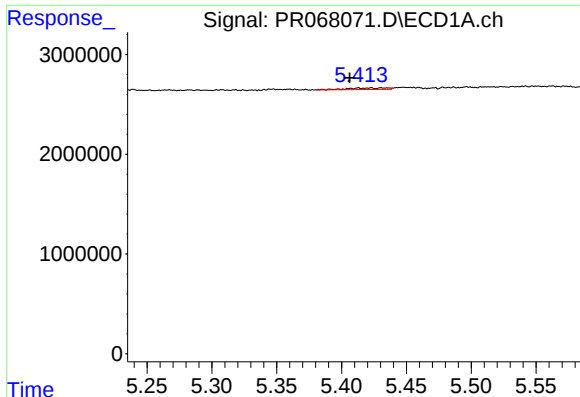

#7 AR-1016-5


R.T.: 5.413 min
Delta R.T.: 0.007 min
Response: 320978
Conc: 6.39 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

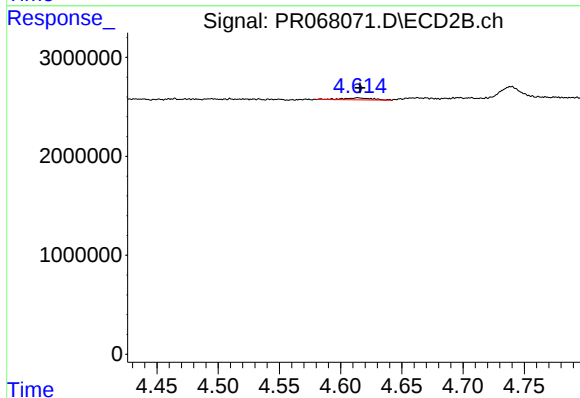


#7 AR-1016-5

R.T.: 4.614 min
Delta R.T.: -0.002 min
Response: 333034
Conc: 2.79 ng/ml

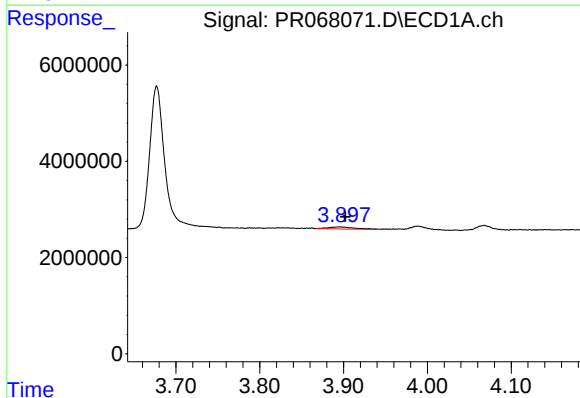


#8 AR-1221-1

R.T.: 3.896 min
Delta R.T.: -0.006 min
Response: 955204
Conc: 34.75 ng/ml

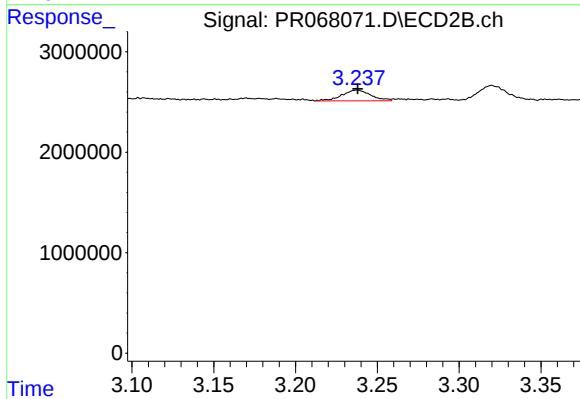

#8 AR-1221-1


R.T.: 3.238 min
Delta R.T.: 0.000 min
Response: 1303564
Conc: 8.39 ng/ml

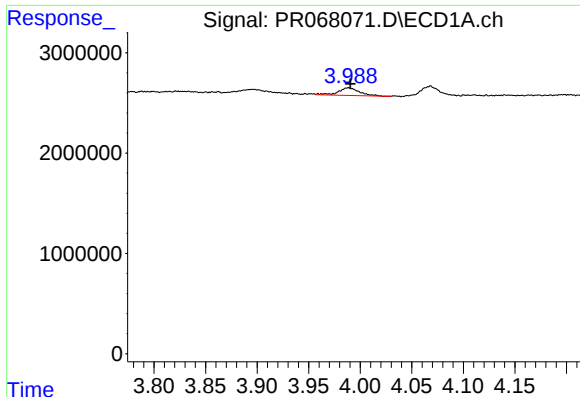

#9 AR-1221-2


R.T.: 3.989 min
Delta R.T.: -0.002 min
Response: 1096891
Conc: 48.81 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

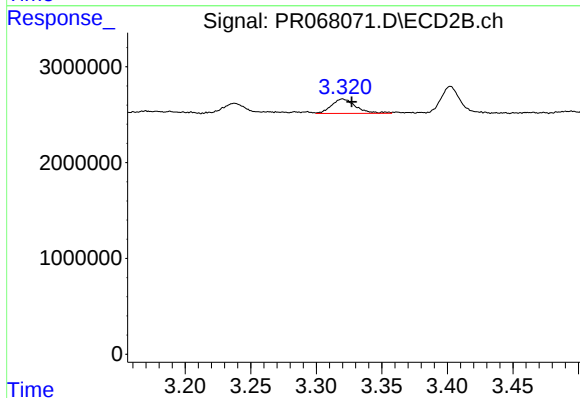


#9 AR-1221-2

R.T.: 3.320 min
Delta R.T.: -0.007 min
Response: 1946660
Conc: 26.50 ng/ml

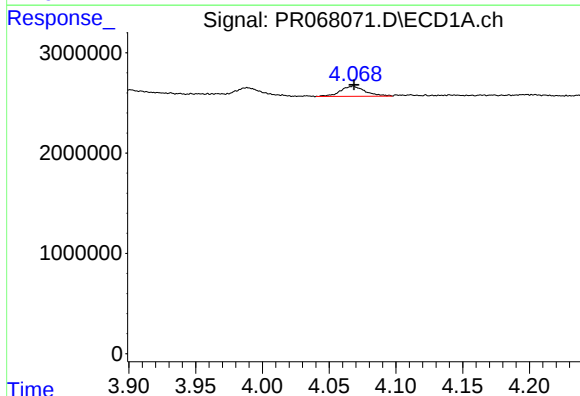


#10 AR-1221-3

R.T.: 4.068 min
Delta R.T.: 0.000 min
Response: 1314174
Conc: 18.39 ng/ml

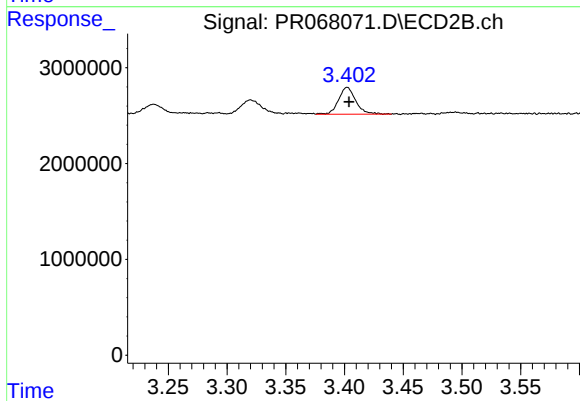

#10 AR-1221-3


R.T.: 3.402 min
Delta R.T.: -0.002 min
Response: 2874710
Conc: 8.87 ng/ml

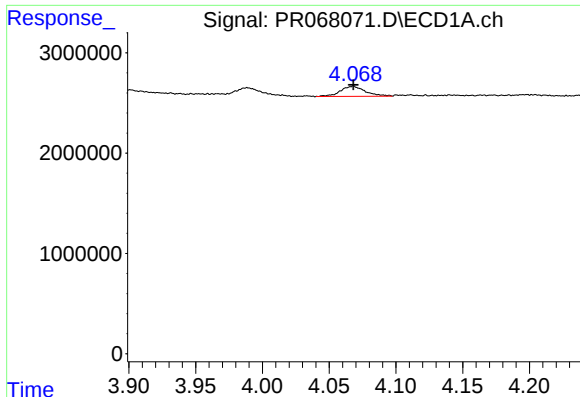

#11 AR-1232-1


R.T.: 4.068 min
Delta R.T.: 0.000 min
Response: 1314174
Conc: 22.33 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

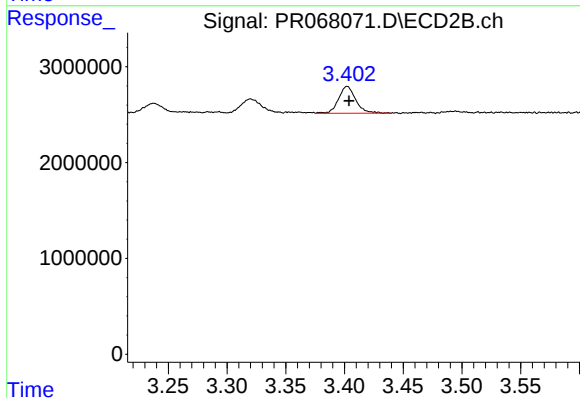


#11 AR-1232-1

R.T.: 3.402 min
Delta R.T.: -0.001 min
Response: 2874710
Conc: 28.38 ng/ml

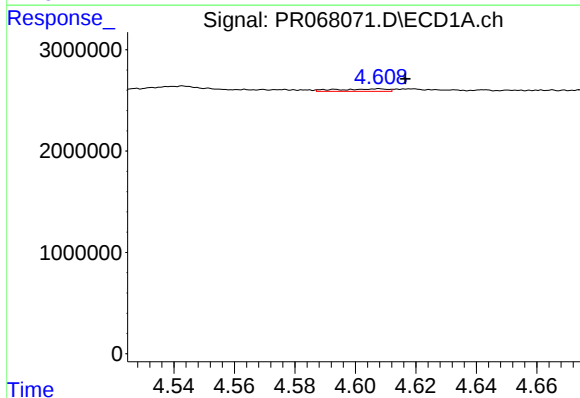


#12 AR-1232-2

R.T.: 4.608 min
Delta R.T.: -0.009 min
Response: 279787
Conc: 8.91 ng/ml

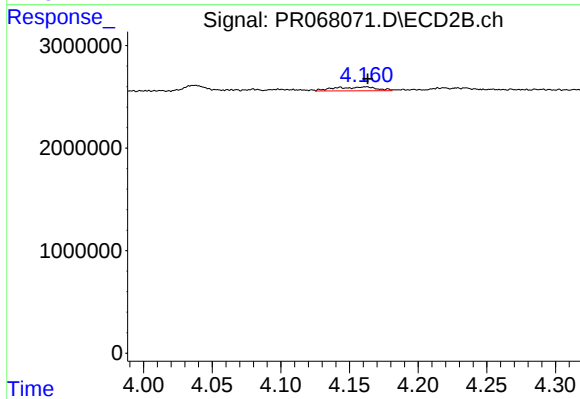

#12 AR-1232-2


R.T.: 4.162 min
Delta R.T.: -0.001 min
Response: 815162
Conc: 8.09 ng/ml

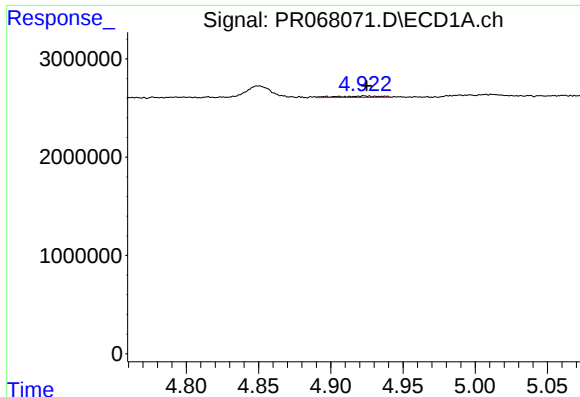

#13 AR-1232-3


R.T.: 4.923 min
Delta R.T.: -0.002 min
Response: 310692
Conc: 5.76 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

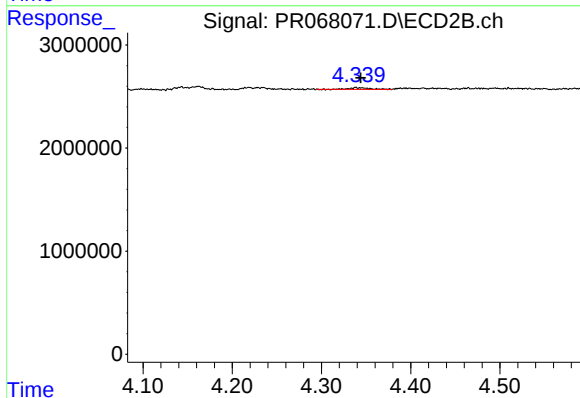


#13 AR-1232-3

R.T.: 4.339 min
Delta R.T.: -0.005 min
Response: 248676
Conc: 4.58 ng/ml

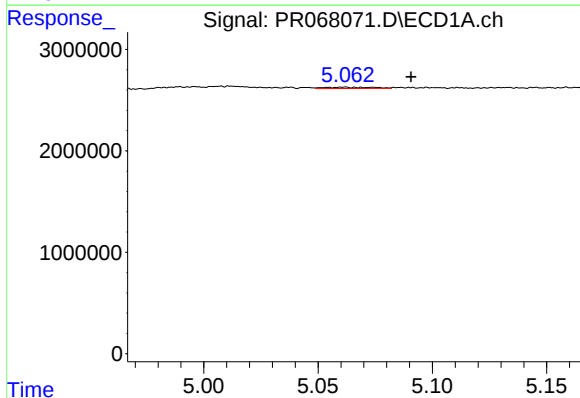


#14 AR-1232-4

R.T.: 5.062 min
Delta R.T.: -0.029 min
Response: 182323
Conc: 6.10 ng/ml

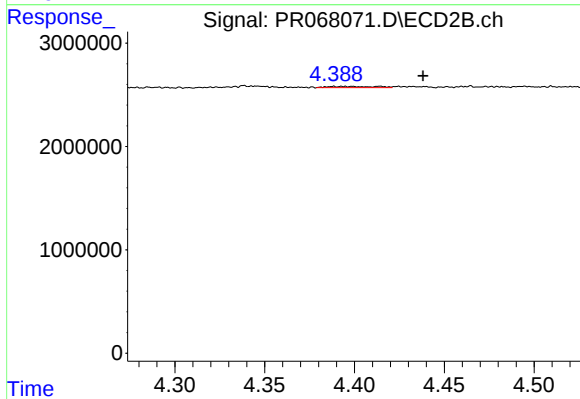

#14 AR-1232-4


R.T.: 4.414 min
Delta R.T.: -0.024 min
Response: 232470
Conc: 4.65 ng/ml

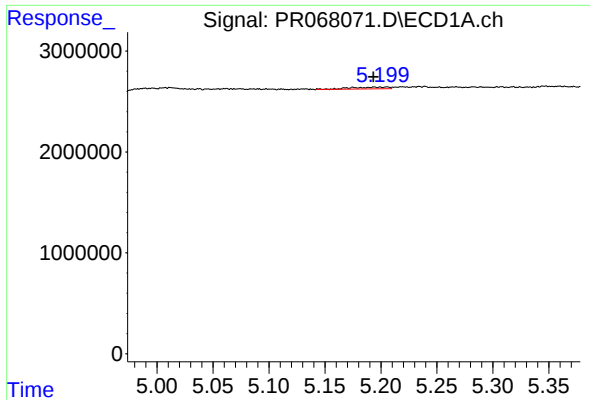

#15 AR-1232-5


R.T.: 5.194 min
Delta R.T.: 0.000 min
Response: 408464
Conc: 26.52 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

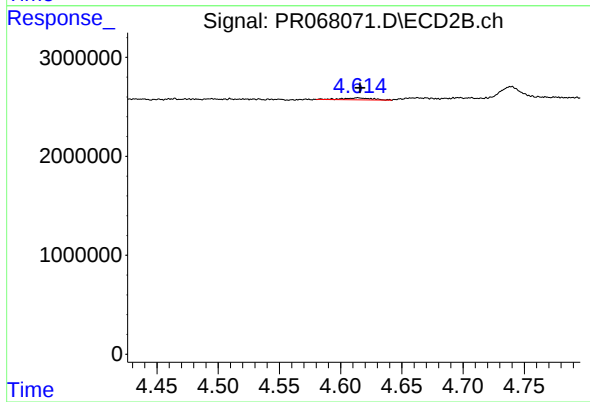


#15 AR-1232-5

R.T.: 4.614 min
Delta R.T.: -0.002 min
Response: 333034
Conc: 6.26 ng/ml

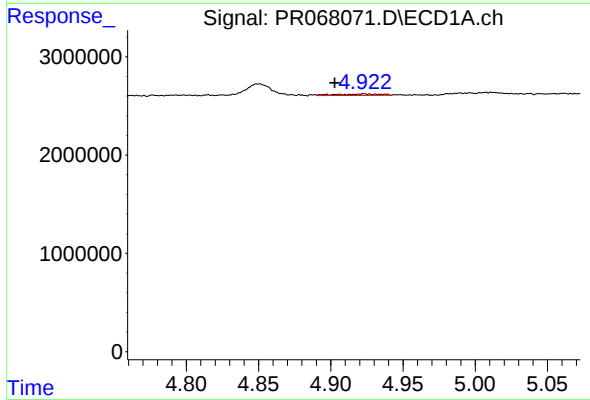


#16 AR-1242-1

R.T.: 4.923 min
Delta R.T.: 0.020 min
Response: 310692
Conc: 6.35 ng/ml

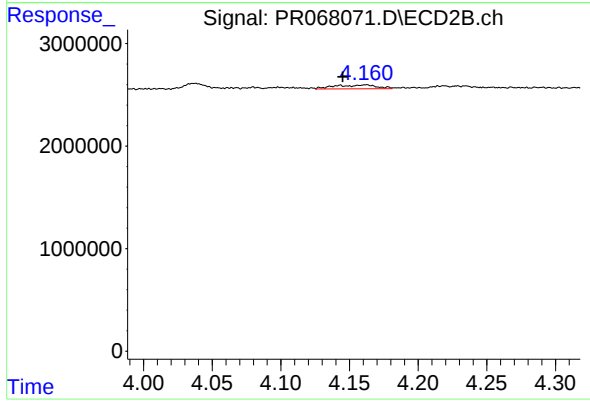

#16 AR-1242-1


R.T.: 4.162 min
Delta R.T.: 0.017 min
Response: 815162
Conc: 5.35 ng/ml

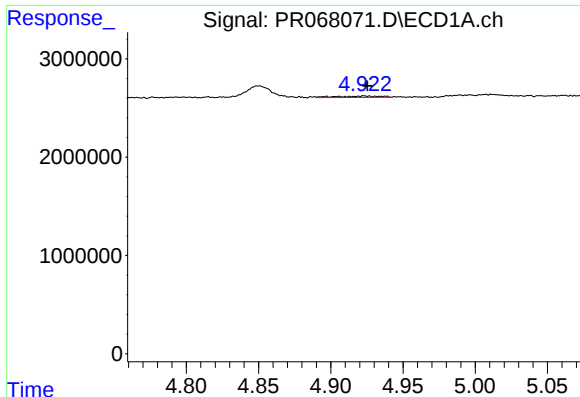

#17 AR-1242-2


R.T.: 4.923 min
Delta R.T.: -0.002 min
Response: 310692
Conc: 3.42 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

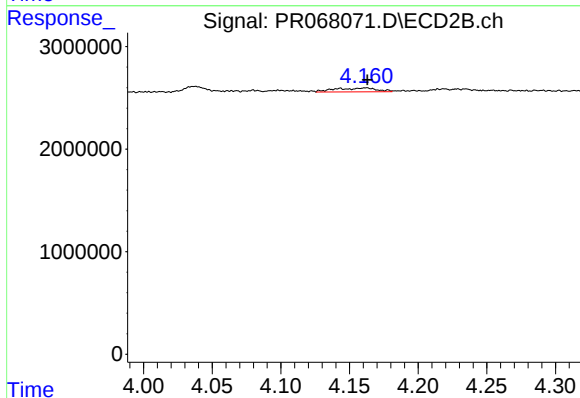


#17 AR-1242-2

R.T.: 4.162 min
Delta R.T.: -0.001 min
Response: 815162
Conc: 3.81 ng/ml

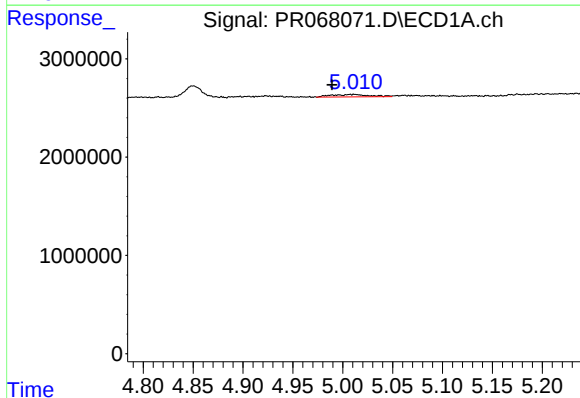


#18 AR-1242-3

R.T.: 5.012 min
Delta R.T.: 0.022 min
Response: 670841
Conc: 10.69 ng/ml

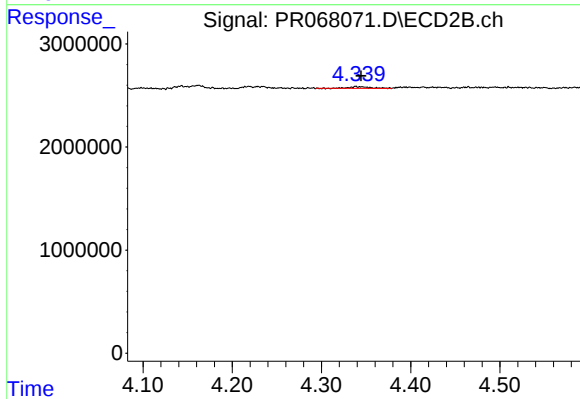

#18 AR-1242-3


R.T.: 4.339 min
Delta R.T.: -0.006 min
Response: 248676
Conc: 2.34 ng/ml

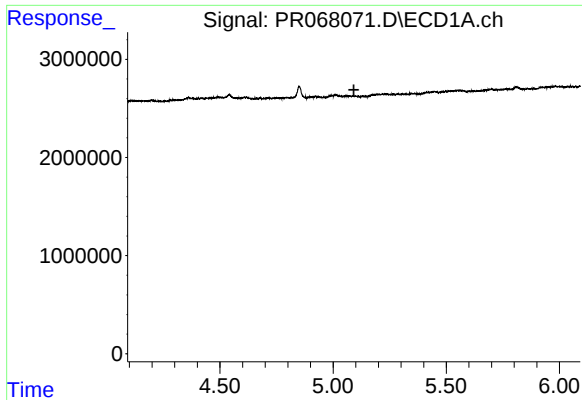

#19 AR-1242-4


R.T.: 0.000 min
Exp R.T.: 5.092 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

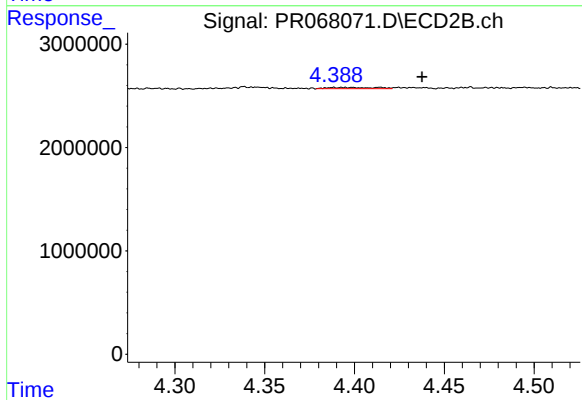


#19 AR-1242-4

R.T.: 4.414 min
Delta R.T.: -0.023 min
Response: 232470
Conc: 2.31 ng/ml

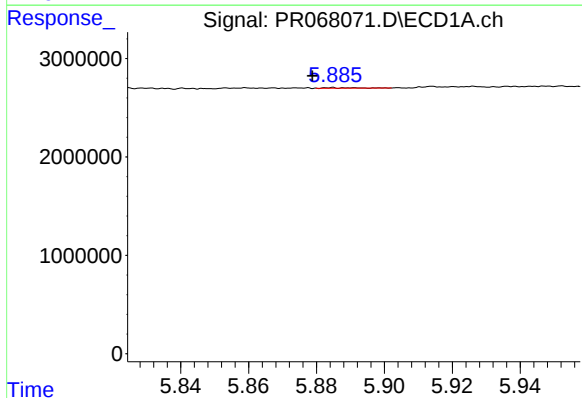


#20 AR-1242-5

R.T.: 5.885 min
Delta R.T.: 0.006 min
Response: 32099
Conc: 0.70 ng/ml

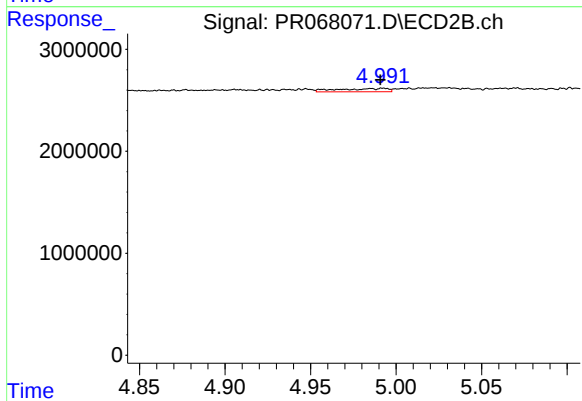

#20 AR-1242-5


R.T.: 4.993 min
Delta R.T.: 0.002 min
Response: 659412
Conc: 4.20 ng/ml

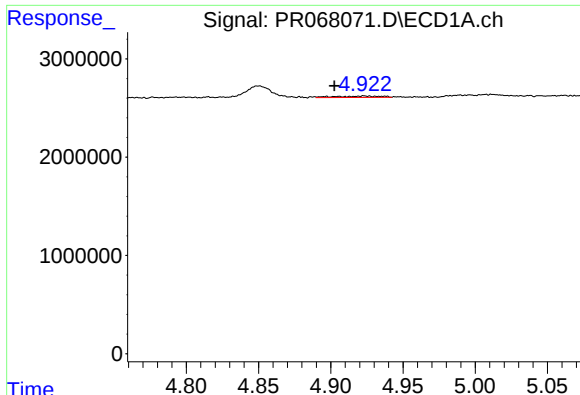

#21 AR-1248-1


R.T.: 4.923 min
Delta R.T.: 0.021 min
Response: 310692
Conc: 8.09 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

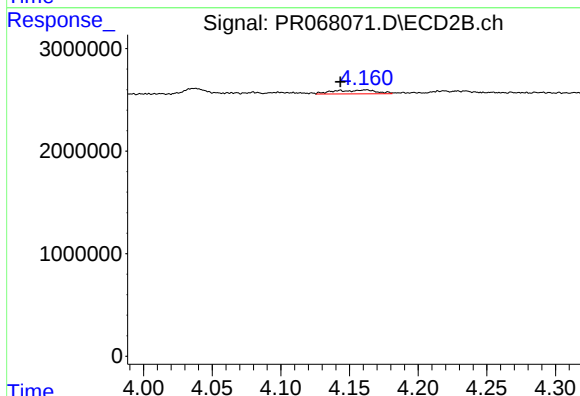


#21 AR-1248-1

R.T.: 4.162 min
Delta R.T.: 0.019 min
Response: 815162
Conc: 6.85 ng/ml

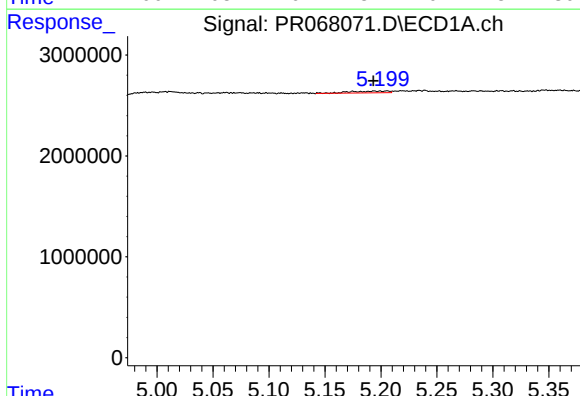


#22 AR-1248-2

R.T.: 5.194 min
Delta R.T.: 0.000 min
Response: 408464
Conc: 7.79 ng/ml

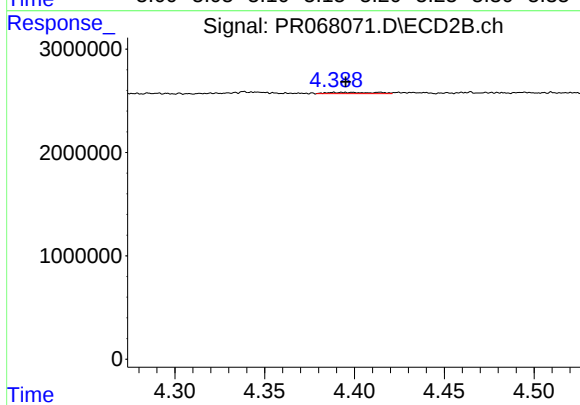

#22 AR-1248-2


R.T.: 4.414 min
Delta R.T.: 0.019 min
Response: 232470
Conc: 1.23 ng/ml

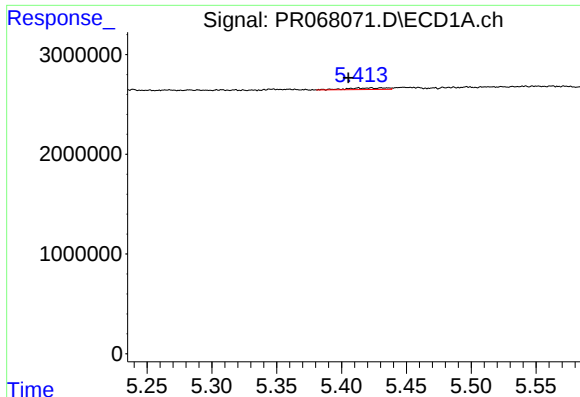

#23 AR-1248-3


R.T.: 5.413 min
Delta R.T.: 0.008 min
Response: 320978
Conc: 4.56 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

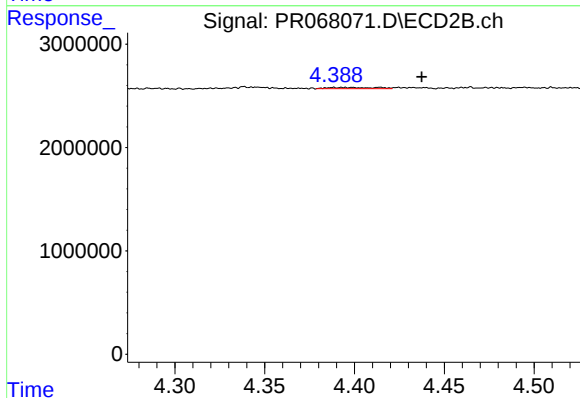


#23 AR-1248-3

R.T.: 4.414 min
Delta R.T.: -0.023 min
Response: 232470
Conc: 1.22 ng/ml

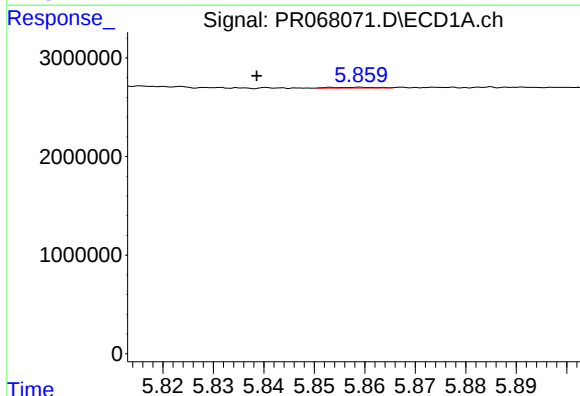


#24 AR-1248-4

R.T.: 5.859 min
Delta R.T.: 0.021 min
Response: 44681
Conc: 0.60 ng/ml

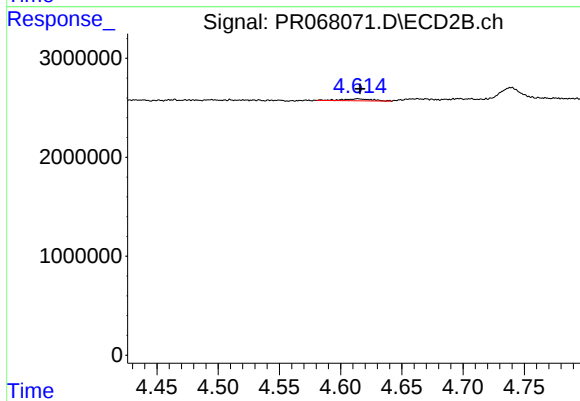

#24 AR-1248-4


R.T.: 4.614 min
Delta R.T.: -0.002 min
Response: 333034
Conc: 1.54 ng/ml

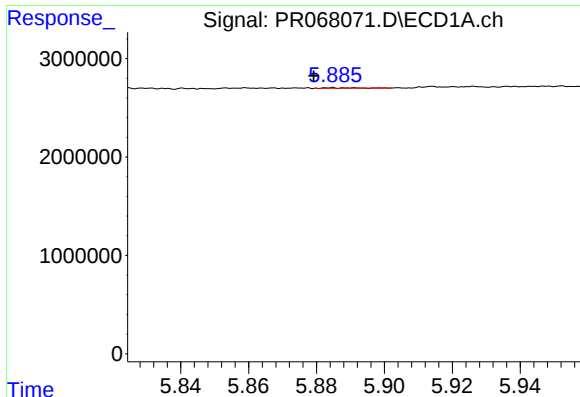

#25 AR-1248-5


R.T.: 5.885 min
Delta R.T.: 0.006 min
Response: 32099
Conc: 0.40 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

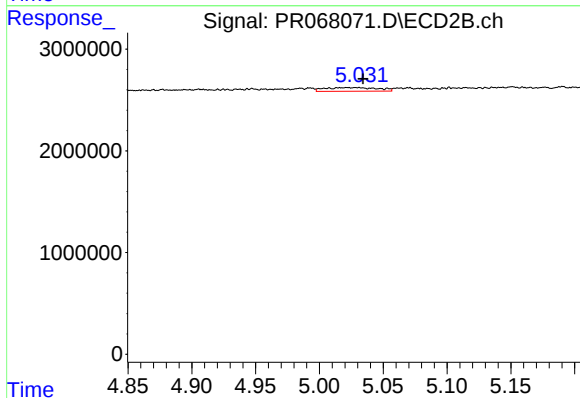


#25 AR-1248-5

R.T.: 5.016 min
Delta R.T.: -0.018 min
Response: 1051805
Conc: 4.95 ng/ml

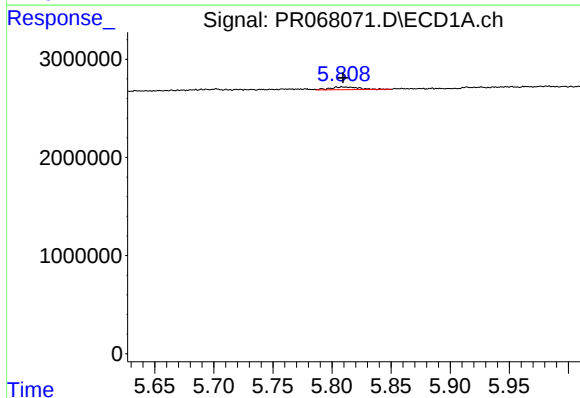


#26 AR-1254-1

R.T.: 5.809 min
Delta R.T.: 0.000 min
Response: 469655
Conc: 6.58 ng/ml

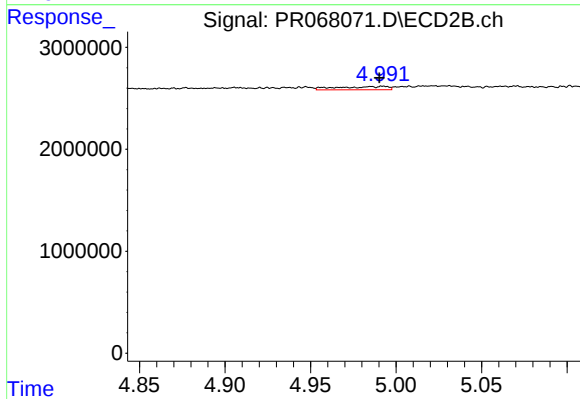

#26 AR-1254-1


R.T.: 4.993 min
Delta R.T.: 0.002 min
Response: 659412
Conc: 2.58 ng/ml

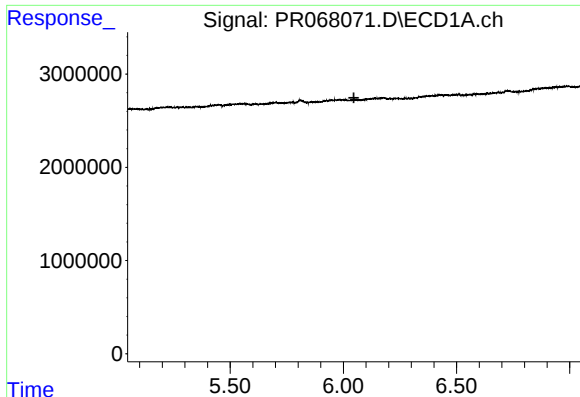

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T.: 6.046 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

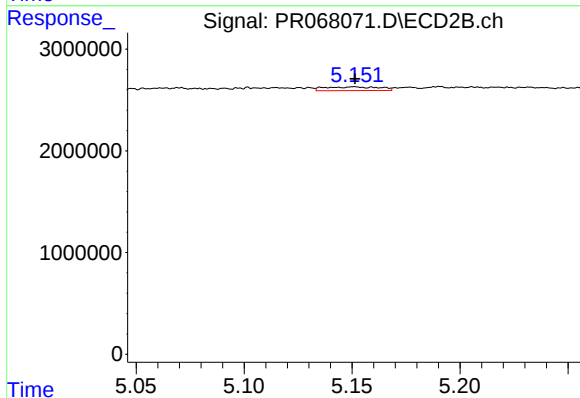


#27 AR-1254-2

R.T.: 5.151 min
Delta R.T.: 0.000 min
Response: 651069
Conc: 2.83 ng/ml

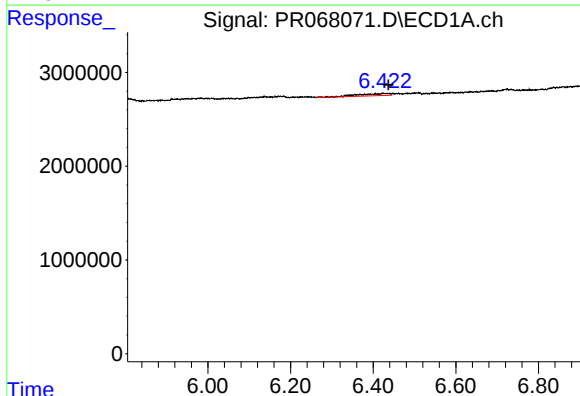


#28 AR-1254-3

R.T.: 6.425 min
Delta R.T.: -0.012 min
Response: 1249005
Conc: 9.29 ng/ml

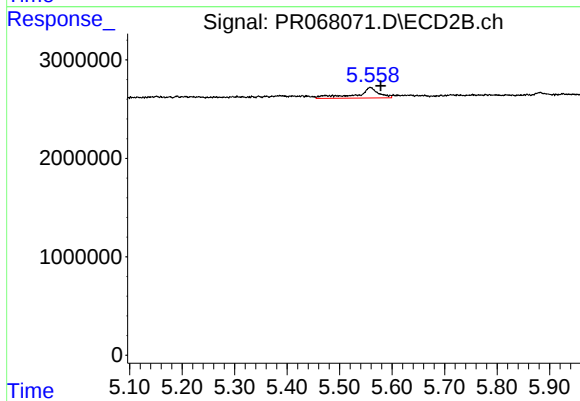

#28 AR-1254-3


R.T.: 5.558 min
Delta R.T.: -0.020 min
Response: 3212603
Conc: 8.90 ng/ml

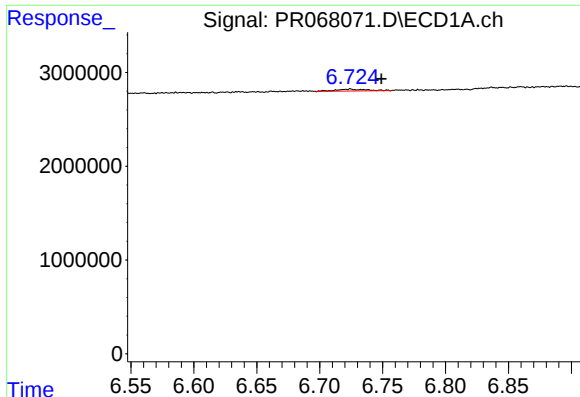

#29 AR-1254-4


R.T.: 6.724 min
Delta R.T.: -0.026 min
Response: 351791
Conc: 3.37 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

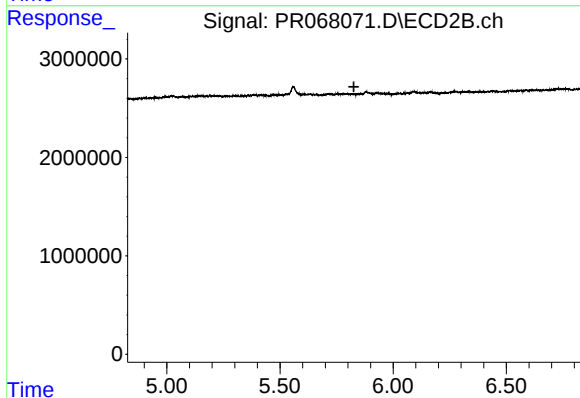


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 5.826 min
Response: 0
Conc: N.D.

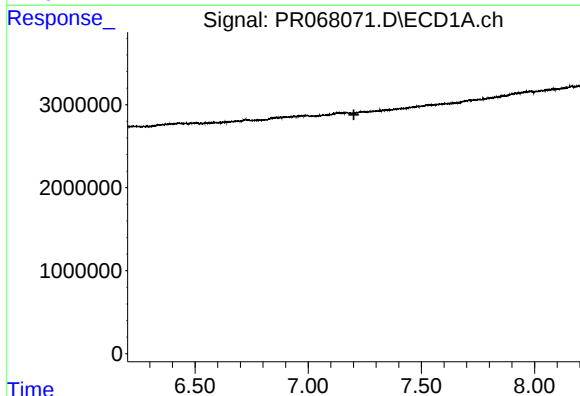


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.202 min
Response: 0
Conc: N.D.

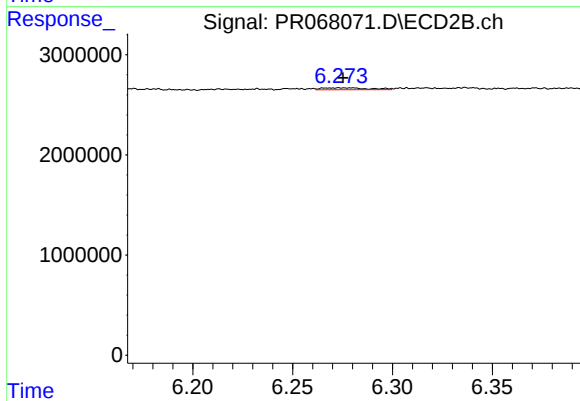

#30 AR-1254-5


R.T.: 6.274 min
Delta R.T.: -0.001 min
Response: 306690
Conc: 0.93 ng/ml

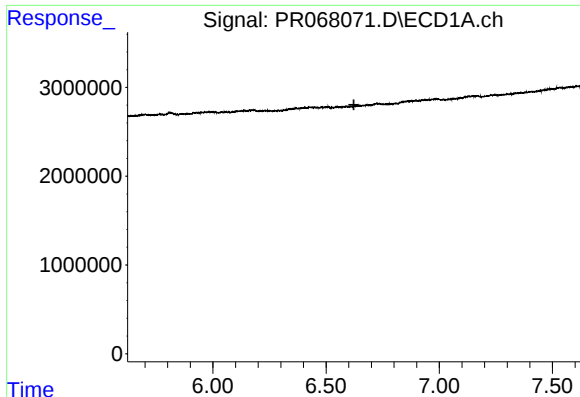

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T.: 6.623 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

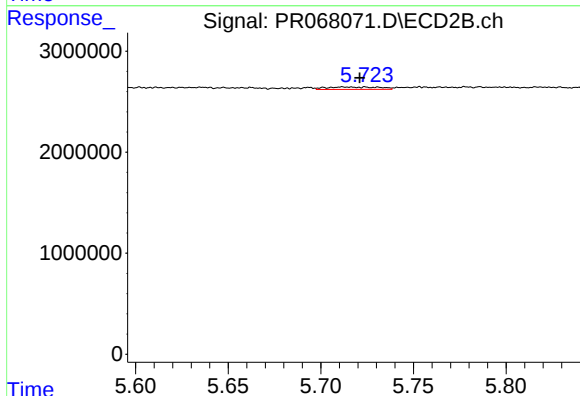


#31 AR-1260-1

R.T.: 5.712 min
Delta R.T.: -0.009 min
Response: 484497
Conc: 1.98 ng/ml

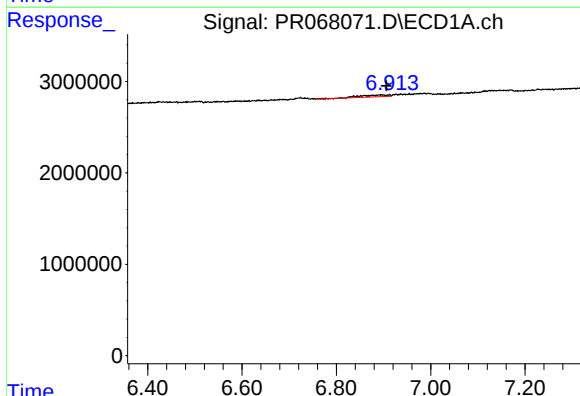


#32 AR-1260-2

R.T.: 6.895 min
Delta R.T.: -0.011 min
Response: 902077
Conc: 6.35 ng/ml

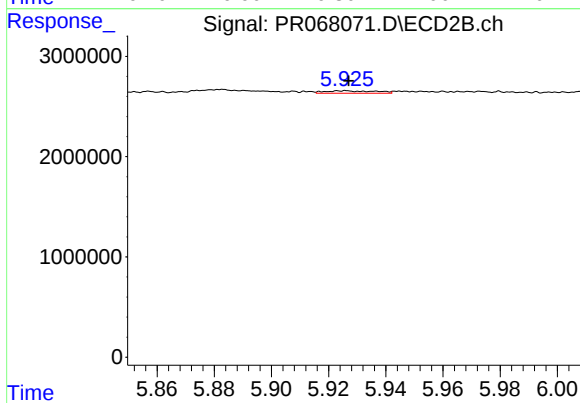

#32 AR-1260-2


R.T.: 5.925 min
Delta R.T.: -0.002 min
Response: 302633
Conc: 1.04 ng/ml

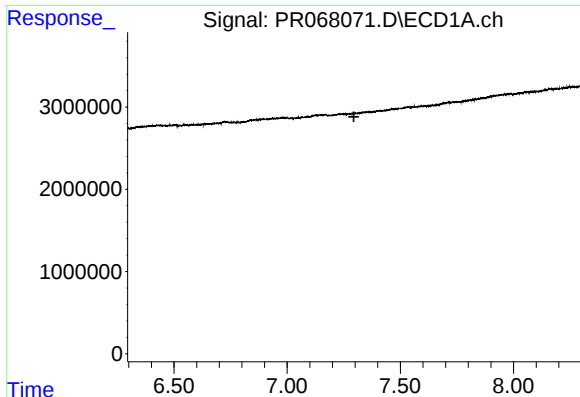

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 7.295 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

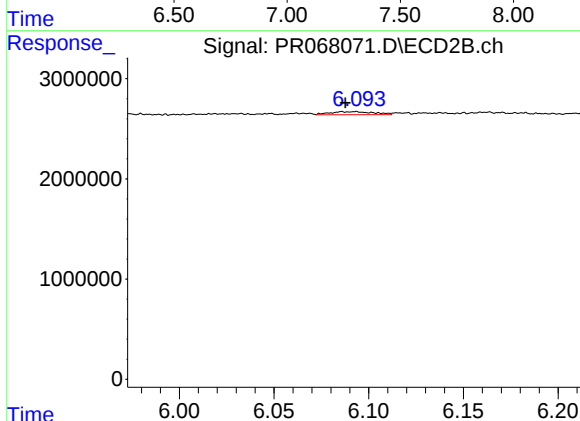


#33 AR-1260-3

R.T.: 6.093 min
Delta R.T.: 0.005 min
Response: 492280
Conc: 1.79 ng/ml

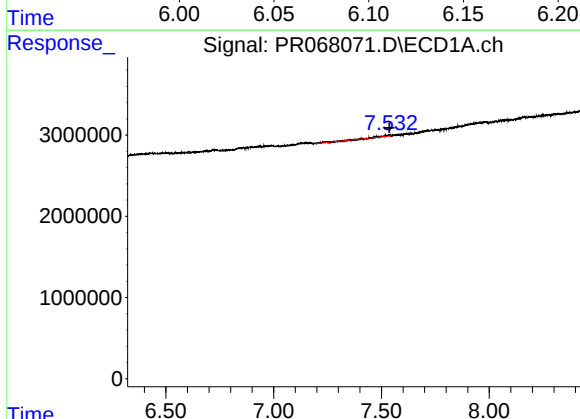


#34 AR-1260-4

R.T.: 7.534 min
Delta R.T.: -0.004 min
Response: 427464
Conc: 3.37 ng/ml

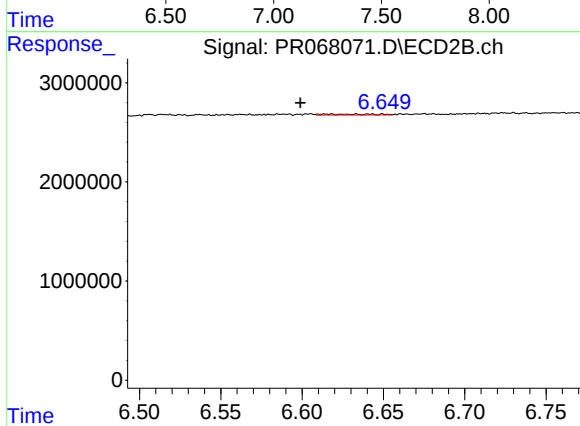

#34 AR-1260-4


R.T.: 6.618 min
Delta R.T.: 0.019 min
Response: 191950
Conc: 0.92 ng/ml

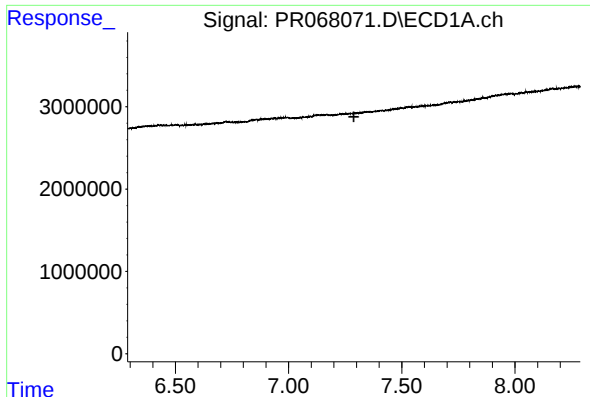

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T.: 7.289 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

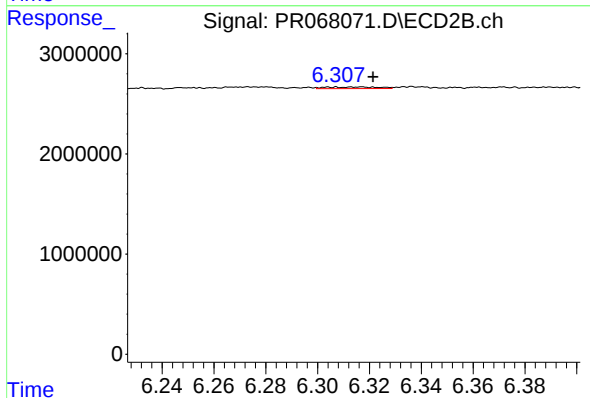


#36 AR-1262-1

R.T.: 6.317 min
Delta R.T.: -0.005 min
Response: 217389
Conc: 0.63 ng/ml

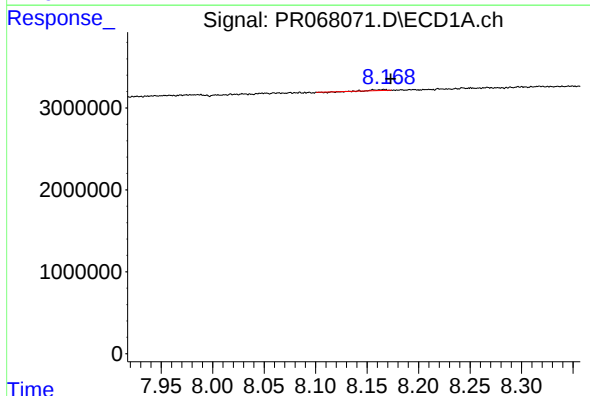


#38 AR-1262-3

R.T.: 8.165 min
Delta R.T.: -0.008 min
Response: 58606
Conc: 0.19 ng/ml

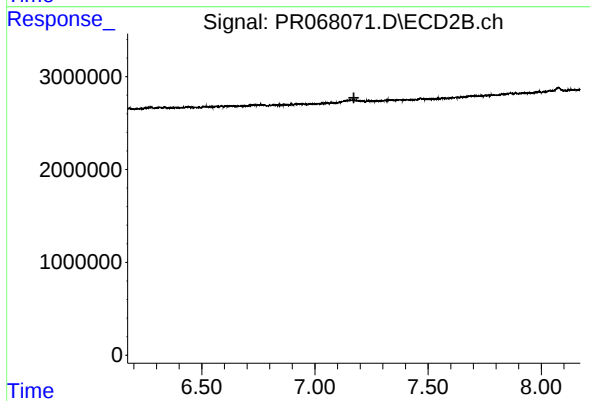

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 7.172 min
Response: 0
Conc: N.D.

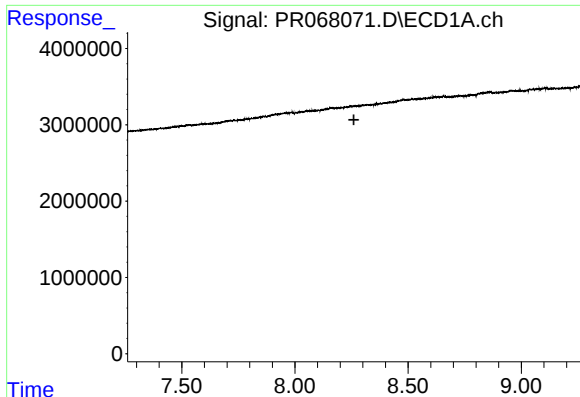

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 8.261 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

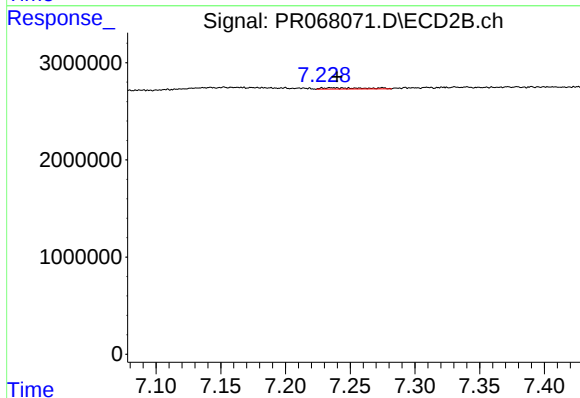


#39 AR-1262-4

R.T.: 7.236 min
Delta R.T.: -0.004 min
Response: 304314
Conc: 0.68 ng/ml

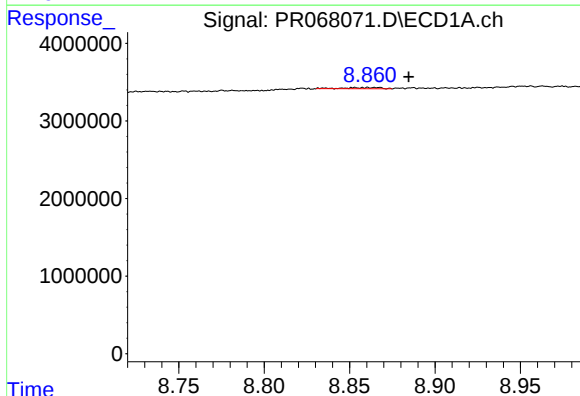


#40 AR-1262-5

R.T.: 8.864 min
Delta R.T.: -0.021 min
Response: 221967
Conc: 1.17 ng/ml

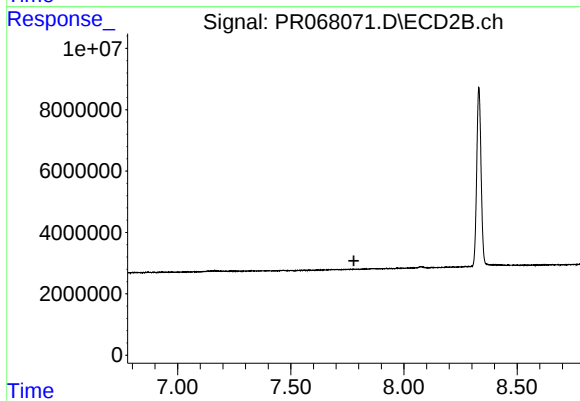

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T.: 7.779 min
Response: 0
Conc: N.D.

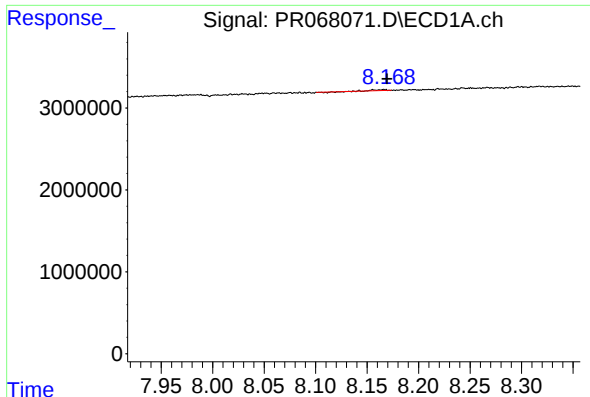

#41 AR-1268-1


R.T.: 8.165 min
Delta R.T.: -0.004 min
Response: 58606
Conc: 0.10 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

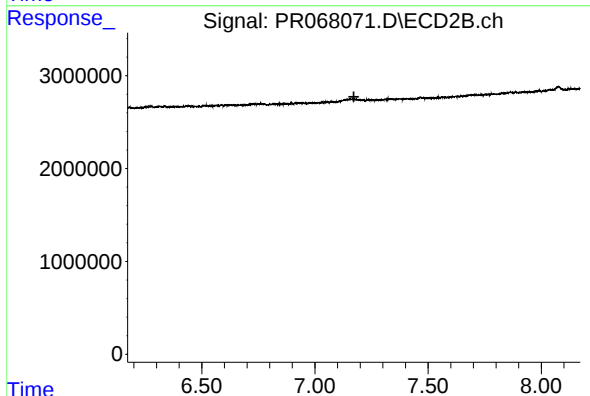


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 7.172 min
Response: 0
Conc: N.D.

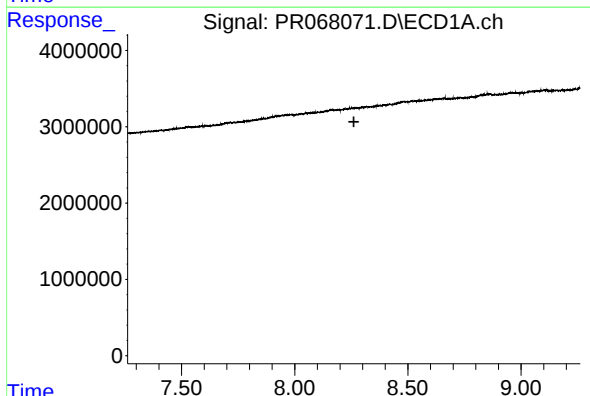


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 8.261 min
Response: 0
Conc: N.D.

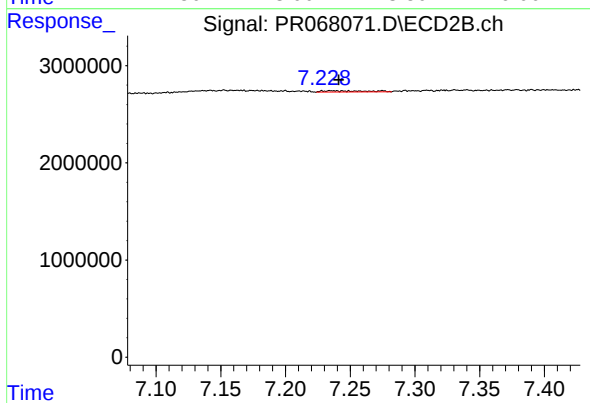

#42 AR-1268-2


R.T.: 7.236 min
Delta R.T.: -0.005 min
Response: 304314
Conc: 0.45 ng/ml

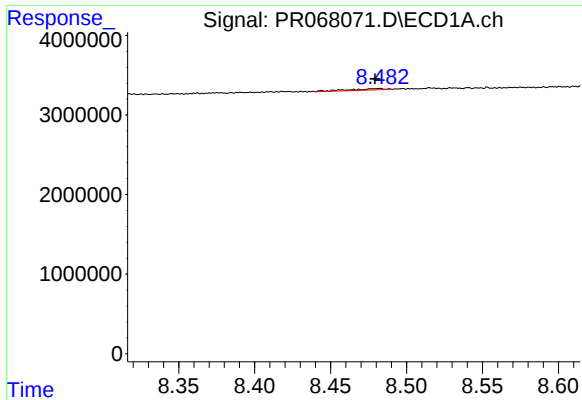

#43 AR-1268-3


R.T.: 8.481 min
Delta R.T.: 0.002 min
Response: 289219
Conc: 0.52 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

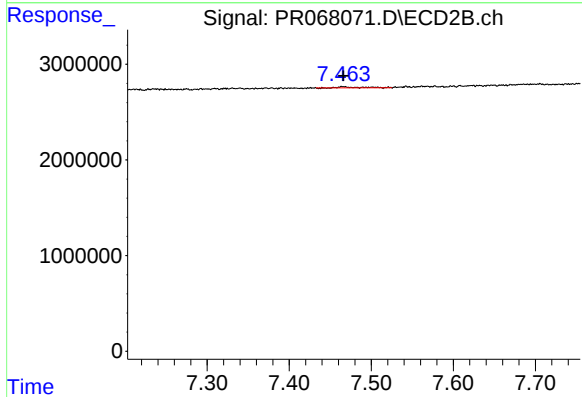


#43 AR-1268-3

R.T.: 7.466 min
Delta R.T.: 0.000 min
Response: 204121
Conc: 0.33 ng/ml

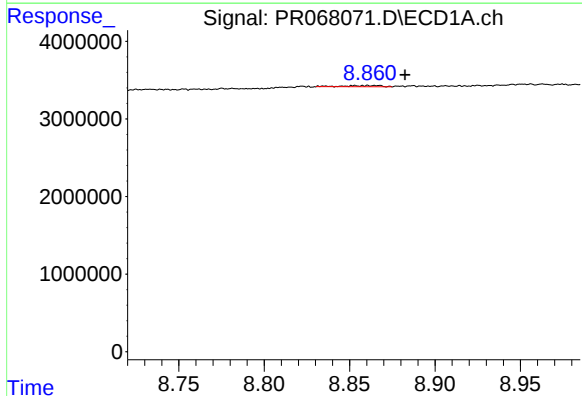


#44 AR-1268-4

R.T.: 8.864 min
Delta R.T.: -0.019 min
Response: 221967
Conc: 1.10 ng/ml

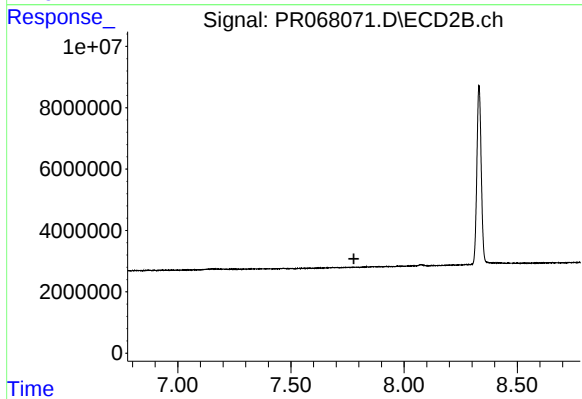

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T. : 7.778 min
Response: 0
Conc: N.D.

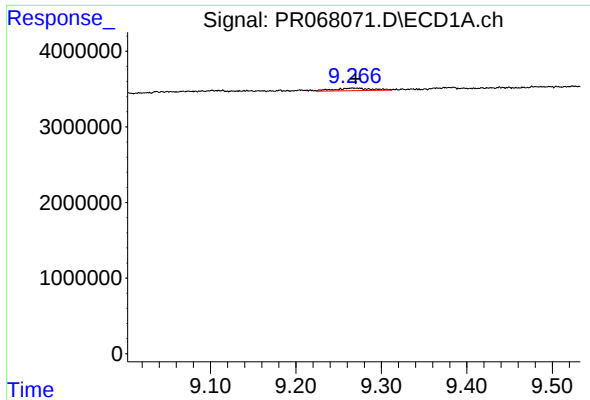

#45 AR-1268-5

R.T.: 9.267 min
Delta R.T.: -0.003 min
Response: 992391
Conc: 0.63 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

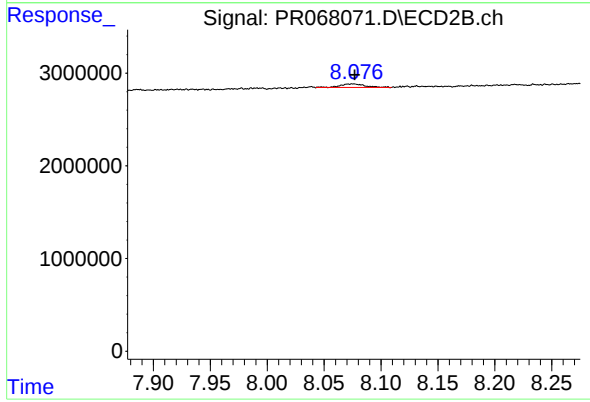

#45 AR-1268-5

R.T.: 8.074 min
Delta R.T.: -0.003 min
Response: 544213
Conc: 0.38 ng/ml