

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR080724\
 Data File : PR068072.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Aug 2024 11:05
 Operator : AJ\MA
 Sample : P3390-09
 Misc : AR1232 MDL 25 PPB
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 07 17:09:20 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 07 00:26:28 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.678	3.011	46964762	90379623	18.462	20.726
2)	SA Decachlor...	9.580	8.332	87417703	98974857	19.922	21.844
Target Compounds							
3)	L1 AR-1016-1	4.903	4.142	919532	2171887	15.734	14.452
4)	L1 AR-1016-2	4.924	4.161	1569075	2803503	14.152	13.360
5)	L1 AR-1016-3	4.990	4.342	1482624	1647899	19.306	14.447 #
6)	L1 AR-1016-4	5.091	4.394	1021324	1261727	16.309	13.194
7)	L1 AR-1016-5	5.403	4.613	371395	1584165	7.396	13.254 #
8)	L2 AR-1221-1	3.899	3.237	601006	1139376	21.866	7.331 #
9)	L2 AR-1221-2	3.989	3.319	1154176	2086865	51.363	28.414 #
10)	L2 AR-1221-3	4.068	3.402	1421908	2819199	19.903	8.702 #
11)	L3 AR-1232-1	4.068	3.402	1421908	2819199	24.162	27.833
12)	L3 AR-1232-2	4.615	4.161	887021	2803503	28.242	27.824
13)	L3 AR-1232-3	4.924	4.342	1569075	1647899	29.105	30.344
14)	L3 AR-1232-4	5.091	4.437	1021324	1472623	34.157	29.470
15)	L3 AR-1232-5	5.194	4.613	537833	1584165	34.921	29.793
16)	L4 AR-1242-1	4.903	4.142	919532	2171887	18.797	14.247
17)	L4 AR-1242-2	4.924	4.161	1569075	2803503	17.269	13.110
18)	L4 AR-1242-3	4.990	4.342	1482624	1647899	23.623	15.512 #
19)	L4 AR-1242-4	5.091	4.437	1021324	1472623	20.464	14.644 #
20)	L4 AR-1242-5	5.877	4.989	620347	2006427	13.495	12.794
21)	L5 AR-1248-1	4.903	4.142	919532	2171887	23.958	18.251
22)	L5 AR-1248-2	5.194	4.394	537833	1261727	10.253	6.695 #
23)	L5 AR-1248-3	5.403	4.437	371395	1472623	5.275	7.726 #
24)	L5 AR-1248-4	5.838	4.613	575990	1584165	7.747	7.336
25)	L5 AR-1248-5	5.877	5.032	620347	1968298	7.685	9.263
26)	L6 AR-1254-1	5.812	4.989	974341	2006427	13.653	7.846 #
27)	L6 AR-1254-2	6.047	5.151	458403	1419359	4.084	6.175 #
28)	L6 AR-1254-3	6.431	5.559f	654374	2975136	4.870	8.246 #
29)	L6 AR-1254-4	6.723f	5.823	759498	671635	7.267	3.125 #
30)	L6 AR-1254-5	0.000	6.272	0	264001	N.D.	0.800 #
31)	L7 AR-1260-1	0.000	5.728	0	811956	N.D.	3.317 #
32)	L7 AR-1260-2	6.929f	5.923	1102507	360497	7.757	1.242 #
33)	L7 AR-1260-3	0.000	6.089	0	789415	N.D.	2.875 #
34)	L7 AR-1260-4	7.557f	6.601	1050488	921951	8.288	4.397 #
35)	L7 AR-1260-5	0.000	6.868	0	365605	N.D.	0.755 #
36)	L8 AR-1262-1	0.000	6.297f	0	274262	N.D.	0.794 #
37)	L8 AR-1262-2	0.000	6.868	0	365605	N.D.	0.601 #
38)	L8 AR-1262-3	0.000	7.168	0	781048	N.D.	3.271 #
39)	L8 AR-1262-4	0.000	7.239	0	122608	N.D.	0.276 #
40)	L8 AR-1262-5	8.875	0.000	608420	0	3.214	N.D. #
41)	L9 AR-1268-1	0.000	7.168	0	781048	N.D.	1.058 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR080724\
Data File : PR068072.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Aug 2024 11:05
Operator : AJ\MA
Sample : P3390-09
Misc : AR1232 MDL 25 PPB
ALS Vial : 58 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 17:09:20 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 07 00:26:28 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	0.000	7.239	0	122608	N.D.	0.182 #
43)	L9 AR-1268-3	8.481	7.471	45895	132827	0.083	0.215 #
44)	L9 AR-1268-4	8.875	0.000	608420	0	3.004	N.D. #
45)	L9 AR-1268-5	9.272	8.075	1262726	693265	0.807	0.485 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR080724\
Data File : PR068072.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Aug 2024 11:05
Operator : AJ\MA
Sample : P3390-09
Misc : AR1232 MDL 25 PPB
ALS Vial : 58 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 17:09:20 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 07 00:26:28 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

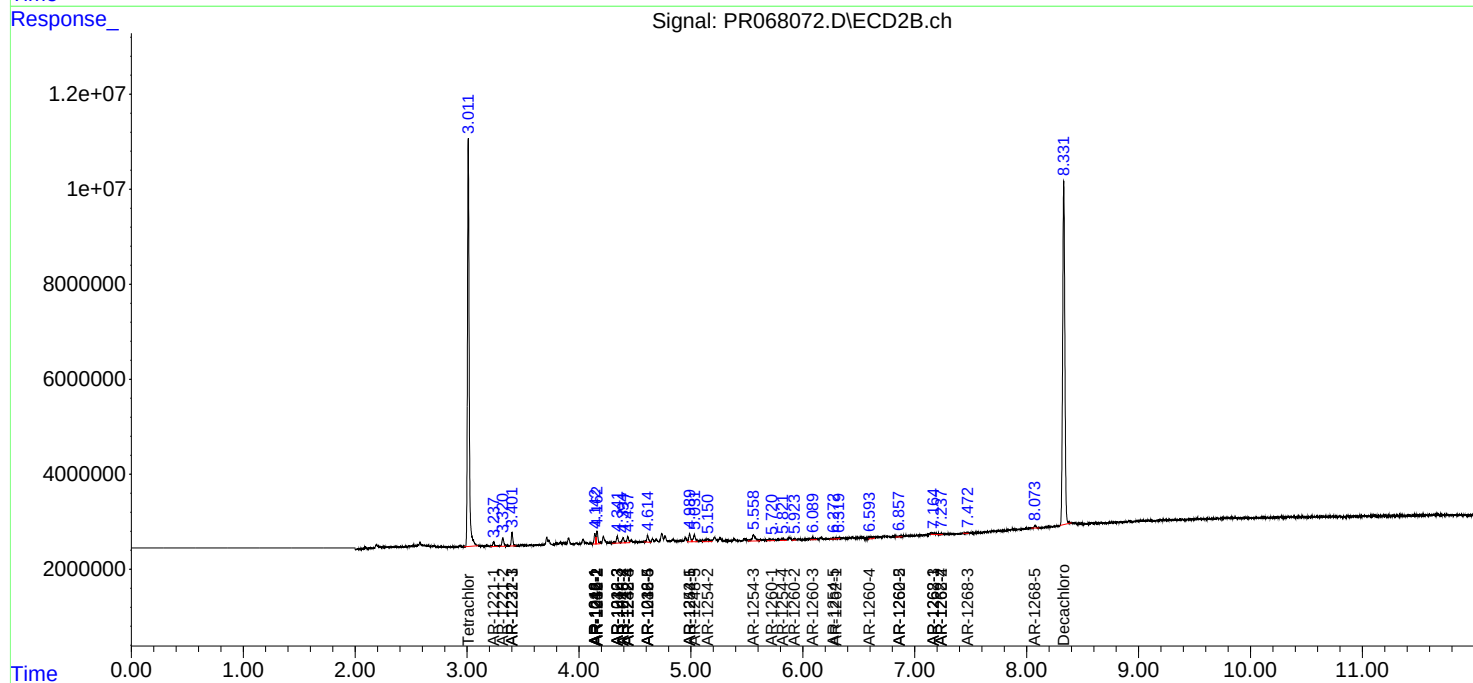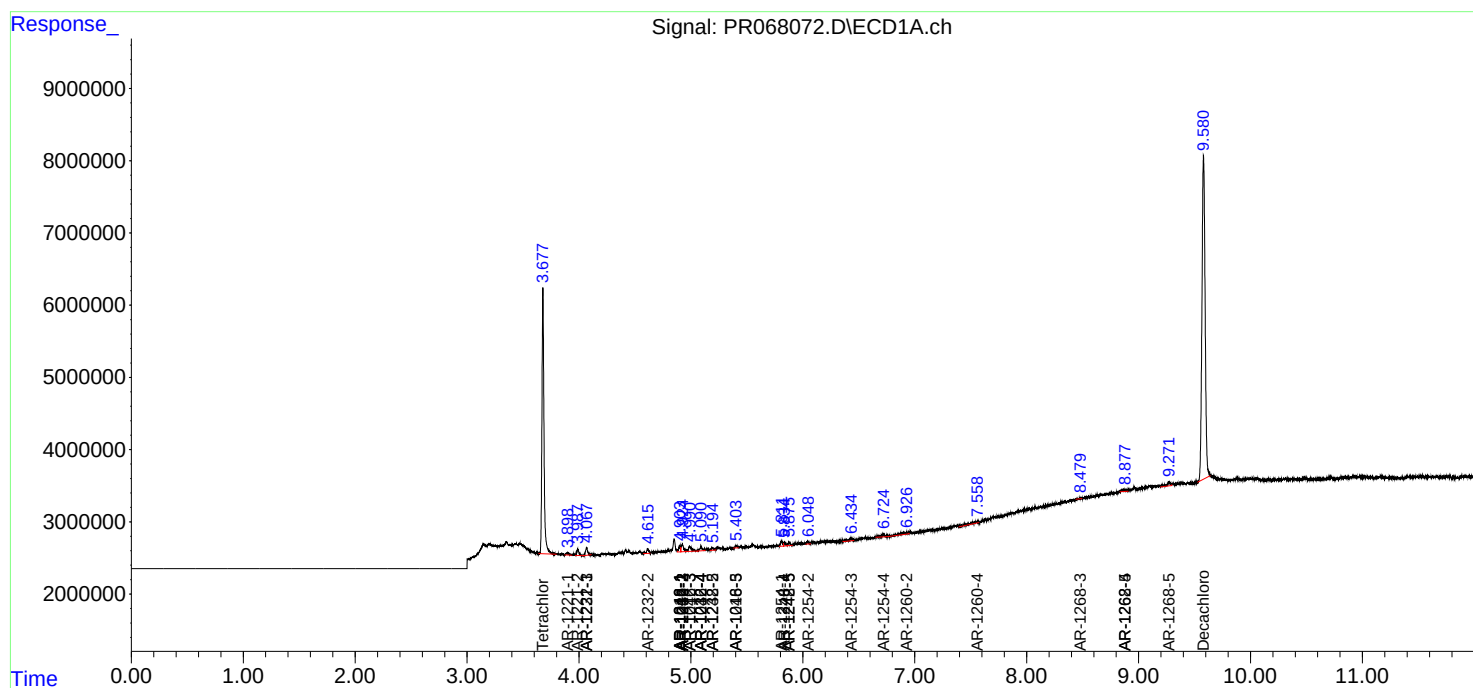


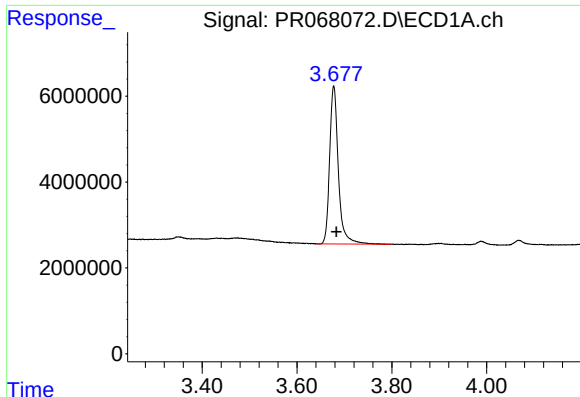

#1 Tetrachloro-m-xylene


R.T.: 3.678 min
Delta R.T.: -0.005 min
Response: 46964762
Conc: 18.46 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

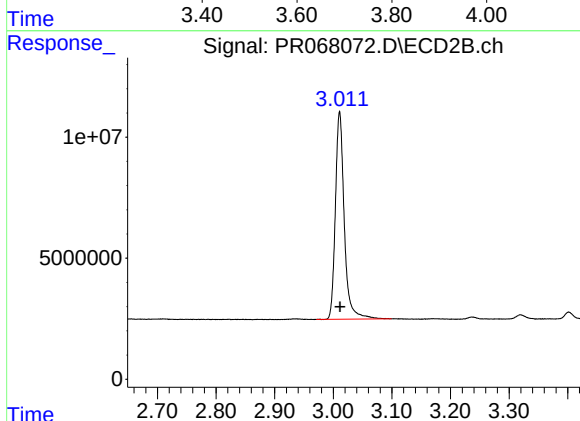


#1 Tetrachloro-m-xylene

R.T.: 3.011 min
Delta R.T.: 0.000 min
Response: 90379623
Conc: 20.73 ng/ml

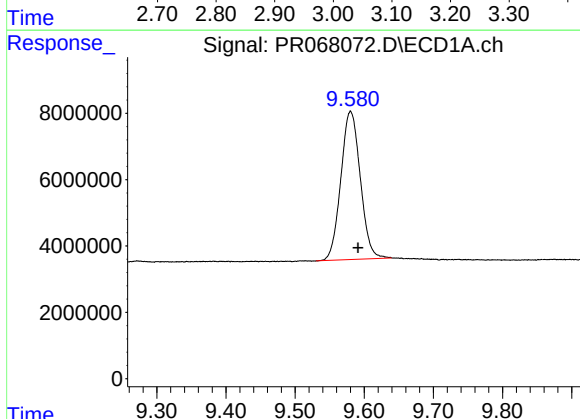


#2 Decachlorobiphenyl

R.T.: 9.580 min
Delta R.T.: -0.011 min
Response: 87417703
Conc: 19.92 ng/ml

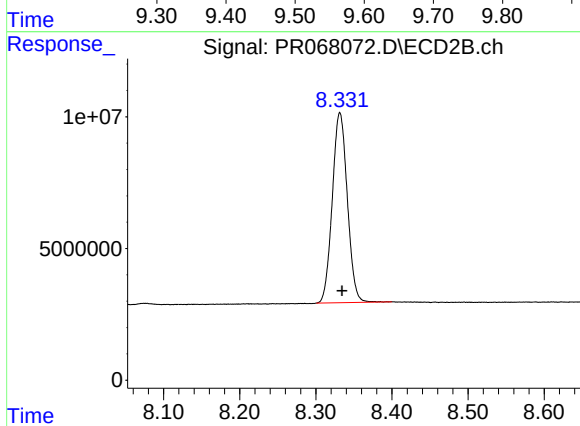

#2 Decachlorobiphenyl


R.T.: 8.332 min
Delta R.T.: -0.003 min
Response: 98974857
Conc: 21.84 ng/ml

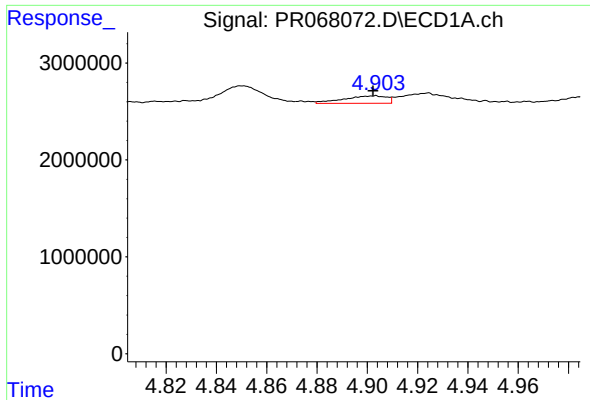

#3 AR-1016-1


R.T.: 4.903 min
Delta R.T.: 0.000 min
Response: 919532
Conc: 15.73 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

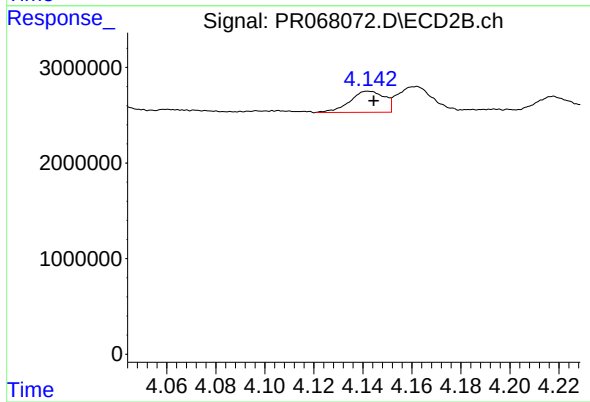


#3 AR-1016-1

R.T.: 4.142 min
Delta R.T.: -0.002 min
Response: 2171887
Conc: 14.45 ng/ml

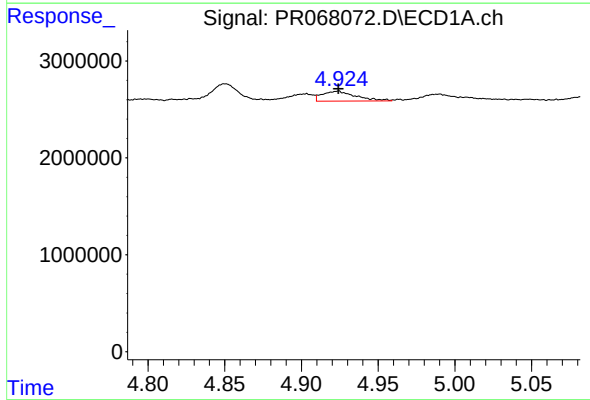


#4 AR-1016-2

R.T.: 4.924 min
Delta R.T.: 0.000 min
Response: 1569075
Conc: 14.15 ng/ml

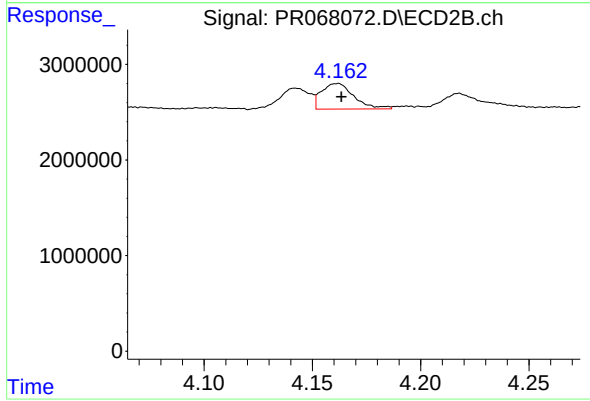

#4 AR-1016-2


R.T.: 4.161 min
Delta R.T.: -0.002 min
Response: 2803503
Conc: 13.36 ng/ml

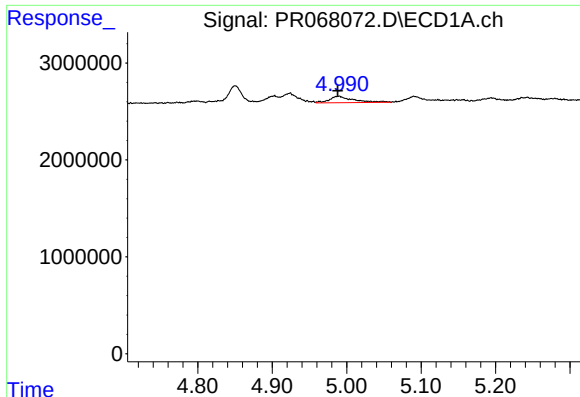

#5 AR-1016-3


R.T.: 4.990 min
Delta R.T.: 0.001 min
Response: 1482624
Conc: 19.31 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

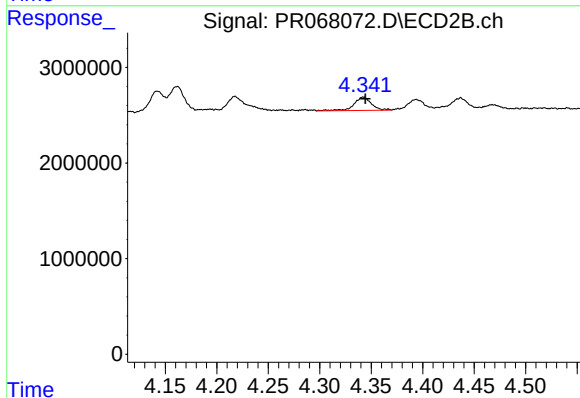


#5 AR-1016-3

R.T.: 4.342 min
Delta R.T.: -0.002 min
Response: 1647899
Conc: 14.45 ng/ml

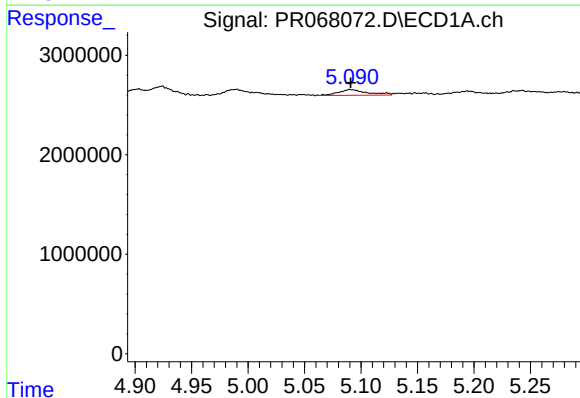


#6 AR-1016-4

R.T.: 5.091 min
Delta R.T.: 0.000 min
Response: 1021324
Conc: 16.31 ng/ml

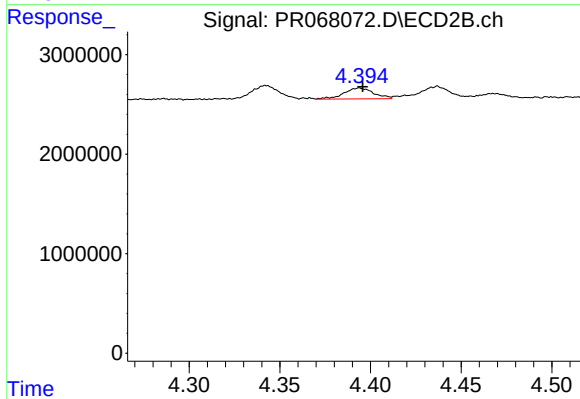

#6 AR-1016-4


R.T.: 4.394 min
Delta R.T.: -0.002 min
Response: 1261727
Conc: 13.19 ng/ml

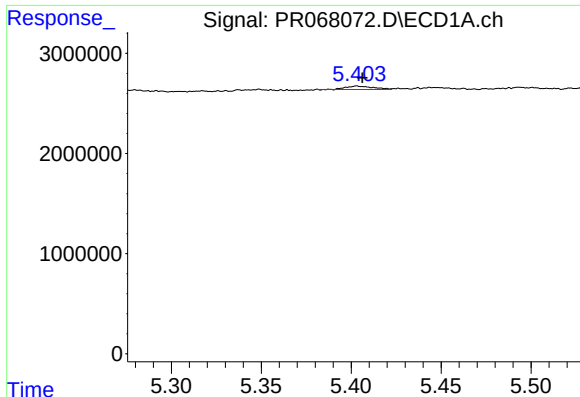

#7 AR-1016-5


R.T.: 5.403 min
Delta R.T.: -0.003 min
Response: 371395
Conc: 7.40 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

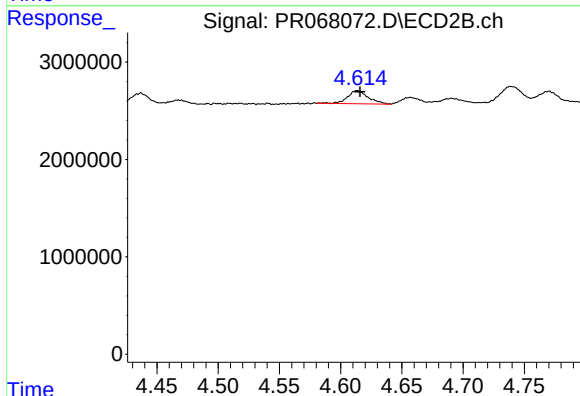


#7 AR-1016-5

R.T.: 4.613 min
Delta R.T.: -0.002 min
Response: 1584165
Conc: 13.25 ng/ml

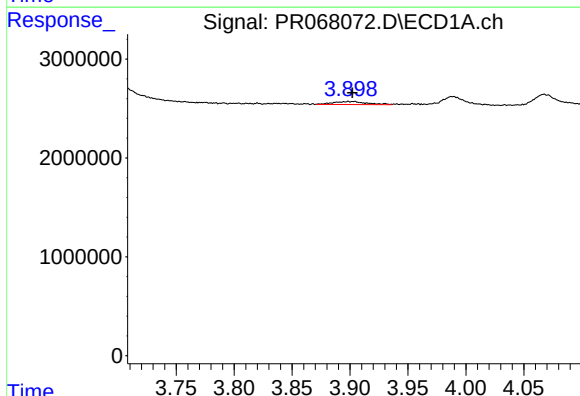


#8 AR-1221-1

R.T.: 3.899 min
Delta R.T.: -0.003 min
Response: 601006
Conc: 21.87 ng/ml

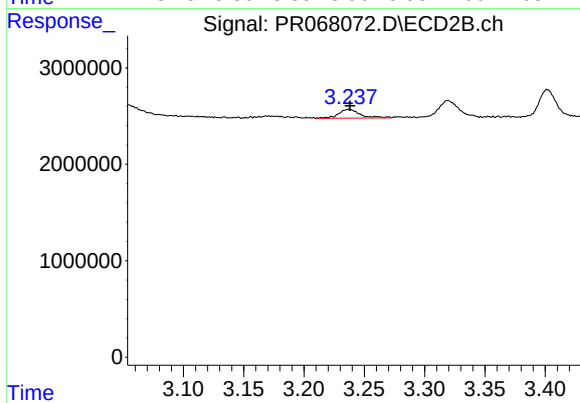

#8 AR-1221-1


R.T.: 3.237 min
Delta R.T.: -0.001 min
Response: 1139376
Conc: 7.33 ng/ml

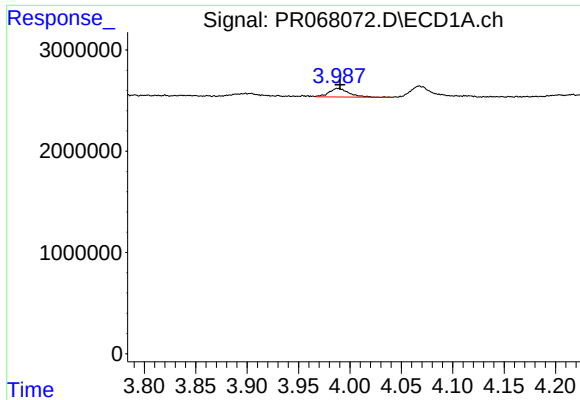

#9 AR-1221-2


R.T.: 3.989 min
Delta R.T.: -0.002 min
Response: 1154176
Conc: 51.36 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

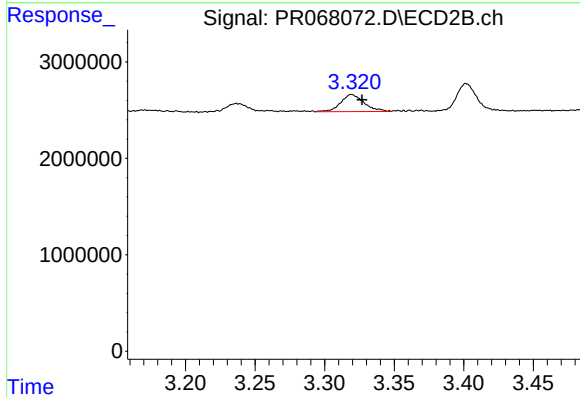


#9 AR-1221-2

R.T.: 3.319 min
Delta R.T.: -0.008 min
Response: 2086865
Conc: 28.41 ng/ml

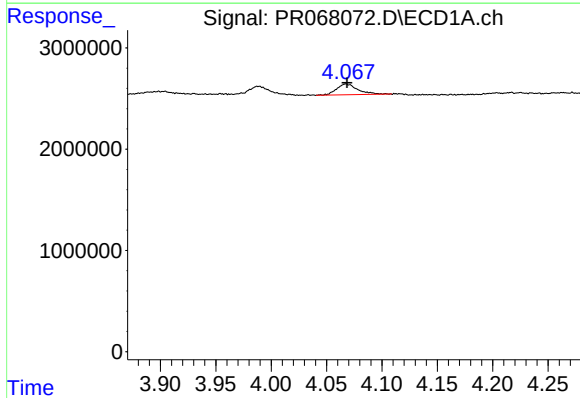


#10 AR-1221-3

R.T.: 4.068 min
Delta R.T.: -0.001 min
Response: 1421908
Conc: 19.90 ng/ml

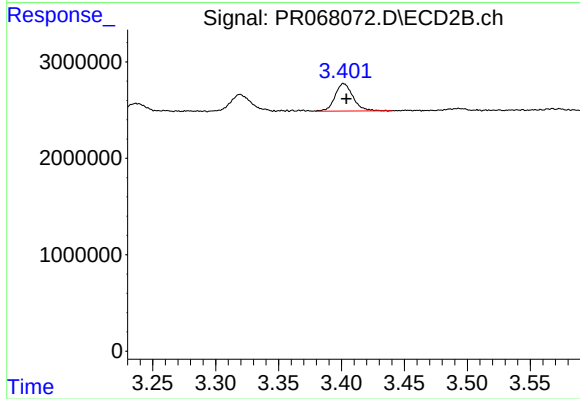

#10 AR-1221-3


R.T.: 3.402 min
Delta R.T.: -0.002 min
Response: 2819199
Conc: 8.70 ng/ml

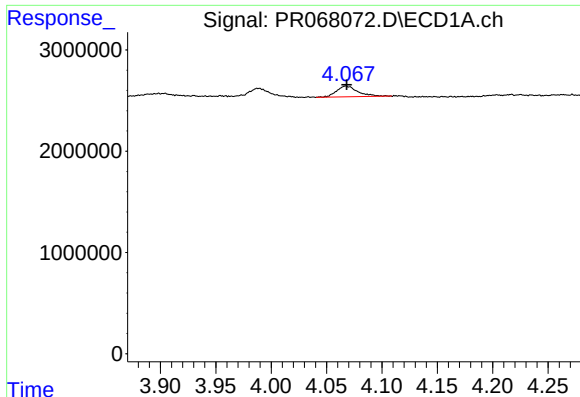

#11 AR-1232-1


R.T.: 4.068 min
Delta R.T.: 0.000 min
Response: 1421908
Conc: 24.16 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

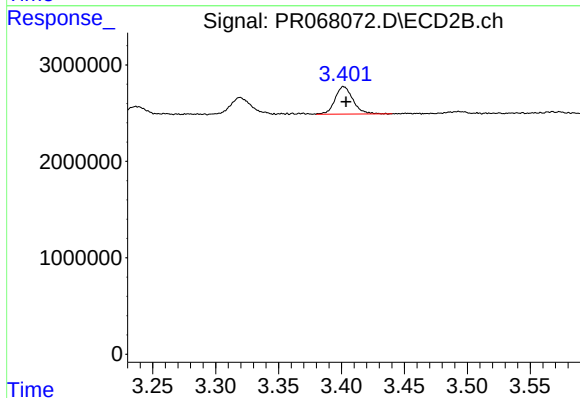


#11 AR-1232-1

R.T.: 3.402 min
Delta R.T.: -0.002 min
Response: 2819199
Conc: 27.83 ng/ml

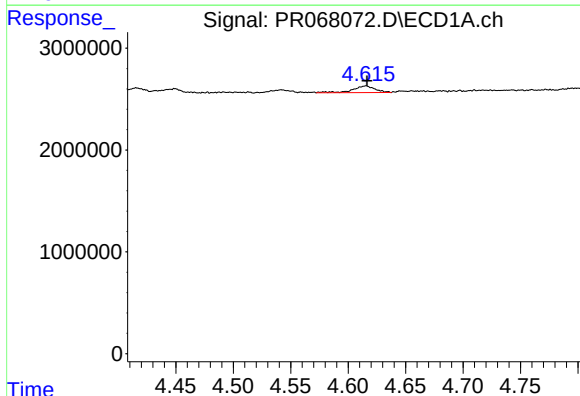


#12 AR-1232-2

R.T.: 4.615 min
Delta R.T.: -0.001 min
Response: 887021
Conc: 28.24 ng/ml

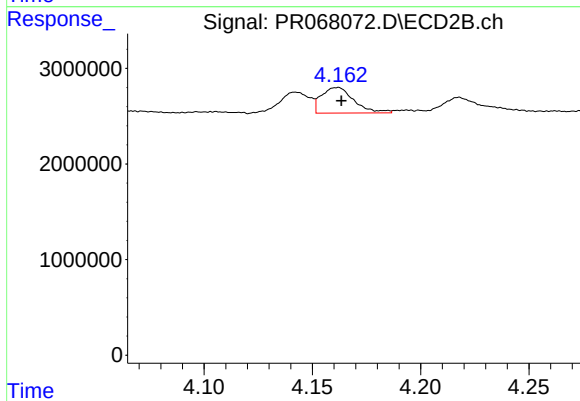

#12 AR-1232-2


R.T.: 4.161 min
Delta R.T.: -0.002 min
Response: 2803503
Conc: 27.82 ng/ml

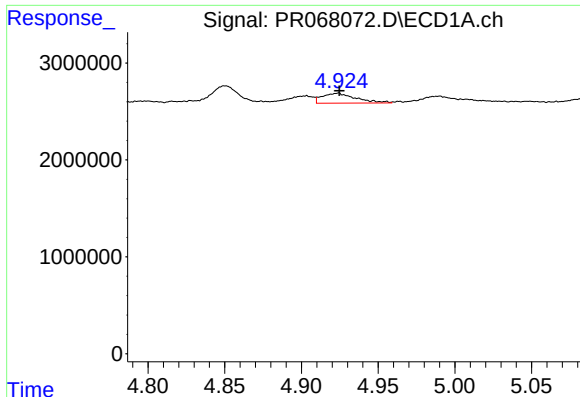

#13 AR-1232-3


R.T.: 4.924 min
Delta R.T.: -0.001 min
Response: 1569075
Conc: 29.11 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

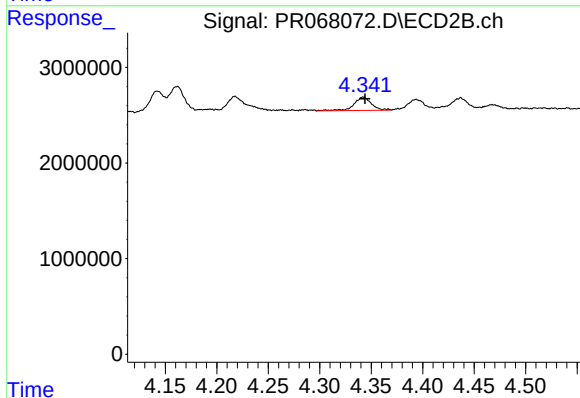


#13 AR-1232-3

R.T.: 4.342 min
Delta R.T.: -0.002 min
Response: 1647899
Conc: 30.34 ng/ml

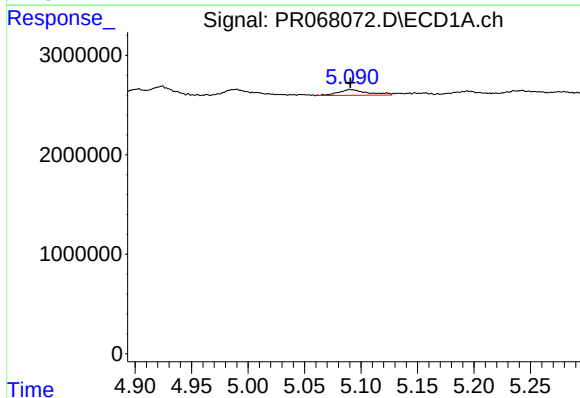


#14 AR-1232-4

R.T.: 5.091 min
Delta R.T.: 0.000 min
Response: 1021324
Conc: 34.16 ng/ml

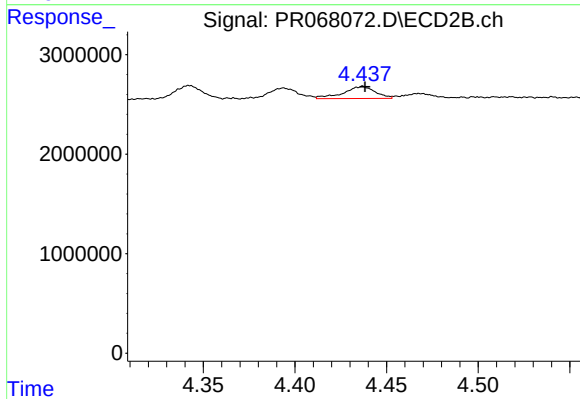

#14 AR-1232-4


R.T.: 4.437 min
Delta R.T.: -0.001 min
Response: 1472623
Conc: 29.47 ng/ml

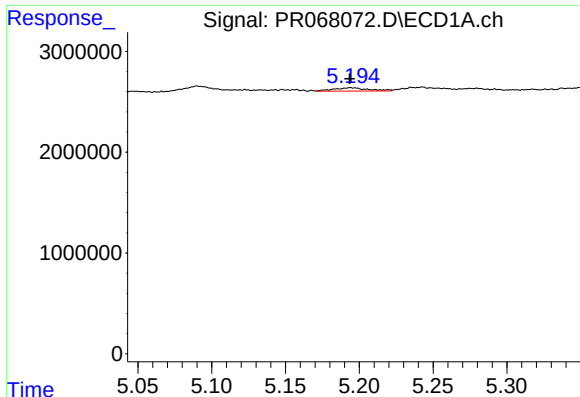

#15 AR-1232-5


R.T.: 5.194 min
Delta R.T.: 0.000 min
Response: 537833
Conc: 34.92 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

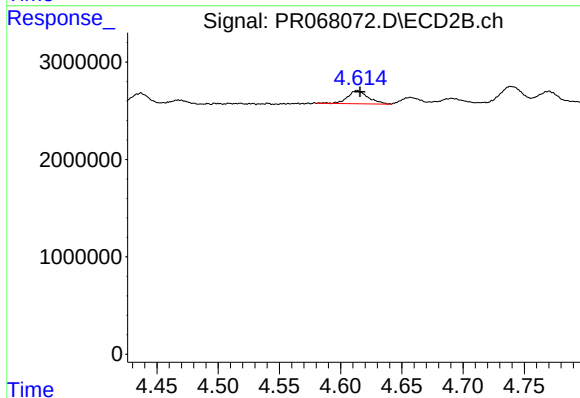


#15 AR-1232-5

R.T.: 4.613 min
Delta R.T.: -0.002 min
Response: 1584165
Conc: 29.79 ng/ml

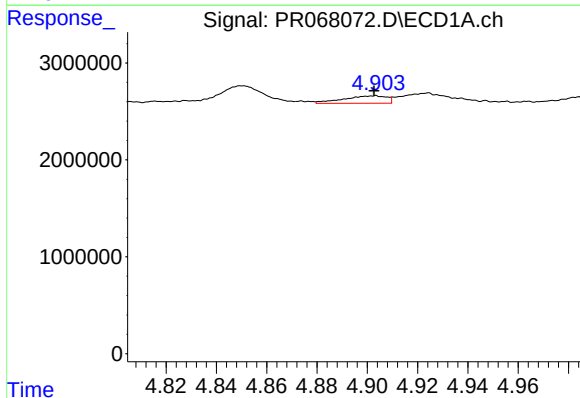


#16 AR-1242-1

R.T.: 4.903 min
Delta R.T.: 0.000 min
Response: 919532
Conc: 18.80 ng/ml

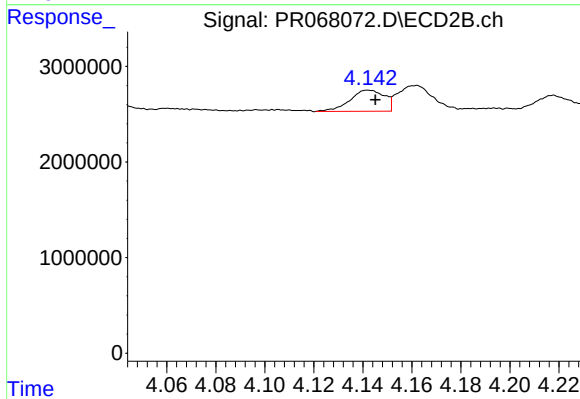

#16 AR-1242-1


R.T.: 4.142 min
Delta R.T.: -0.003 min
Response: 2171887
Conc: 14.25 ng/ml

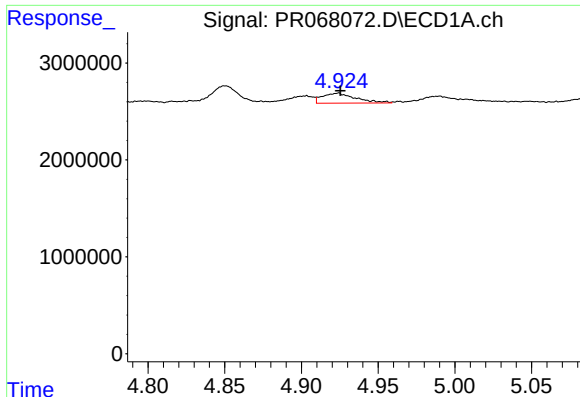

#17 AR-1242-2


R.T.: 4.924 min
Delta R.T.: -0.002 min
Response: 1569075
Conc: 17.27 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

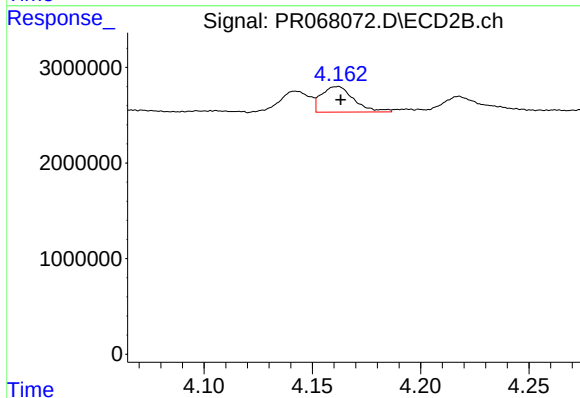


#17 AR-1242-2

R.T.: 4.161 min
Delta R.T.: -0.002 min
Response: 2803503
Conc: 13.11 ng/ml

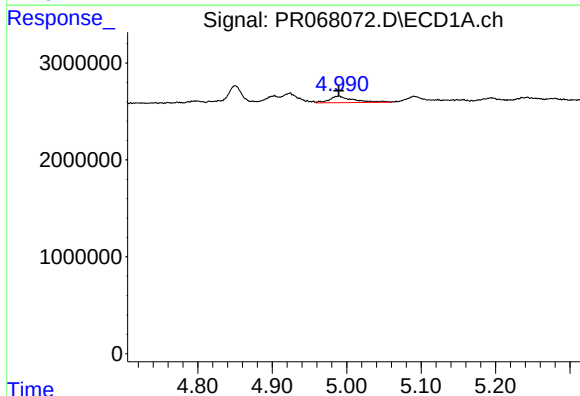


#18 AR-1242-3

R.T.: 4.990 min
Delta R.T.: 0.000 min
Response: 1482624
Conc: 23.62 ng/ml

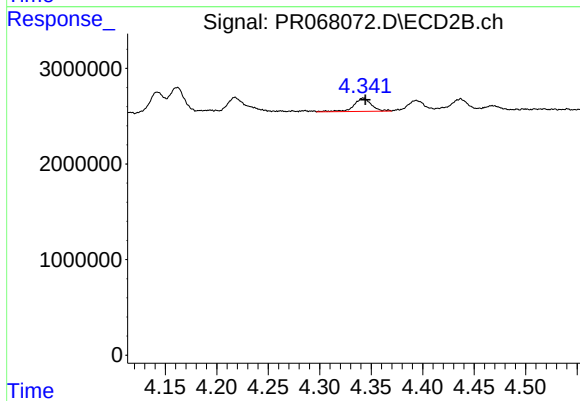

#18 AR-1242-3


R.T.: 4.342 min
Delta R.T.: -0.002 min
Response: 1647899
Conc: 15.51 ng/ml

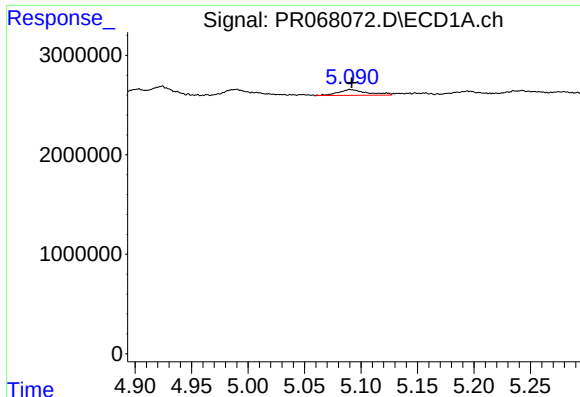

#19 AR-1242-4


R.T.: 5.091 min
Delta R.T.: -0.001 min
Response: 1021324
Conc: 20.46 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

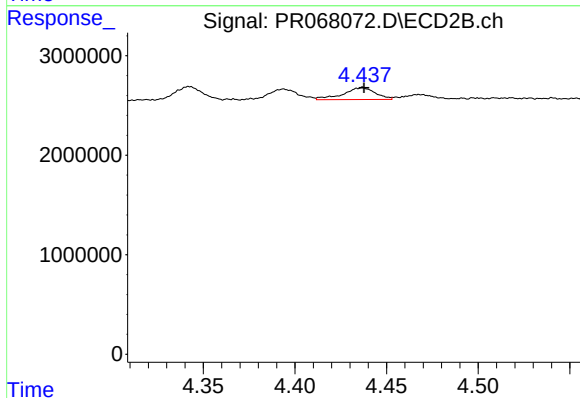


#19 AR-1242-4

R.T.: 4.437 min
Delta R.T.: 0.000 min
Response: 1472623
Conc: 14.64 ng/ml

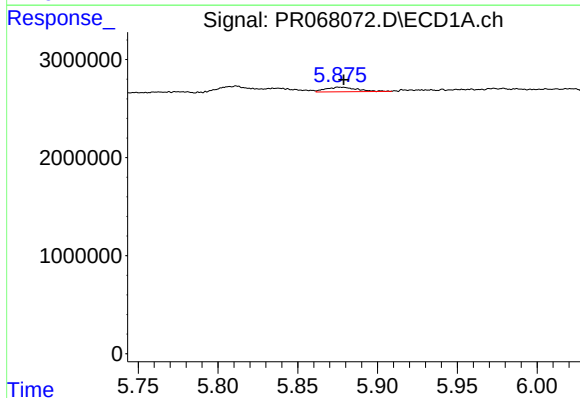


#20 AR-1242-5

R.T.: 5.877 min
Delta R.T.: -0.002 min
Response: 620347
Conc: 13.49 ng/ml

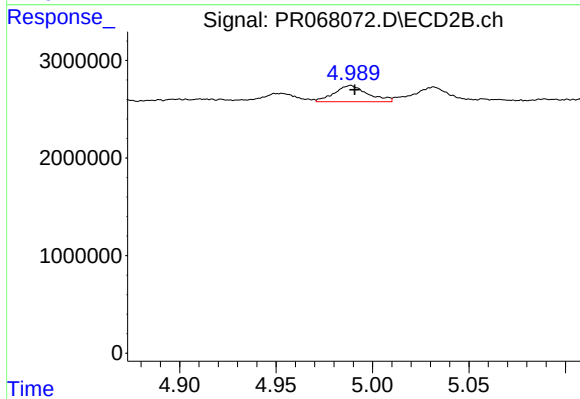

#20 AR-1242-5


R.T.: 4.989 min
Delta R.T.: -0.002 min
Response: 2006427
Conc: 12.79 ng/ml

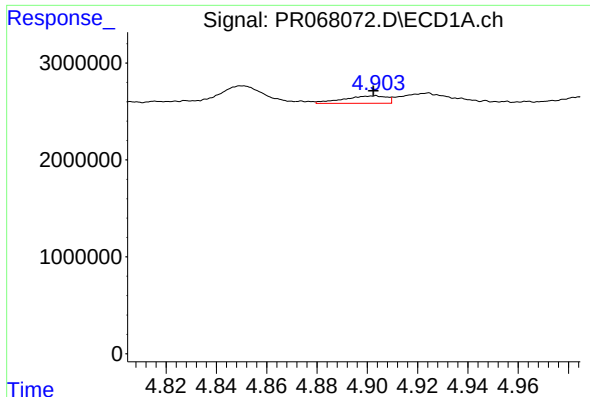

#21 AR-1248-1


R.T.: 4.903 min
Delta R.T.: 0.000 min
Response: 919532
Conc: 23.96 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

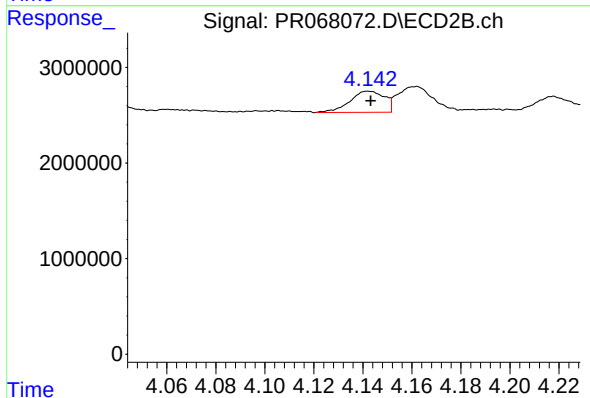


#21 AR-1248-1

R.T.: 4.142 min
Delta R.T.: 0.000 min
Response: 2171887
Conc: 18.25 ng/ml

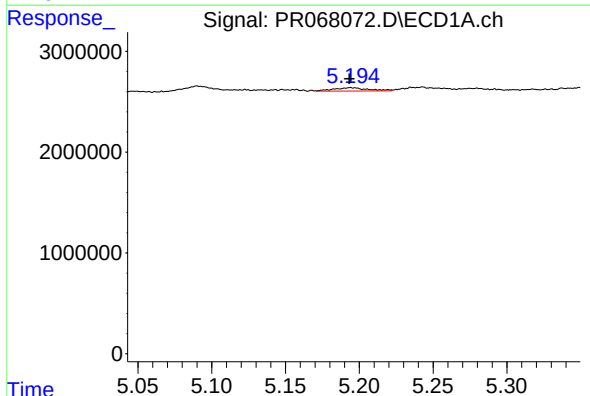


#22 AR-1248-2

R.T.: 5.194 min
Delta R.T.: 0.001 min
Response: 537833
Conc: 10.25 ng/ml

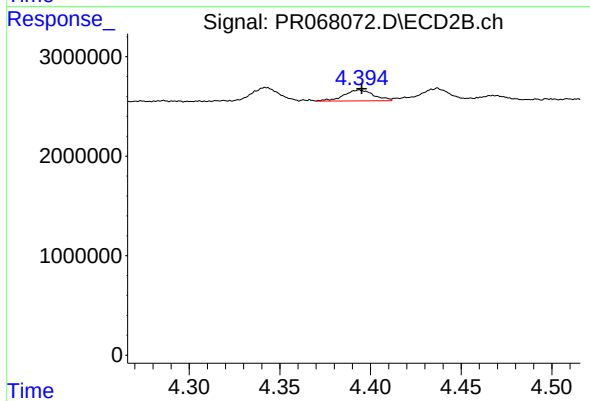

#22 AR-1248-2


R.T.: 4.394 min
Delta R.T.: -0.001 min
Response: 1261727
Conc: 6.69 ng/ml

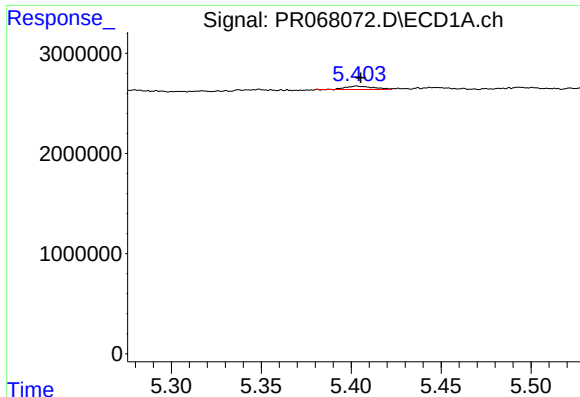

#23 AR-1248-3


R.T.: 5.403 min
Delta R.T.: -0.002 min
Response: 371395
Conc: 5.27 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

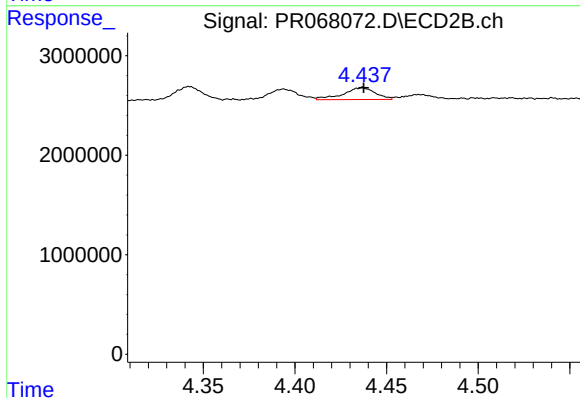


#23 AR-1248-3

R.T.: 4.437 min
Delta R.T.: 0.000 min
Response: 1472623
Conc: 7.73 ng/ml

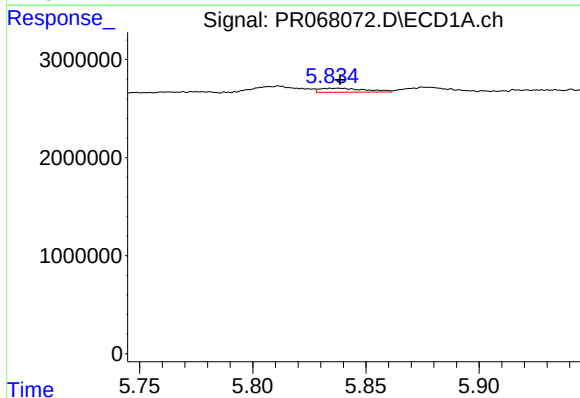


#24 AR-1248-4

R.T.: 5.838 min
Delta R.T.: -0.001 min
Response: 575990
Conc: 7.75 ng/ml

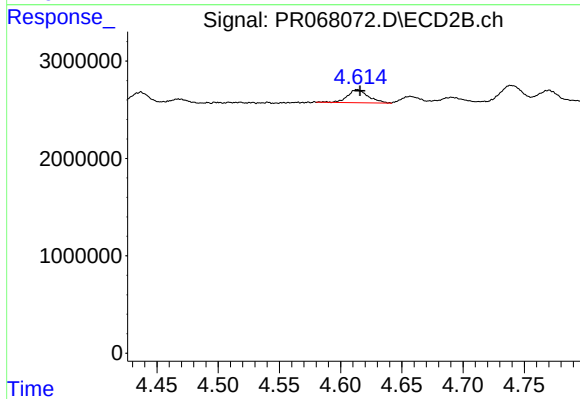

#24 AR-1248-4


R.T.: 4.613 min
Delta R.T.: -0.002 min
Response: 1584165
Conc: 7.34 ng/ml

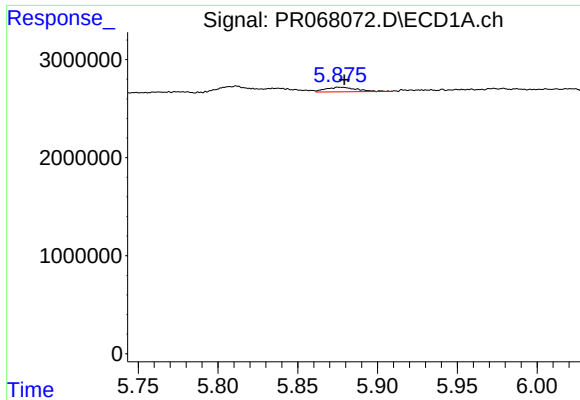

#25 AR-1248-5


R.T.: 5.877 min
Delta R.T.: -0.003 min
Response: 620347
Conc: 7.68 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

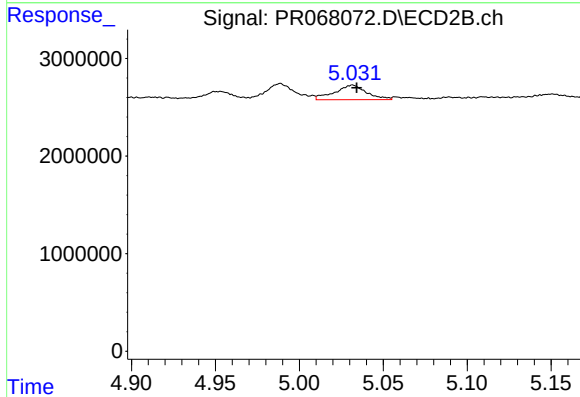


#25 AR-1248-5

R.T.: 5.032 min
Delta R.T.: -0.002 min
Response: 1968298
Conc: 9.26 ng/ml

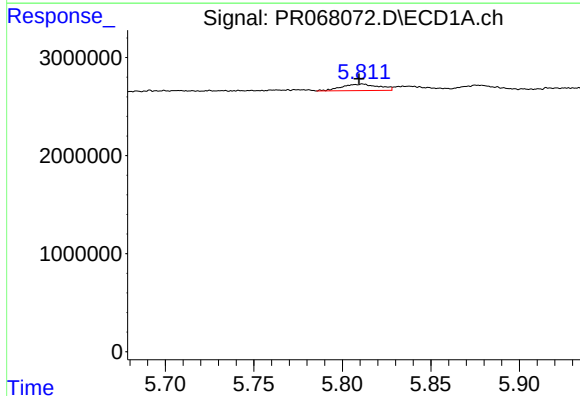


#26 AR-1254-1

R.T.: 5.812 min
Delta R.T.: 0.002 min
Response: 974341
Conc: 13.65 ng/ml

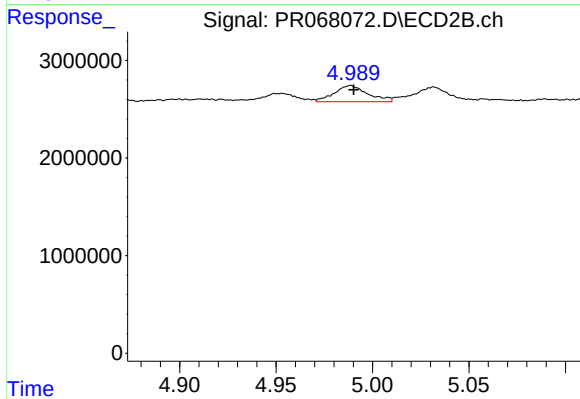

#26 AR-1254-1


R.T.: 4.989 min
Delta R.T.: -0.002 min
Response: 2006427
Conc: 7.85 ng/ml

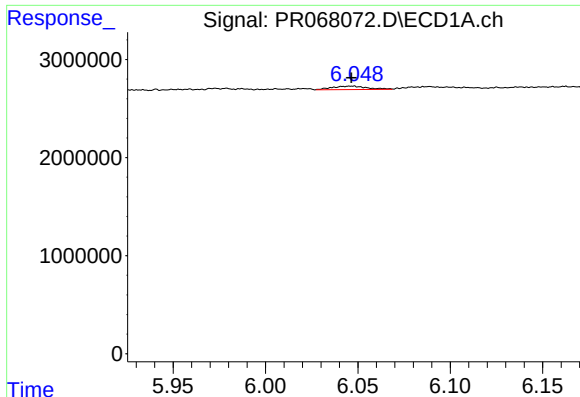

#27 AR-1254-2


R.T.: 6.047 min
Delta R.T.: 0.000 min
Response: 458403
Conc: 4.08 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

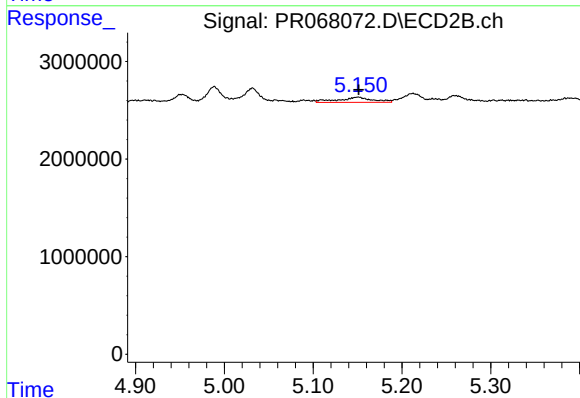


#27 AR-1254-2

R.T.: 5.151 min
Delta R.T.: 0.000 min
Response: 1419359
Conc: 6.17 ng/ml

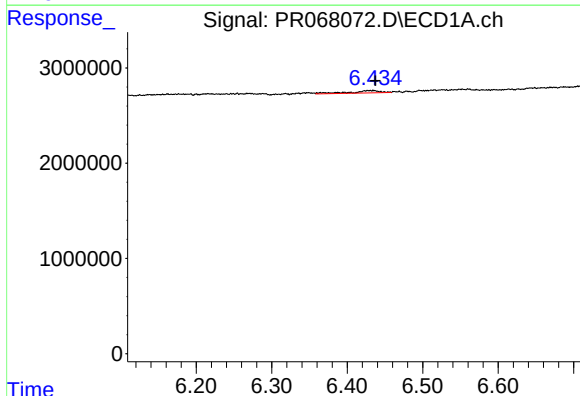


#28 AR-1254-3

R.T.: 6.431 min
Delta R.T.: -0.006 min
Response: 654374
Conc: 4.87 ng/ml

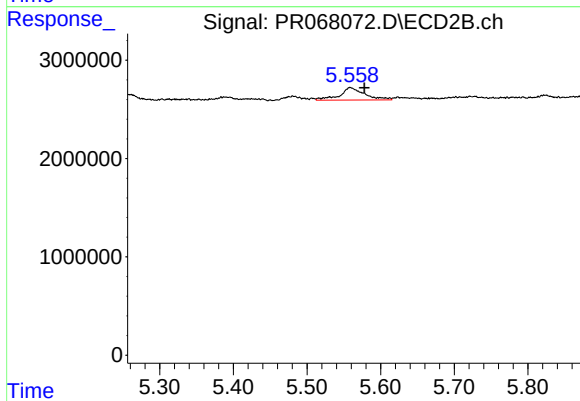

#28 AR-1254-3


R.T.: 5.559 min
Delta R.T.: -0.019 min
Response: 2975136
Conc: 8.25 ng/ml

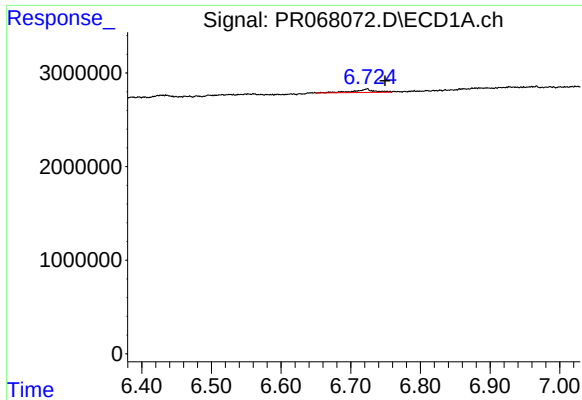

#29 AR-1254-4


R.T.: 6.723 min
Delta R.T.: -0.026 min
Response: 759498
Conc: 7.27 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

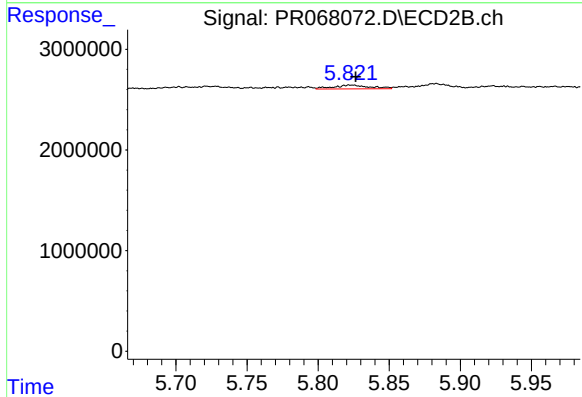


#29 AR-1254-4

R.T.: 5.823 min
Delta R.T.: -0.003 min
Response: 671635
Conc: 3.13 ng/ml

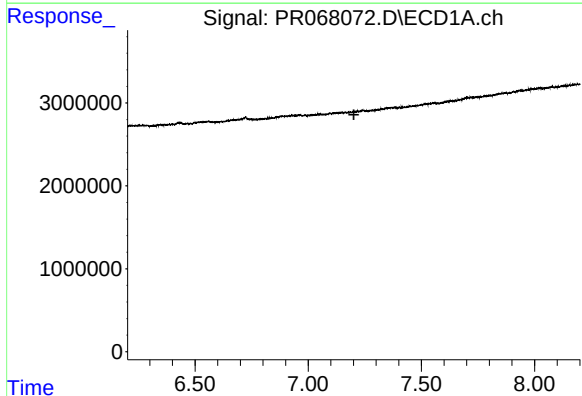


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.202 min
Response: 0
Conc: N.D.

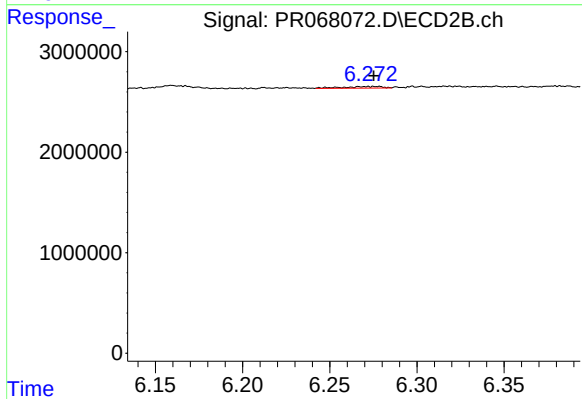

#30 AR-1254-5


R.T.: 6.272 min
Delta R.T.: -0.003 min
Response: 264001
Conc: 0.80 ng/ml

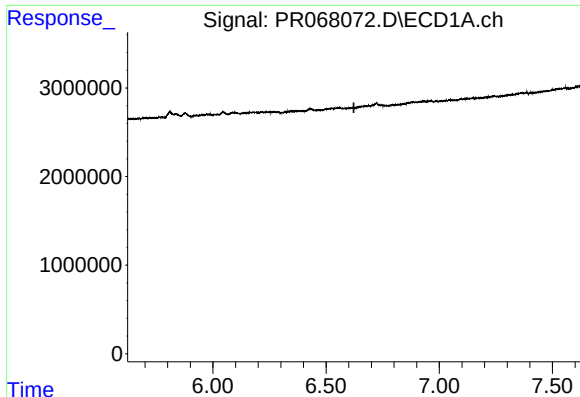

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T.: 6.623 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

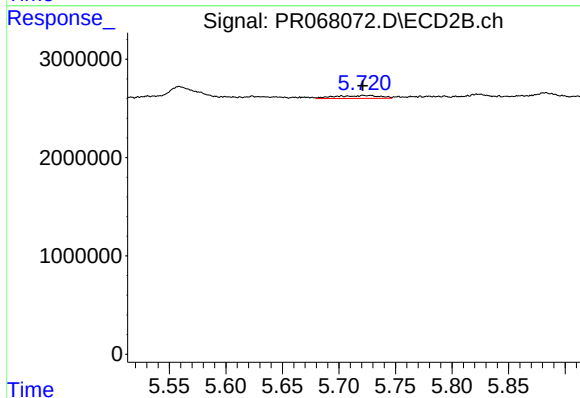


#31 AR-1260-1

R.T.: 5.728 min
Delta R.T.: 0.007 min
Response: 811956
Conc: 3.32 ng/ml

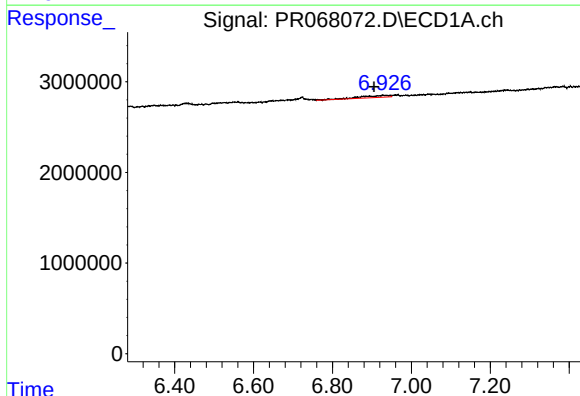


#32 AR-1260-2

R.T.: 6.929 min
Delta R.T.: 0.023 min
Response: 1102507
Conc: 7.76 ng/ml

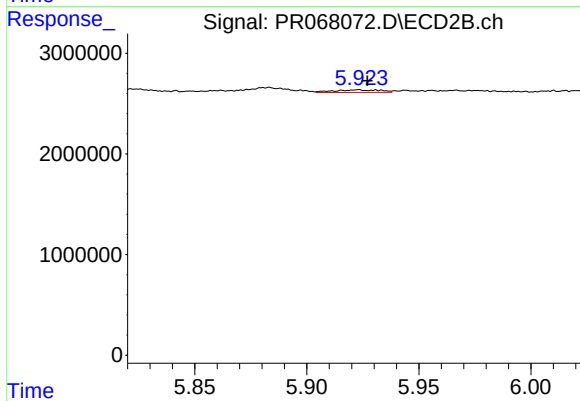

#32 AR-1260-2


R.T.: 5.923 min
Delta R.T.: -0.004 min
Response: 360497
Conc: 1.24 ng/ml

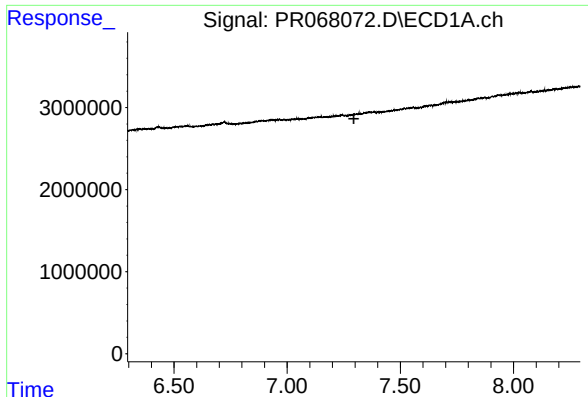

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 7.295 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

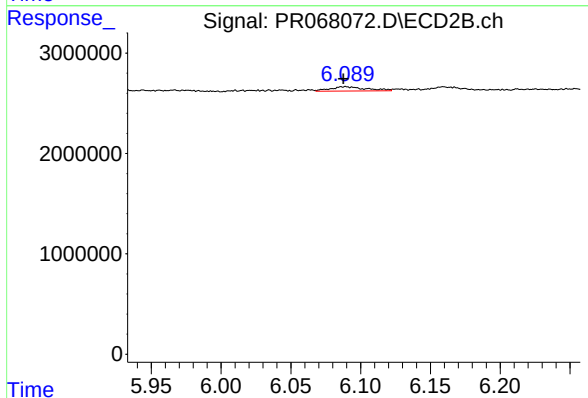


#33 AR-1260-3

R.T.: 6.089 min
Delta R.T.: 0.001 min
Response: 789415
Conc: 2.87 ng/ml

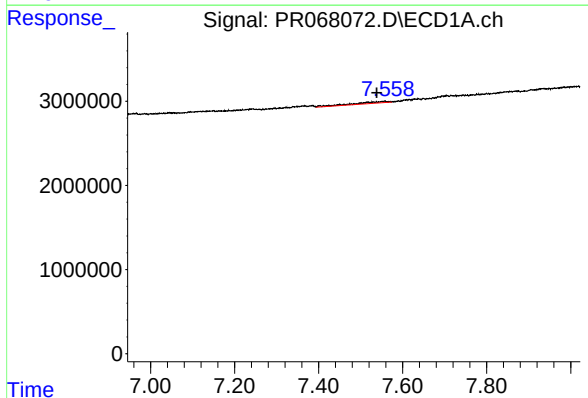


#34 AR-1260-4

R.T.: 7.557 min
Delta R.T.: 0.019 min
Response: 1050488
Conc: 8.29 ng/ml

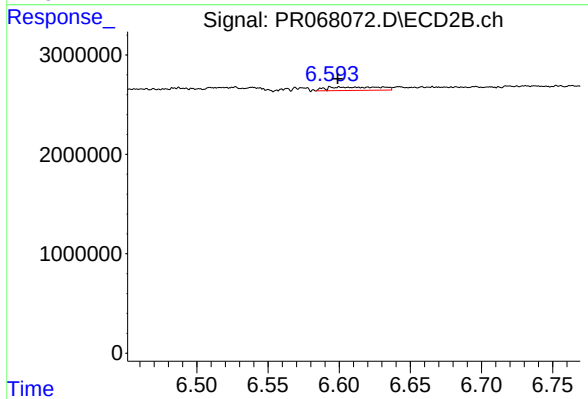

#34 AR-1260-4


R.T.: 6.601 min
Delta R.T.: 0.002 min
Response: 921951
Conc: 4.40 ng/ml

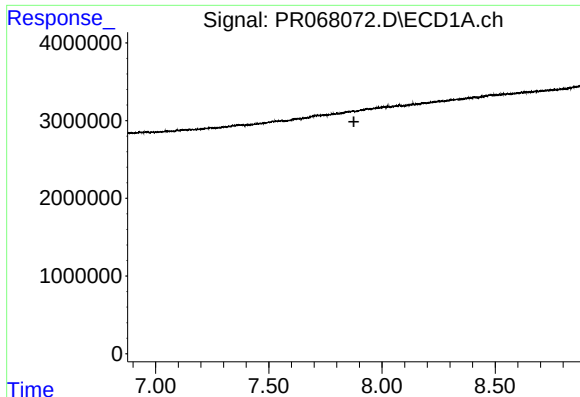

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 7.876 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

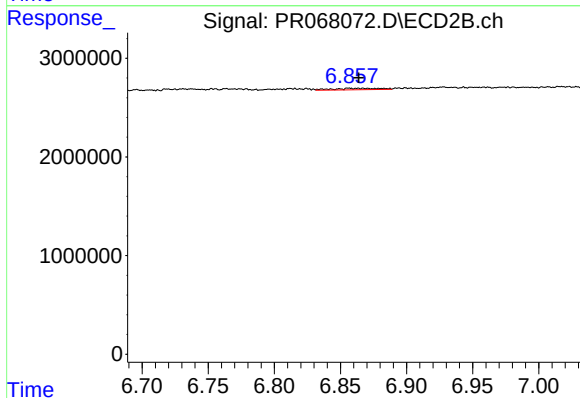


#35 AR-1260-5

R.T.: 6.868 min
Delta R.T.: 0.004 min
Response: 365605
Conc: 0.76 ng/ml

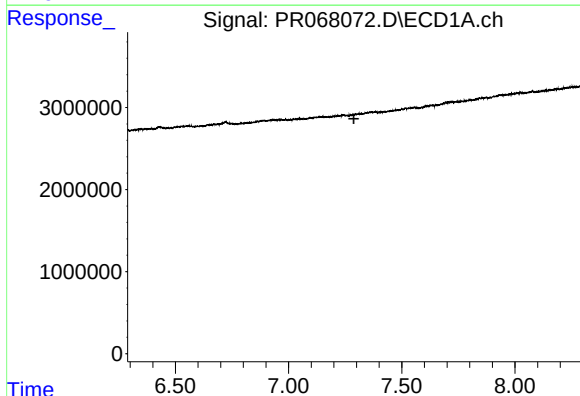


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 7.289 min
Response: 0
Conc: N.D.

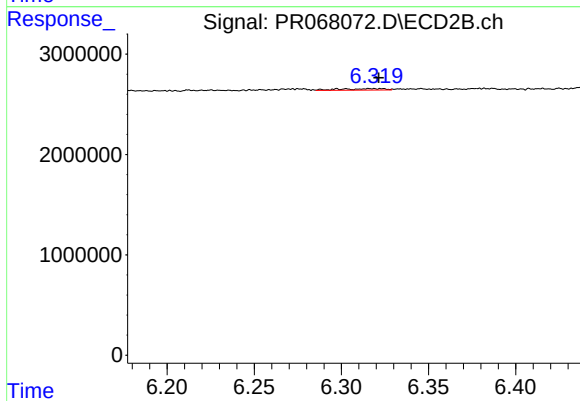

#36 AR-1262-1


R.T.: 6.297 min
Delta R.T.: -0.024 min
Response: 274262
Conc: 0.79 ng/ml

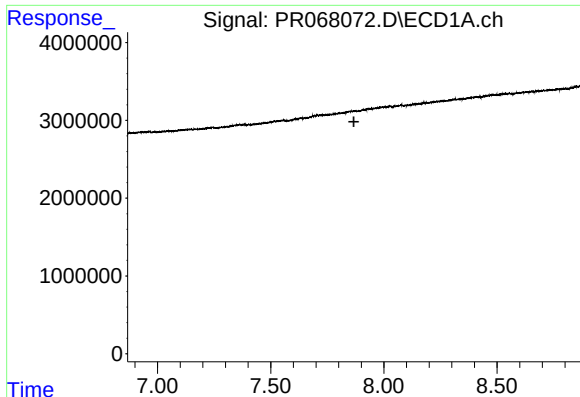

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 7.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

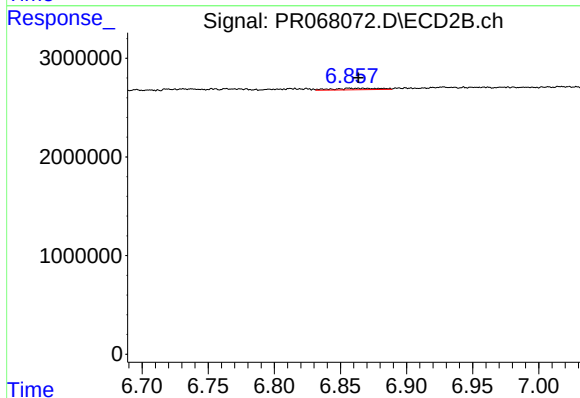


#37 AR-1262-2

R.T.: 6.868 min
Delta R.T.: 0.004 min
Response: 365605
Conc: 0.60 ng/ml

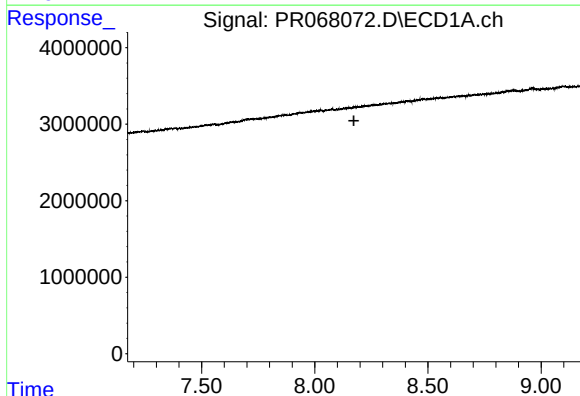


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T.: 8.173 min
Response: 0
Conc: N.D.

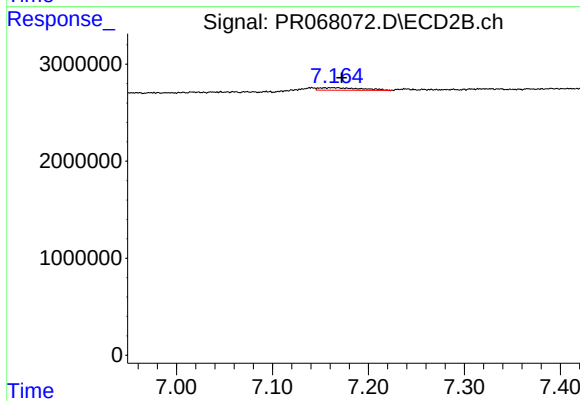

#38 AR-1262-3


R.T.: 7.168 min
Delta R.T.: -0.004 min
Response: 781048
Conc: 3.27 ng/ml

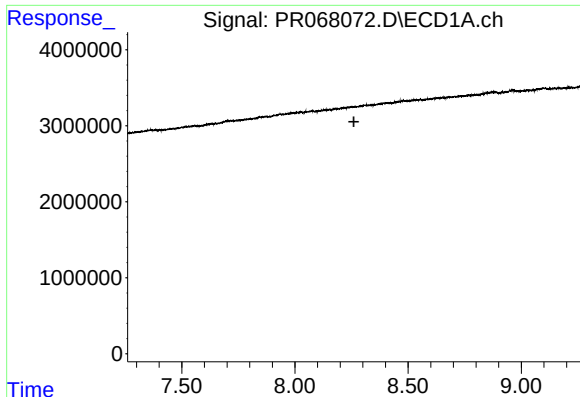

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 8.261 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

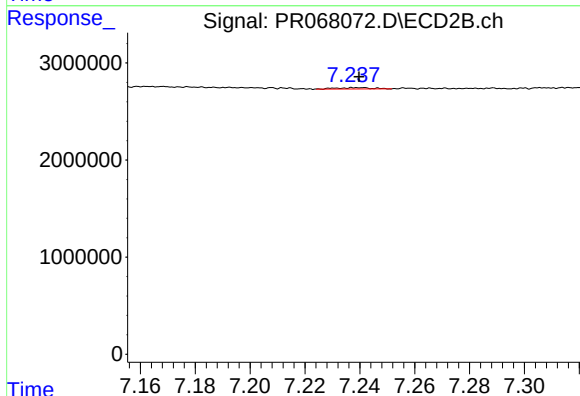


#39 AR-1262-4

R.T.: 7.239 min
Delta R.T.: 0.000 min
Response: 122608
Conc: 0.28 ng/ml

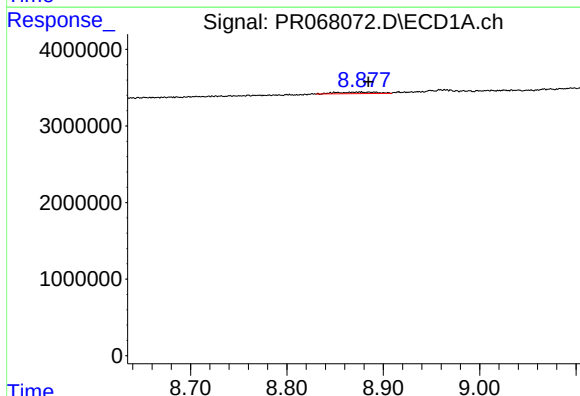


#40 AR-1262-5

R.T.: 8.875 min
Delta R.T.: -0.009 min
Response: 608420
Conc: 3.21 ng/ml

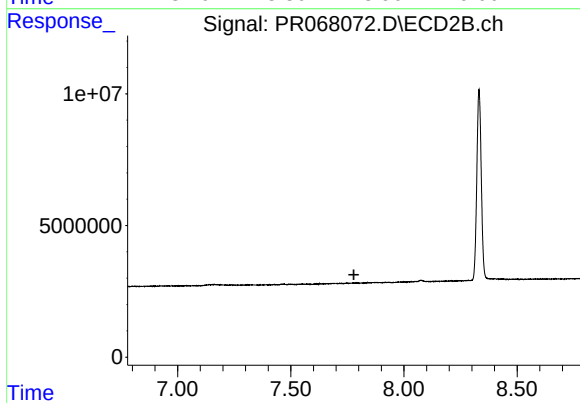

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T.: 7.779 min
Response: 0
Conc: N.D.

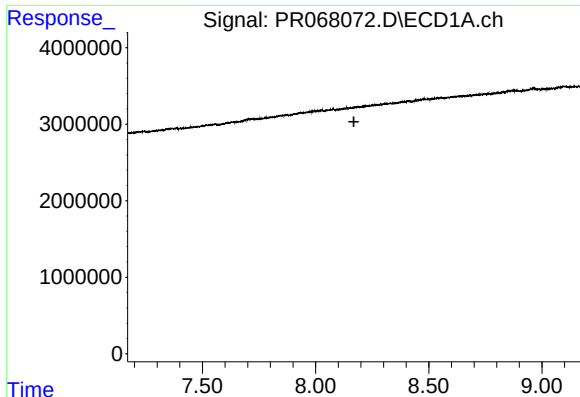

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 8.169 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

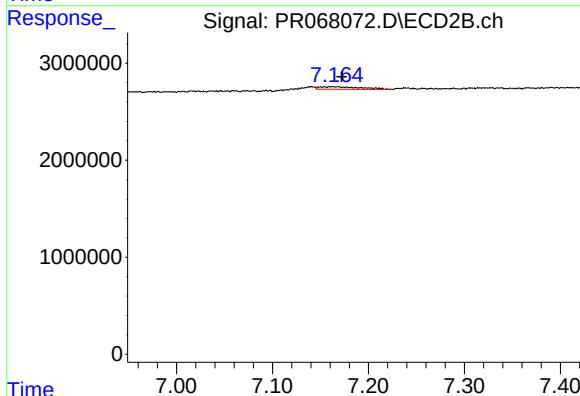


#41 AR-1268-1

R.T.: 7.168 min
Delta R.T.: -0.004 min
Response: 781048
Conc: 1.06 ng/ml

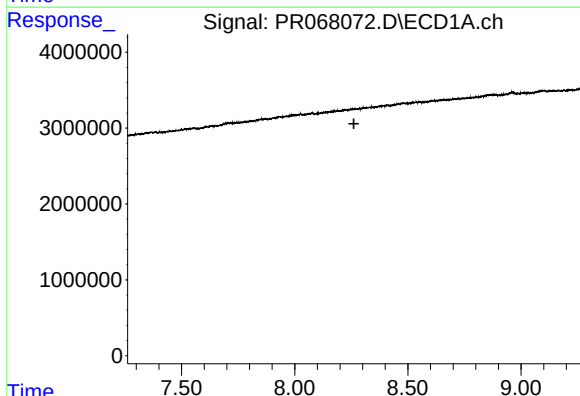


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 8.261 min
Response: 0
Conc: N.D.

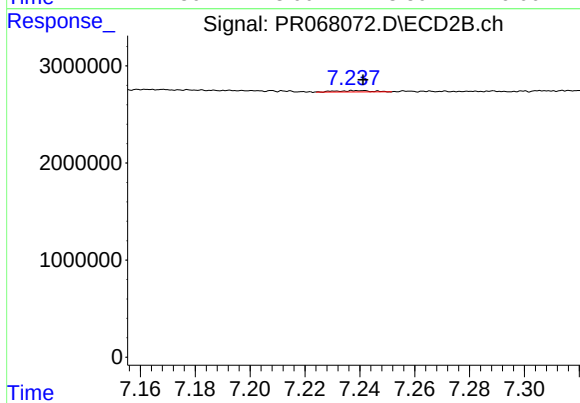

#42 AR-1268-2


R.T.: 7.239 min
Delta R.T.: -0.002 min
Response: 122608
Conc: 0.18 ng/ml

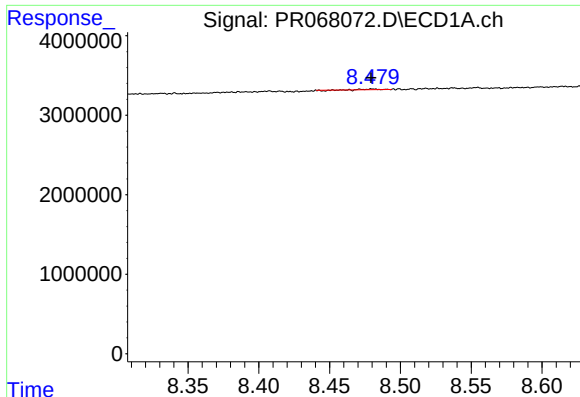

#43 AR-1268-3


R.T.: 8.481 min
Delta R.T.: 0.001 min
Response: 45895
Conc: 0.08 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

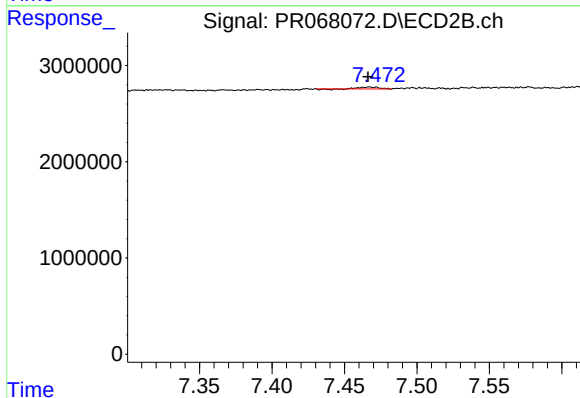


#43 AR-1268-3

R.T.: 7.471 min
Delta R.T.: 0.005 min
Response: 132827
Conc: 0.22 ng/ml

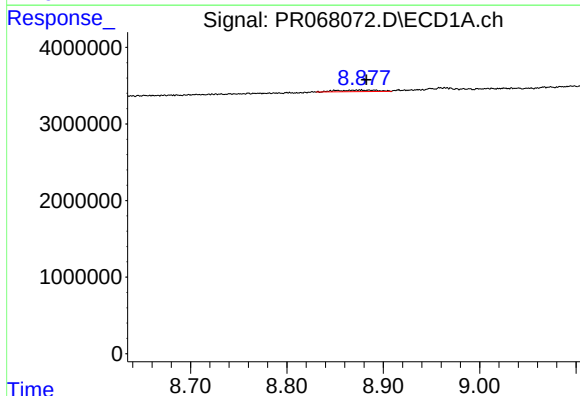


#44 AR-1268-4

R.T.: 8.875 min
Delta R.T.: -0.007 min
Response: 608420
Conc: 3.00 ng/ml

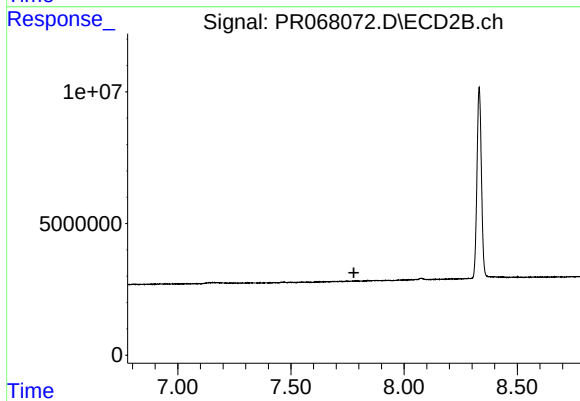

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T. : 7.778 min
Response: 0
Conc: N.D.

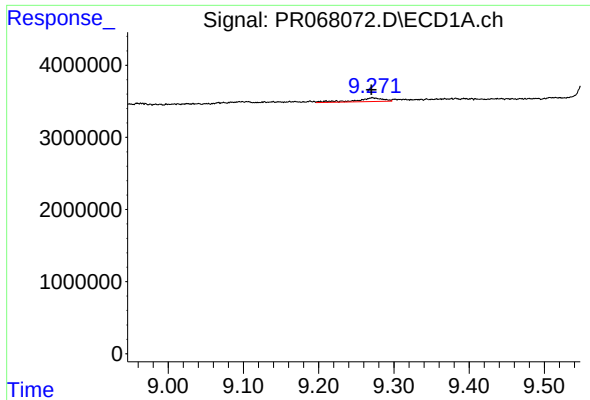

#45 AR-1268-5

R.T.: 9.272 min
Delta R.T.: 0.002 min
Response: 1262726
Conc: 0.81 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

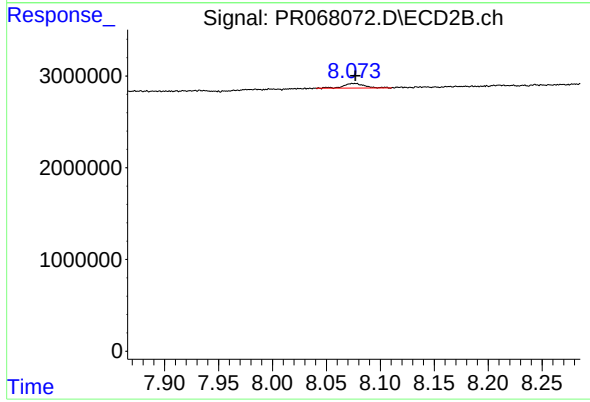

#45 AR-1268-5

R.T.: 8.075 min
Delta R.T.: -0.002 min
Response: 693265
Conc: 0.49 ng/ml