

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR080724\
 Data File : PR068076.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Aug 2024 12:04
 Operator : AJ\MA
 Sample : P3390-09
 Misc : AR1262 MDL 25 PPB
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 07 17:13:03 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 07 00:26:28 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.677	3.011	34732553	67348893	13.653	15.445
2)	SA Decachlor...	9.582	8.331	64087164	74628541	14.605	16.470
Target Compounds							
3)	L1 AR-1016-1	4.903	4.165f	94629	433682	1.619	2.886 #
4)	L1 AR-1016-2	4.920	4.165	234139	433682	2.112	2.067
5)	L1 AR-1016-3	5.013f	4.338	240161	214928	3.127	1.884 #
6)	L1 AR-1016-4	0.000	4.395	0	371331	N.D.	3.883 #
9)	L2 AR-1221-2	3.989	3.318	669029	987590	29.773	13.447 #
10)	L2 AR-1221-3	4.081	0.000	317991	0	4.451	N.D. #
11)	L3 AR-1232-1	4.081	0.000	317991	0	5.404	N.D. #
12)	L3 AR-1232-2	4.615	4.165	153839	433682	4.898	4.304
13)	L3 AR-1232-3	4.920	4.338	234139	214928	4.343	3.958
14)	L3 AR-1232-4	0.000	4.435	0	379862	N.D.	7.602 #
15)	L3 AR-1232-5	5.189	0.000	211679	0	13.744	N.D. #
16)	L4 AR-1242-1	4.903	4.165f	94629	433682	1.934	2.845 #
17)	L4 AR-1242-2	4.920	4.165	234139	433682	2.577	2.028
18)	L4 AR-1242-3	5.013f	4.338	240161	214928	3.827	2.023 #
19)	L4 AR-1242-4	0.000	4.435	0	379862	N.D.	3.777 #
20)	L4 AR-1242-5	0.000	4.989	0	1152327	N.D.	7.348 #
21)	L5 AR-1248-1	4.903	4.165f	94629	433682	2.466	3.644 #
22)	L5 AR-1248-2	5.189	4.395	211679	371331	4.035	1.970 #
23)	L5 AR-1248-3	0.000	4.435	0	379862	N.D.	1.993 #
24)	L5 AR-1248-4	5.848	0.000	123646	0	1.663	N.D. #
25)	L5 AR-1248-5	0.000	5.032	0	210258	N.D.	0.989 #
26)	L6 AR-1254-1	5.808	4.989	2286349	1152327	32.037	4.506 #
27)	L6 AR-1254-2	6.045	5.150	437261	1162486	3.896	5.057 #
28)	L6 AR-1254-3	6.429	5.596f	322212	3198238	2.398	8.865 #
29)	L6 AR-1254-4	6.745	5.821	495012	446990	4.736	2.080 #
30)	L6 AR-1254-5	7.198	6.273	2095290	3941542	16.868	11.938 #
31)	L7 AR-1260-1	6.616	5.718	1458398	4944756	15.779	20.197 #
32)	L7 AR-1260-2	6.899	5.924	2322952	5477602	16.345	18.867
33)	L7 AR-1260-3	7.287	6.087	4851188	5832720	35.034	21.239 #
34)	L7 AR-1260-4	7.529	6.595	3592830	6602900	28.347	31.493
35)	L7 AR-1260-5	7.867	6.861	9461816	11788685	25.957	24.354
36)	L8 AR-1262-1	7.287	6.318	4851188	7891243	24.355	22.845
37)	L8 AR-1262-2	7.867	6.861	9461816	11788685	21.850	19.381
38)	L8 AR-1262-3	8.173	7.169	5612209	5352422	17.923	22.416 #
39)	L8 AR-1262-4	8.259	7.237	4996875	9189246	18.198	20.679
40)	L8 AR-1262-5	8.884	7.777	3452326	4193110	18.238	20.586
41)	L9 AR-1268-1	8.173	7.169	5612209	5352422	9.307	7.249
42)	L9 AR-1268-2	8.259	7.237	4996875	9189246	8.768	13.611 #
43)	L9 AR-1268-3	8.482	7.464	472204	606679	0.851	0.984

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR080724\
Data File : PR068076.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Aug 2024 12:04
Operator : AJ\MA
Sample : P3390-09
Misc : AR1262 MDL 25 PPB
ALS Vial : 62 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 17:13:03 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 07 00:26:28 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
44)	L9 AR-1268-4	8.884	7.777	3452326	4193110	17.043	20.107
45)	L9 AR-1268-5	9.266	8.075	4378826	1986682	2.800	1.391 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR080724\
Data File : PR068076.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Aug 2024 12:04
Operator : AJ\MA
Sample : P3390-09
Misc : AR1262 MDL 25 PPB
ALS Vial : 62 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 17:13:03 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 07 00:26:28 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

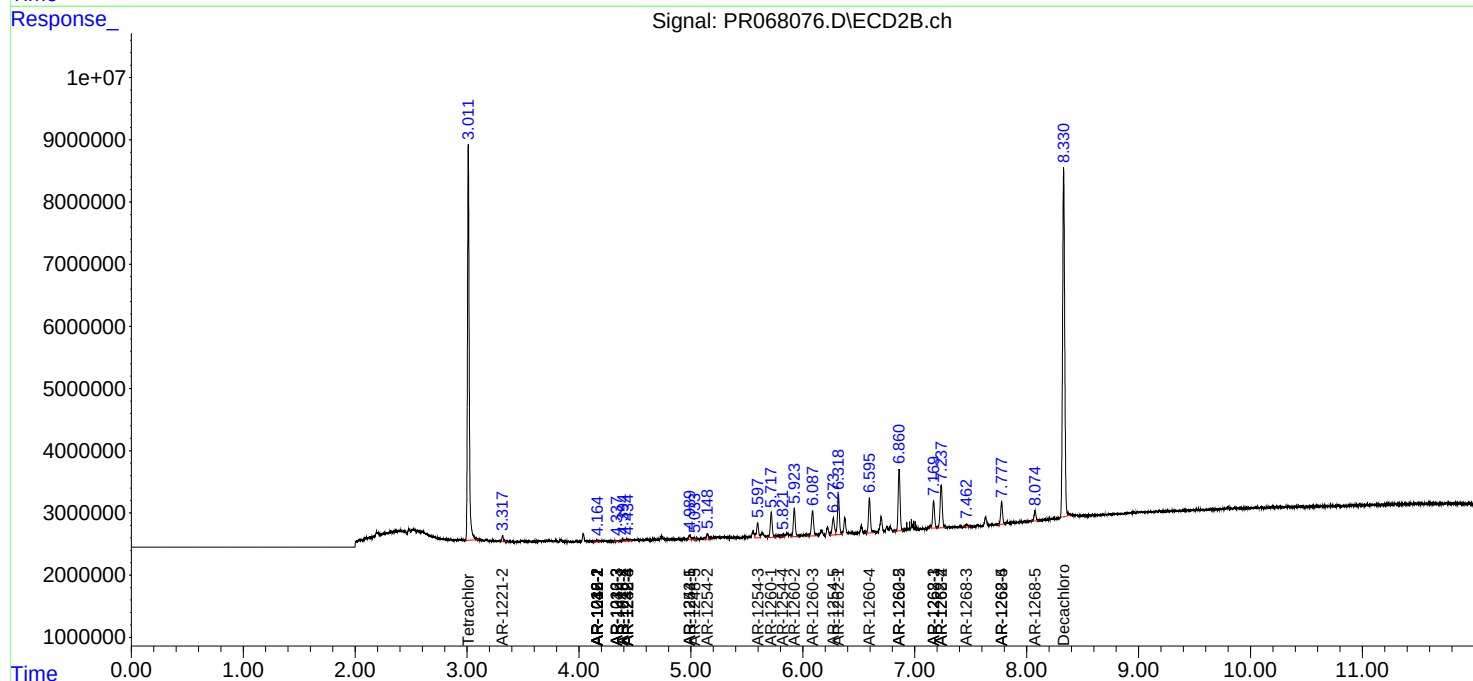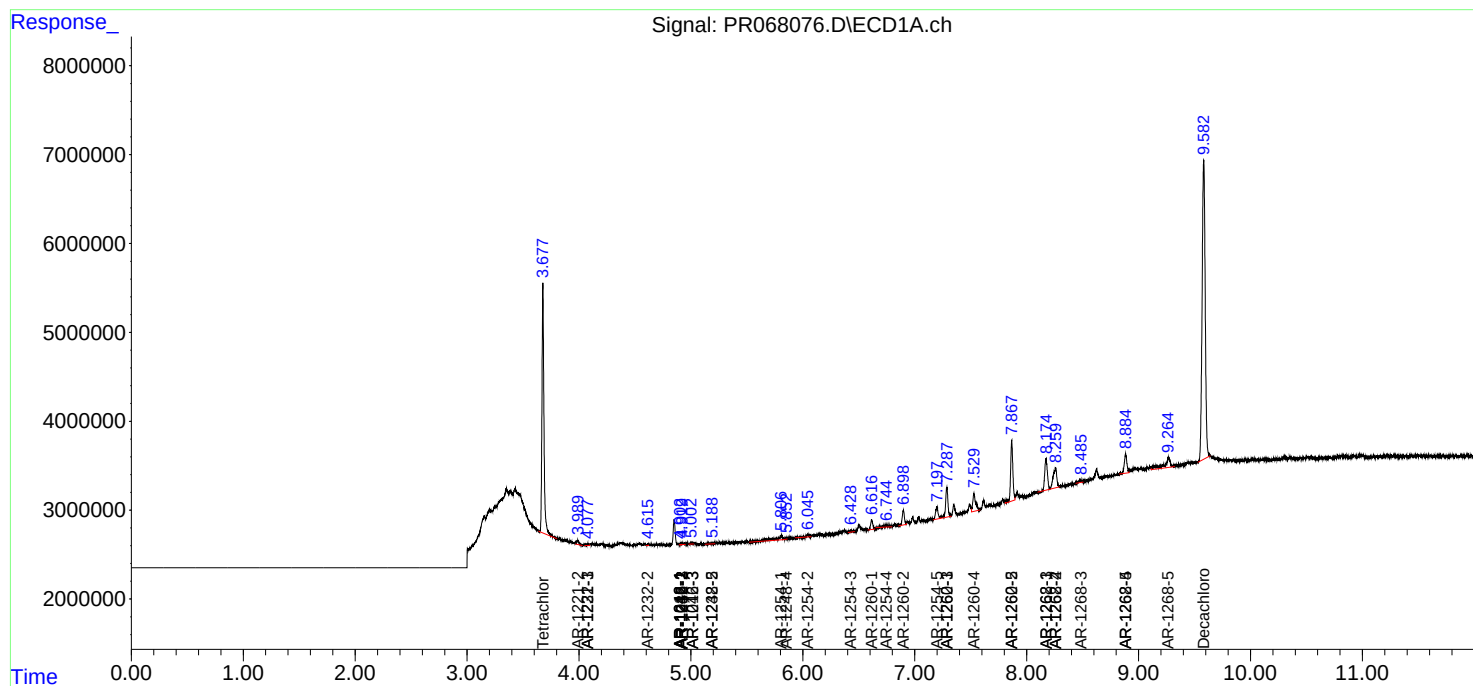


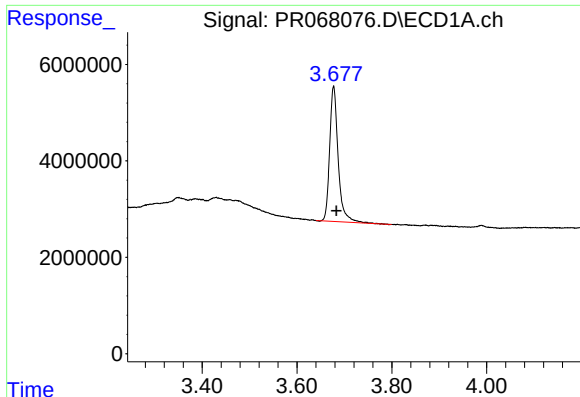

#1 Tetrachloro-m-xylene


R.T.: 3.677 min
Delta R.T.: -0.006 min
Response: 34732553
Conc: 13.65 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

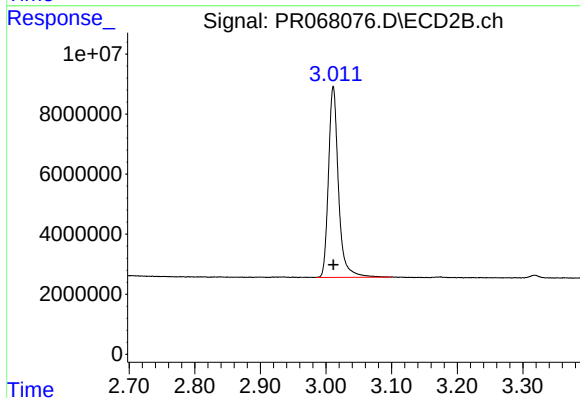


#1 Tetrachloro-m-xylene

R.T.: 3.011 min
Delta R.T.: 0.000 min
Response: 67348893
Conc: 15.44 ng/ml

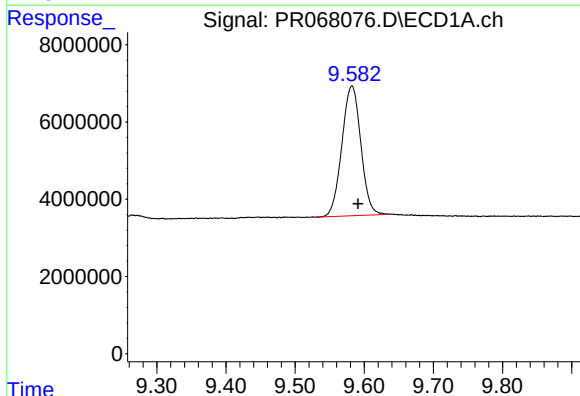


#2 Decachlorobiphenyl

R.T.: 9.582 min
Delta R.T.: -0.009 min
Response: 64087164
Conc: 14.61 ng/ml

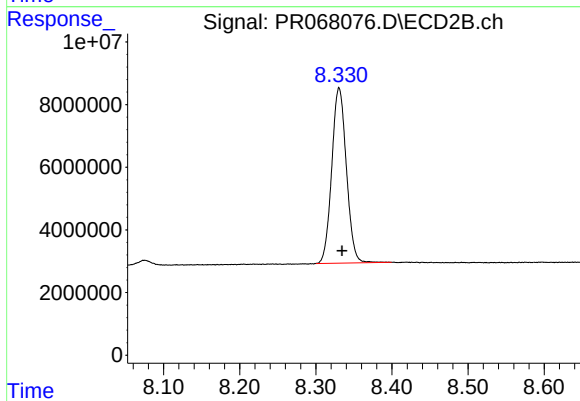

#2 Decachlorobiphenyl


R.T.: 8.331 min
Delta R.T.: -0.004 min
Response: 74628541
Conc: 16.47 ng/ml

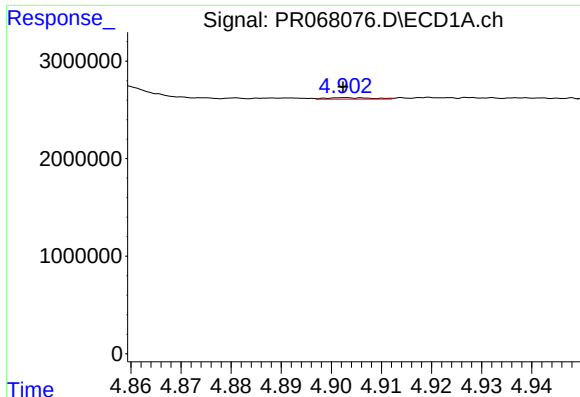

#3 AR-1016-1


R.T.: 4.903 min
Delta R.T.: 0.000 min
Response: 94629
Conc: 1.62 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

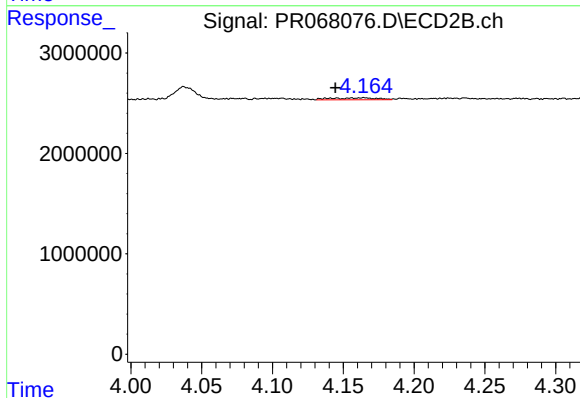


#3 AR-1016-1

R.T.: 4.165 min
Delta R.T.: 0.020 min
Response: 433682
Conc: 2.89 ng/ml

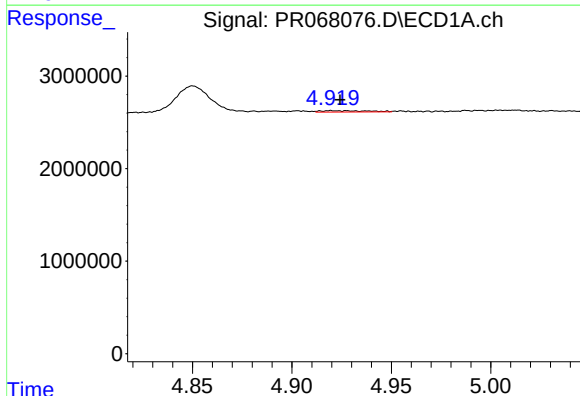


#4 AR-1016-2

R.T.: 4.920 min
Delta R.T.: -0.004 min
Response: 234139
Conc: 2.11 ng/ml

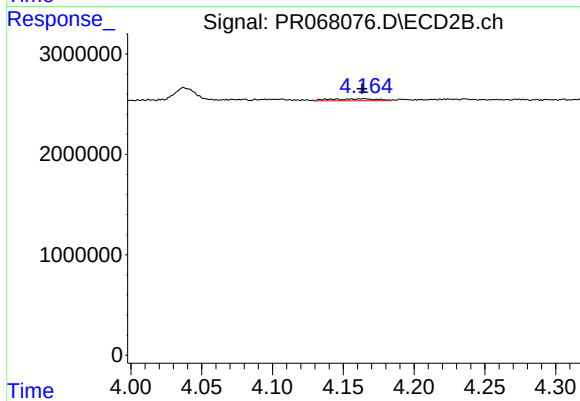

#4 AR-1016-2


R.T.: 4.165 min
Delta R.T.: 0.001 min
Response: 433682
Conc: 2.07 ng/ml

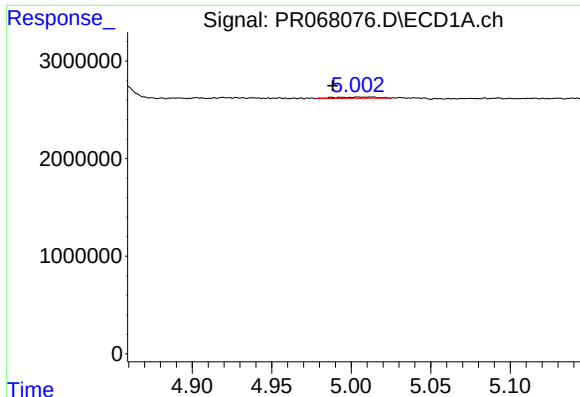

#5 AR-1016-3


R.T.: 5.013 min
Delta R.T.: 0.024 min
Response: 240161
Conc: 3.13 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

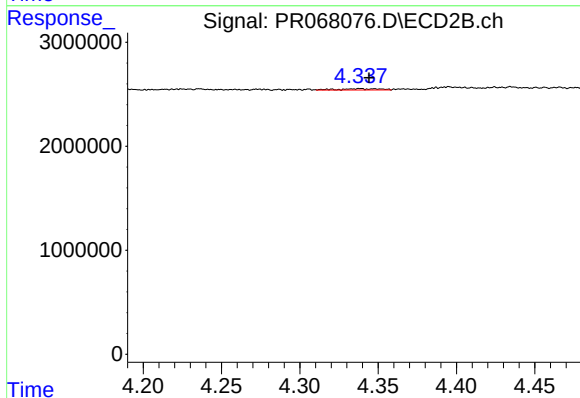


#5 AR-1016-3

R.T.: 4.338 min
Delta R.T.: -0.006 min
Response: 214928
Conc: 1.88 ng/ml

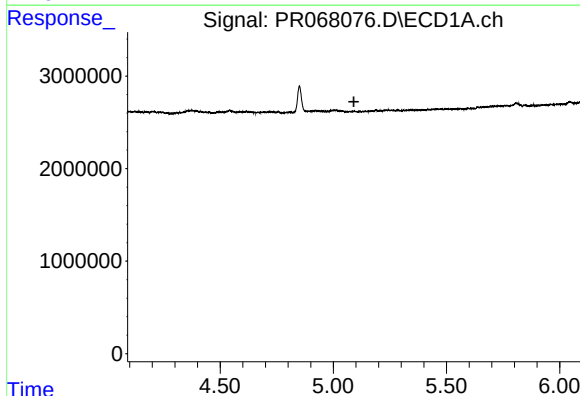


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T. : 5.091 min
Response: 0
Conc: N.D.

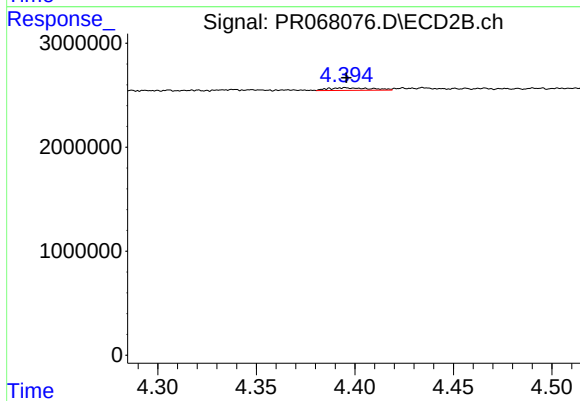

#6 AR-1016-4


R.T.: 4.395 min
Delta R.T.: 0.000 min
Response: 371331
Conc: 3.88 ng/ml

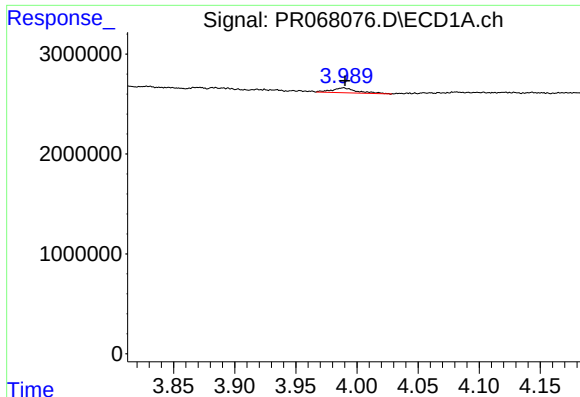

#9 AR-1221-2


R.T.: 3.989 min
Delta R.T.: -0.002 min
Response: 669029
Conc: 29.77 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

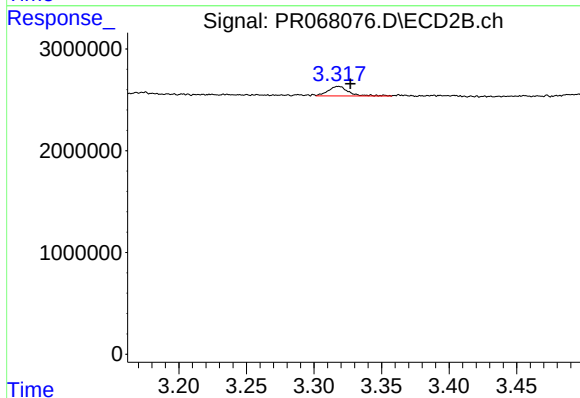


#9 AR-1221-2

R.T.: 3.318 min
Delta R.T.: -0.009 min
Response: 987590
Conc: 13.45 ng/ml

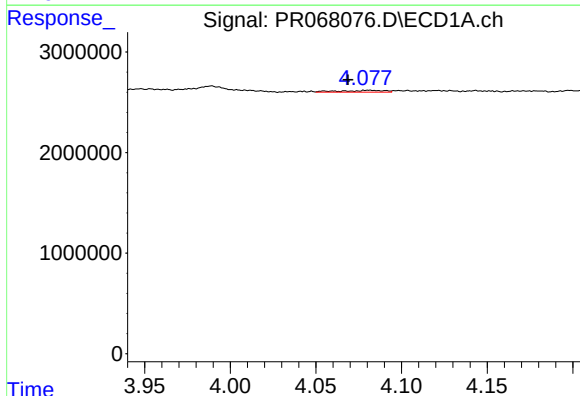


#10 AR-1221-3

R.T.: 4.081 min
Delta R.T.: 0.013 min
Response: 317991
Conc: 4.45 ng/ml

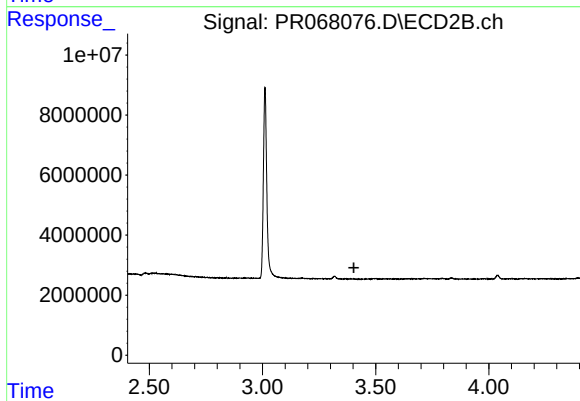

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 3.404 min
Response: 0
Conc: N.D.

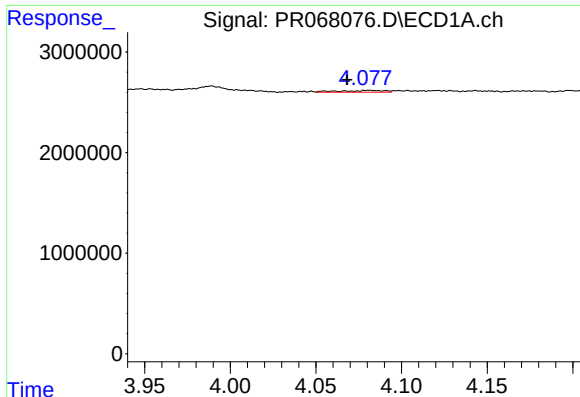

#11 AR-1232-1


R.T.: 4.081 min
Delta R.T.: 0.013 min
Response: 317991
Conc: 5.40 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

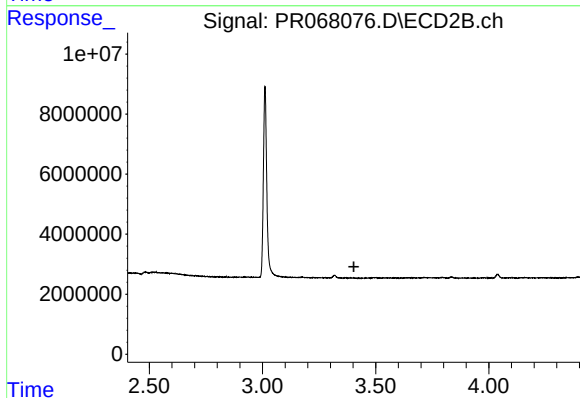


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 3.404 min
Response: 0
Conc: N.D.

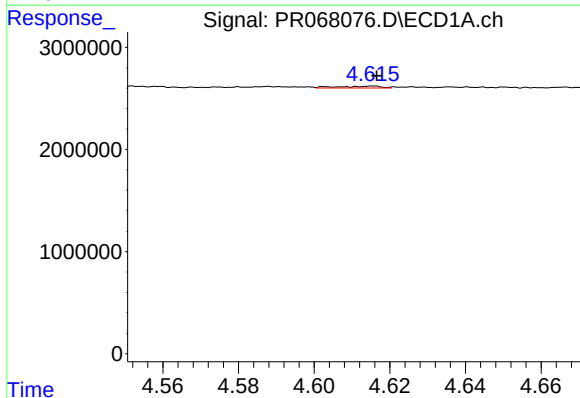


#12 AR-1232-2

R.T.: 4.615 min
Delta R.T.: -0.001 min
Response: 153839
Conc: 4.90 ng/ml

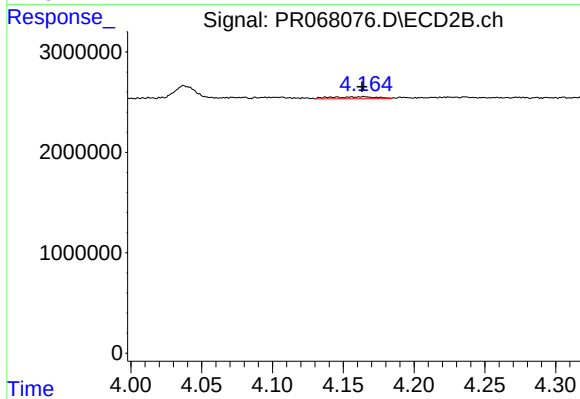

#12 AR-1232-2


R.T.: 4.165 min
Delta R.T.: 0.001 min
Response: 433682
Conc: 4.30 ng/ml

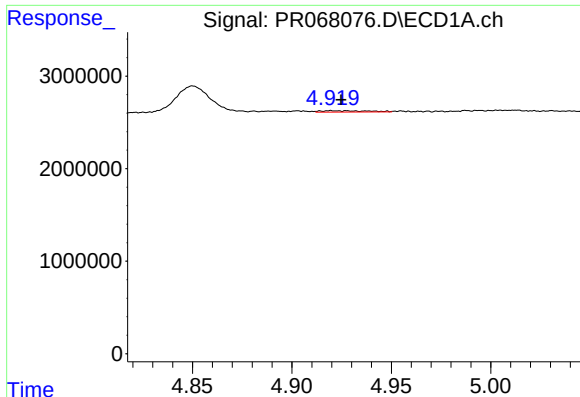

#13 AR-1232-3


R.T.: 4.920 min
Delta R.T.: -0.005 min
Response: 234139
Conc: 4.34 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

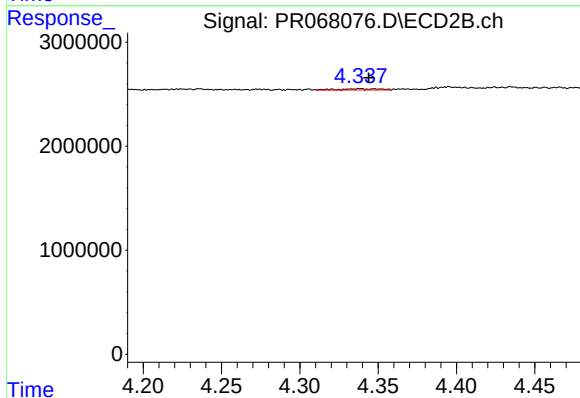


#13 AR-1232-3

R.T.: 4.338 min
Delta R.T.: -0.006 min
Response: 214928
Conc: 3.96 ng/ml

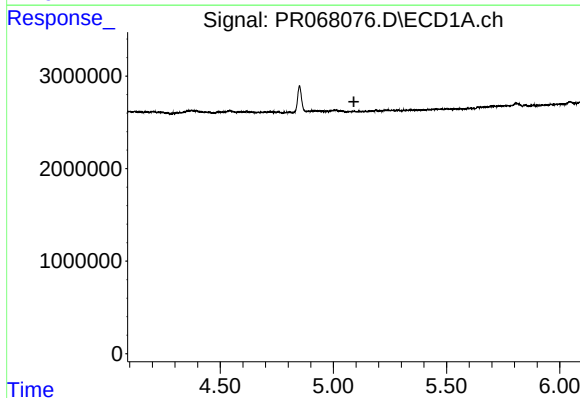


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T. : 5.091 min
Response: 0
Conc: N.D.

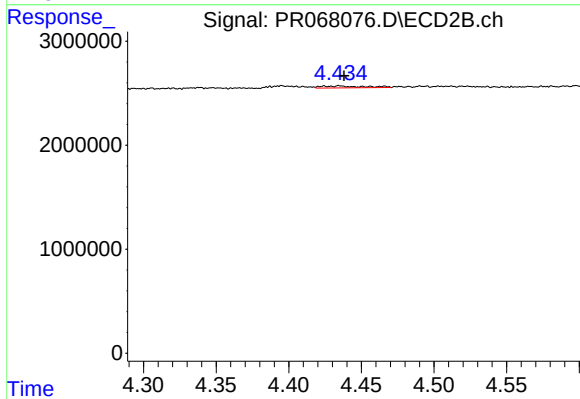

#14 AR-1232-4


R.T.: 4.435 min
Delta R.T.: -0.003 min
Response: 379862
Conc: 7.60 ng/ml

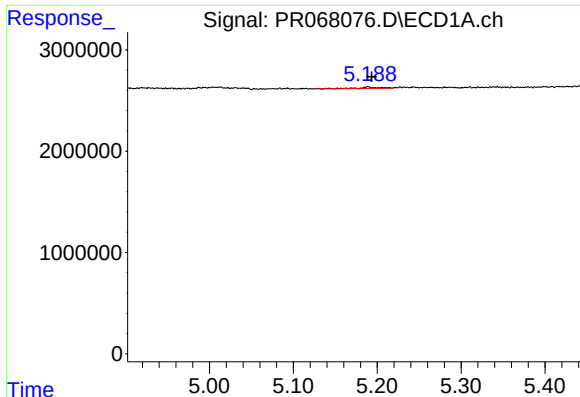

#15 AR-1232-5


R.T.: 5.189 min
Delta R.T.: -0.005 min
Response: 211679
Conc: 13.74 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

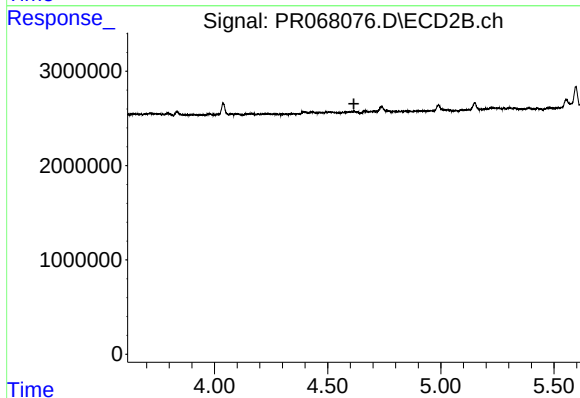


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T. : 4.616 min
Response: 0
Conc: N.D.

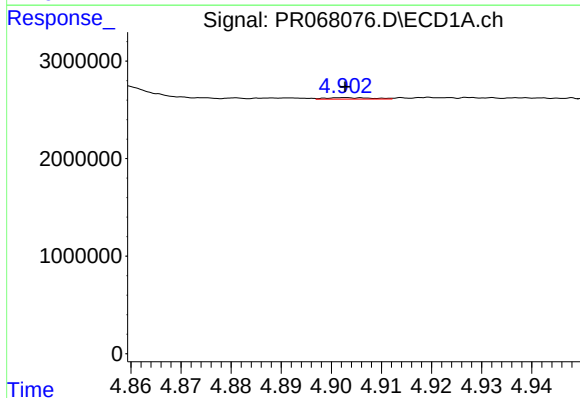


#16 AR-1242-1

R.T.: 4.903 min
Delta R.T.: 0.000 min
Response: 94629
Conc: 1.93 ng/ml

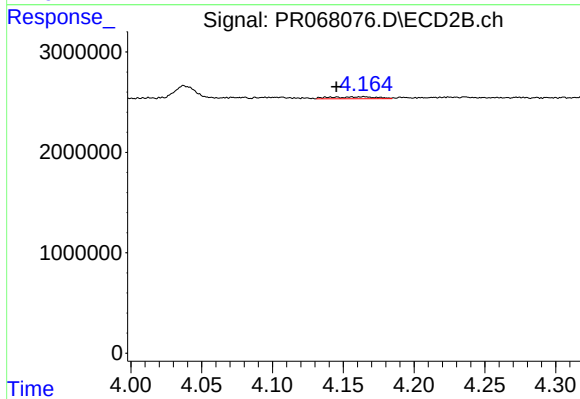

#16 AR-1242-1


R.T.: 4.165 min
Delta R.T.: 0.020 min
Response: 433682
Conc: 2.84 ng/ml

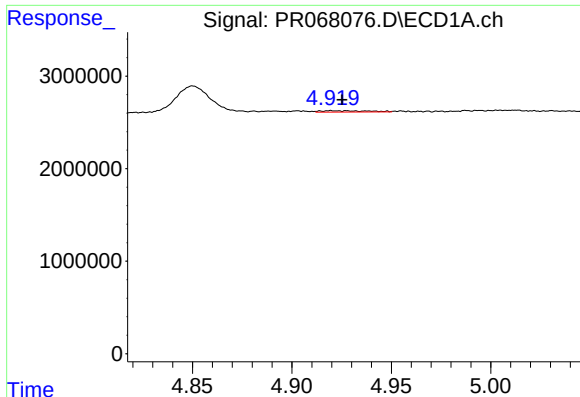

#17 AR-1242-2


R.T.: 4.920 min
Delta R.T.: -0.005 min
Response: 234139
Conc: 2.58 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

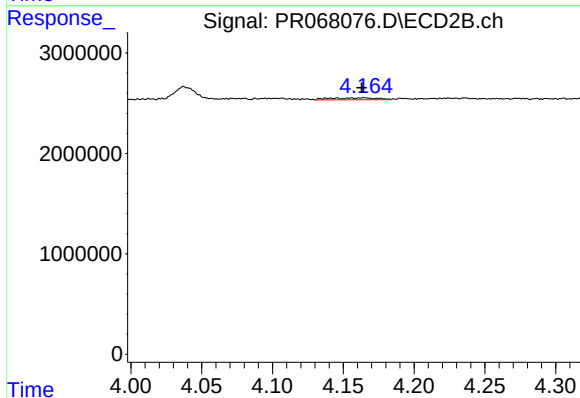


#17 AR-1242-2

R.T.: 4.165 min
Delta R.T.: 0.002 min
Response: 433682
Conc: 2.03 ng/ml

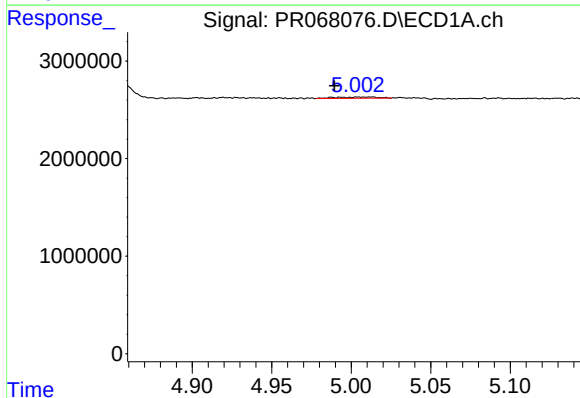


#18 AR-1242-3

R.T.: 5.013 min
Delta R.T.: 0.023 min
Response: 240161
Conc: 3.83 ng/ml

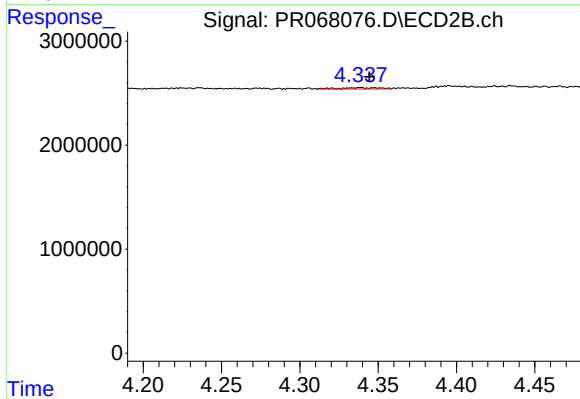

#18 AR-1242-3


R.T.: 4.338 min
Delta R.T.: -0.006 min
Response: 214928
Conc: 2.02 ng/ml

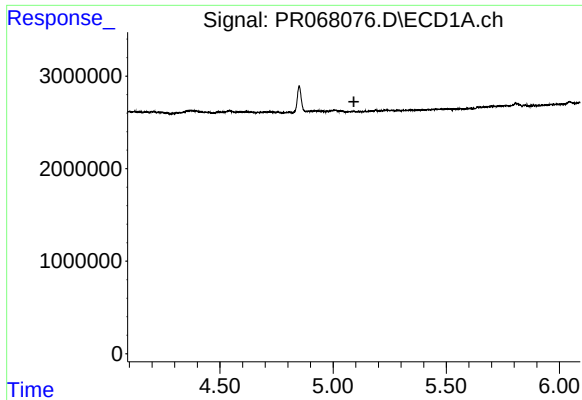

#19 AR-1242-4


R.T.: 0.000 min
Exp R.T.: 5.092 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

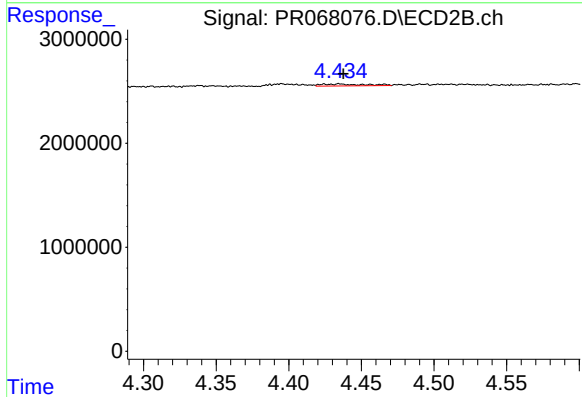


#19 AR-1242-4

R.T.: 4.435 min
Delta R.T.: -0.003 min
Response: 379862
Conc: 3.78 ng/ml

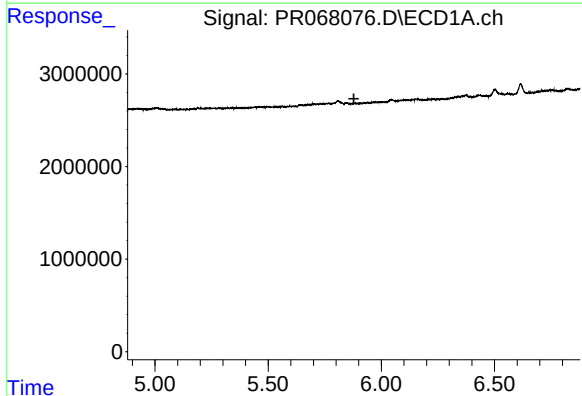


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T.: 5.879 min
Response: 0
Conc: N.D.

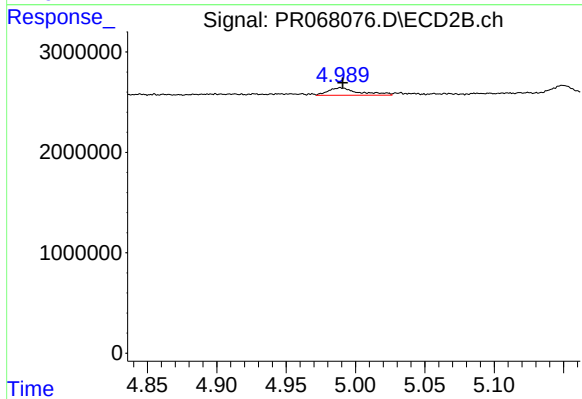

#20 AR-1242-5


R.T.: 4.989 min
Delta R.T.: -0.001 min
Response: 1152327
Conc: 7.35 ng/ml

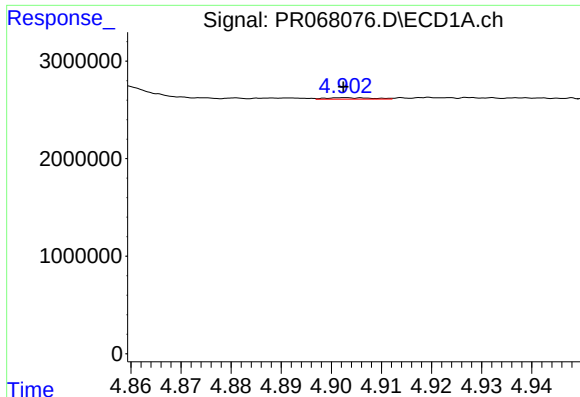

#21 AR-1248-1


R.T.: 4.903 min
Delta R.T.: 0.000 min
Response: 94629
Conc: 2.47 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

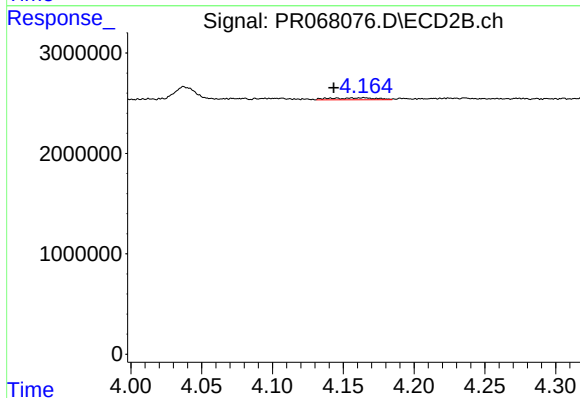


#21 AR-1248-1

R.T.: 4.165 min
Delta R.T.: 0.021 min
Response: 433682
Conc: 3.64 ng/ml

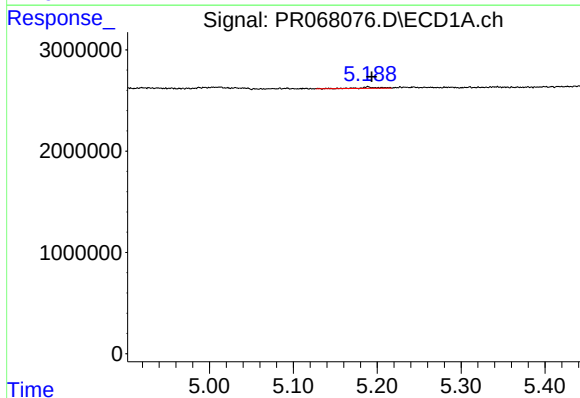


#22 AR-1248-2

R.T.: 5.189 min
Delta R.T.: -0.004 min
Response: 211679
Conc: 4.04 ng/ml

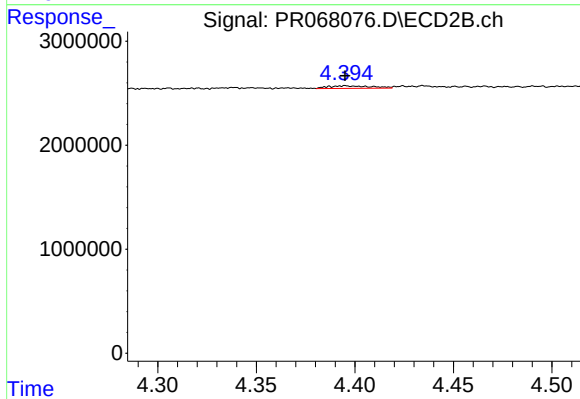

#22 AR-1248-2


R.T.: 4.395 min
Delta R.T.: 0.000 min
Response: 371331
Conc: 1.97 ng/ml

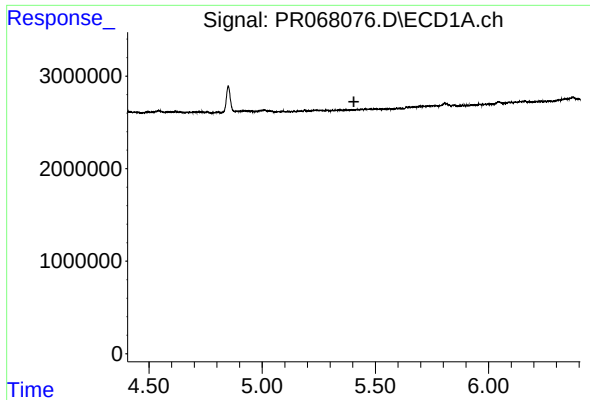

#23 AR-1248-3


R.T.: 0.000 min
Exp R.T.: 5.405 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

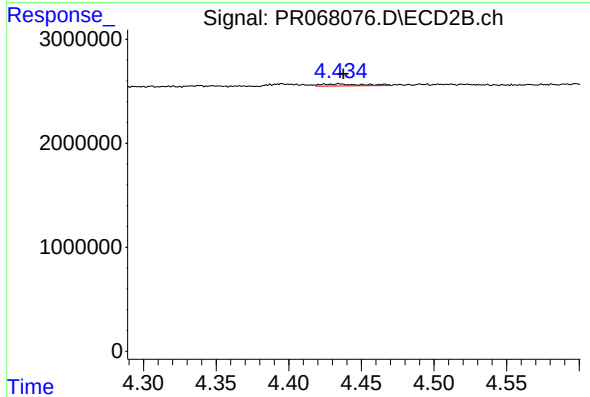


#23 AR-1248-3

R.T.: 4.435 min
Delta R.T.: -0.002 min
Response: 379862
Conc: 1.99 ng/ml

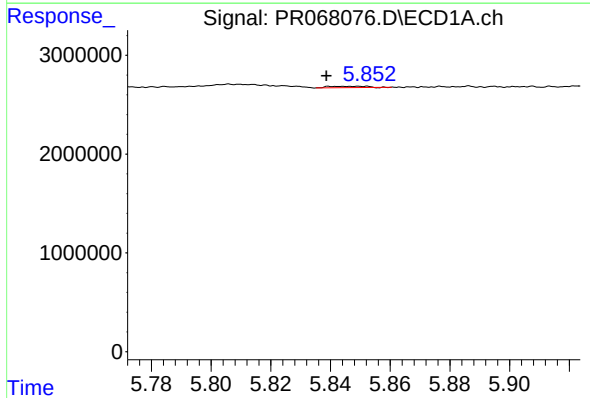


#24 AR-1248-4

R.T.: 5.848 min
Delta R.T.: 0.009 min
Response: 123646
Conc: 1.66 ng/ml

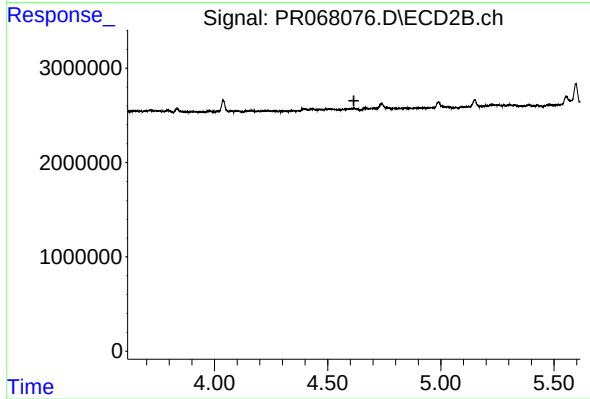

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 4.616 min
Response: 0
Conc: N.D.

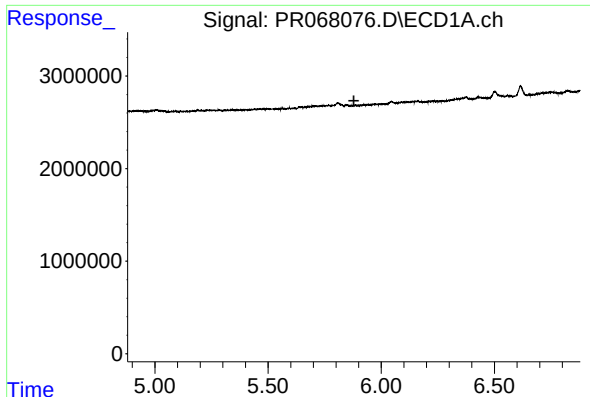

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 5.879 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

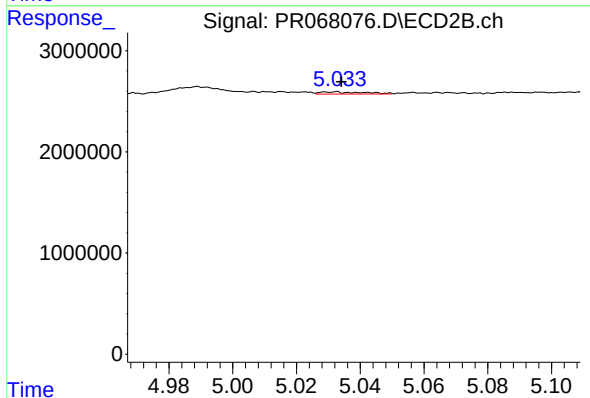


#25 AR-1248-5

R.T.: 5.032 min
Delta R.T.: -0.002 min
Response: 210258
Conc: 0.99 ng/ml

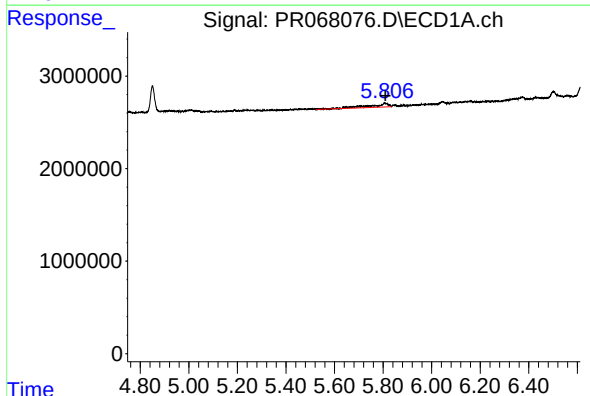


#26 AR-1254-1

R.T.: 5.808 min
Delta R.T.: -0.001 min
Response: 2286349
Conc: 32.04 ng/ml

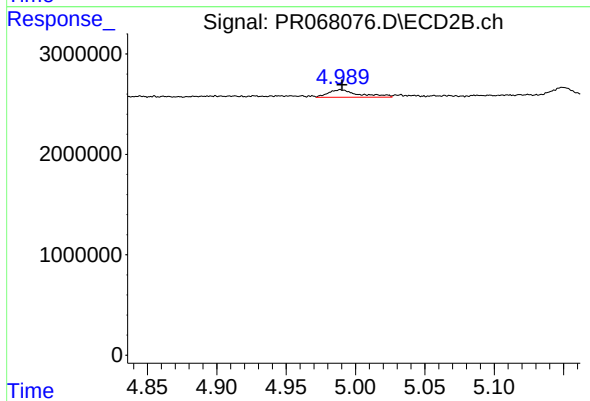

#26 AR-1254-1


R.T.: 4.989 min
Delta R.T.: 0.000 min
Response: 1152327
Conc: 4.51 ng/ml

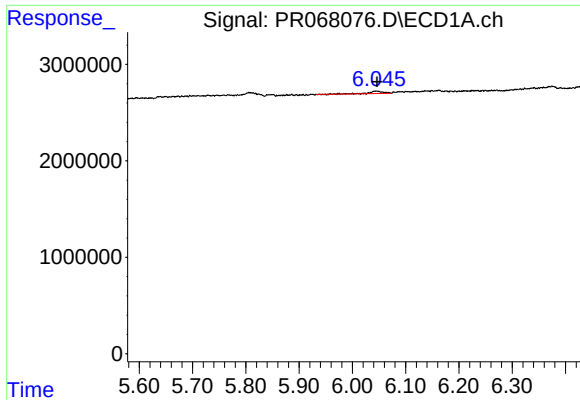

#27 AR-1254-2


R.T.: 6.045 min
Delta R.T.: -0.002 min
Response: 437261
Conc: 3.90 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

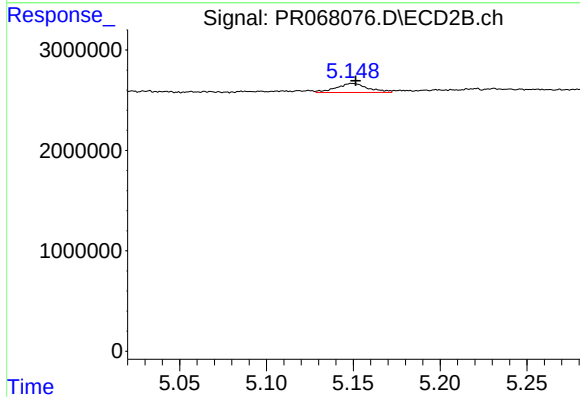


#27 AR-1254-2

R.T.: 5.150 min
Delta R.T.: -0.002 min
Response: 1162486
Conc: 5.06 ng/ml

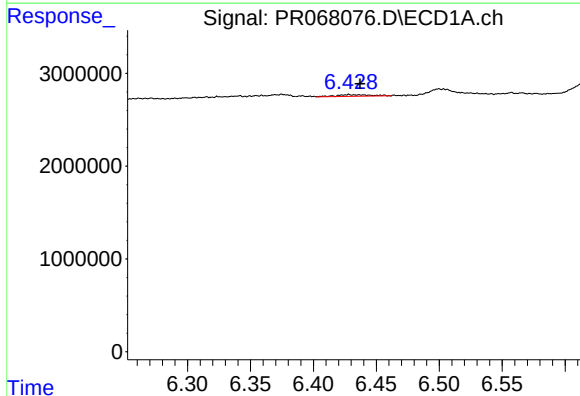


#28 AR-1254-3

R.T.: 6.429 min
Delta R.T.: -0.008 min
Response: 322212
Conc: 2.40 ng/ml

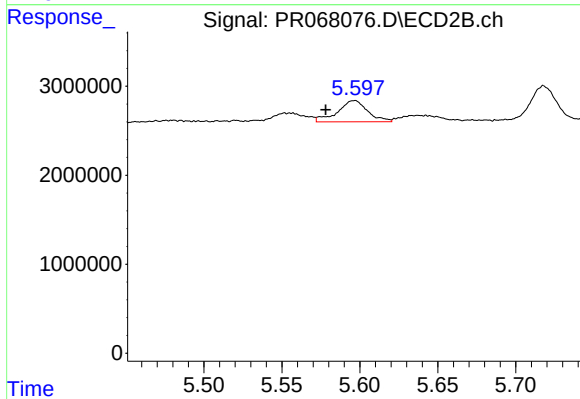

#28 AR-1254-3


R.T.: 5.596 min
Delta R.T.: 0.018 min
Response: 3198238
Conc: 8.86 ng/ml

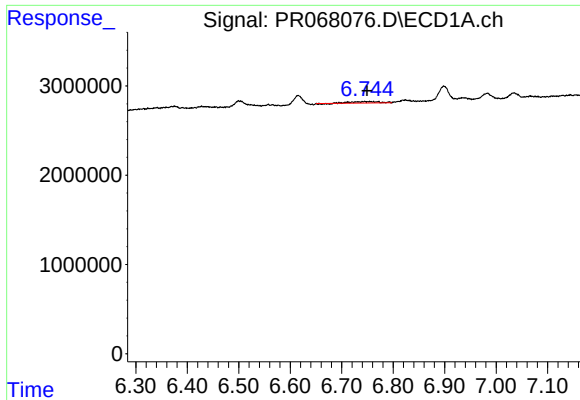

#29 AR-1254-4


R.T.: 6.745 min
Delta R.T.: -0.004 min
Response: 495012
Conc: 4.74 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

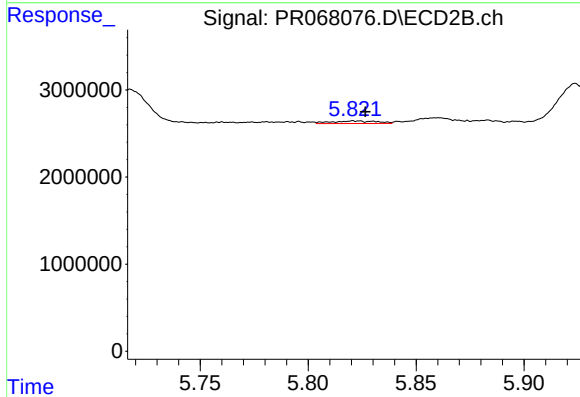


#29 AR-1254-4

R.T.: 5.821 min
Delta R.T.: -0.005 min
Response: 446990
Conc: 2.08 ng/ml

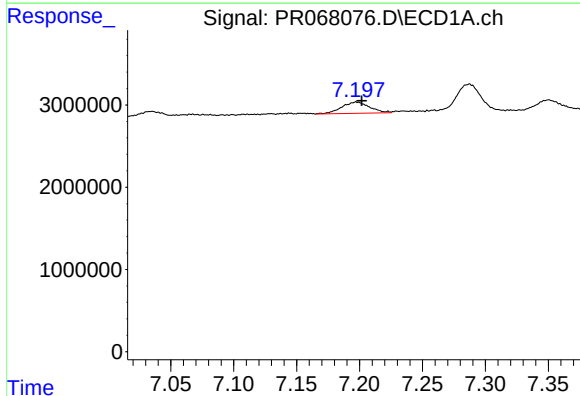


#30 AR-1254-5

R.T.: 7.198 min
Delta R.T.: -0.004 min
Response: 2095290
Conc: 16.87 ng/ml

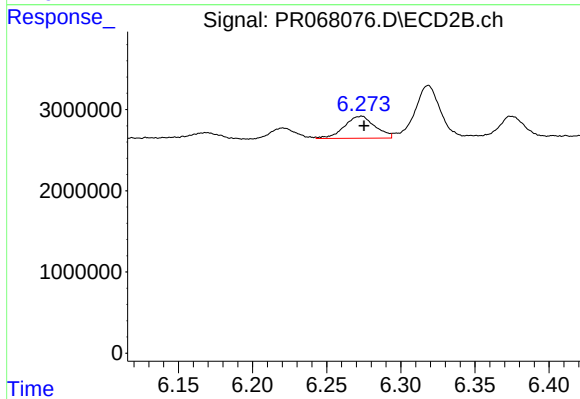

#30 AR-1254-5


R.T.: 6.273 min
Delta R.T.: -0.002 min
Response: 3941542
Conc: 11.94 ng/ml

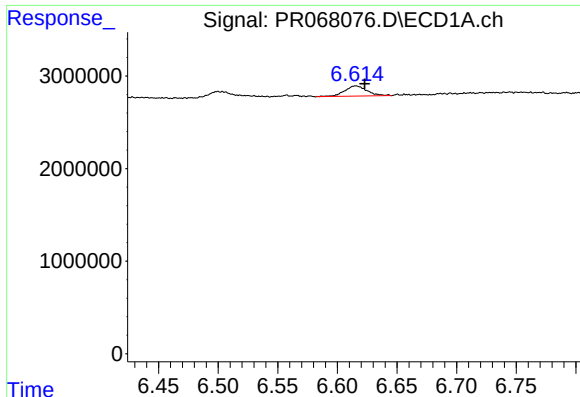

#31 AR-1260-1


R.T.: 6.616 min
Delta R.T.: -0.007 min
Response: 1458398
Conc: 15.78 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

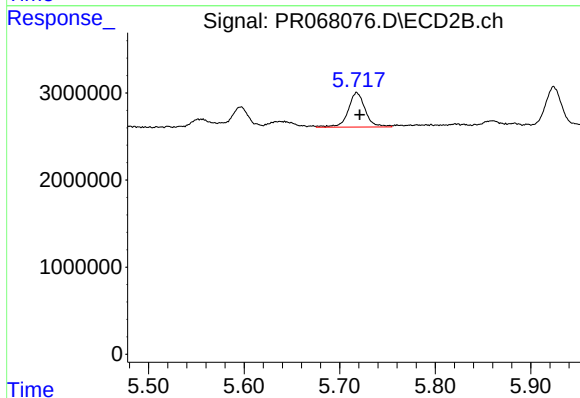


#31 AR-1260-1

R.T.: 5.718 min
Delta R.T.: -0.003 min
Response: 4944756
Conc: 20.20 ng/ml

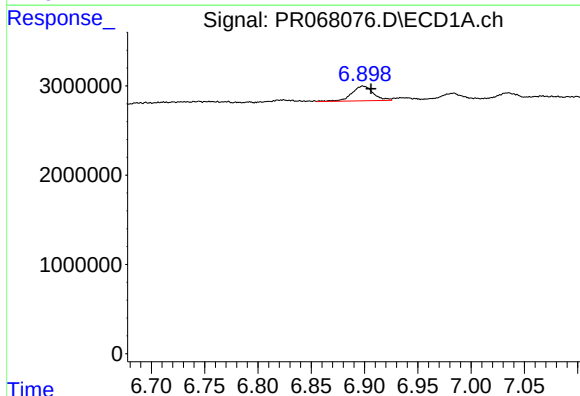


#32 AR-1260-2

R.T.: 6.899 min
Delta R.T.: -0.007 min
Response: 2322952
Conc: 16.34 ng/ml

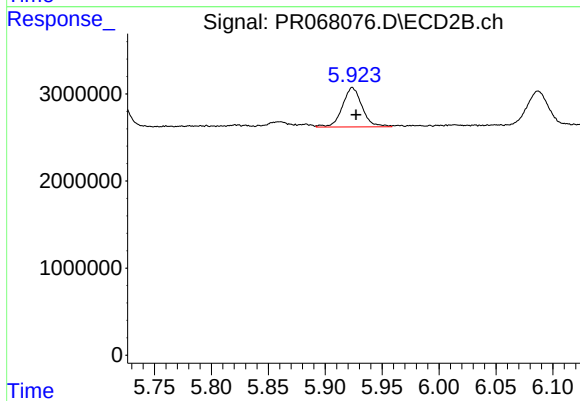

#32 AR-1260-2


R.T.: 5.924 min
Delta R.T.: -0.003 min
Response: 5477602
Conc: 18.87 ng/ml

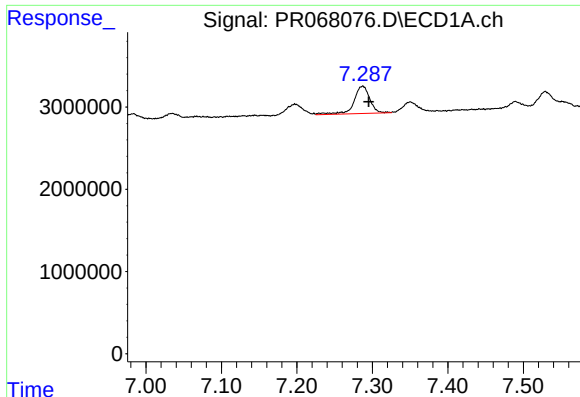

#33 AR-1260-3


R.T.: 7.287 min
Delta R.T.: -0.008 min
Response: 4851188
Conc: 35.03 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

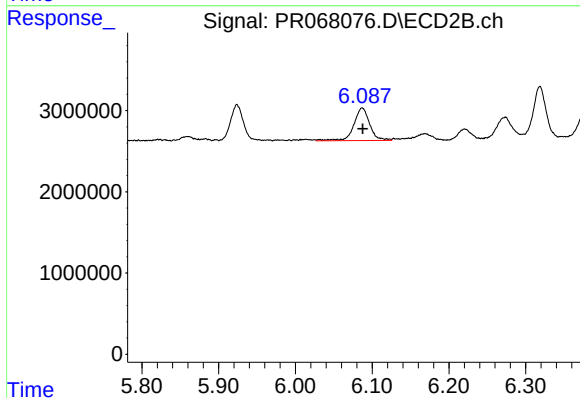


#33 AR-1260-3

R.T.: 6.087 min
Delta R.T.: 0.000 min
Response: 5832720
Conc: 21.24 ng/ml

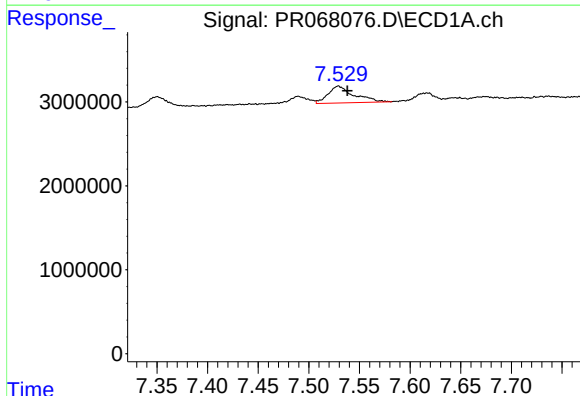


#34 AR-1260-4

R.T.: 7.529 min
Delta R.T.: -0.009 min
Response: 3592830
Conc: 28.35 ng/ml

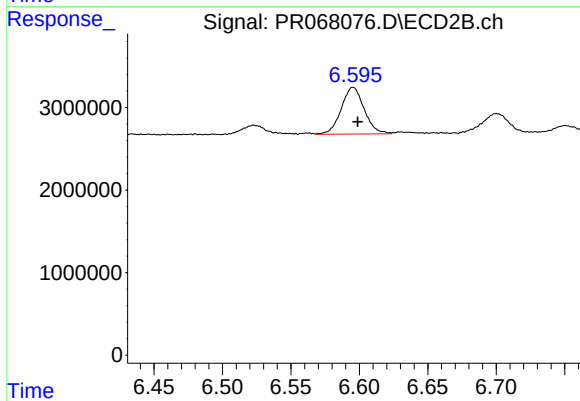

#34 AR-1260-4


R.T.: 6.595 min
Delta R.T.: -0.003 min
Response: 6602900
Conc: 31.49 ng/ml

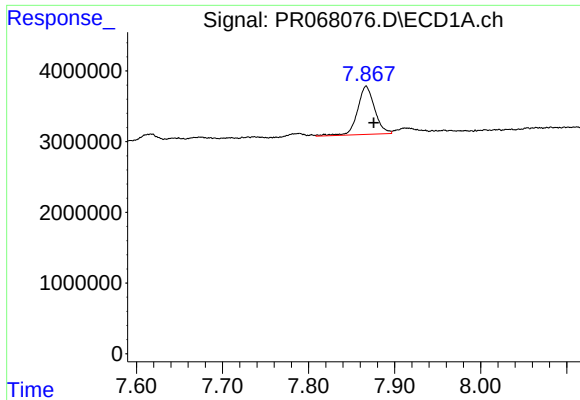

#35 AR-1260-5


R.T.: 7.867 min
Delta R.T.: -0.009 min
Response: 9461816
Conc: 25.96 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

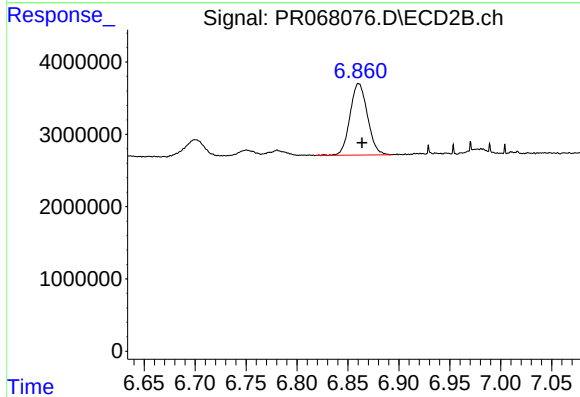


#35 AR-1260-5

R.T.: 6.861 min
Delta R.T.: -0.003 min
Response: 11788685
Conc: 24.35 ng/ml

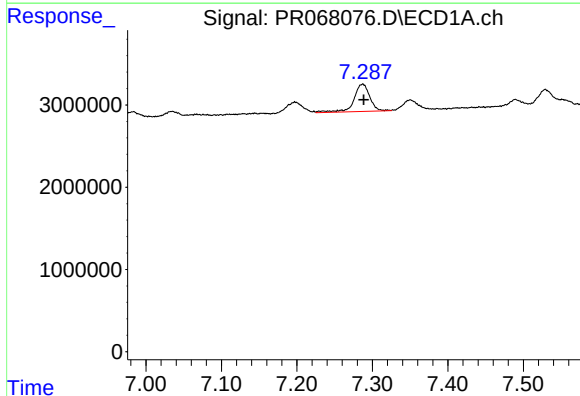


#36 AR-1262-1

R.T.: 7.287 min
Delta R.T.: -0.002 min
Response: 4851188
Conc: 24.36 ng/ml

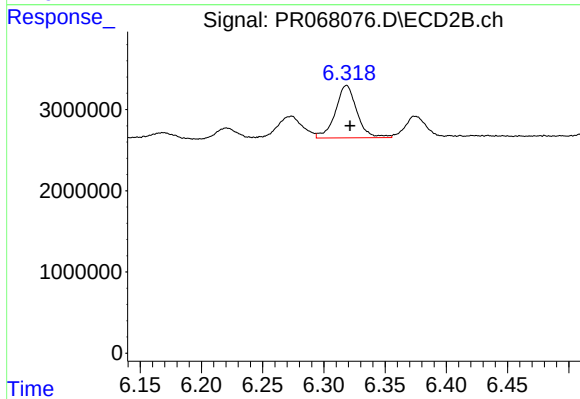

#36 AR-1262-1


R.T.: 6.318 min
Delta R.T.: -0.003 min
Response: 7891243
Conc: 22.84 ng/ml

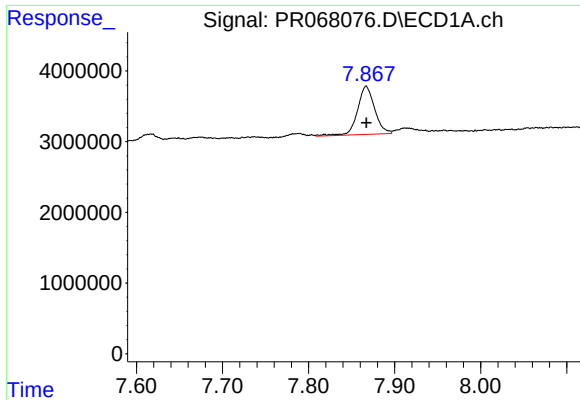

#37 AR-1262-2


R.T.: 7.867 min
Delta R.T.: 0.000 min
Response: 9461816
Conc: 21.85 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

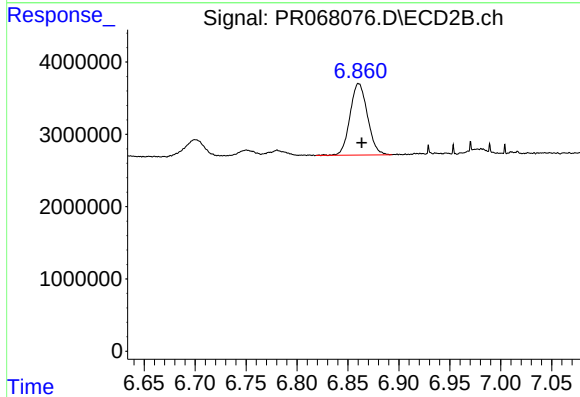


#37 AR-1262-2

R.T.: 6.861 min
Delta R.T.: -0.003 min
Response: 11788685
Conc: 19.38 ng/ml

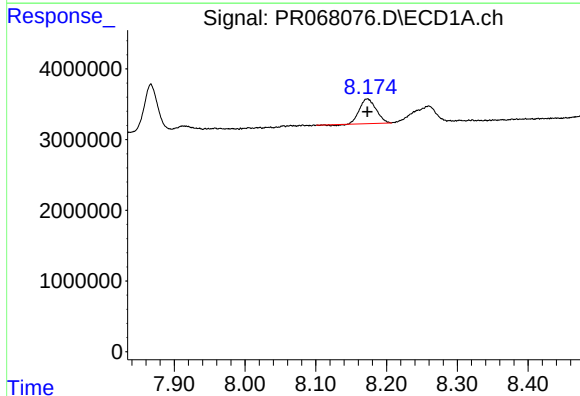


#38 AR-1262-3

R.T.: 8.173 min
Delta R.T.: 0.000 min
Response: 5612209
Conc: 17.92 ng/ml

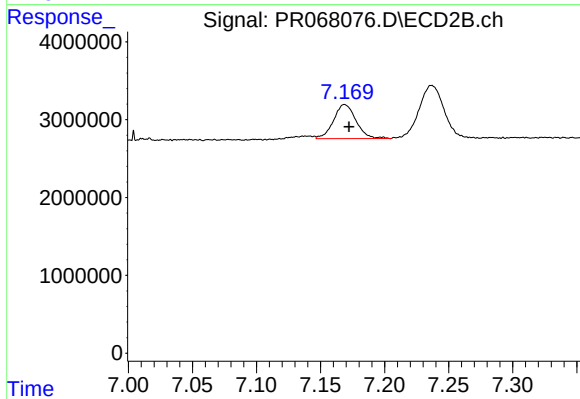

#38 AR-1262-3


R.T.: 7.169 min
Delta R.T.: -0.003 min
Response: 5352422
Conc: 22.42 ng/ml

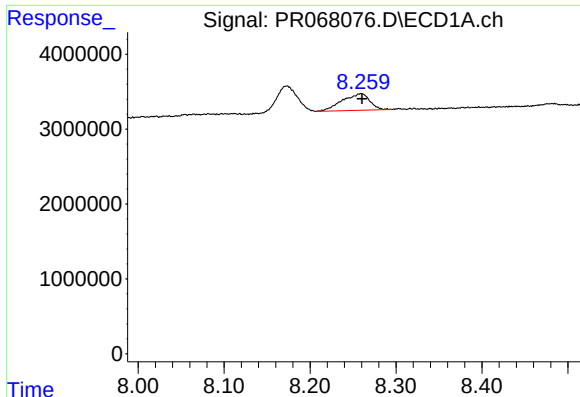

#39 AR-1262-4


R.T.: 8.259 min
Delta R.T.: -0.001 min
Response: 4996875
Conc: 18.20 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

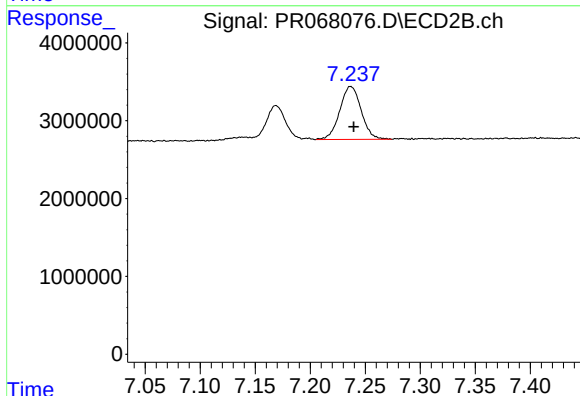


#39 AR-1262-4

R.T.: 7.237 min
Delta R.T.: -0.003 min
Response: 9189246
Conc: 20.68 ng/ml

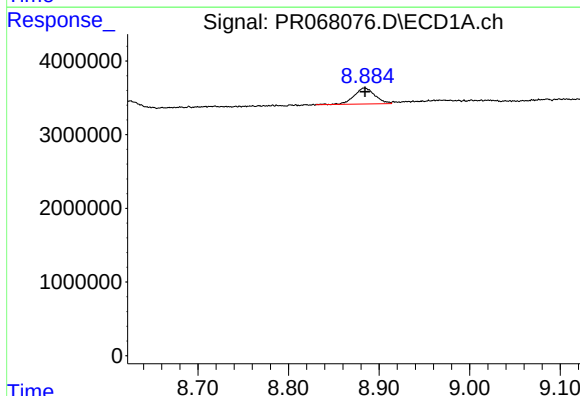


#40 AR-1262-5

R.T.: 8.884 min
Delta R.T.: 0.000 min
Response: 3452326
Conc: 18.24 ng/ml

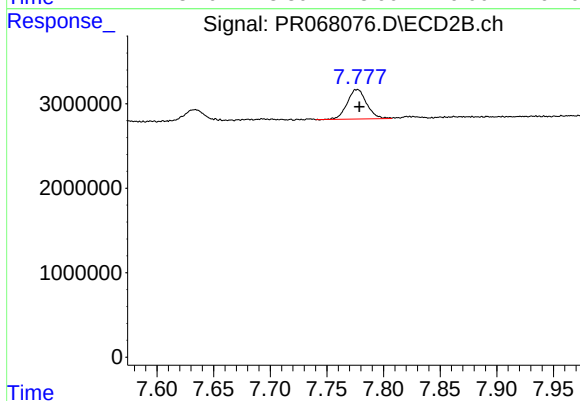

#40 AR-1262-5


R.T.: 7.777 min
Delta R.T.: -0.002 min
Response: 4193110
Conc: 20.59 ng/ml

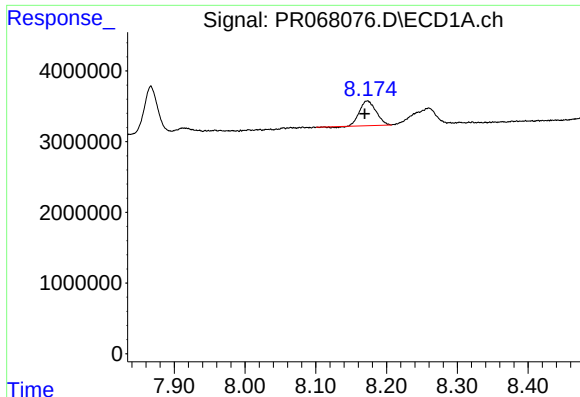

#41 AR-1268-1


R.T.: 8.173 min
Delta R.T.: 0.004 min
Response: 5612209
Conc: 9.31 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

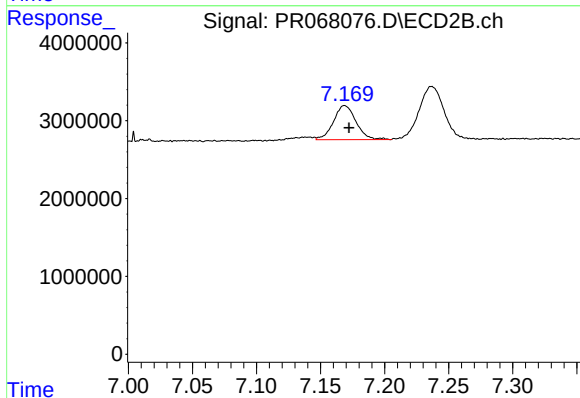


#41 AR-1268-1

R.T.: 7.169 min
Delta R.T.: -0.003 min
Response: 5352422
Conc: 7.25 ng/ml

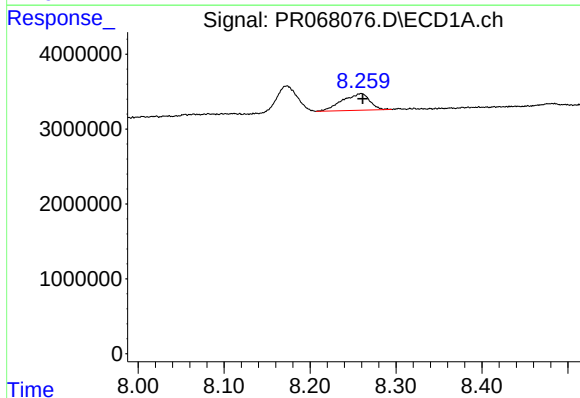


#42 AR-1268-2

R.T.: 8.259 min
Delta R.T.: -0.002 min
Response: 4996875
Conc: 8.77 ng/ml

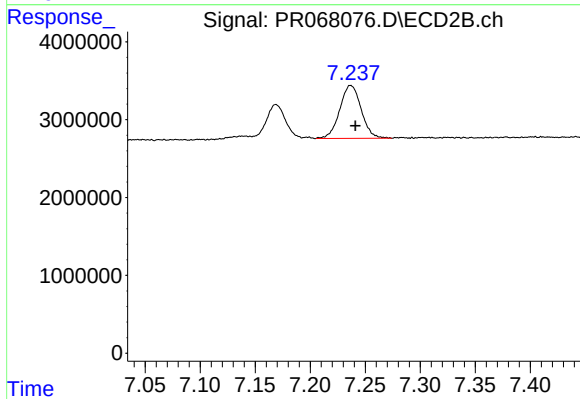

#42 AR-1268-2


R.T.: 7.237 min
Delta R.T.: -0.004 min
Response: 9189246
Conc: 13.61 ng/ml

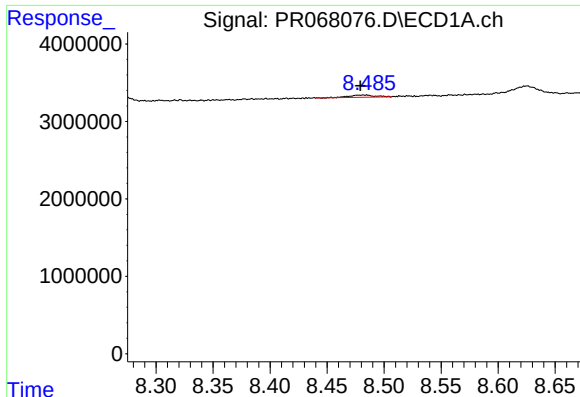

#43 AR-1268-3


R.T.: 8.482 min
Delta R.T.: 0.003 min
Response: 472204
Conc: 0.85 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

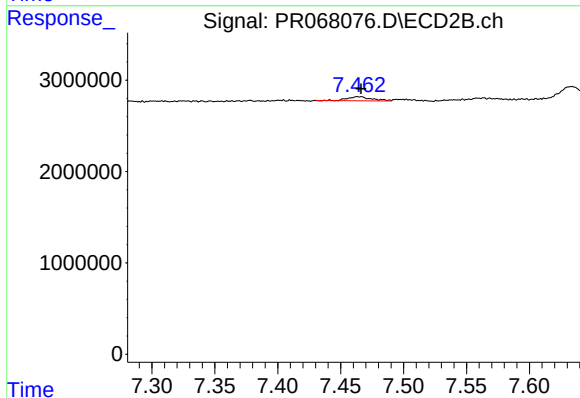


#43 AR-1268-3

R.T.: 7.464 min
Delta R.T.: -0.002 min
Response: 606679
Conc: 0.98 ng/ml

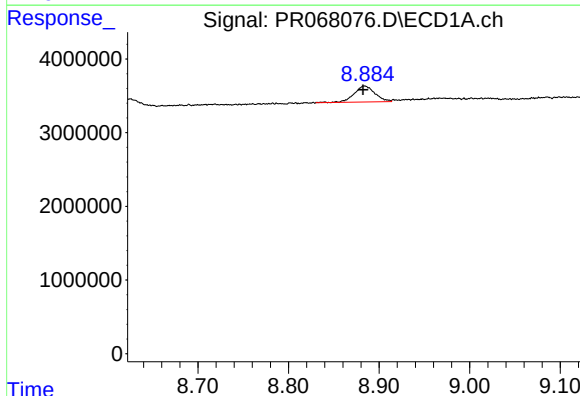


#44 AR-1268-4

R.T.: 8.884 min
Delta R.T.: 0.002 min
Response: 3452326
Conc: 17.04 ng/ml

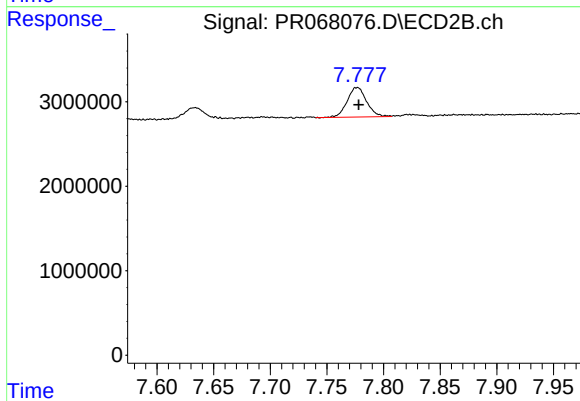

#44 AR-1268-4


R.T.: 7.777 min
Delta R.T.: -0.002 min
Response: 4193110
Conc: 20.11 ng/ml

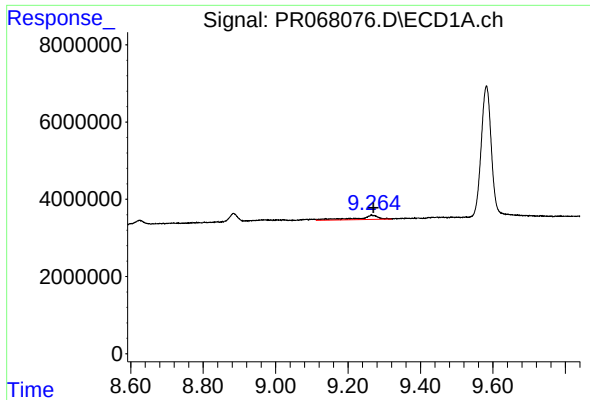

#45 AR-1268-5

R.T.: 9.266 min
Delta R.T.: -0.004 min
Response: 4378826
Conc: 2.80 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

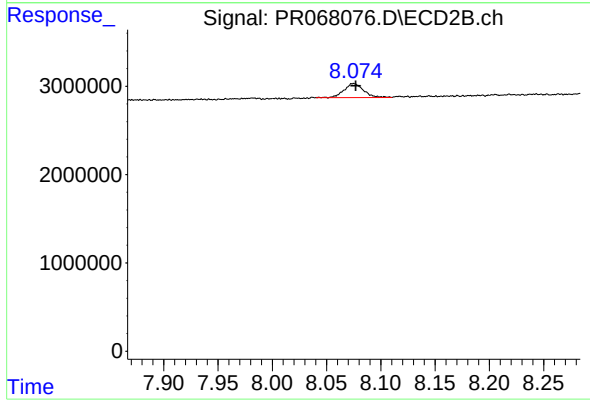

#45 AR-1268-5

R.T.: 8.075 min
Delta R.T.: -0.002 min
Response: 1986682
Conc: 1.39 ng/ml