

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR080724\
 Data File : PR068077.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Aug 2024 12:19
 Operator : AJ\MA
 Sample : P3390-09
 Misc : AR1268 MDL 25 PPB
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 07 17:13:50 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 07 00:26:28 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.677	3.011	41452709	81099630	16.295	18.598
2)	SA Decachlor...	9.579	8.331	84511616	96615738	19.260	21.323
Target Compounds							
3)	L1 AR-1016-1	4.903	4.158	80003	330900	1.369	2.202 #
4)	L1 AR-1016-2	4.913	4.158	95593	330900	0.862	1.577 #
5)	L1 AR-1016-3	4.981	4.346	109701	302317	1.428	2.650 #
6)	L1 AR-1016-4	5.108f	4.382	190550	236916	3.043	2.477
8)	L2 AR-1221-1	3.883f	3.260f	370568	173771	13.482	1.118 #
9)	L2 AR-1221-2	3.989	3.317	711844	1435279	31.678	19.542 #
10)	L2 AR-1221-3	4.072	3.422f	37170	96641	0.520	0.298 #
11)	L3 AR-1232-1	4.072	3.422f	37170	96641	0.632	0.954 #
12)	L3 AR-1232-2	4.612	4.158	172378	330900	5.488	3.284 #
13)	L3 AR-1232-3	4.913	4.346	95593	302317	1.773	5.567 #
14)	L3 AR-1232-4	5.108f	4.425	190550	82456	6.373	1.650 #
15)	L3 AR-1232-5	5.198	0.000	236007	0	15.324	N.D. #
16)	L4 AR-1242-1	4.903	4.158	80003	330900	1.635	2.171 #
17)	L4 AR-1242-2	4.913	4.158	95593	330900	1.052	1.547 #
18)	L4 AR-1242-3	4.981	4.346	109701	302317	1.748	2.846 #
19)	L4 AR-1242-4	5.108f	4.425	190550	82456	3.818	0.820 #
20)	L4 AR-1242-5	0.000	4.987	0	284802	N.D.	1.816 #
21)	L5 AR-1248-1	4.903	4.158f	80003	330900	2.084	2.781 #
22)	L5 AR-1248-2	5.198	4.382	236007	236916	4.499	1.257 #
23)	L5 AR-1248-3	0.000	4.425	0	82456	N.D.	0.433 #
24)	L5 AR-1248-4	5.823f	0.000	1702651	0	22.899	N.D. #
25)	L5 AR-1248-5	0.000	5.014f	0	617940	N.D.	2.908 #
26)	L6 AR-1254-1	5.823	4.987	1702651	284802	23.858	1.114 #
27)	L6 AR-1254-2	6.051	5.149	142297	1280127	1.268	5.569 #
28)	L6 AR-1254-3	6.434	5.559f	518123	1591417	3.856	4.411
29)	L6 AR-1254-4	0.766f	0.000	68880	0	0.659	N.D. #
30)	L6 AR-1254-5	0.000	6.275	0	299875	N.D.	0.908 #
31)	L7 AR-1260-1	0.000	5.728	0	650893	N.D.	2.659 #
32)	L7 AR-1260-2	6.899	5.922	194712	372815	1.370	1.284
33)	L7 AR-1260-3	7.287	6.091	3892010	1006300	28.107	3.664 #
34)	L7 AR-1260-4	7.553	6.596	3760299	4864580	29.668	23.202
35)	L7 AR-1260-5	7.867	6.860	1675274	1681631	4.596	3.474
36)	L8 AR-1262-1	7.287	6.319	3892010	3561737	19.540	10.311 #
37)	L8 AR-1262-2	7.867	6.860	1675274	1681631	3.869	2.765 #
38)	L8 AR-1262-3	8.170	7.170	14588519	17886241	46.590	74.908 #
39)	L8 AR-1262-4	8.261	7.239	13783971	15532647	50.201	34.954 #
40)	L8 AR-1262-5	8.884	7.777	5538254	5312280	29.258	26.081
41)	L9 AR-1268-1	8.170	7.170	14588519	17886241	24.192	24.226
42)	L9 AR-1268-2	8.261	7.239	13783971	15532647	24.186	23.007

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR080724\
Data File : PR068077.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Aug 2024 12:19
Operator : AJ\MA
Sample : P3390-09
Misc : AR1268 MDL 25 PPB
ALS Vial : 63 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 17:13:50 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 07 00:26:28 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43)	L9 AR-1268-3	8.480	7.465	13043808	14459234	23.499	23.445
44)	L9 AR-1268-4	8.884	7.777	5538254	5312280	27.341	25.474
45)	L9 AR-1268-5	9.269	8.075	38028932	40415422	24.317	28.303



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR080724\
Data File : PR068077.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Aug 2024 12:19
Operator : AJ\MA
Sample : P3390-09
Misc : AR1268 MDL 25 PPB
ALS Vial : 63 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 17:13:50 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 07 00:26:28 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

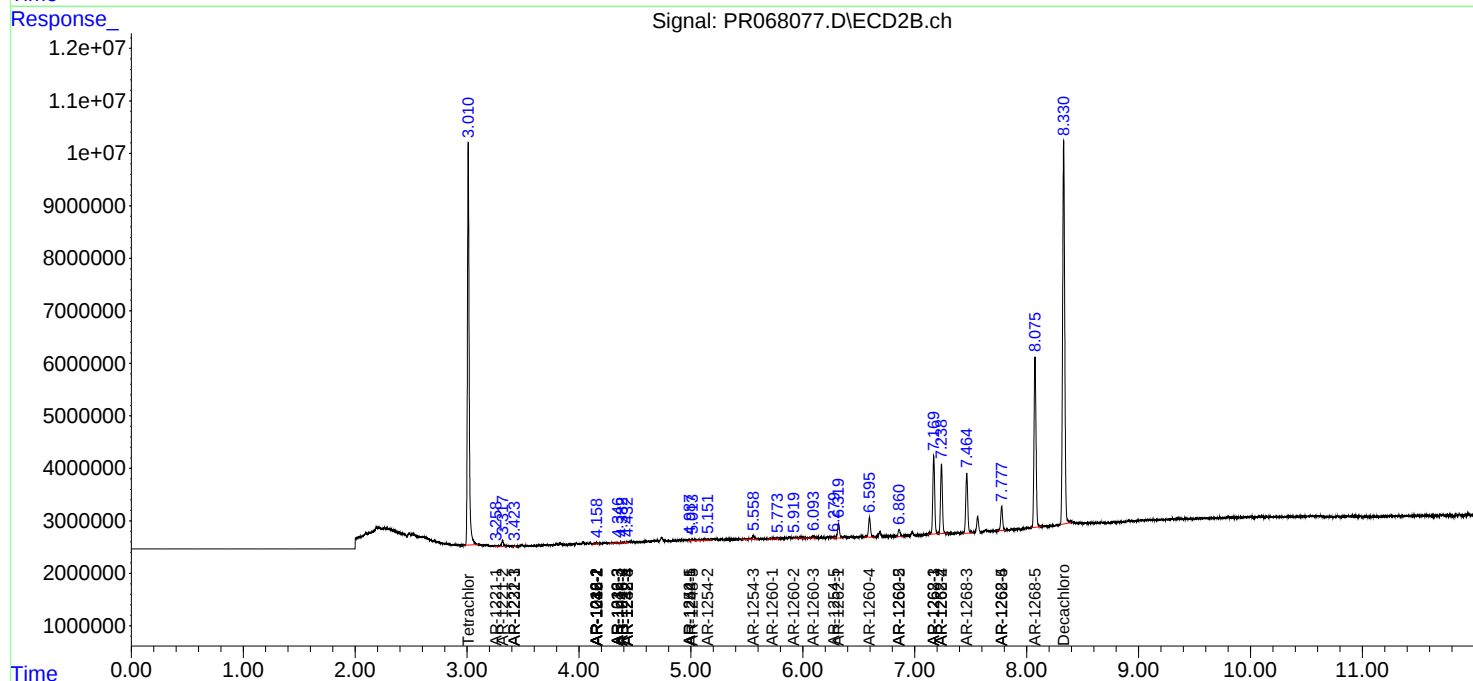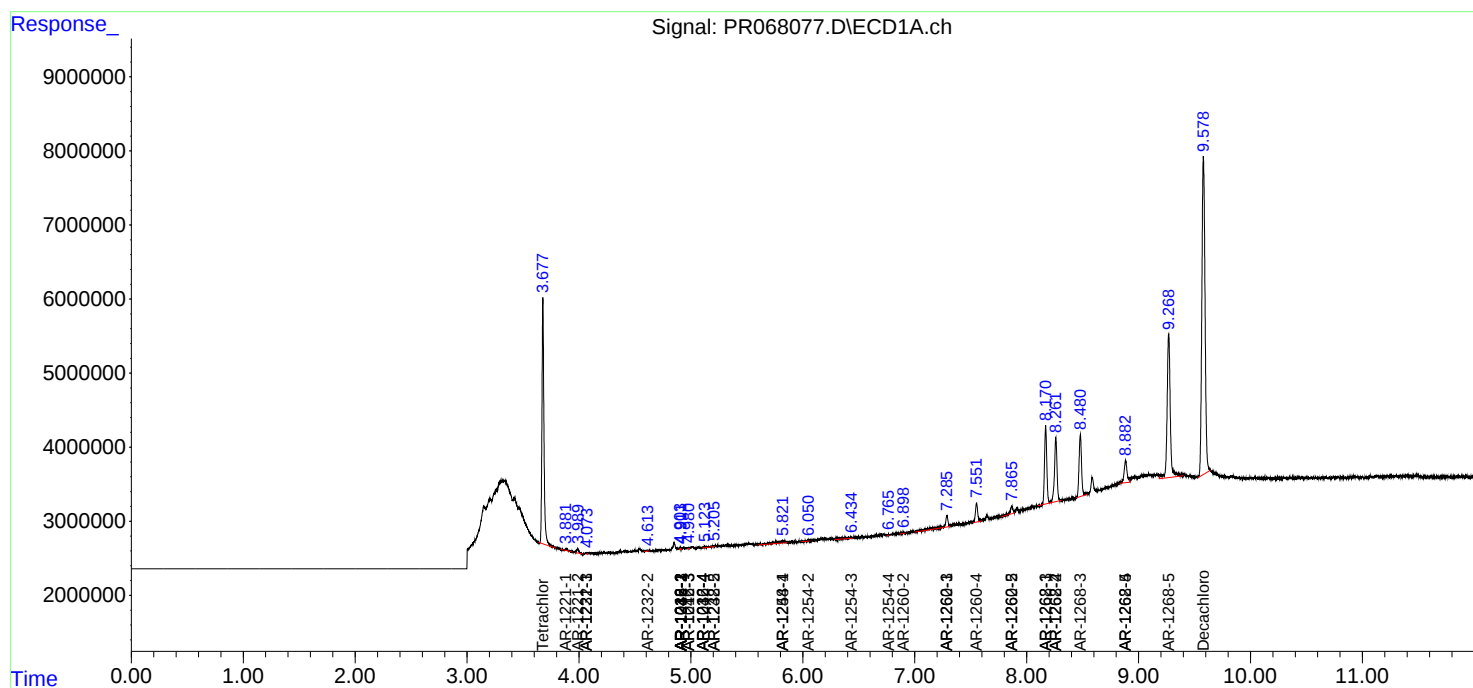


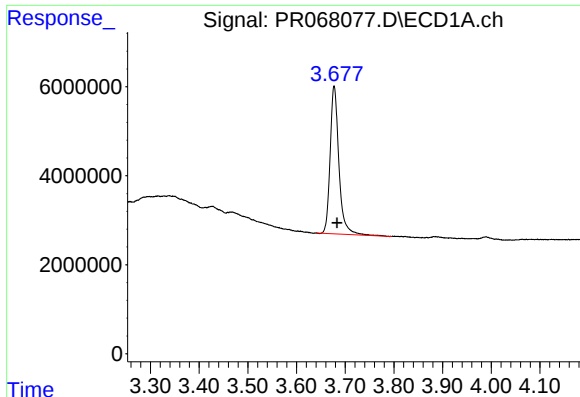

#1 Tetrachloro-m-xylene


R.T.: 3.677 min
Delta R.T.: -0.006 min
Response: 41452709
Conc: 16.29 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

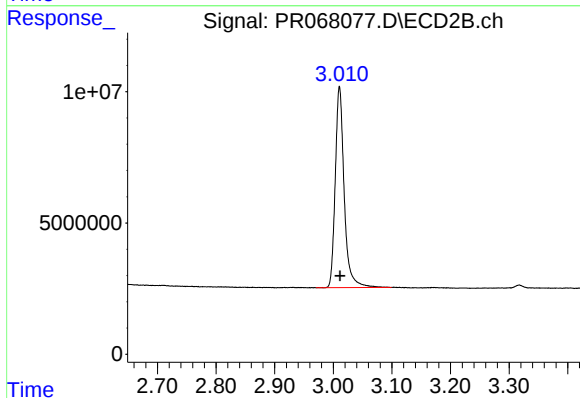


#1 Tetrachloro-m-xylene

R.T.: 3.011 min
Delta R.T.: 0.000 min
Response: 81099630
Conc: 18.60 ng/ml

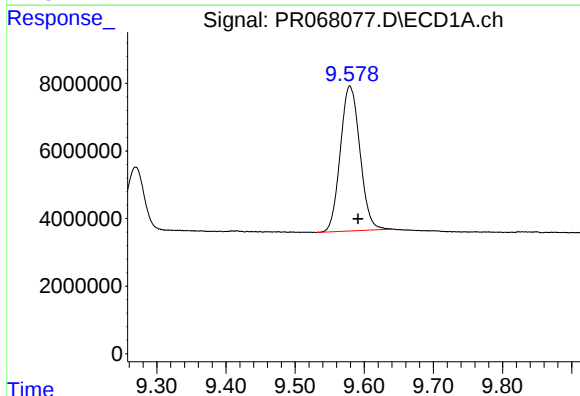


#2 Decachlorobiphenyl

R.T.: 9.579 min
Delta R.T.: -0.012 min
Response: 84511616
Conc: 19.26 ng/ml

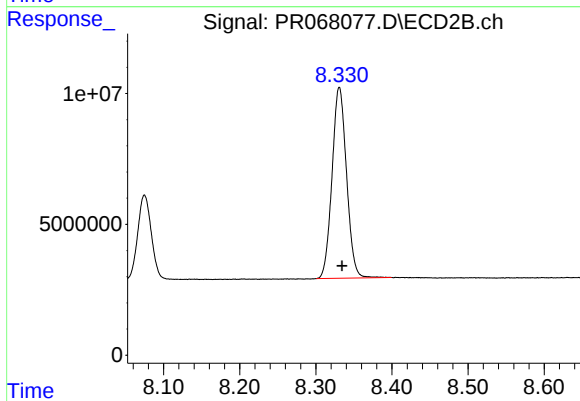

#2 Decachlorobiphenyl


R.T.: 8.331 min
Delta R.T.: -0.004 min
Response: 96615738
Conc: 21.32 ng/ml

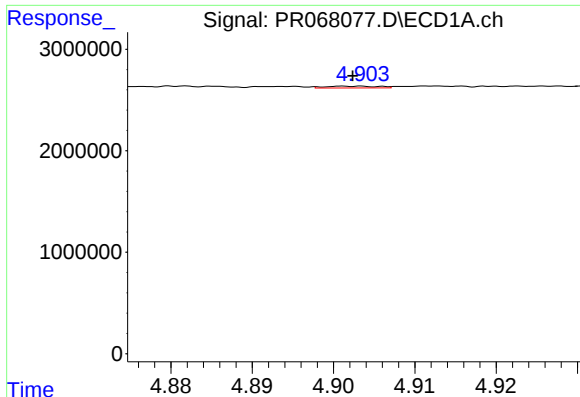

#3 AR-1016-1


R.T.: 4.903 min
Delta R.T.: 0.000 min
Response: 80003
Conc: 1.37 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

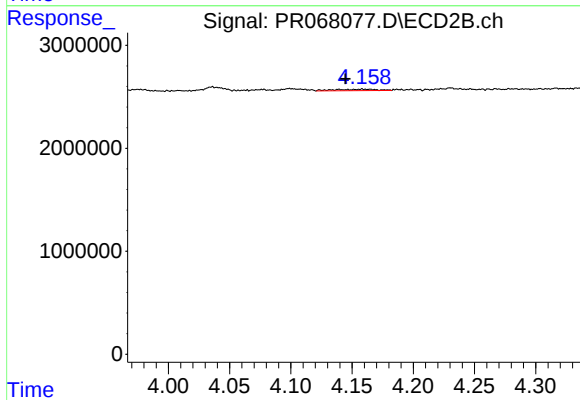


#3 AR-1016-1

R.T.: 4.158 min
Delta R.T.: 0.014 min
Response: 330900
Conc: 2.20 ng/ml

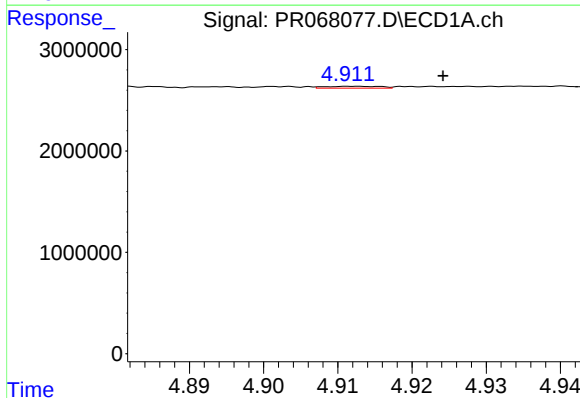


#4 AR-1016-2

R.T.: 4.913 min
Delta R.T.: -0.011 min
Response: 95593
Conc: 0.86 ng/ml

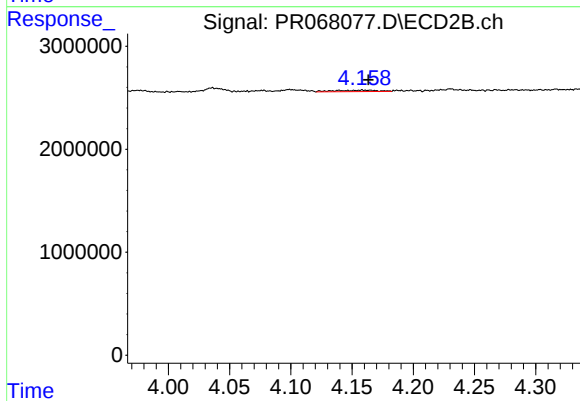

#4 AR-1016-2


R.T.: 4.158 min
Delta R.T.: -0.005 min
Response: 330900
Conc: 1.58 ng/ml

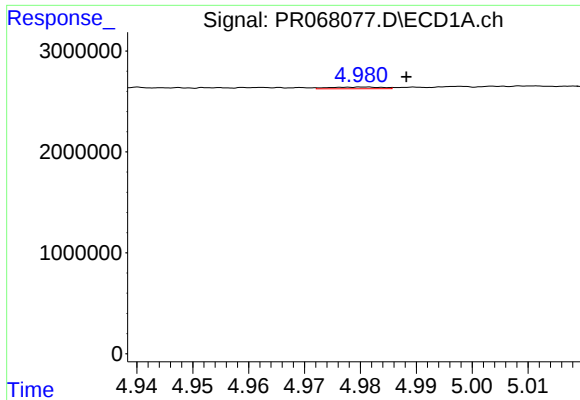

#5 AR-1016-3


R.T.: 4.981 min
Delta R.T.: -0.008 min
Response: 109701
Conc: 1.43 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

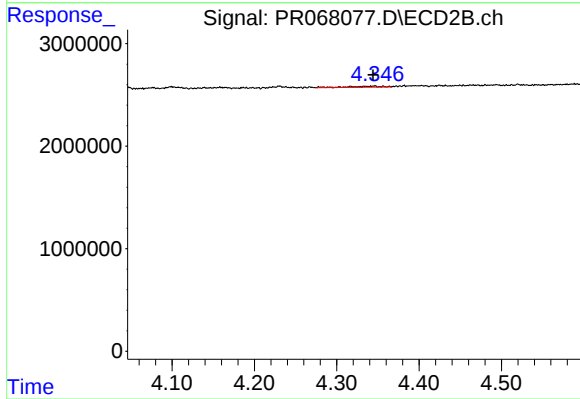


#5 AR-1016-3

R.T.: 4.346 min
Delta R.T.: 0.002 min
Response: 302317
Conc: 2.65 ng/ml

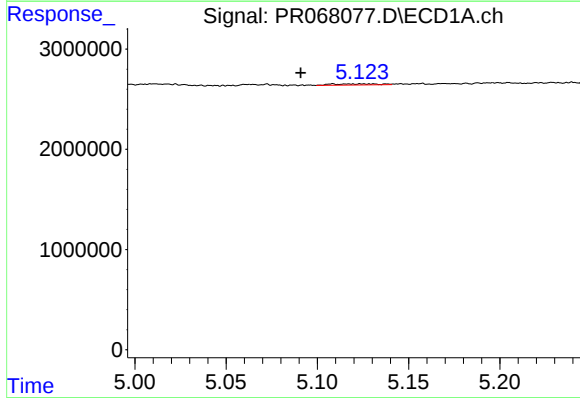


#6 AR-1016-4

R.T.: 5.108 min
Delta R.T.: 0.017 min
Response: 190550
Conc: 3.04 ng/ml

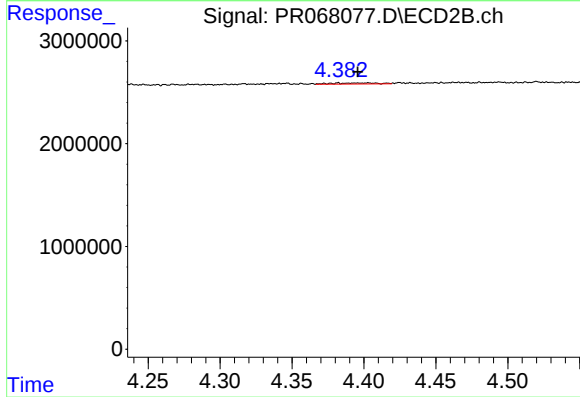

#6 AR-1016-4


R.T.: 4.382 min
Delta R.T.: -0.014 min
Response: 236916
Conc: 2.48 ng/ml

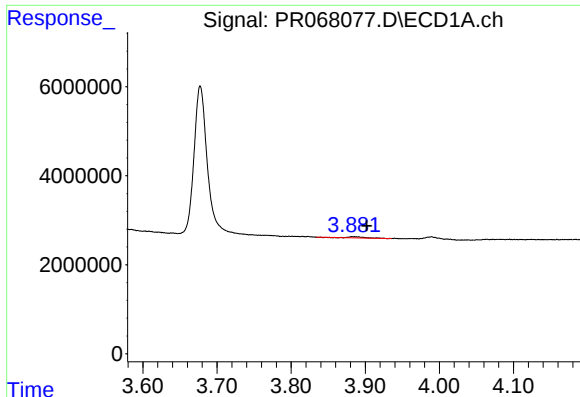

#8 AR-1221-1


R.T.: 3.883 min
Delta R.T.: -0.019 min
Response: 370568
Conc: 13.48 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

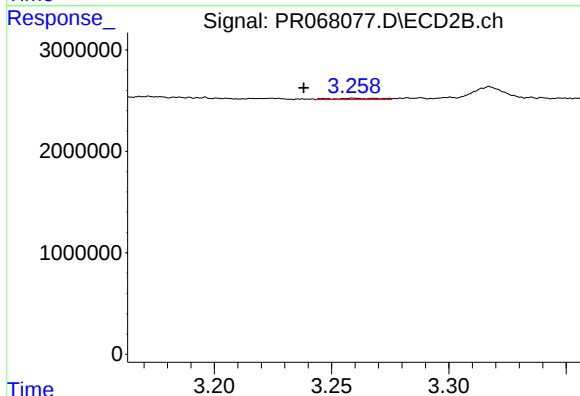


#8 AR-1221-1

R.T.: 3.260 min
Delta R.T.: 0.021 min
Response: 173771
Conc: 1.12 ng/ml

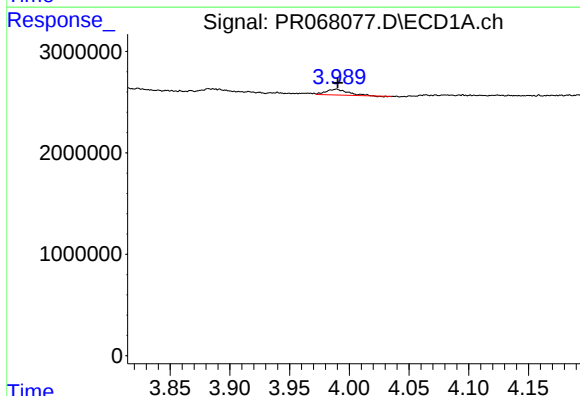


#9 AR-1221-2

R.T.: 3.989 min
Delta R.T.: -0.001 min
Response: 711844
Conc: 31.68 ng/ml

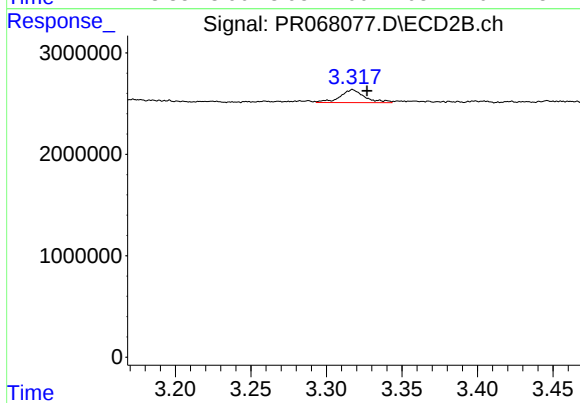

#9 AR-1221-2


R.T.: 3.317 min
Delta R.T.: -0.010 min
Response: 1435279
Conc: 19.54 ng/ml

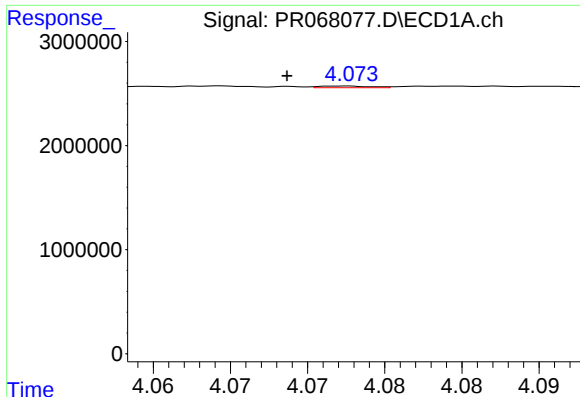

#10 AR-1221-3


R.T.: 4.072 min
Delta R.T.: 0.004 min
Response: 37170
Conc: 0.52 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

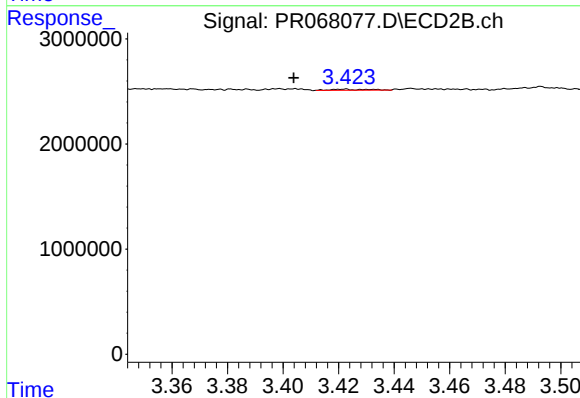


#10 AR-1221-3

R.T.: 3.422 min
Delta R.T.: 0.018 min
Response: 96641
Conc: 0.30 ng/ml

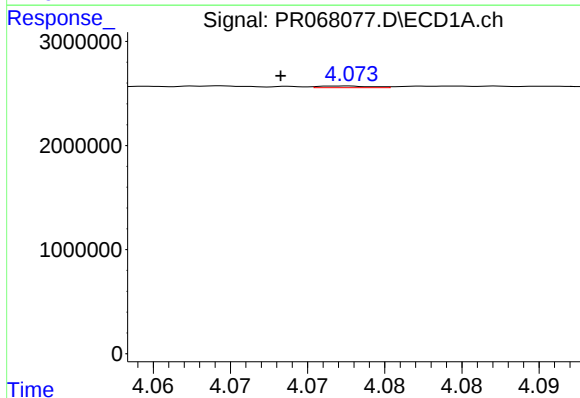


#11 AR-1232-1

R.T.: 4.072 min
Delta R.T.: 0.004 min
Response: 37170
Conc: 0.63 ng/ml

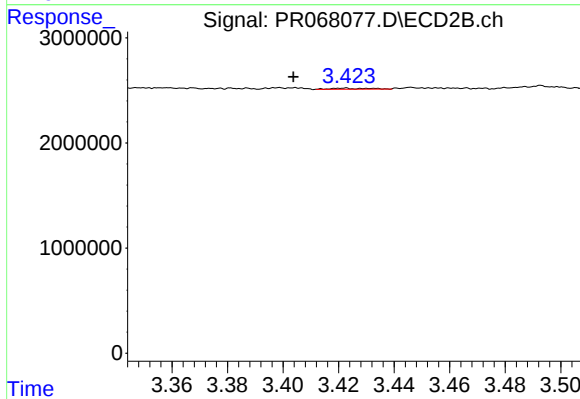

#11 AR-1232-1


R.T.: 3.422 min
Delta R.T.: 0.018 min
Response: 96641
Conc: 0.95 ng/ml

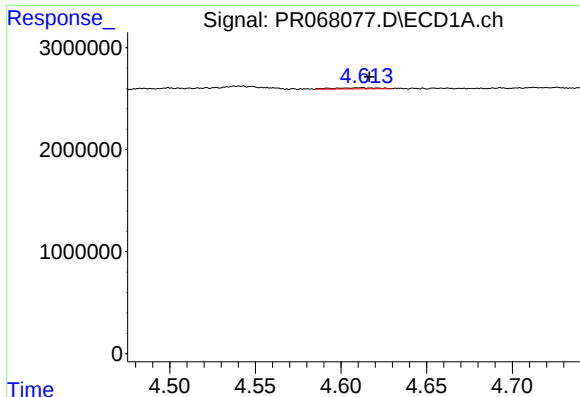

#12 AR-1232-2


R.T.: 4.612 min
Delta R.T.: -0.005 min
Response: 172378
Conc: 5.49 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

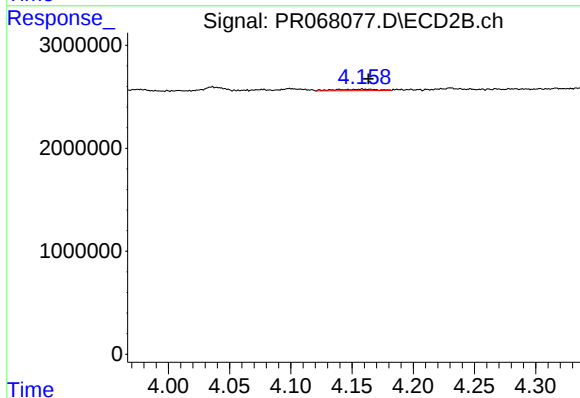


#12 AR-1232-2

R.T.: 4.158 min
Delta R.T.: -0.005 min
Response: 330900
Conc: 3.28 ng/ml

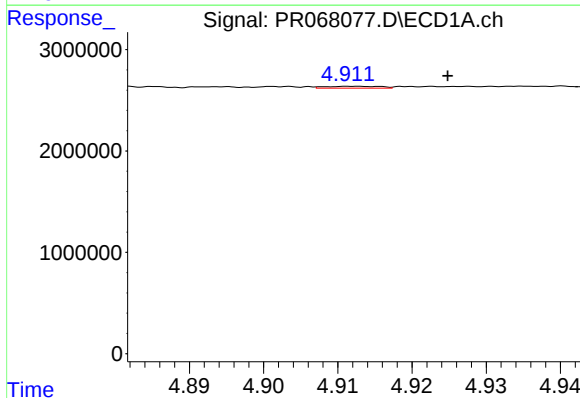


#13 AR-1232-3

R.T.: 4.913 min
Delta R.T.: -0.012 min
Response: 95593
Conc: 1.77 ng/ml

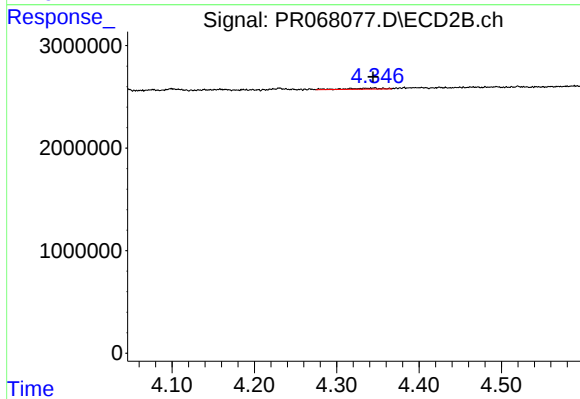

#13 AR-1232-3


R.T.: 4.346 min
Delta R.T.: 0.002 min
Response: 302317
Conc: 5.57 ng/ml

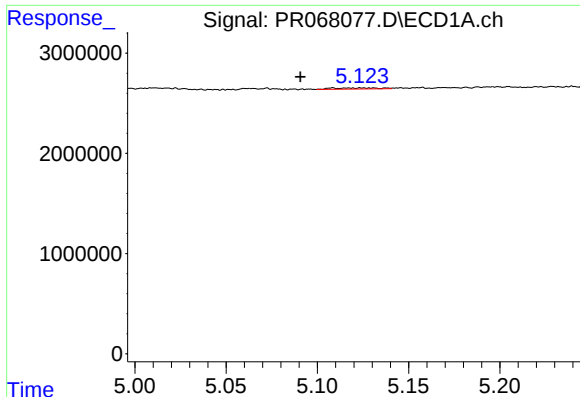

#14 AR-1232-4


R.T.: 5.108 min
Delta R.T.: 0.018 min
Response: 190550
Conc: 6.37 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

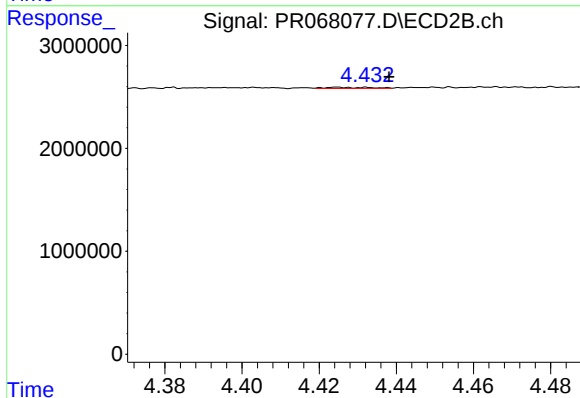


#14 AR-1232-4

R.T.: 4.425 min
Delta R.T.: -0.013 min
Response: 82456
Conc: 1.65 ng/ml

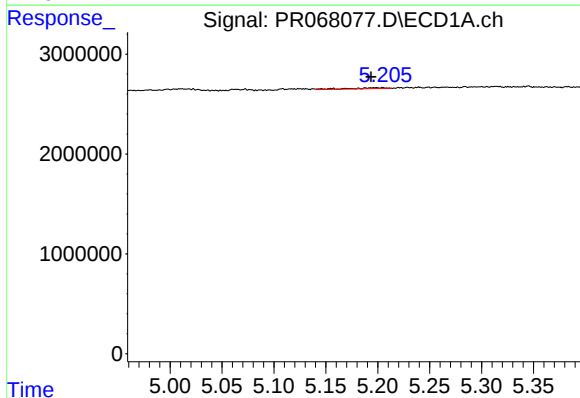


#15 AR-1232-5

R.T.: 5.198 min
Delta R.T.: 0.005 min
Response: 236007
Conc: 15.32 ng/ml

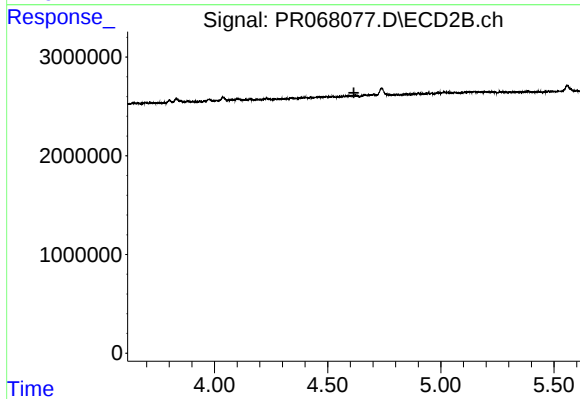

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T.: 4.616 min
Response: 0
Conc: N.D.

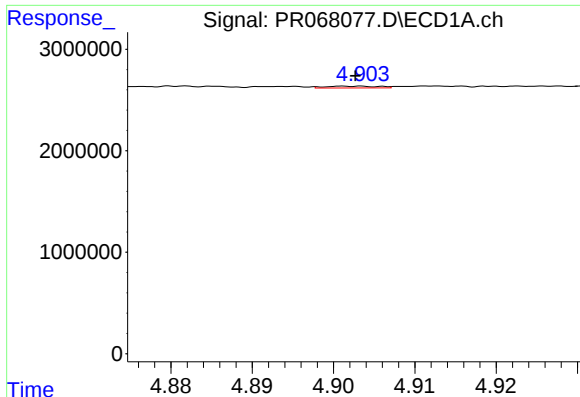

#16 AR-1242-1


R.T.: 4.903 min
Delta R.T.: 0.000 min
Response: 80003
Conc: 1.64 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

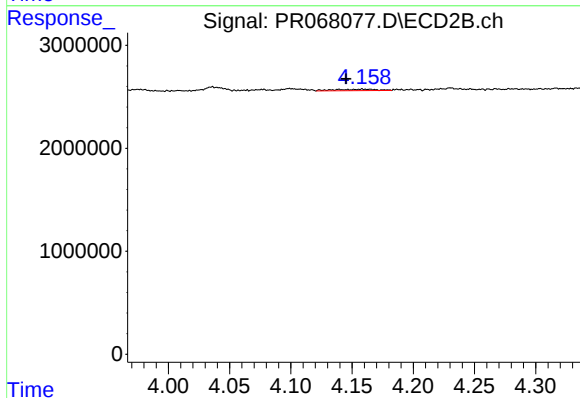


#16 AR-1242-1

R.T.: 4.158 min
Delta R.T.: 0.013 min
Response: 330900
Conc: 2.17 ng/ml

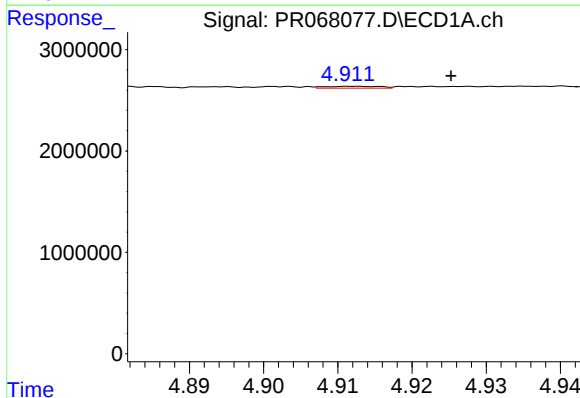


#17 AR-1242-2

R.T.: 4.913 min
Delta R.T.: -0.013 min
Response: 95593
Conc: 1.05 ng/ml

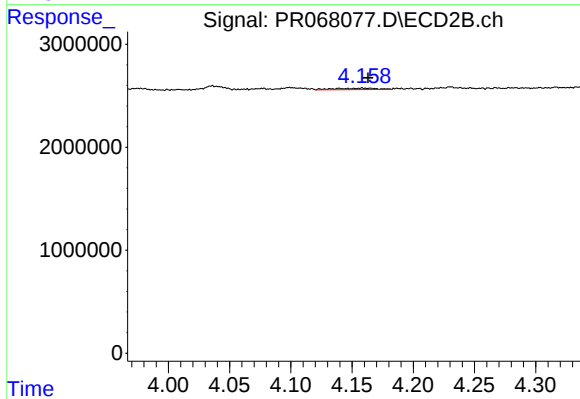

#17 AR-1242-2


R.T.: 4.158 min
Delta R.T.: -0.005 min
Response: 330900
Conc: 1.55 ng/ml

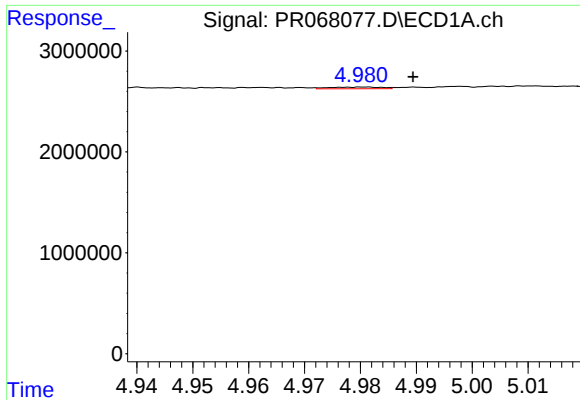

#18 AR-1242-3


R.T.: 4.981 min
Delta R.T.: -0.009 min
Response: 109701
Conc: 1.75 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

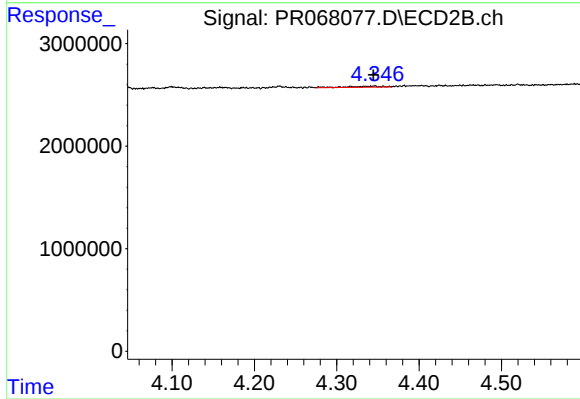


#18 AR-1242-3

R.T.: 4.346 min
Delta R.T.: 0.002 min
Response: 302317
Conc: 2.85 ng/ml

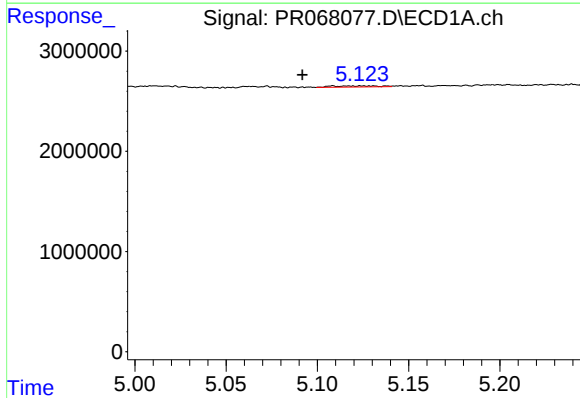


#19 AR-1242-4

R.T.: 5.108 min
Delta R.T.: 0.016 min
Response: 190550
Conc: 3.82 ng/ml

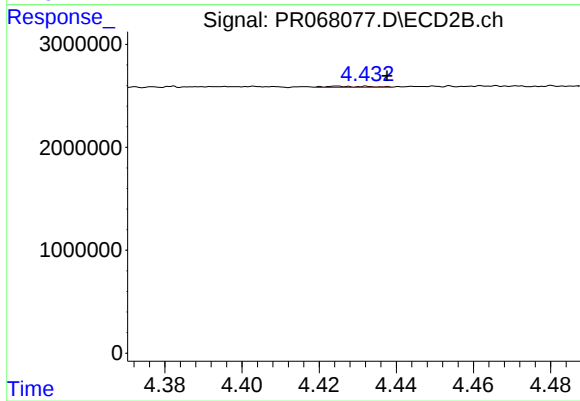

#19 AR-1242-4


R.T.: 4.425 min
Delta R.T.: -0.013 min
Response: 82456
Conc: 0.82 ng/ml

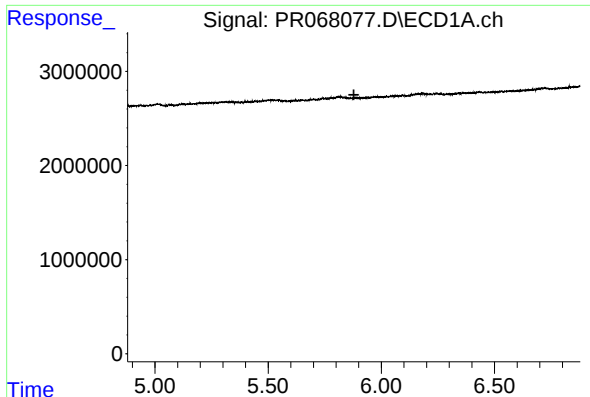

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 5.879 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

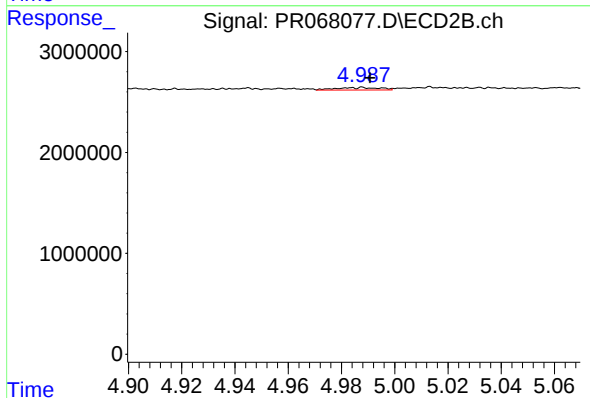


#20 AR-1242-5

R.T.: 4.987 min
Delta R.T.: -0.004 min
Response: 284802
Conc: 1.82 ng/ml

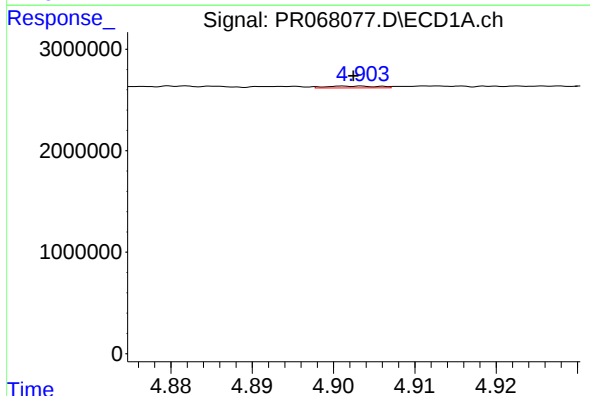


#21 AR-1248-1

R.T.: 4.903 min
Delta R.T.: 0.000 min
Response: 80003
Conc: 2.08 ng/ml

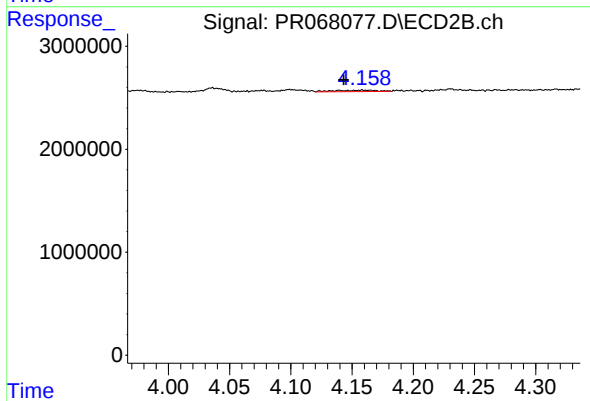

#21 AR-1248-1


R.T.: 4.158 min
Delta R.T.: 0.015 min
Response: 330900
Conc: 2.78 ng/ml

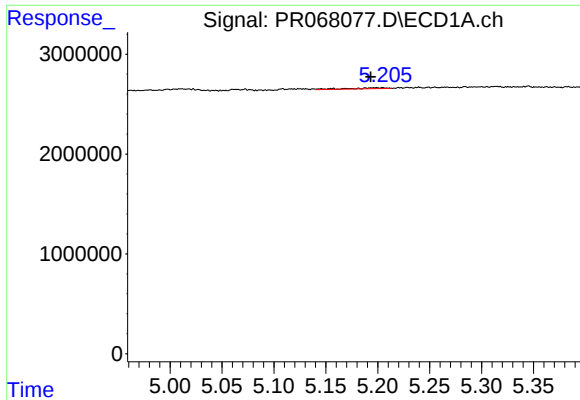

#22 AR-1248-2


R.T.: 5.198 min
Delta R.T.: 0.005 min
Response: 236007
Conc: 4.50 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

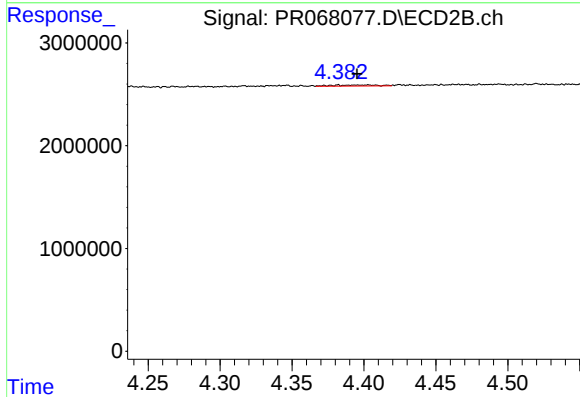


#22 AR-1248-2

R.T.: 4.382 min
Delta R.T.: -0.013 min
Response: 236916
Conc: 1.26 ng/ml

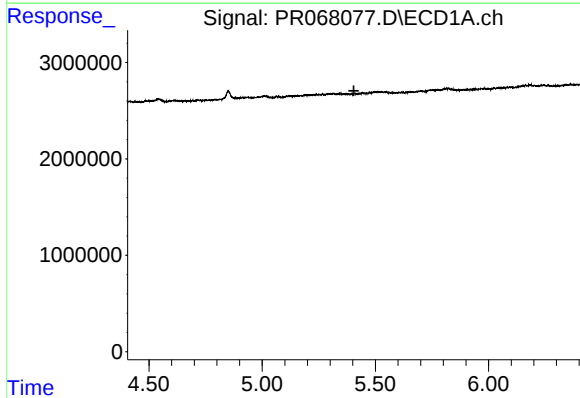


#23 AR-1248-3

R.T.: 0.000 min
Exp R.T. : 5.405 min
Response: 0
Conc: N.D.

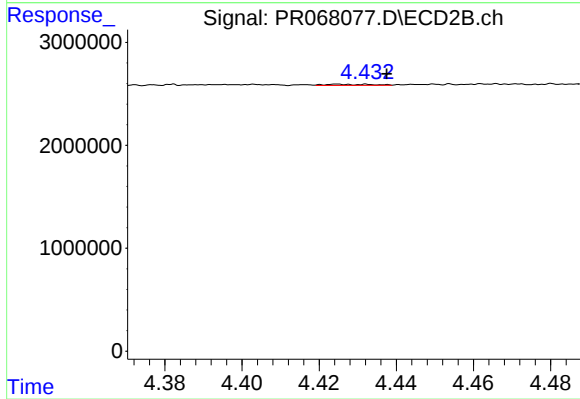

#23 AR-1248-3


R.T.: 4.425 min
Delta R.T.: -0.012 min
Response: 82456
Conc: 0.43 ng/ml

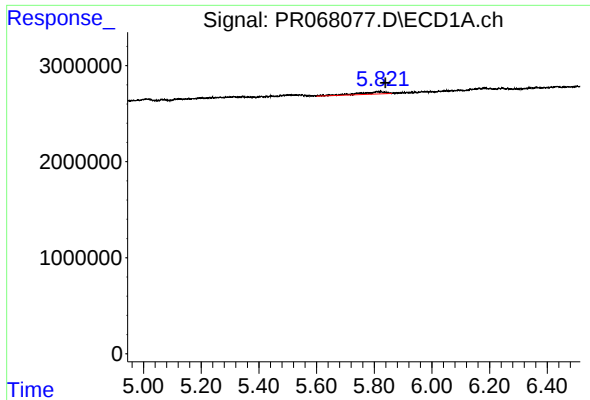

#24 AR-1248-4


R.T.: 5.823 min
Delta R.T.: -0.016 min
Response: 1702651
Conc: 22.90 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

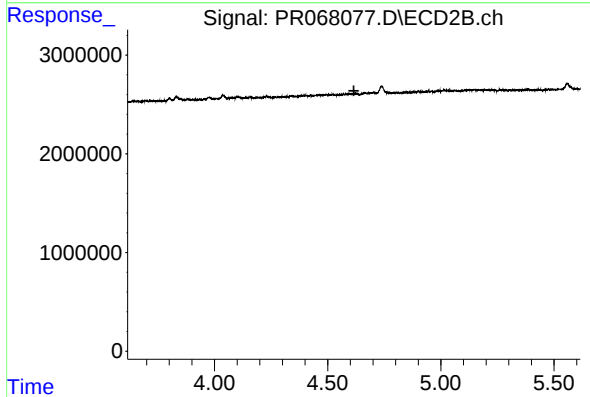


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 4.616 min
Response: 0
Conc: N.D.

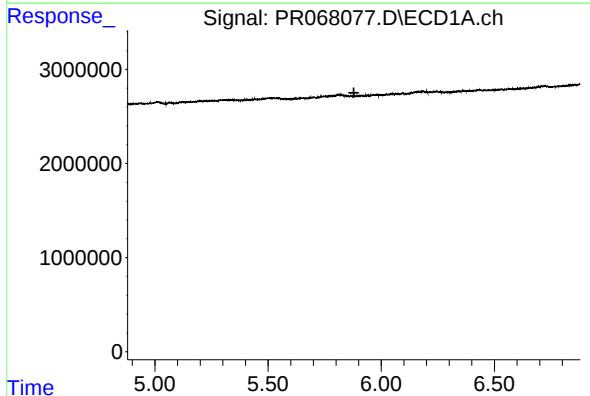


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 5.879 min
Response: 0
Conc: N.D.

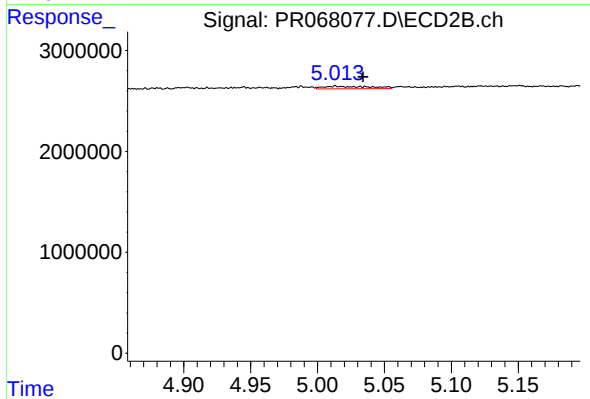

#25 AR-1248-5


R.T.: 5.014 min
Delta R.T.: -0.020 min
Response: 617940
Conc: 2.91 ng/ml

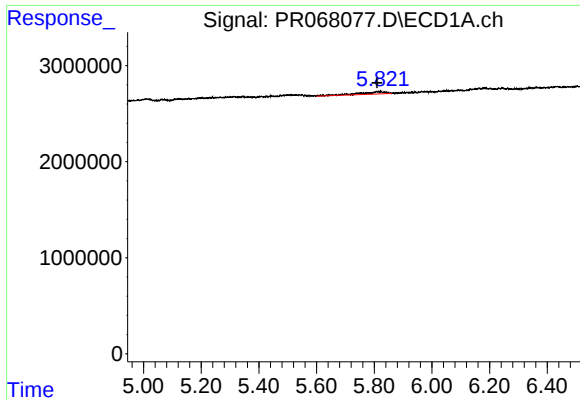

#26 AR-1254-1


R.T.: 5.823 min
Delta R.T.: 0.013 min
Response: 1702651
Conc: 23.86 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

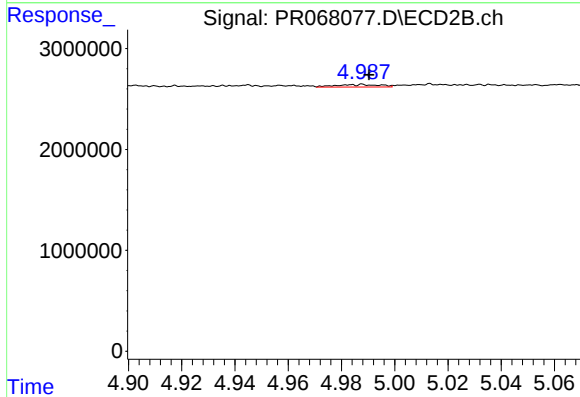


#26 AR-1254-1

R.T.: 4.987 min
Delta R.T.: -0.003 min
Response: 284802
Conc: 1.11 ng/ml

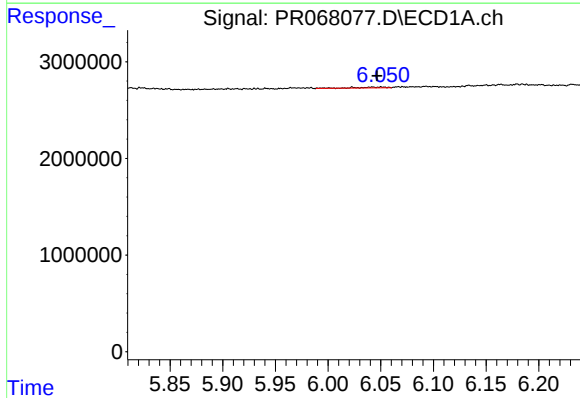


#27 AR-1254-2

R.T.: 6.051 min
Delta R.T.: 0.004 min
Response: 142297
Conc: 1.27 ng/ml

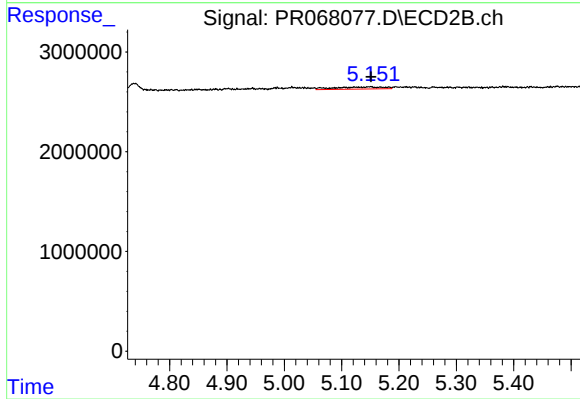

#27 AR-1254-2


R.T.: 5.149 min
Delta R.T.: -0.002 min
Response: 1280127
Conc: 5.57 ng/ml

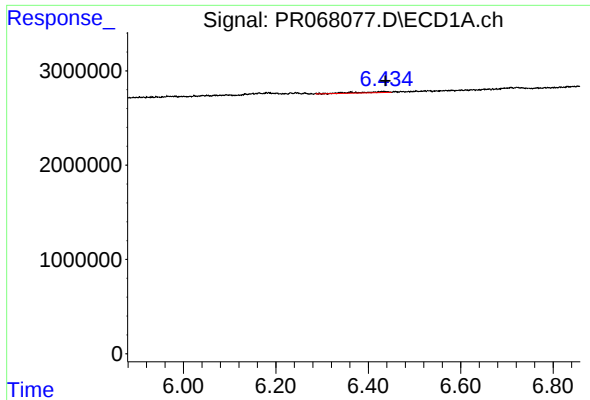

#28 AR-1254-3


R.T.: 6.434 min
Delta R.T.: -0.003 min
Response: 518123
Conc: 3.86 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

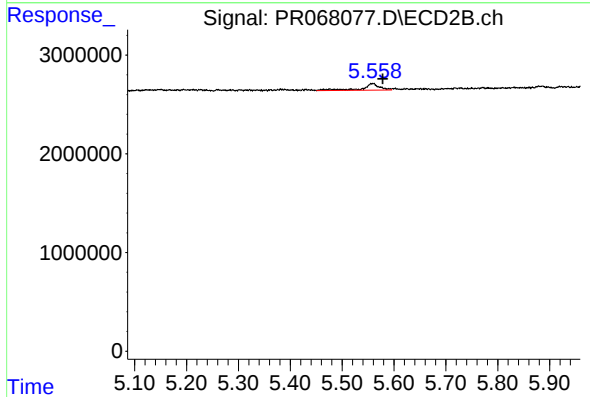


#28 AR-1254-3

R.T.: 5.559 min
Delta R.T.: -0.019 min
Response: 1591417
Conc: 4.41 ng/ml

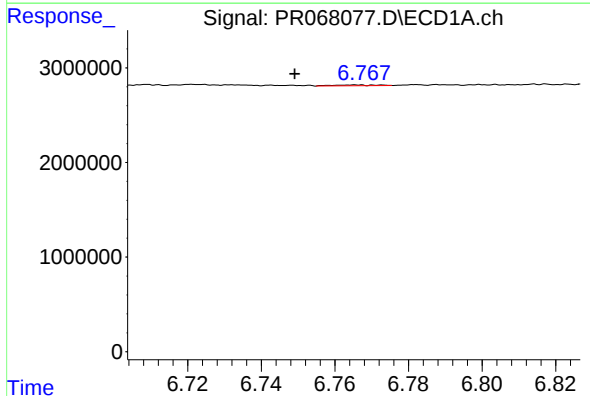


#29 AR-1254-4

R.T.: 6.766 min
Delta R.T.: 0.017 min
Response: 68880
Conc: 0.66 ng/ml

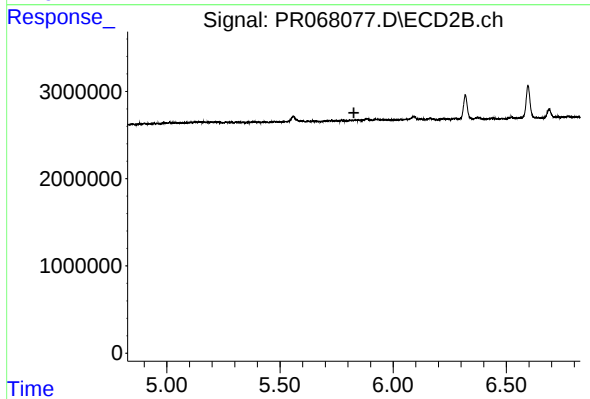

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T.: 5.826 min
Response: 0
Conc: N.D.

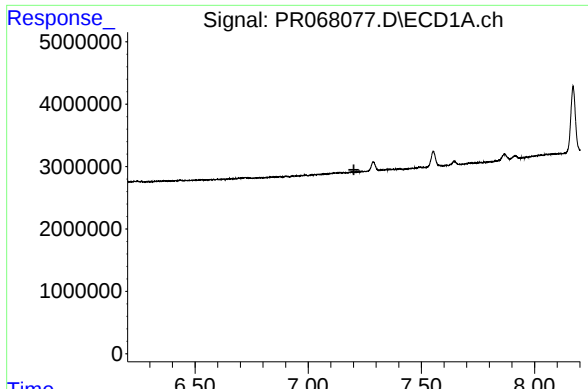

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T.: 7.202 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

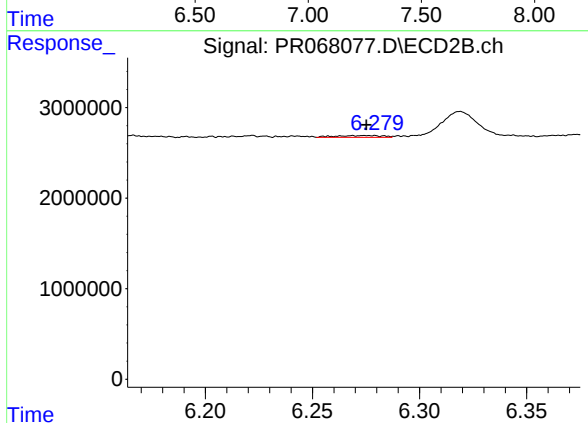


#30 AR-1254-5

R.T.: 6.275 min
Delta R.T.: 0.000 min
Response: 299875
Conc: 0.91 ng/ml

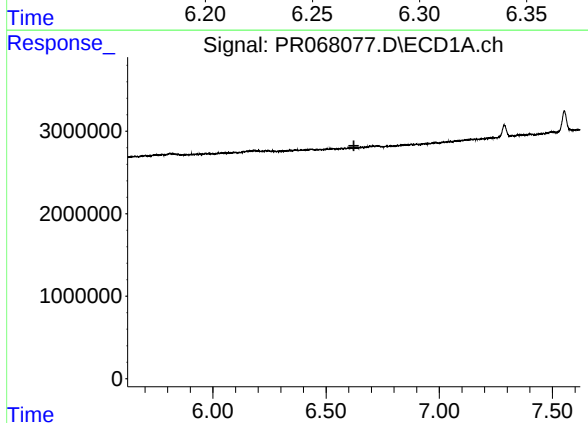


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T.: 6.623 min
Response: 0
Conc: N.D.

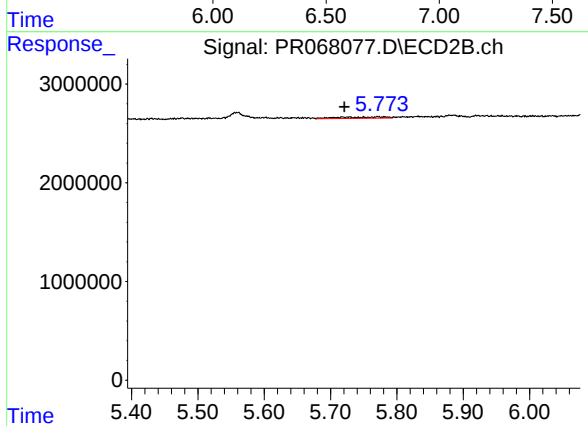

#31 AR-1260-1


R.T.: 5.728 min
Delta R.T.: 0.007 min
Response: 650893
Conc: 2.66 ng/ml

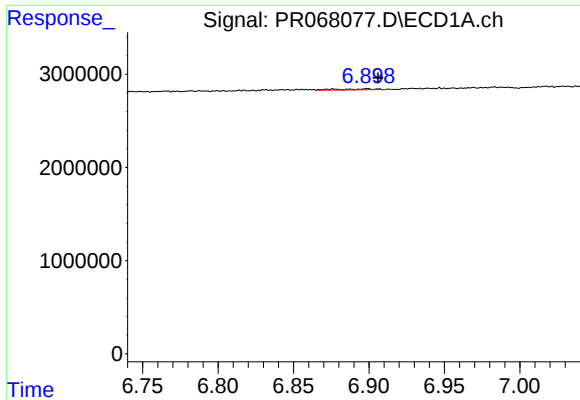

#32 AR-1260-2


R.T.: 6.899 min
Delta R.T.: -0.007 min
Response: 194712
Conc: 1.37 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

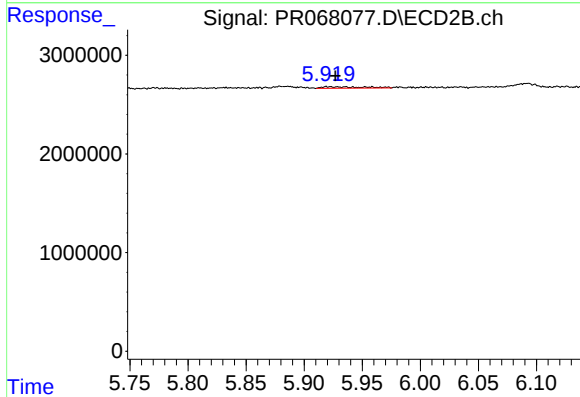


#32 AR-1260-2

R.T.: 5.922 min
Delta R.T.: -0.005 min
Response: 372815
Conc: 1.28 ng/ml

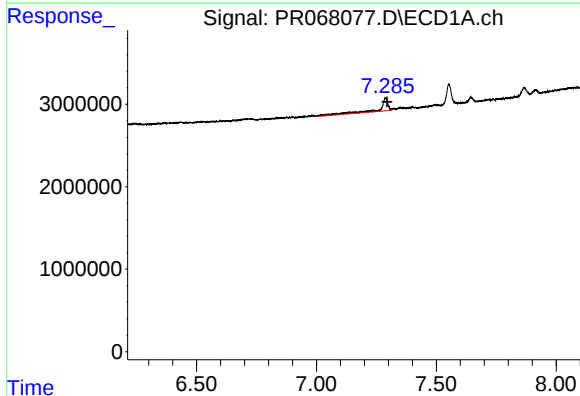


#33 AR-1260-3

R.T.: 7.287 min
Delta R.T.: -0.008 min
Response: 3892010
Conc: 28.11 ng/ml

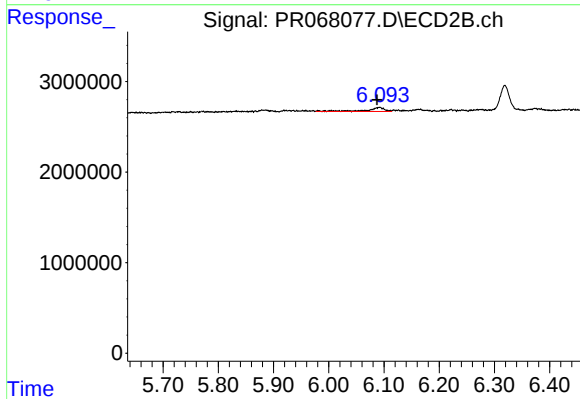

#33 AR-1260-3


R.T.: 6.091 min
Delta R.T.: 0.003 min
Response: 1006300
Conc: 3.66 ng/ml

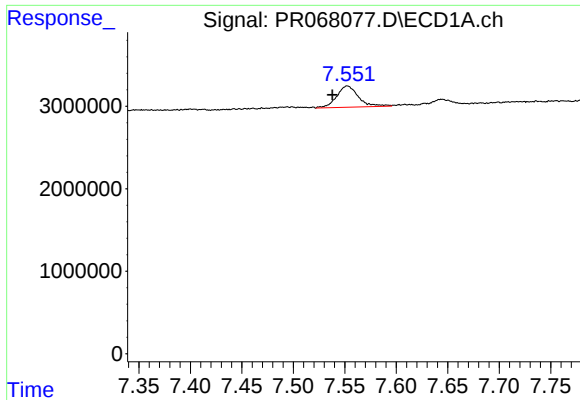

#34 AR-1260-4


R.T.: 7.553 min
Delta R.T.: 0.015 min
Response: 3760299
Conc: 29.67 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

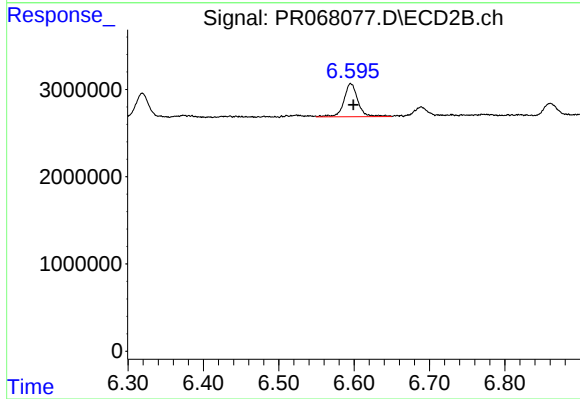


#34 AR-1260-4

R.T.: 6.596 min
Delta R.T.: -0.003 min
Response: 4864580
Conc: 23.20 ng/ml

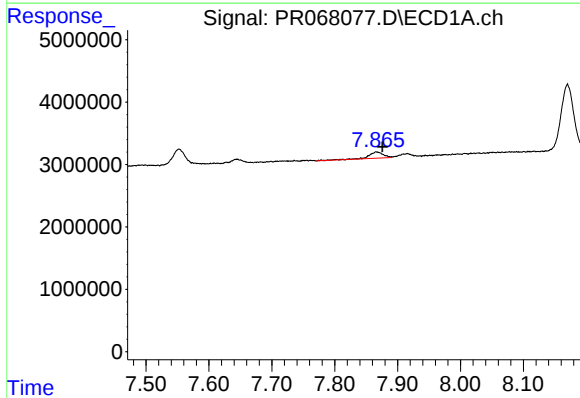


#35 AR-1260-5

R.T.: 7.867 min
Delta R.T.: -0.009 min
Response: 1675274
Conc: 4.60 ng/ml

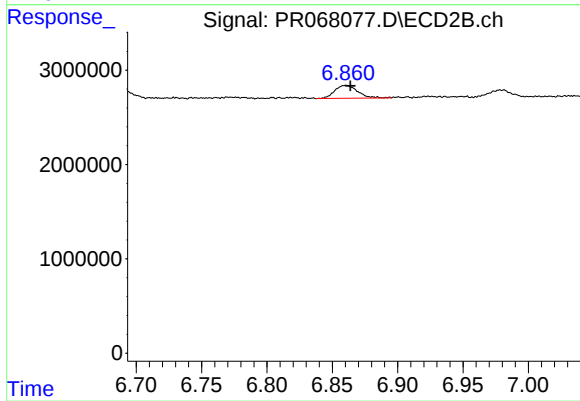

#35 AR-1260-5


R.T.: 6.860 min
Delta R.T.: -0.003 min
Response: 1681631
Conc: 3.47 ng/ml

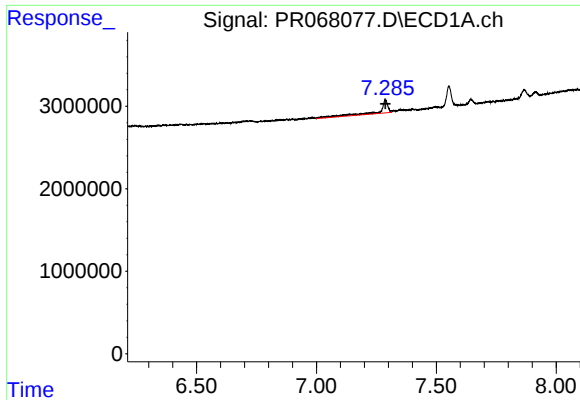

#36 AR-1262-1


R.T.: 7.287 min
Delta R.T.: -0.001 min
Response: 3892010
Conc: 19.54 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

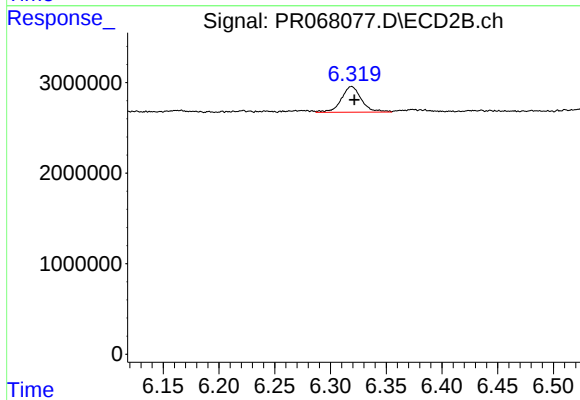


#36 AR-1262-1

R.T.: 6.319 min
Delta R.T.: -0.002 min
Response: 3561737
Conc: 10.31 ng/ml

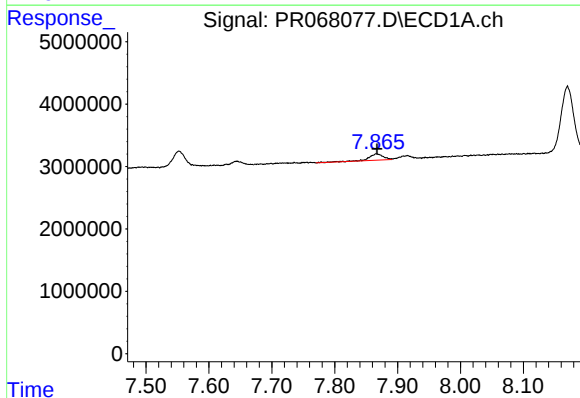


#37 AR-1262-2

R.T.: 7.867 min
Delta R.T.: 0.000 min
Response: 1675274
Conc: 3.87 ng/ml

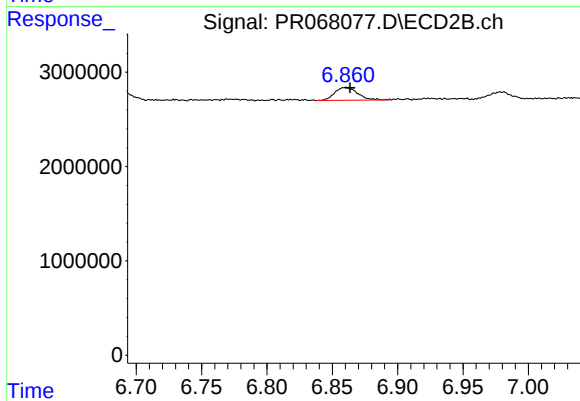

#37 AR-1262-2


R.T.: 6.860 min
Delta R.T.: -0.003 min
Response: 1681631
Conc: 2.76 ng/ml

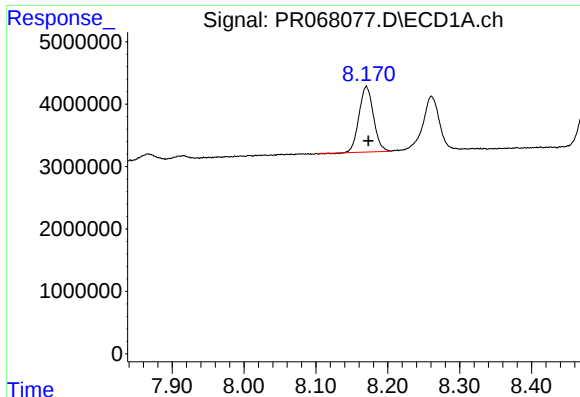

#38 AR-1262-3


R.T.: 8.170 min
Delta R.T.: -0.003 min
Response: 14588519
Conc: 46.59 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

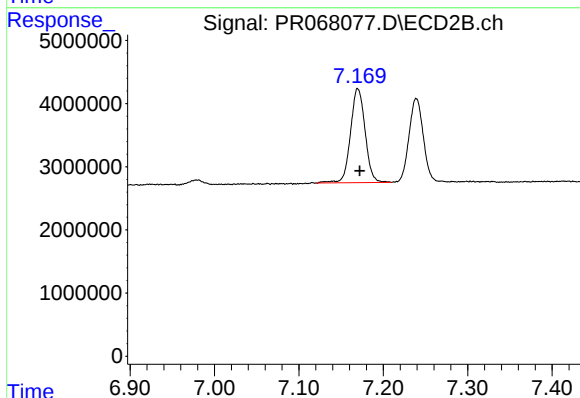


#38 AR-1262-3

R.T.: 7.170 min
Delta R.T.: -0.002 min
Response: 17886241
Conc: 74.91 ng/ml

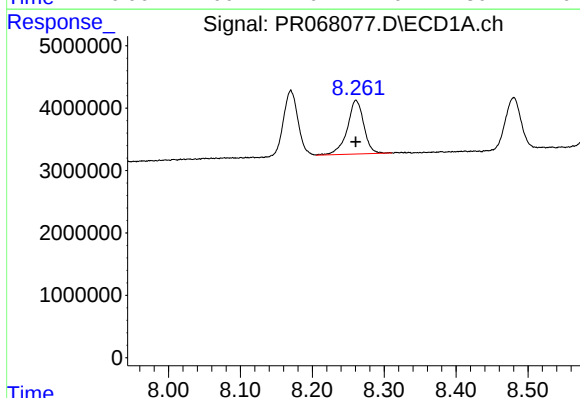


#39 AR-1262-4

R.T.: 8.261 min
Delta R.T.: 0.000 min
Response: 13783971
Conc: 50.20 ng/ml

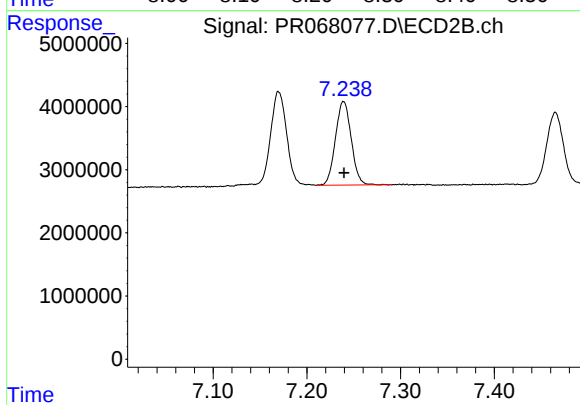

#39 AR-1262-4


R.T.: 7.239 min
Delta R.T.: 0.000 min
Response: 15532647
Conc: 34.95 ng/ml

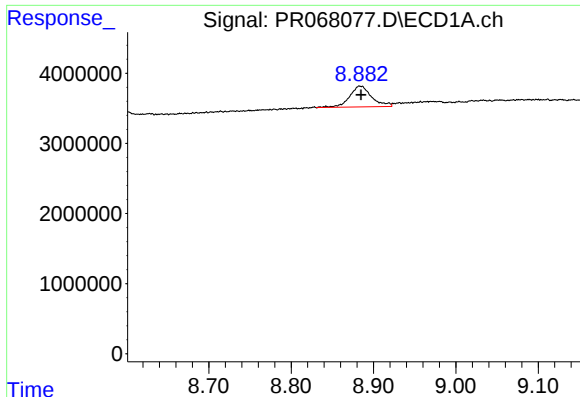

#40 AR-1262-5


R.T.: 8.884 min
Delta R.T.: 0.000 min
Response: 5538254
Conc: 29.26 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

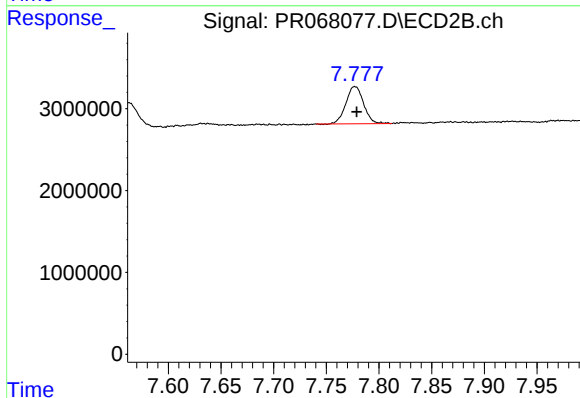


#40 AR-1262-5

R.T.: 7.777 min
Delta R.T.: -0.002 min
Response: 5312280
Conc: 26.08 ng/ml

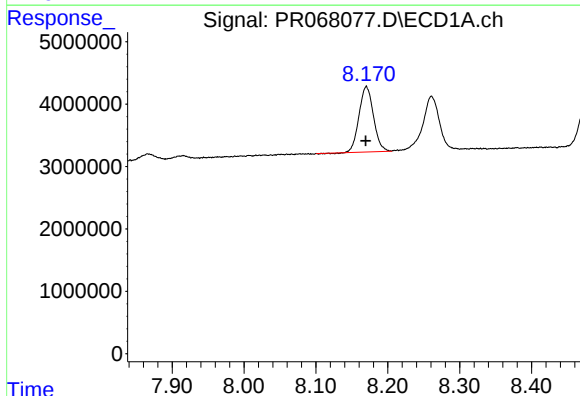


#41 AR-1268-1

R.T.: 8.170 min
Delta R.T.: 0.000 min
Response: 14588519
Conc: 24.19 ng/ml

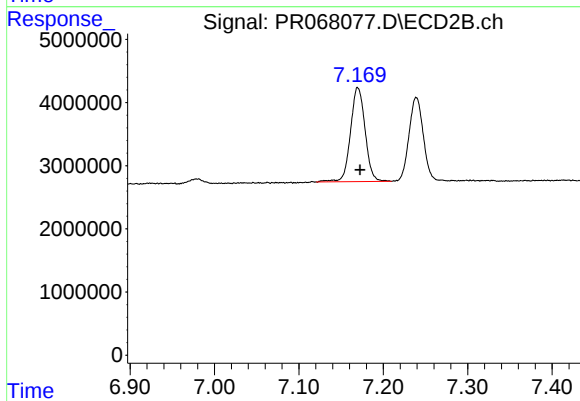

#41 AR-1268-1


R.T.: 7.170 min
Delta R.T.: -0.002 min
Response: 17886241
Conc: 24.23 ng/ml

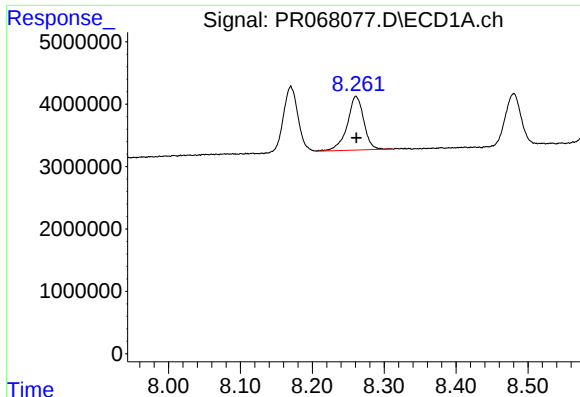

#42 AR-1268-2


R.T.: 8.261 min
Delta R.T.: 0.000 min
Response: 13783971
Conc: 24.19 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

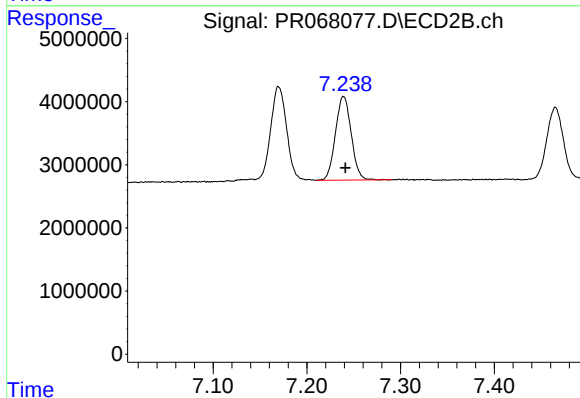


#42 AR-1268-2

R.T.: 7.239 min
Delta R.T.: -0.002 min
Response: 15532647
Conc: 23.01 ng/ml

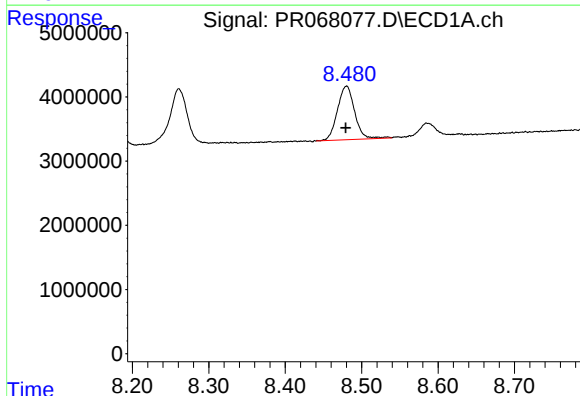


#43 AR-1268-3

R.T.: 8.480 min
Delta R.T.: 0.000 min
Response: 13043808
Conc: 23.50 ng/ml

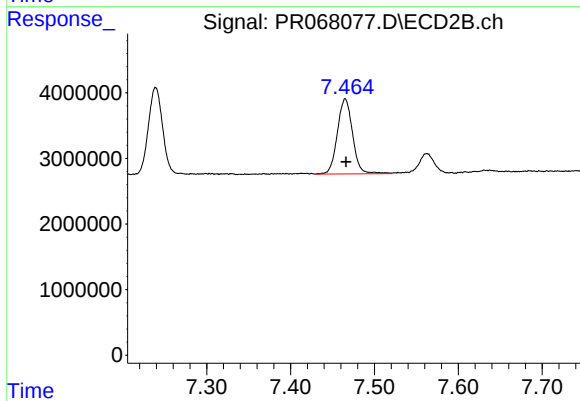

#43 AR-1268-3


R.T.: 7.465 min
Delta R.T.: -0.001 min
Response: 14459234
Conc: 23.45 ng/ml

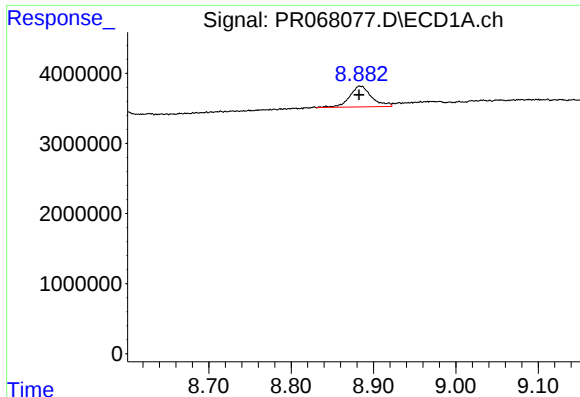

#44 AR-1268-4


R.T.: 8.884 min
Delta R.T.: 0.002 min
Response: 5538254
Conc: 27.34 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

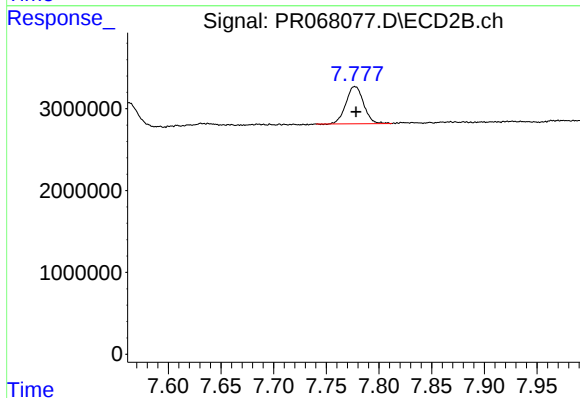


#44 AR-1268-4

R.T.: 7.777 min
Delta R.T.: 0.000 min
Response: 5312280
Conc: 25.47 ng/ml

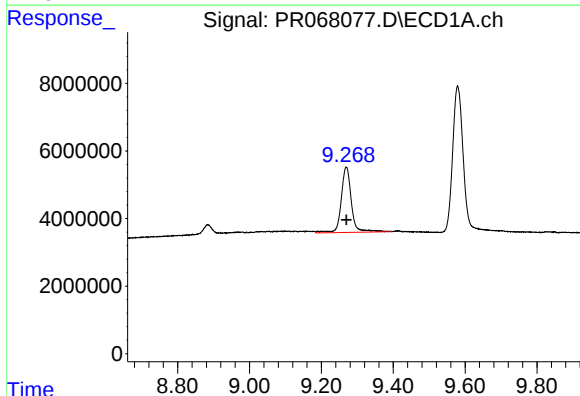

#45 AR-1268-5

R.T.: 9.269 min
Delta R.T.: 0.000 min
Response: 38028932
Conc: 24.32 ng/ml

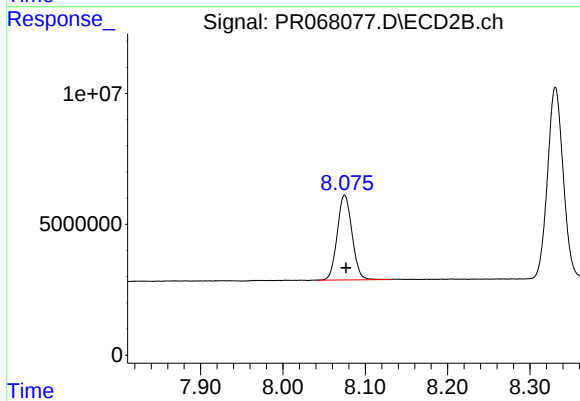

#45 AR-1268-5

R.T.: 8.075 min
Delta R.T.: -0.002 min
Response: 40415422
Conc: 28.30 ng/ml