

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR080724\
 Data File : PR068074.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Aug 2024 11:34
 Operator : AJ\MA
 Sample : P3390-09
 Misc : AR1248 MDL 25 PPB
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 07 17:11:11 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 07 00:26:28 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.677	3.011	39714558	76082554	15.612	17.448
2) SA Decachlor...	9.580	8.331	75162654	84522225	17.129	18.654
Target Compounds						
21) L5 AR-1248-1	4.901	4.142	819184	2290741	21.344	19.250
22) L5 AR-1248-2	5.193	4.393	1178124	3667957	22.460	19.462
23) L5 AR-1248-3	5.404	4.436	1517609	3627049	21.554	19.029
24) L5 AR-1248-4	5.838	4.614	1390310	4150351	18.698	19.220
25) L5 AR-1248-5	5.878	5.030	1475054	4403801	18.273	20.724



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR080724\
Data File : PR068074.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Aug 2024 11:34
Operator : AJ\MA
Sample : P3390-09
Misc : AR1248 MDL 25 PPB
ALS Vial : 60 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 17:11:11 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 07 00:26:28 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

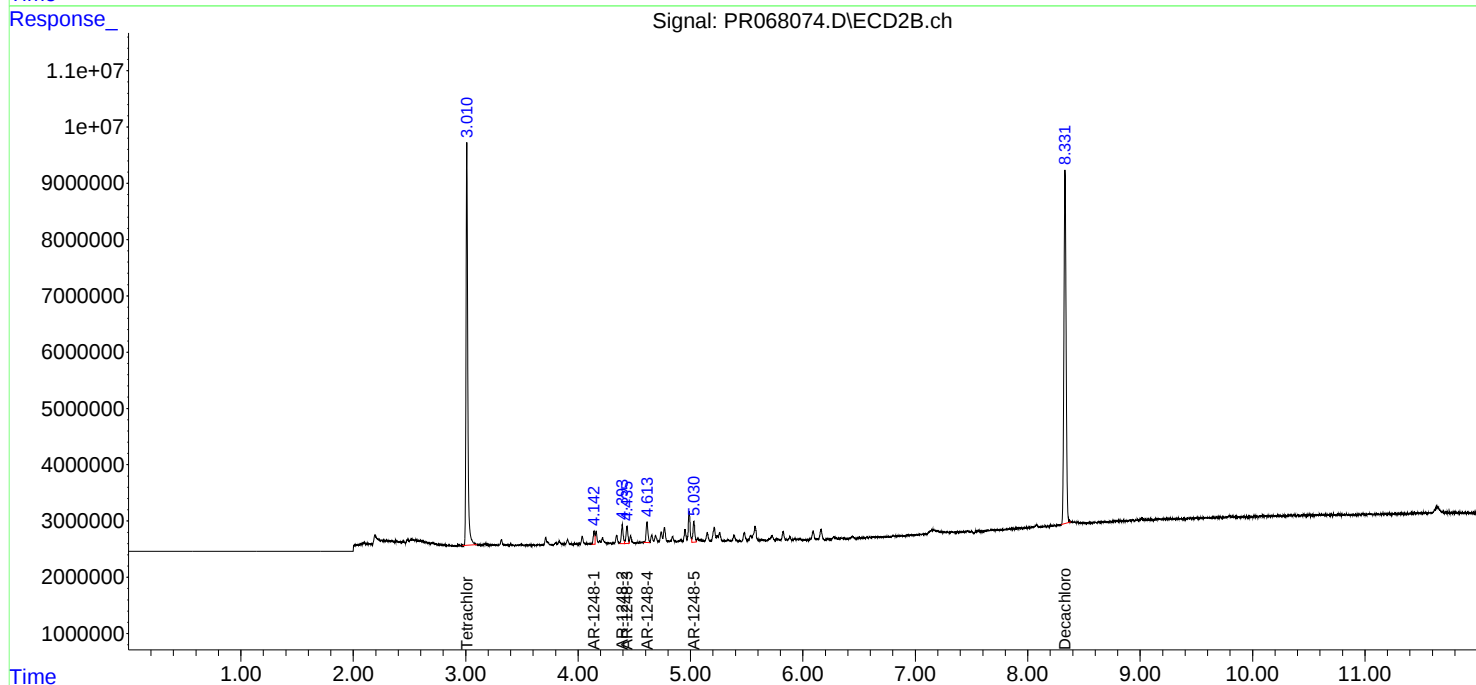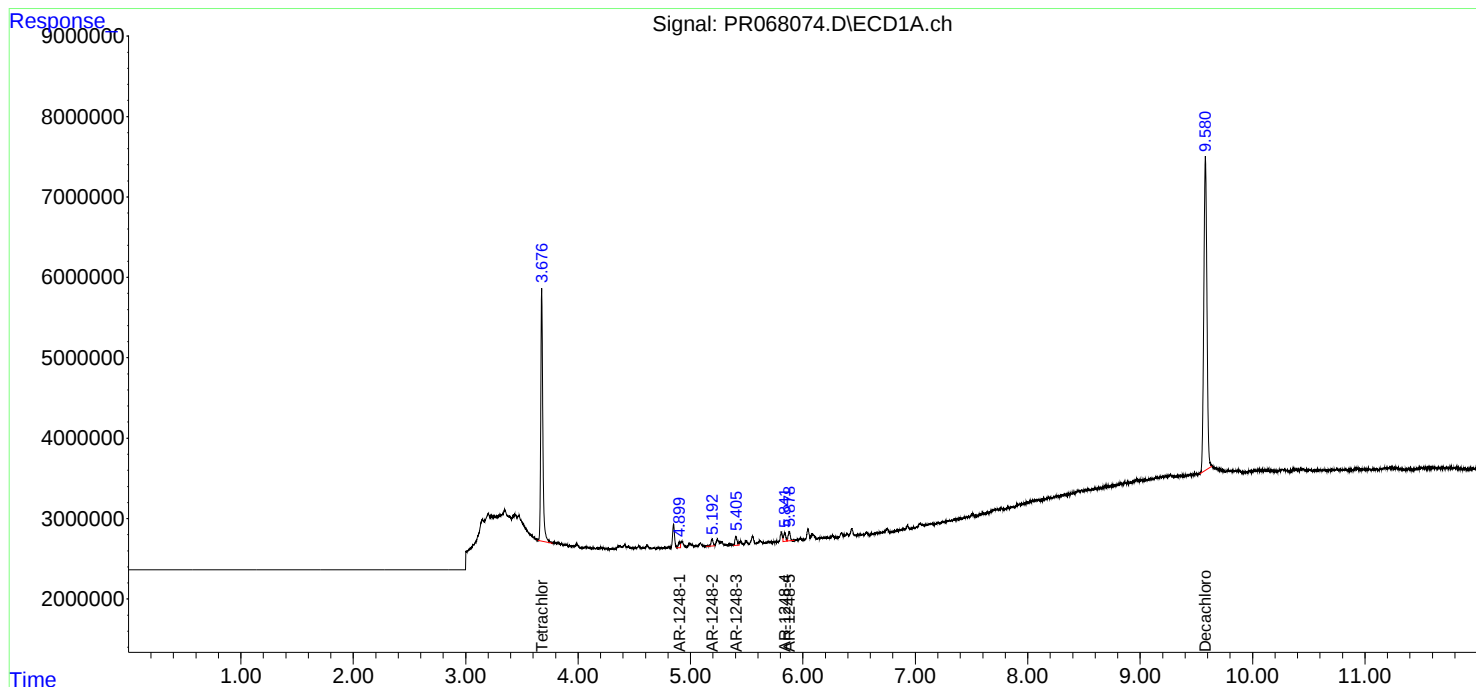


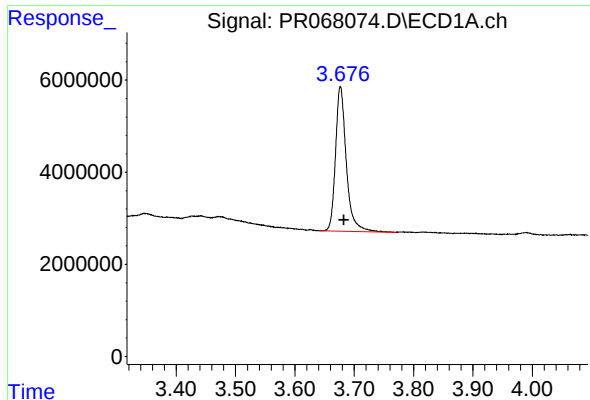

#1 Tetrachloro-m-xylene


R.T.: 3.677 min
Delta R.T.: -0.006 min
Response: 39714558
Conc: 15.61 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

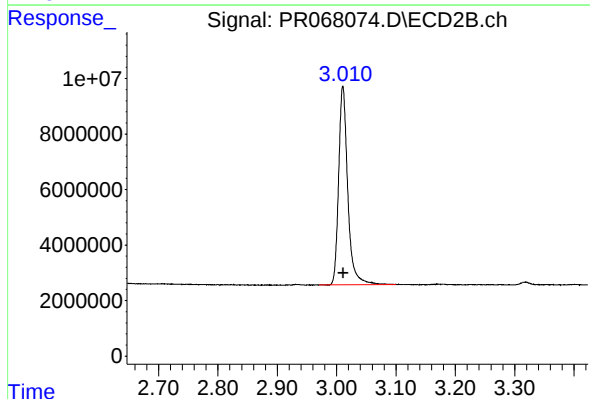


#1 Tetrachloro-m-xylene

R.T.: 3.011 min
Delta R.T.: 0.000 min
Response: 76082554
Conc: 17.45 ng/ml

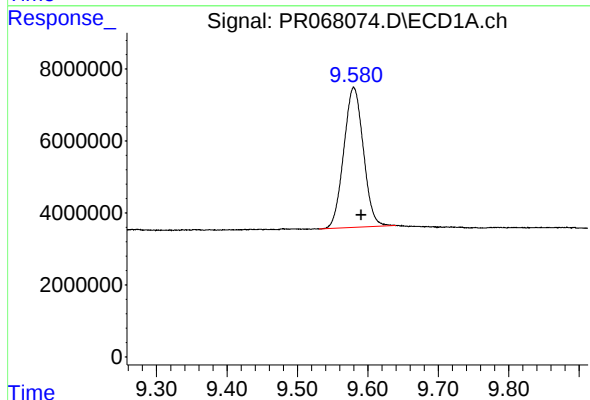


#2 Decachlorobiphenyl

R.T.: 9.580 min
Delta R.T.: -0.011 min
Response: 75162654
Conc: 17.13 ng/ml

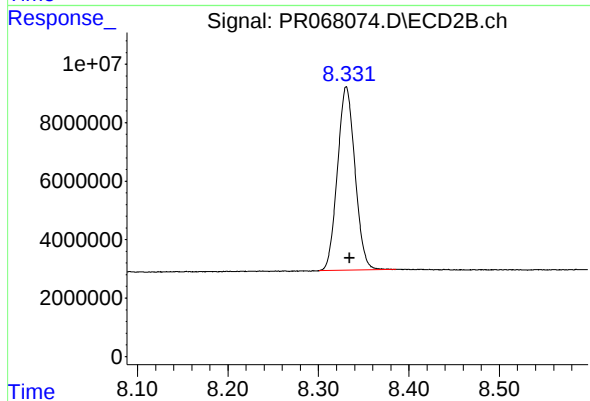

#2 Decachlorobiphenyl


R.T.: 8.331 min
Delta R.T.: -0.004 min
Response: 84522225
Conc: 18.65 ng/ml

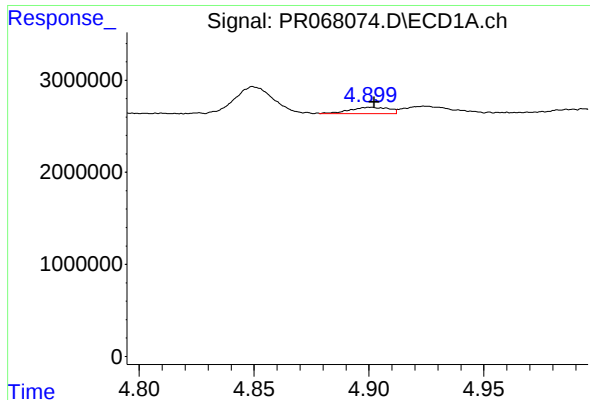

#21 AR-1248-1


R.T.: 4.901 min
Delta R.T.: -0.001 min
Response: 819184
Conc: 21.34 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

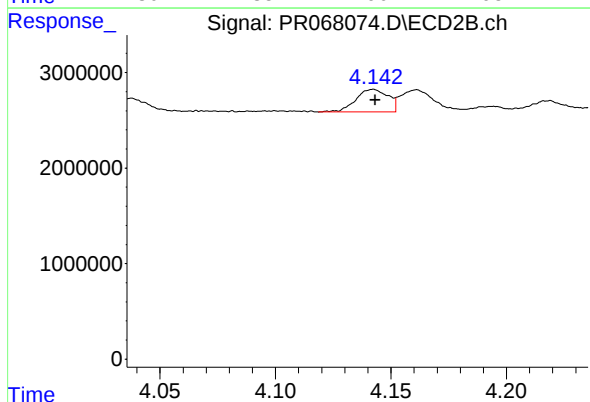


#21 AR-1248-1

R.T.: 4.142 min
Delta R.T.: -0.001 min
Response: 2290741
Conc: 19.25 ng/ml

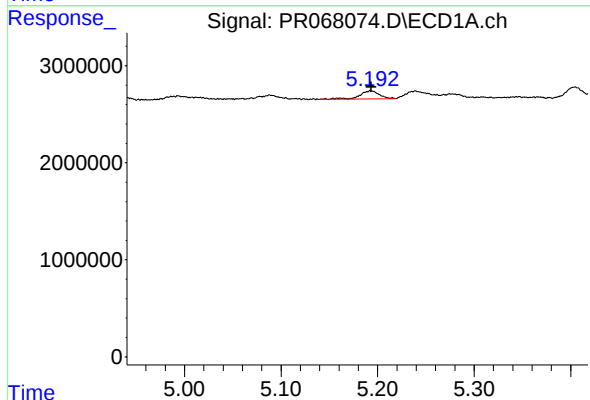


#22 AR-1248-2

R.T.: 5.193 min
Delta R.T.: 0.000 min
Response: 1178124
Conc: 22.46 ng/ml

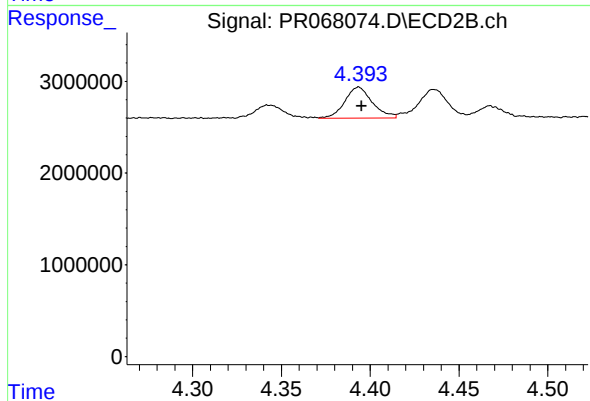

#22 AR-1248-2


R.T.: 4.393 min
Delta R.T.: -0.002 min
Response: 3667957
Conc: 19.46 ng/ml

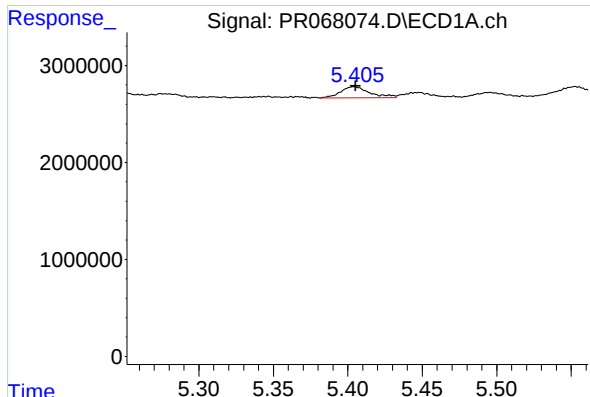

#23 AR-1248-3


R.T.: 5.404 min
Delta R.T.: -0.001 min
Response: 1517609
Conc: 21.55 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

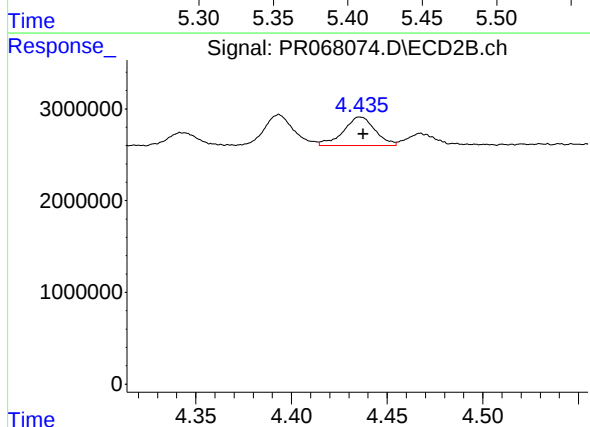


#23 AR-1248-3

R.T.: 4.436 min
Delta R.T.: -0.002 min
Response: 3627049
Conc: 19.03 ng/ml

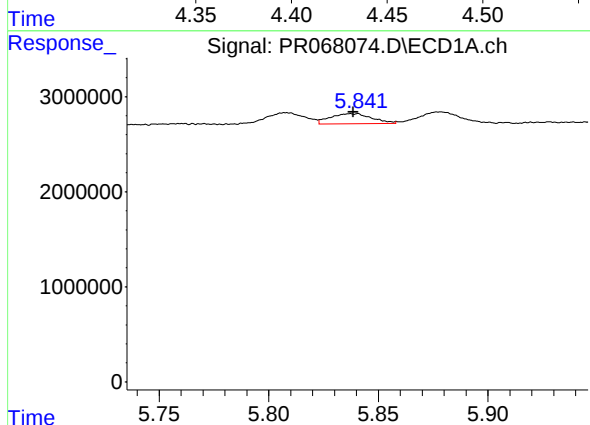


#24 AR-1248-4

R.T.: 5.838 min
Delta R.T.: 0.000 min
Response: 1390310
Conc: 18.70 ng/ml

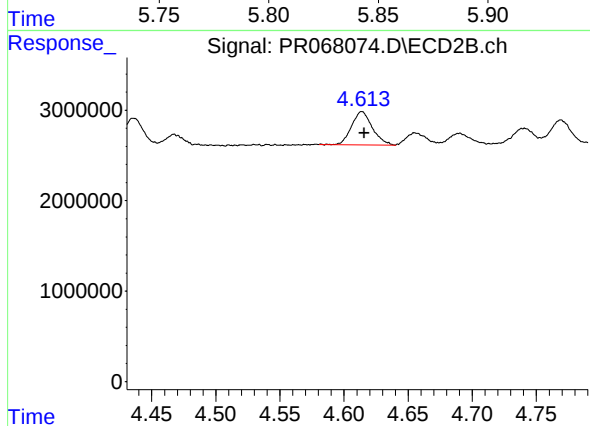

#24 AR-1248-4


R.T.: 4.614 min
Delta R.T.: -0.002 min
Response: 4150351
Conc: 19.22 ng/ml

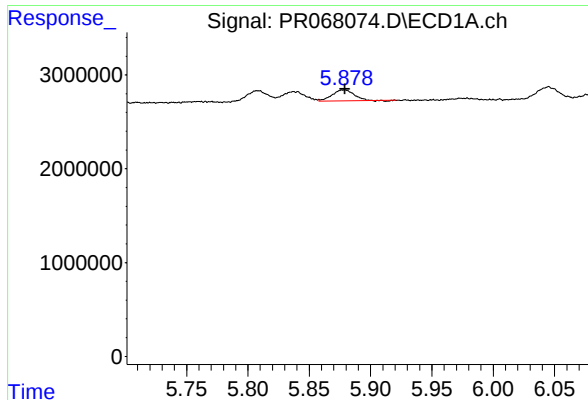

#25 AR-1248-5

R.T.: 5.878 min
Delta R.T.: -0.001 min
Response: 1475054
Conc: 18.27 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

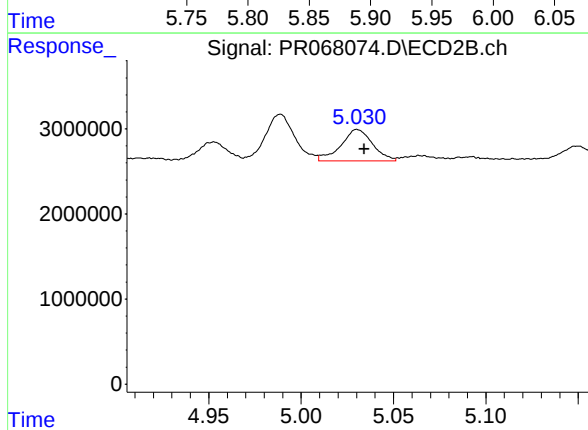

#25 AR-1248-5

R.T.: 5.030 min
Delta R.T.: -0.004 min
Response: 4403801
Conc: 20.72 ng/ml