

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR080822\
 Data File : PR055740.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Aug 2022 12:19
 Operator : AJ\MA
 Sample : N3980-09
 Misc : AR1660 MDL 25 PPB
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-WATER-03-QT3-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 00:05:31 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080522.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 05 12:39:02 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.634	2.905	80330374	37650772	18.826	18.752
2) SA Decachlor...	9.527	8.120	36539877	35429545	20.551	19.477
Target Compounds						
3) L1 AR-1016-1	4.856	4.013	3191649	1572594	27.563	24.283
4) L1 AR-1016-2	4.878	4.030	4507759	2233119	27.467	24.450
5) L1 AR-1016-3	4.942	4.207	2644211	1390597	26.737	27.272
6) L1 AR-1016-4	5.044	4.258	2225893	1087678	28.100	28.629
7) L1 AR-1016-5	5.359	4.473	2095986	1217002	28.989	24.671
31) L7 AR-1260-1	6.571	5.555	3235685	2814799	29.888	27.936
32) L7 AR-1260-2	6.854	5.759	3917921	3677562	31.664	30.079
33) L7 AR-1260-3	7.244	5.915	2820095	3293728	31.242	29.124
34) L7 AR-1260-4	7.487	6.418	3233422	2457632	31.494	25.681
35) L7 AR-1260-5	7.826	6.682	5925739	5944621	30.484	26.473



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR080822\
Data File : PR055740.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2022 12:19
Operator : AJ\MA
Sample : N3980-09
Misc : AR1660 MDL 25 PPB
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 00:05:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080522.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 05 12:39:02 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

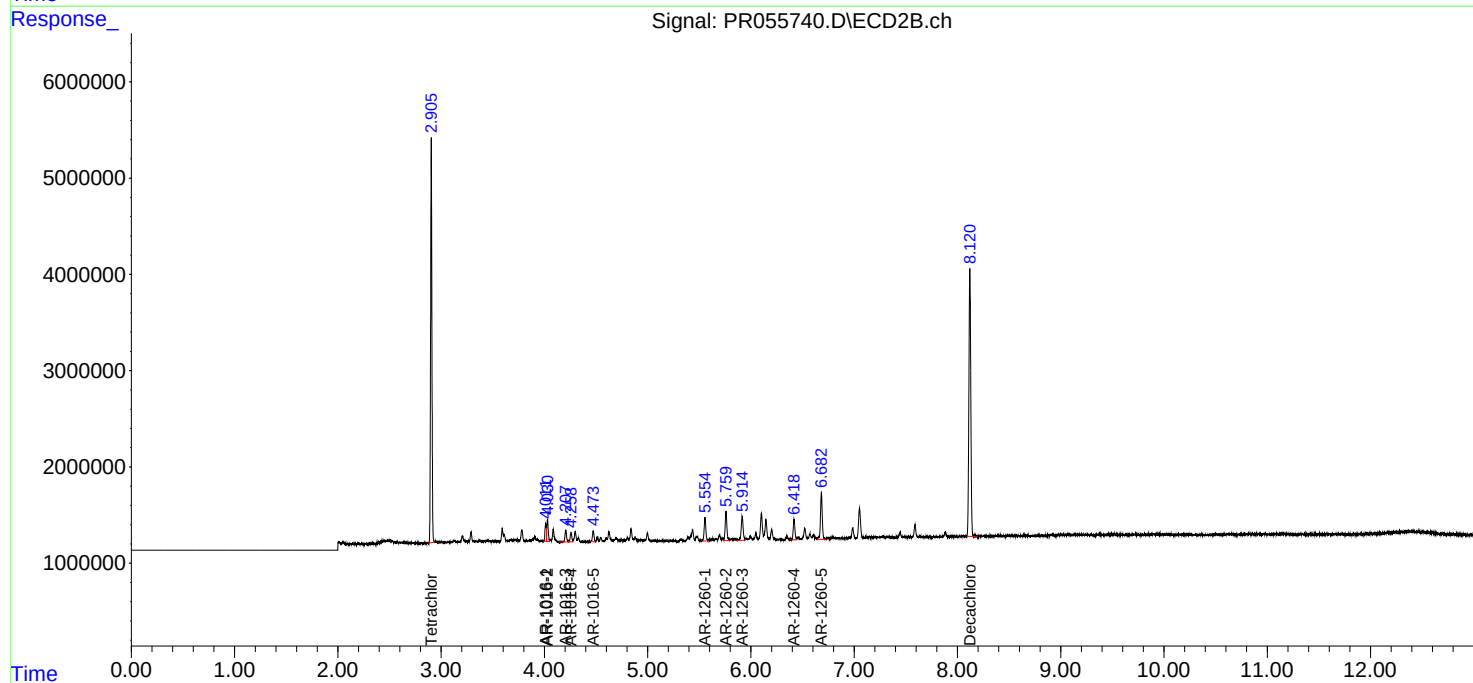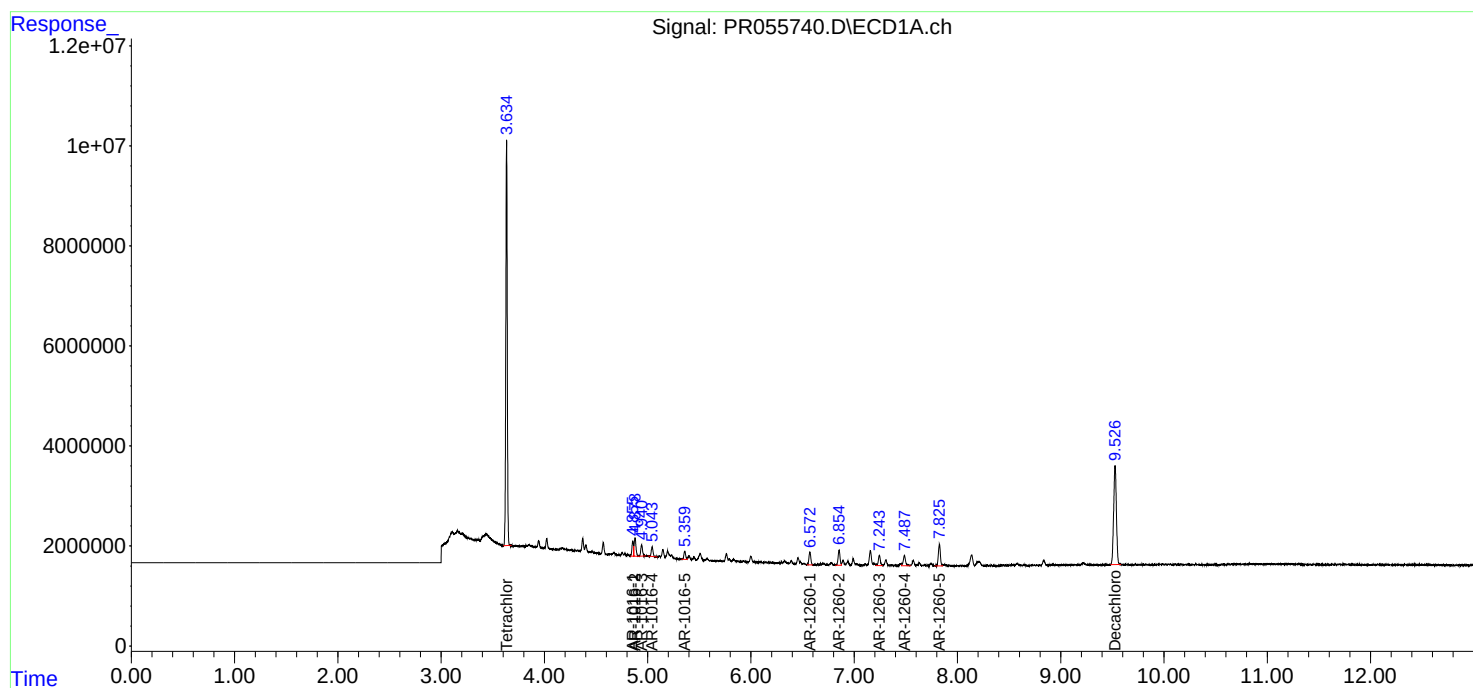


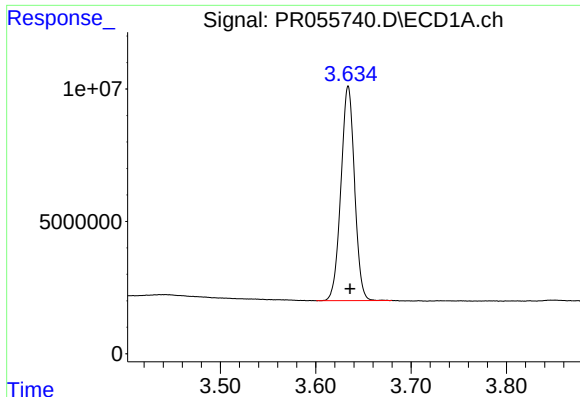

#1 Tetrachloro-m-xylene


R.T.: 3.634 min
Delta R.T.: -0.002 min
Response: 80330374
Conc: 18.83 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2022

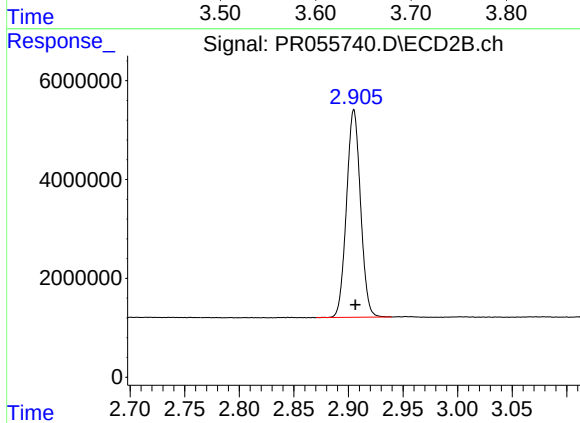


#1 Tetrachloro-m-xylene

R.T.: 2.905 min
Delta R.T.: -0.001 min
Response: 37650772
Conc: 18.75 ng/ml

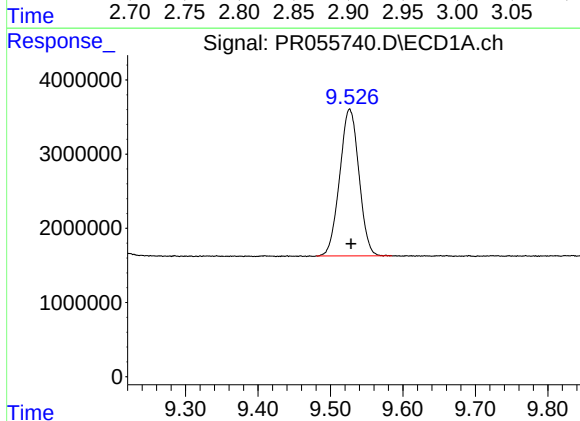


#2 Decachlorobiphenyl

R.T.: 9.527 min
Delta R.T.: -0.002 min
Response: 36539877
Conc: 20.55 ng/ml

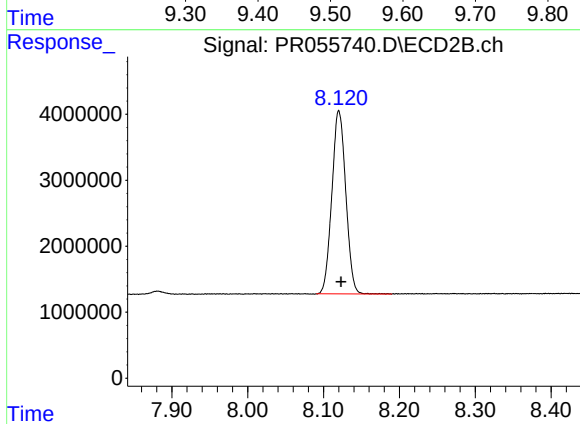

#2 Decachlorobiphenyl


R.T.: 8.120 min
Delta R.T.: -0.003 min
Response: 35429545
Conc: 19.48 ng/ml

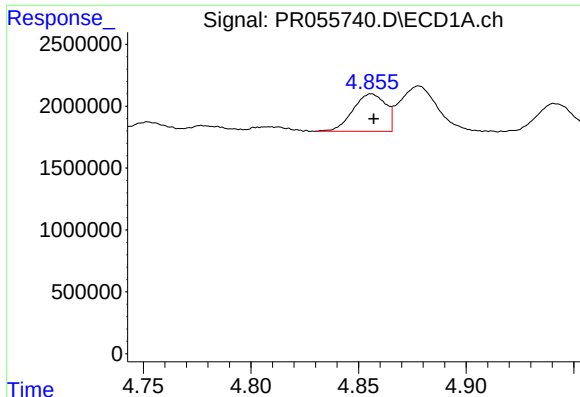

#3 AR-1016-1


R.T.: 4.856 min
Delta R.T.: 0.000 min
Response: 3191649
Conc: 27.56 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2022

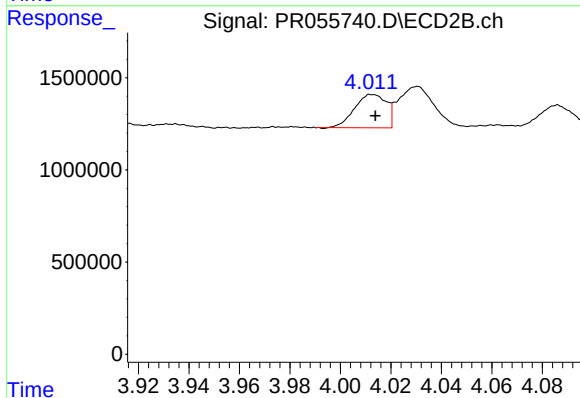


#3 AR-1016-1

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 1572594
Conc: 24.28 ng/ml

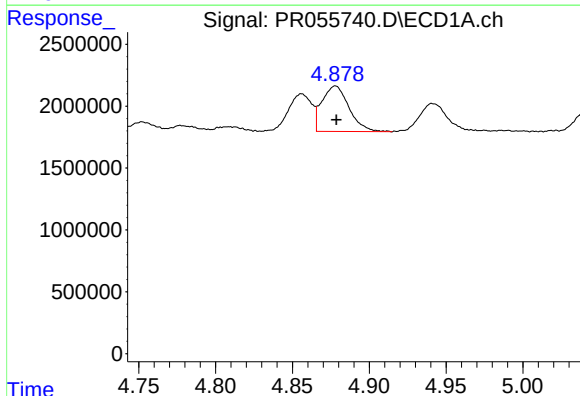


#4 AR-1016-2

R.T.: 4.878 min
Delta R.T.: 0.000 min
Response: 4507759
Conc: 27.47 ng/ml

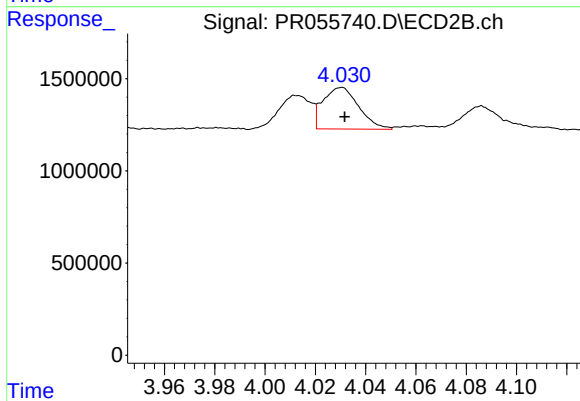

#4 AR-1016-2


R.T.: 4.030 min
Delta R.T.: -0.001 min
Response: 2233119
Conc: 24.45 ng/ml

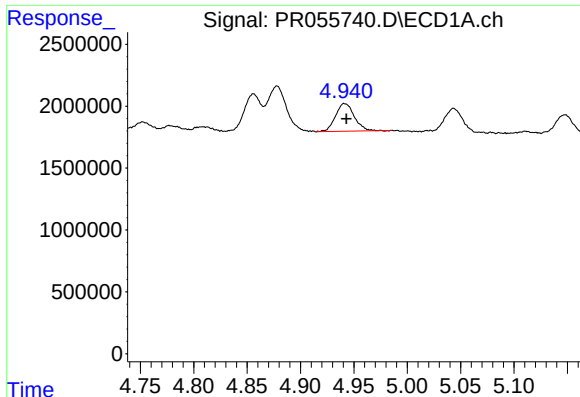

#5 AR-1016-3


R.T.: 4.942 min
Delta R.T.: -0.001 min
Response: 2644211
Conc: 26.74 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2022

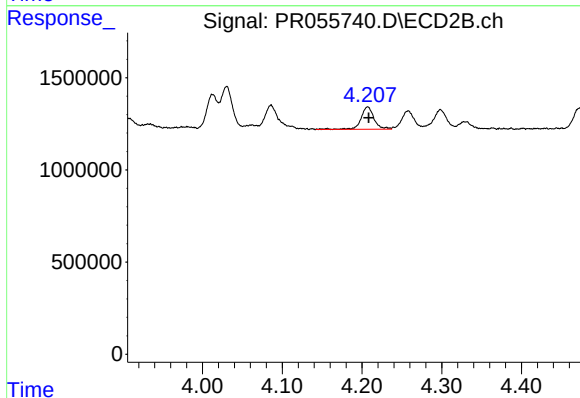


#5 AR-1016-3

R.T.: 4.207 min
Delta R.T.: -0.001 min
Response: 1390597
Conc: 27.27 ng/ml

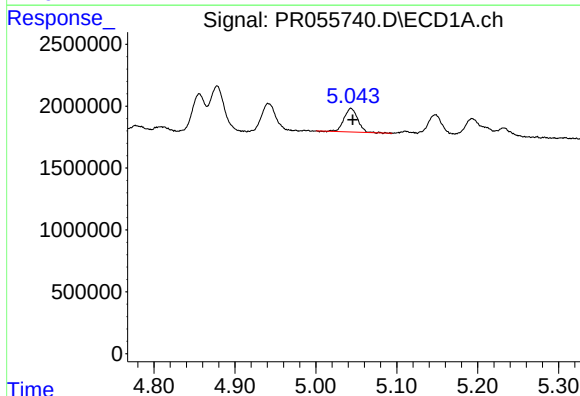


#6 AR-1016-4

R.T.: 5.044 min
Delta R.T.: -0.002 min
Response: 2225893
Conc: 28.10 ng/ml

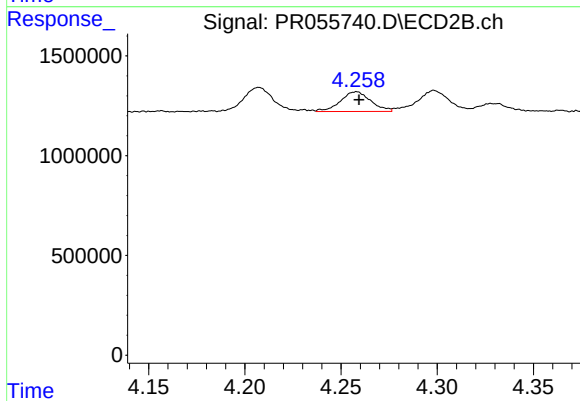

#6 AR-1016-4


R.T.: 4.258 min
Delta R.T.: -0.002 min
Response: 1087678
Conc: 28.63 ng/ml

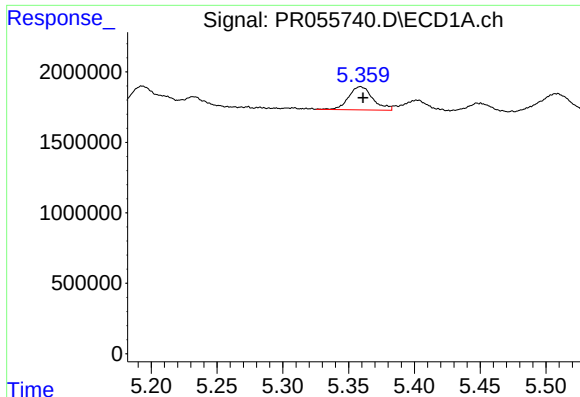

#7 AR-1016-5


R.T.: 5.359 min
Delta R.T.: -0.002 min
Response: 2095986
Conc: 28.99 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2022

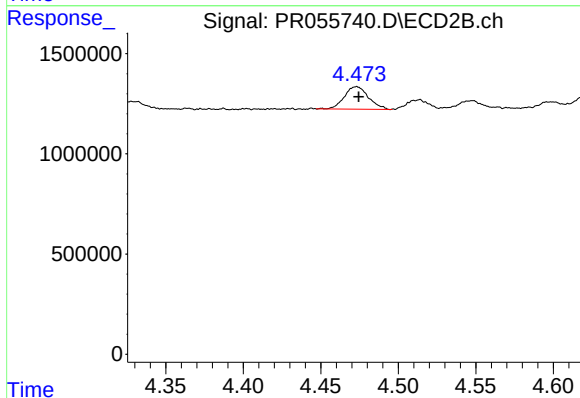


#7 AR-1016-5

R.T.: 4.473 min
Delta R.T.: -0.001 min
Response: 1217002
Conc: 24.67 ng/ml

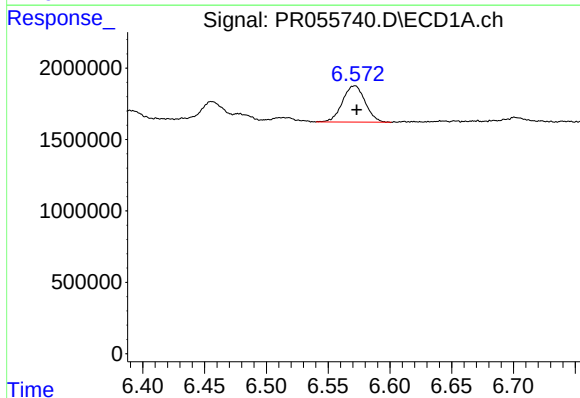


#31 AR-1260-1

R.T.: 6.571 min
Delta R.T.: -0.002 min
Response: 3235685
Conc: 29.89 ng/ml

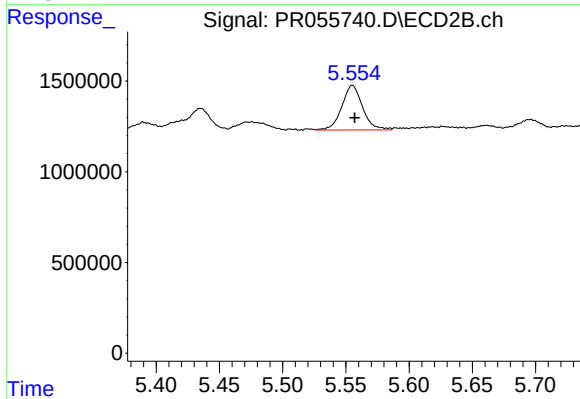

#31 AR-1260-1


R.T.: 5.555 min
Delta R.T.: -0.002 min
Response: 2814799
Conc: 27.94 ng/ml

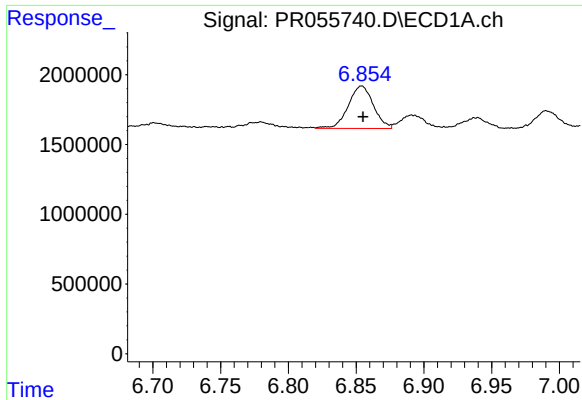

#32 AR-1260-2


R.T.: 6.854 min
Delta R.T.: -0.001 min
Response: 3917921
Conc: 31.66 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2022

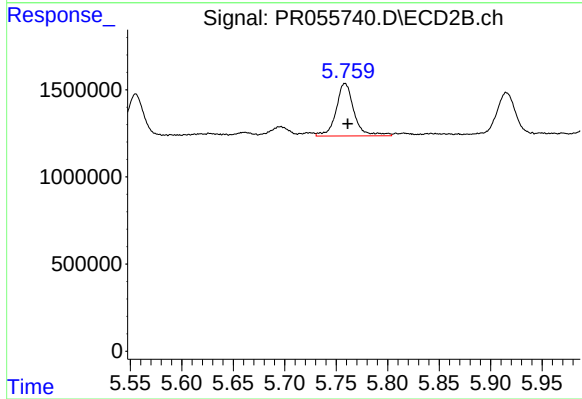


#32 AR-1260-2

R.T.: 5.759 min
Delta R.T.: -0.003 min
Response: 3677562
Conc: 30.08 ng/ml

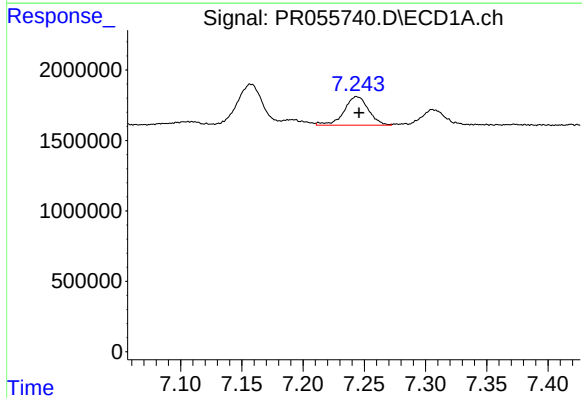


#33 AR-1260-3

R.T.: 7.244 min
Delta R.T.: -0.002 min
Response: 2820095
Conc: 31.24 ng/ml

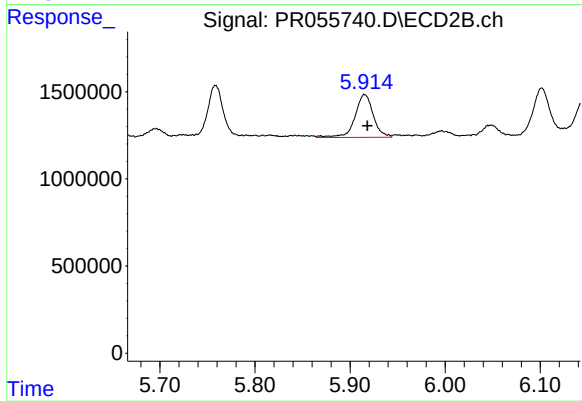

#33 AR-1260-3


R.T.: 5.915 min
Delta R.T.: -0.003 min
Response: 3293728
Conc: 29.12 ng/ml

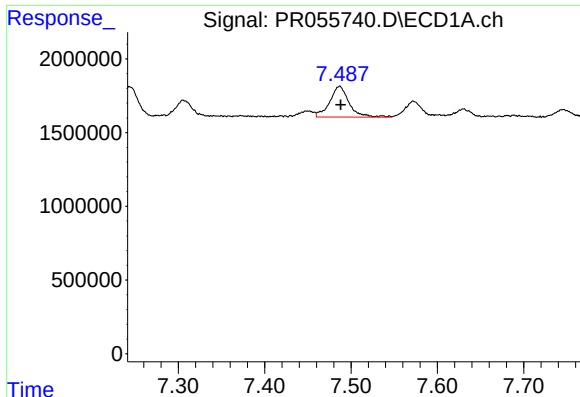

#34 AR-1260-4


R.T.: 7.487 min
Delta R.T.: -0.002 min
Response: 3233422
Conc: 31.49 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2022

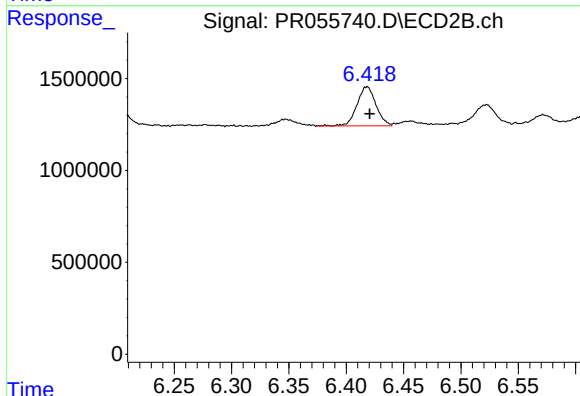


#34 AR-1260-4

R.T.: 6.418 min
Delta R.T.: -0.002 min
Response: 2457632
Conc: 25.68 ng/ml

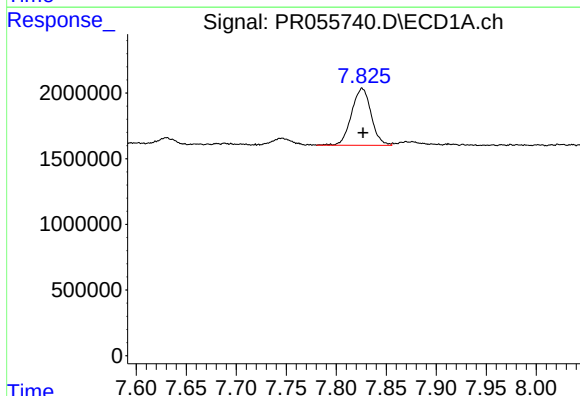

#35 AR-1260-5

R.T.: 7.826 min
Delta R.T.: 0.000 min
Response: 5925739
Conc: 30.48 ng/ml

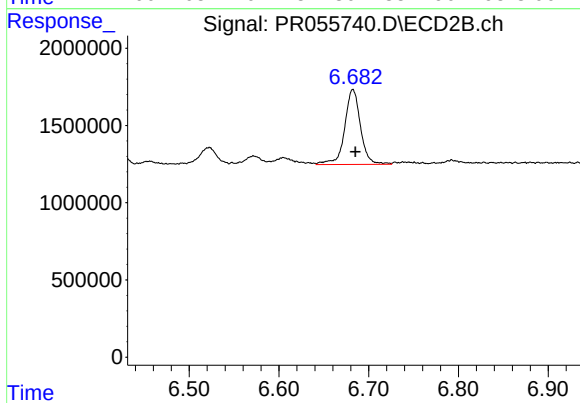

#35 AR-1260-5

R.T.: 6.682 min
Delta R.T.: -0.003 min
Response: 5944621
Conc: 26.47 ng/ml