

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR081023\
 Data File : PR062577.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2023 15:56
 Operator : YP\AJ
 Sample : 03572-09
 Misc : AR1232 MDL 25 PPB
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-WATER-03-QT3-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 22:10:37 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080923.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 09 01:27:38 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.685	2.956	34806369	54996773	17.240	18.944
2) SA Decachlor...	9.618	8.236	31298162	82272317	21.013	19.827
Target Compounds						
11) L3 AR-1232-1	4.075	3.345	1464849	2396970	29.494	32.005
12) L3 AR-1232-2	4.629	4.097	699568	1570744	28.329	22.774
13) L3 AR-1232-3	4.936	4.278	1075747	886849	25.185	23.899
14) L3 AR-1232-4	5.104	4.370	689065	893880	32.597	26.398
15) L3 AR-1232-5	5.208	4.546	721862	1030219	41.508	26.219 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR081023\
Data File : PR062577.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2023 15:56
Operator : YP\AJ
Sample : 03572-09
Misc : AR1232 MDL 25 PPB
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 22:10:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080923.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 09 01:27:38 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

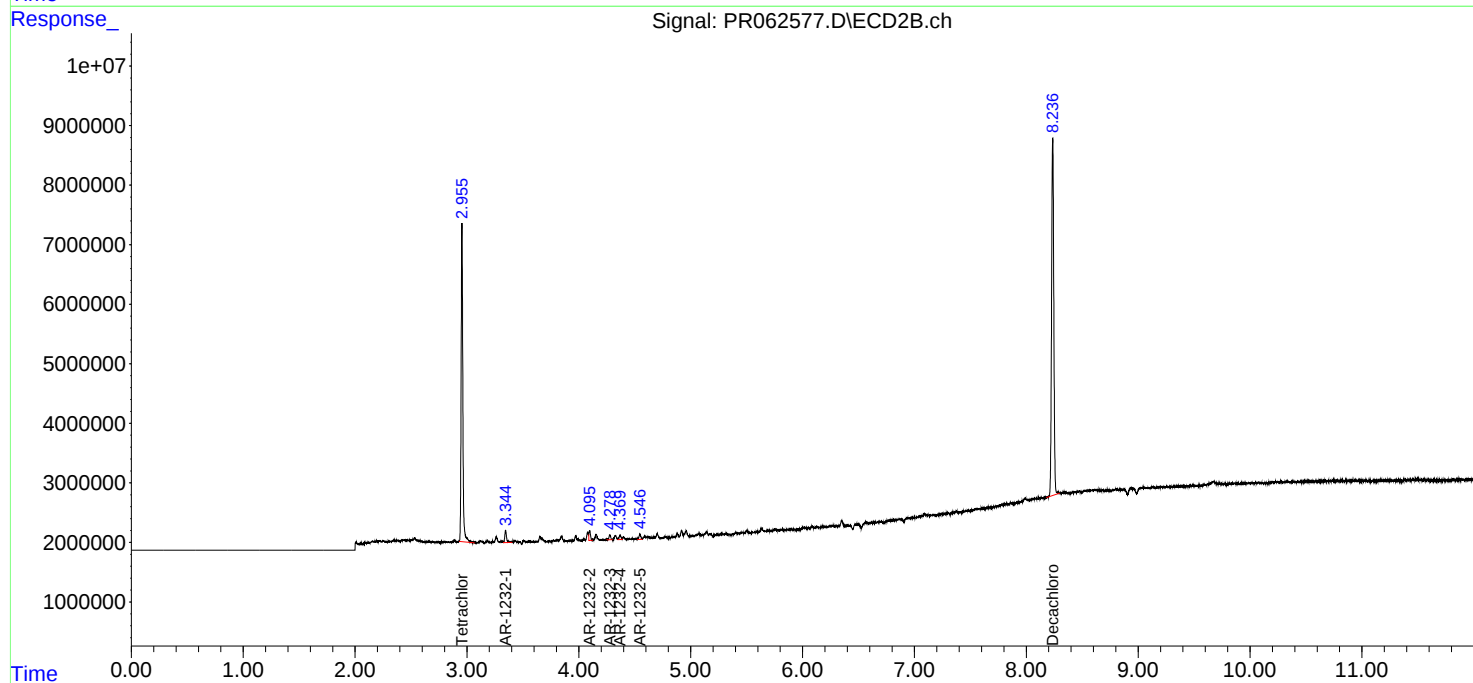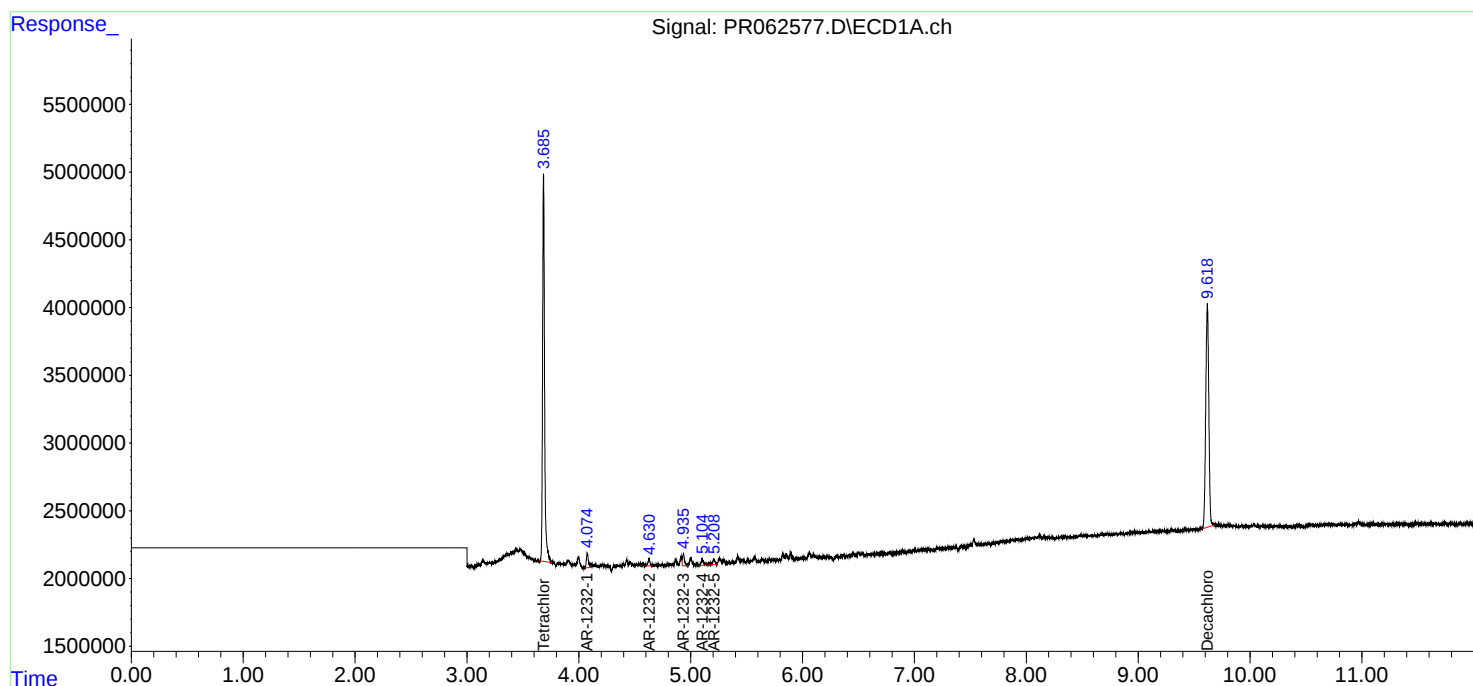


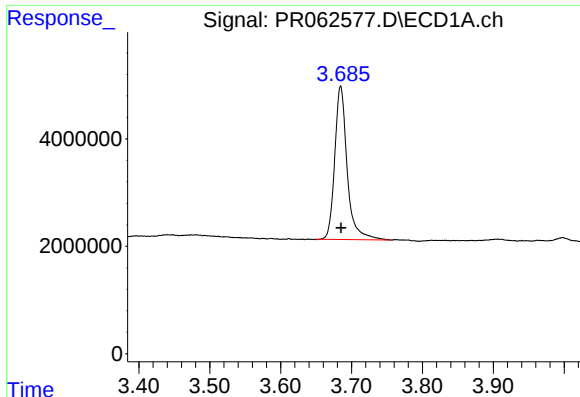

#1 Tetrachloro-m-xylene


R.T.: 3.685 min
Delta R.T.: 0.000 min
Response: 34806369
Conc: 17.24 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2023

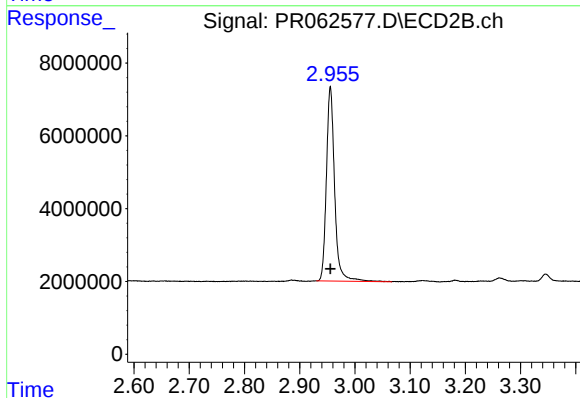


#1 Tetrachloro-m-xylene

R.T.: 2.956 min
Delta R.T.: 0.000 min
Response: 54996773
Conc: 18.94 ng/ml

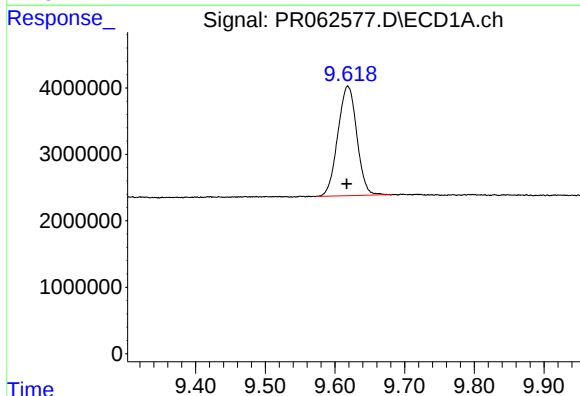


#2 Decachlorobiphenyl

R.T.: 9.618 min
Delta R.T.: 0.002 min
Response: 31298162
Conc: 21.01 ng/ml

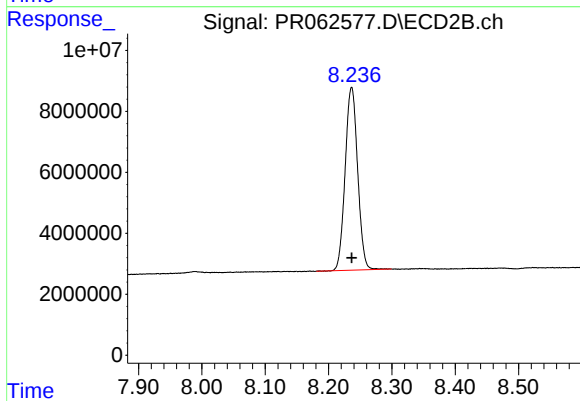

#2 Decachlorobiphenyl


R.T.: 8.236 min
Delta R.T.: 0.000 min
Response: 82272317
Conc: 19.83 ng/ml

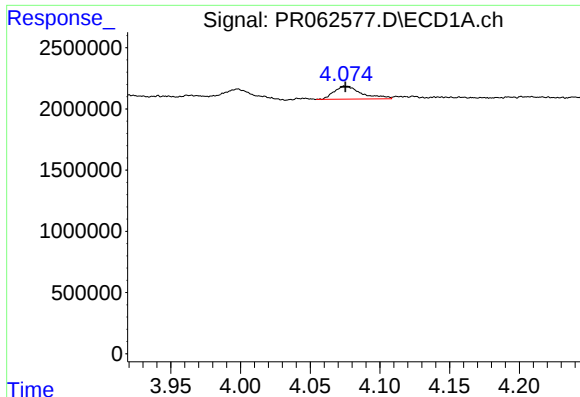

#11 AR-1232-1


R.T.: 4.075 min
Delta R.T.: 0.000 min
Response: 1464849
Conc: 29.49 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2023

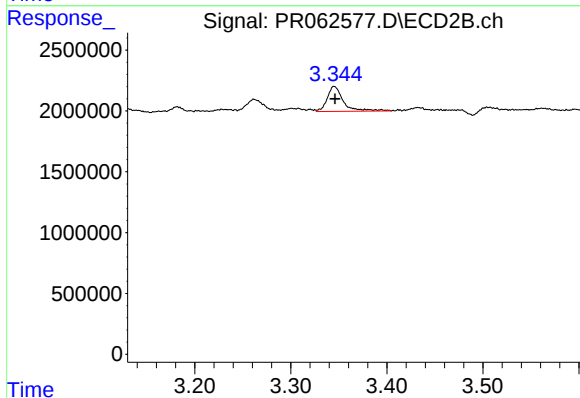


#11 AR-1232-1

R.T.: 3.345 min
Delta R.T.: 0.000 min
Response: 2396970
Conc: 32.01 ng/ml

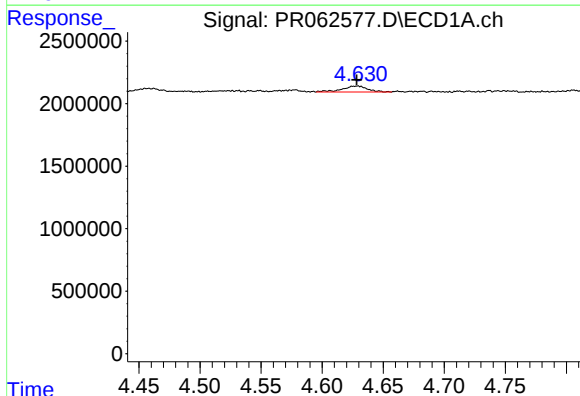


#12 AR-1232-2

R.T.: 4.629 min
Delta R.T.: 0.000 min
Response: 699568
Conc: 28.33 ng/ml

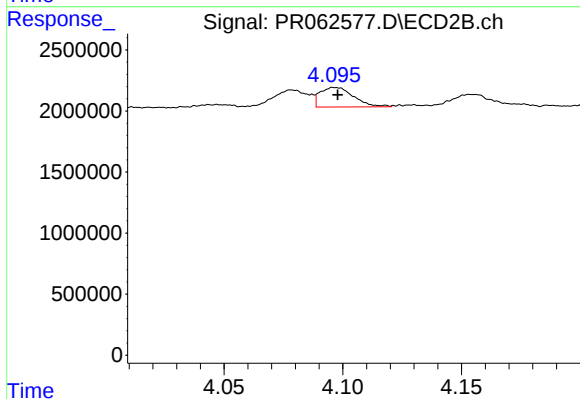

#12 AR-1232-2


R.T.: 4.097 min
Delta R.T.: -0.001 min
Response: 1570744
Conc: 22.77 ng/ml

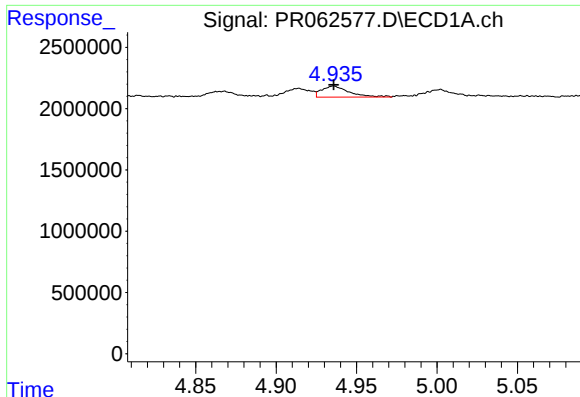

#13 AR-1232-3


R.T.: 4.936 min
Delta R.T.: 0.000 min
Response: 1075747
Conc: 25.19 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2023

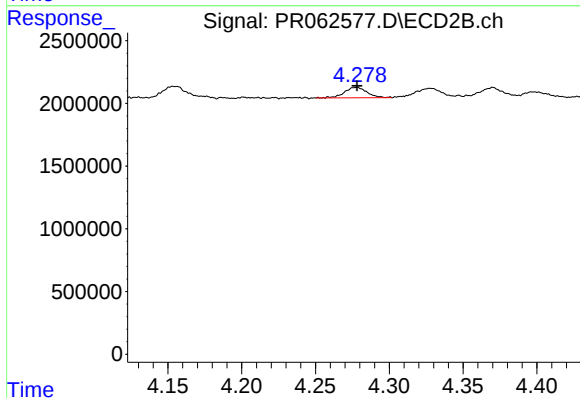


#13 AR-1232-3

R.T.: 4.278 min
Delta R.T.: 0.000 min
Response: 886849
Conc: 23.90 ng/ml

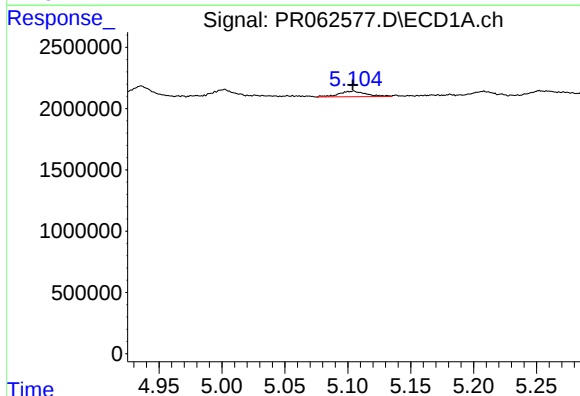


#14 AR-1232-4

R.T.: 5.104 min
Delta R.T.: 0.000 min
Response: 689065
Conc: 32.60 ng/ml

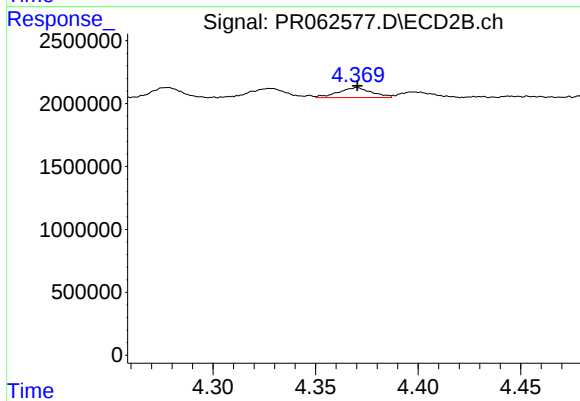

#14 AR-1232-4


R.T.: 4.370 min
Delta R.T.: 0.000 min
Response: 893880
Conc: 26.40 ng/ml

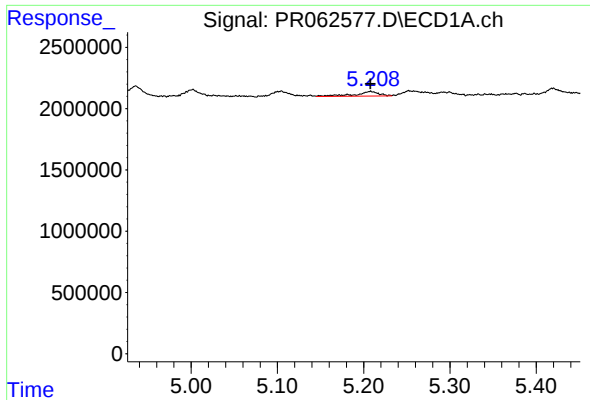

#15 AR-1232-5

R.T.: 5.208 min
Delta R.T.: 0.000 min
Response: 721862
Conc: 41.51 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2023

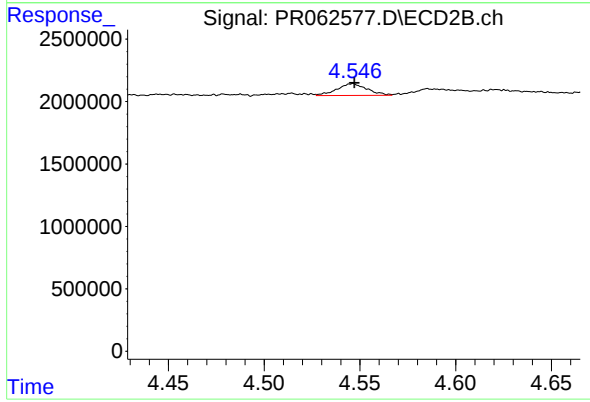

#15 AR-1232-5

R.T.: 4.546 min
Delta R.T.: -0.001 min
Response: 1030219
Conc: 26.22 ng/ml