

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR081023\
 Data File : PR062579.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2023 16:25
 Operator : YP\AJ
 Sample : 03572-09
 Misc : AR1248 MDL 25 PPB
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-WATER-03-QT3-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 22:11:31 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080923.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 09 01:27:38 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.685	2.956	35295076	54878245	17.482	18.903
2) SA Decachlor...	9.619	8.239	31648139	83363821	21.248	20.090
Target Compounds						
21) L5 AR-1248-1	4.914	4.078	1055644	1845348	25.701	27.578
22) L5 AR-1248-2	5.207	4.327	1806938	2611450	29.834	27.251
23) L5 AR-1248-3	5.420	4.369	1720339	2523797	24.531	25.563
24) L5 AR-1248-4	5.854	4.546	1959170	2822674	27.088	23.791
25) L5 AR-1248-5	5.894	4.960	2200472	3362377	31.066	28.136



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR081023\
Data File : PR062579.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2023 16:25
Operator : YP\AJ
Sample : 03572-09
Misc : AR1248 MDL 25 PPB
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 22:11:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080923.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 09 01:27:38 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

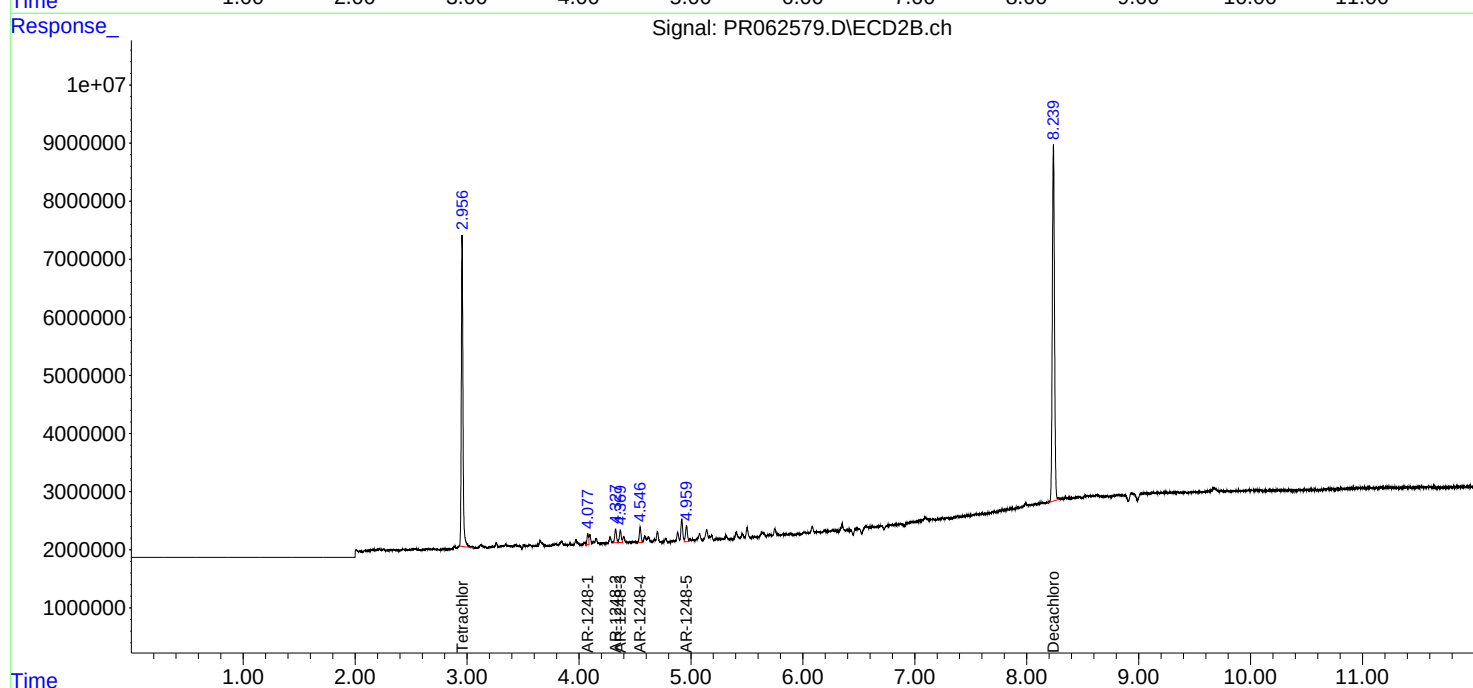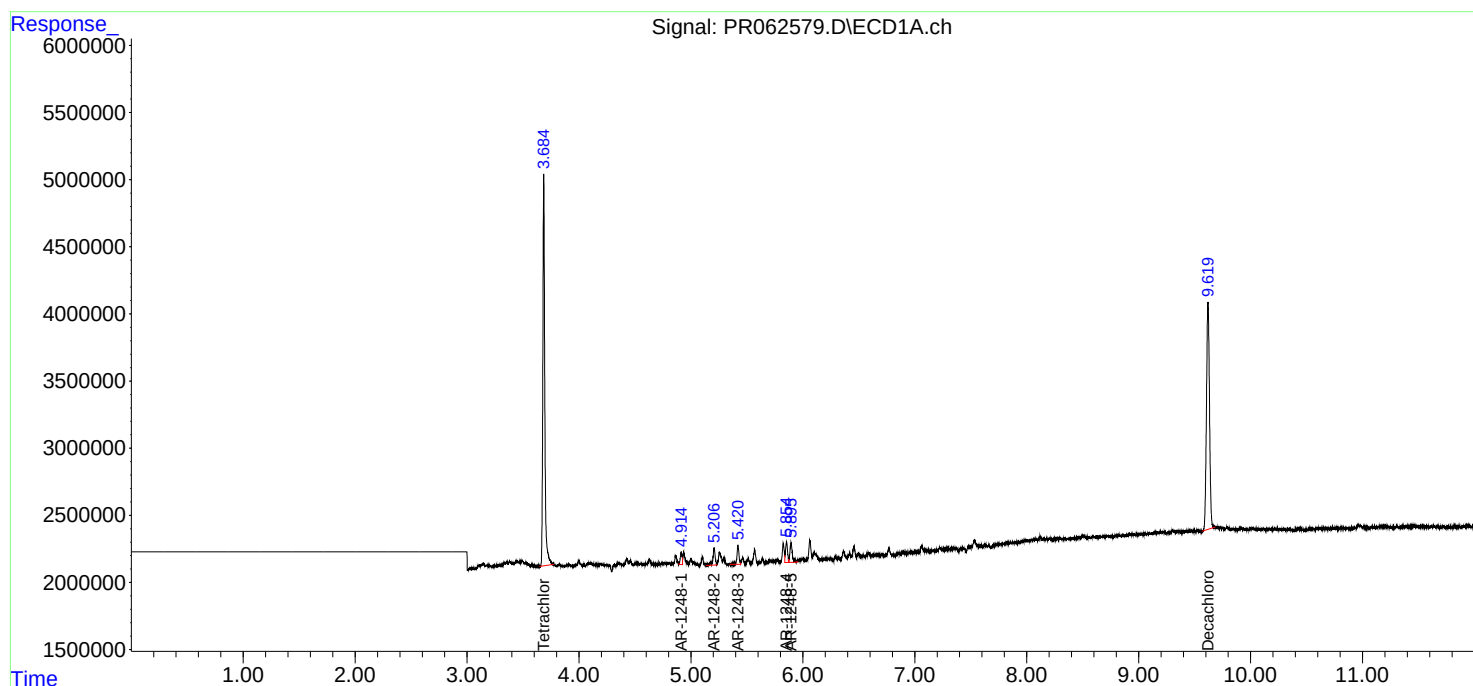


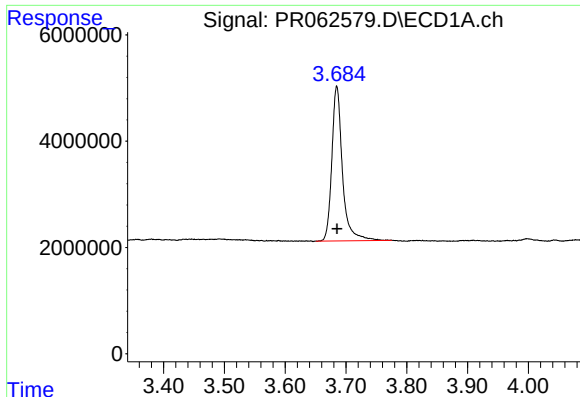

#1 Tetrachloro-m-xylene


R.T.: 3.685 min
Delta R.T.: 0.000 min
Response: 35295076
Conc: 17.48 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2023

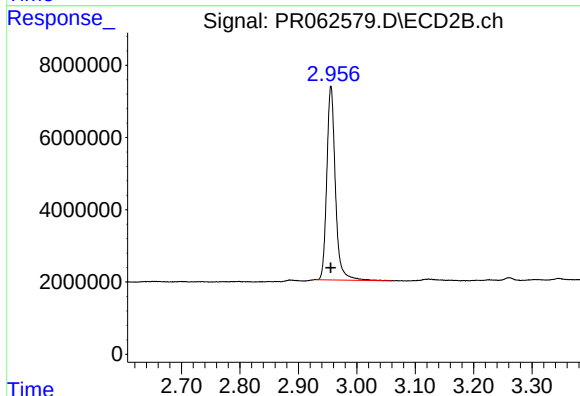


#1 Tetrachloro-m-xylene

R.T.: 2.956 min
Delta R.T.: 0.000 min
Response: 54878245
Conc: 18.90 ng/ml

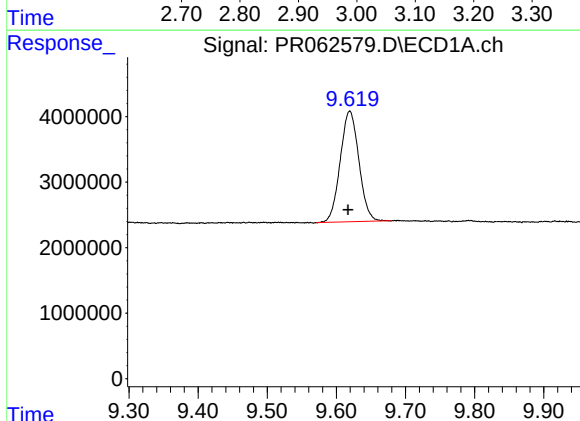


#2 Decachlorobiphenyl

R.T.: 9.619 min
Delta R.T.: 0.003 min
Response: 31648139
Conc: 21.25 ng/ml

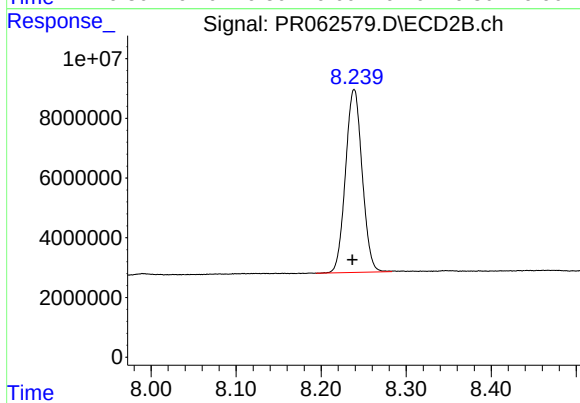

#2 Decachlorobiphenyl


R.T.: 8.239 min
Delta R.T.: 0.002 min
Response: 83363821
Conc: 20.09 ng/ml

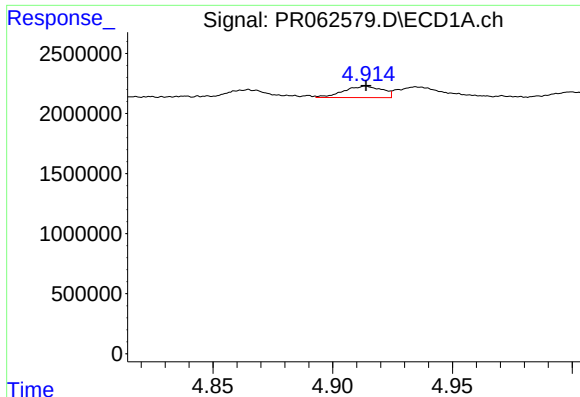

#21 AR-1248-1


R.T.: 4.914 min
Delta R.T.: 0.000 min
Response: 1055644
Conc: 25.70 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2023

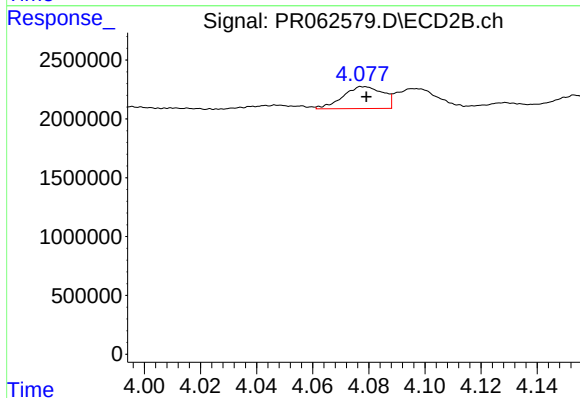


#21 AR-1248-1

R.T.: 4.078 min
Delta R.T.: 0.000 min
Response: 1845348
Conc: 27.58 ng/ml

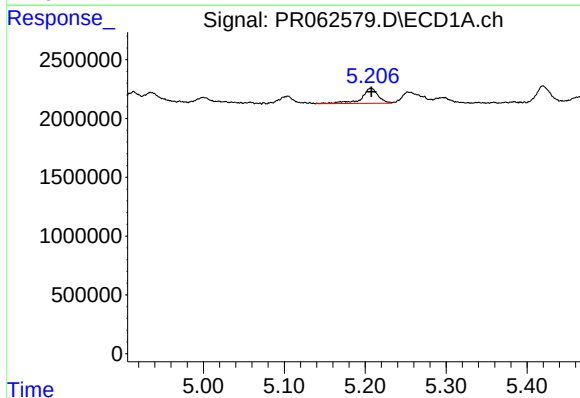


#22 AR-1248-2

R.T.: 5.207 min
Delta R.T.: 0.000 min
Response: 1806938
Conc: 29.83 ng/ml

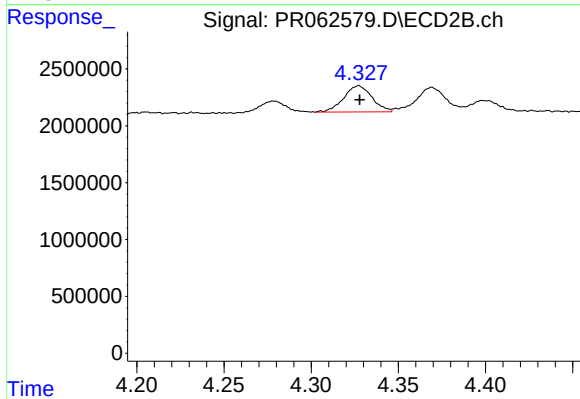

#22 AR-1248-2


R.T.: 4.327 min
Delta R.T.: 0.000 min
Response: 2611450
Conc: 27.25 ng/ml

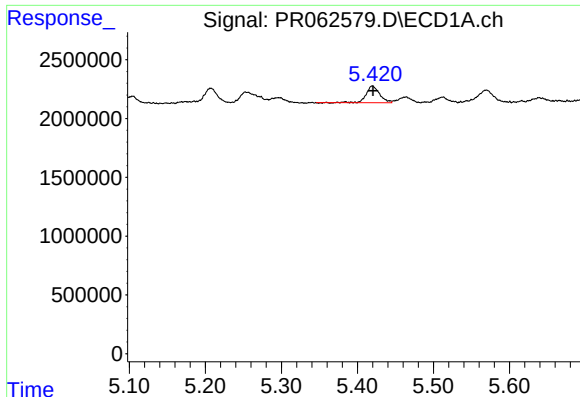

#23 AR-1248-3


R.T.: 5.420 min
Delta R.T.: 0.000 min
Response: 1720339
Conc: 24.53 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2023

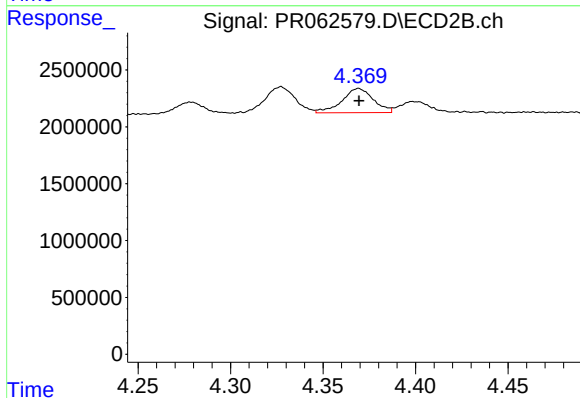


#23 AR-1248-3

R.T.: 4.369 min
Delta R.T.: 0.000 min
Response: 2523797
Conc: 25.56 ng/ml

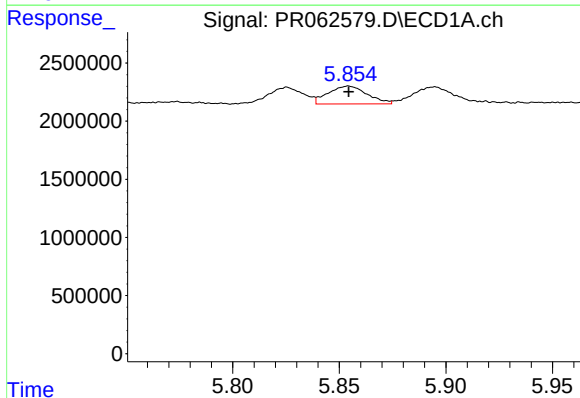


#24 AR-1248-4

R.T.: 5.854 min
Delta R.T.: 0.000 min
Response: 1959170
Conc: 27.09 ng/ml

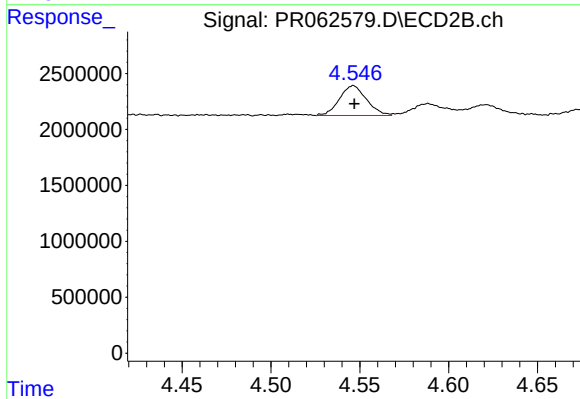

#24 AR-1248-4


R.T.: 4.546 min
Delta R.T.: 0.000 min
Response: 2822674
Conc: 23.79 ng/ml

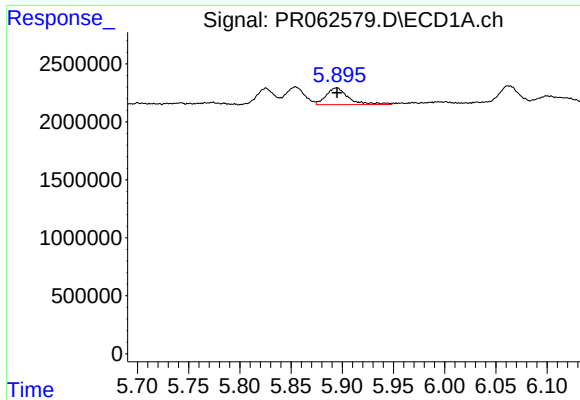

#25 AR-1248-5

R.T.: 5.894 min
Delta R.T.: 0.000 min
Response: 2200472
Conc: 31.07 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2023

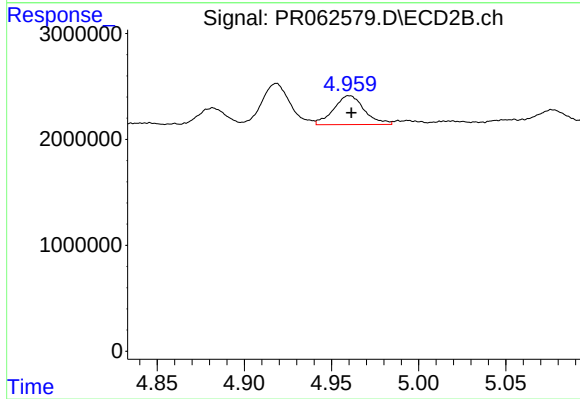

#25 AR-1248-5

R.T.: 4.960 min
Delta R.T.: -0.001 min
Response: 3362377
Conc: 28.14 ng/ml