

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR081023\
 Data File : PR062580.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2023 16:40
 Operator : YP\AJ
 Sample : 03572-09
 Misc : AR1254 MDL 25 PPB
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-WATER-03-QT3-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 22:11:57 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080923.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 09 01:27:38 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.685	2.956	35127709	55234923	17.399	19.026
2)	SA Decachlor...	9.617	8.236	32145587	82010637	21.582	19.764
Target Compounds							
26)	L6 AR-1254-1	5.825	4.918	2253306	5382822	28.193	30.053
27)	L6 AR-1254-2	6.063	5.077	3449925	5553192	28.903	35.508
28)	L6 AR-1254-3	6.455	5.502	3375362	6647820	28.518	25.604
29)	L6 AR-1254-4	6.767	5.749	2622300	4508490	31.503	26.910
30)	L6 AR-1254-5	7.224	6.196	3001014	8051651	33.385	32.379



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR081023\
Data File : PR062580.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2023 16:40
Operator : YP\AJ
Sample : 03572-09
Misc : AR1254 MDL 25 PPB
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 22:11:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080923.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 09 01:27:38 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

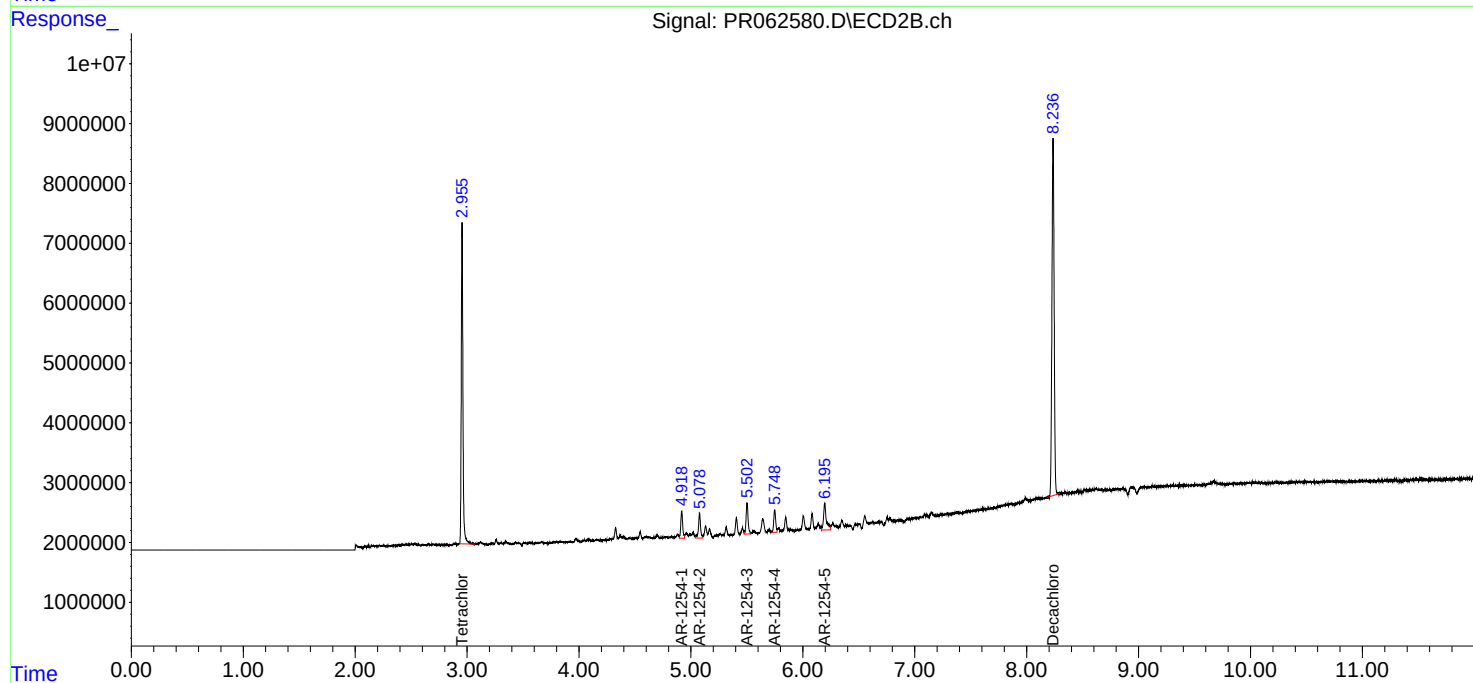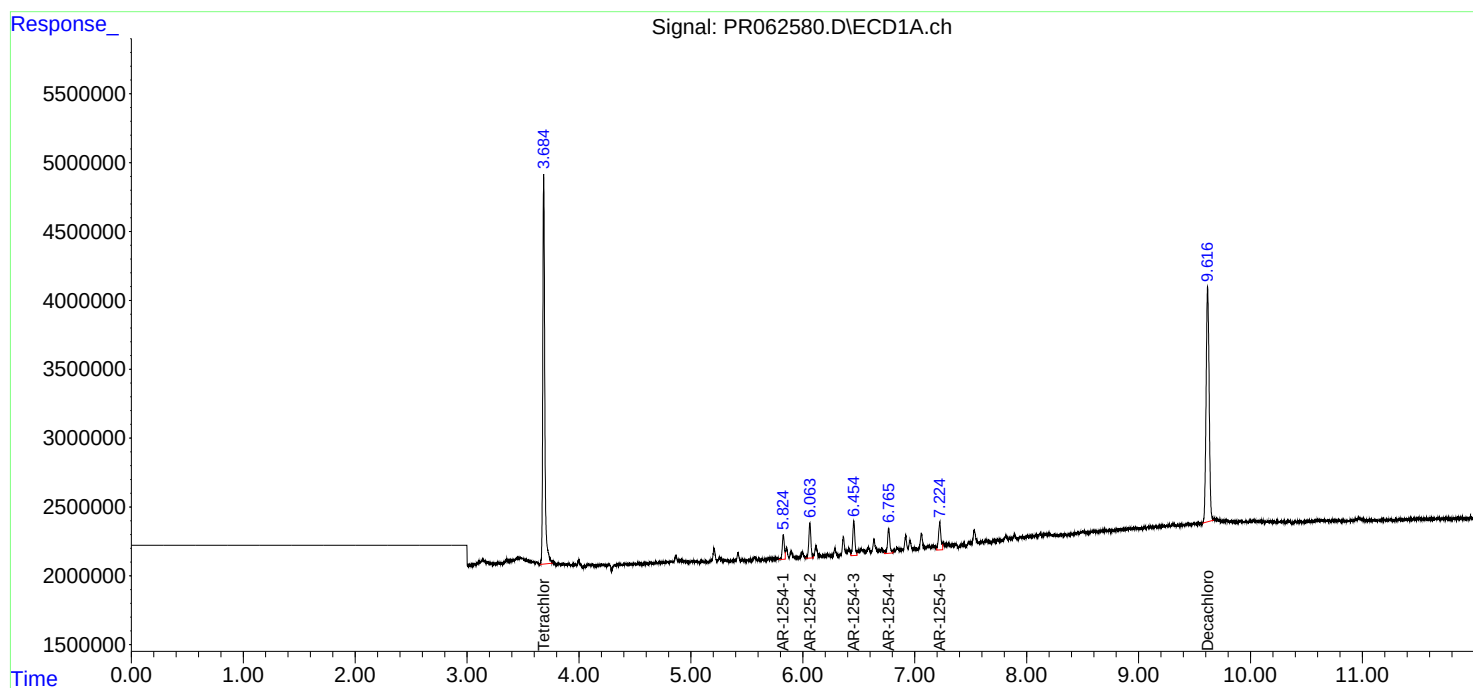


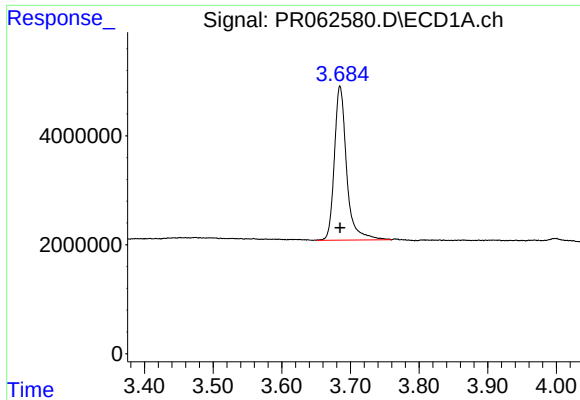

#1 Tetrachloro-m-xylene


R.T.: 3.685 min
Delta R.T.: 0.000 min
Response: 35127709
Conc: 17.40 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2023

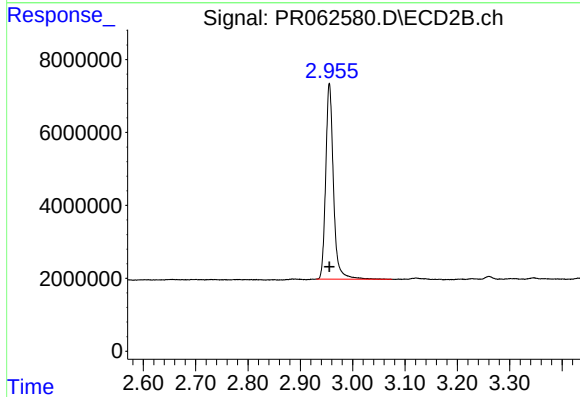


#1 Tetrachloro-m-xylene

R.T.: 2.956 min
Delta R.T.: 0.000 min
Response: 55234923
Conc: 19.03 ng/ml

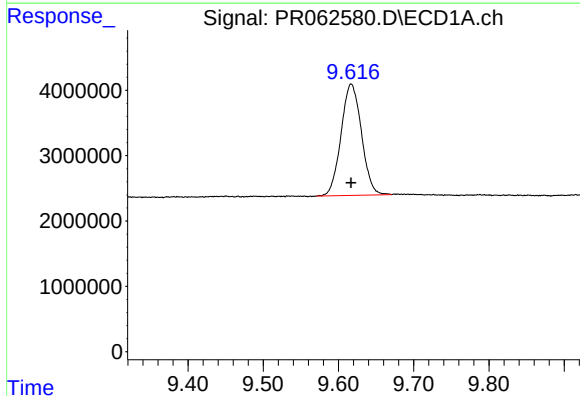


#2 Decachlorobiphenyl

R.T.: 9.617 min
Delta R.T.: 0.000 min
Response: 32145587
Conc: 21.58 ng/ml

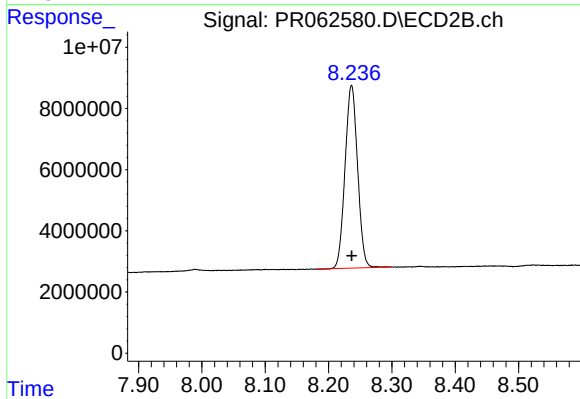

#2 Decachlorobiphenyl


R.T.: 8.236 min
Delta R.T.: 0.000 min
Response: 82010637
Conc: 19.76 ng/ml

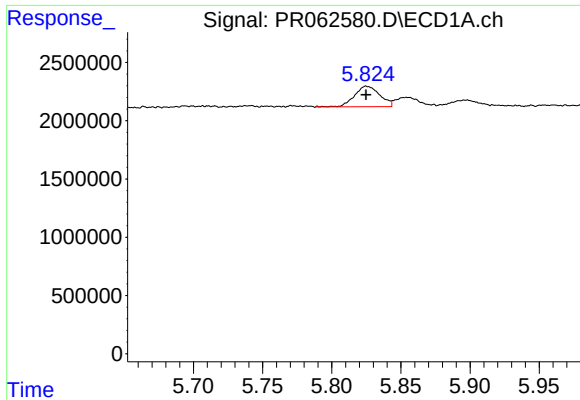

#26 AR-1254-1


R.T.: 5.825 min
Delta R.T.: 0.000 min
Response: 2253306
Conc: 28.19 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2023

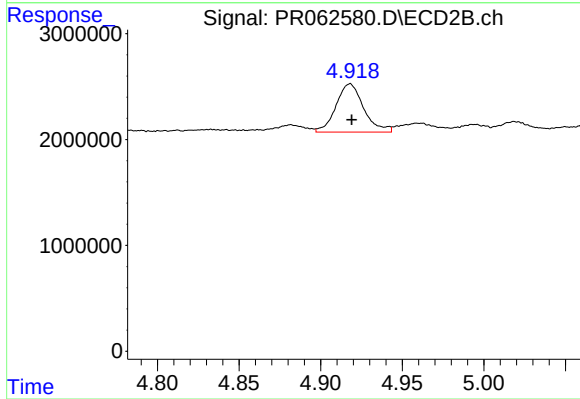


#26 AR-1254-1

R.T.: 4.918 min
Delta R.T.: -0.001 min
Response: 5382822
Conc: 30.05 ng/ml

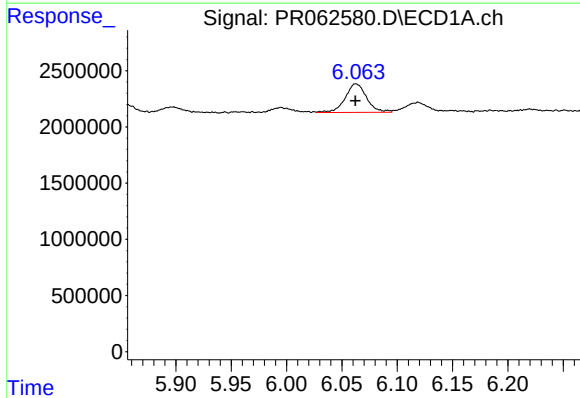


#27 AR-1254-2

R.T.: 6.063 min
Delta R.T.: 0.000 min
Response: 3449925
Conc: 28.90 ng/ml

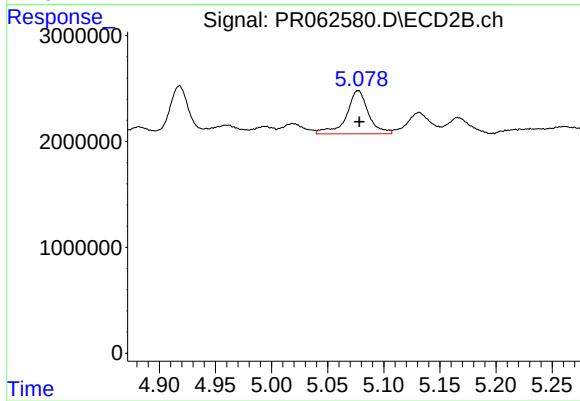

#27 AR-1254-2


R.T.: 5.077 min
Delta R.T.: 0.000 min
Response: 5553192
Conc: 35.51 ng/ml

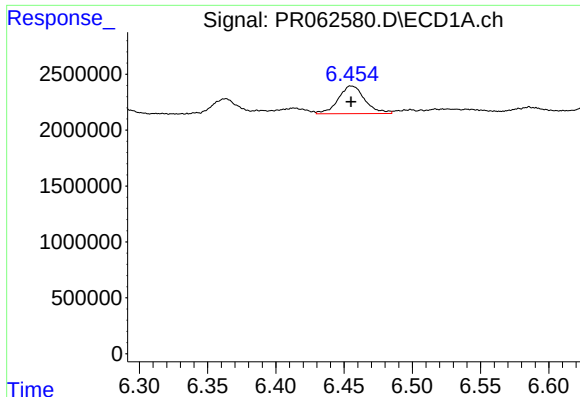

#28 AR-1254-3


R.T.: 6.455 min
Delta R.T.: 0.000 min
Response: 3375362
Conc: 28.52 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2023

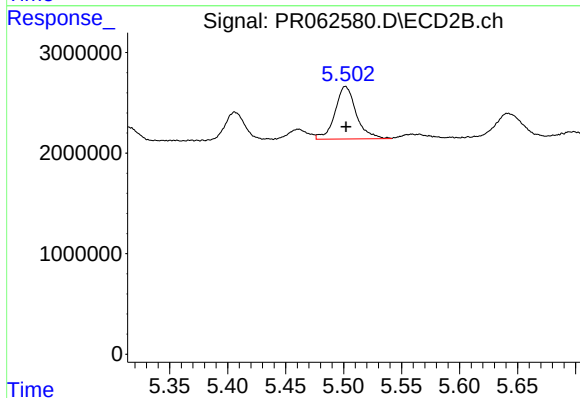


#28 AR-1254-3

R.T.: 5.502 min
Delta R.T.: 0.000 min
Response: 6647820
Conc: 25.60 ng/ml

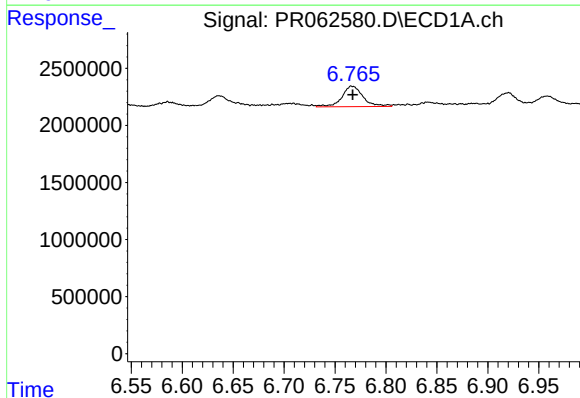


#29 AR-1254-4

R.T.: 6.767 min
Delta R.T.: 0.000 min
Response: 2622300
Conc: 31.50 ng/ml

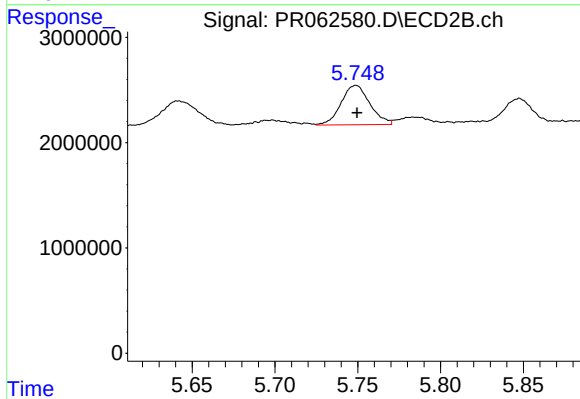

#29 AR-1254-4


R.T.: 5.749 min
Delta R.T.: 0.000 min
Response: 4508490
Conc: 26.91 ng/ml

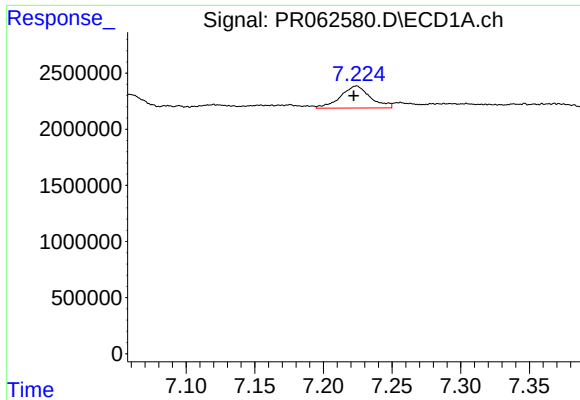

#30 AR-1254-5

R.T.: 7.224 min
Delta R.T.: 0.002 min
Response: 3001014
Conc: 33.38 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2023

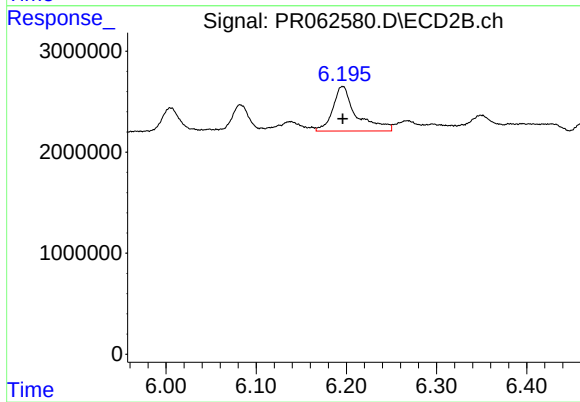

#30 AR-1254-5

R.T.: 6.196 min
Delta R.T.: 0.000 min
Response: 8051651
Conc: 32.38 ng/ml