

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR081118\
Data File : PR031356.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2018 23:16
Operator : SM\SJ
Sample : J4301-21MS
Misc :
ALS Vial : 27 Sample Multiplier: 1


Instrument :
ECD_R
ClientSampleId :
C0AG1MS

Manual Integrations
APPROVED

Sohil
8/11/2018 9:27:47 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 00:44:50 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080918CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 10 04:14:30 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

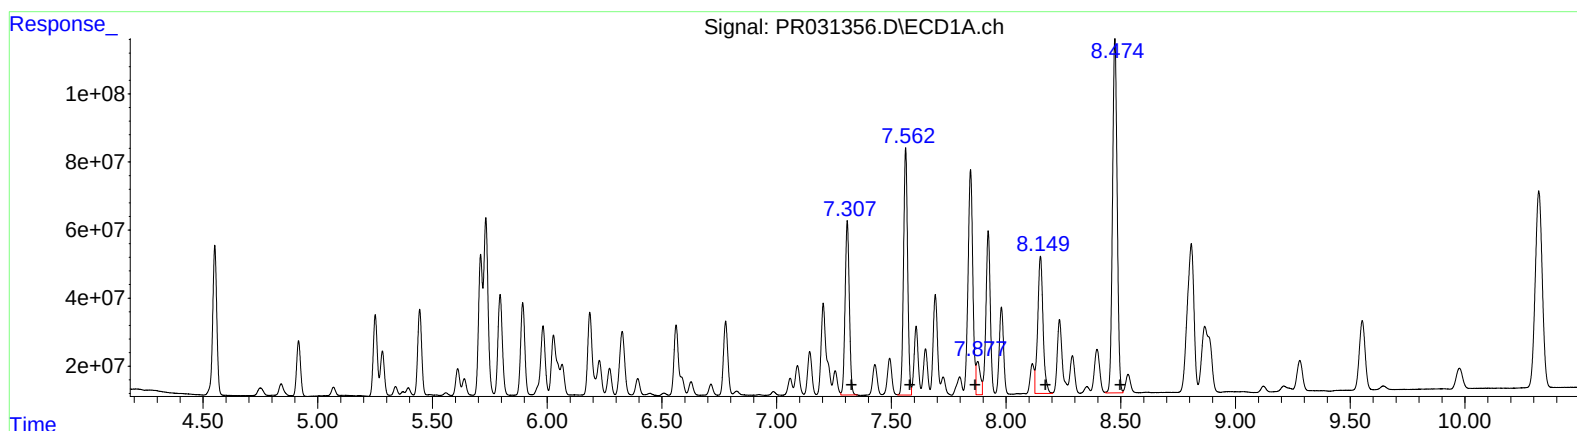

(31) AR-1260-1 (L7)
R.T. Response Conc
7.31 656630449 467.56
7.56 899270514 463.37
7.88 124562125 59.67
8.15 648020534 429.73
8.47 1469707044 419.99

(31) AR-1260-1 #2 (L7)
R.T. Response Conc
6.18 1357800856 413.61
6.36 1720486080 433.54
6.52 1445431738 440.22
6.98 778367568 395.67
7.22 1622046006 404.94

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR081118\
Data File : PR031356.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2018 23:16
Operator : SM\SJ
Sample : J4301-21MS
Misc :
ALS Vial : 27 Sample Multiplier: 1


Instrument :
ECD_R
ClientSampleId :
C0AG1MS

Manual Integrations
APPROVED

Sohil
8/11/2018 9:27:47 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 00:44:50 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080918CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 10 04:14:30 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

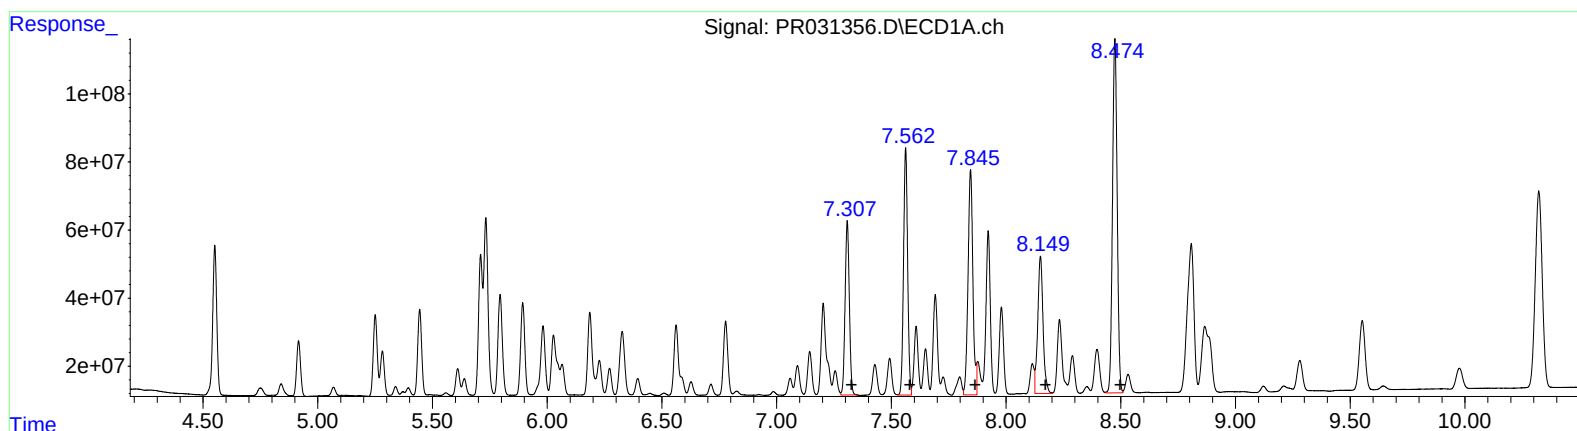

(31) AR-1260-1 #2 (L7)
R.T. Response Conc
7.31 656630449 467.56
7.56 899270514 463.37
7.85 978702173 468.87
8.15 648020534 429.73
8.47 1469707044 419.99

(31) AR-1260-1 #2 (L7)
R.T. Response Conc
6.18 1357800856 413.61
6.36 1720486080 433.54
6.52 1445431738 440.22
6.98 778367568 395.67
7.22 1622046006 404.94

ta Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR081118\
 ta File : PR031356.D
 gnal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 q On : 08 Aug 2018 23:16
 erator : SM\SJ
 mple : J4301-21MS
 sc :
 S Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_R
 Client Sampled :
 C0AG1MS

Manual Integrations
 APPROVED

Sohil
 8/11/2018 9:27:47 AM

tegration File signal 1: autoint1.e
 tegration File signal 2: autoint2.e
 ant Time: Aug 11 00:44:50 2018
 ant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080918CLP.M
 ant Title : GC EXTRACTABLES
 ast Update : Fri Aug 10 04:14:30 2018
 sponse via : Initial Calibration
 tegrator: ChemStation

lume Inj. : 1 µl
 gnal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 gnal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
System Monitoring Compounds						
SA Tetrachlo...	4.551	3.680	544.5E6	935.7E6	23.371	23.097
SA Decachlor...	10.322	8.563	1226.4E6	759.4E6	40.568	37.214
Target Compounds						
L1 AR-1016-1	5.251	4.334	288.6E6	582.7E6	525.907	519.299
L1 AR-1016-2	5.444	4.736	304.1E6	803.6E6	523.066	461.668
L1 AR-1016-3	5.733	4.753	684.7E6	1480.1E6	791.238	533.468 #
L1 AR-1016-4	5.795	4.809	395.9E6	875.3E6	527.355	496.836
L1 AR-1016-5	6.186	5.174	333.3E6	738.5E6	502.195	453.866
L6 AR-1254-1	6.778	5.884	290.4E6	46918730	147.442	36.529 #
L6 AR-1254-2	7.059	5.967	63316583	134.9E6	52.557	54.211
L6 AR-1254-3	7.144	6.282	166.1E6	120.6E6	78.201	29.384 #
L6 AR-1254-4	7.428	6.591	120.2E6	168.3E6	66.301	83.353 #
L6 AR-1254-5	7.692	6.687	388.2E6	1579.3E6	301.816	443.019 #
L7 AR-1260-1	7.308	6.180	656.6E6	1357.8E6	467.559	413.608
L7 AR-1260-2	7.562	6.365	899.3E6	1720.5E6	463.371	433.544
L7 AR-1260-3	7.845	6.516	978.7E6	1445.4E6	468.873m	440.217
L7 AR-1260-4	8.150	6.978	648.0E6	778.4E6	429.729	395.675
L7 AR-1260-5	8.474	7.218	1469.7E6	1622.0E6	419.993	404.936

S.M
 08-10-18

)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.