

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR081118\
Data File : PR031367.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2018 01:55
Operator : SM\SJ
Sample : J4268-06
Misc :
ALS Vial : 38 Sample Multiplier: 1


Instrument :
ECD_R
ClientSampled :
C0AC4

Manual Integrations
APPROVED

Sohil
8/9/2018 1:43:37 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 03:31:48 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080918CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 08 06:03:09 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

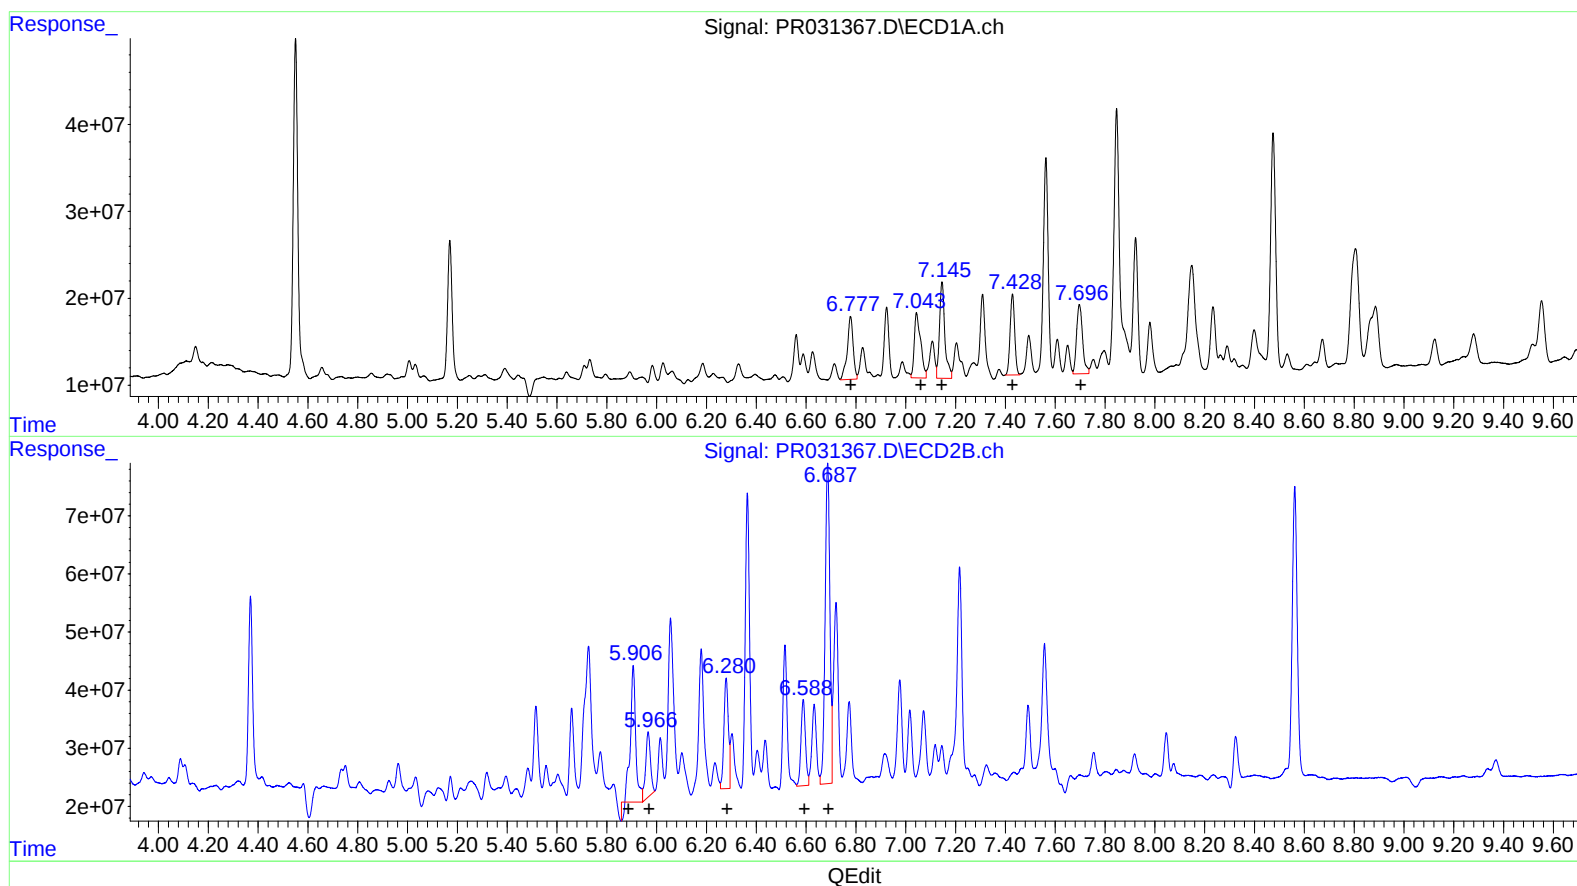

(26) AR-1254-1 (L6)
R.T. Response Conc
6.78 118749283 60.28
7.04 132722533 110.17
7.15 165900987 78.10
7.43 118430200 65.32
7.70 133722460 103.98

(26) AR-1254-1 #2 (L6)
R.T. Response Conc
5.91 423327356 329.59
5.97 151950648 61.05
6.28 235433748 57.38
6.59 185078724 91.66
6.69 732022176 205.34

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR081118\
Data File : PR031367.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2018 01:55
Operator : SM\SJ
Sample : J4268-06
Misc :
ALS Vial : 38 Sample Multiplier: 1


Instrument :
ECD_R
ClientSampleId :
C0AC4

Manual Integrations
APPROVED

Sohil
8/9/2018 1:43:37 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 03:31:48 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080918CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 08 06:03:09 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

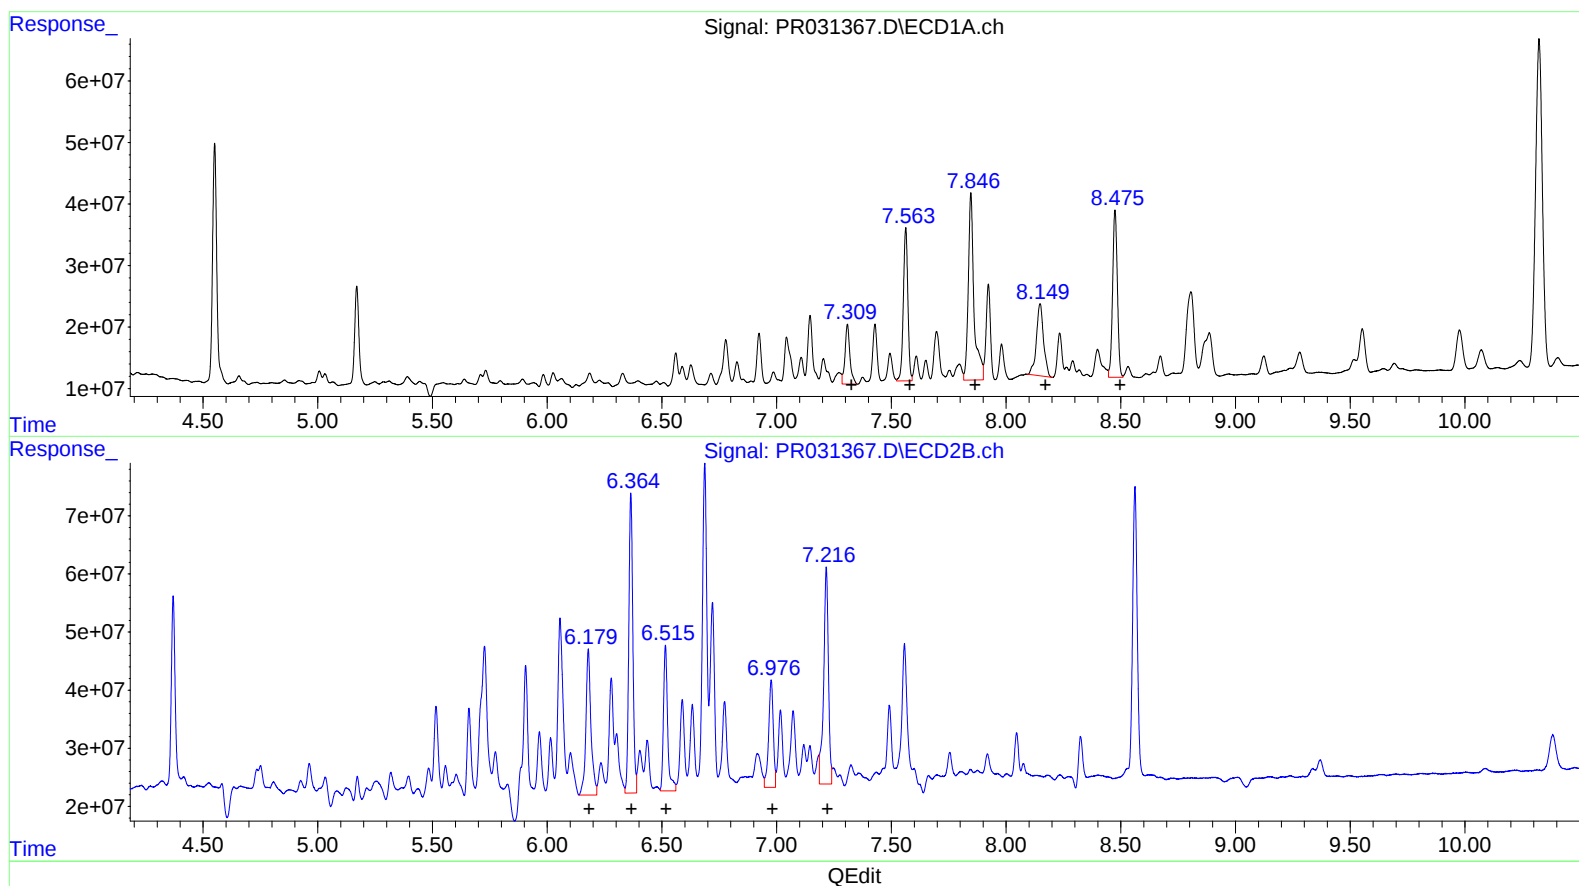

(31) AR-1260-1 #2 (L7)
R.T. Response Conc
7.31 143691574 102.32
7.56 341148289 175.78
7.85 526869233 252.41
8.15 253075324 167.82
8.47 392034962 112.03

(31) AR-1260-1 #2 (L7)
R.T. Response Conc
6.18 386394492 117.70
6.36 631896188 159.23
6.52 317853002 96.80
6.98 259463329 131.90
7.22 539945026 134.79

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR081118\
Data File : PR031367.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2018 01:55
Operator : SM\SJ
Sample : J4268-06
Misc :
ALS Vial : 38 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
C0AC4

Manual Integrations
APPROVED

Sohil
8/9/2018 1:43:37 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 03:31:48 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080918CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 08 06:03:09 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

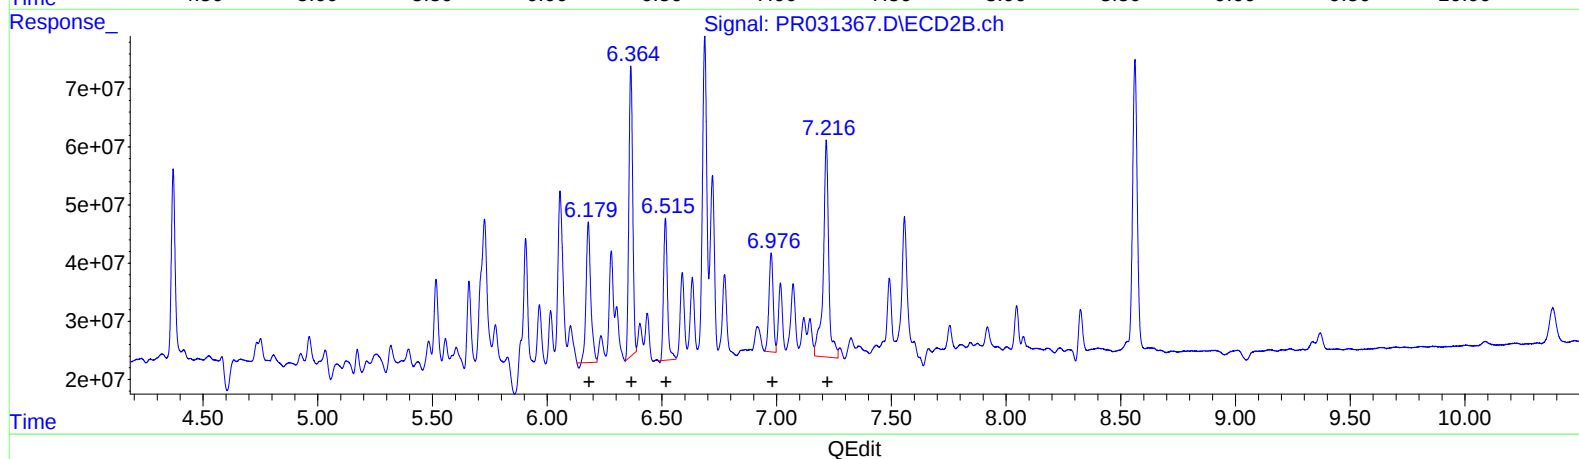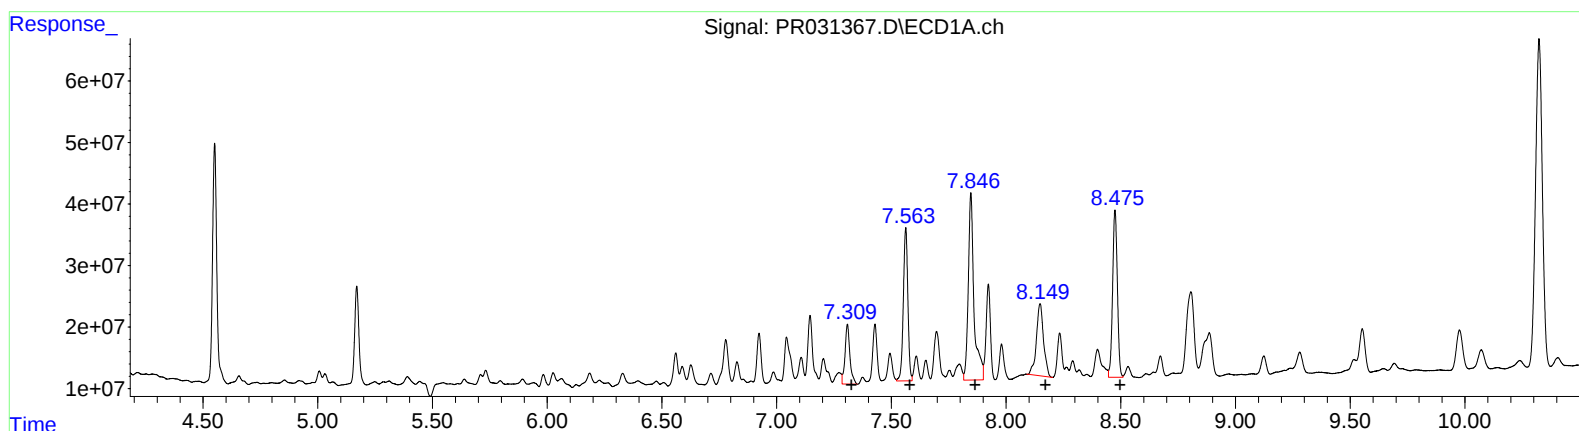

(31) AR-1260-1 (L7)
R.T. Response Conc
7.31 143691574 102.32
7.56 341148289 175.78
7.85 526869233 252.41
8.15 253075324 167.82
8.47 392034962 112.03

(31) AR-1260-1 #2 (L7)
R.T. Response Conc
6.18 339467632 103.41
6.36 580483792 146.28
6.52 290209081 88.39
6.98 216433526 110.02
7.22 622402598 155.38

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR081118\
Data File : PR031367.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2018 01:55
Operator : SM\SJ
Sample : J4268-06
Misc :
ALS Vial : 38 Sample Multiplier: 1


Instrument :
ECD_R
ClientSampled :
C0AC4

Manual Integrations
APPROVED

Sohil
8/9/2018 1:43:37 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 03:31:48 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080918CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 08 06:03:09 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

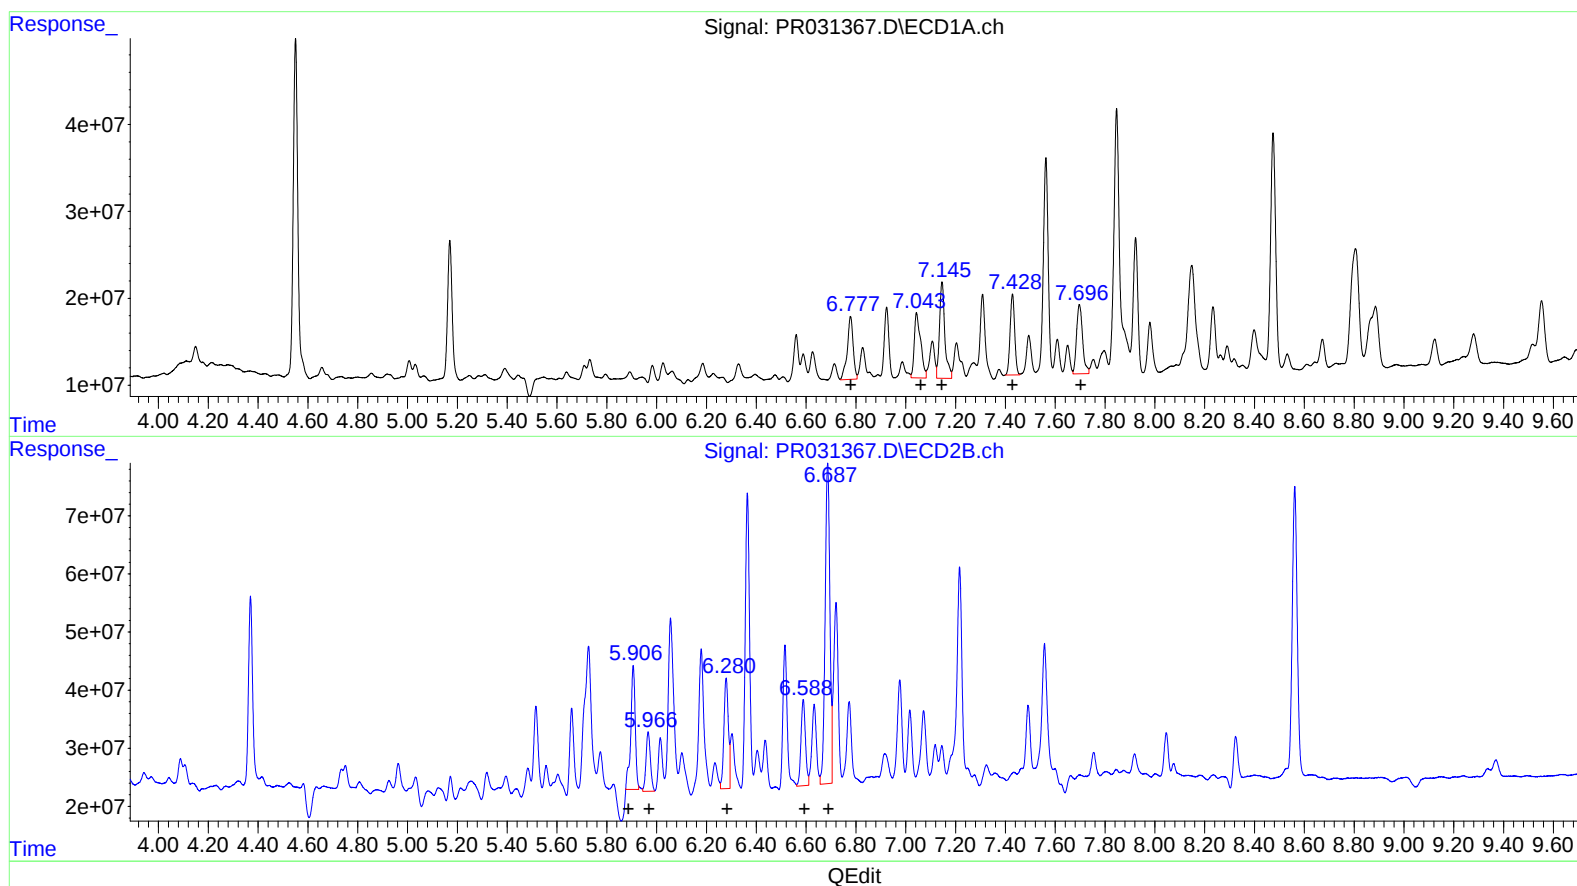

(26) AR-1254-1 #2 (L6)
R.T. Response Conc
6.78 118749283 60.28
7.04 132722533 110.17
7.15 165900987 78.10
7.43 118430200 65.32
7.70 133722460 103.98

(26) AR-1254-1 #2 (L6)
R.T. Response Conc
5.91 267503739 208.27
5.97 125235036 50.32
6.28 235433748 57.38
6.59 185078724 91.66
6.69 732022176 205.34

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR081118\
 Data File : PR031367.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2018 01:55
 Operator : SM\SJ
 Sample : J4268-06
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_R
 Client Sample Id :
 C0AC4

Manual Integrations
 APPROVED

Sohil
 8/9/2018 1:43:37 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 03:31:48 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080918CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 08 06:03:09 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.551	3.678	504.4E6	797.3E6	21.649	19.681
2) SA Decachlor...	10.323	8.562	1091.0E6	669.2E6	36.089	32.794
Target Compounds						
26) L6 AR-1254-1	6.778	5.906	118.7E6	267.5E6	60.283	208.268m#)
27) L6 AR-1254-2	7.043	5.966	132.7E6	125.2E6	110.169	50.319m#)
28) L6 AR-1254-3	7.146	6.279	165.9E6	235.4E6	78.099	57.377 #
29) L6 AR-1254-4	7.429	6.589	118.4E6	185.1E6	65.324	91.664 #
30) L6 AR-1254-5	7.697	6.687	133.7E6	732.0E6	103.979	205.342 #
31) L7 AR-1260-1	7.309	6.179	143.7E6	386.4E6	102.317	117.702m)
32) L7 AR-1260-2	7.563	6.364	341.1E6	631.9E6	175.785	159.231m)
33) L7 AR-1260-3	7.847	6.515	526.9E6	317.9E6	252.410	96.805m#)
34) L7 AR-1260-4	8.148	6.976	253.1E6	259.5E6	167.825	131.895m)
35) L7 AR-1260-5	8.475	7.216	392.0E6	539.9E6	112.030	134.795m)

} SM08/10/18

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.