

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR081219\
 Data File : PR040313.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2019 21:18
 Operator : SM\AJ
 Sample : K4230-29
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 REACTOR-3A-(0-3)-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 04:35:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR081019.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 10 07:38:17 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
35)	L7	AR-1260-5	0.000	8.510	0 48732655	56.885 #
37)	L8	AR-1262-2	0.000	8.510	0 48732655	49.968 #
38)	L8	AR-1262-3	0.000	8.825	0 26964420	41.465 #
39)	L8	AR-1262-4	0.000	8.825	0 26964420	54.071 #
40)	L8	AR-1262-5	8.167	0.000	4582645 0	46.769 N.D. #
41)	L9	AR-1268-1	0.000	8.825	0 26964420	18.792 #
44)	L9	AR-1268-4	8.167	0.000	4582645 0	32.860 N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR081219\
Data File : PR040313.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2019 21:18
Operator : SM\AJ
Sample : K4230-29
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
REACTOR-3A-(0-3)-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 04:35:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR081019.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 10 07:38:17 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

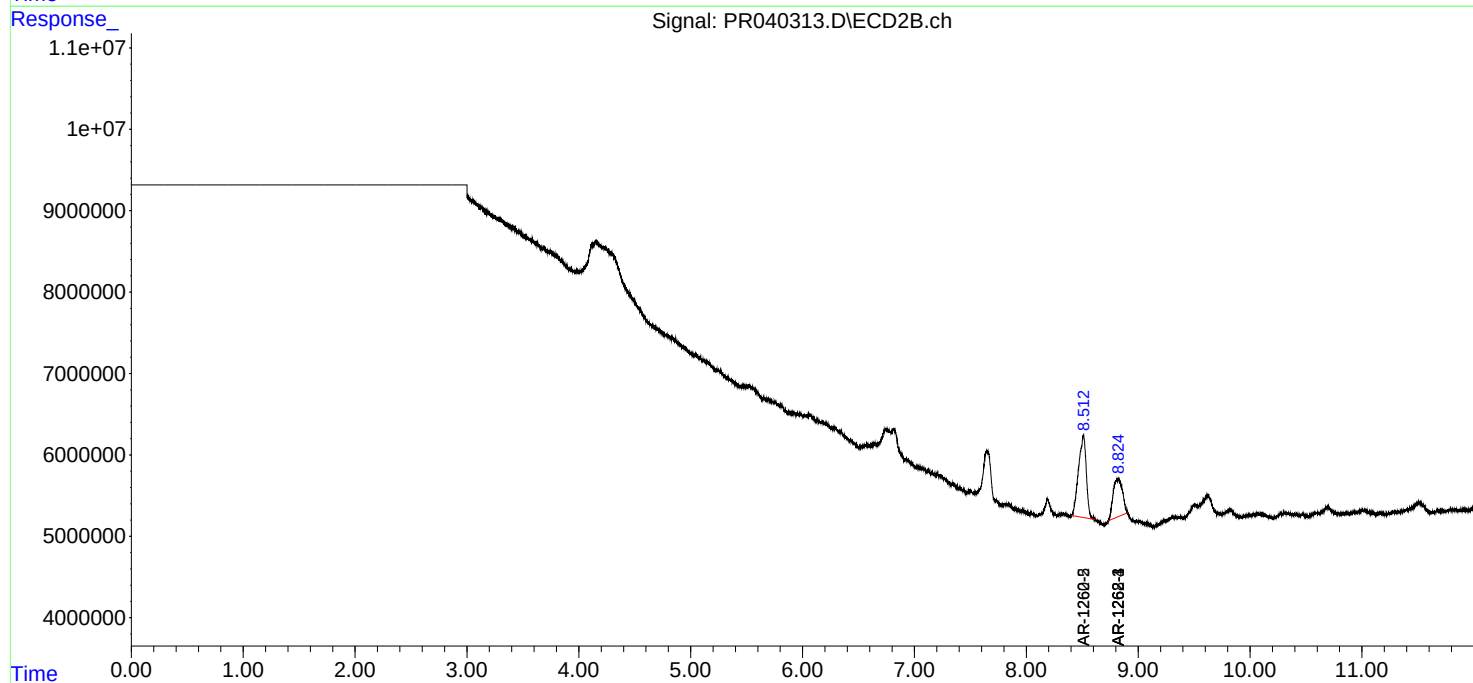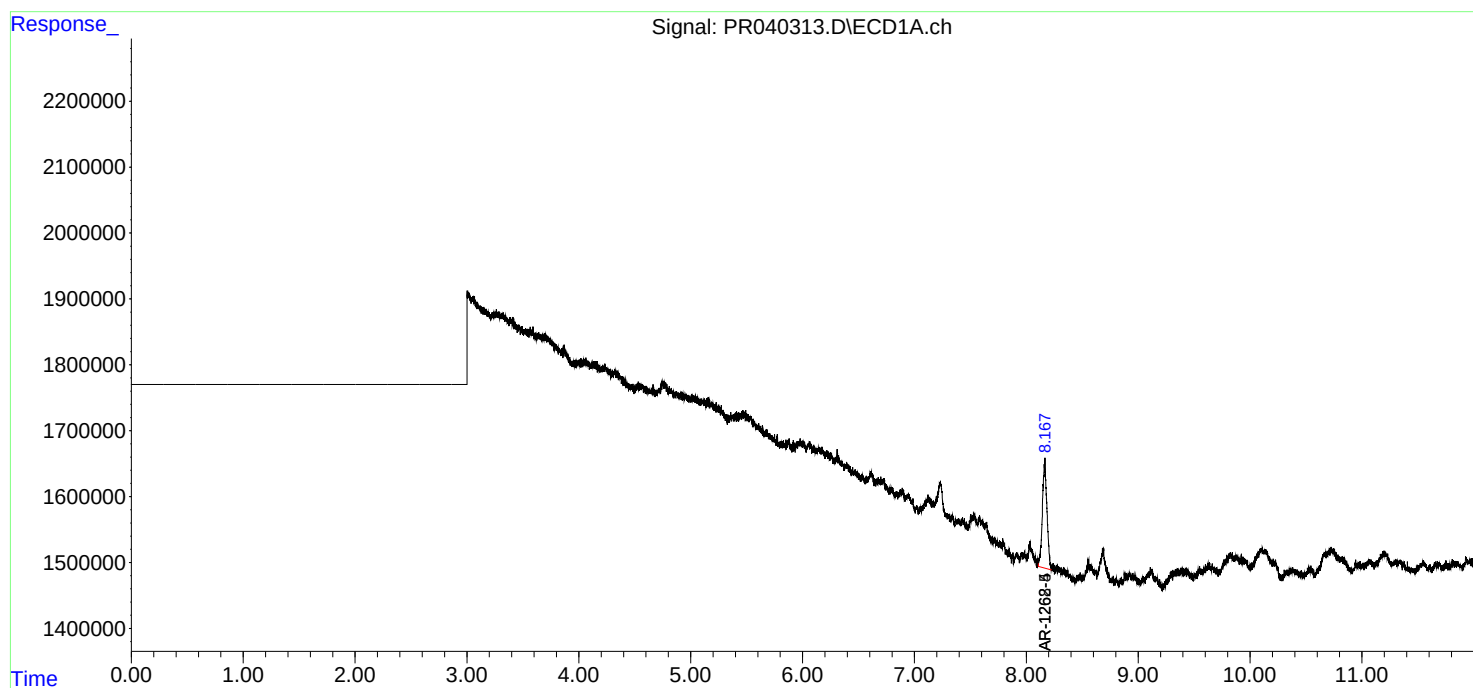


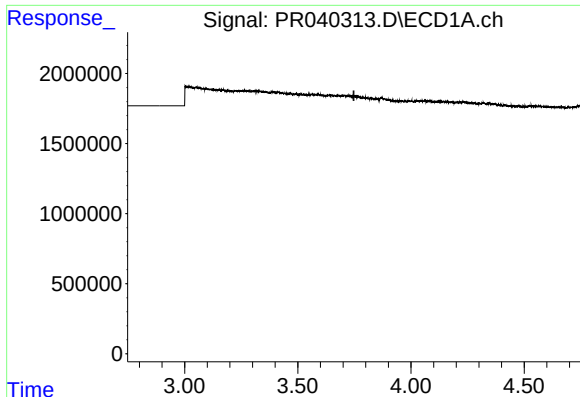

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.748 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
REACTOR-3A-(0-3)-COMP

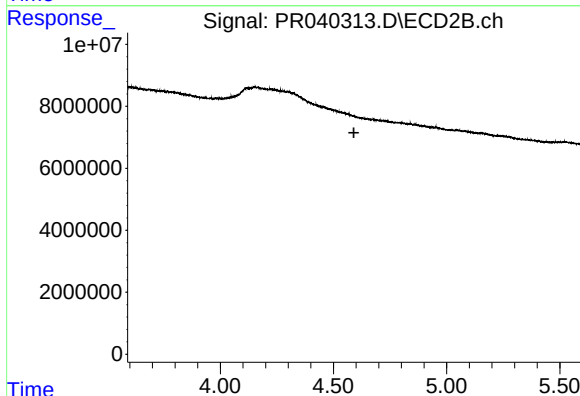


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.590 min
Response: 0
Conc: N.D.

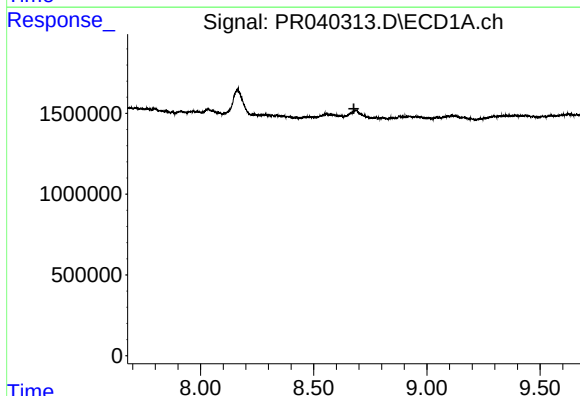


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.678 min
Response: 0
Conc: N.D.

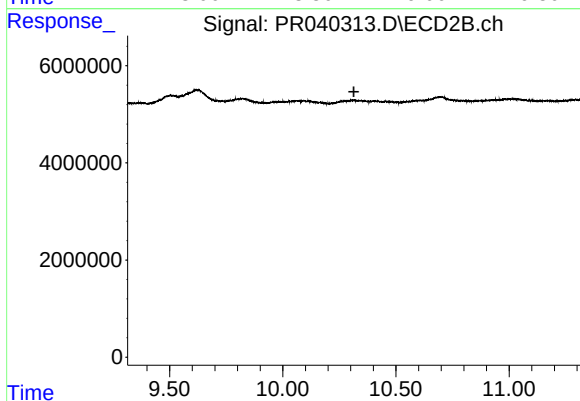

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 10.314 min
Response: 0
Conc: N.D.

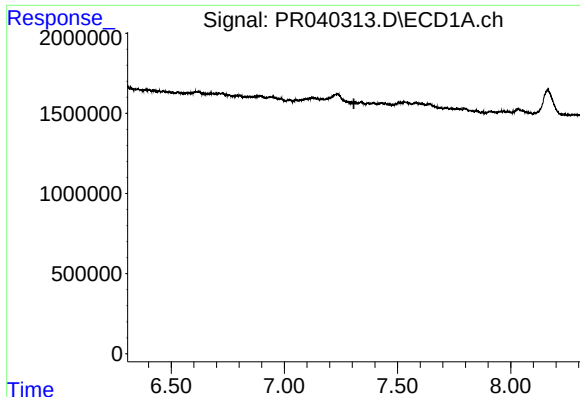

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 7.307 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
REACTOR-3A-(0-3)-COMP

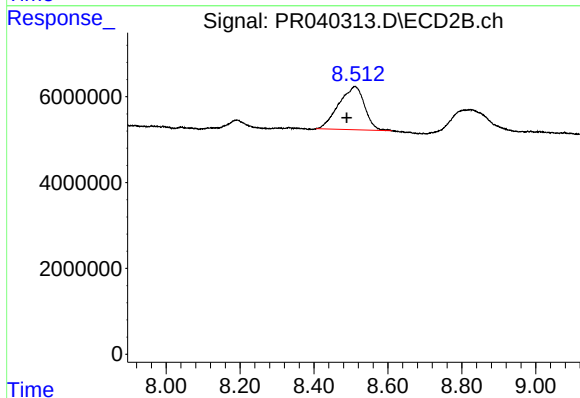


#35 AR-1260-5

R.T.: 8.510 min
Delta R.T.: 0.021 min
Response: 48732655
Conc: 56.88 ng/ml

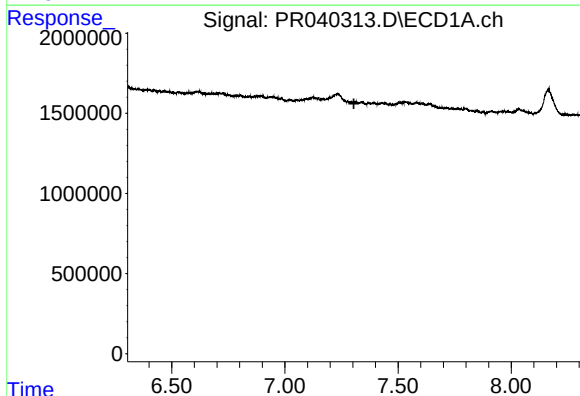


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T.: 7.305 min
Response: 0
Conc: N.D.

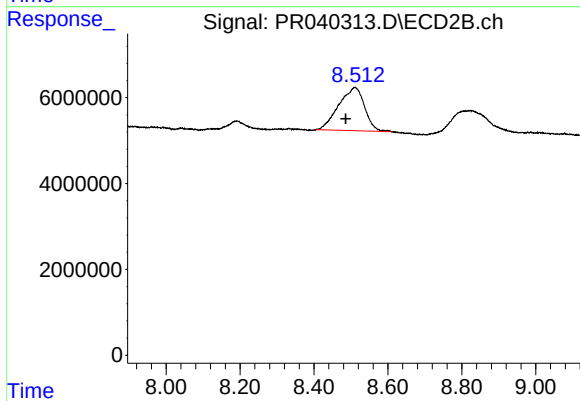

#37 AR-1262-2


R.T.: 8.510 min
Delta R.T.: 0.024 min
Response: 48732655
Conc: 49.97 ng/ml

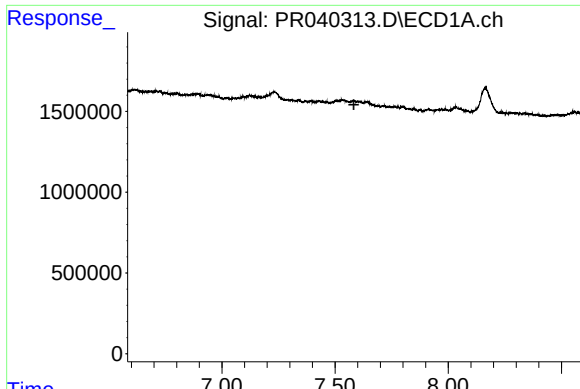

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 7.583 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
REACTOR-3A-(0-3)-COMP

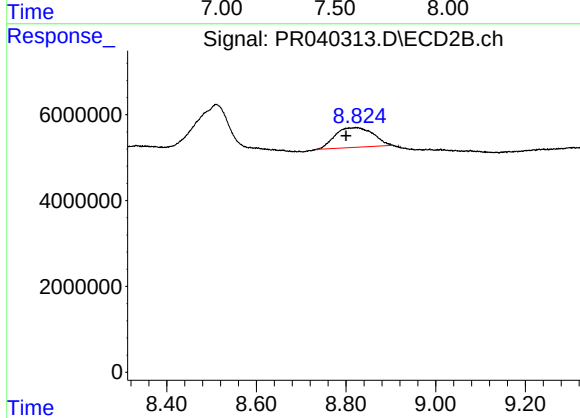


#38 AR-1262-3

R.T.: 8.825 min
Delta R.T.: 0.025 min
Response: 26964420
Conc: 41.47 ng/ml

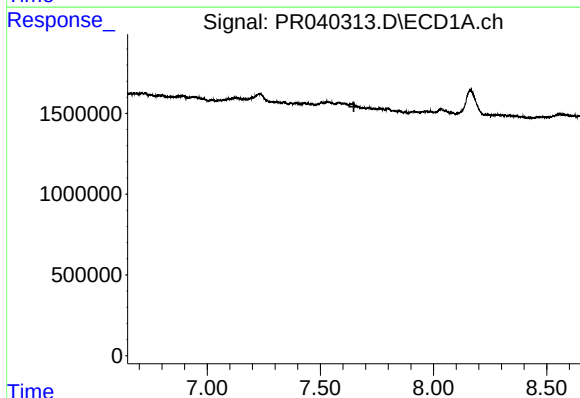


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T.: 7.648 min
Response: 0
Conc: N.D.

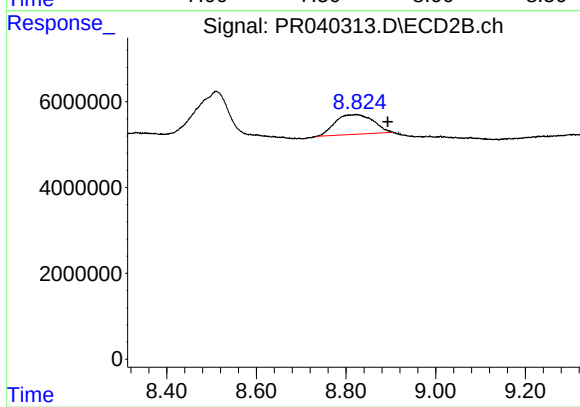

#39 AR-1262-4


R.T.: 8.825 min
Delta R.T.: -0.068 min
Response: 26964420
Conc: 54.07 ng/ml

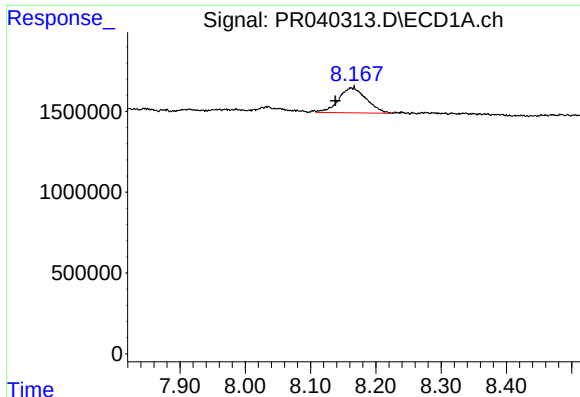

#40 AR-1262-5


R.T.: 8.167 min
Delta R.T.: 0.029 min
Response: 4582645
Conc: 46.77 ng/ml

Instrument :
ECD_R
ClientSampleId :
REACTOR-3A-(0-3)-COMP

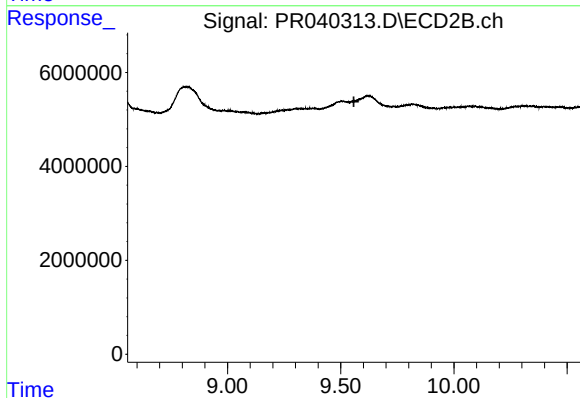


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 9.558 min
Response: 0
Conc: N.D.

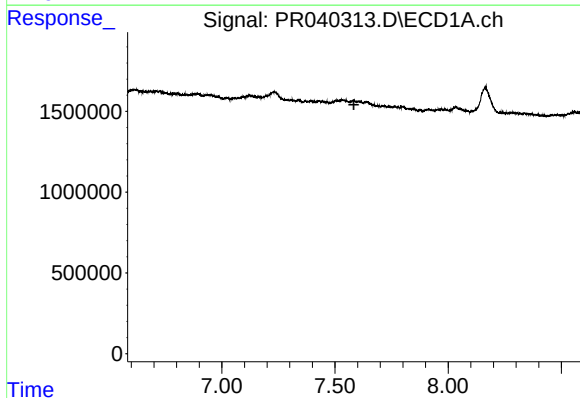


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 7.584 min
Response: 0
Conc: N.D.

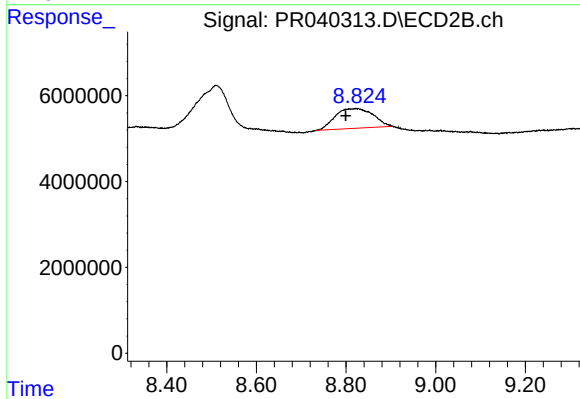

#41 AR-1268-1


R.T.: 8.825 min
Delta R.T.: 0.025 min
Response: 26964420
Conc: 18.79 ng/ml

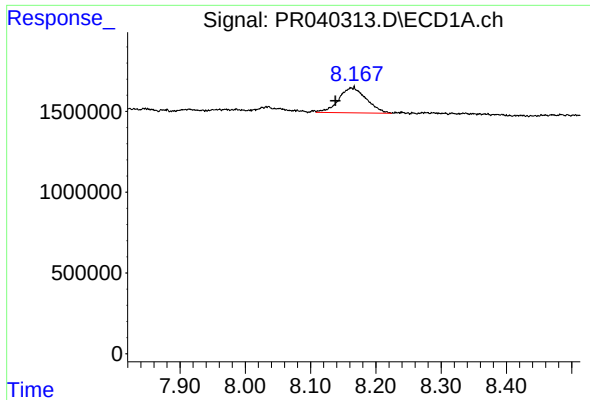

#44 AR-1268-4

R.T.: 8.167 min
Delta R.T.: 0.029 min
Response: 4582645
Conc: 32.86 ng/ml

Instrument :
ECD_R
ClientSampleId :
REACTOR-3A-(0-3)-COMP

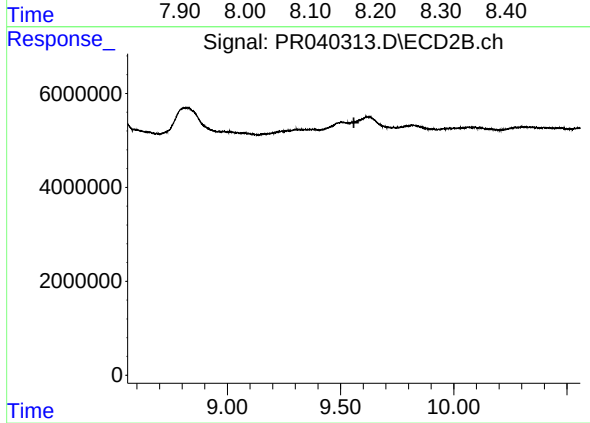

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 9.559 min
Response: 0
Conc: N.D.