

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR081224\
 Data File : PR068139.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2024 10:01
 Operator : AJ\MA
 Sample : P3390-09
 Misc : AR1221 MDL 25 PPB
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 11:08:02 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 08 22:24:34 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.677	3.010	36387813	82828181	14.650	16.646
2)	SA Decachlor...	9.584	8.328	76178179	87308795	16.966	16.647
Target Compounds							
3)	L1 AR-1016-1	4.905	4.141	377927	338203	6.413	1.929 #
4)	L1 AR-1016-2	4.919	4.160	492421	612591	4.397	2.493 #
5)	L1 AR-1016-3	4.987	4.340	231295	551476	3.071	4.069 #
6)	L1 AR-1016-4	0.000	4.391	0	198232	N.D.	1.747 #
7)	L1 AR-1016-5	5.420f	0.000	75671	0	1.569	N.D. #
8)	L2 AR-1221-1	3.896	3.236	1241502	1532560	44.827	23.824 #
9)	L2 AR-1221-2	3.989	3.320	1234002	2297060	54.068	48.108
10)	L2 AR-1221-3	4.067	3.401	1657963	3157624	23.625	23.576
11)	L3 AR-1232-1	4.067	3.401	1657963	3157624	28.205	28.558
12)	L3 AR-1232-2	4.613	4.160	678561	612591	20.736	5.486 #
13)	L3 AR-1232-3	4.919	4.340	492421	551476	9.108	8.835
14)	L3 AR-1232-4	0.000	4.429	0	99954	N.D.	1.762 #
15)	L3 AR-1232-5	5.186	0.000	97473	0	6.655	N.D. #
16)	L4 AR-1242-1	4.905	4.141	377927	338203	8.551	2.654 #
17)	L4 AR-1242-2	4.919	4.160	492421	612591	5.801	3.445 #
18)	L4 AR-1242-3	4.987	4.340	231295	551476	3.966	5.511 #
19)	L4 AR-1242-4	0.000	4.429	0	99954	N.D.	0.979 #
20)	L4 AR-1242-5	5.865	4.985	155785	96760	3.590	0.756 #
21)	L5 AR-1248-1	4.905	4.141	377927	338203	10.378	3.204 #
22)	L5 AR-1248-2	5.186	4.391	97473	198232	1.979	1.265 #
23)	L5 AR-1248-3	5.420f	4.429	75671	99954	1.116	0.629 #
24)	L5 AR-1248-4	5.865f	0.000	155785	0	2.171	N.D. #
25)	L5 AR-1248-5	5.865	5.013f	155785	504395	1.988	2.776 #
26)	L6 AR-1254-1	5.810	4.985	819697	96760	12.094	0.352 #
27)	L6 AR-1254-2	6.046	5.151	137225	446365	1.279	1.786 #
28)	L6 AR-1254-3	6.429	5.555f	304110	2701120	2.336	6.964 #
29)	L6 AR-1254-4	6.729f	0.000	543350	0	5.080	N.D. #
30)	L6 AR-1254-5	7.178f	0.000	332689	0	2.626	N.D. #
31)	L7 AR-1260-1	6.611	5.720	40420	402242	0.449	1.363 #
32)	L7 AR-1260-2	6.896	5.924	271257	58810	1.878	0.171 #
33)	L7 AR-1260-3	0.000	6.088	0	608744	N.D.	1.883 #
34)	L7 AR-1260-4	0.000	6.589	0	193188	N.D.	0.780 #
35)	L7 AR-1260-5	0.000	6.866	0	287512	N.D.	0.510 #
36)	L8 AR-1262-1	0.000	6.307	0	63170	N.D.	0.172 #
37)	L8 AR-1262-2	0.000	6.866	0	287512	N.D.	0.460 #
38)	L8 AR-1262-3	8.169	0.000	200190	0	0.610	N.D. #
39)	L8 AR-1262-4	8.267	7.238	505267	159590	1.773	0.338 #
41)	L9 AR-1268-1	8.169	0.000	200190	0	0.315	N.D. #
42)	L9 AR-1268-2	8.267	7.238	505267	159590	0.859	0.244 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR081224\
Data File : PR068139.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2024 10:01
Operator : AJ\MA
Sample : P3390-09
Misc : AR1221 MDL 25 PPB
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 12 11:08:02 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080824.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 08 22:24:34 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43)	L9 AR-1268-3	0.000	7.467	0	130516	N.D.	0.222 #
45)	L9 AR-1268-5	9.270	8.075	1512171	615811	0.935	0.375 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR081224\
Data File : PR068139.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2024 10:01
Operator : AJ\MA
Sample : P3390-09
Misc : AR1221 MDL 25 PPB
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 12 11:08:02 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080824.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 08 22:24:34 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

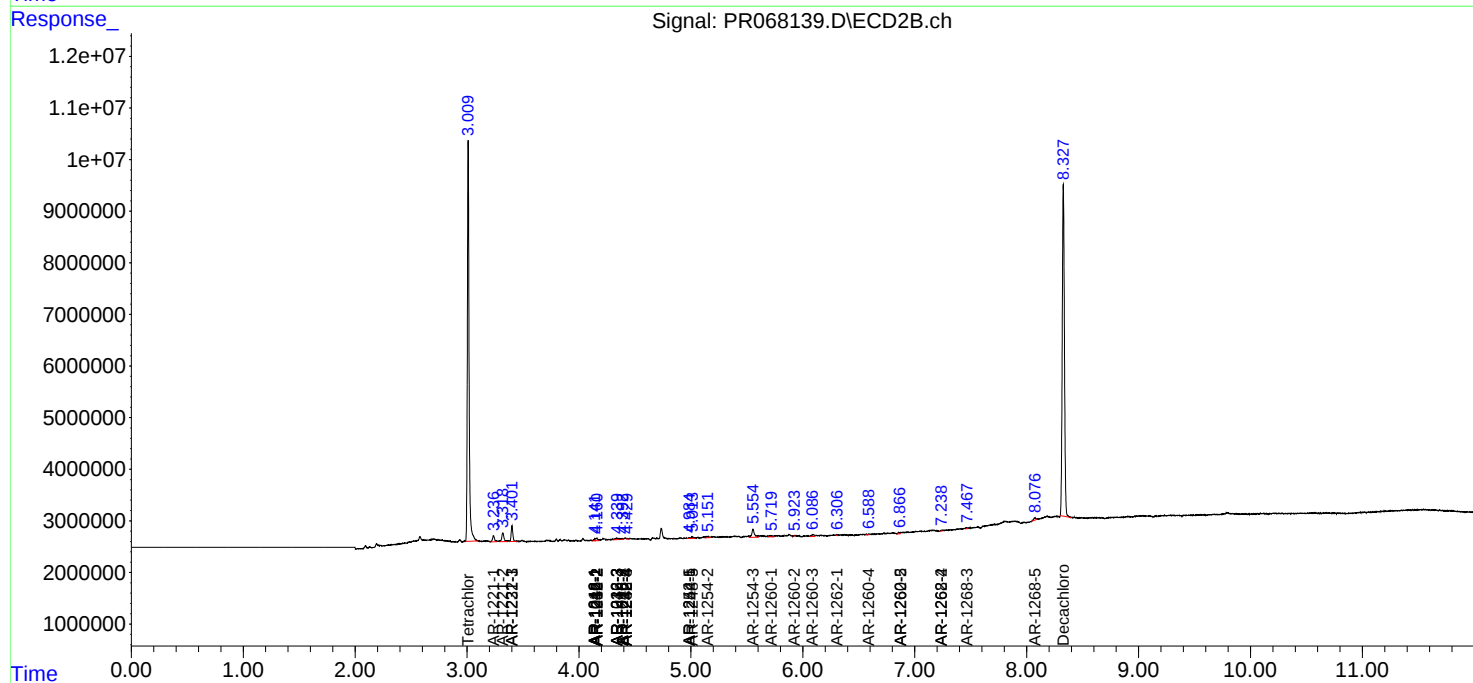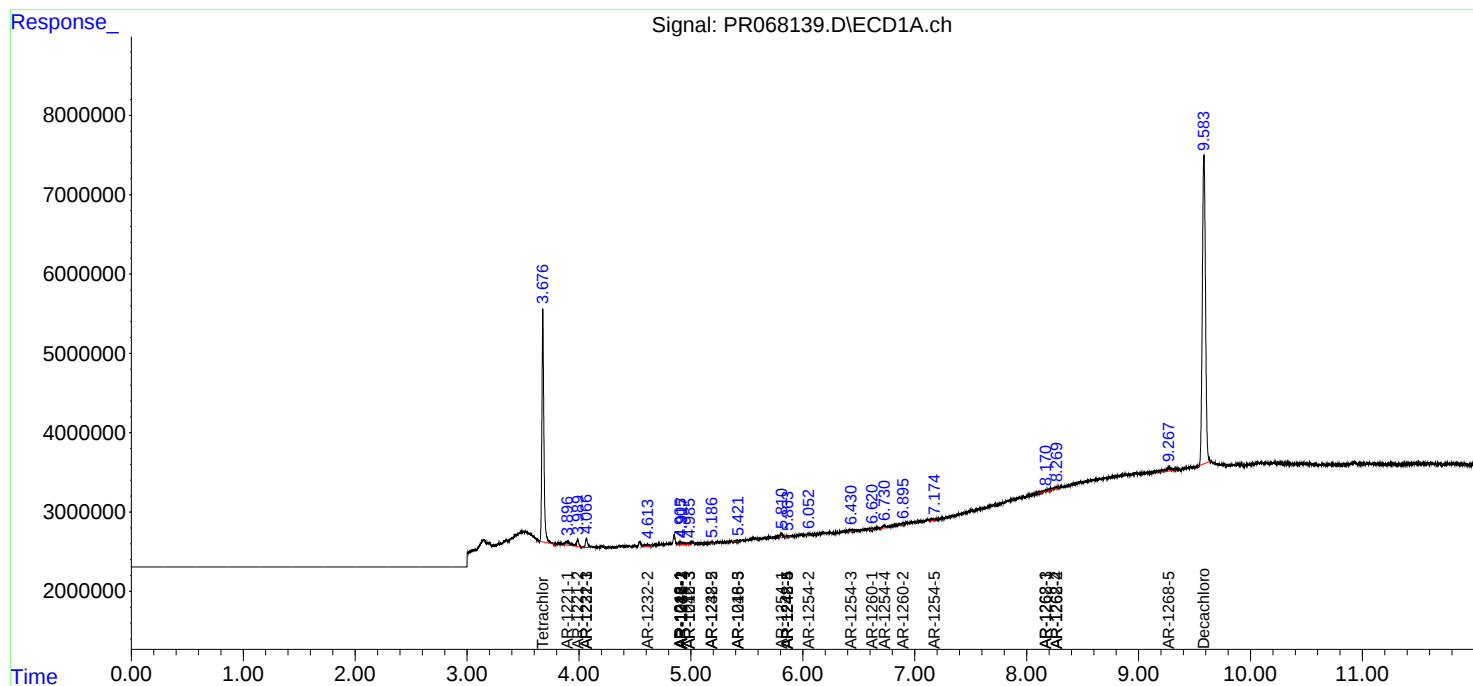


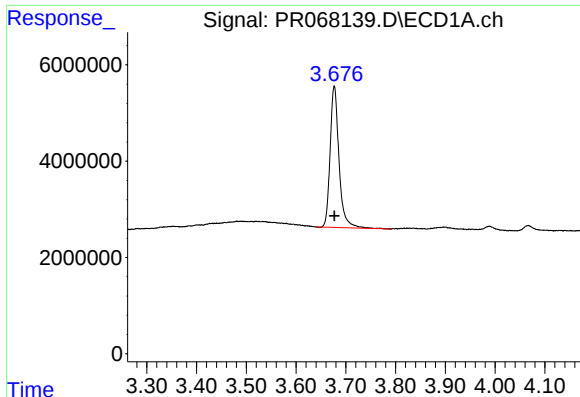

#1 Tetrachloro-m-xylene


R.T.: 3.677 min
Delta R.T.: 0.000 min
Response: 36387813
Conc: 14.65 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

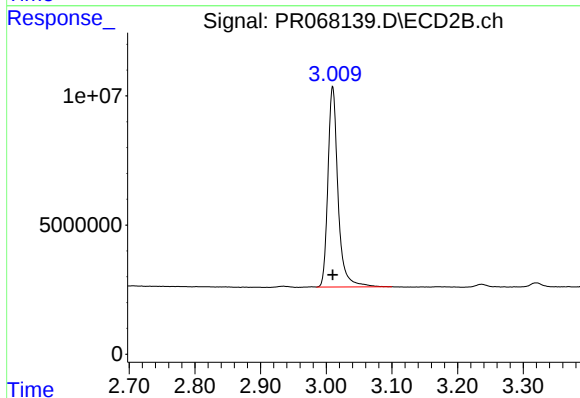


#1 Tetrachloro-m-xylene

R.T.: 3.010 min
Delta R.T.: 0.000 min
Response: 82828181
Conc: 16.65 ng/ml

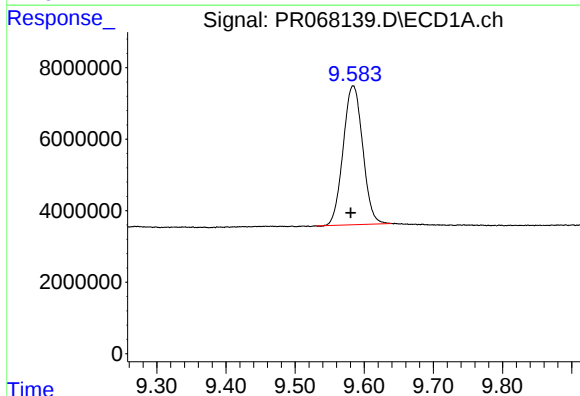


#2 Decachlorobiphenyl

R.T.: 9.584 min
Delta R.T.: 0.003 min
Response: 76178179
Conc: 16.97 ng/ml

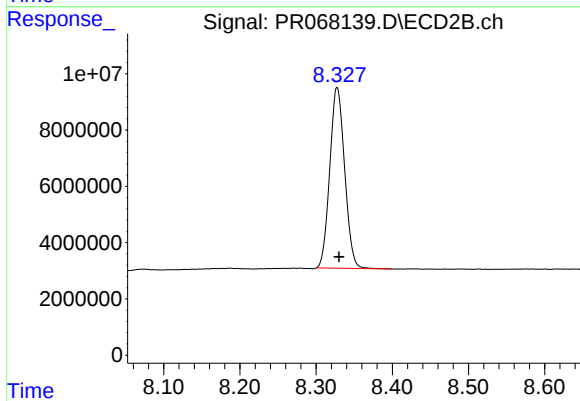

#2 Decachlorobiphenyl


R.T.: 8.328 min
Delta R.T.: -0.003 min
Response: 87308795
Conc: 16.65 ng/ml

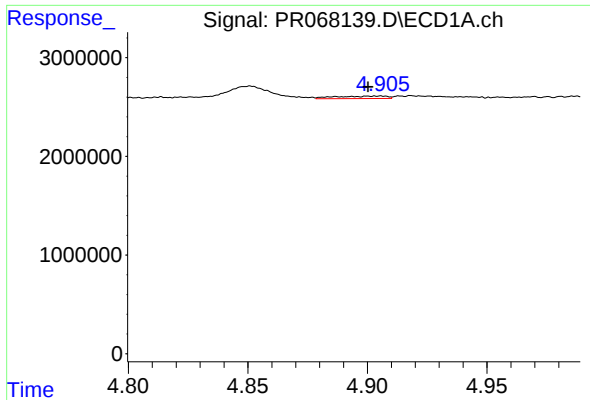

#3 AR-1016-1


R.T.: 4.905 min
Delta R.T.: 0.005 min
Response: 377927
Conc: 6.41 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

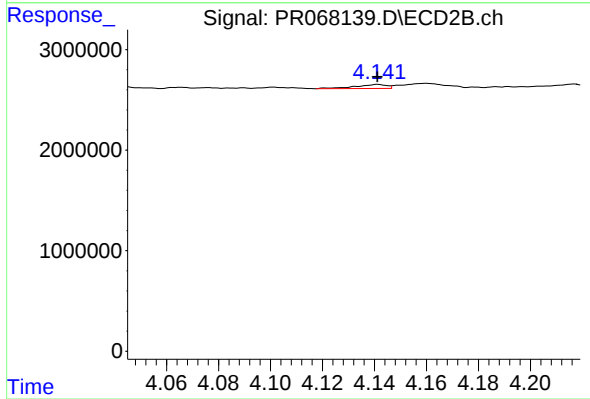


#3 AR-1016-1

R.T.: 4.141 min
Delta R.T.: 0.000 min
Response: 338203
Conc: 1.93 ng/ml

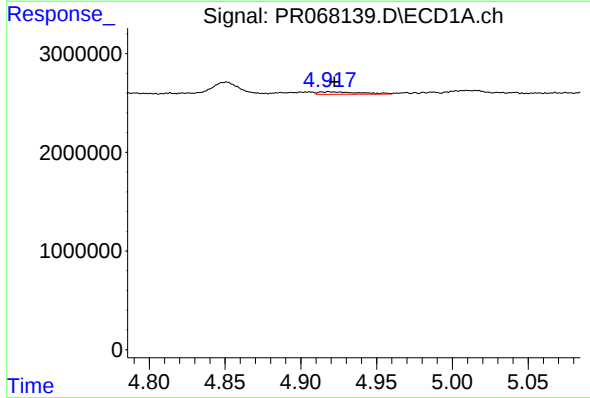


#4 AR-1016-2

R.T.: 4.919 min
Delta R.T.: -0.003 min
Response: 492421
Conc: 4.40 ng/ml

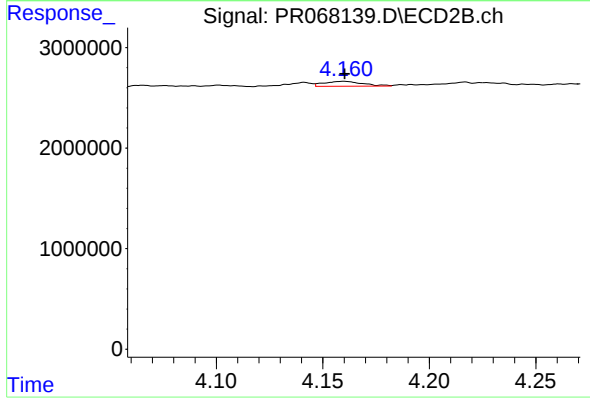

#4 AR-1016-2


R.T.: 4.160 min
Delta R.T.: 0.000 min
Response: 612591
Conc: 2.49 ng/ml

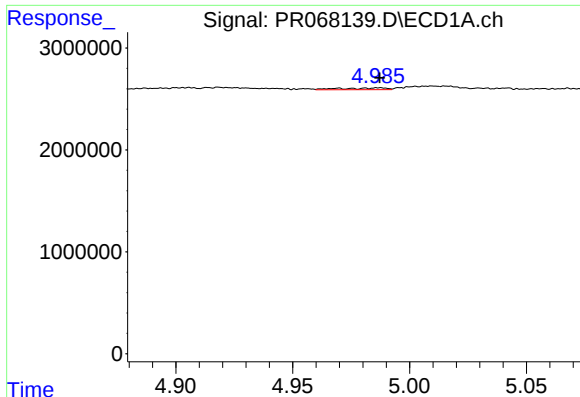

#5 AR-1016-3


R.T.: 4.987 min
Delta R.T.: 0.000 min
Response: 231295
Conc: 3.07 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

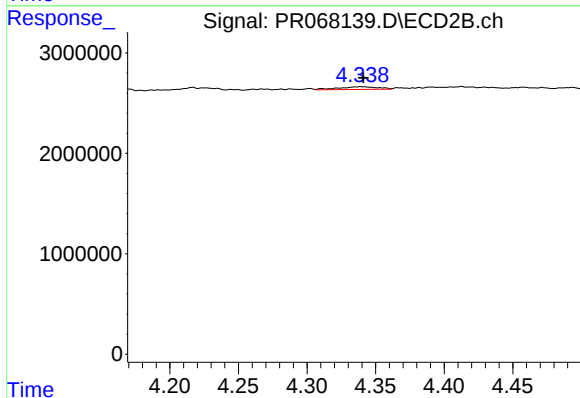


#5 AR-1016-3

R.T.: 4.340 min
Delta R.T.: -0.002 min
Response: 551476
Conc: 4.07 ng/ml

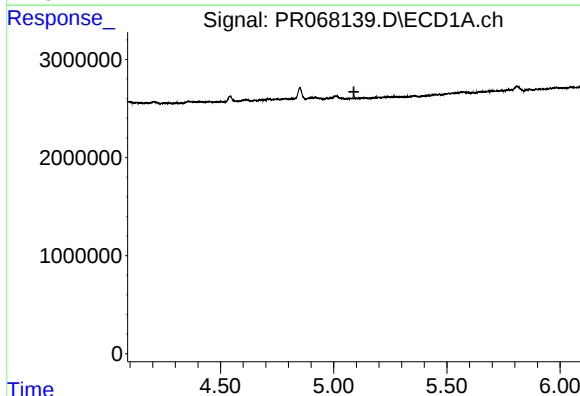


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T. : 5.089 min
Response: 0
Conc: N.D.

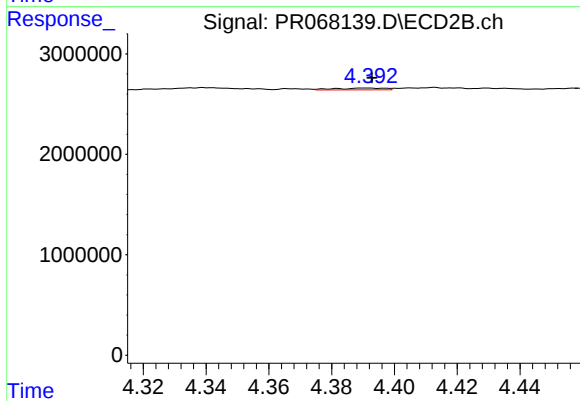

#6 AR-1016-4


R.T.: 4.391 min
Delta R.T.: -0.002 min
Response: 198232
Conc: 1.75 ng/ml

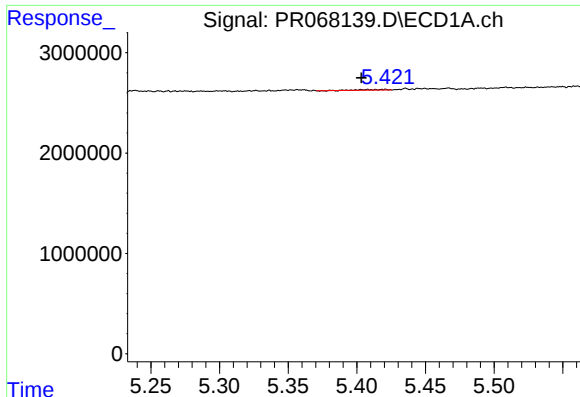

#7 AR-1016-5


R.T.: 5.420 min
Delta R.T.: 0.017 min
Response: 75671
Conc: 1.57 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

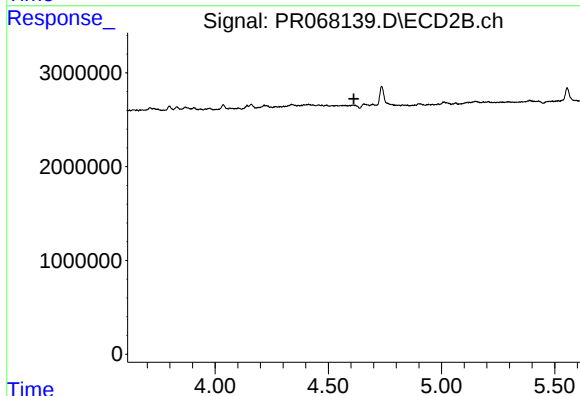


#7 AR-1016-5

R.T.: 0.000 min
Exp R.T. : 4.613 min
Response: 0
Conc: N.D.

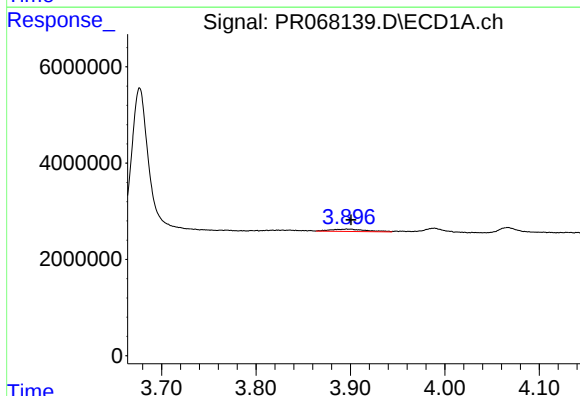


#8 AR-1221-1

R.T.: 3.896 min
Delta R.T.: -0.004 min
Response: 1241502
Conc: 44.83 ng/ml

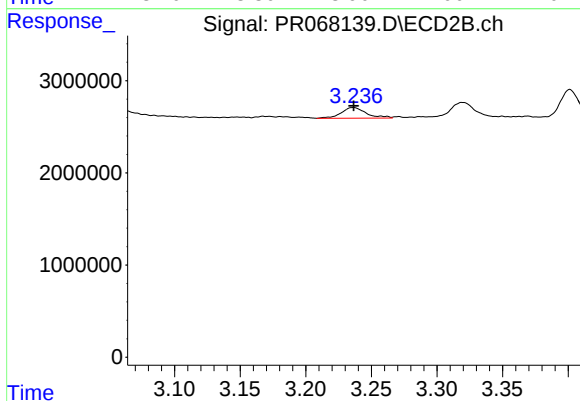

#8 AR-1221-1


R.T.: 3.236 min
Delta R.T.: 0.000 min
Response: 1532560
Conc: 23.82 ng/ml

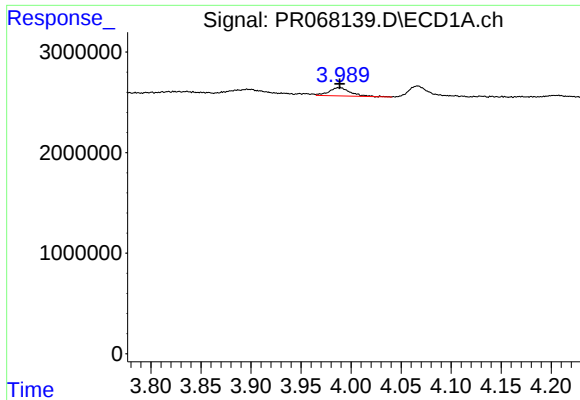

#9 AR-1221-2


R.T.: 3.989 min
Delta R.T.: 0.000 min
Response: 1234002
Conc: 54.07 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

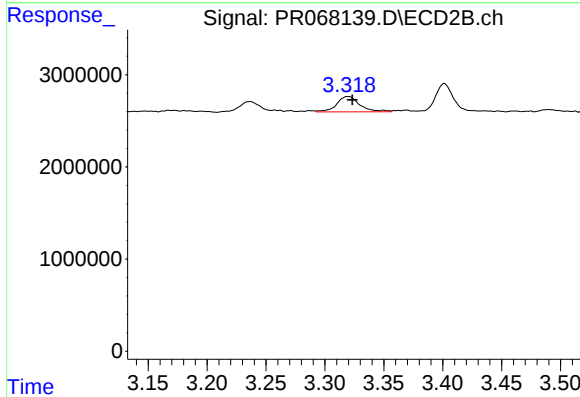


#9 AR-1221-2

R.T.: 3.320 min
Delta R.T.: -0.004 min
Response: 2297060
Conc: 48.11 ng/ml

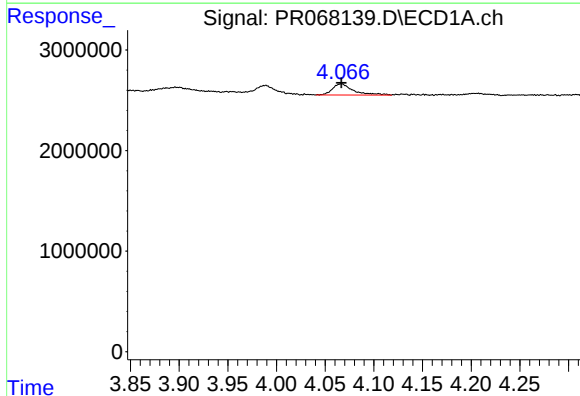


#10 AR-1221-3

R.T.: 4.067 min
Delta R.T.: 0.000 min
Response: 1657963
Conc: 23.62 ng/ml

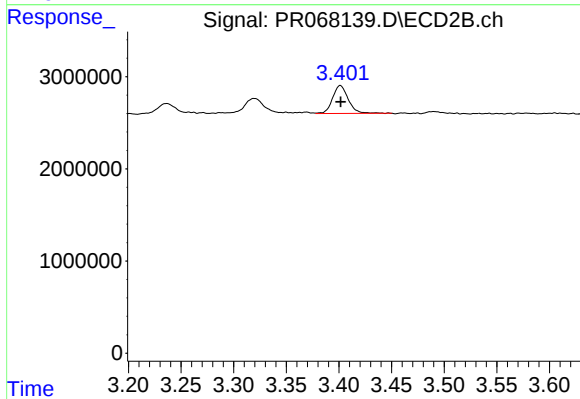

#10 AR-1221-3


R.T.: 3.401 min
Delta R.T.: 0.000 min
Response: 3157624
Conc: 23.58 ng/ml

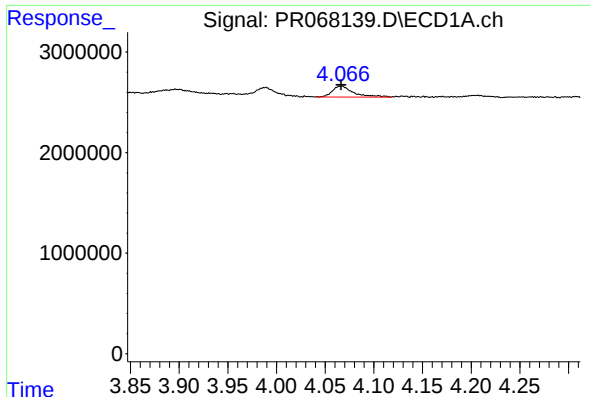

#11 AR-1232-1


R.T.: 4.067 min
Delta R.T.: 0.000 min
Response: 1657963
Conc: 28.21 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

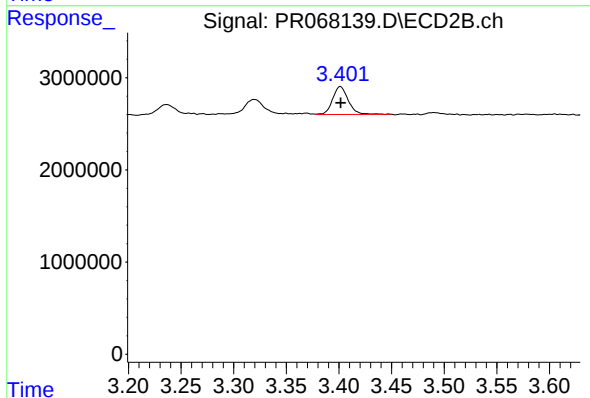


#11 AR-1232-1

R.T.: 3.401 min
Delta R.T.: 0.000 min
Response: 3157624
Conc: 28.56 ng/ml

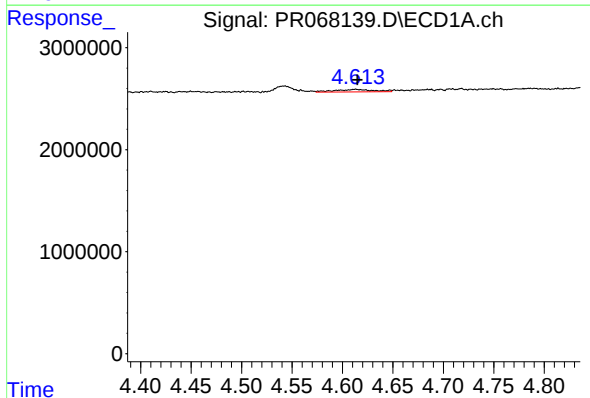


#12 AR-1232-2

R.T.: 4.613 min
Delta R.T.: -0.002 min
Response: 678561
Conc: 20.74 ng/ml

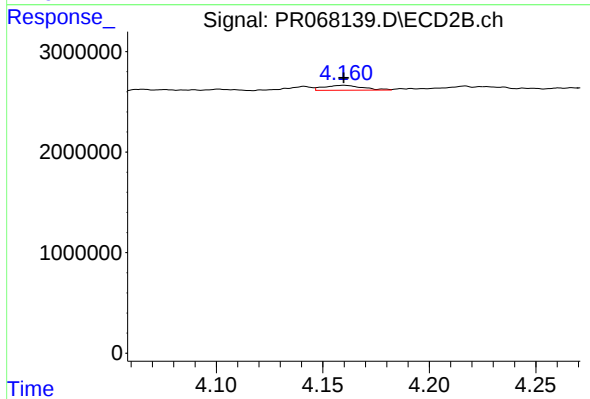

#12 AR-1232-2


R.T.: 4.160 min
Delta R.T.: 0.000 min
Response: 612591
Conc: 5.49 ng/ml

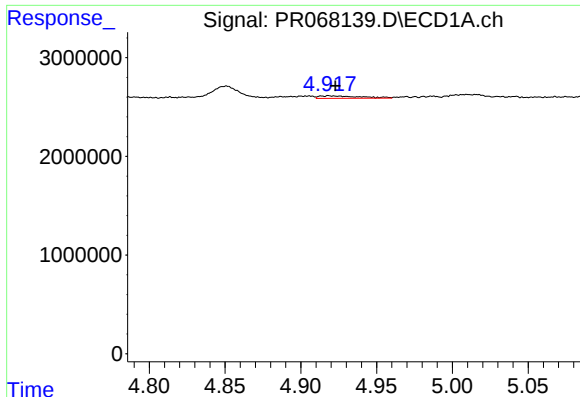

#13 AR-1232-3


R.T.: 4.919 min
Delta R.T.: -0.004 min
Response: 492421
Conc: 9.11 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

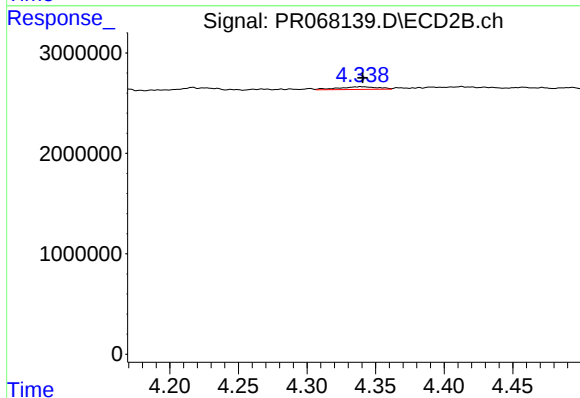


#13 AR-1232-3

R.T.: 4.340 min
Delta R.T.: 0.000 min
Response: 551476
Conc: 8.84 ng/ml

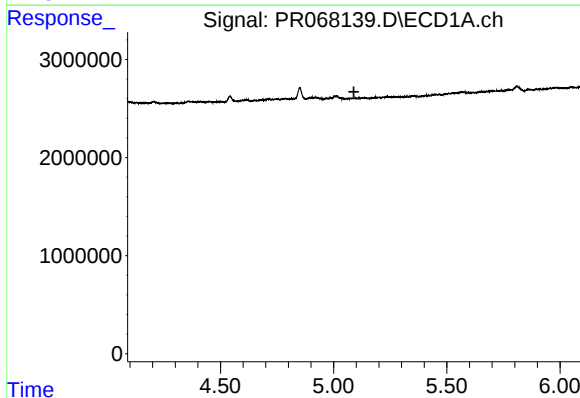


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T. : 5.089 min
Response: 0
Conc: N.D.

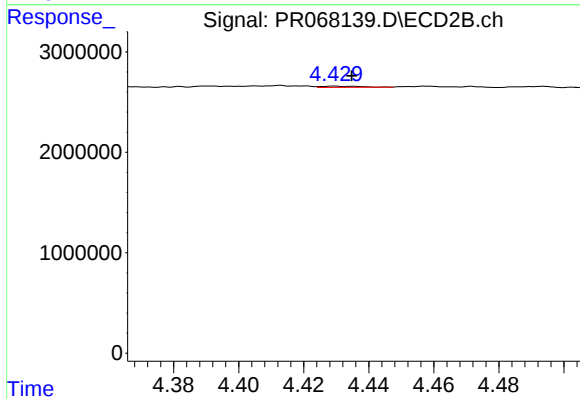

#14 AR-1232-4


R.T.: 4.429 min
Delta R.T.: -0.005 min
Response: 99954
Conc: 1.76 ng/ml

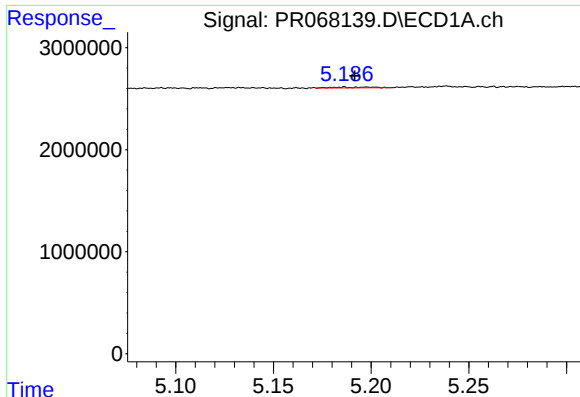

#15 AR-1232-5


R.T.: 5.186 min
Delta R.T.: -0.005 min
Response: 97473
Conc: 6.65 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

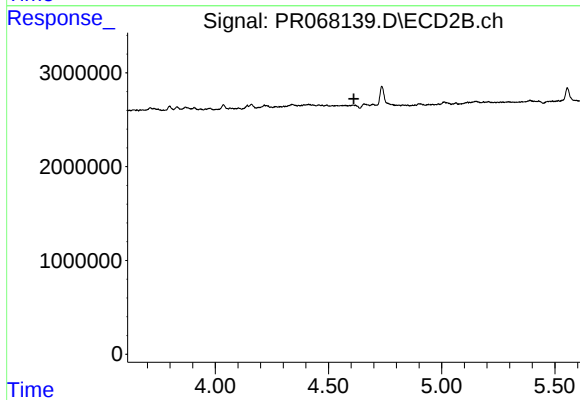


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T. : 4.612 min
Response: 0
Conc: N.D.

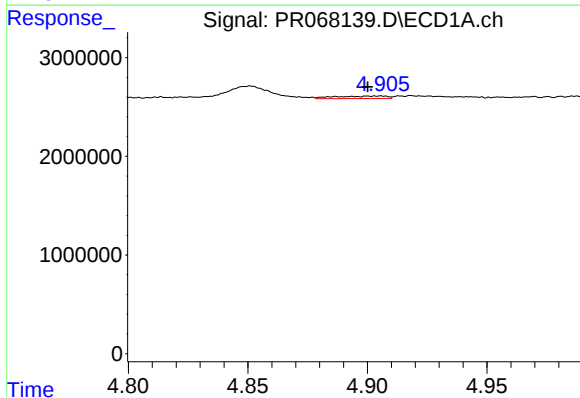


#16 AR-1242-1

R.T.: 4.905 min
Delta R.T.: 0.005 min
Response: 377927
Conc: 8.55 ng/ml

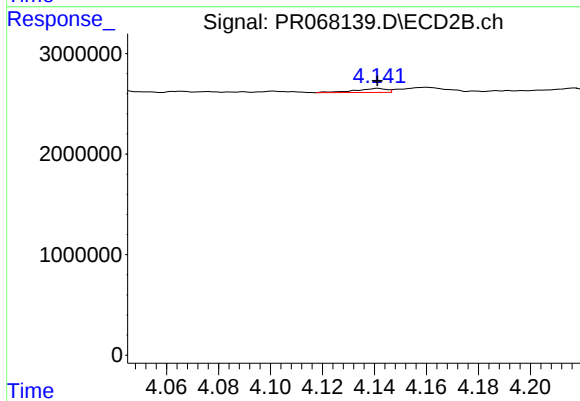

#16 AR-1242-1


R.T.: 4.141 min
Delta R.T.: 0.000 min
Response: 338203
Conc: 2.65 ng/ml

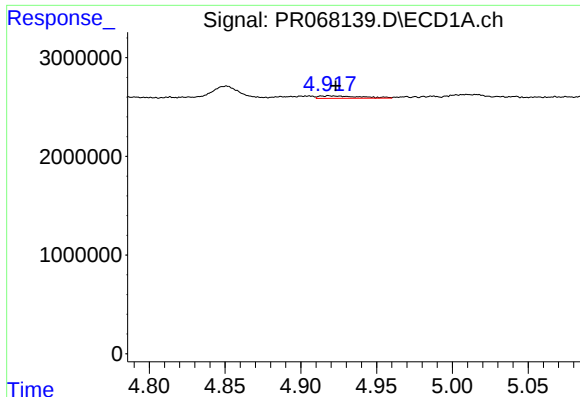

#17 AR-1242-2


R.T.: 4.919 min
Delta R.T.: -0.004 min
Response: 492421
Conc: 5.80 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

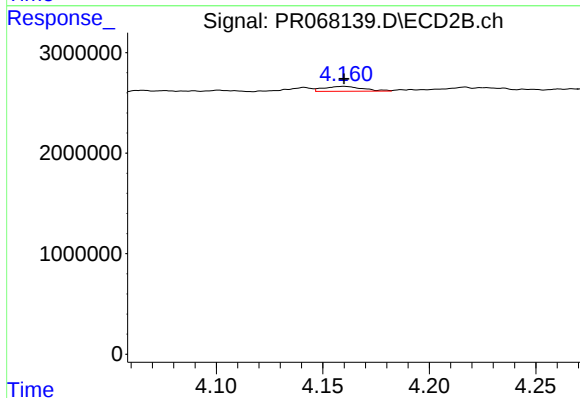


#17 AR-1242-2

R.T.: 4.160 min
Delta R.T.: 0.000 min
Response: 612591
Conc: 3.44 ng/ml

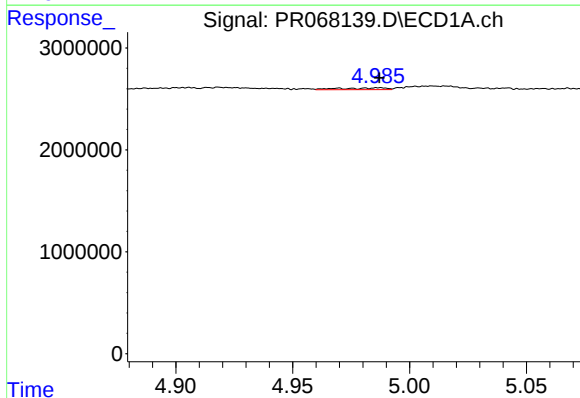


#18 AR-1242-3

R.T.: 4.987 min
Delta R.T.: 0.000 min
Response: 231295
Conc: 3.97 ng/ml

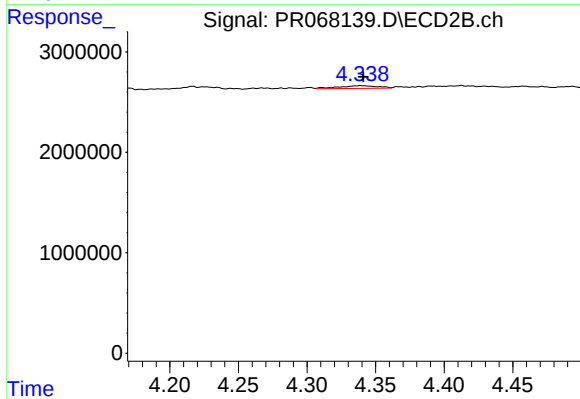

#18 AR-1242-3


R.T.: 4.340 min
Delta R.T.: -0.001 min
Response: 551476
Conc: 5.51 ng/ml

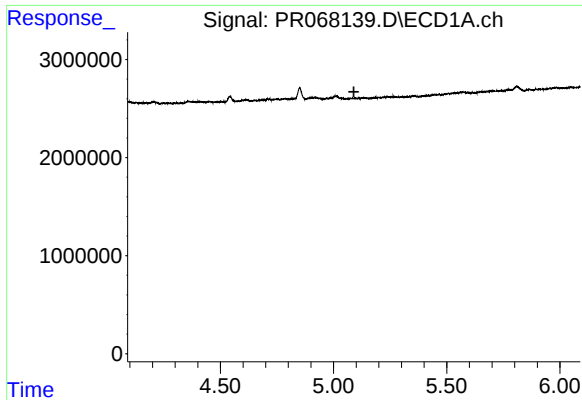

#19 AR-1242-4


R.T.: 0.000 min
Exp R.T.: 5.090 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

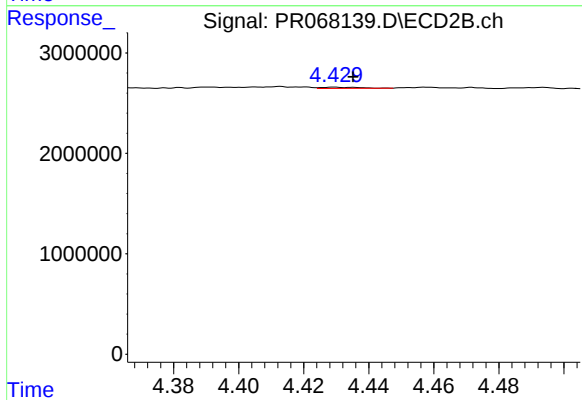


#19 AR-1242-4

R.T.: 4.429 min
Delta R.T.: -0.006 min
Response: 99954
Conc: 0.98 ng/ml

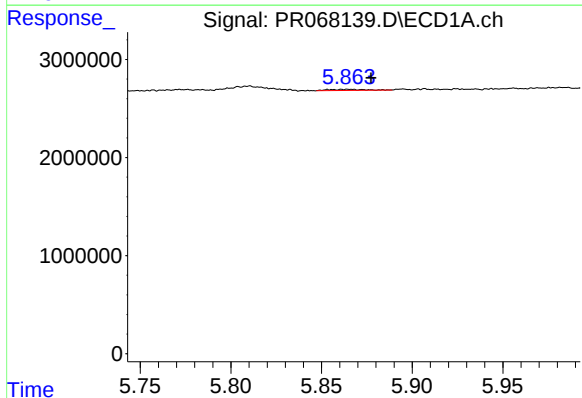


#20 AR-1242-5

R.T.: 5.865 min
Delta R.T.: -0.013 min
Response: 155785
Conc: 3.59 ng/ml

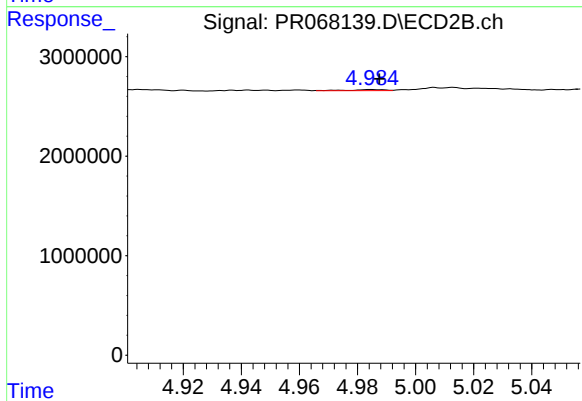

#20 AR-1242-5


R.T.: 4.985 min
Delta R.T.: -0.003 min
Response: 96760
Conc: 0.76 ng/ml

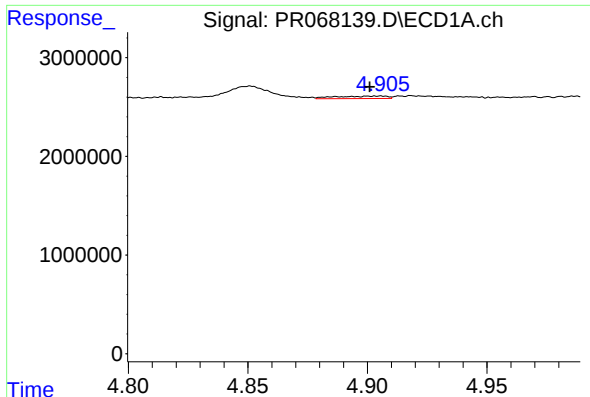

#21 AR-1248-1


R.T.: 4.905 min
Delta R.T.: 0.004 min
Response: 377927
Conc: 10.38 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

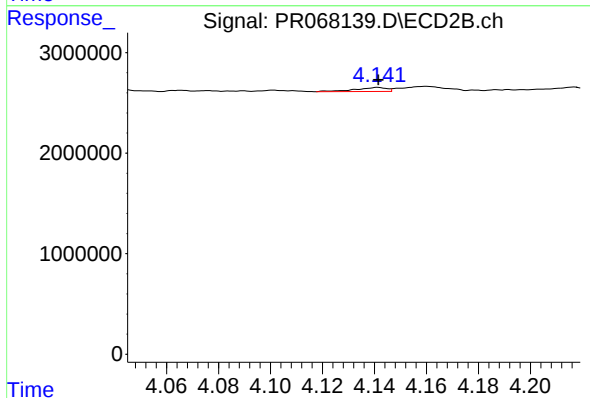


#21 AR-1248-1

R.T.: 4.141 min
Delta R.T.: 0.000 min
Response: 338203
Conc: 3.20 ng/ml

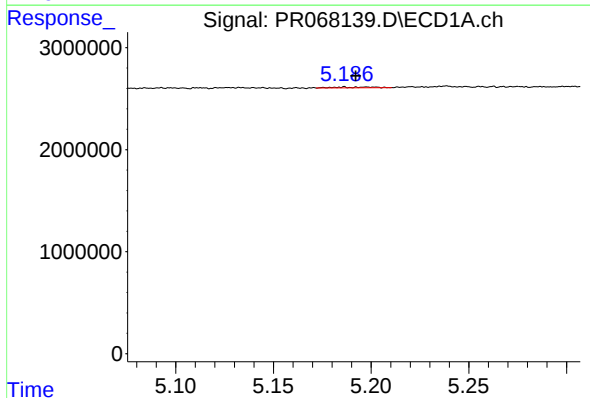


#22 AR-1248-2

R.T.: 5.186 min
Delta R.T.: -0.006 min
Response: 97473
Conc: 1.98 ng/ml

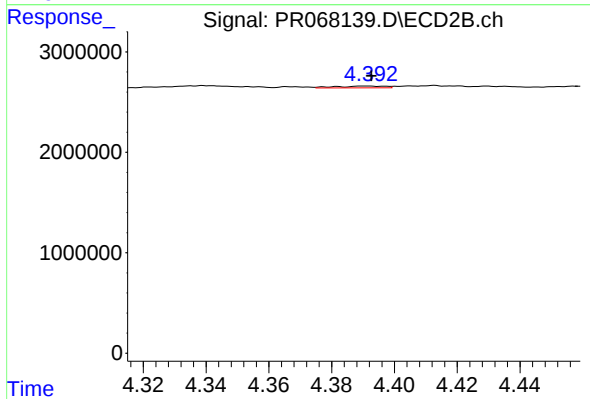

#22 AR-1248-2


R.T.: 4.391 min
Delta R.T.: -0.002 min
Response: 198232
Conc: 1.27 ng/ml

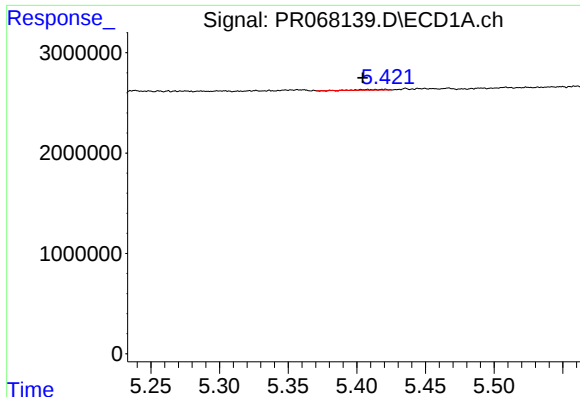

#23 AR-1248-3


R.T.: 5.420 min
Delta R.T.: 0.016 min
Response: 75671
Conc: 1.12 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

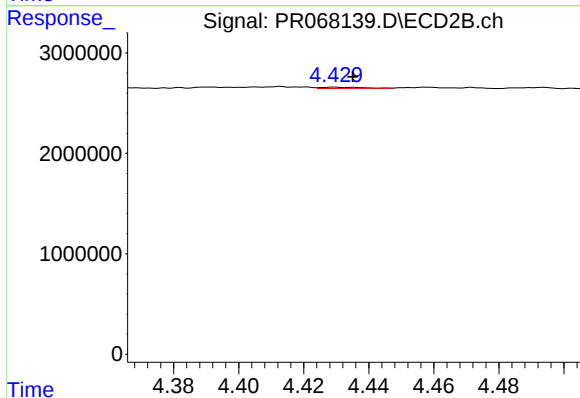


#23 AR-1248-3

R.T.: 4.429 min
Delta R.T.: -0.006 min
Response: 99954
Conc: 0.63 ng/ml

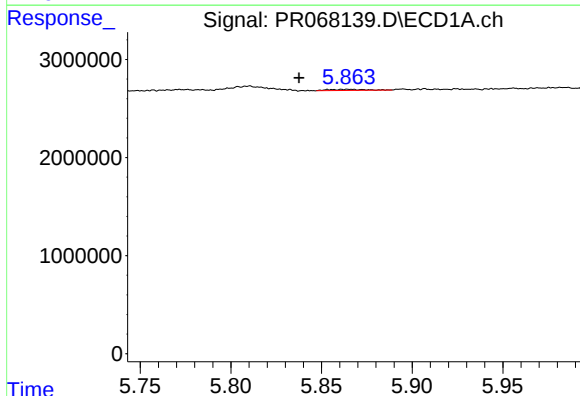


#24 AR-1248-4

R.T.: 5.865 min
Delta R.T.: 0.027 min
Response: 155785
Conc: 2.17 ng/ml

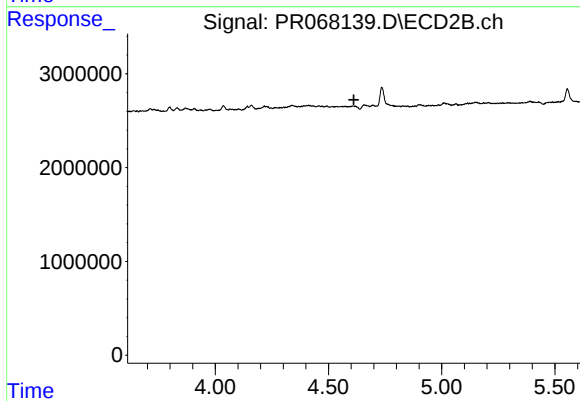

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 4.612 min
Response: 0
Conc: N.D.

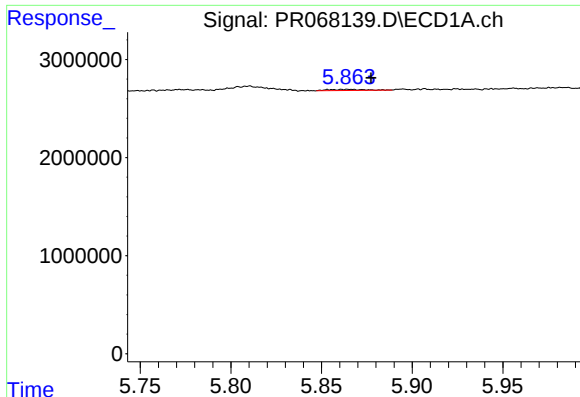

#25 AR-1248-5


R.T.: 5.865 min
Delta R.T.: -0.013 min
Response: 155785
Conc: 1.99 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

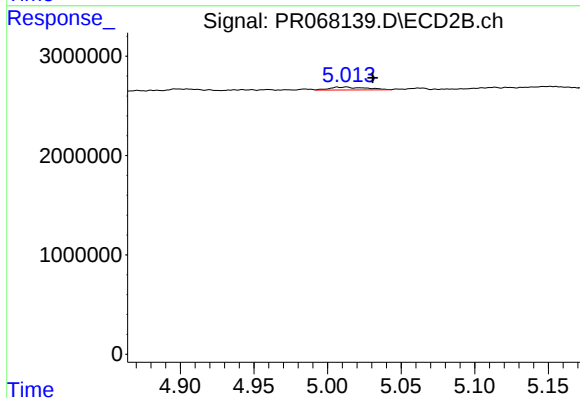


#25 AR-1248-5

R.T.: 5.013 min
Delta R.T.: -0.018 min
Response: 504395
Conc: 2.78 ng/ml

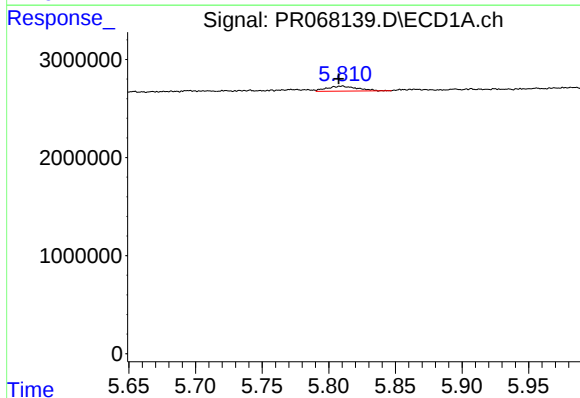


#26 AR-1254-1

R.T.: 5.810 min
Delta R.T.: 0.002 min
Response: 819697
Conc: 12.09 ng/ml

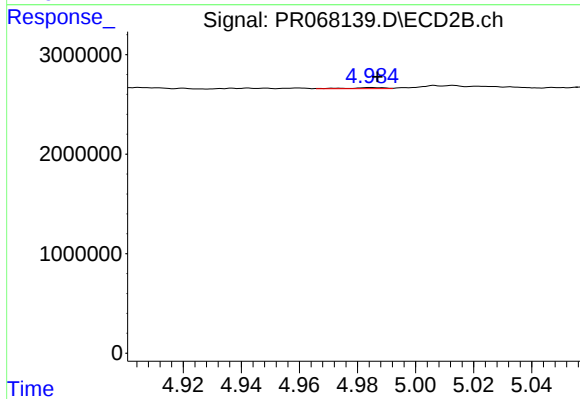

#26 AR-1254-1


R.T.: 4.985 min
Delta R.T.: -0.002 min
Response: 96760
Conc: 0.35 ng/ml

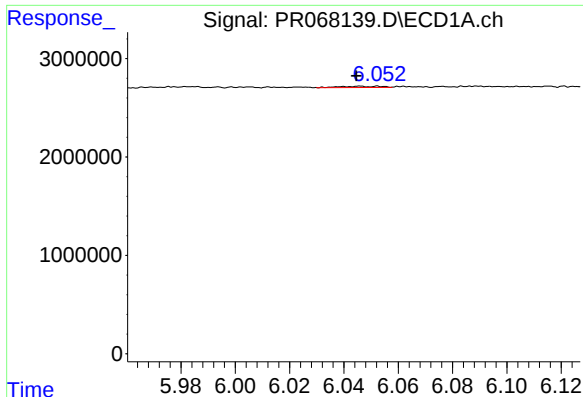

#27 AR-1254-2


R.T.: 6.046 min
Delta R.T.: 0.001 min
Response: 137225
Conc: 1.28 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

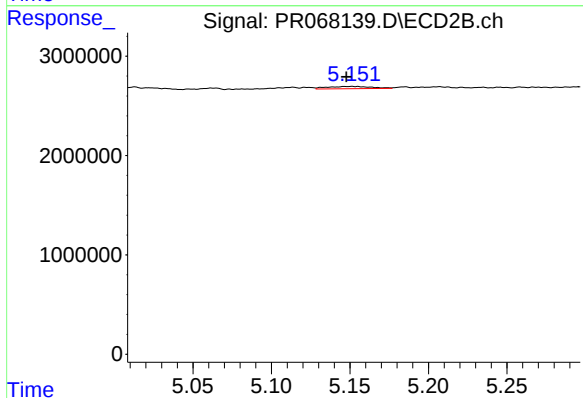


#27 AR-1254-2

R.T.: 5.151 min
Delta R.T.: 0.004 min
Response: 446365
Conc: 1.79 ng/ml

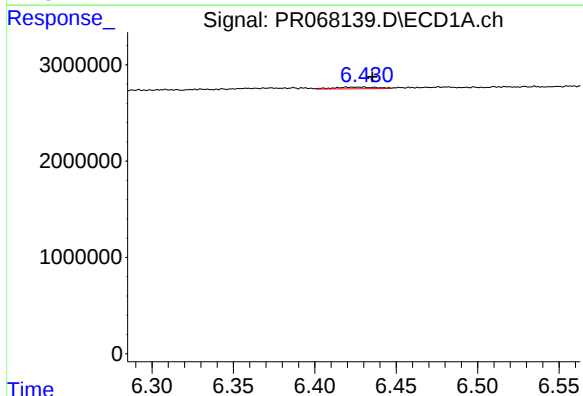


#28 AR-1254-3

R.T.: 6.429 min
Delta R.T.: -0.006 min
Response: 304110
Conc: 2.34 ng/ml

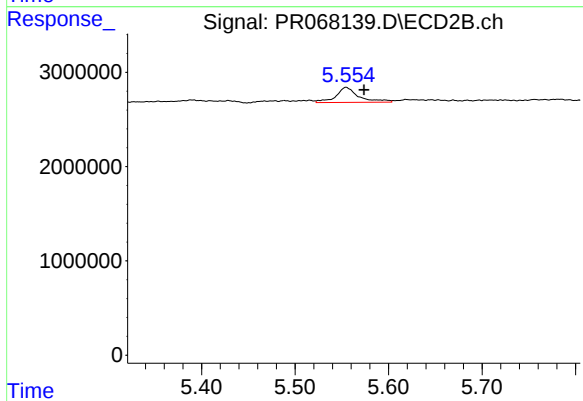

#28 AR-1254-3


R.T.: 5.555 min
Delta R.T.: -0.019 min
Response: 2701120
Conc: 6.96 ng/ml

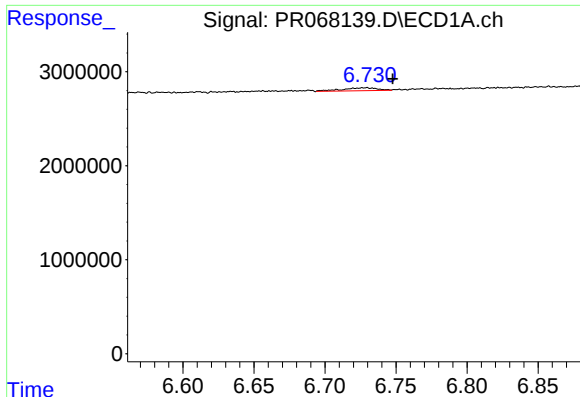

#29 AR-1254-4


R.T.: 6.729 min
Delta R.T.: -0.019 min
Response: 543350
Conc: 5.08 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

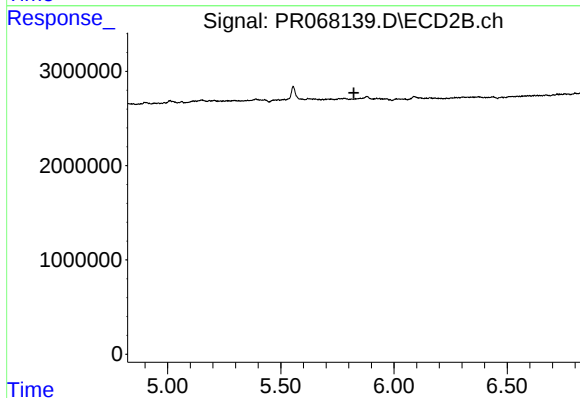


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 5.823 min
Response: 0
Conc: N.D.

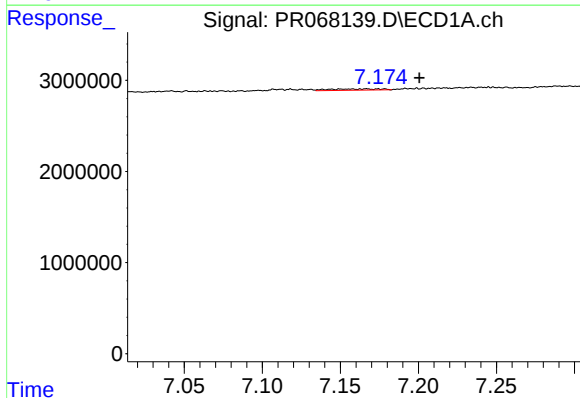


#30 AR-1254-5

R.T.: 7.178 min
Delta R.T.: -0.022 min
Response: 332689
Conc: 2.63 ng/ml

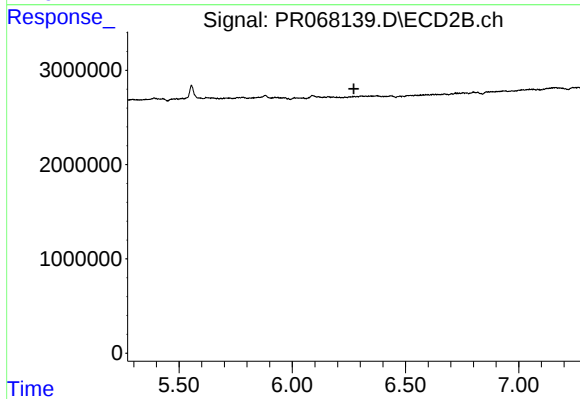

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 6.272 min
Response: 0
Conc: N.D.

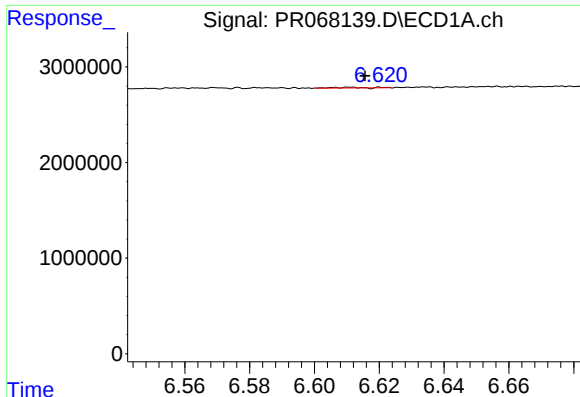

#31 AR-1260-1


R.T.: 6.611 min
Delta R.T.: -0.004 min
Response: 40420
Conc: 0.45 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

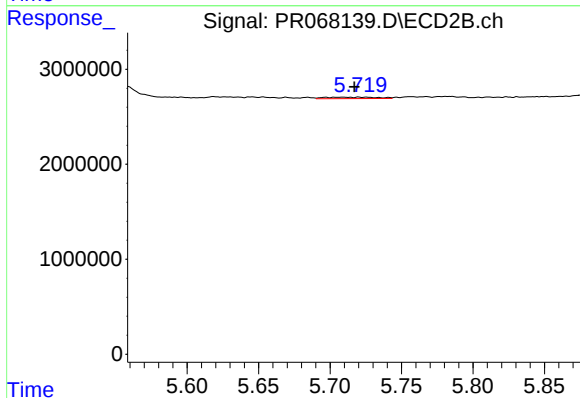


#31 AR-1260-1

R.T.: 5.720 min
Delta R.T.: 0.003 min
Response: 402242
Conc: 1.36 ng/ml

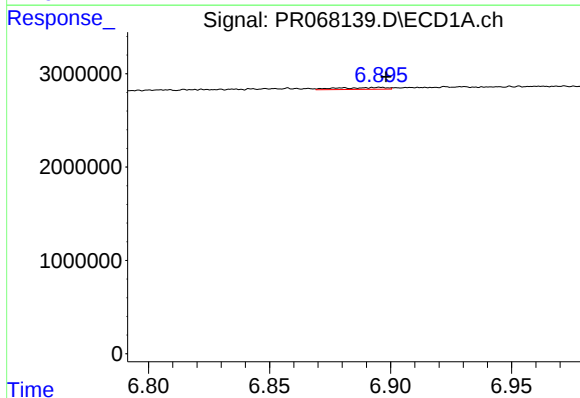


#32 AR-1260-2

R.T.: 6.896 min
Delta R.T.: -0.003 min
Response: 271257
Conc: 1.88 ng/ml

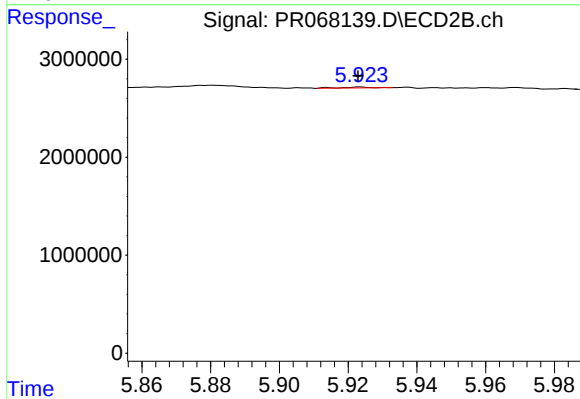

#32 AR-1260-2


R.T.: 5.924 min
Delta R.T.: 0.000 min
Response: 58810
Conc: 0.17 ng/ml

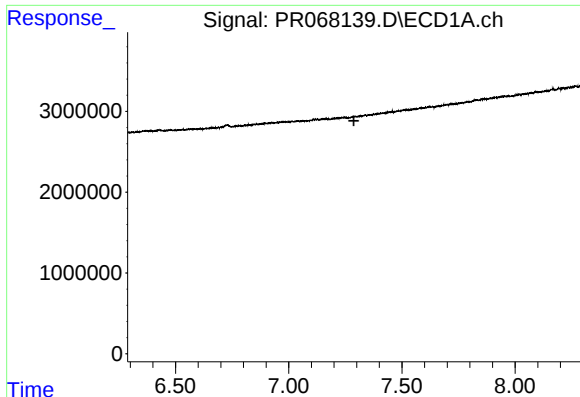

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 7.288 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

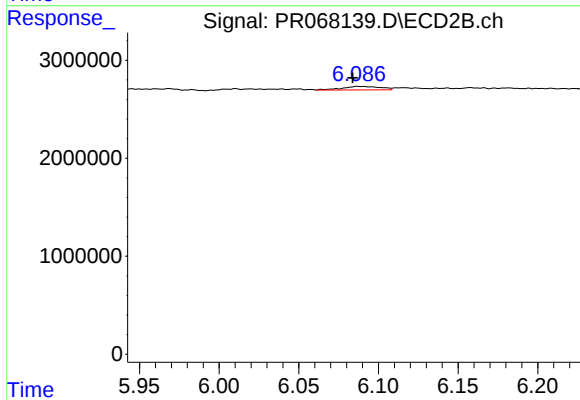


#33 AR-1260-3

R.T.: 6.088 min
Delta R.T.: 0.004 min
Response: 608744
Conc: 1.88 ng/ml

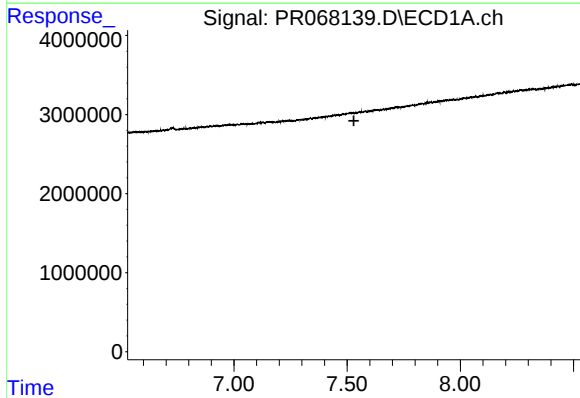


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T.: 7.530 min
Response: 0
Conc: N.D.

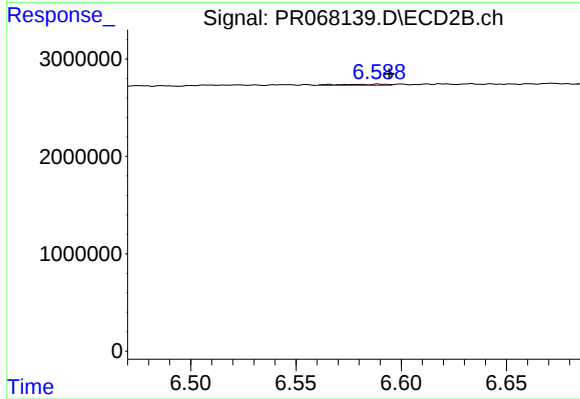

#34 AR-1260-4


R.T.: 6.589 min
Delta R.T.: -0.005 min
Response: 193188
Conc: 0.78 ng/ml

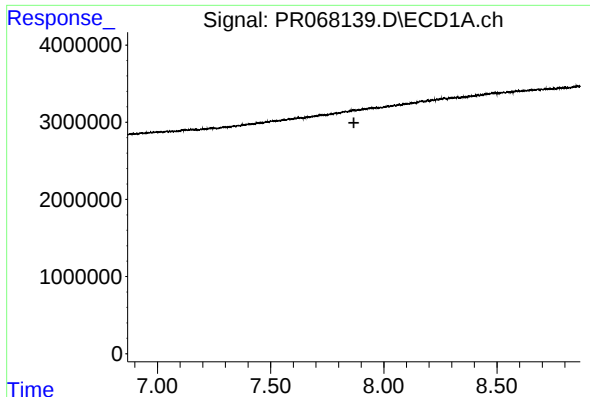

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 7.868 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

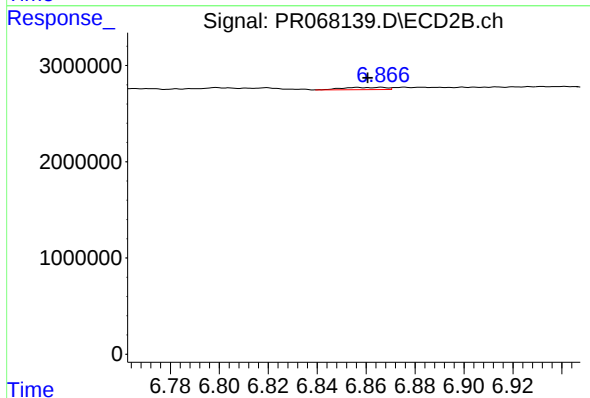


#35 AR-1260-5

R.T.: 6.866 min
Delta R.T.: 0.006 min
Response: 287512
Conc: 0.51 ng/ml

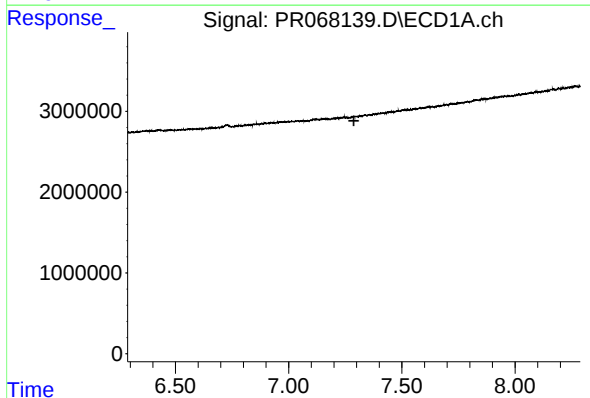


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 7.288 min
Response: 0
Conc: N.D.

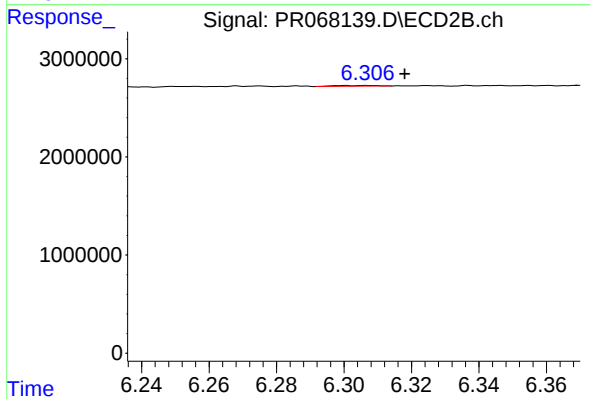

#36 AR-1262-1


R.T.: 6.307 min
Delta R.T.: -0.011 min
Response: 63170
Conc: 0.17 ng/ml

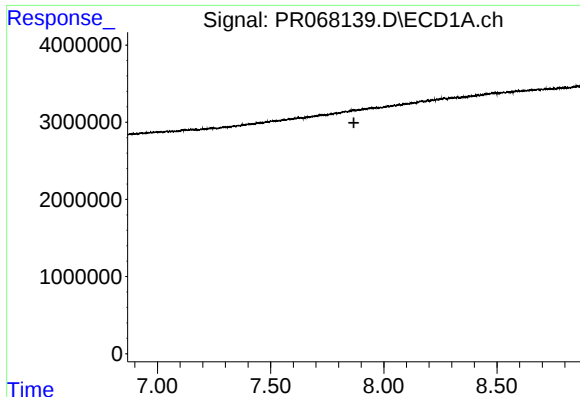

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 7.868 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

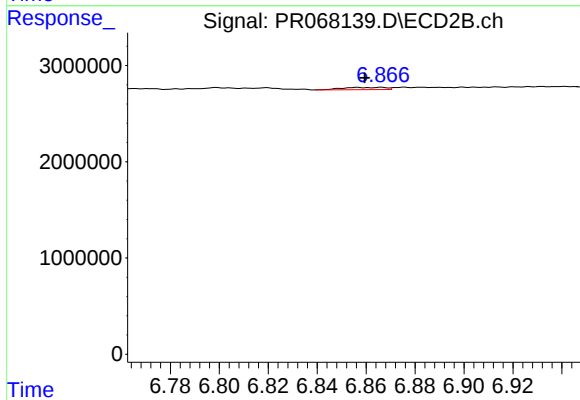


#37 AR-1262-2

R.T.: 6.866 min
Delta R.T.: 0.007 min
Response: 287512
Conc: 0.46 ng/ml

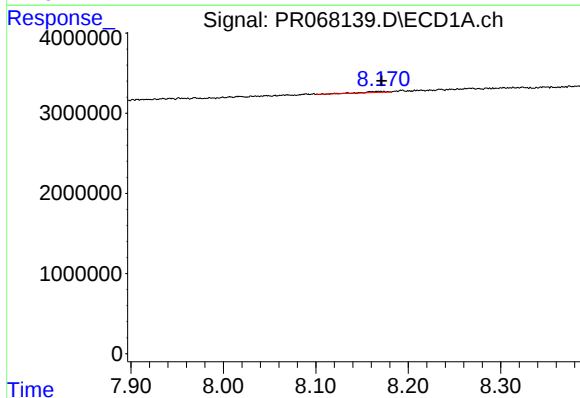


#38 AR-1262-3

R.T.: 8.169 min
Delta R.T.: -0.003 min
Response: 200190
Conc: 0.61 ng/ml

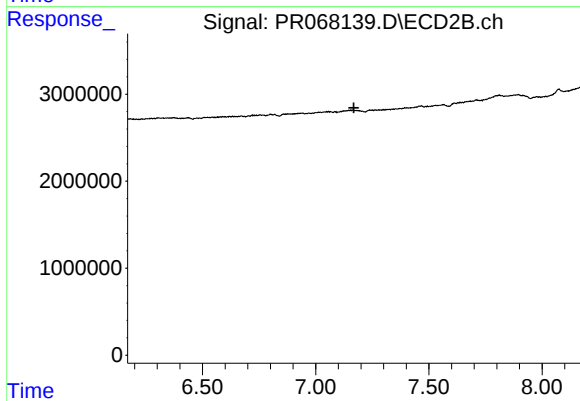

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 7.168 min
Response: 0
Conc: N.D.

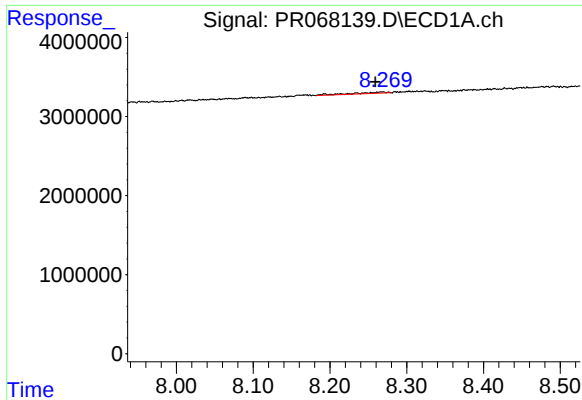

#39 AR-1262-4


R.T.: 8.267 min
Delta R.T.: 0.008 min
Response: 505267
Conc: 1.77 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

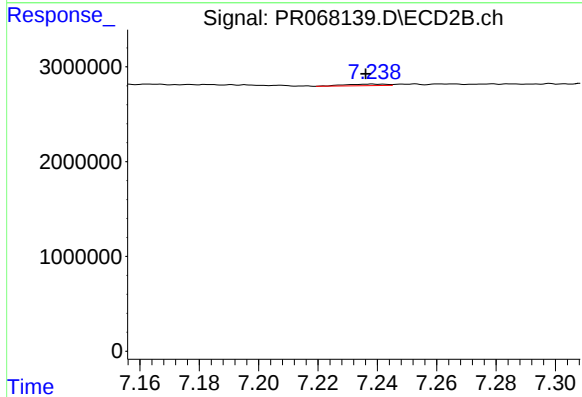


#39 AR-1262-4

R.T.: 7.238 min
Delta R.T.: 0.002 min
Response: 159590
Conc: 0.34 ng/ml

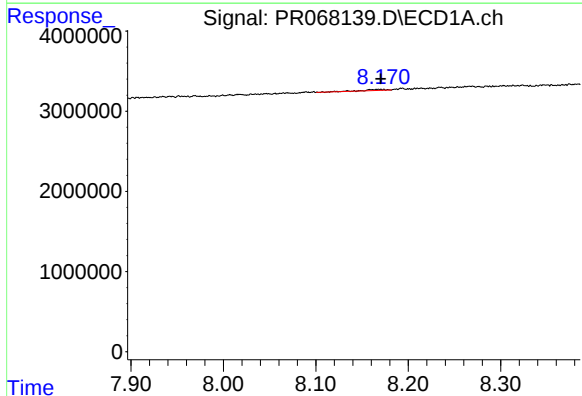


#41 AR-1268-1

R.T.: 8.169 min
Delta R.T.: -0.001 min
Response: 200190
Conc: 0.31 ng/ml

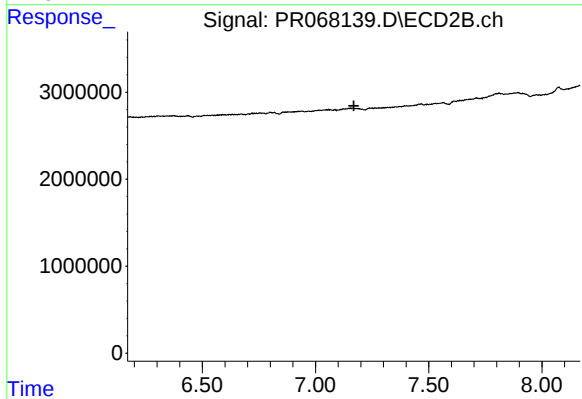

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 7.169 min
Response: 0
Conc: N.D.

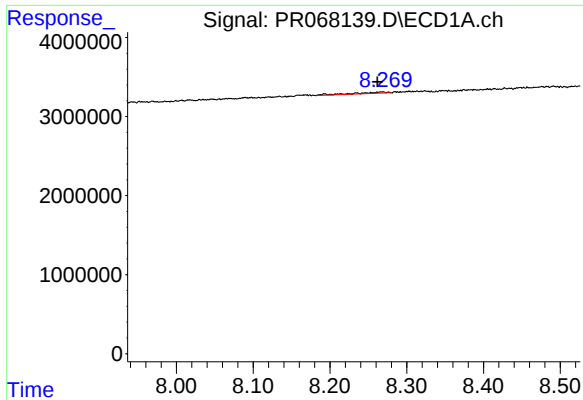

#42 AR-1268-2


R.T.: 8.267 min
Delta R.T.: 0.005 min
Response: 505267
Conc: 0.86 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

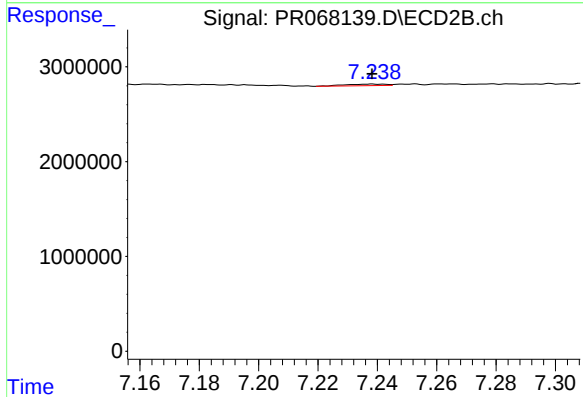


#42 AR-1268-2

R.T.: 7.238 min
Delta R.T.: 0.000 min
Response: 159590
Conc: 0.24 ng/ml

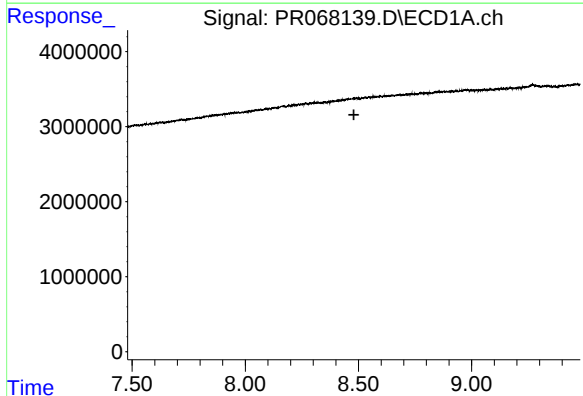


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 8.480 min
Response: 0
Conc: N.D.

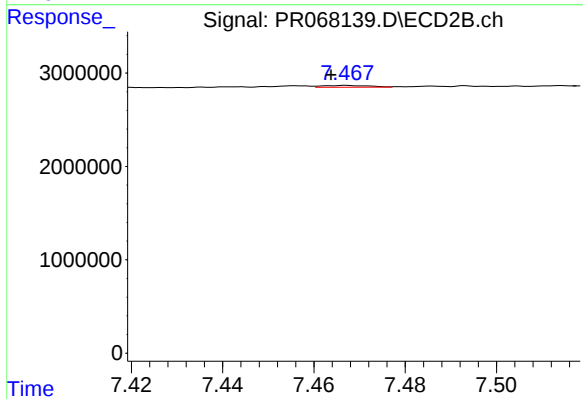

#43 AR-1268-3


R.T.: 7.467 min
Delta R.T.: 0.003 min
Response: 130516
Conc: 0.22 ng/ml

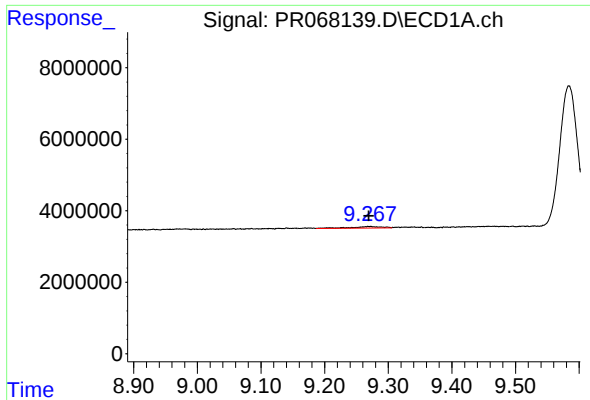

#45 AR-1268-5

R.T.: 9.270 min
Delta R.T.: 0.000 min
Response: 1512171
Conc: 0.94 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT3-2024

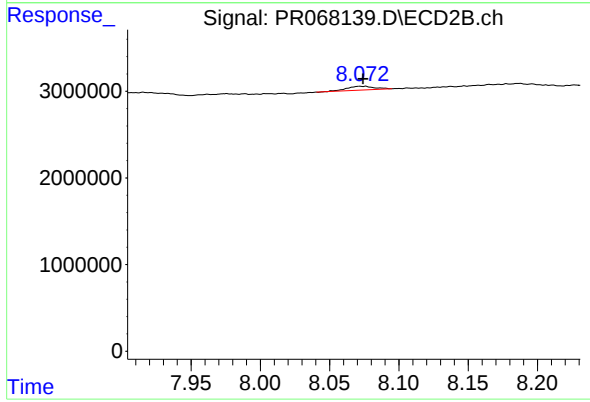

#45 AR-1268-5

R.T.: 8.075 min
Delta R.T.: 0.000 min
Response: 615811
Conc: 0.37 ng/ml