

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR081224\
 Data File : PR068153.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2024 14:04
 Operator : AJ\MA
 Sample : P3520-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 OU4-CF-09-080624

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/14/2024
 Supervised By :Ankita Jodhani 08/14/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 03:57:20 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 08 22:24:34 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.676	3.009	52604447	136.9E6	21.179	27.503m#
2) SA Decachlor...	9.583	8.328	100.5E6	108.6E6	22.381	20.697

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR081224\
Data File : PR068153.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2024 14:04
Operator : AJ\MA
Sample : P3520-03
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
OU4-CF-09-080624


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/14/2024
Supervised By :Ankita Jodhani 08/14/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 03:57:20 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080824.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 08 22:24:34 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

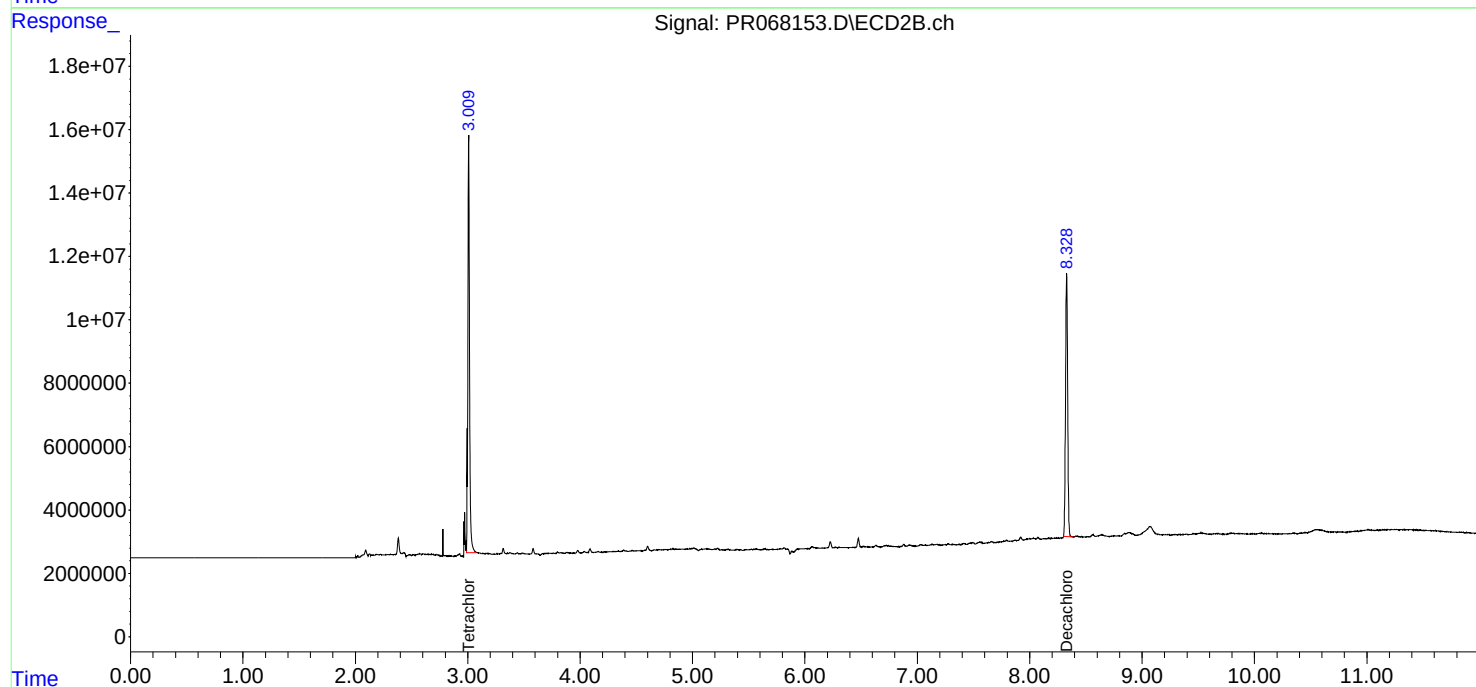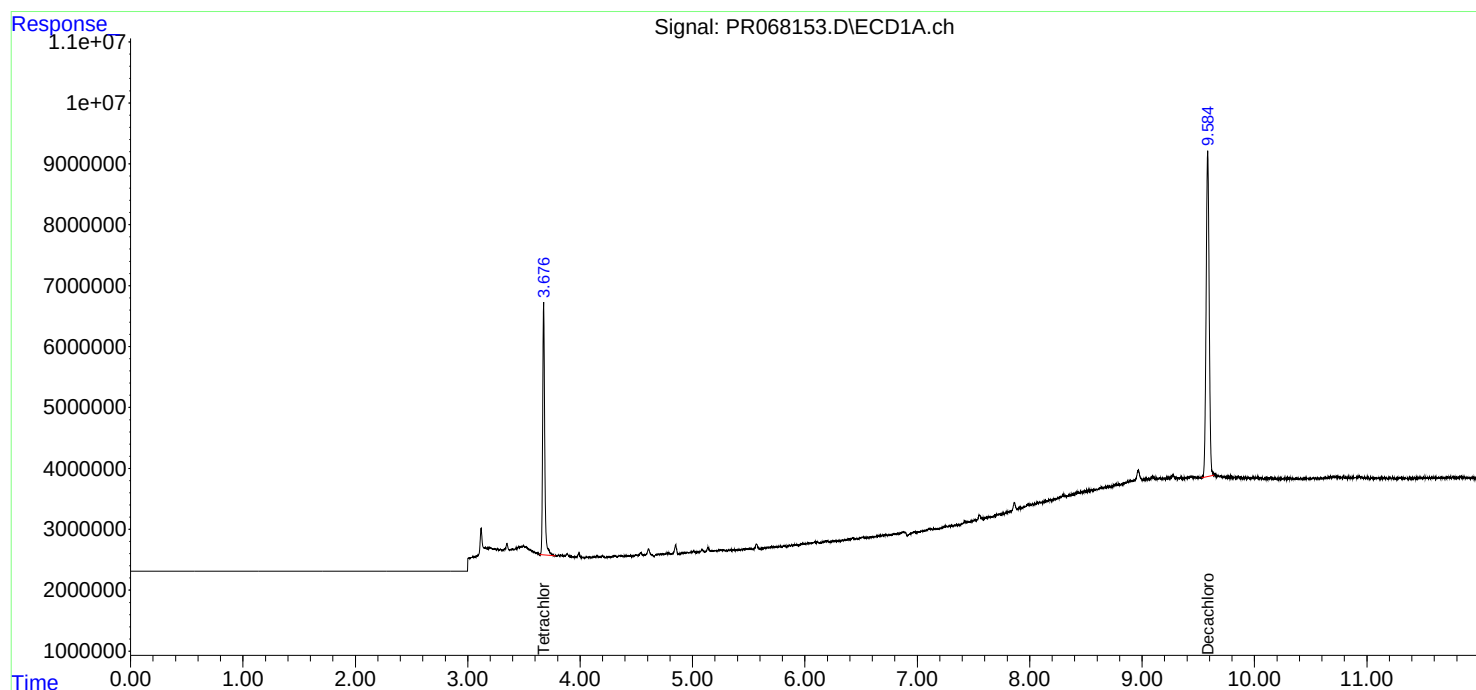

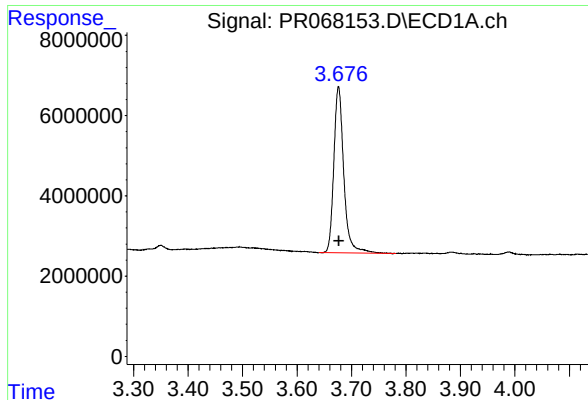


#1 Tetrachloro-m-xylene

R.T.: 3.676 min
Delta R.T.: 0.000 min
Response: 52604447
Conc: 21.18 ng/ml

Instrument :
ECD_R
ClientSampleId :
OU4-CF-09-080624


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/14/2024
Supervised By :Ankita Jodhani 08/14/2024

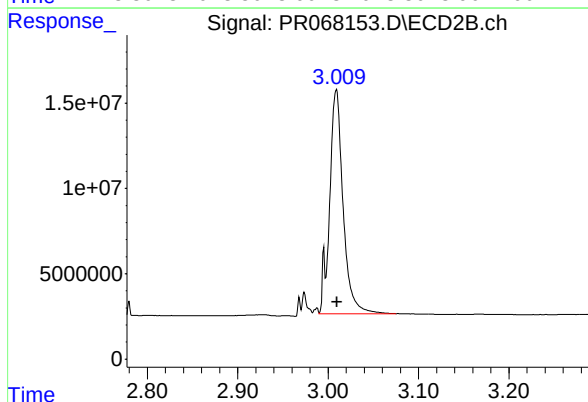


#1 Tetrachloro-m-xylene

R.T.: 3.009 min
Delta R.T.: 0.000 min
Response: 136852102
Conc: 27.50 ng/ml m

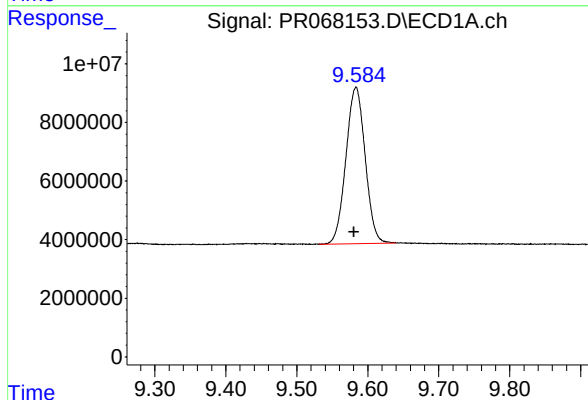

#2 Decachlorobiphenyl

R.T.: 9.583 min
Delta R.T.: 0.003 min
Response: 100492538
Conc: 22.38 ng/ml

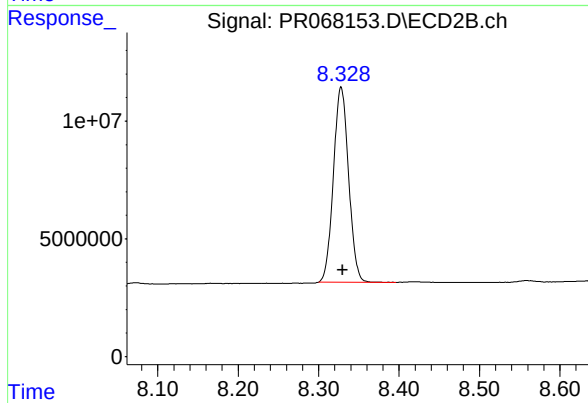

#2 Decachlorobiphenyl

R.T.: 8.328 min
Delta R.T.: -0.002 min
Response: 108552031
Conc: 20.70 ng/ml